

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110822\
 Data File : PL078924.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2022 18:06
 Operator : AR\AJ
 Sample : N5436-11RE
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 250FERRYBLVD-TFS-11RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 17:50:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.321	2.568	28476165	21260567	14.932	8.327 #
28)	SA Decachlor...	8.768	7.634	247.8E6	307.5E6	164.726	162.321
Target Compounds							
13)	MA Dieldrin	6.114	5.105	154.8E6	36978639	71.791	12.480m#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110822\
Data File : PL078924.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2022 18:06
Operator : AR\AJ
Sample : N5436-11RE
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-11RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 17:50:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

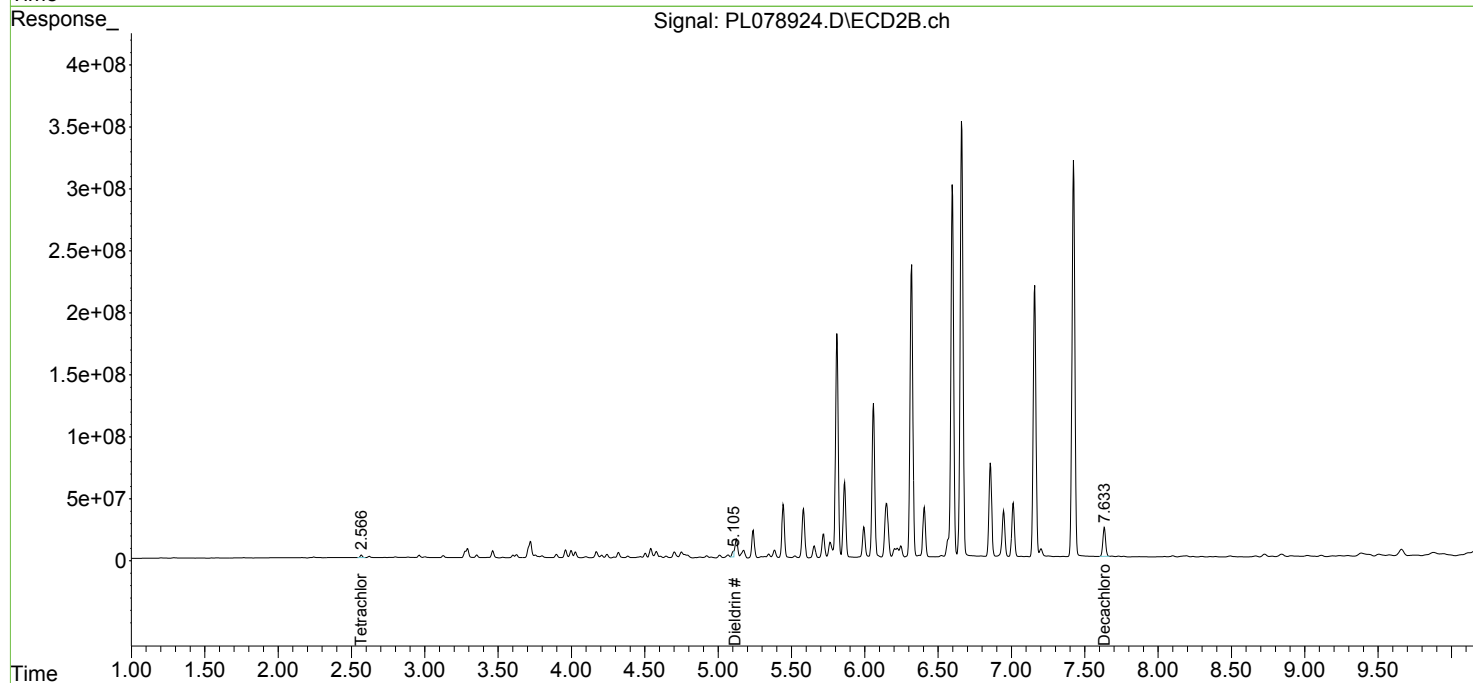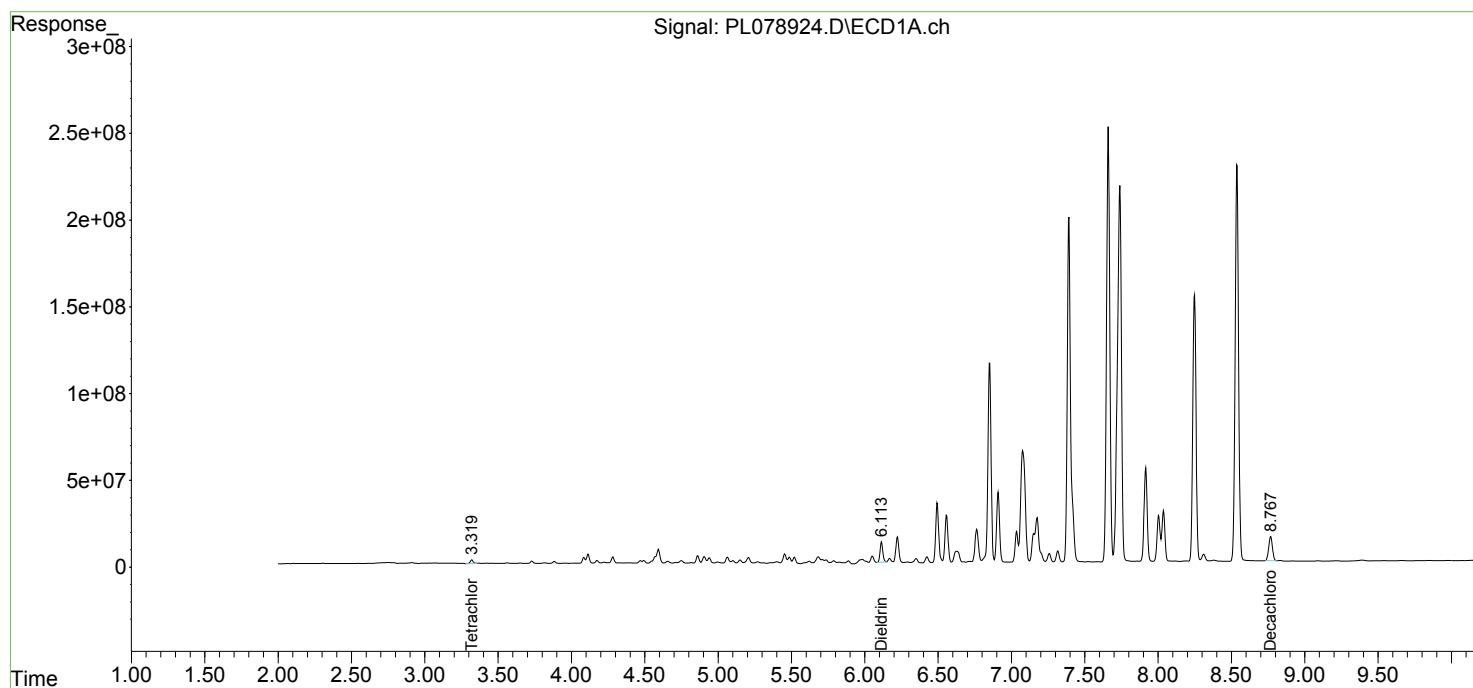


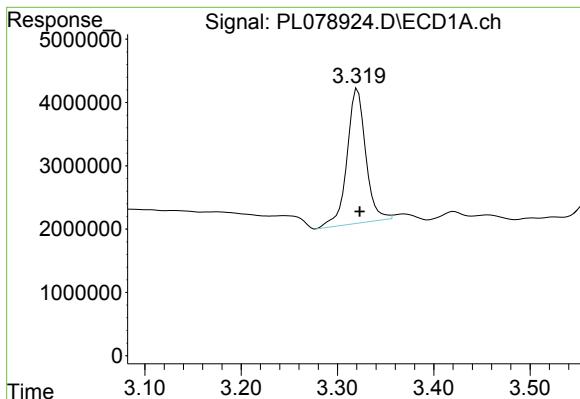

#1 Tetrachloro-m-xylene


R.T.: 3.321 min
Delta R.T.: -0.002 min
Response: 28476165
Conc: 14.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-11RE

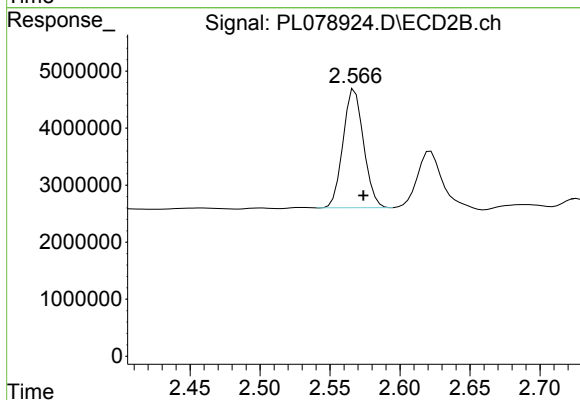


#1 Tetrachloro-m-xylene

R.T.: 2.568 min
Delta R.T.: -0.006 min
Response: 21260567
Conc: 8.33 ng/ml

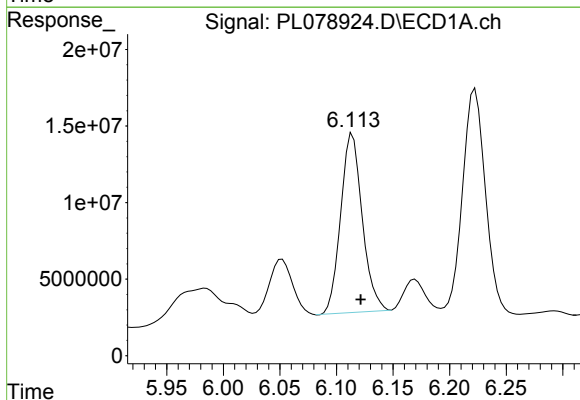


#13 Dieldrin

R.T.: 6.114 min
Delta R.T.: -0.007 min
Response: 154817652
Conc: 71.79 ng/ml

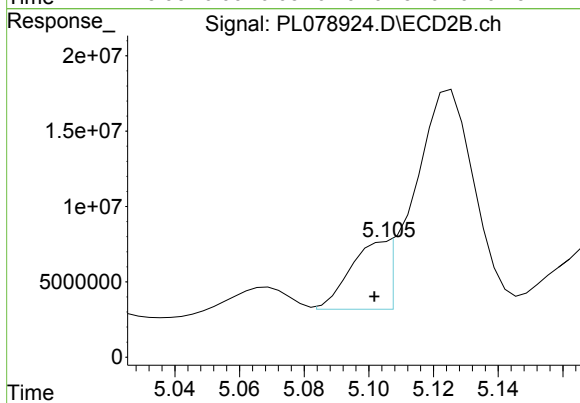

#13 Dieldrin

R.T.: 5.105 min
Delta R.T.: 0.004 min
Response: 36978639
Conc: 12.48 ng/ml m

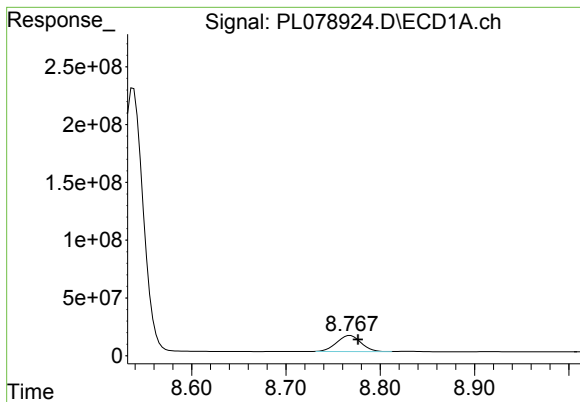

#28 Decachlorobiphenyl


R.T.: 8.768 min

Delta R.T.: -0.008 min

Response: 247807686

Conc: 164.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-11RE

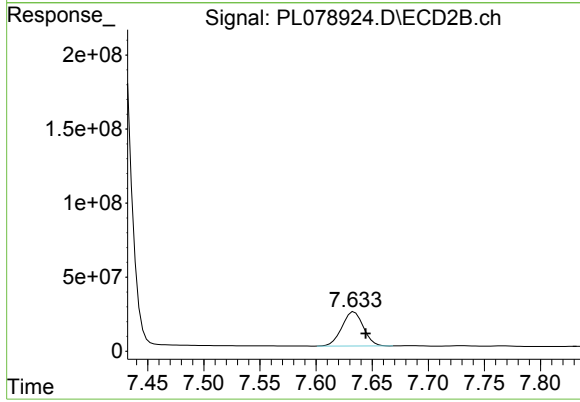

#28 Decachlorobiphenyl

R.T.: 7.634 min

Delta R.T.: -0.010 min

Response: 307452056

Conc: 162.32 ng/ml