

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110822\
 Data File : PL078926.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2022 18:34
 Operator : AR\AJ
 Sample : N5436-13RE
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 250FERRYBLVD-TFS-13RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 17:51:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.321	2.567	39110868	25540443	20.509	10.003 #
28)	SA Decachlor...	8.767	7.634	363.2E6	408.5E6	241.453	215.653
Target Compounds							
13)	MA Dieldrin	6.113	5.102	205.0E6	80203857	95.059	27.068m#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110822\
Data File : PL078926.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2022 18:34
Operator : AR\AJ
Sample : N5436-13RE
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-13RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 17:51:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

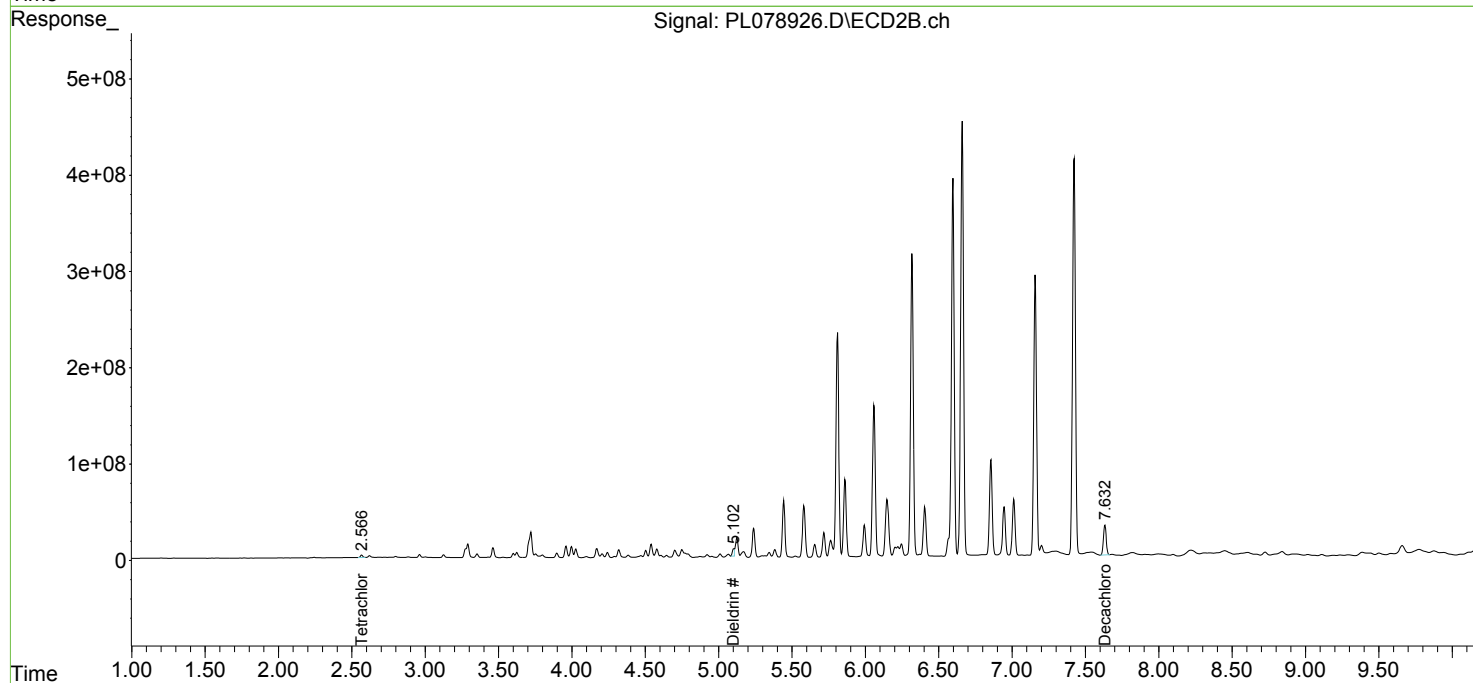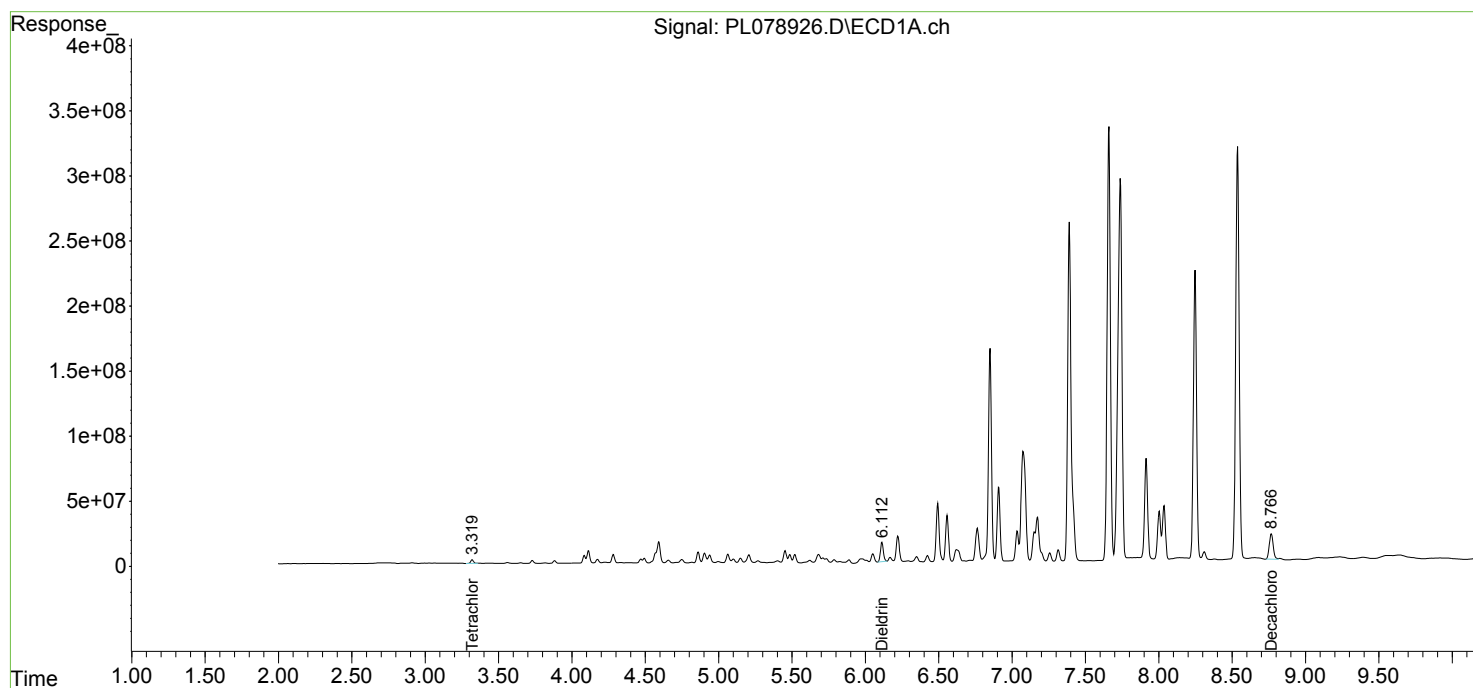


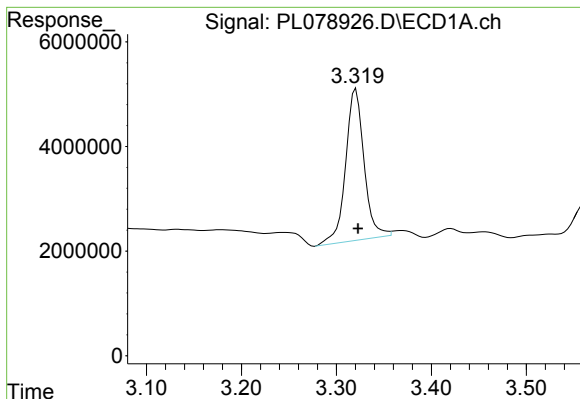

#1 Tetrachloro-m-xylene


R.T.: 3.321 min
Delta R.T.: -0.002 min
Response: 39110868
Conc: 20.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-13RE

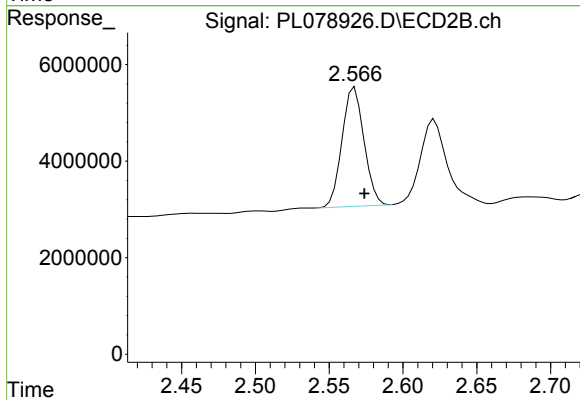


#1 Tetrachloro-m-xylene

R.T.: 2.567 min
Delta R.T.: -0.007 min
Response: 25540443
Conc: 10.00 ng/ml

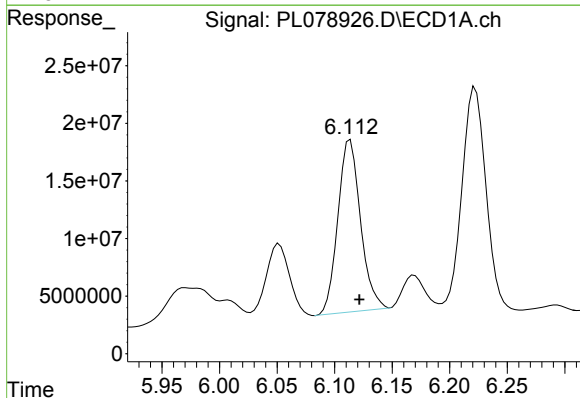


#13 Dieldrin

R.T.: 6.113 min
Delta R.T.: -0.008 min
Response: 204995916
Conc: 95.06 ng/ml

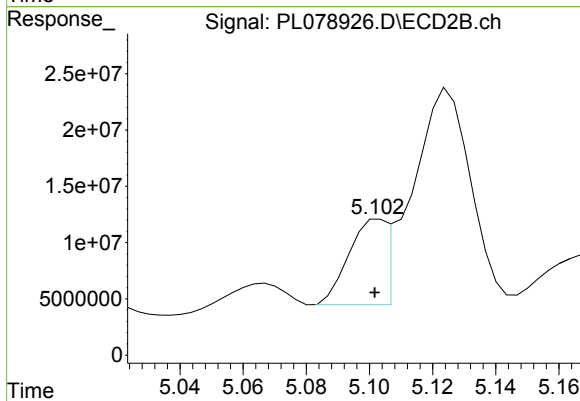

#13 Dieldrin


R.T.: 5.102 min
Delta R.T.: 0.000 min
Response: 80203857
Conc: 27.07 ng/ml m

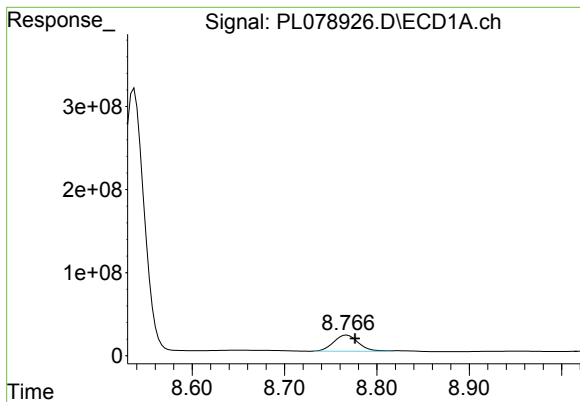

#28 Decachlorobiphenyl

R.T.: 8.767 min
Delta R.T.: -0.009 min
Response: 363232124
Conc: 241.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-13RE

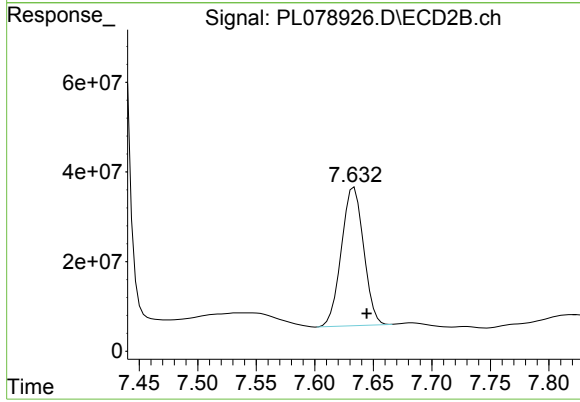

#28 Decachlorobiphenyl

R.T.: 7.634 min
Delta R.T.: -0.011 min
Response: 408469802
Conc: 215.65 ng/ml