

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110823\
 Data File : PL086523.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2023 10:18
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 10:55:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110823.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 08 10:47:46 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.352	2.617	228.8E6	88204230	73.938	74.766
28)	SA Decachlor...	8.851	7.767	198.4E6	83135043	74.593	74.582
Target Compounds							
23)	Chlordane-1	4.508	3.605	101.0E6	25714698	736.482	743.250
24)	Chlordane-2	5.041	4.183	106.9E6	32125865	740.700	743.837
25)	Chlordane-3	5.753	4.811	441.0E6	91556045	754.581	751.214
26)	Chlordane-4	5.835	4.873	536.5E6	97897366	753.795	748.230
27)	Chlordane-5	6.682	5.544	92960001	26983933	757.012	747.080



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110823\
Data File : PL086523.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2023 10:18
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 10:55:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110823.M
Quant Title : GC Extractables
QLast Update : Wed Nov 08 10:47:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

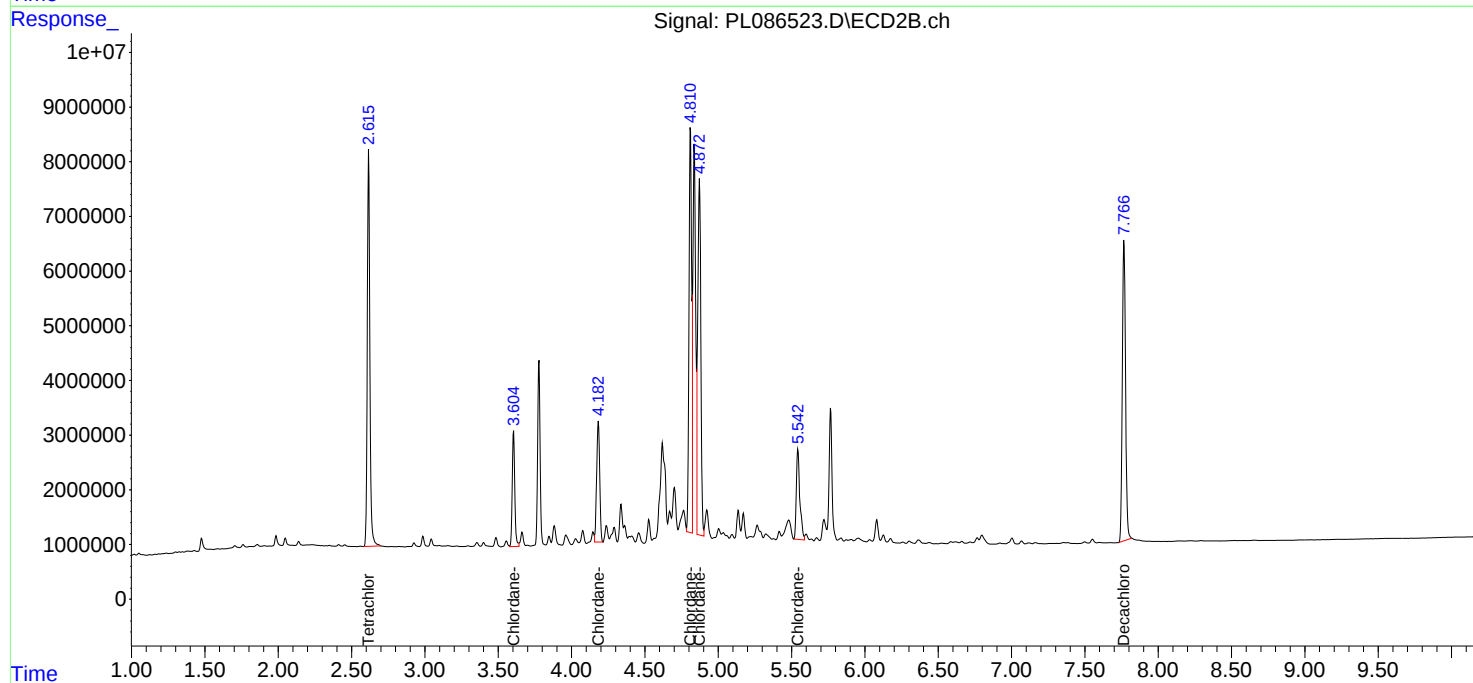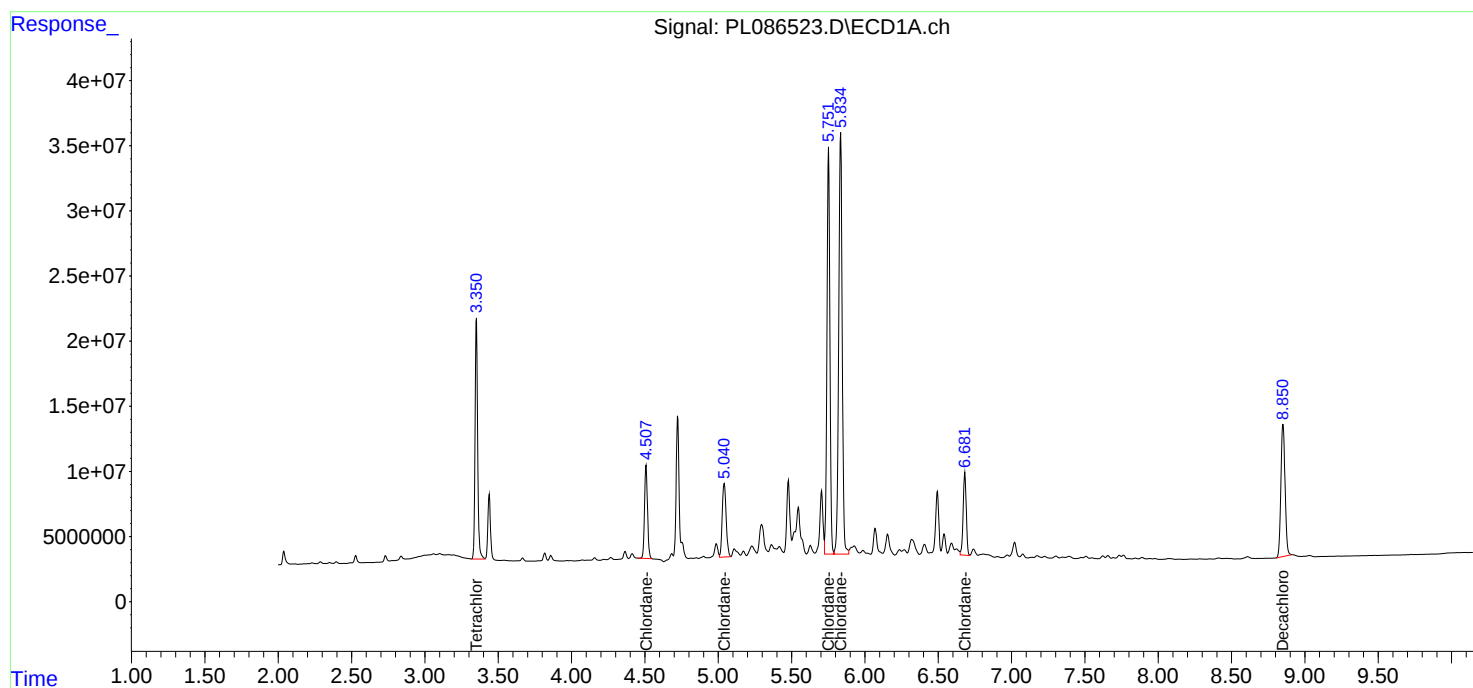


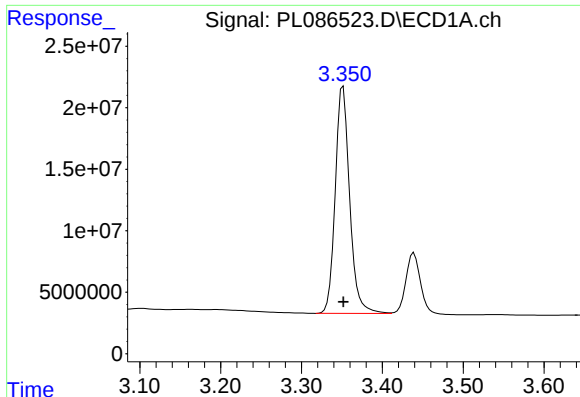

#1 Tetrachloro-m-xylene


R.T.: 3.352 min
Delta R.T.: 0.000 min
Response: 228826950
Conc: 73.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

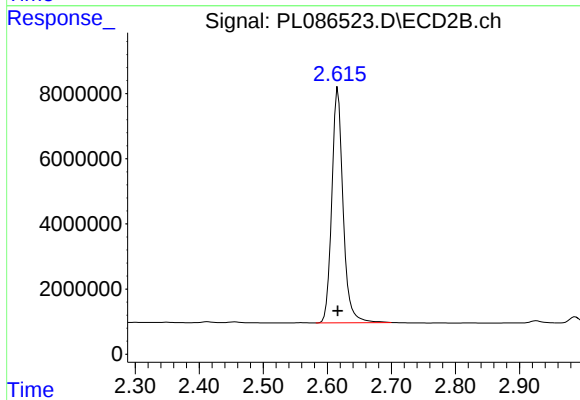


#1 Tetrachloro-m-xylene

R.T.: 2.617 min
Delta R.T.: 0.000 min
Response: 88204230
Conc: 74.77 ng/ml

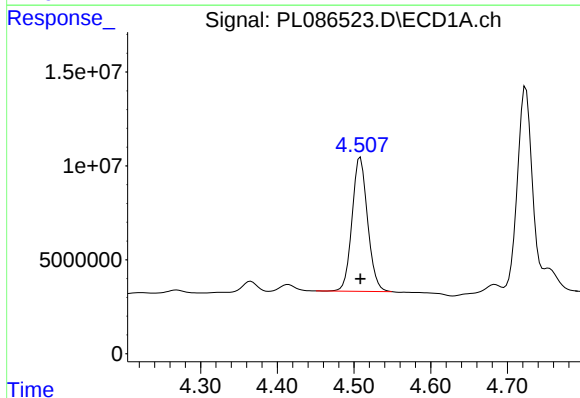


#23 Chlordane-1

R.T.: 4.508 min
Delta R.T.: 0.000 min
Response: 101048786
Conc: 736.48 ng/ml

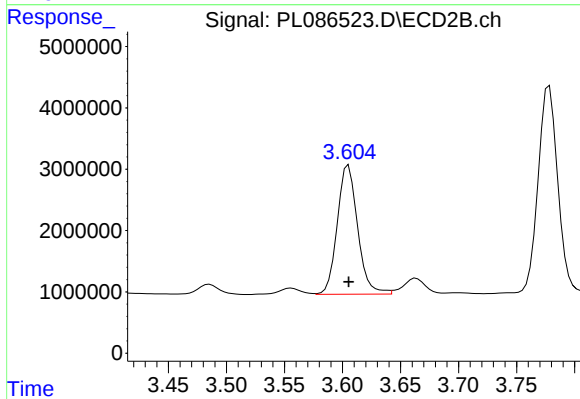

#23 Chlordane-1


R.T.: 3.605 min
Delta R.T.: 0.000 min
Response: 25714698
Conc: 743.25 ng/ml

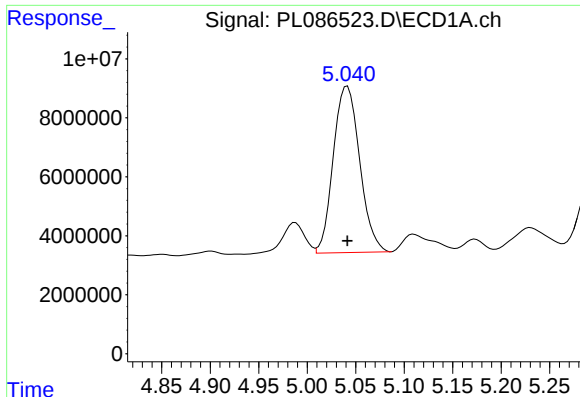

#24 Chlordane-2


R.T.: 5.041 min
Delta R.T.: 0.000 min
Response: 106856984
Conc: 740.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

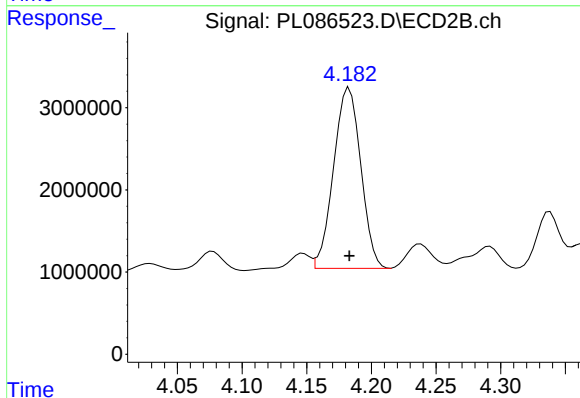


#24 Chlordane-2

R.T.: 4.183 min
Delta R.T.: 0.000 min
Response: 32125865
Conc: 743.84 ng/ml

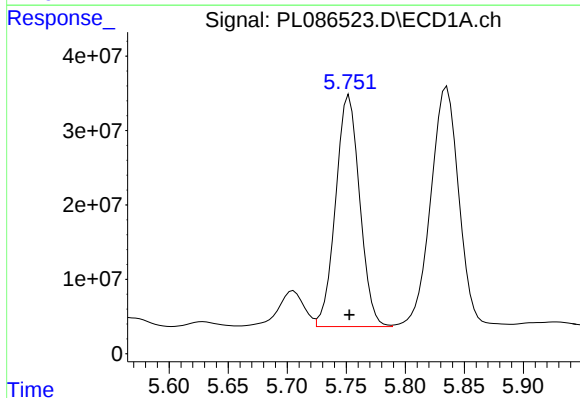


#25 Chlordane-3

R.T.: 5.753 min
Delta R.T.: 0.000 min
Response: 440976445
Conc: 754.58 ng/ml

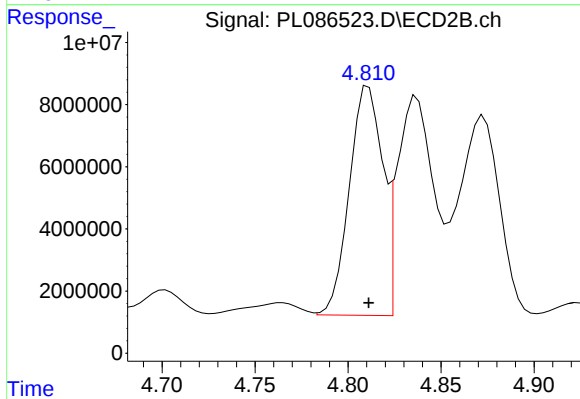

#25 Chlordane-3


R.T.: 4.811 min
Delta R.T.: 0.000 min
Response: 91556045
Conc: 751.21 ng/ml

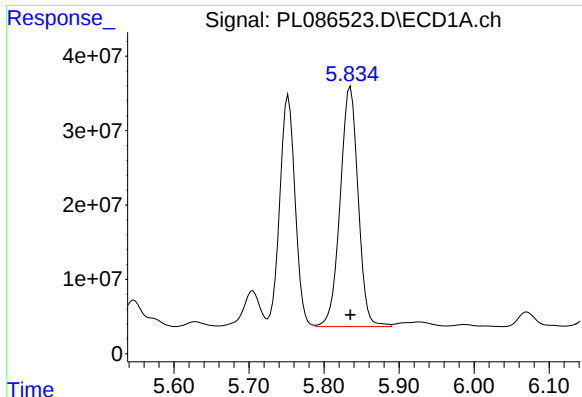

#26 Chlordane-4


R.T.: 5.835 min
Delta R.T.: 0.000 min
Response: 536450268
Conc: 753.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

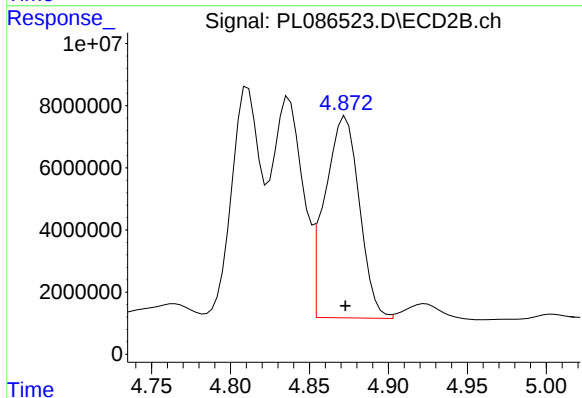


#26 Chlordane-4

R.T.: 4.873 min
Delta R.T.: 0.000 min
Response: 97897366
Conc: 748.23 ng/ml

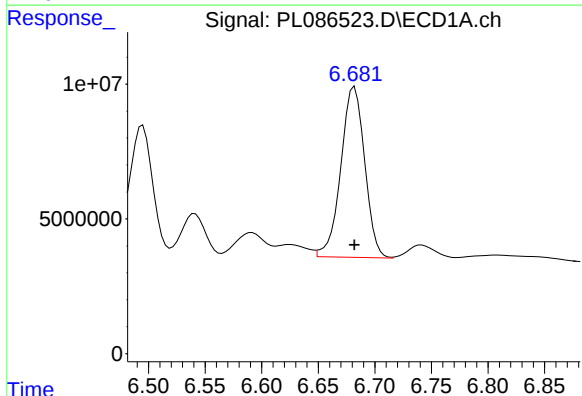


#27 Chlordane-5

R.T.: 6.682 min
Delta R.T.: 0.000 min
Response: 92960001
Conc: 757.01 ng/ml

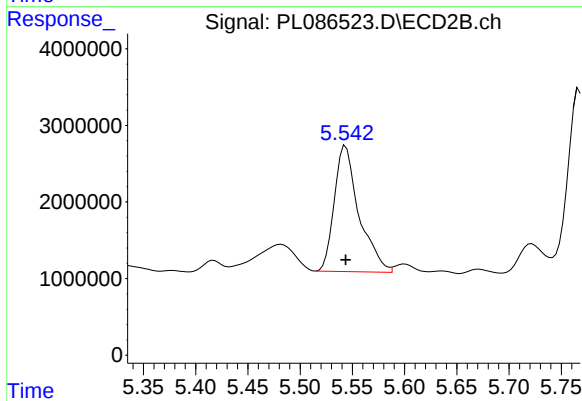

#27 Chlordane-5

R.T.: 5.544 min
Delta R.T.: 0.000 min
Response: 26983933
Conc: 747.08 ng/ml

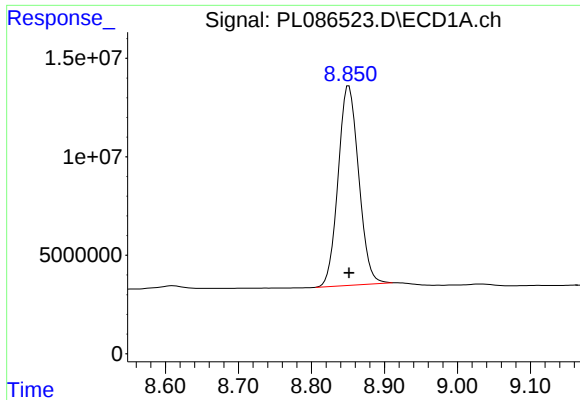

#28 Decachlorobiphenyl


R.T.: 8.851 min

Delta R.T.: 0.000 min

Response: 198365688

Conc: 74.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

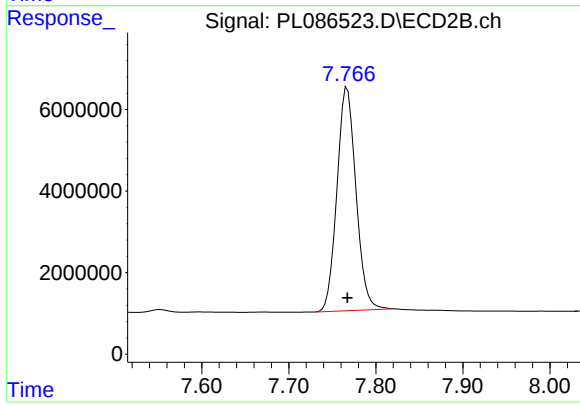

#28 Decachlorobiphenyl

R.T.: 7.767 min

Delta R.T.: 0.000 min

Response: 83135043

Conc: 74.58 ng/ml