

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110823\
 Data File : PL086524.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2023 10:31
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 10:48:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110823.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 08 10:47:46 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.351	2.617	151.6E6	57730749	50.000	50.000
28)	SA Decachlor...	8.852	7.768	133.7E6	56052009	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.508	3.605	67207307	17073321	500.000	500.000
24)	Chlordane-2	5.040	4.183	72253720	21734040	500.000	500.000
25)	Chlordane-3	5.752	4.811	278.4E6	57982279	500.000	500.000
26)	Chlordane-4	5.834	4.873	342.2E6	62580836	500.000	500.000
27)	Chlordane-5	6.682	5.543	59170864	17595890	500.000	500.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110823\
Data File : PL086524.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2023 10:31
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 10:48:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110823.M
Quant Title : GC Extractables
QLast Update : Wed Nov 08 10:47:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

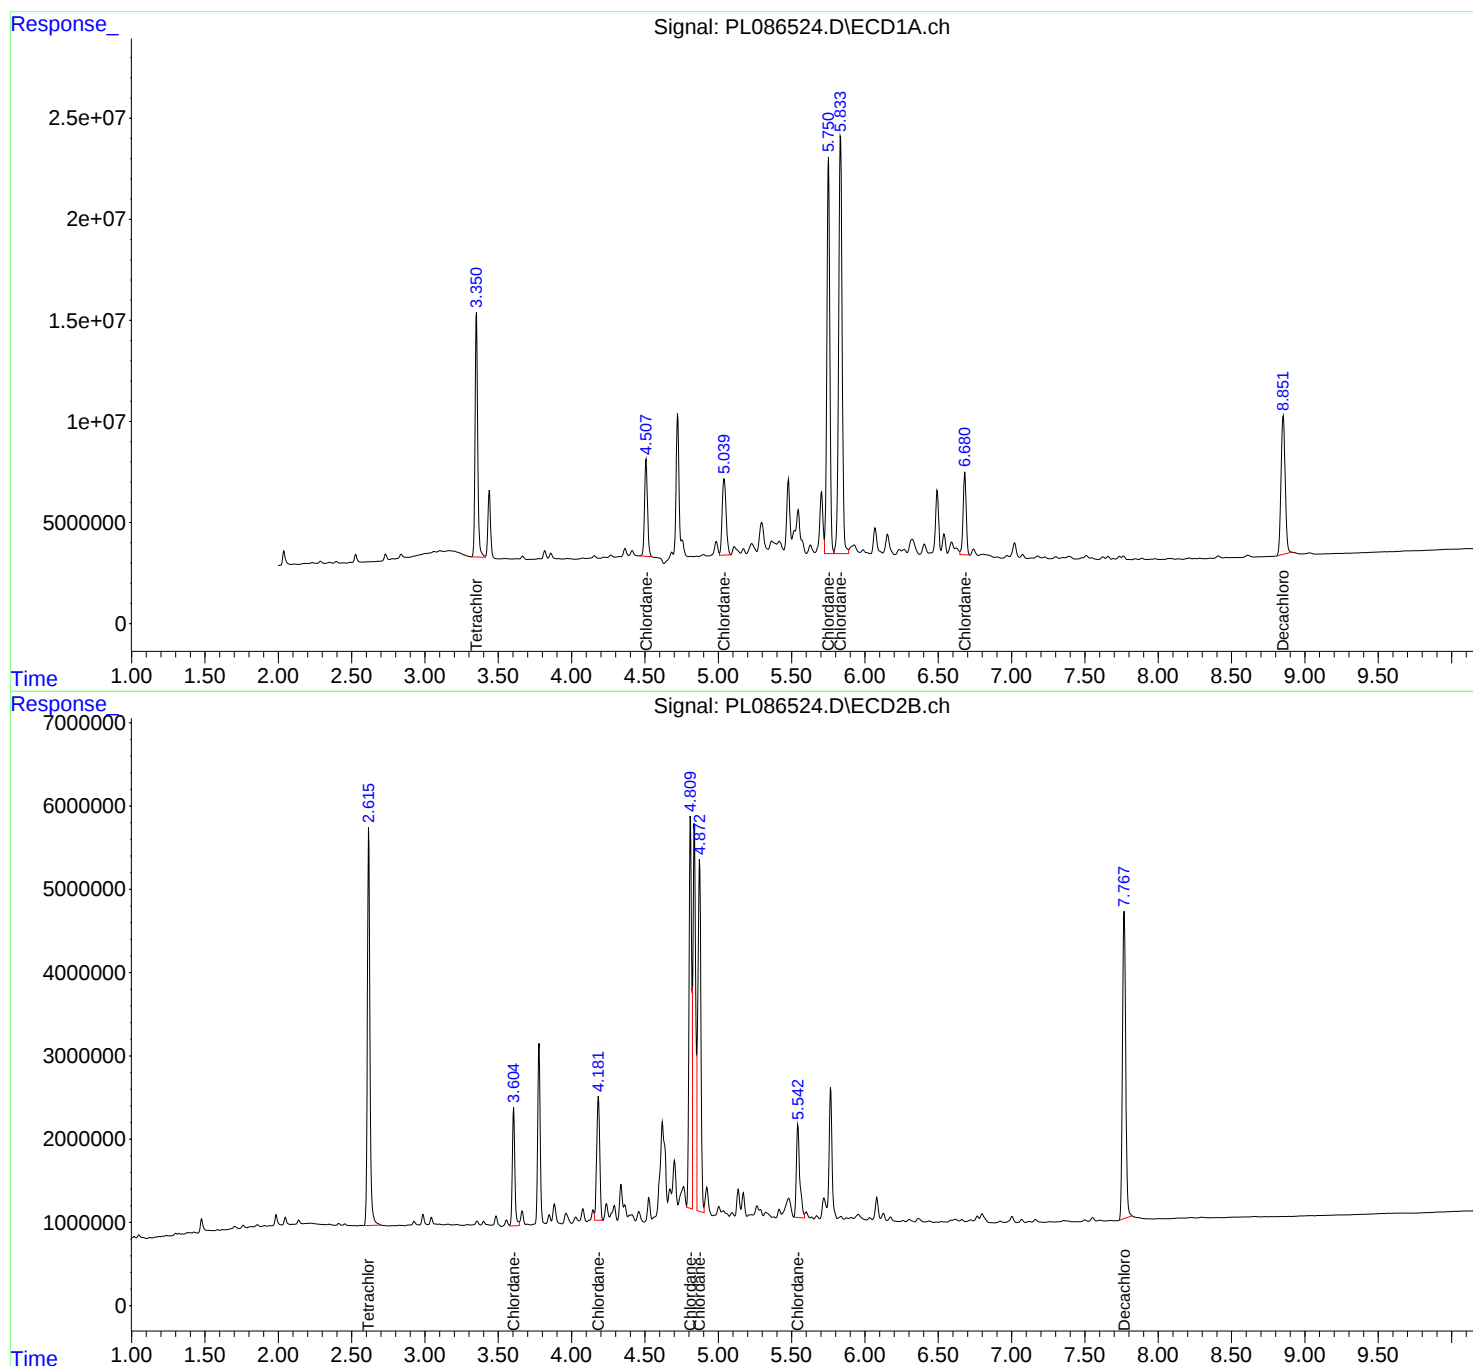


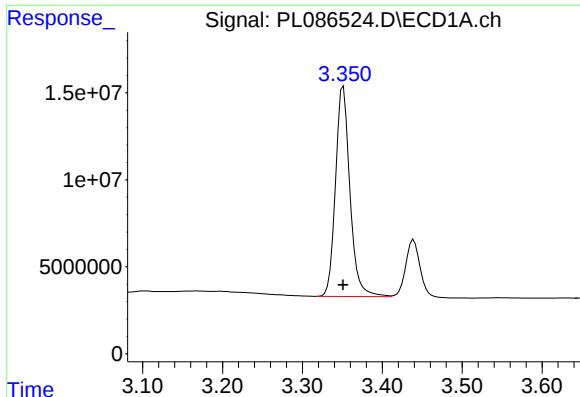

#1 Tetrachloro-m-xylene


R.T.: 3.351 min
Delta R.T.: 0.000 min
Response: 151576104
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

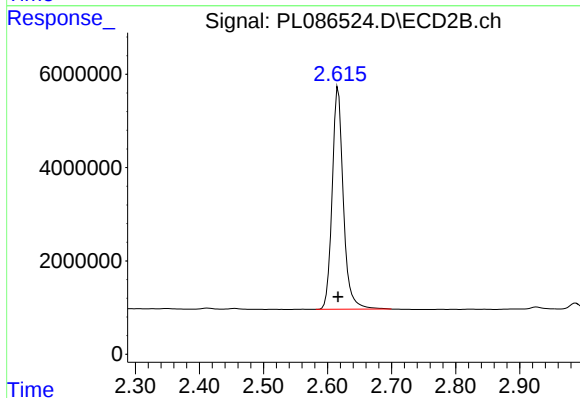


#1 Tetrachloro-m-xylene

R.T.: 2.617 min
Delta R.T.: 0.000 min
Response: 57730749
Conc: 50.00 ng/ml

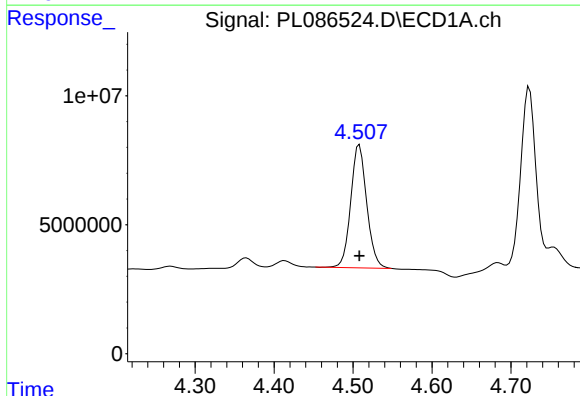


#23 Chlordane-1

R.T.: 4.508 min
Delta R.T.: 0.000 min
Response: 67207307
Conc: 500.00 ng/ml

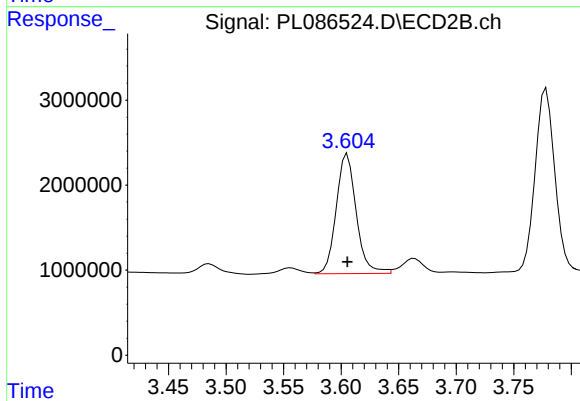

#23 Chlordane-1


R.T.: 3.605 min
Delta R.T.: 0.000 min
Response: 17073321
Conc: 500.00 ng/ml

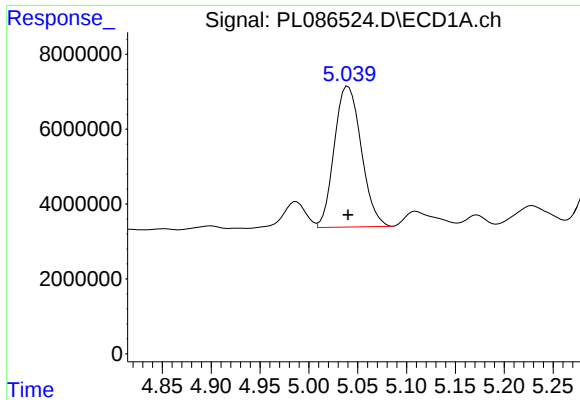

#24 Chlordane-2


R.T.: 5.040 min
Delta R.T.: 0.000 min
Response: 72253720
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

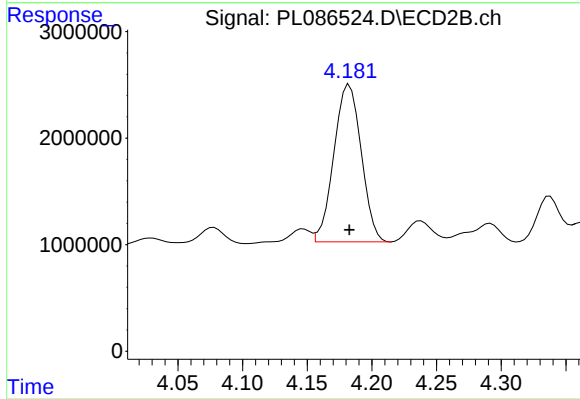


#24 Chlordane-2

R.T.: 4.183 min
Delta R.T.: 0.000 min
Response: 21734040
Conc: 500.00 ng/ml

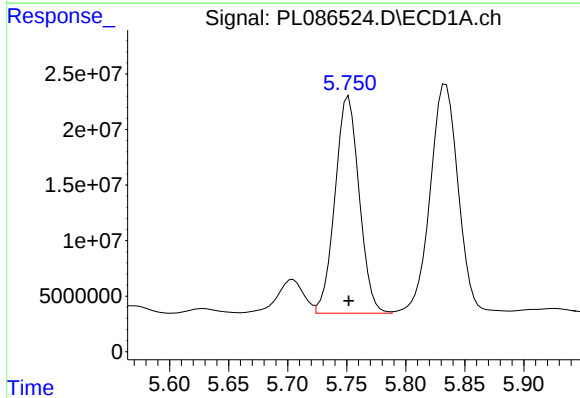


#25 Chlordane-3

R.T.: 5.752 min
Delta R.T.: 0.000 min
Response: 278352400
Conc: 500.00 ng/ml

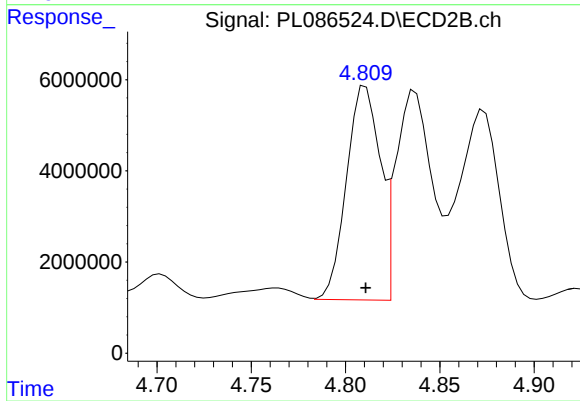

#25 Chlordane-3


R.T.: 4.811 min
Delta R.T.: 0.000 min
Response: 57982279
Conc: 500.00 ng/ml

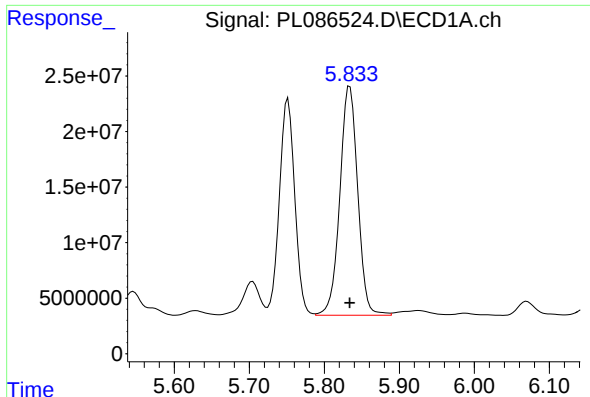

#26 Chlordane-4


R.T.: 5.834 min
Delta R.T.: 0.000 min
Response: 342175541
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

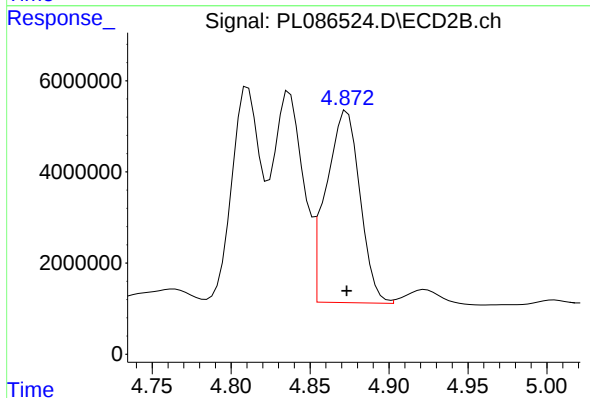


#26 Chlordane-4

R.T.: 4.873 min
Delta R.T.: 0.000 min
Response: 62580836
Conc: 500.00 ng/ml

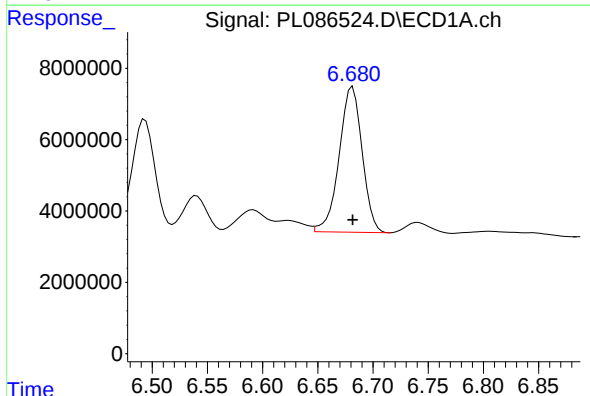


#27 Chlordane-5

R.T.: 6.682 min
Delta R.T.: 0.000 min
Response: 59170864
Conc: 500.00 ng/ml

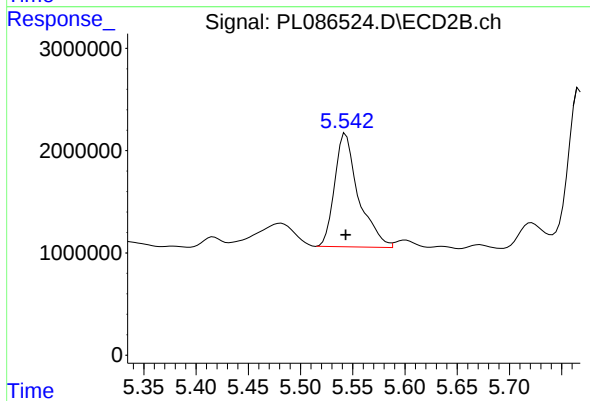

#27 Chlordane-5


R.T.: 5.543 min
Delta R.T.: 0.000 min
Response: 17595890
Conc: 500.00 ng/ml

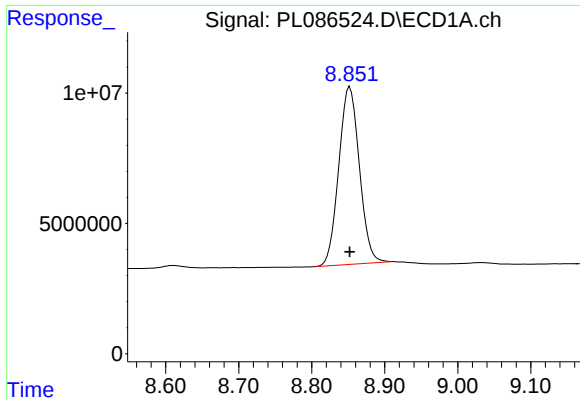

#28 Decachlorobiphenyl

R.T.: 8.852 min
Delta R.T.: 0.000 min
Response: 133712602
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

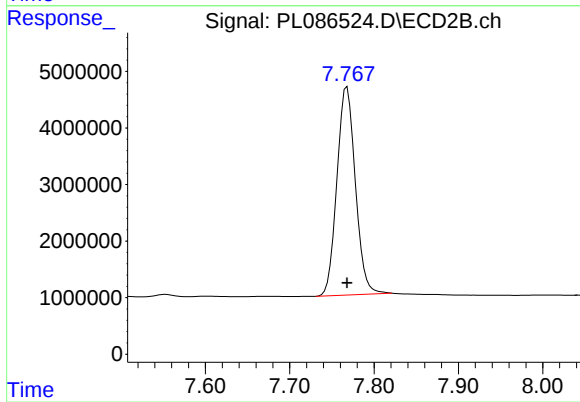

#28 Decachlorobiphenyl

R.T.: 7.768 min
Delta R.T.: 0.000 min
Response: 56052009
Conc: 50.00 ng/ml