

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110823\
 Data File : PL086525.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2023 10:45
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 10:59:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110823.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 08 10:47:46 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.351	2.616	78077303	28747926	25.171	24.523
28)	SA Decachlor...	8.851	7.766	72013316	29752537	26.528	26.248
Target Compounds							
23)	Chlordane-1	4.508	3.605	35301125	8633312	255.426	249.651
24)	Chlordane-2	5.039	4.182	38587053	11293004	262.880	258.510
25)	Chlordane-3	5.752	4.811	141.5E6	28031750	244.050	234.694
26)	Chlordane-4	5.834	4.873	176.9E6	30402496	248.914	236.537
27)	Chlordane-5	6.681	5.542	31656075	8862968	255.796	246.520



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110823\
Data File : PL086525.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2023 10:45
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 10:59:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110823.M
Quant Title : GC Extractables
QLast Update : Wed Nov 08 10:47:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

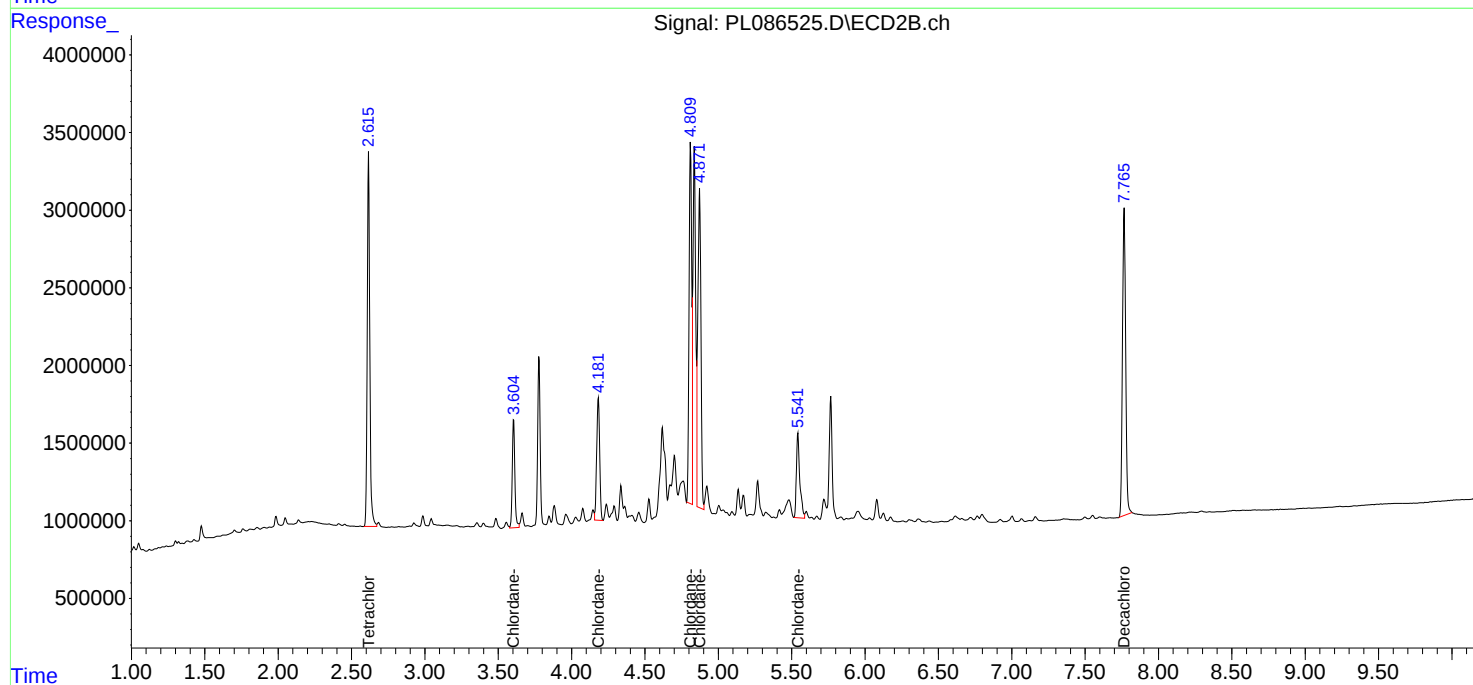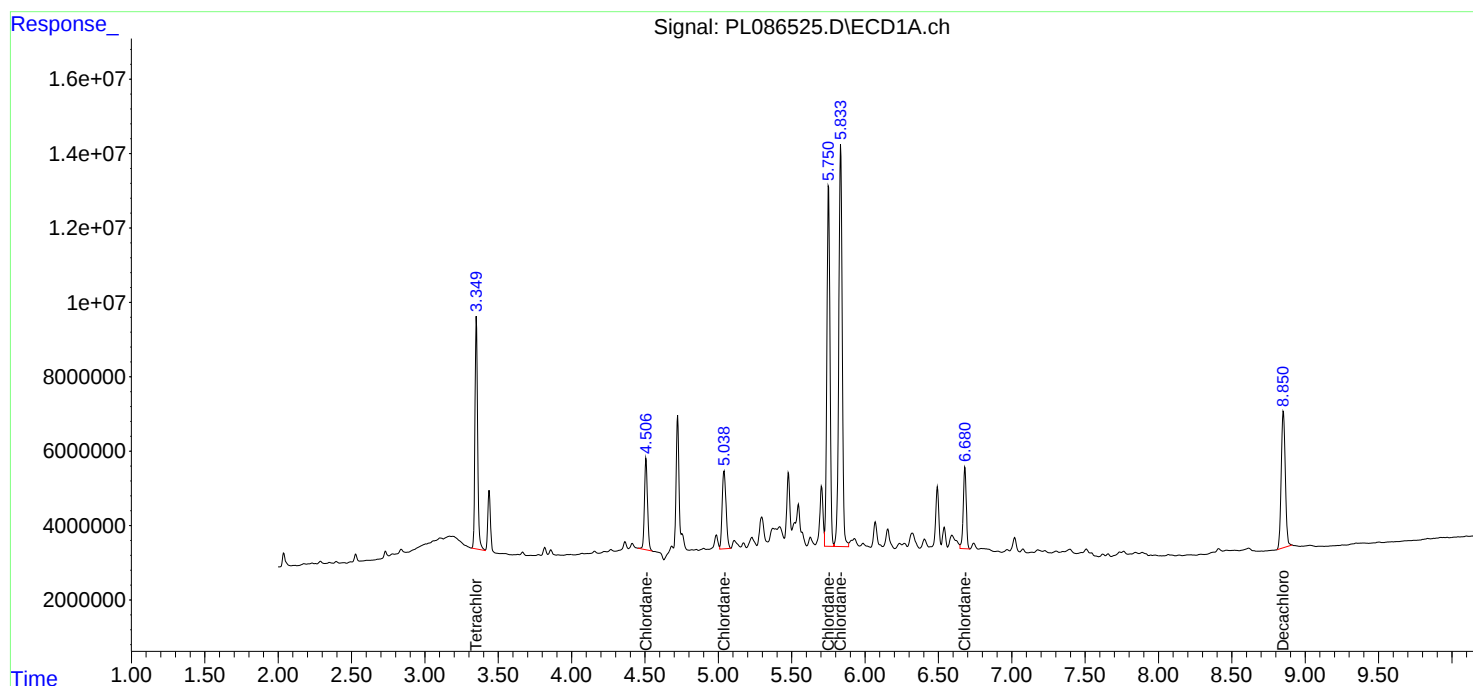


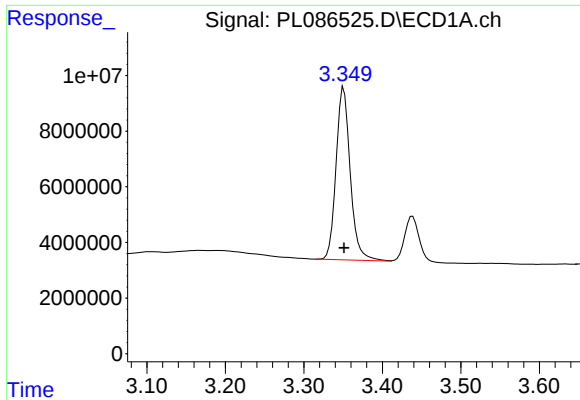

#1 Tetrachloro-m-xylene


R.T.: 3.351 min
Delta R.T.: 0.000 min
Response: 78077303
Conc: 25.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

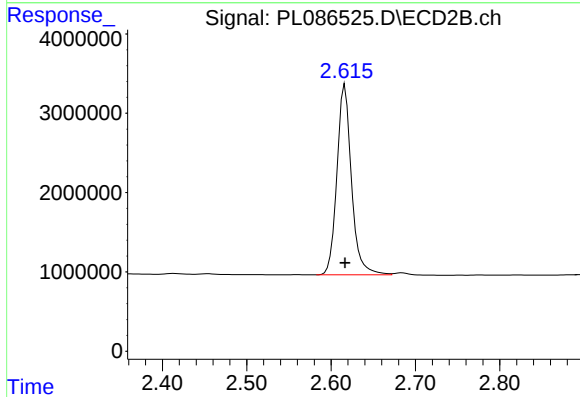


#1 Tetrachloro-m-xylene

R.T.: 2.616 min
Delta R.T.: 0.000 min
Response: 28747926
Conc: 24.52 ng/ml

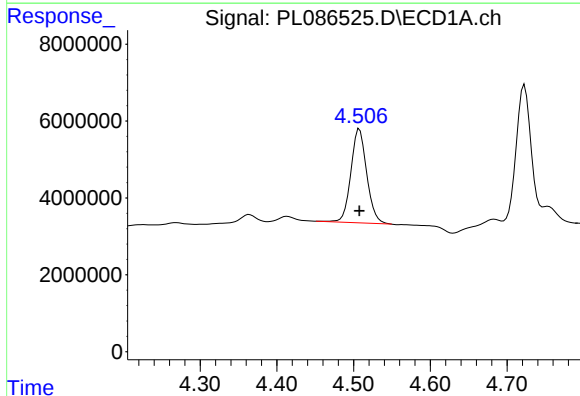


#23 Chlordane-1

R.T.: 4.508 min
Delta R.T.: 0.000 min
Response: 35301125
Conc: 255.43 ng/ml

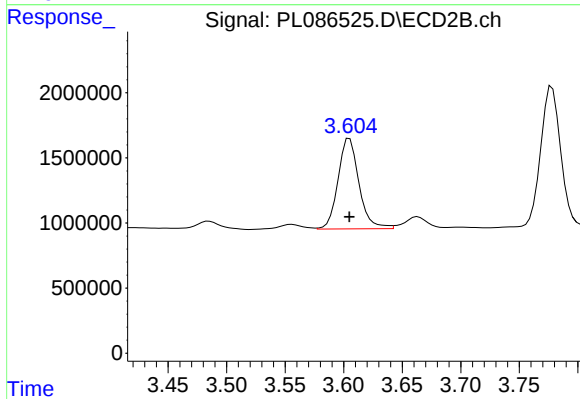

#23 Chlordane-1


R.T.: 3.605 min
Delta R.T.: 0.000 min
Response: 8633312
Conc: 249.65 ng/ml

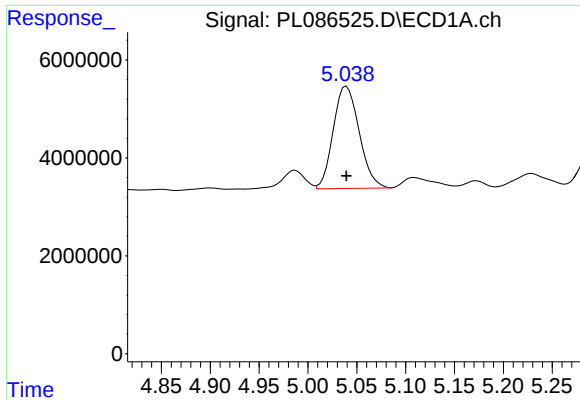

#24 Chlordane-2


R.T.: 5.039 min
Delta R.T.: 0.000 min
Response: 38587053
Conc: 262.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

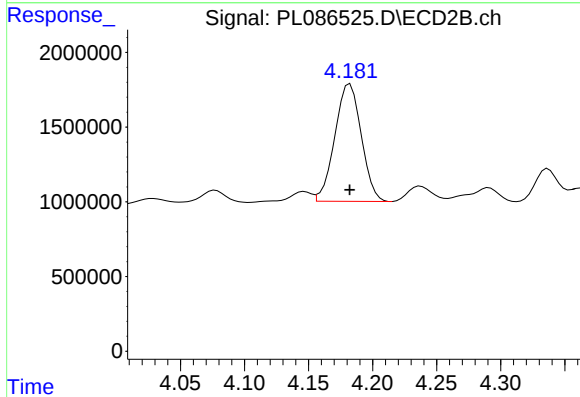


#24 Chlordane-2

R.T.: 4.182 min
Delta R.T.: 0.000 min
Response: 11293004
Conc: 258.51 ng/ml

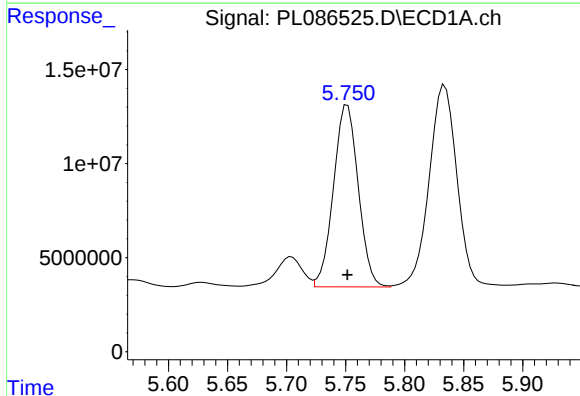


#25 Chlordane-3

R.T.: 5.752 min
Delta R.T.: 0.000 min
Response: 141499831
Conc: 244.05 ng/ml

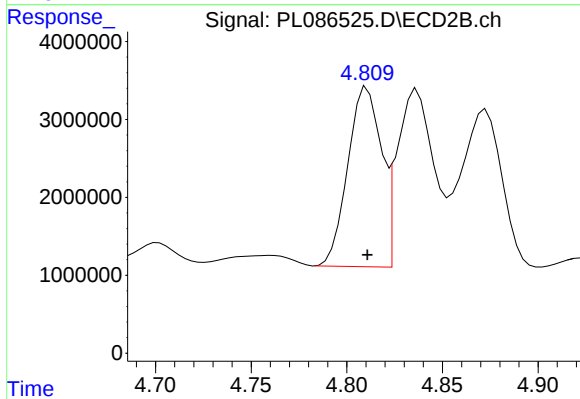

#25 Chlordane-3


R.T.: 4.811 min
Delta R.T.: 0.000 min
Response: 28031750
Conc: 234.69 ng/ml

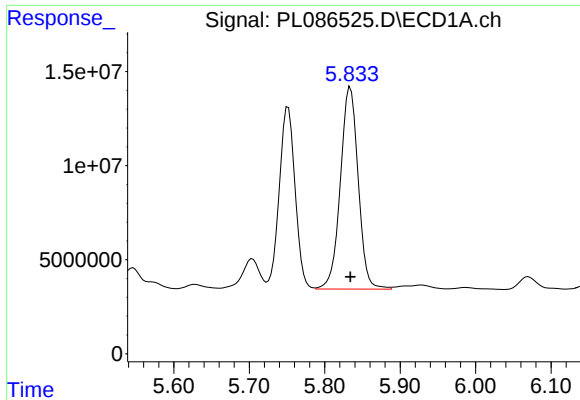

#26 Chlordane-4


R.T.: 5.834 min
Delta R.T.: 0.000 min
Response: 176887435
Conc: 248.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

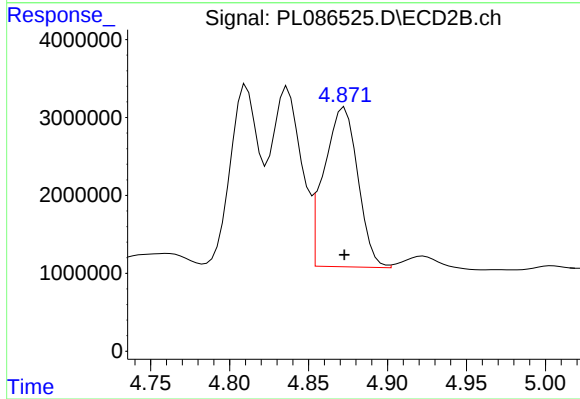


#26 Chlordane-4

R.T.: 4.873 min
Delta R.T.: 0.000 min
Response: 30402496
Conc: 236.54 ng/ml

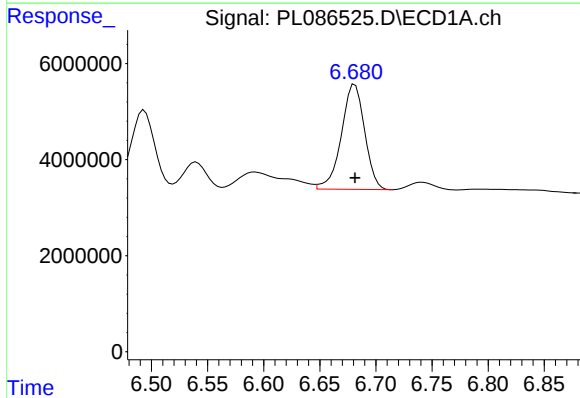


#27 Chlordane-5

R.T.: 6.681 min
Delta R.T.: 0.000 min
Response: 31656075
Conc: 255.80 ng/ml

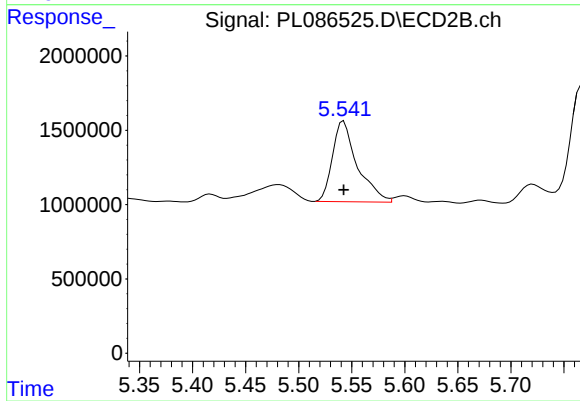

#27 Chlordane-5


R.T.: 5.542 min
Delta R.T.: 0.000 min
Response: 8862968
Conc: 246.52 ng/ml

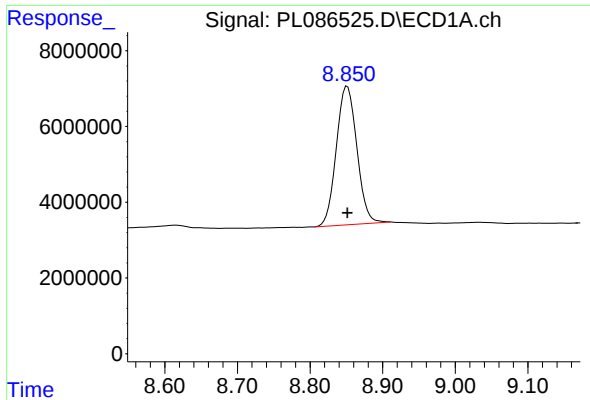

#28 Decachlorobiphenyl

R.T.: 8.851 min
Delta R.T.: 0.000 min
Response: 72013316
Conc: 26.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

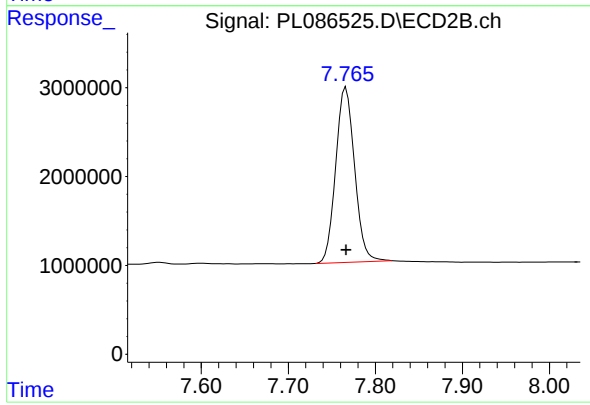

#28 Decachlorobiphenyl

R.T.: 7.766 min
Delta R.T.: 0.000 min
Response: 29752537
Conc: 26.25 ng/ml