

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110824\
 Data File : PL092938.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2024 17:36
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 22:25:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.779	54480374	60226829	22.235	22.133
28)	SA Decachlor...	9.061	7.919	39168296	52921969	20.352	19.391
Target Compounds							
2)	A alpha-BHC	0.000	3.269	0	181286	N.D.	0.045 #
3)	MA gamma-BHC...	0.000	3.617	0	19087	N.D.	0.005 #
4)	MA Heptachlor	0.000	3.969f	0	74294	N.D.	0.020 #
6)	B beta-BHC	0.000	3.920	0	60177	N.D.	0.037 #
7)	B delta-BHC	4.765	4.137	2623589	196906	0.838	0.051 #
8)	B Heptachlo...	0.000	4.716f	0	27274	N.D.	0.008 #
10)	B gamma-Chl...	0.000	4.968	0	49930	N.D.	0.015 #
17)	MA 4,4'-DDT	0.000	6.040	0	2088030	N.D.	0.778 #
20)	A Methoxychlor	0.000	6.616	0	3421173	N.D.	2.396 #
22)	Mirex	0.000	7.049f	0	12852	N.D.	0.005 #
23)	Chlordane-1	0.000	3.770	0	142763	N.D.	1.345 #
25)	Chlordane-3	0.000	4.968	0	49930	N.D.	0.138 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110824\
Data File : PL092938.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2024 17:36
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 22:25:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

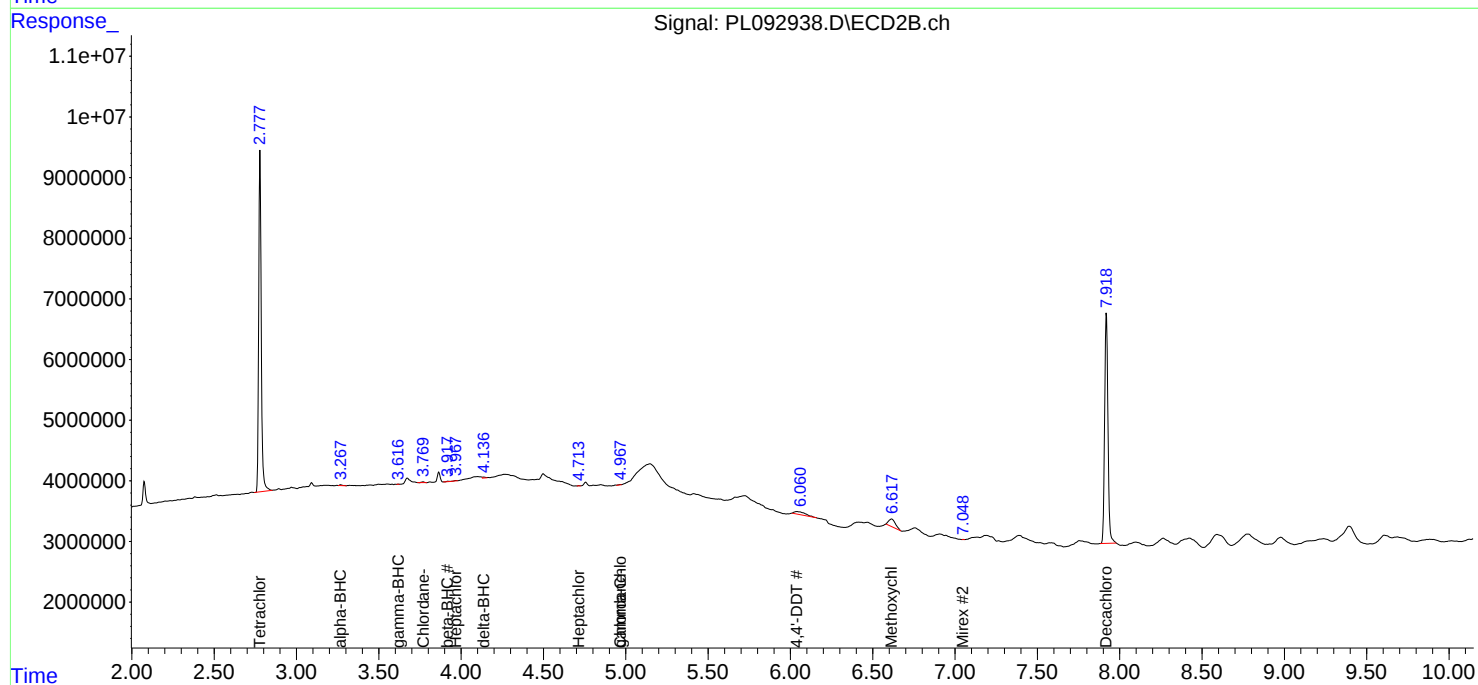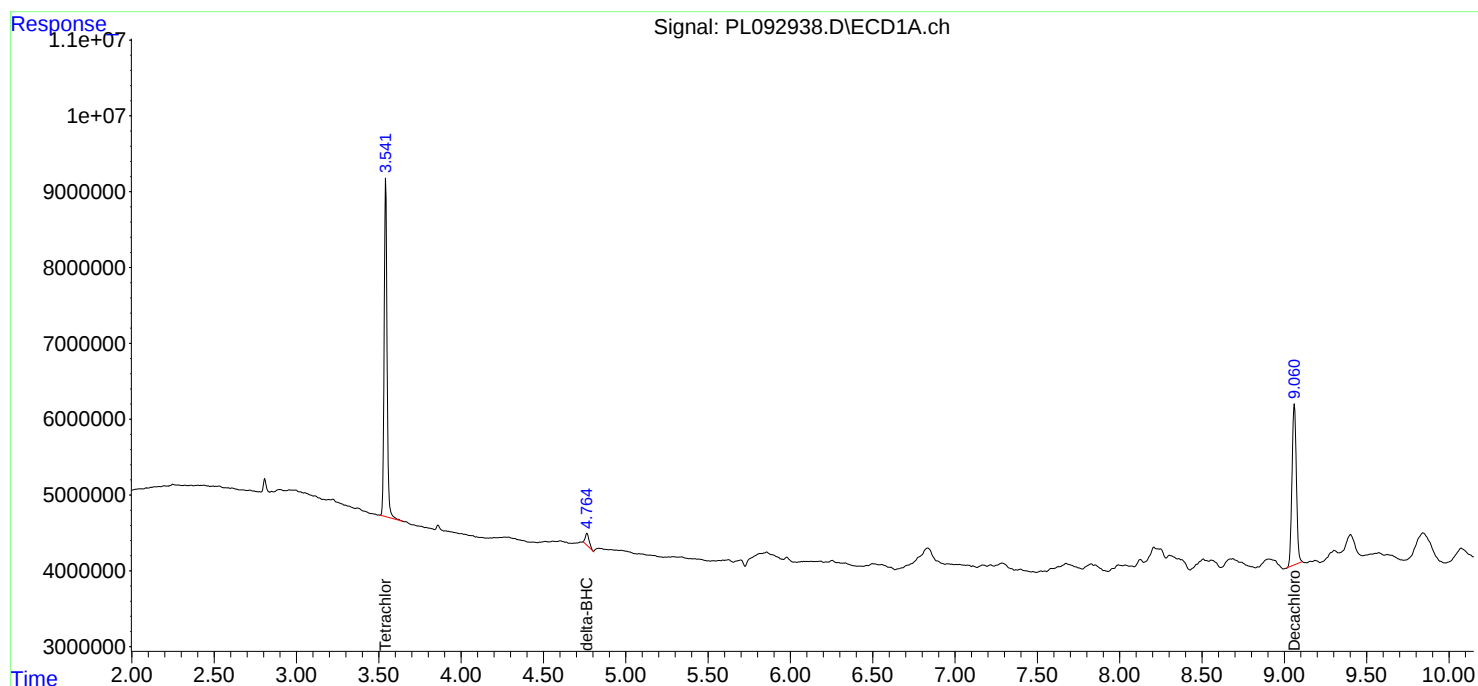


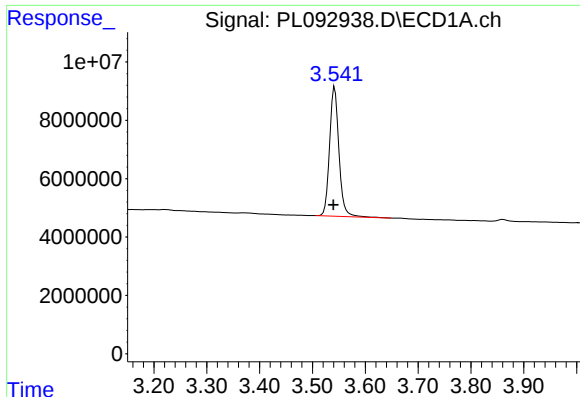

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: 0.002 min
Response: 54480374
Conc: 22.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

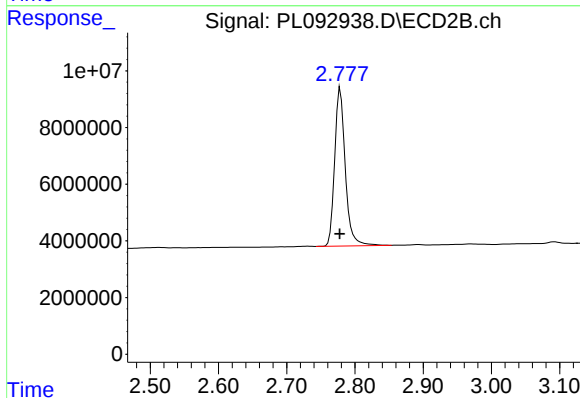


#1 Tetrachloro-m-xylene

R.T.: 2.779 min
Delta R.T.: 0.000 min
Response: 60226829
Conc: 22.13 ng/ml

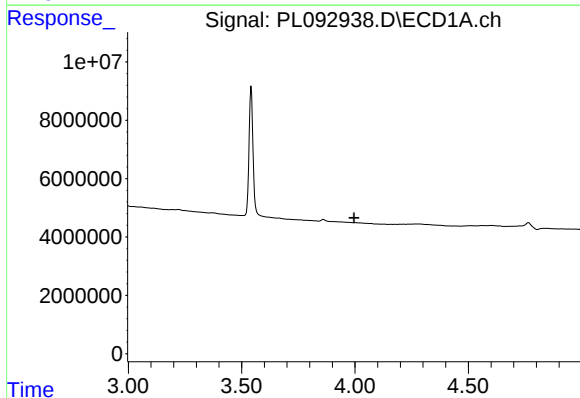


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.996 min
Response: 0
Conc: N.D.

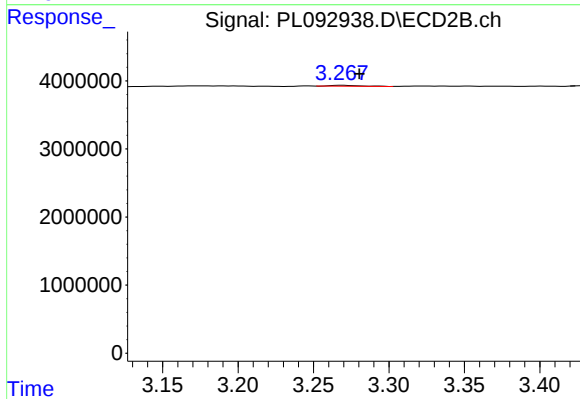

#2 alpha-BHC


R.T.: 3.269 min
Delta R.T.: -0.012 min
Response: 181286
Conc: 0.05 ng/ml

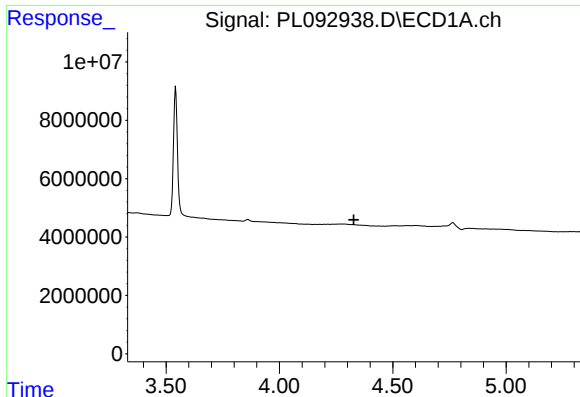

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

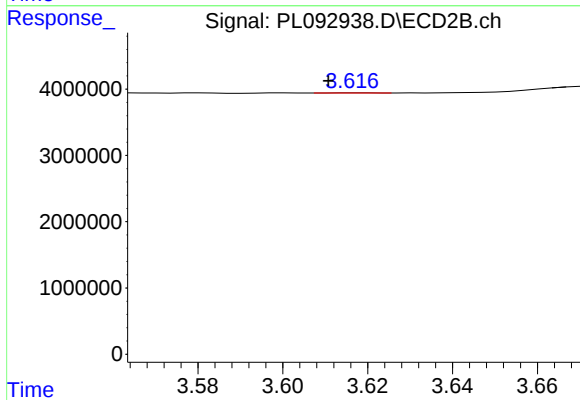


#3 gamma-BHC (Lindane)

R.T.: 3.617 min
Delta R.T.: 0.007 min
Response: 19087
Conc: 0.00 ng/ml

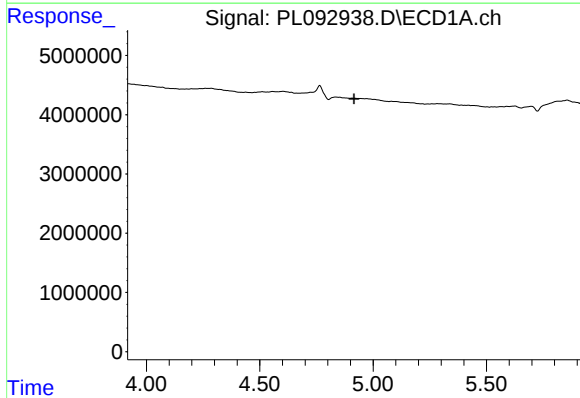


#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 4.917 min
Response: 0
Conc: N.D.

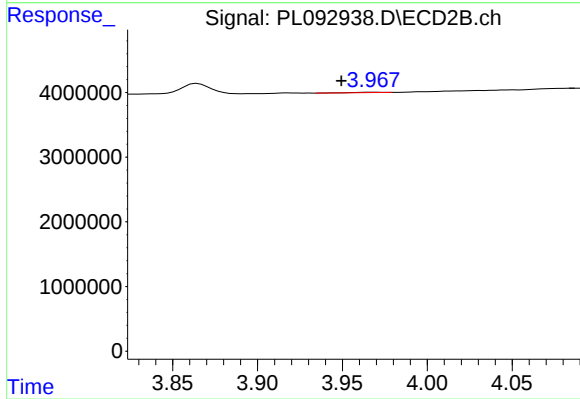

#4 Heptachlor


R.T.: 3.969 min
Delta R.T.: 0.019 min
Response: 74294
Conc: 0.02 ng/ml

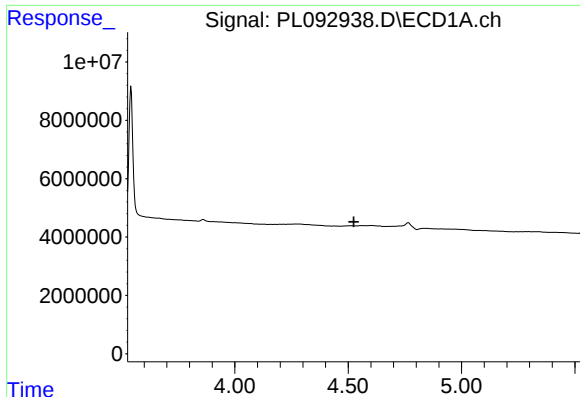

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.525 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

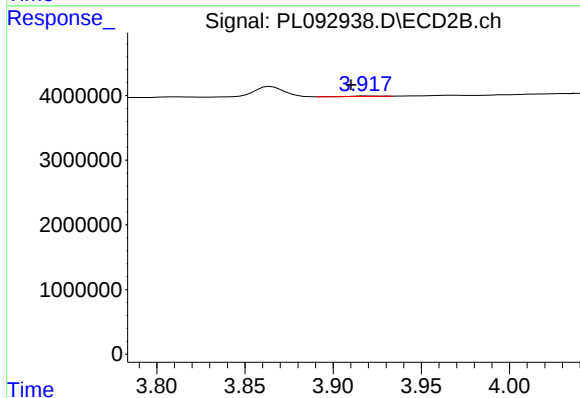


#6 beta-BHC

R.T.: 3.920 min
Delta R.T.: 0.010 min
Response: 60177
Conc: 0.04 ng/ml

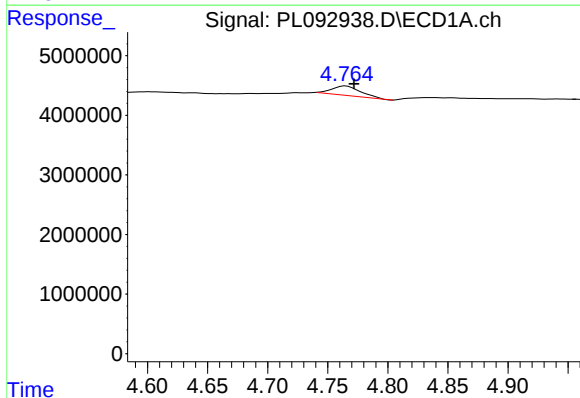


#7 delta-BHC

R.T.: 4.765 min
Delta R.T.: -0.007 min
Response: 2623589
Conc: 0.84 ng/ml

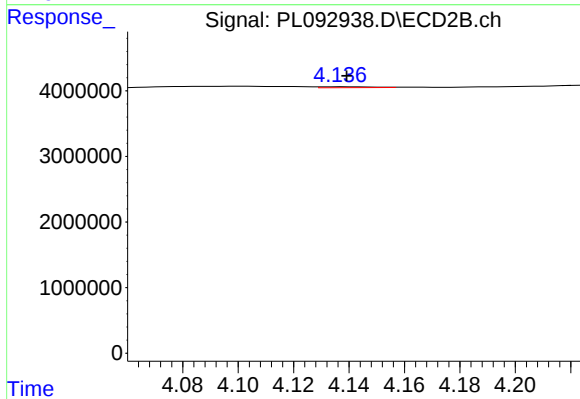

#7 delta-BHC


R.T.: 4.137 min
Delta R.T.: -0.003 min
Response: 196906
Conc: 0.05 ng/ml

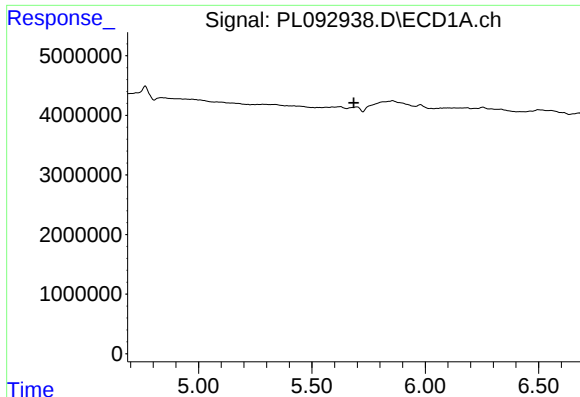

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.684 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

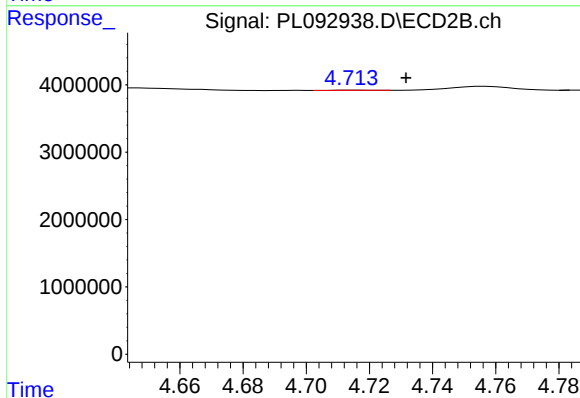


#8 Heptachlor epoxide

R.T.: 4.716 min
Delta R.T.: -0.016 min
Response: 27274
Conc: 0.01 ng/ml

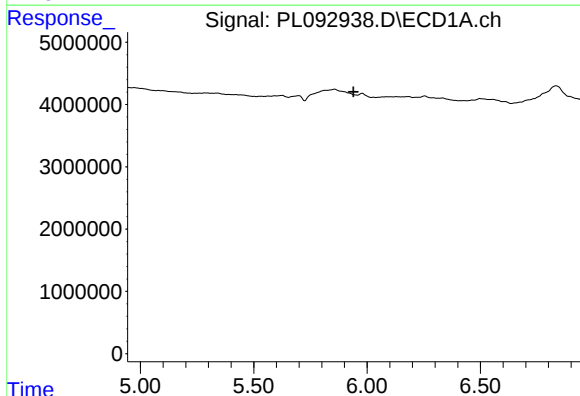


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.941 min
Response: 0
Conc: N.D.

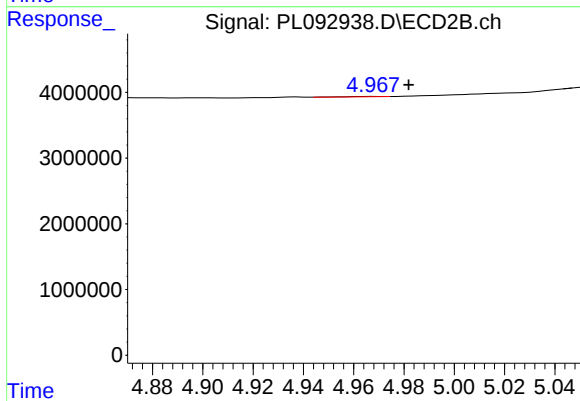

#10 gamma-Chlordane


R.T.: 4.968 min
Delta R.T.: -0.014 min
Response: 49930
Conc: 0.01 ng/ml

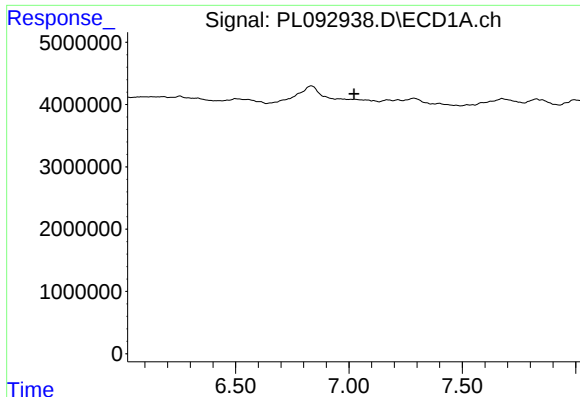

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.023 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

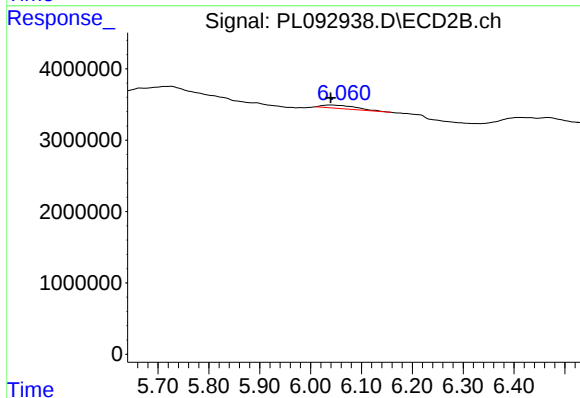


#17 4,4'-DDT

R.T.: 6.040 min
Delta R.T.: 0.000 min
Response: 2088030
Conc: 0.78 ng/ml

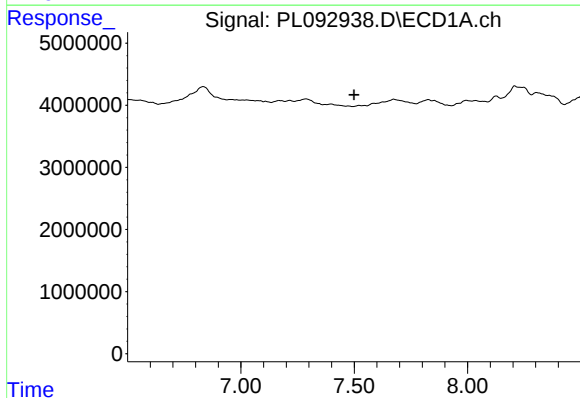


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.499 min
Response: 0
Conc: N.D.

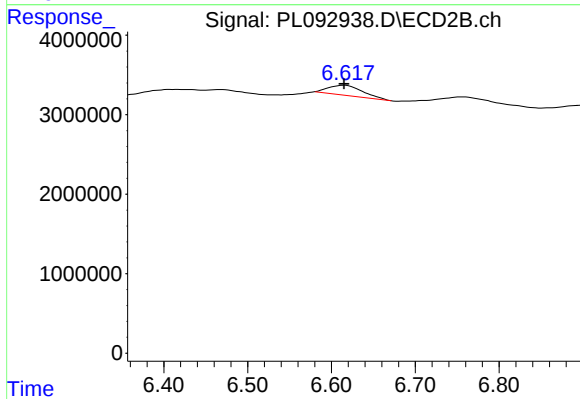

#20 Methoxychlor


R.T.: 6.616 min
Delta R.T.: 0.000 min
Response: 3421173
Conc: 2.40 ng/ml

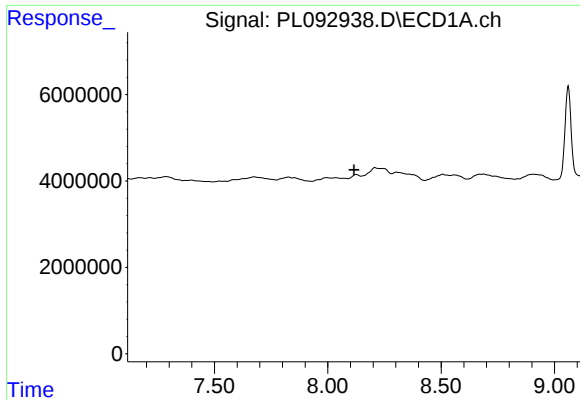

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 8.116 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

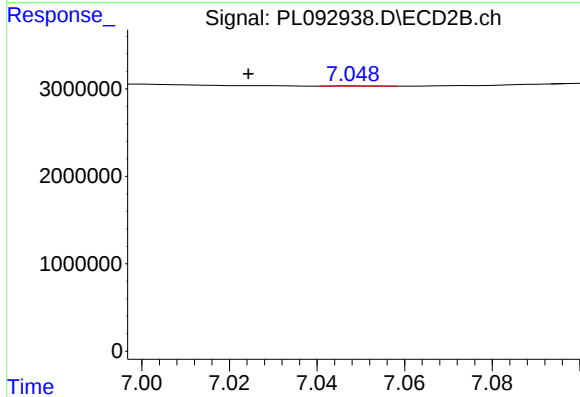


#22 Mirex

R.T.: 7.049 min
Delta R.T.: 0.025 min
Response: 12852
Conc: 0.00 ng/ml

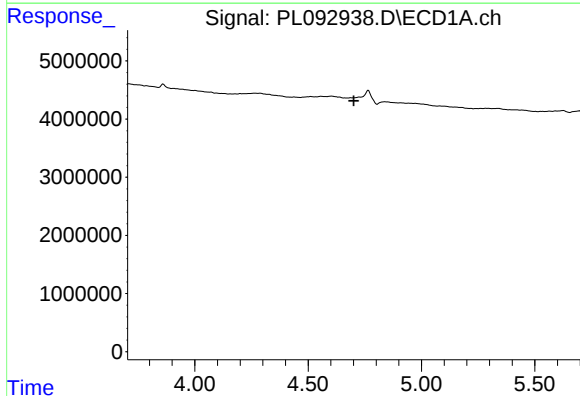


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.702 min
Response: 0
Conc: N.D.

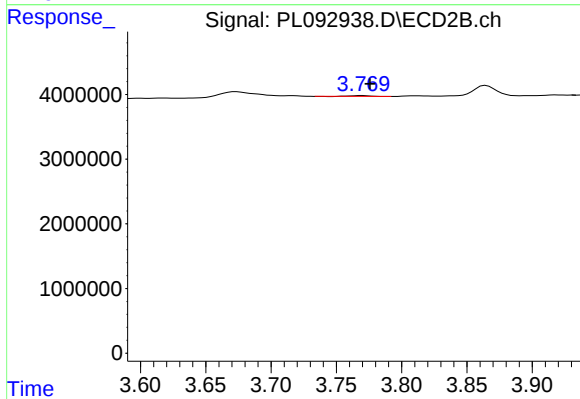

#23 Chlordane-1


R.T.: 3.770 min
Delta R.T.: -0.006 min
Response: 142763
Conc: 1.34 ng/ml

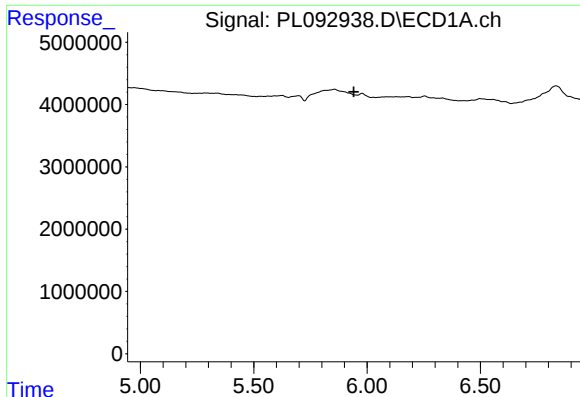

#25 Chlorodane-3


R.T.: 0.000 min
Exp R.T.: 5.941 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

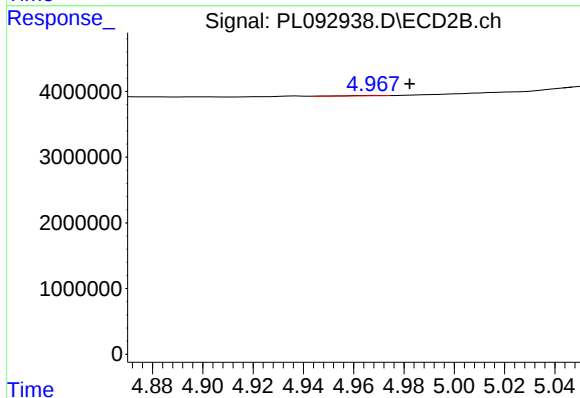


#25 Chlorodane-3

R.T.: 4.968 min
Delta R.T.: -0.014 min
Response: 49930
Conc: 0.14 ng/ml

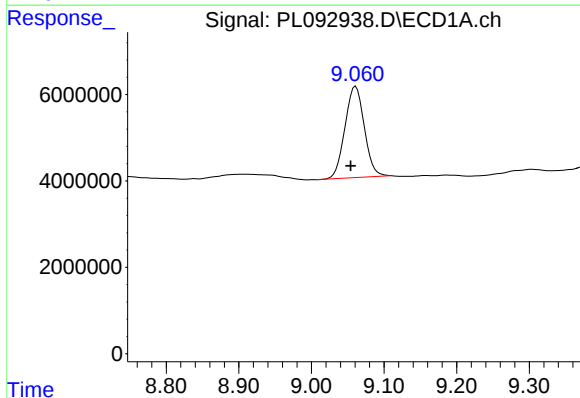

#28 Decachlorobiphenyl

R.T.: 9.061 min
Delta R.T.: 0.007 min
Response: 39168296
Conc: 20.35 ng/ml

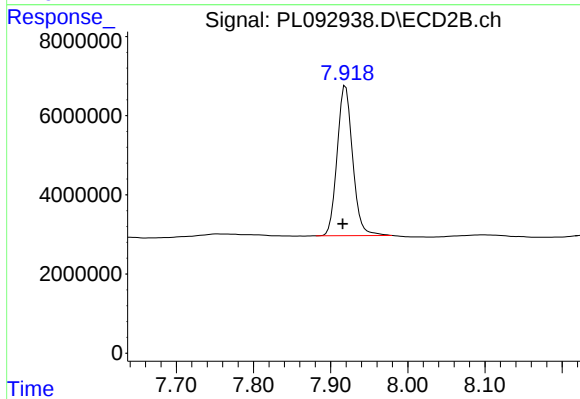

#28 Decachlorobiphenyl

R.T.: 7.919 min
Delta R.T.: 0.004 min
Response: 52921969
Conc: 19.39 ng/ml