

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110824\
 Data File : PL092933.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2024 16:26
 Operator : AR\AJ
 Sample : P4768-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 B-5

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/11/2024
 Supervised By : Ankita Jodhani 11/11/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 22:21:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.778	46279973	48347487	18.888	17.767m
28)	SA Decachlor...	9.062	7.921	26409335	34519168	13.722m	12.648

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110824\
Data File : PL092933.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2024 16:26
Operator : AR\AJ
Sample : P4768-05
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
B-5


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/11/2024
Supervised By : Ankita Jodhani 11/11/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 22:21:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

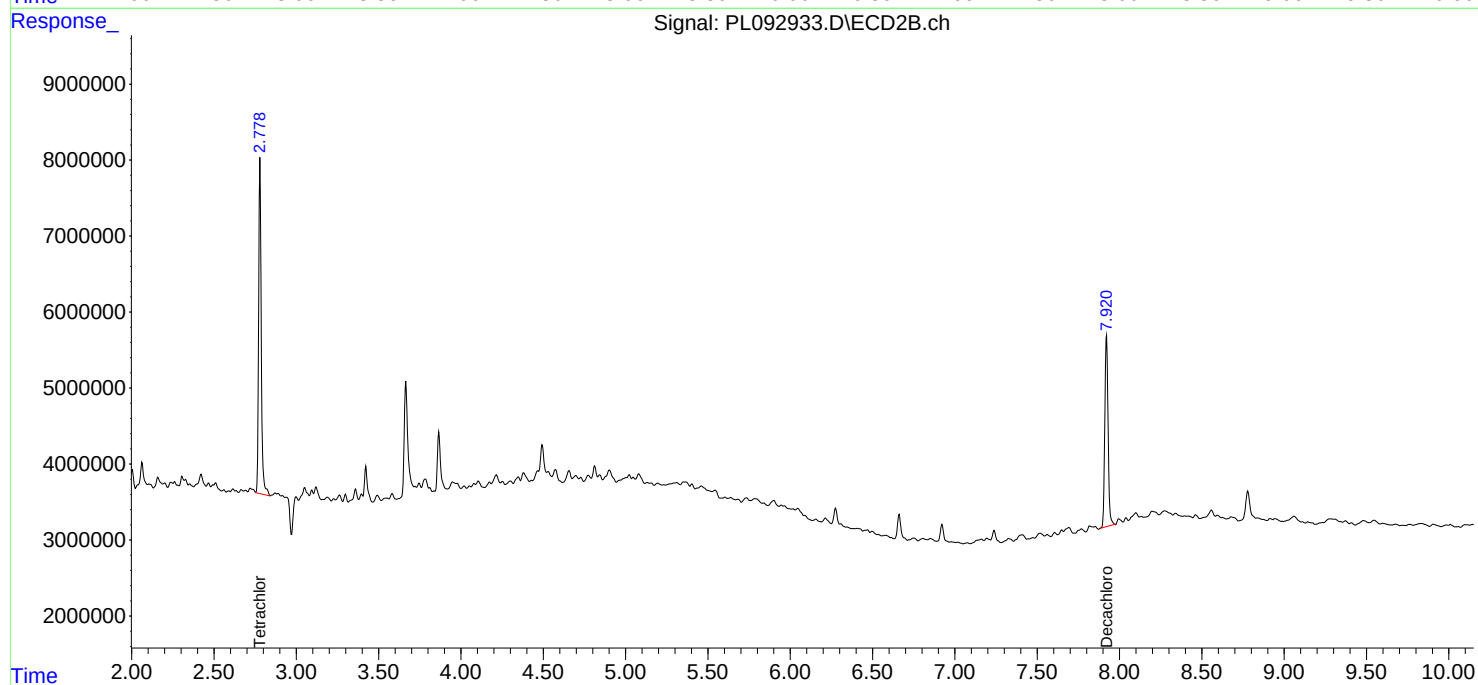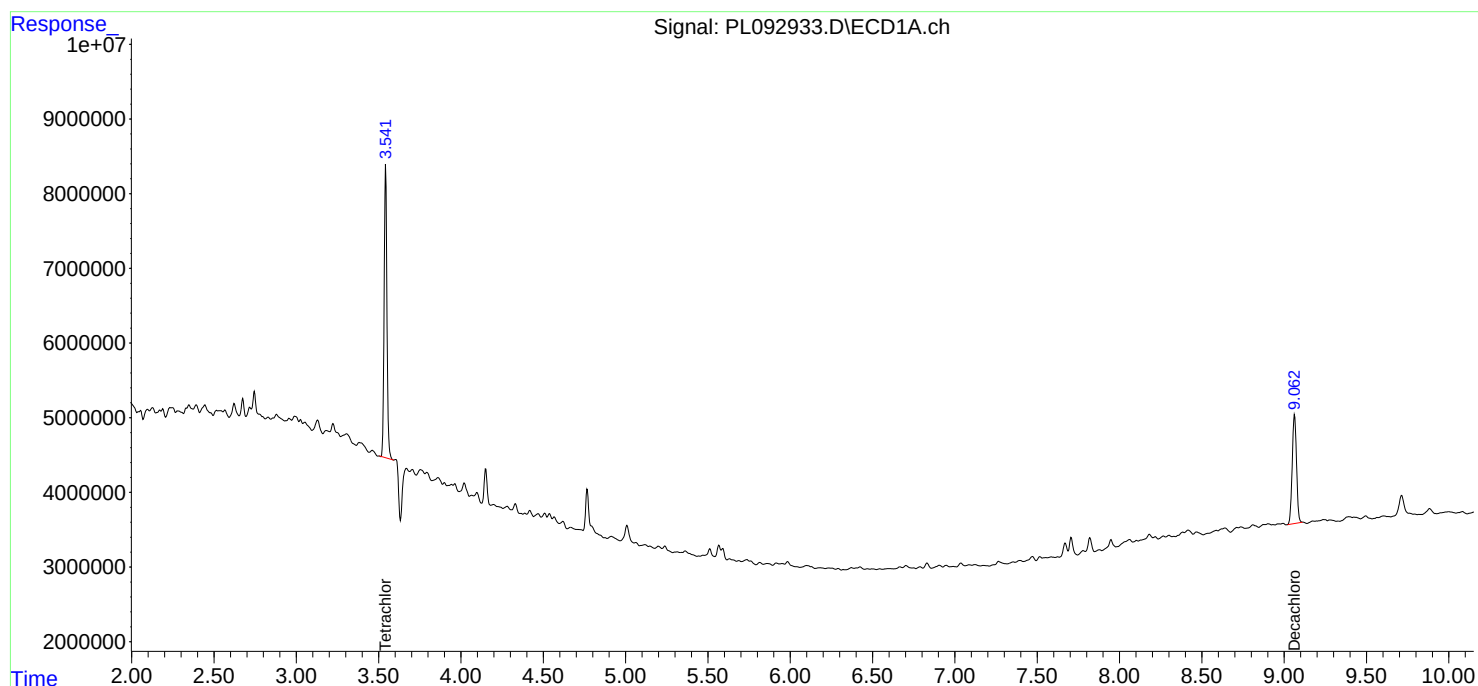

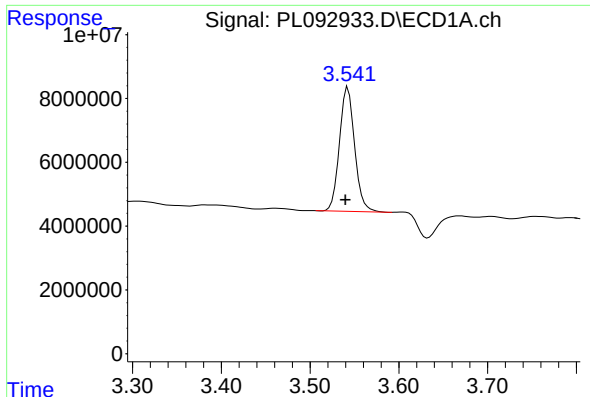


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: 0.003 min
Response: 46279973
Conc: 18.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
B-5


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/11/2024
Supervised By :Ankita Jodhani 11/11/2024

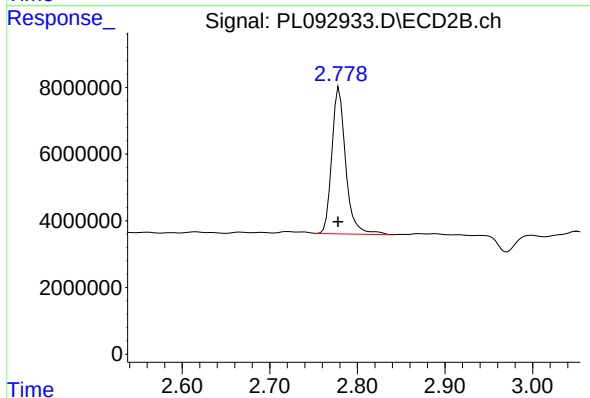


#1 Tetrachloro-m-xylene

R.T.: 2.778 min
Delta R.T.: 0.000 min
Response: 48347487
Conc: 17.77 ng/ml m

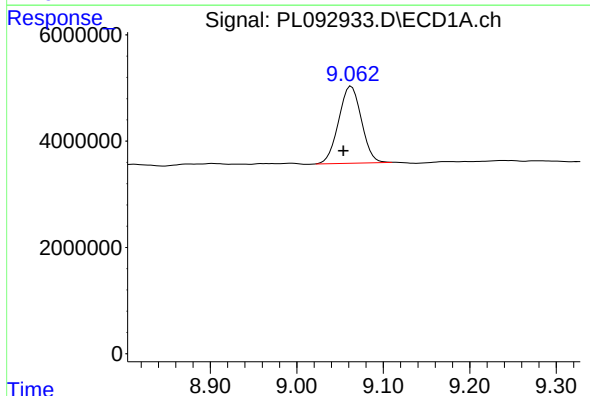

#28 Decachlorobiphenyl

R.T.: 9.062 min
Delta R.T.: 0.008 min
Response: 26409335
Conc: 13.72 ng/ml m

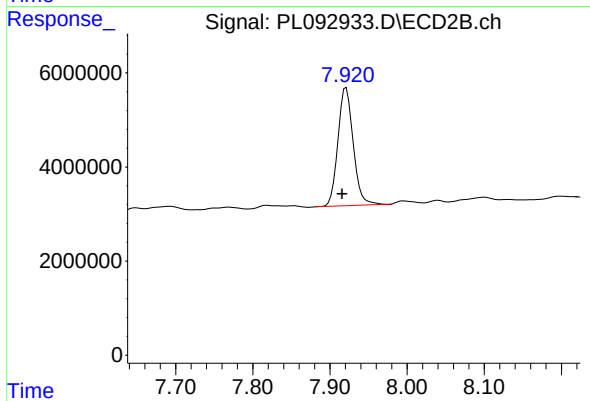

#28 Decachlorobiphenyl

R.T.: 7.921 min
Delta R.T.: 0.005 min
Response: 34519168
Conc: 12.65 ng/ml