

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110918\
 Data File : PL041959.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2018 11:13
 Operator : AJ\SJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 11:55:29 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 11:54:49 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	4.102	645.3E6	293.3E6	97.809	95.898
28)	SA Decachlor...	8.209	9.231	636.0E6	244.1E6	94.327	95.599
Target Compounds							
23)	Chlordane-1	4.337	5.112	294.9E6	144.4E6	991.413	980.426
24)	Chlordane-2	4.837	5.583	298.4E6	138.3E6	944.807	954.497
25)	Chlordane-3	5.404	6.233	945.7E6	501.7E6	993.802	980.338
26)	Chlordane-4	5.461	6.308	839.4E6	580.7E6	992.705	973.652
27)	Chlordane-5	6.296	7.118	264.4E6	116.2E6	1001.681	1013.047



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110918\
Data File : PL041959.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2018 11:13
Operator : AJ\SJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 11:55:29 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 11:54:49 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

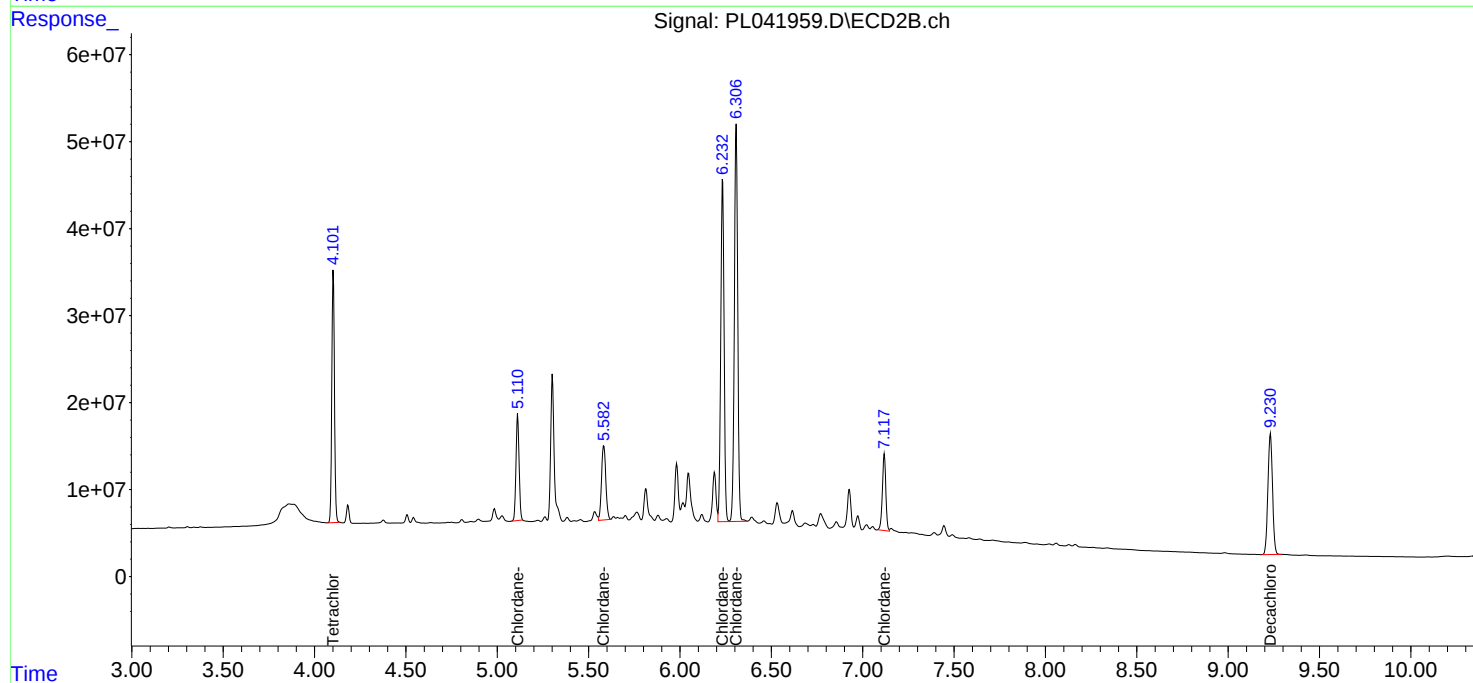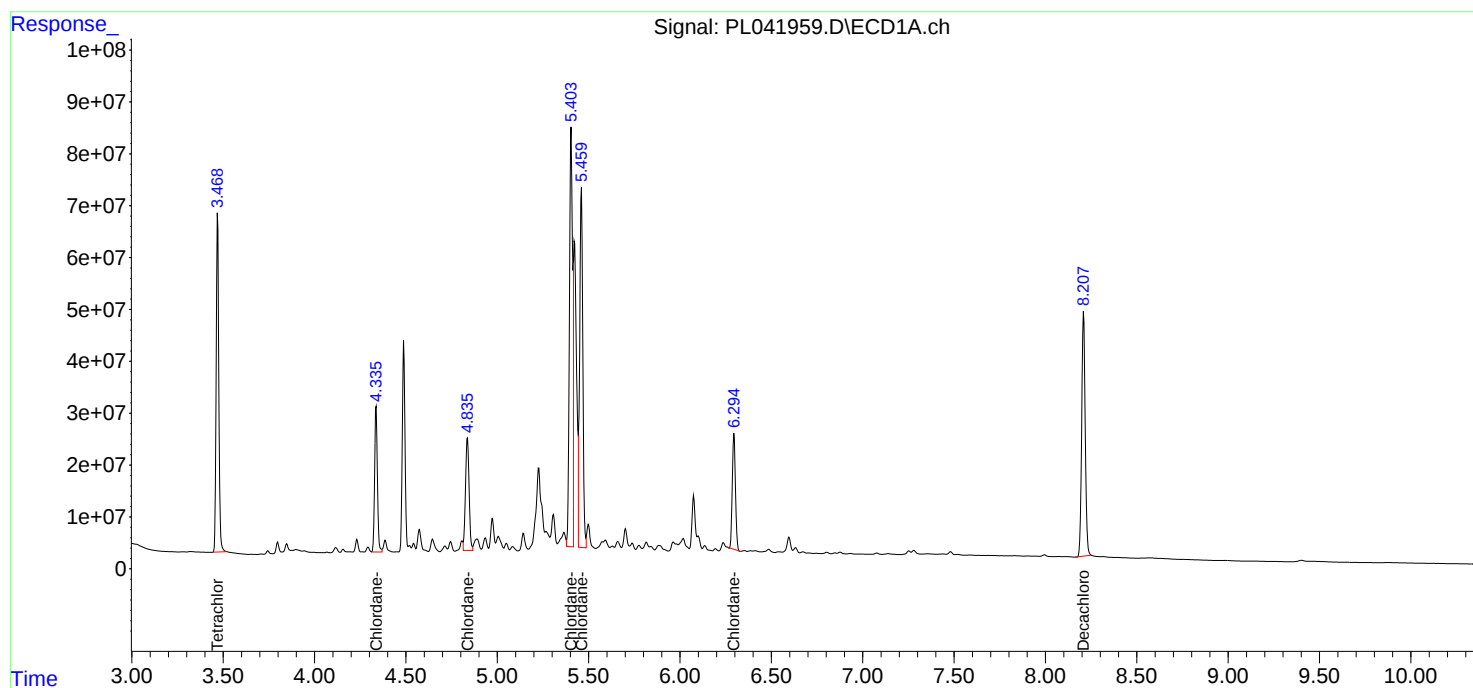


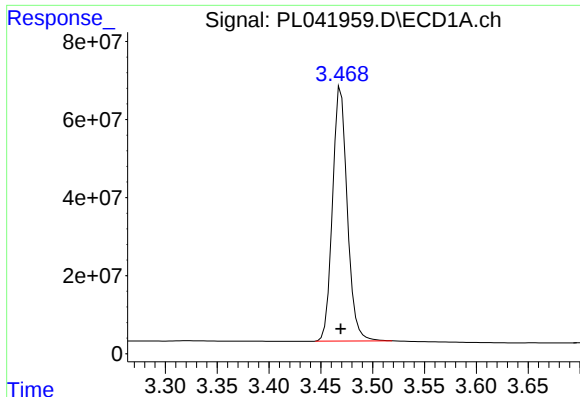

#1 Tetrachloro-m-xylene


R.T.: 3.469 min
Delta R.T.: 0.000 min
Response: 645338224
Conc: 97.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

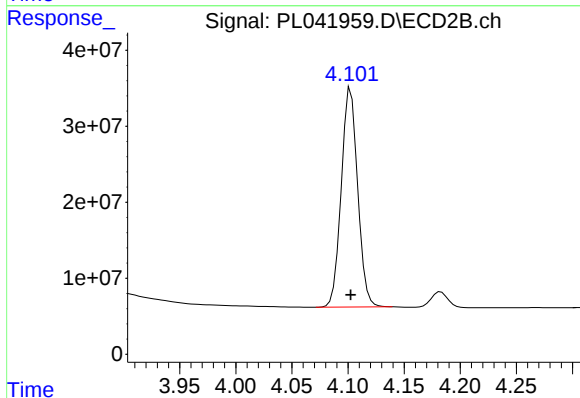


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 293281028
Conc: 95.90 ng/ml

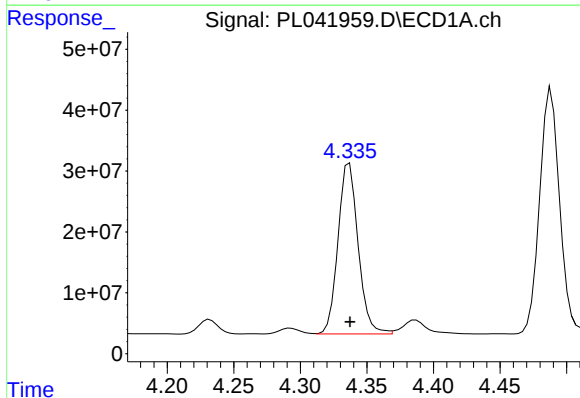


#23 Chlordane-1

R.T.: 4.337 min
Delta R.T.: 0.000 min
Response: 294943722
Conc: 991.41 ng/ml

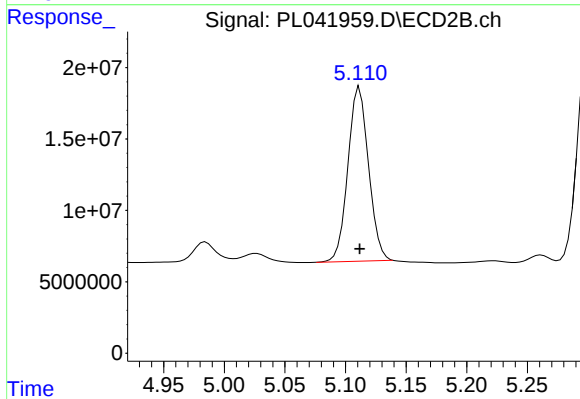

#23 Chlordane-1


R.T.: 5.112 min
Delta R.T.: 0.000 min
Response: 144357701
Conc: 980.43 ng/ml

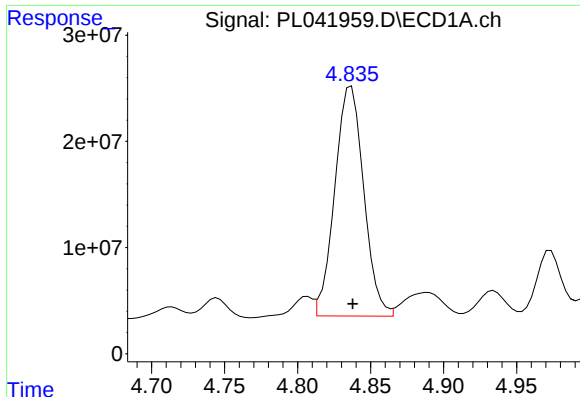

#24 Chlordane-2


R.T.: 4.837 min
Delta R.T.: 0.000 min
Response: 298350001
Conc: 944.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

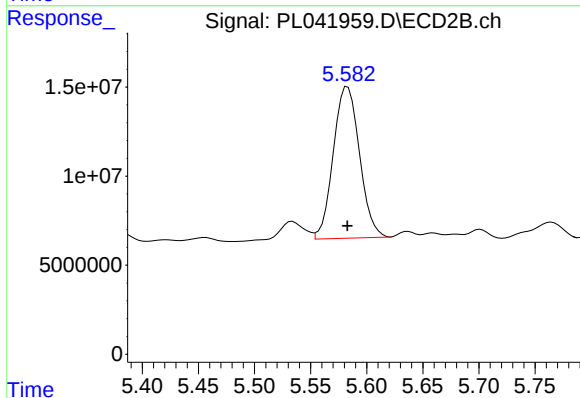


#24 Chlordane-2

R.T.: 5.583 min
Delta R.T.: 0.000 min
Response: 138329850
Conc: 954.50 ng/ml

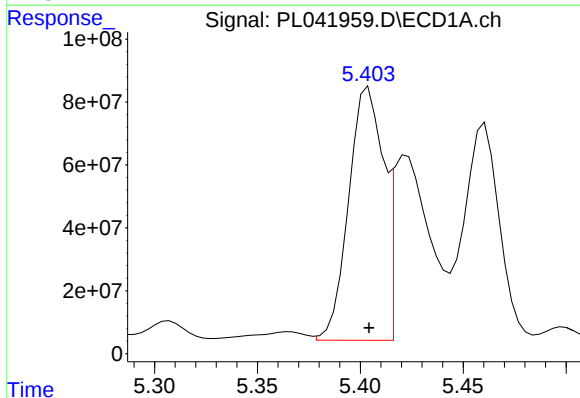


#25 Chlordane-3

R.T.: 5.404 min
Delta R.T.: 0.000 min
Response: 945738223
Conc: 993.80 ng/ml

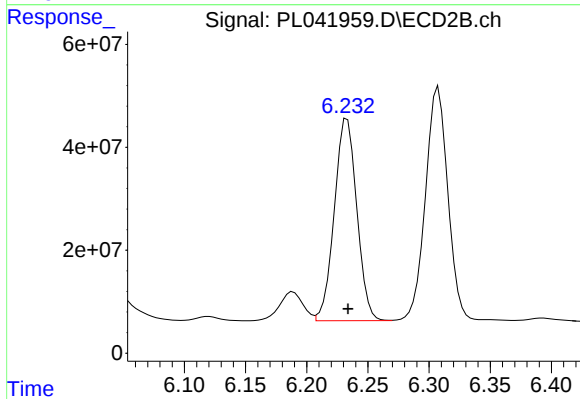

#25 Chlordane-3


R.T.: 6.233 min
Delta R.T.: 0.000 min
Response: 501735742
Conc: 980.34 ng/ml

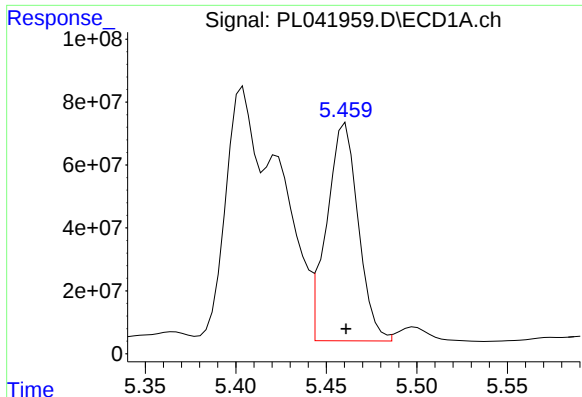

#26 Chlordane-4


R.T.: 5.461 min
Delta R.T.: 0.000 min
Response: 839383607
Conc: 992.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

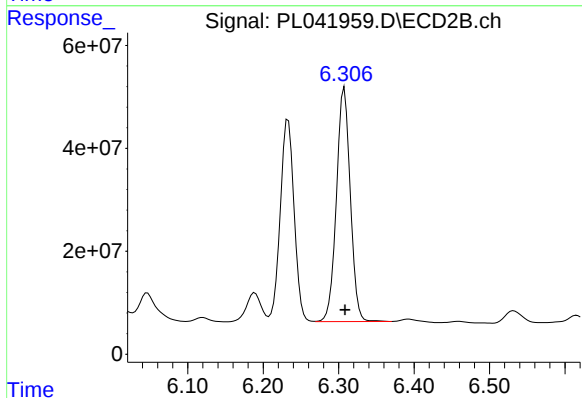


#26 Chlordane-4

R.T.: 6.308 min
Delta R.T.: -0.001 min
Response: 580671645
Conc: 973.65 ng/ml

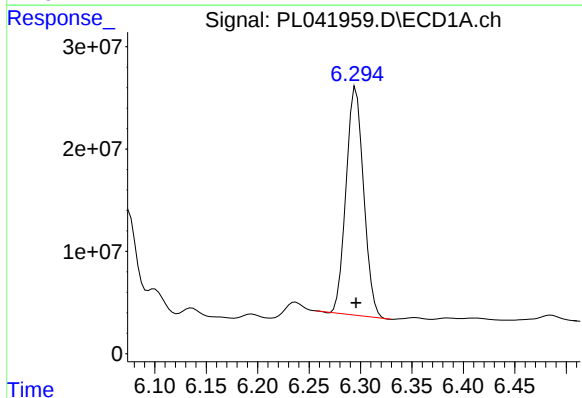


#27 Chlordane-5

R.T.: 6.296 min
Delta R.T.: 0.000 min
Response: 264386655
Conc: 1001.68 ng/ml

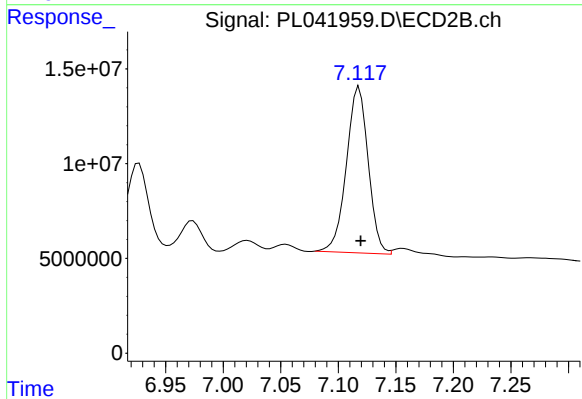

#27 Chlordane-5

R.T.: 7.118 min
Delta R.T.: -0.001 min
Response: 116243838
Conc: 1013.05 ng/ml

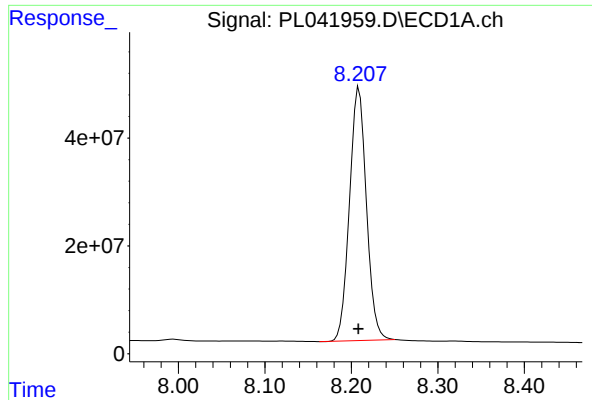

#28 Decachlorobiphenyl


R.T.: 8.209 min

Delta R.T.: 0.000 min

Response: 635992436

Conc: 94.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

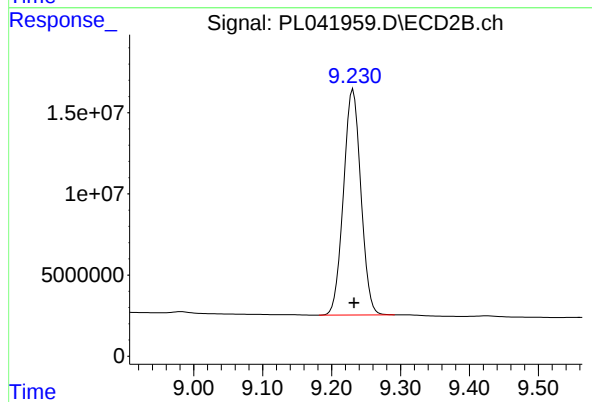

#28 Decachlorobiphenyl

R.T.: 9.231 min

Delta R.T.: -0.001 min

Response: 244110944

Conc: 95.60 ng/ml