

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110918\
 Data File : PL042002.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2018 21:19
 Operator : AJ\SJ
 Sample : J5877-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 22:01:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.470	4.104	110.4E6	56125595	17.884	18.944
28)	SA Decachlor...	8.211	9.236	113.3E6	46039833	16.537	18.051
Target Compounds							
6)	B beta-BHC	4.405f	0.000	9154953	0	2.481	N.D. #
7)	B delta-BHC	0.000	5.150	0	978334	N.D.	0.247 #
9)	A Endosulfan I	5.464f	0.000	2237978	0	0.307	N.D. #
10)	B gamma-Chl...	5.464f	0.000	2237978	0	0.278	N.D. #
11)	B alpha-Chl...	5.464	0.000	2237978	0	0.281	N.D. #
23)	Chlordane-1	4.382	5.150	3508881	978334	11.757	6.795 #
25)	Chlordane-3	5.464	0.000	2237978	0	2.394	N.D. #
26)	Chlordane-4	5.464	0.000	2237978	0	2.679	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110918\
Data File : PL042002.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2018 21:19
Operator : AJ\SJ
Sample : J5877-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 22:01:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

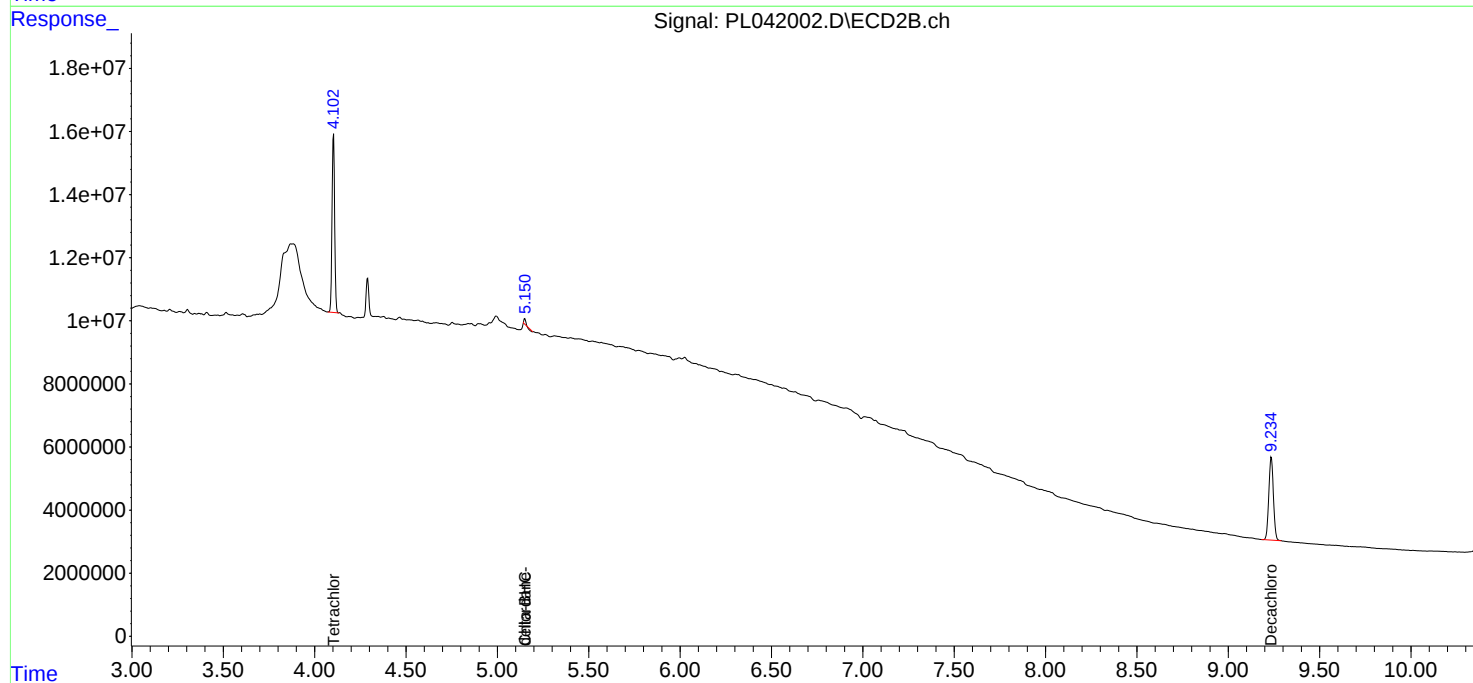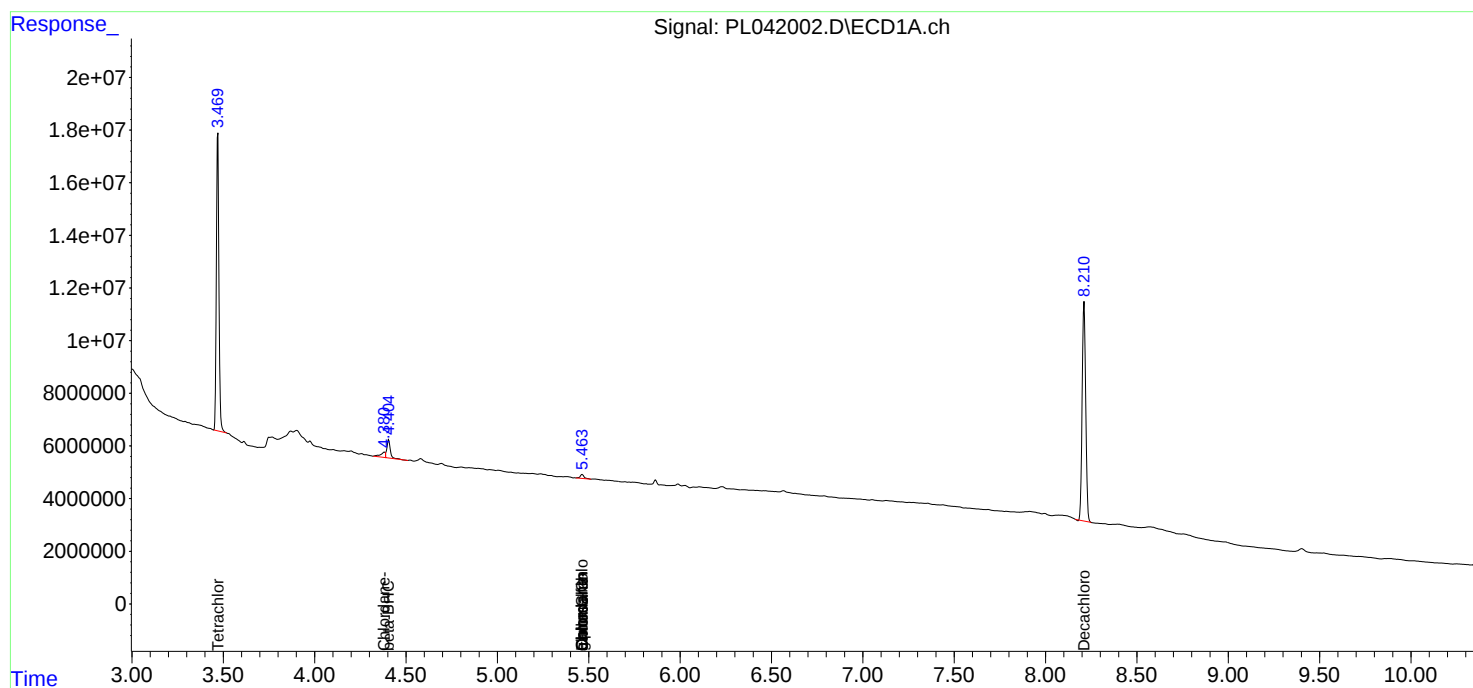


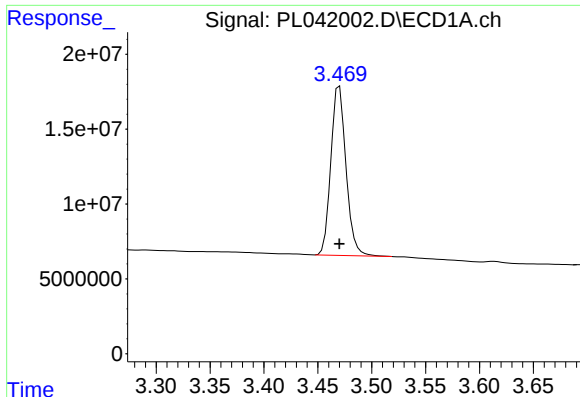

#1 Tetrachloro-m-xylene


R.T.: 3.470 min
Delta R.T.: 0.000 min
Response: 110430285
Conc: 17.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

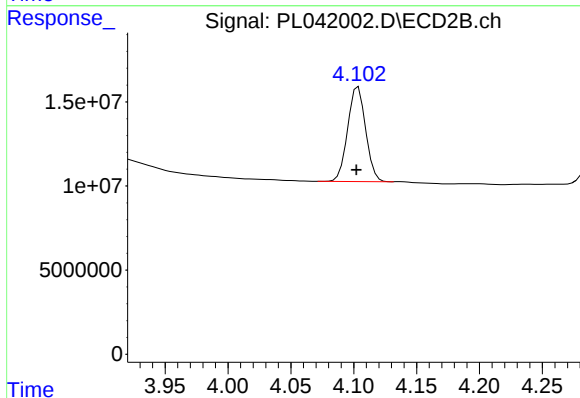


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.001 min
Response: 56125595
Conc: 18.94 ng/ml

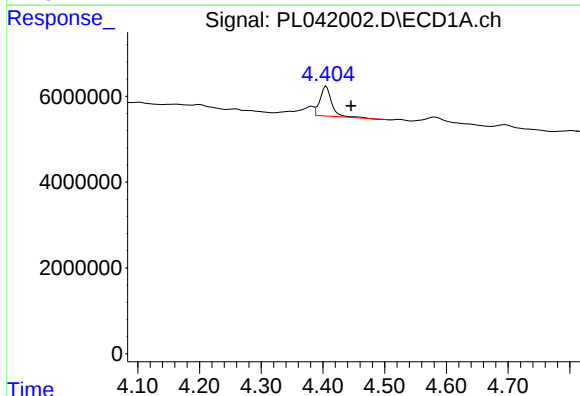


#6 beta-BHC

R.T.: 4.405 min
Delta R.T.: -0.040 min
Response: 9154953
Conc: 2.48 ng/ml

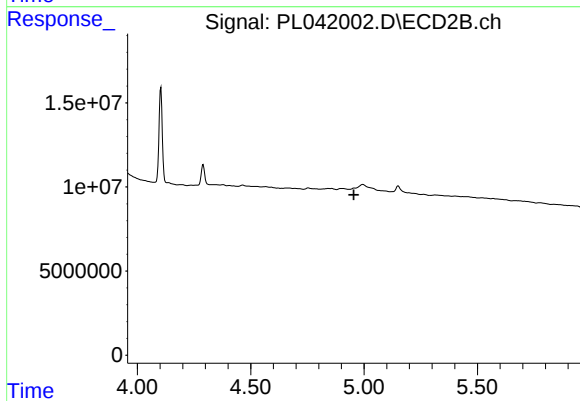

#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

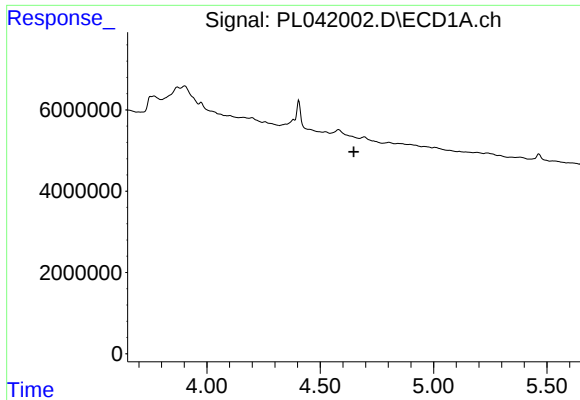

#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.648 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

#7 delta-BHC


R.T.: 5.150 min
Delta R.T.: -0.025 min
Response: 978334
Conc: 0.25 ng/ml

#9 Endosulfan I

R.T.: 5.464 min
Delta R.T.: -0.051 min
Response: 2237978
Conc: 0.31 ng/ml

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.358 min
Response: 0
Conc: N.D.

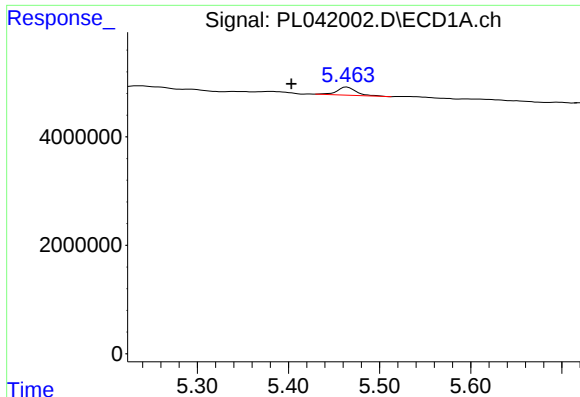

#10 gamma-Chlordane


R.T.: 5.464 min
Delta R.T.: 0.061 min
Response: 2237978
Conc: 0.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

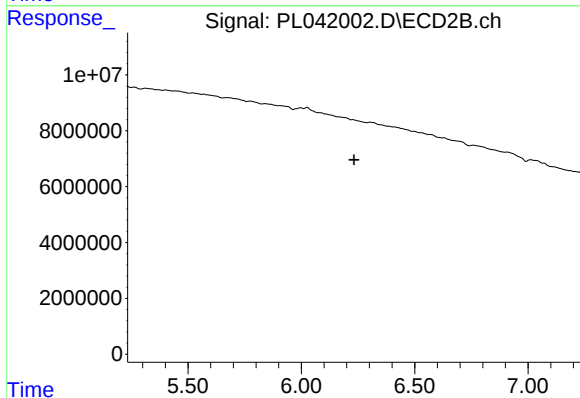


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.233 min
Response: 0
Conc: N.D.

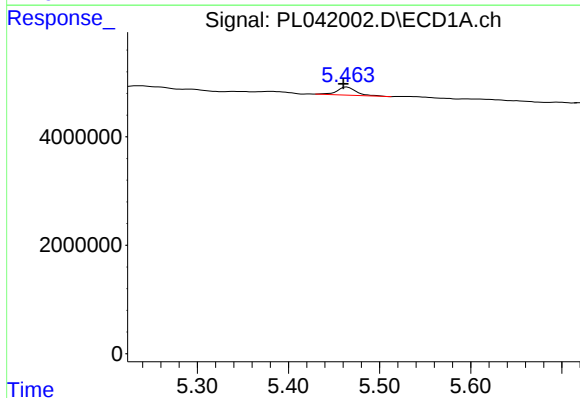


#11 alpha-Chlordane

R.T.: 5.464 min
Delta R.T.: 0.004 min
Response: 2237978
Conc: 0.28 ng/ml

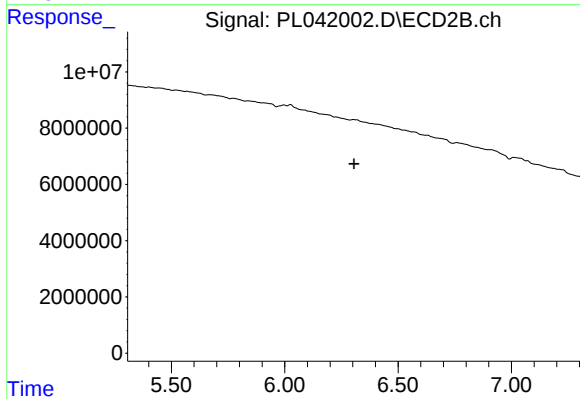

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.307 min
Response: 0
Conc: N.D.

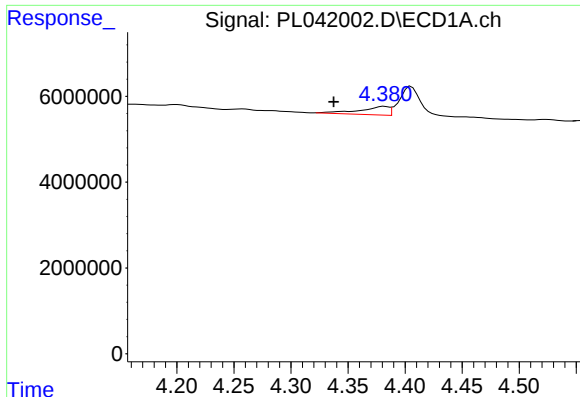

#23 Chlordane-1


R.T.: 4.382 min
Delta R.T.: 0.044 min
Response: 3508881
Conc: 11.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

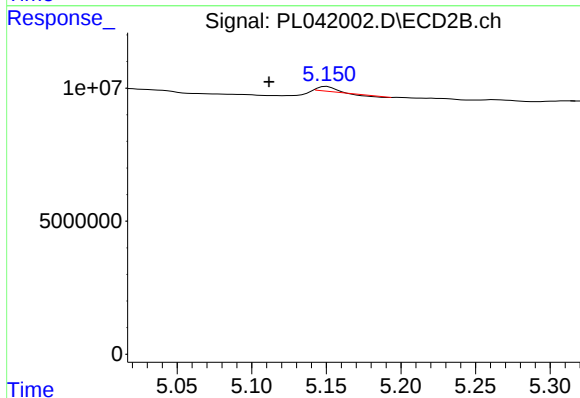


#23 Chlordane-1

R.T.: 5.150 min
Delta R.T.: 0.039 min
Response: 978334
Conc: 6.79 ng/ml

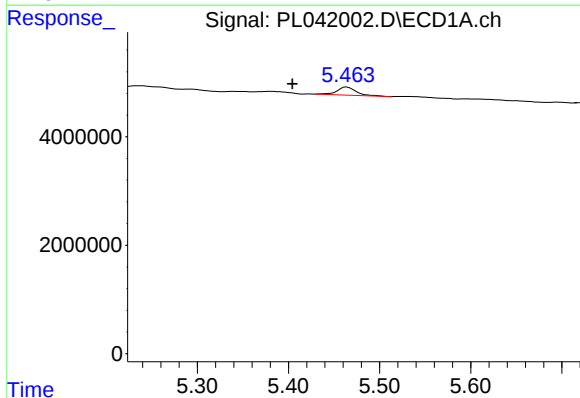


#25 Chlordane-3

R.T.: 5.464 min
Delta R.T.: 0.060 min
Response: 2237978
Conc: 2.39 ng/ml

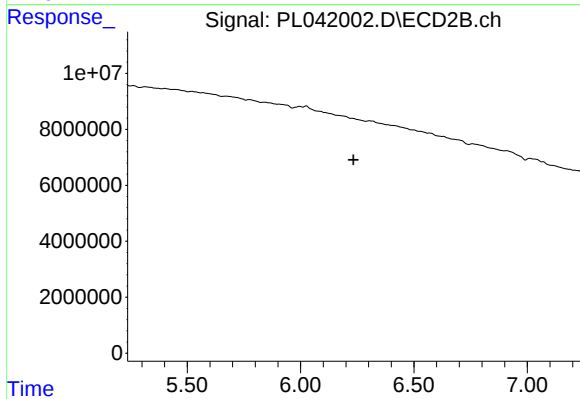

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.234 min
Response: 0
Conc: N.D.

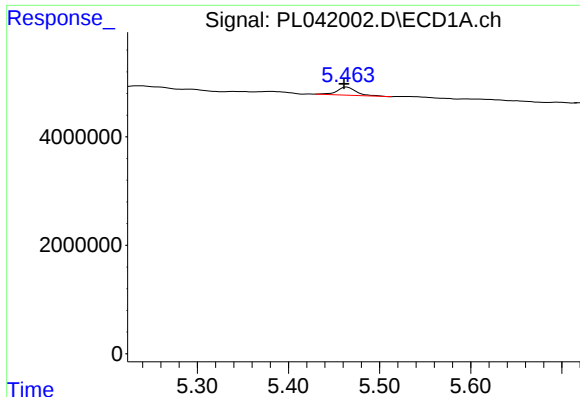

#26 Chlordane-4


R.T.: 5.464 min
Delta R.T.: 0.003 min
Response: 2237978
Conc: 2.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

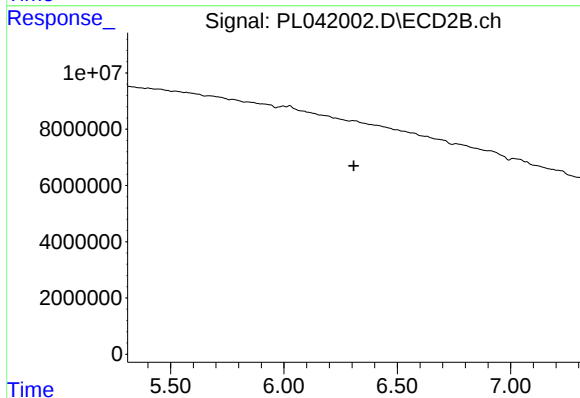


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.309 min
Response: 0
Conc: N.D.

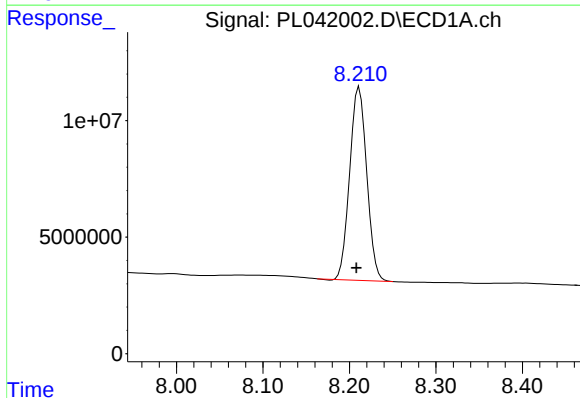

#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: 0.003 min
Response: 113285176
Conc: 16.54 ng/ml

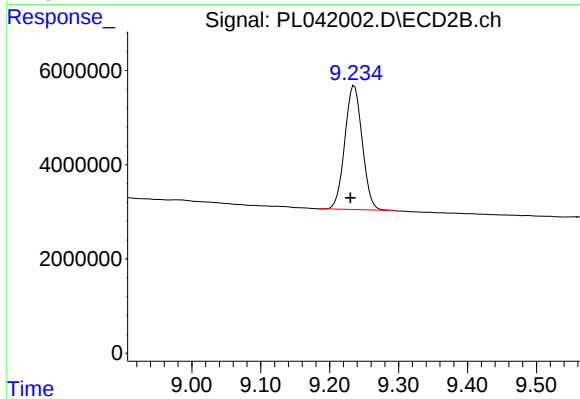

#28 Decachlorobiphenyl

R.T.: 9.236 min
Delta R.T.: 0.005 min
Response: 46039833
Conc: 18.05 ng/ml