

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110918\
 Data File : PL042012.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2018 23:41
 Operator : AJ\SJ
 Sample : J5269-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 03:10:27 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.470	4.104	120.9E6	63202219	19.585	21.333
28)	SA Decachlor...	8.211	9.235	137.4E6	56308339	20.050	22.077
Target Compounds							
6)	B beta-BHC	4.406f	0.000	8477887	0	2.297	N.D. #
7)	B delta-BHC	0.000	5.151	0	1265560	N.D.	0.320 #
9)	A Endosulfan I	5.465f	0.000	1709490	0	0.235	N.D. #
10)	B gamma-Chl...	5.465f	0.000	1709490	0	0.212	N.D. #
11)	B alpha-Chl...	5.465	0.000	1709490	0	0.215	N.D. #
14)	MA Endrin	6.040	0.000	2191019	0	0.308	N.D. #
15)	B Endosulfa...	6.230f	0.000	3034249	0	0.445	N.D. #
17)	MA 4,4'-DDT	6.386	0.000	3170797	0	0.557	N.D. #
23)	Chlordane-1	4.406	5.151	8477887	1265560	28.407	8.790 #
25)	Chlordane-3	5.465	0.000	1709490	0	1.828	N.D. #
26)	Chlordane-4	5.465	0.000	1709490	0	2.046	N.D. #
27)	Chlordane-5	6.230	0.000	3034249	0	11.583	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110918\
Data File : PL042012.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2018 23:41
Operator : AJ\SJ
Sample : J5269-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 03:10:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

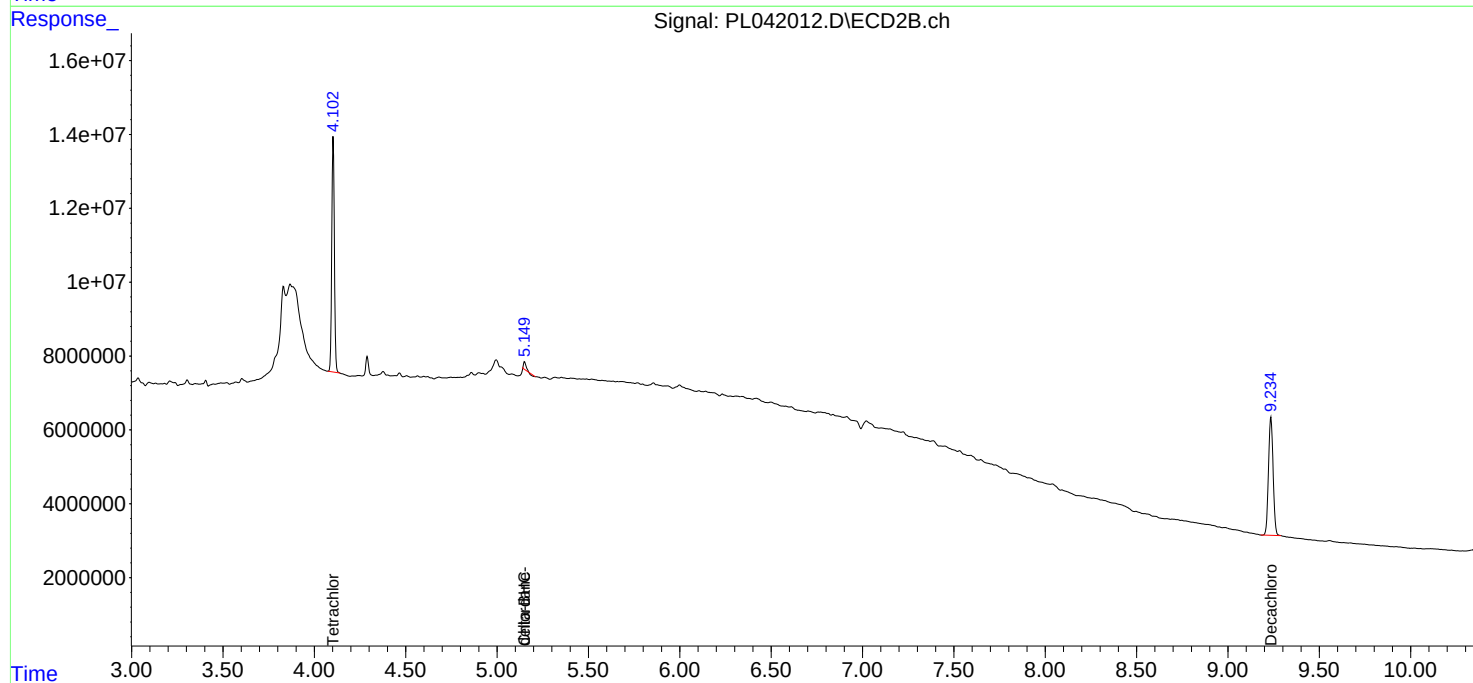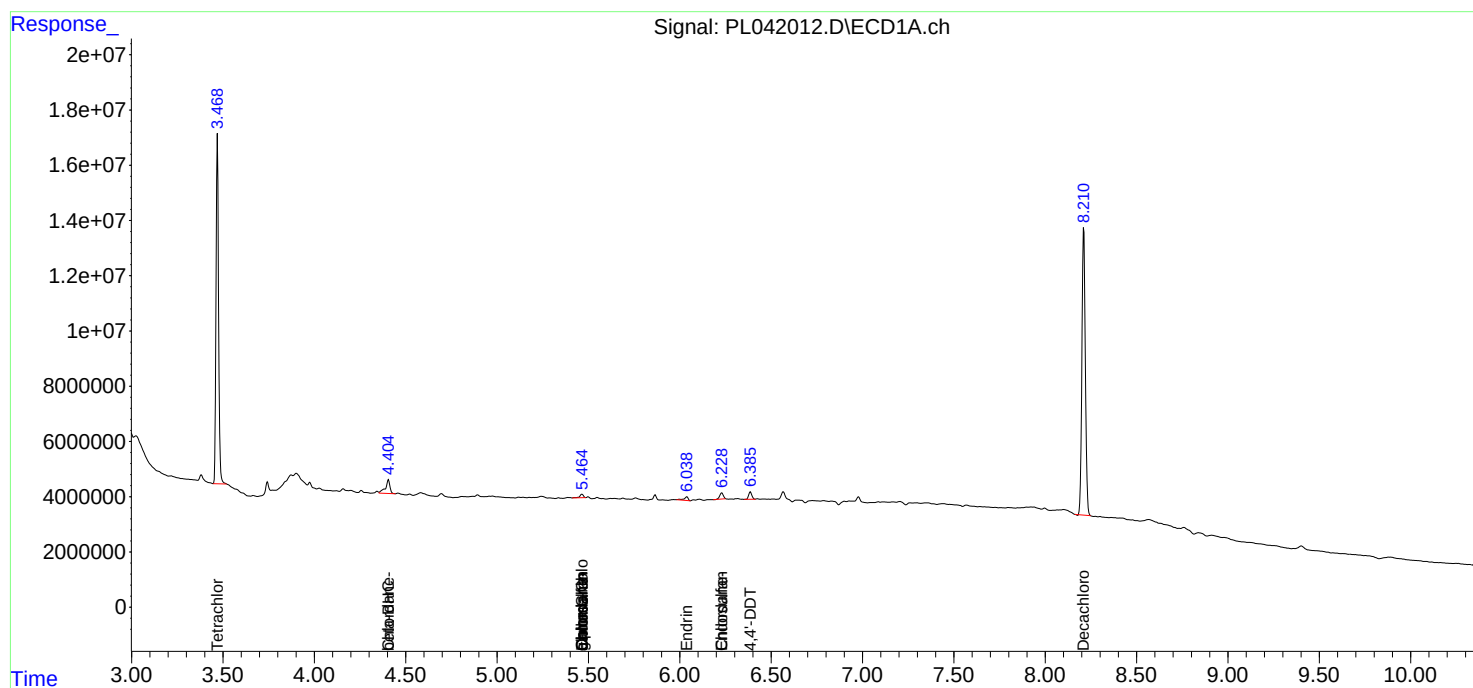


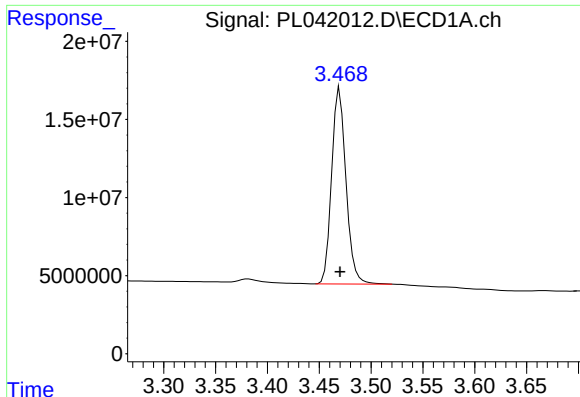

#1 Tetrachloro-m-xylene


R.T.: 3.470 min
Delta R.T.: 0.000 min
Response: 120939077
Conc: 19.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

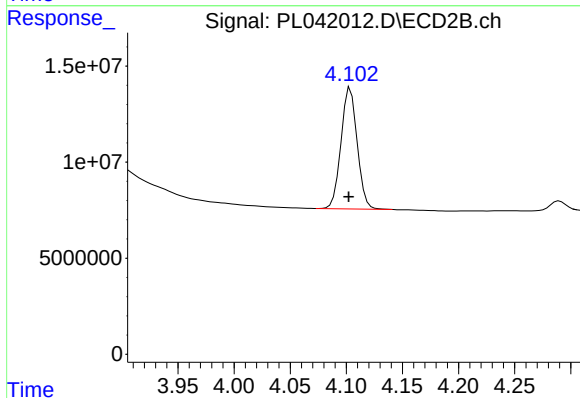


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.002 min
Response: 63202219
Conc: 21.33 ng/ml

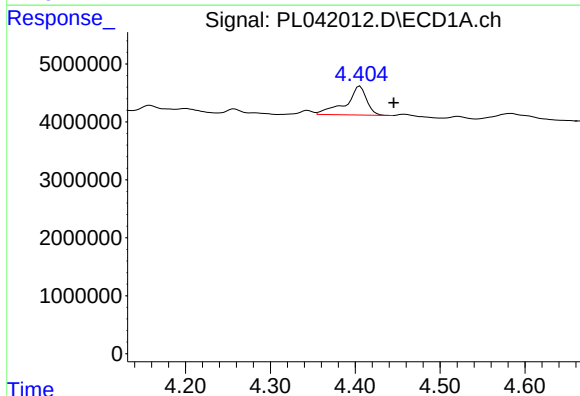


#6 beta-BHC

R.T.: 4.406 min
Delta R.T.: -0.040 min
Response: 8477887
Conc: 2.30 ng/ml

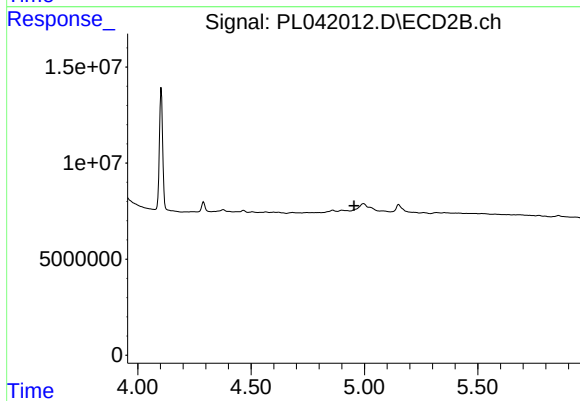

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

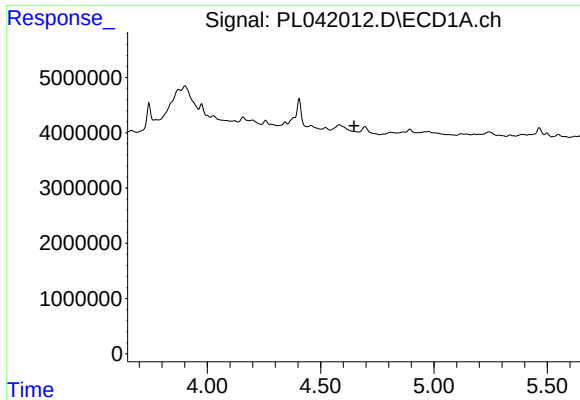

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.648 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

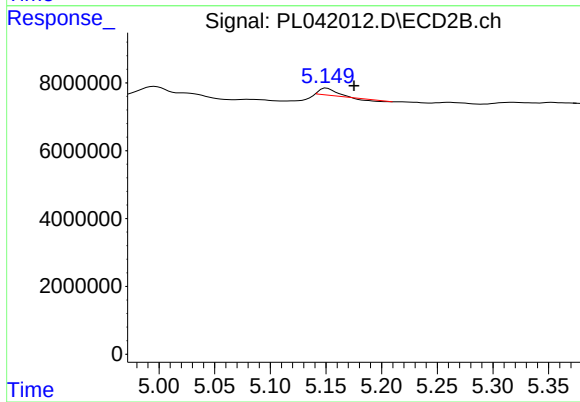


#7 delta-BHC

R.T.: 5.151 min
Delta R.T.: -0.025 min
Response: 1265560
Conc: 0.32 ng/ml

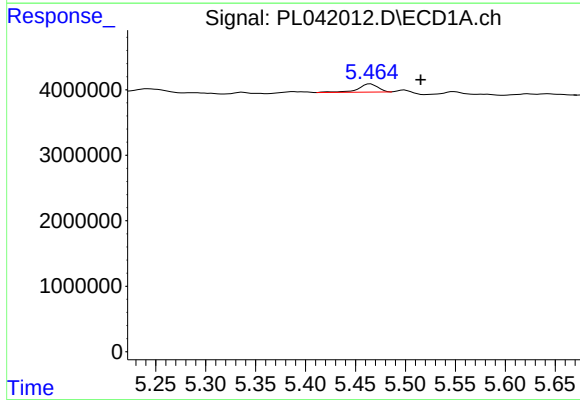


#9 Endosulfan I

R.T.: 5.465 min
Delta R.T.: -0.051 min
Response: 1709490
Conc: 0.23 ng/ml

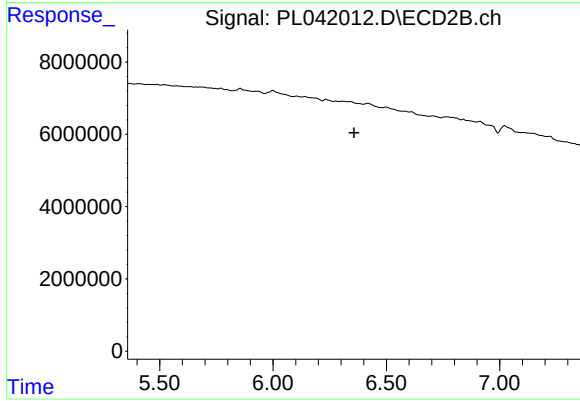

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.358 min
Response: 0
Conc: N.D.

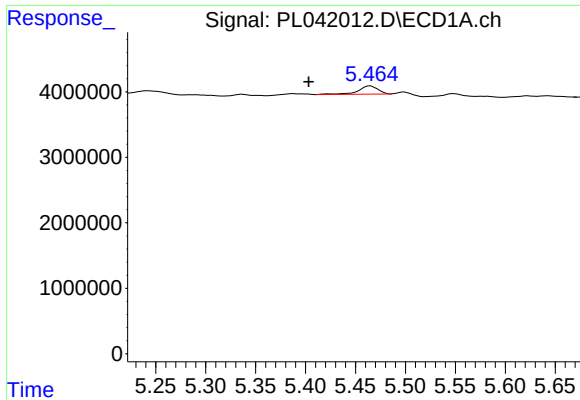

#10 gamma-Chlordane


R.T.: 5.465 min
Delta R.T.: 0.062 min
Response: 1709490
Conc: 0.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

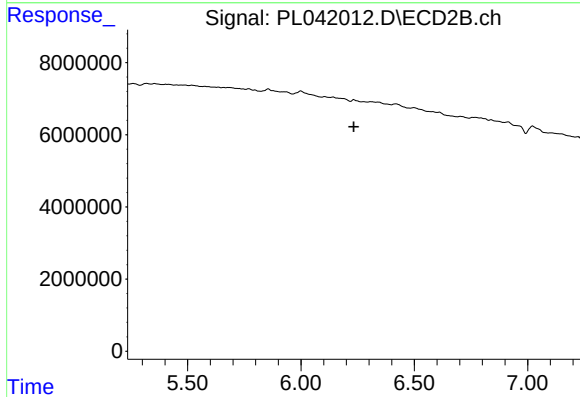


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.233 min
Response: 0
Conc: N.D.

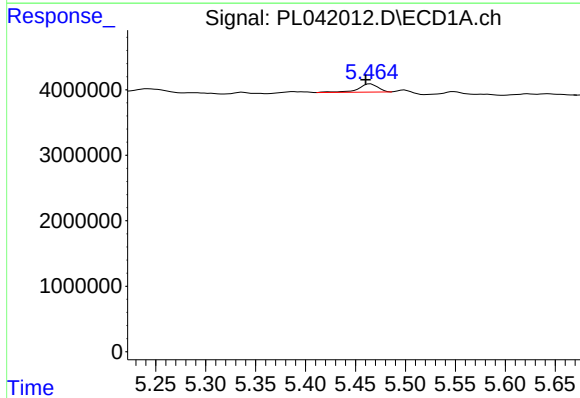


#11 alpha-Chlordane

R.T.: 5.465 min
Delta R.T.: 0.005 min
Response: 1709490
Conc: 0.21 ng/ml

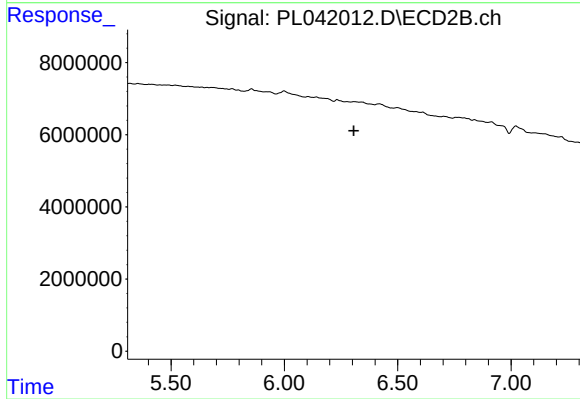

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.307 min
Response: 0
Conc: N.D.

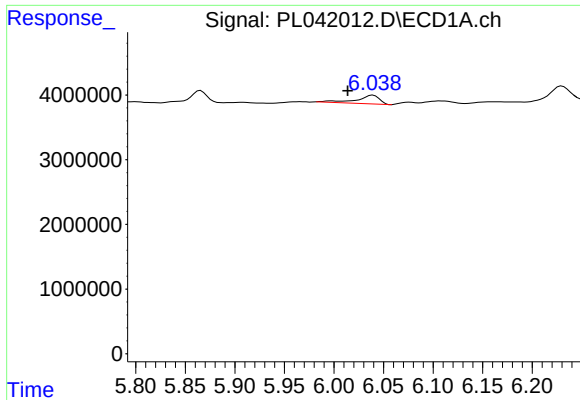

#14 Endrin


R.T.: 6.040 min
Delta R.T.: 0.026 min
Response: 2191019
Conc: 0.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

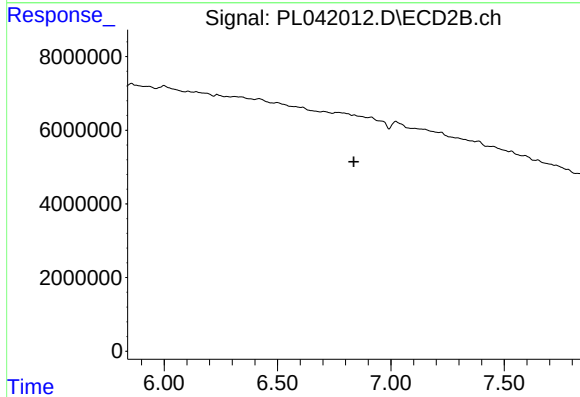


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.836 min
Response: 0
Conc: N.D.

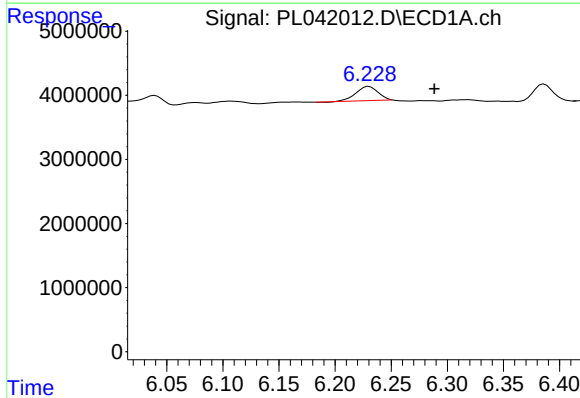


#15 Endosulfan II

R.T.: 6.230 min
Delta R.T.: -0.058 min
Response: 3034249
Conc: 0.44 ng/ml

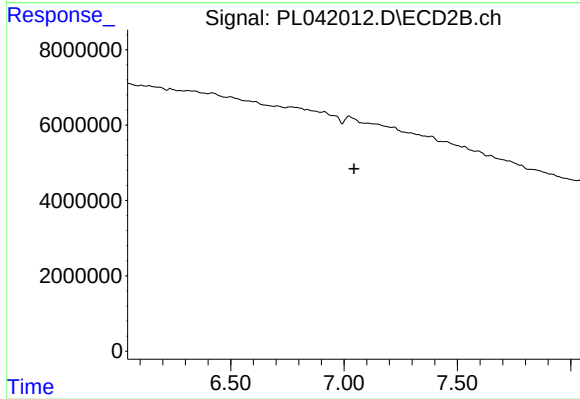

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 7.044 min
Response: 0
Conc: N.D.

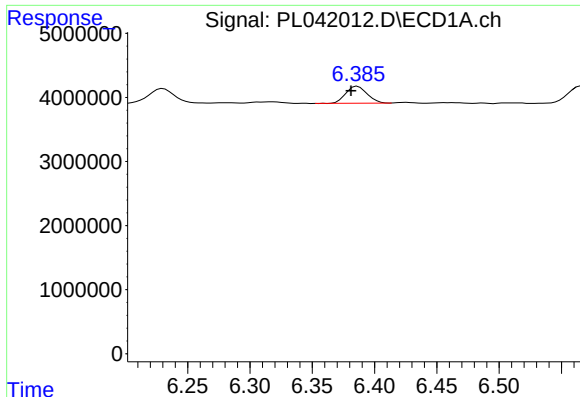

#17 4,4'-DDT


R.T.: 6.386 min
Delta R.T.: 0.005 min
Response: 3170797
Conc: 0.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

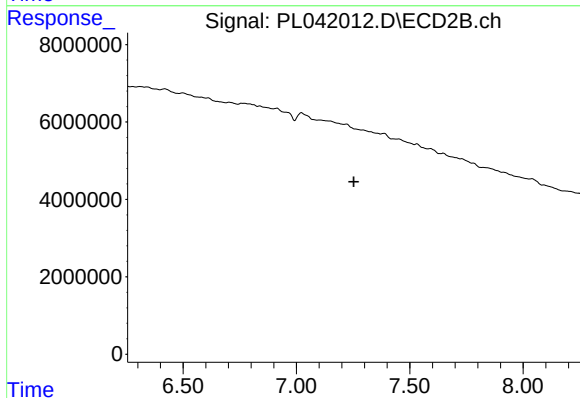


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.253 min
Response: 0
Conc: N.D.

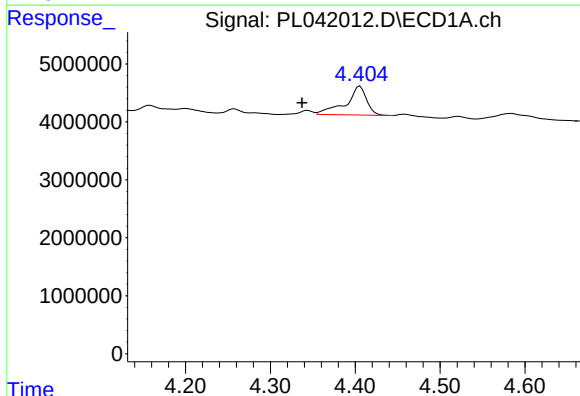


#23 Chlordane-1

R.T.: 4.406 min
Delta R.T.: 0.068 min
Response: 8477887
Conc: 28.41 ng/ml

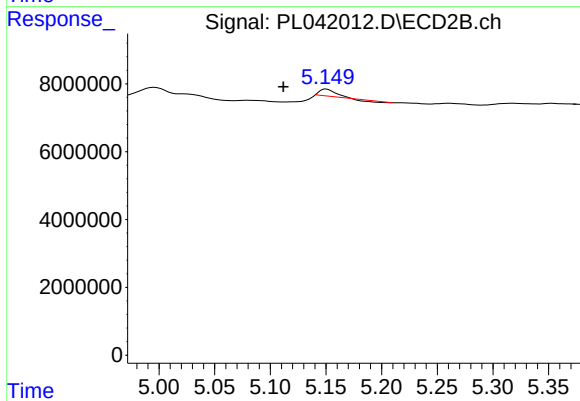

#23 Chlordane-1


R.T.: 5.151 min
Delta R.T.: 0.039 min
Response: 1265560
Conc: 8.79 ng/ml

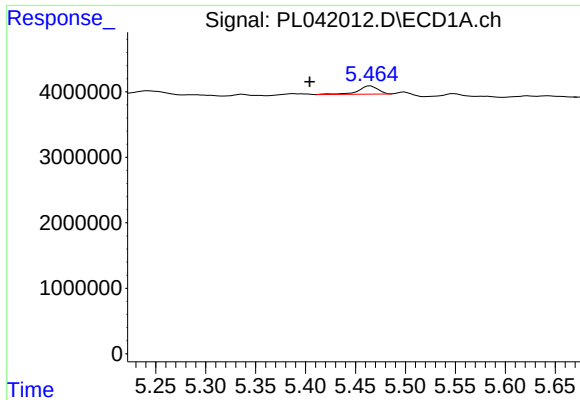

#25 Chlordane-3


R.T.: 5.465 min
Delta R.T.: 0.061 min
Response: 1709490
Conc: 1.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

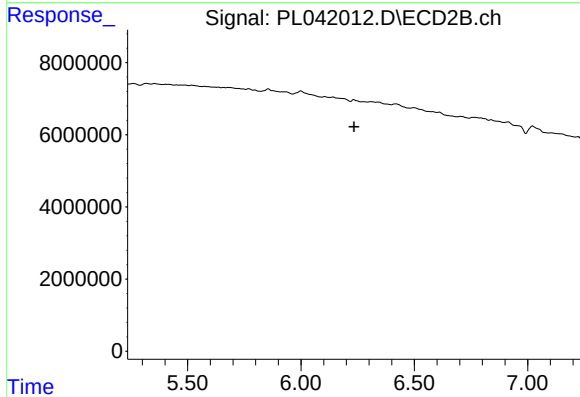


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.234 min
Response: 0
Conc: N.D.

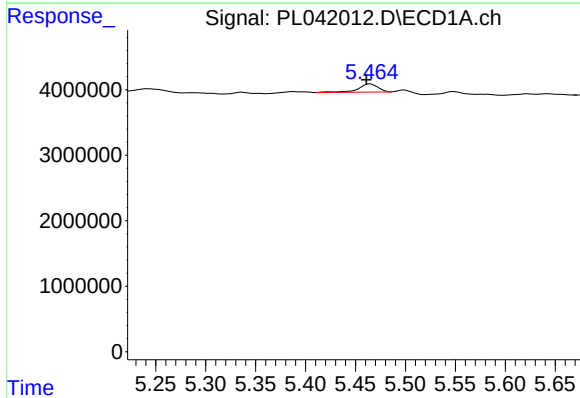


#26 Chlordane-4

R.T.: 5.465 min
Delta R.T.: 0.004 min
Response: 1709490
Conc: 2.05 ng/ml

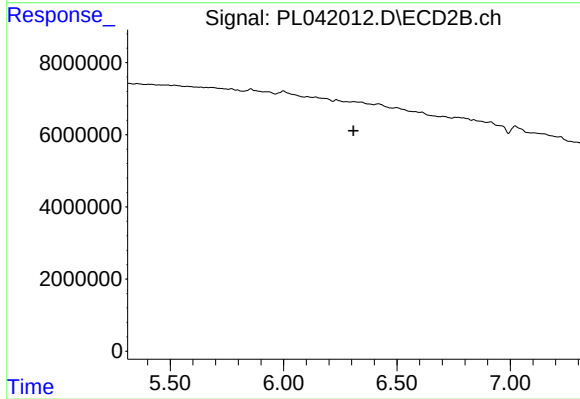

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.309 min
Response: 0
Conc: N.D.

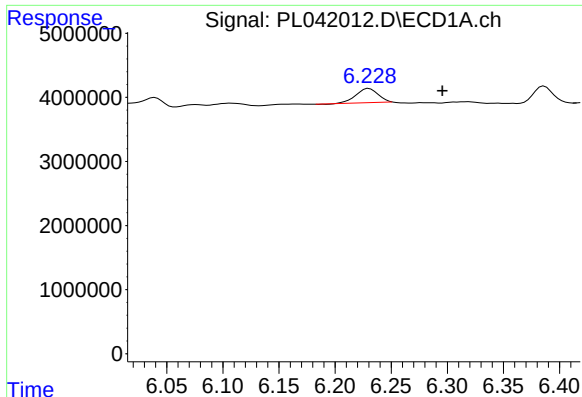

#27 Chlordane-5


R.T.: 6.230 min
Delta R.T.: -0.065 min
Response: 3034249
Conc: 11.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

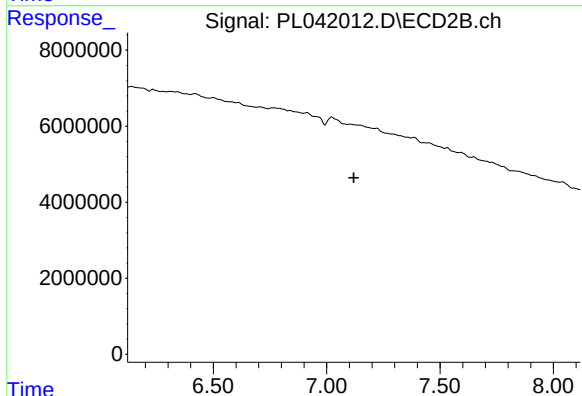


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.119 min
Response: 0
Conc: N.D.

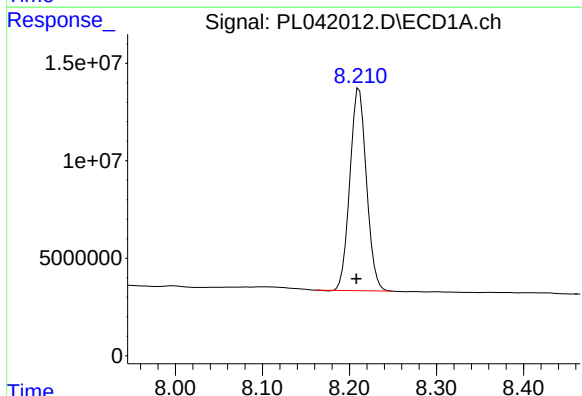

#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: 0.003 min
Response: 137350459
Conc: 20.05 ng/ml

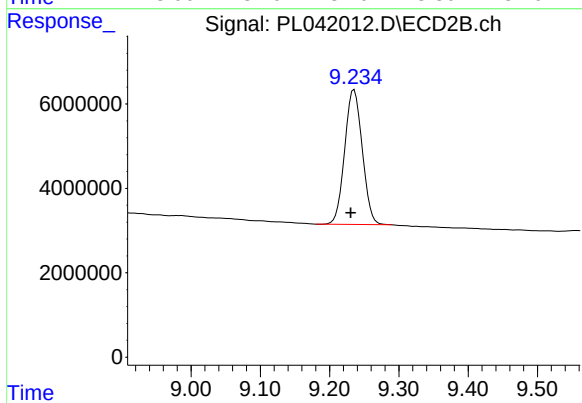

#28 Decachlorobiphenyl

R.T.: 9.235 min
Delta R.T.: 0.005 min
Response: 56308339
Conc: 22.08 ng/ml