

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110918\
 Data File : PL042034.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2018 04:51
 Operator : AJ\SJ
 Sample : J5884-03
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 05:40:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.470	4.103	39980749	18972335	6.475	6.404
28)	SA Decachlor...	8.211	9.235	24301218	9630695	3.547	3.776
Target Compounds							
6)	B beta-BHC	4.405f	4.905f	6217934	590066	1.685	0.359 #
20)	A Methoxychlor	0.000	7.643f	0	2160844	N.D.	1.573 #
23)	Chlordane-1	4.405	0.000	6217934	0	20.835	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110918\
Data File : PL042034.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2018 04:51
Operator : AJ\SJ
Sample : J5884-03
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 05:40:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

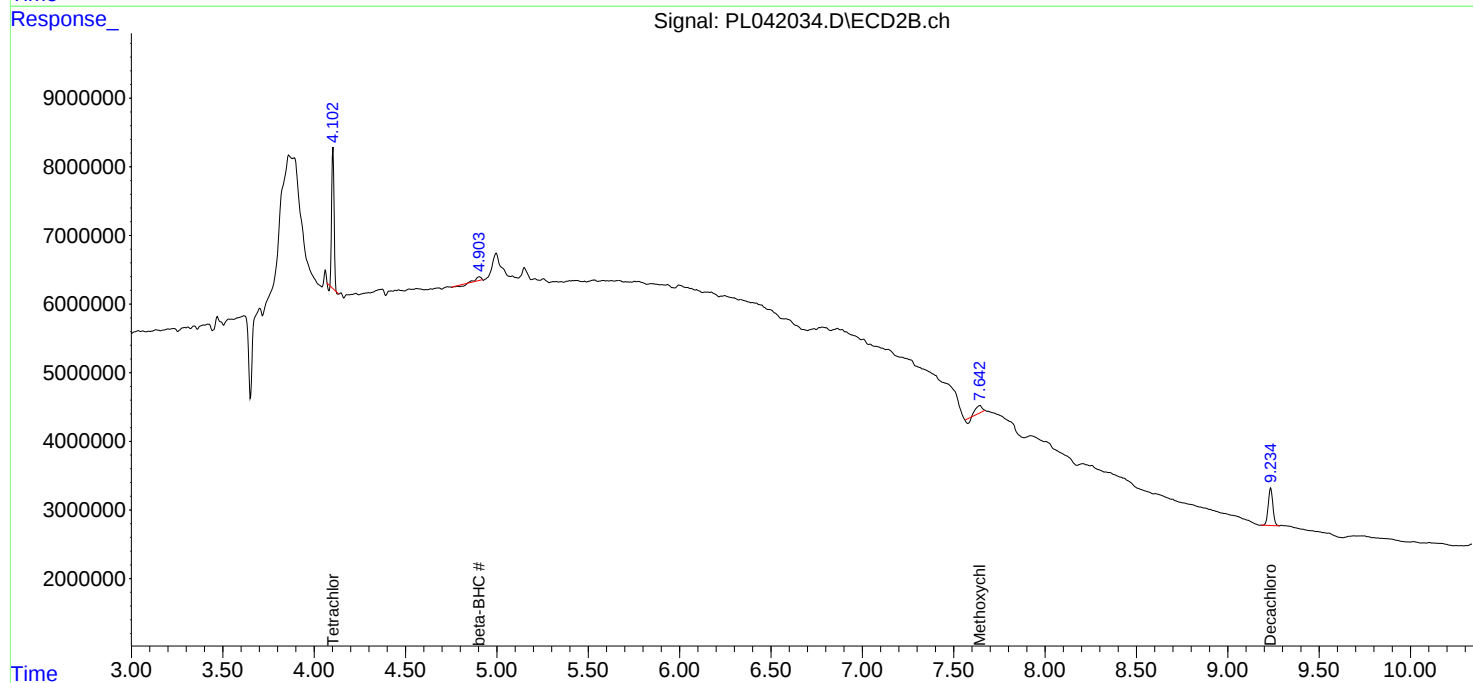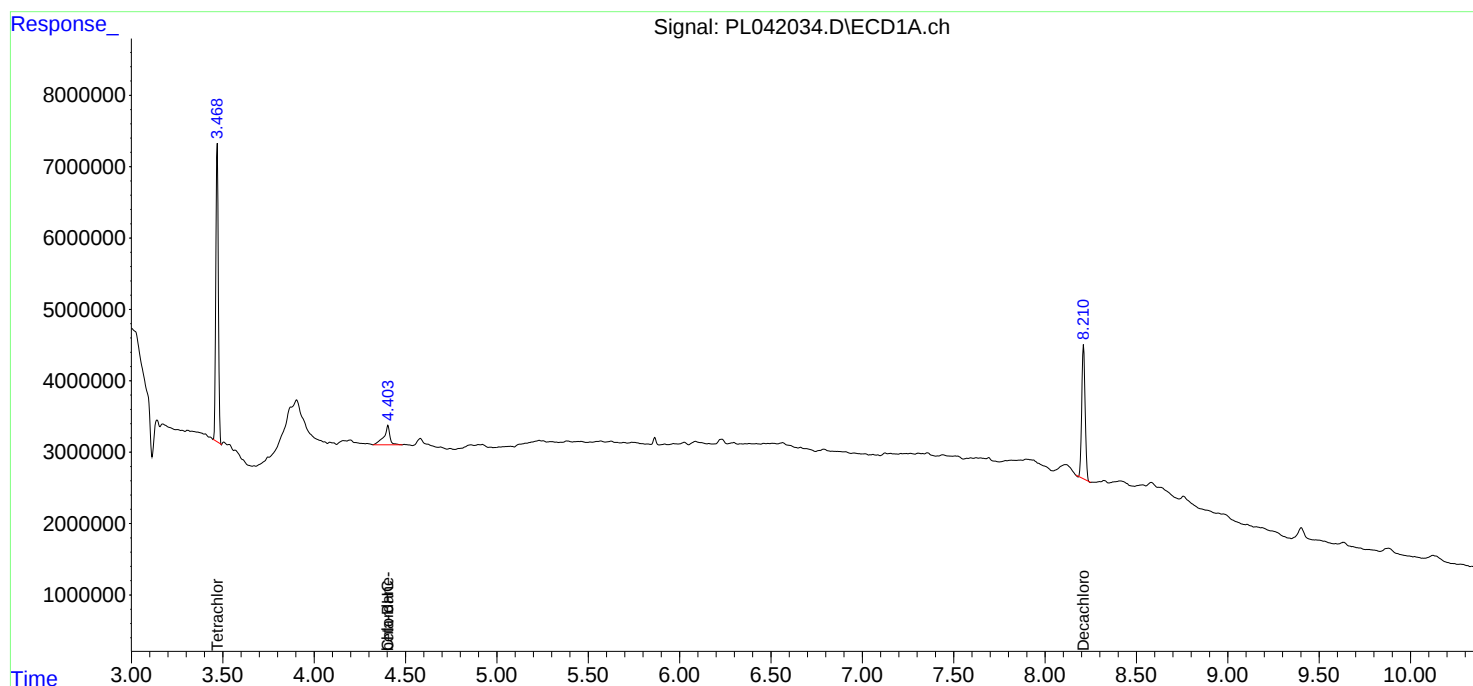


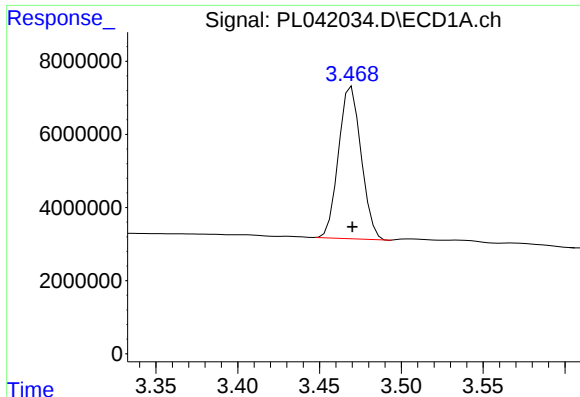

#1 Tetrachloro-m-xylene


R.T.: 3.470 min
Delta R.T.: 0.000 min
Response: 39980749
Conc: 6.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

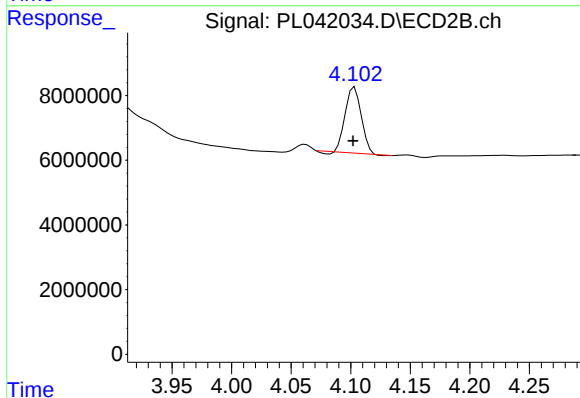


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: 0.001 min
Response: 18972335
Conc: 6.40 ng/ml

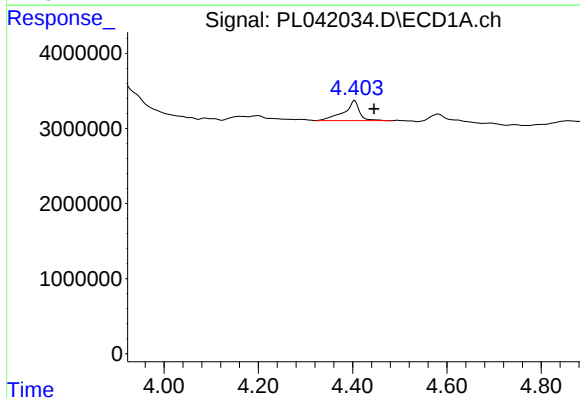


#6 beta-BHC

R.T.: 4.405 min
Delta R.T.: -0.041 min
Response: 6217934
Conc: 1.68 ng/ml

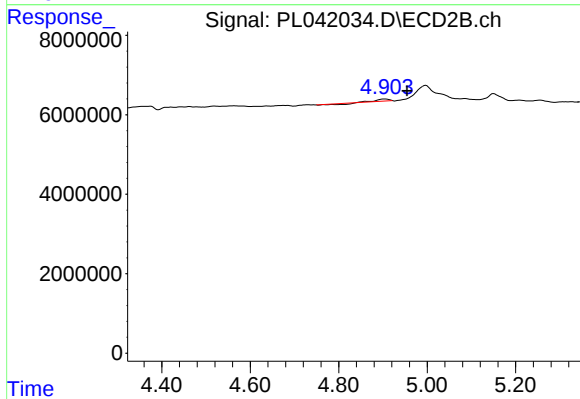

#6 beta-BHC


R.T.: 4.905 min
Delta R.T.: -0.050 min
Response: 590066
Conc: 0.36 ng/ml

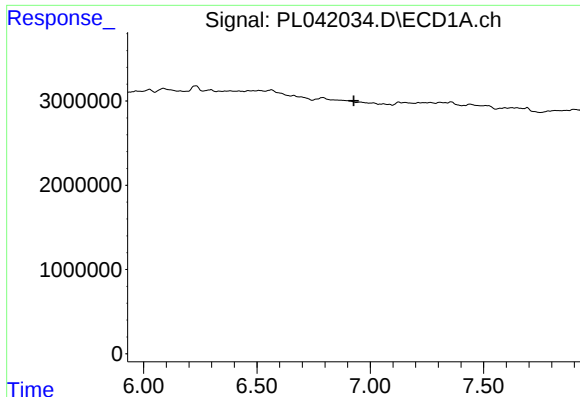

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.928 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

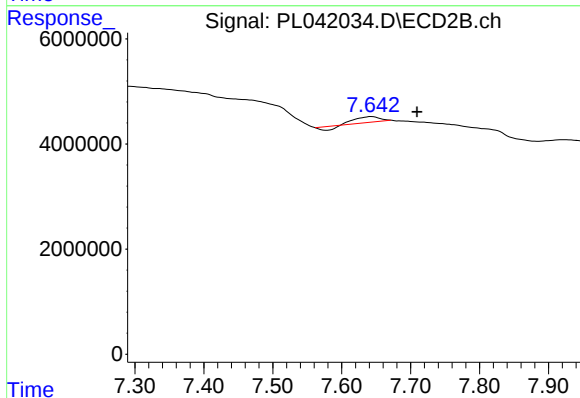


#20 Methoxychlor

R.T.: 7.643 min
Delta R.T.: -0.066 min
Response: 2160844
Conc: 1.57 ng/ml

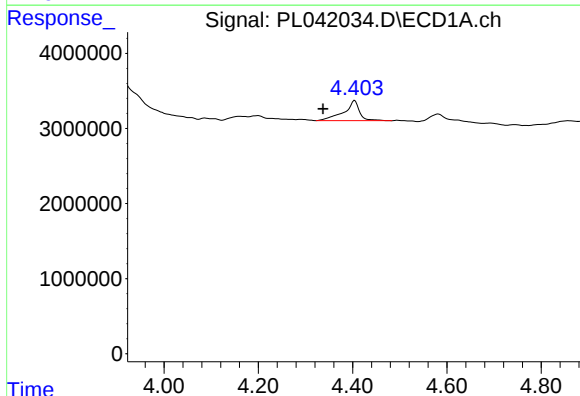


#23 Chlordane-1

R.T.: 4.405 min
Delta R.T.: 0.067 min
Response: 6217934
Conc: 20.83 ng/ml

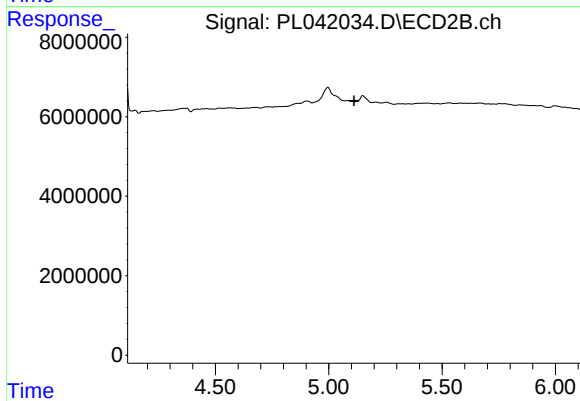

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.112 min
Response: 0
Conc: N.D.

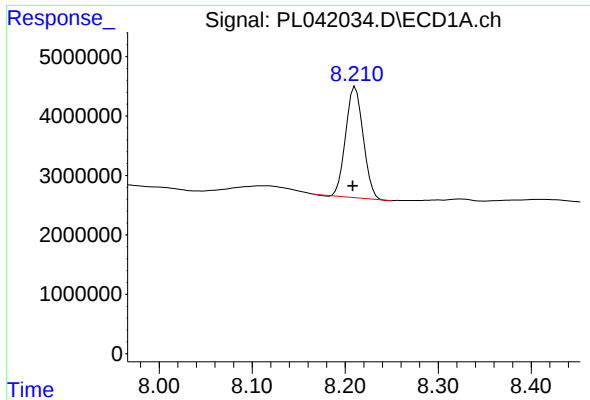

#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: 0.003 min
Response: 24301218
Conc: 3.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

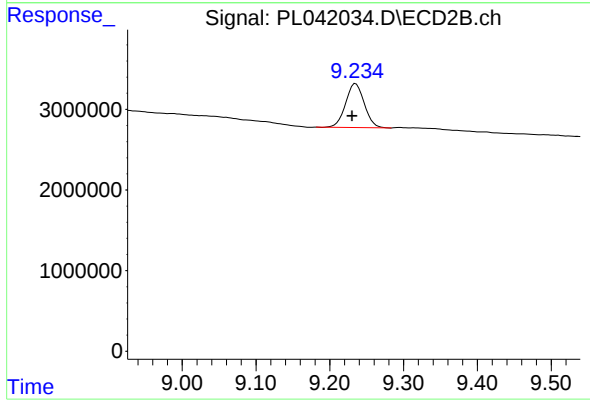

#28 Decachlorobiphenyl

R.T.: 9.235 min
Delta R.T.: 0.005 min
Response: 9630695
Conc: 3.78 ng/ml