

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110918\
 Data File : PL042040.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2018 06:16
 Operator : AJ\SJ
 Sample : J5887-11
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 02:50:03 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	4.103	48105807	25948940	7.791	8.759
28)	SA Decachlor...	8.210	9.235	64757684	26717950	9.453	10.475
Target Compounds							
6)	B beta-BHC	4.404f	0.000	4742947	0	1.285	N.D. #
9)	A Endosulfan I	5.462f	0.000	1651427	0	0.227	N.D. #
10)	B gamma-Chl...	5.424	0.000	3780246	0	0.469	N.D. #
11)	B alpha-Chl...	5.462	0.000	1651427	0	0.207	N.D. #
16)	A 4,4'-DDD	6.208f	0.000	2633786	0	0.477	N.D. #
17)	MA 4,4'-DDT	6.378	0.000	2700623	0	0.475	N.D. #
19)	B Endosulfa...	6.664	0.000	1486732	0	0.233	N.D. #
20)	A Methoxychlor	6.908	0.000	4279003	0	1.343	N.D. #
21)	B Endrin ke...	0.000	7.827f	0	1627570	N.D.	0.562 #
23)	Chlordane-1	4.404	0.000	4742947	0	15.892	N.D. #
25)	Chlordane-3	5.424	0.000	3780246	0	4.043	N.D. #
26)	Chlordane-4	5.462	0.000	1651427	0	1.977	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110918\
Data File : PL042040.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2018 06:16
Operator : AJ\SJ
Sample : J5887-11
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 02:50:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

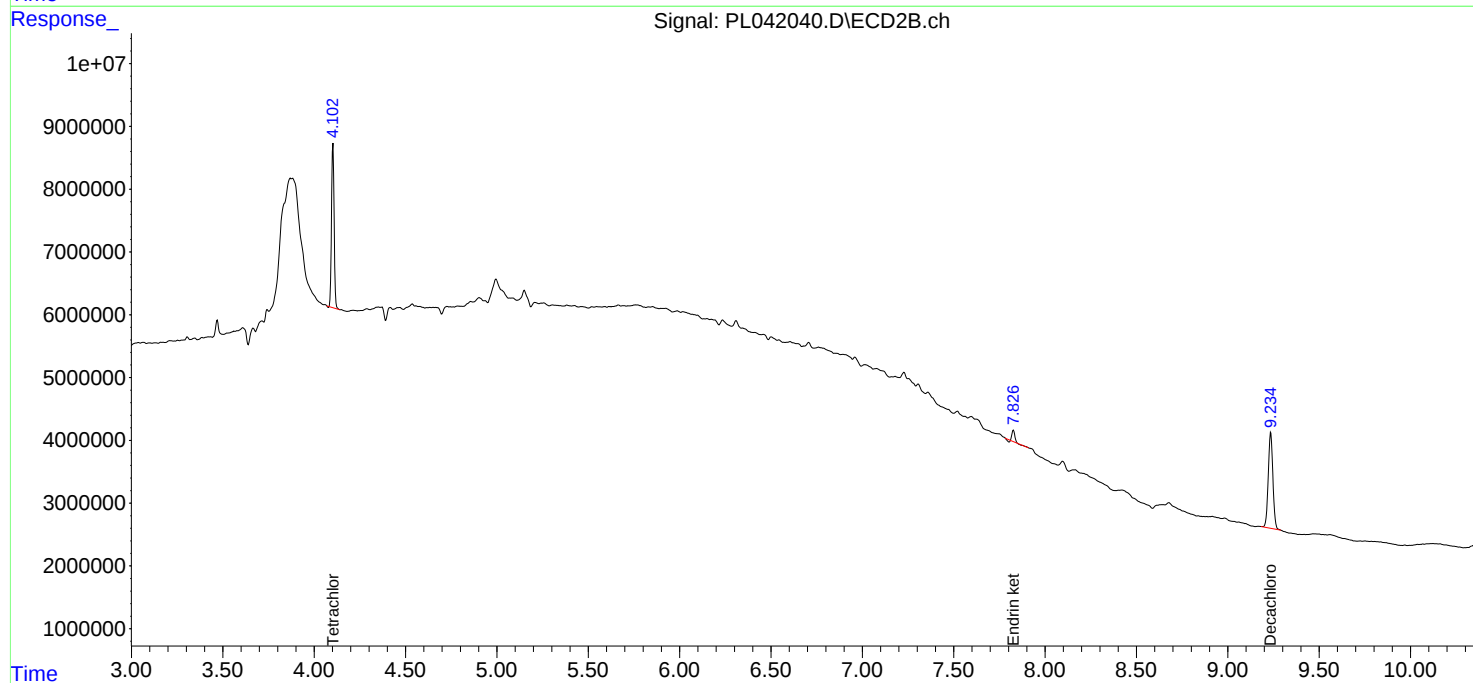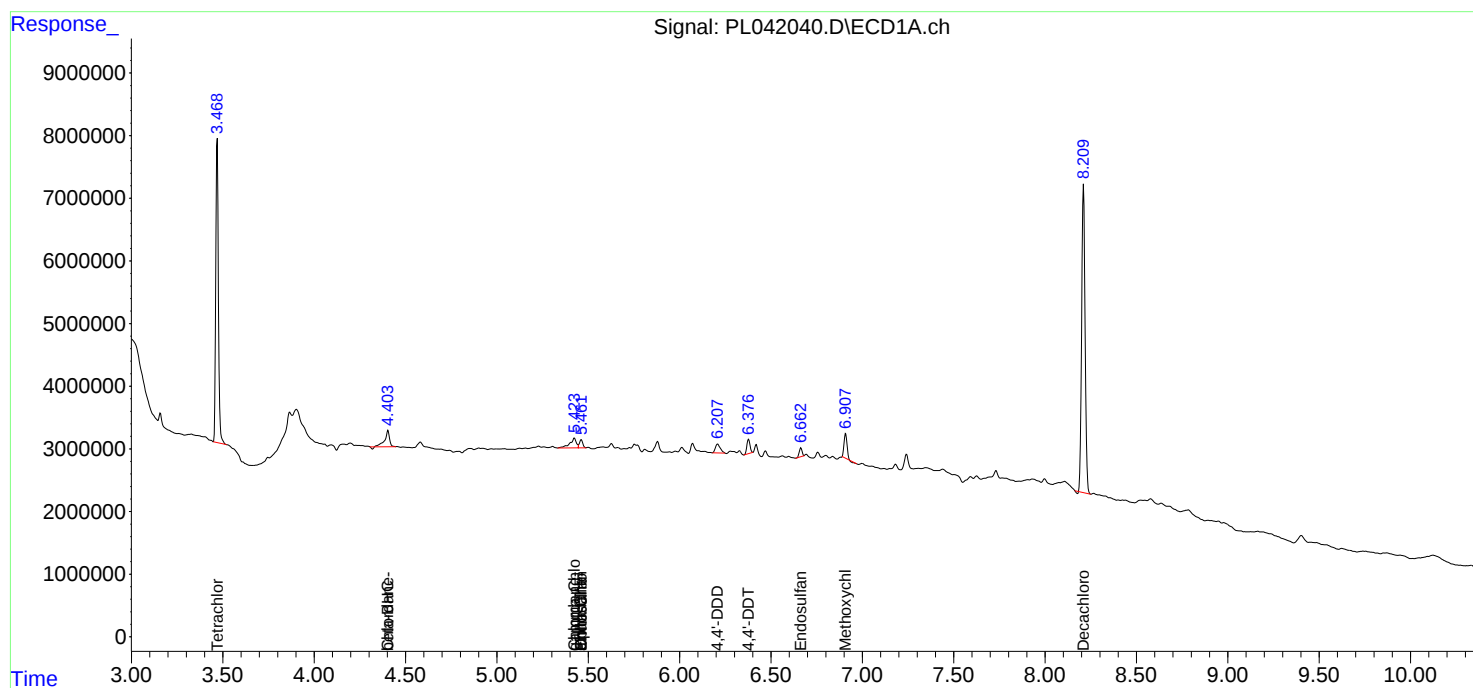


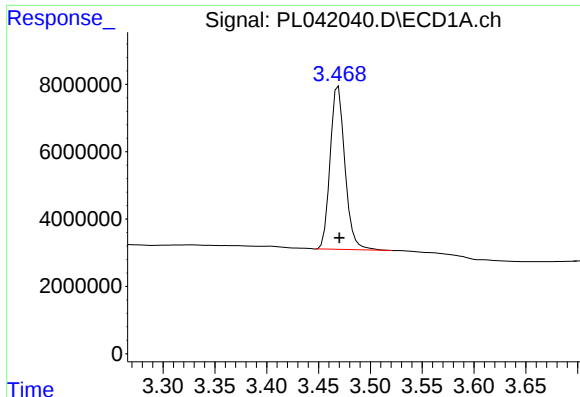

#1 Tetrachloro-m-xylene


R.T.: 3.469 min
Delta R.T.: 0.000 min
Response: 48105807
Conc: 7.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

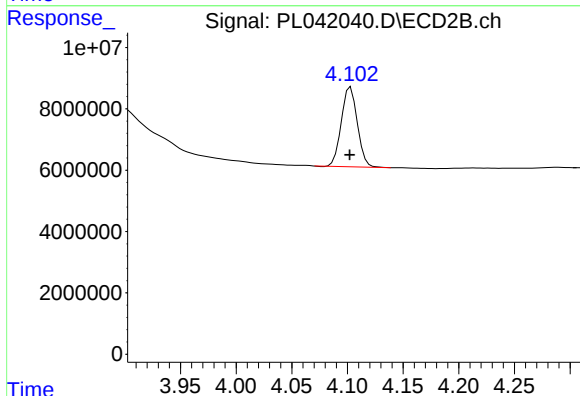


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: 0.000 min
Response: 25948940
Conc: 8.76 ng/ml

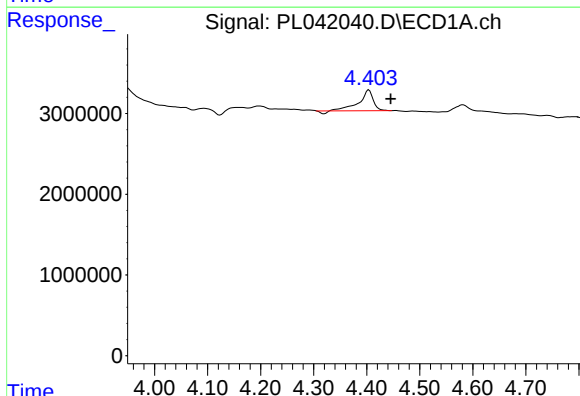


#6 beta-BHC

R.T.: 4.404 min
Delta R.T.: -0.041 min
Response: 4742947
Conc: 1.29 ng/ml

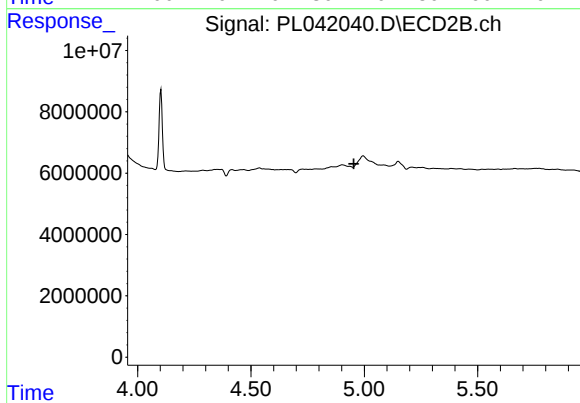

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

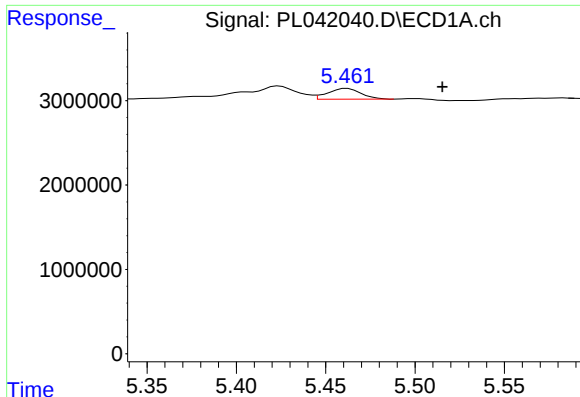

#9 Endosulfan I


R.T.: 5.462 min
Delta R.T.: -0.053 min
Response: 1651427
Conc: 0.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

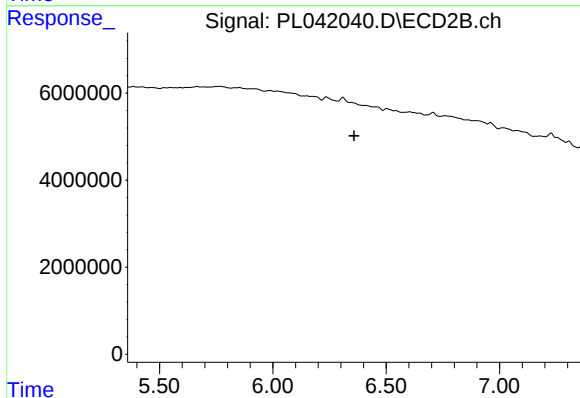


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.358 min
Response: 0
Conc: N.D.

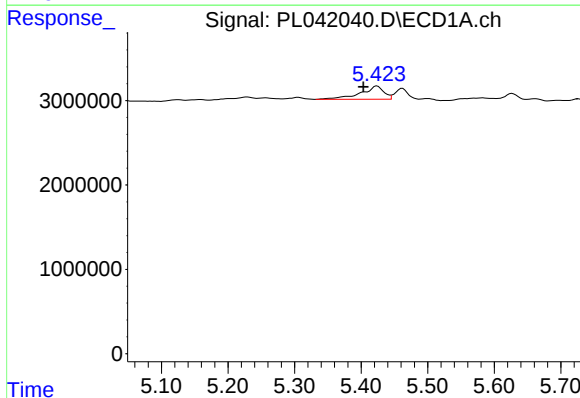


#10 gamma-Chlordane

R.T.: 5.424 min
Delta R.T.: 0.021 min
Response: 3780246
Conc: 0.47 ng/ml

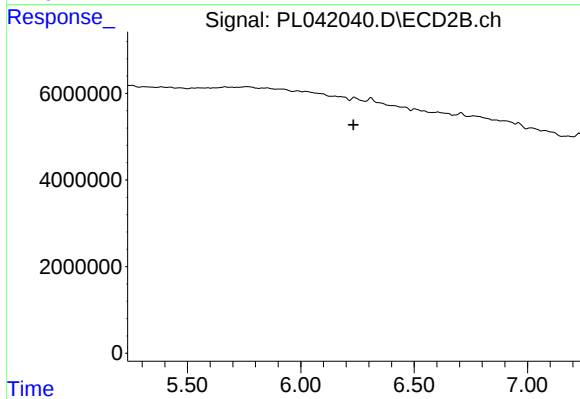

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.233 min
Response: 0
Conc: N.D.

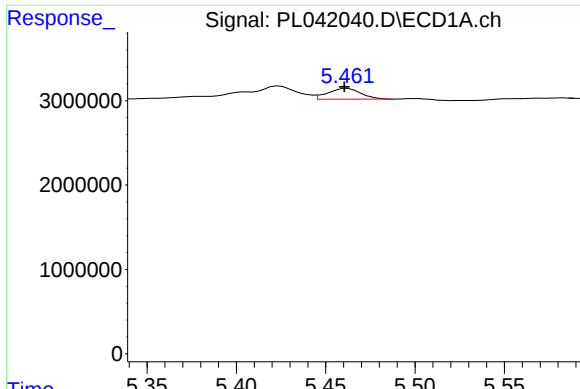

#11 alpha-Chlordane


R.T.: 5.462 min
Delta R.T.: 0.002 min
Response: 1651427
Conc: 0.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

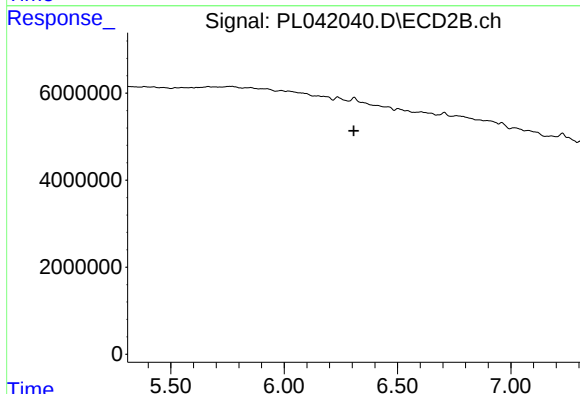


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.307 min
Response: 0
Conc: N.D.

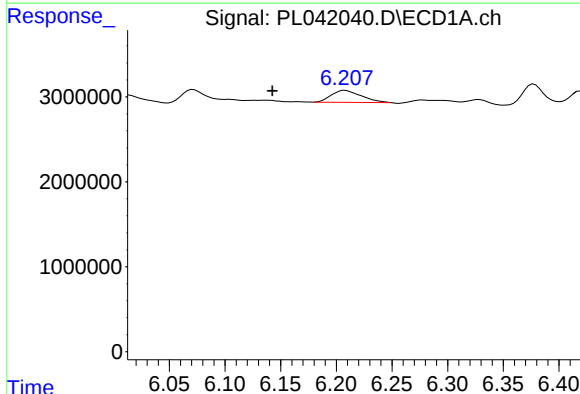


#16 4,4'-DDD

R.T.: 6.208 min
Delta R.T.: 0.066 min
Response: 2633786
Conc: 0.48 ng/ml

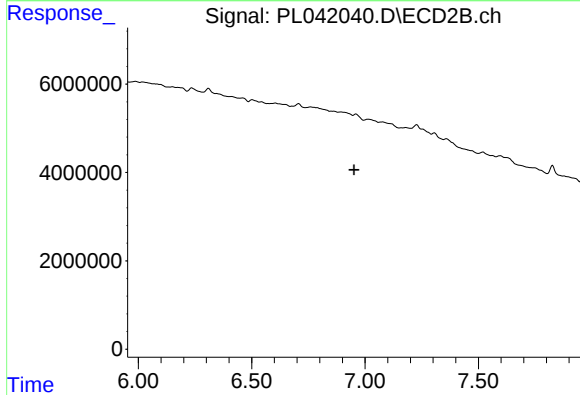

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.952 min
Response: 0
Conc: N.D.

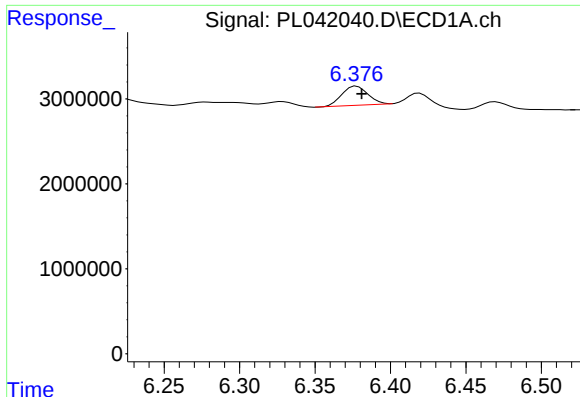

#17 4,4'-DDT


R.T.: 6.378 min
Delta R.T.: -0.003 min
Response: 2700623
Conc: 0.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

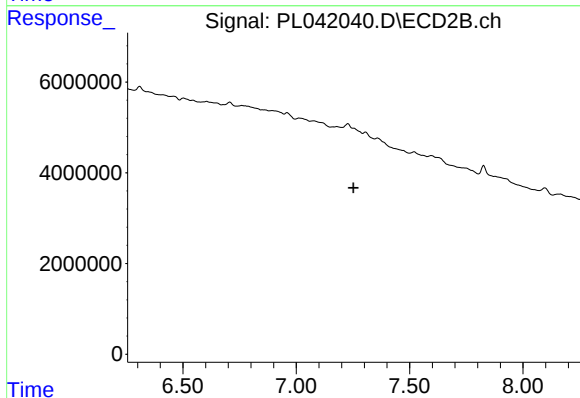


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.253 min
Response: 0
Conc: N.D.

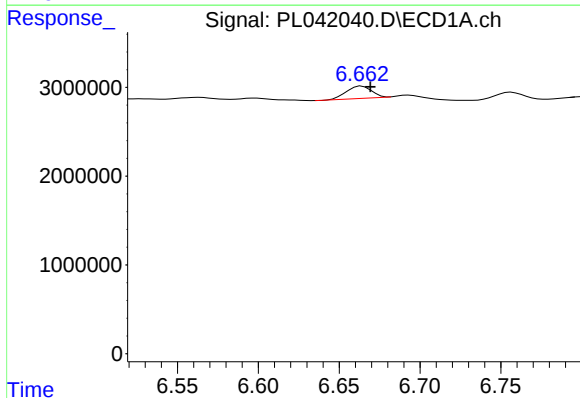


#19 Endosulfan Sulfate

R.T.: 6.664 min
Delta R.T.: -0.005 min
Response: 1486732
Conc: 0.23 ng/ml

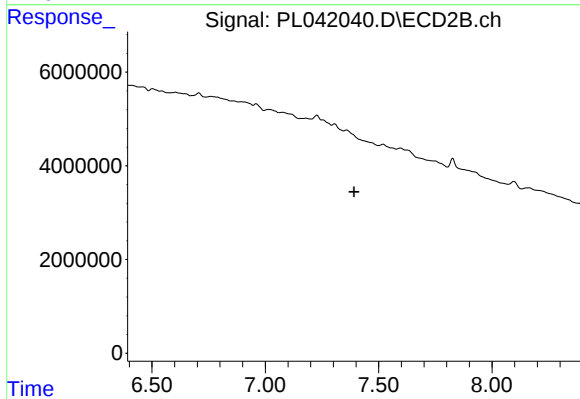

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.392 min
Response: 0
Conc: N.D.

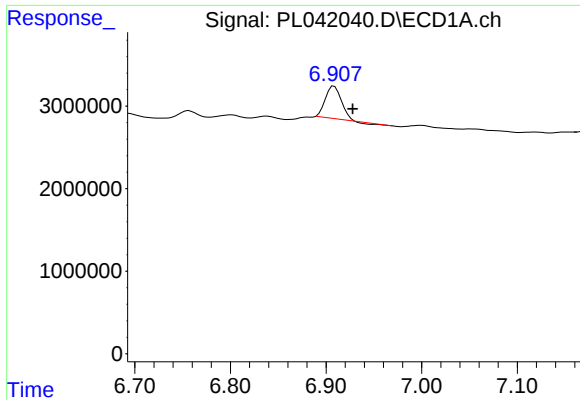

#20 Methoxychlor


R.T.: 6.908 min
Delta R.T.: -0.019 min
Response: 4279003
Conc: 1.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

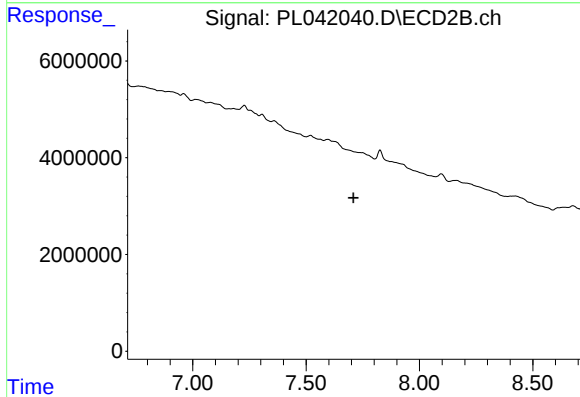


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.709 min
Response: 0
Conc: N.D.

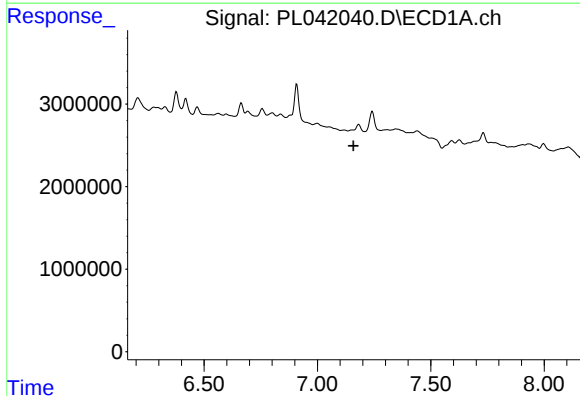


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.159 min
Response: 0
Conc: N.D.

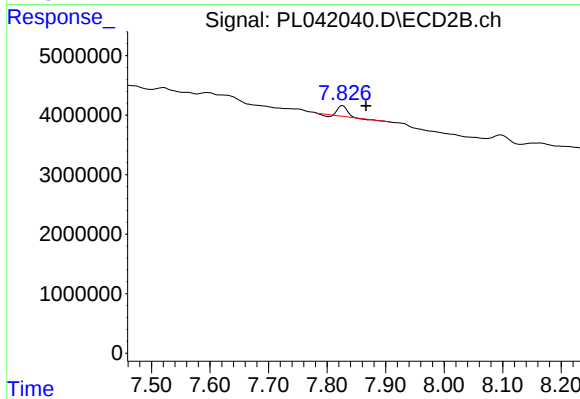

#21 Endrin ketone


R.T.: 7.827 min
Delta R.T.: -0.040 min
Response: 1627570
Conc: 0.56 ng/ml

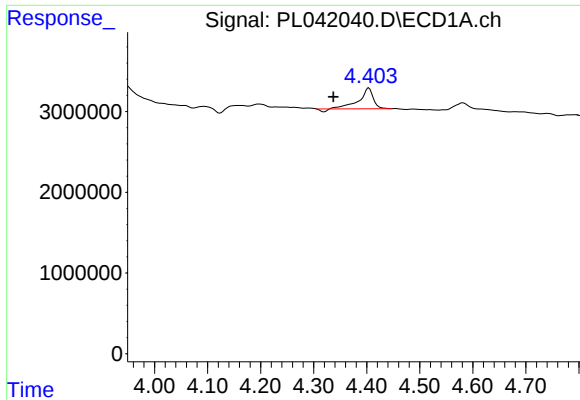

#23 Chlordane-1


R.T.: 4.404 min
Delta R.T.: 0.067 min
Response: 4742947
Conc: 15.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

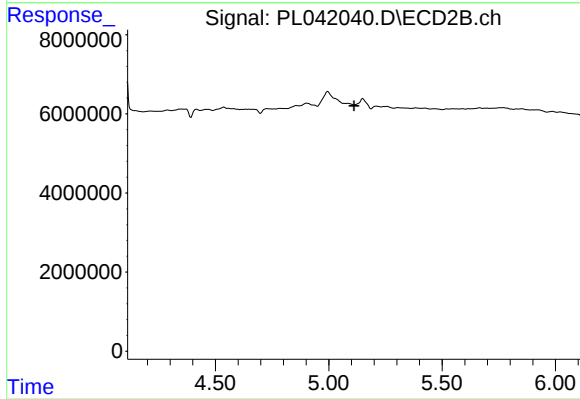


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.112 min
Response: 0
Conc: N.D.

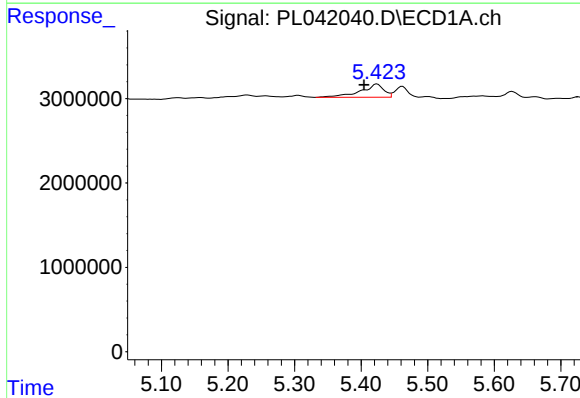


#25 Chlordane-3

R.T.: 5.424 min
Delta R.T.: 0.020 min
Response: 3780246
Conc: 4.04 ng/ml

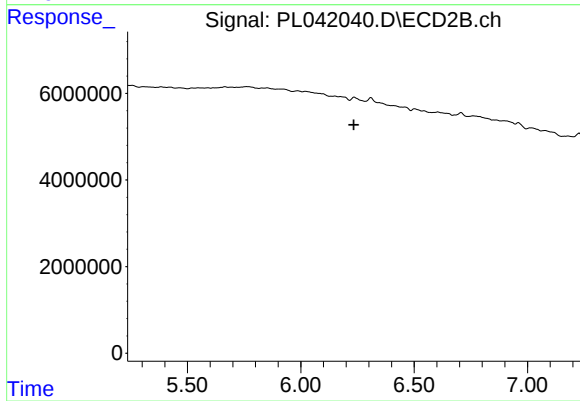

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.234 min
Response: 0
Conc: N.D.

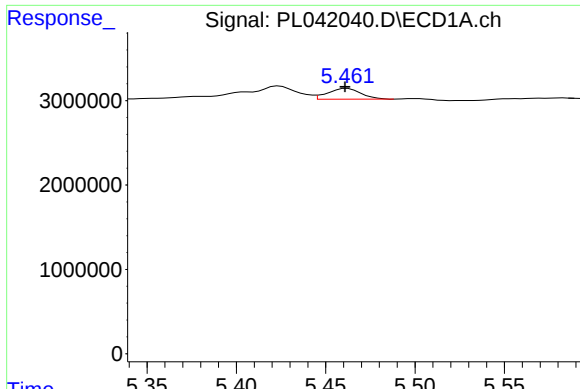

#26 Chlordane-4


R.T.: 5.462 min
Delta R.T.: 0.001 min
Response: 1651427
Conc: 1.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

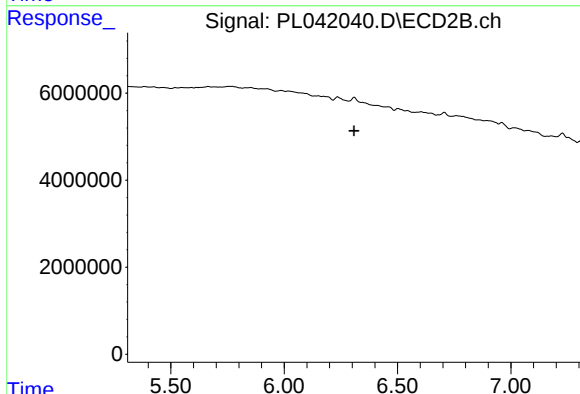


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.309 min
Response: 0
Conc: N.D.

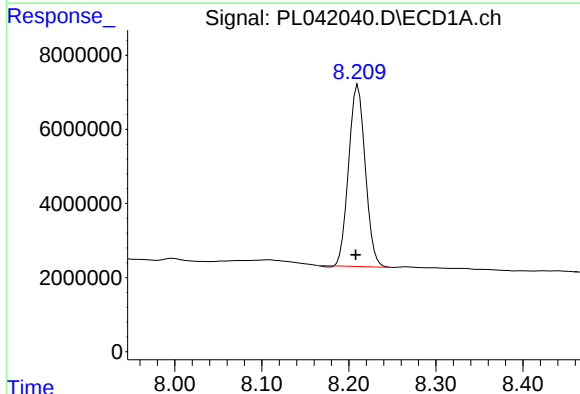

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: 0.002 min
Response: 64757684
Conc: 9.45 ng/ml

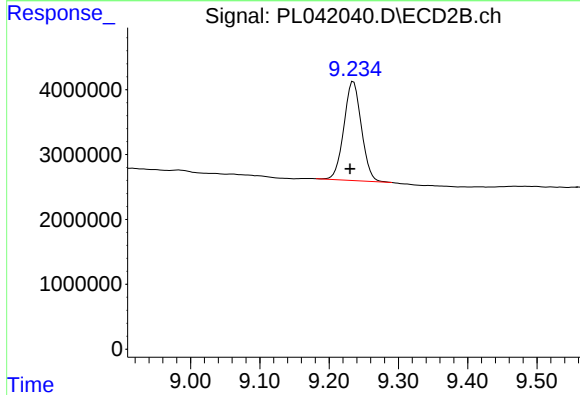

#28 Decachlorobiphenyl

R.T.: 9.235 min
Delta R.T.: 0.005 min
Response: 26717950
Conc: 10.48 ng/ml