

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110918\
 Data File : PL042041.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2018 06:30
 Operator : AJ\SJ
 Sample : J5887-15
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 02:50:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	4.103	31843689	16282315	5.157	5.496
28)	SA Decachlor...	8.211	9.235	46332279	18798698	6.763	7.370
Target Compounds							
2)	A alpha-BHC	3.864f	0.000	4997503	0	0.527	N.D. #
6)	B beta-BHC	4.404f	0.000	6269879	0	1.699	N.D. #
10)	B gamma-Chl...	5.424	0.000	1928346	0	0.239	N.D. #
11)	B alpha-Chl...	5.424f	0.000	1928346	0	0.242	N.D. #
12)	B 4,4'-DDE	5.627	0.000	1992467	0	0.291	N.D. #
23)	Chlordane-1	4.338	0.000	2584159	0	8.659	N.D. #
24)	Chlordane-2	4.839	0.000	3306970	0	10.424	N.D. #
25)	Chlordane-3	5.424	0.000	1928346	0	2.062	N.D. #
26)	Chlordane-4	5.424	0.000	1928346	0	2.308	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110918\
Data File : PL042041.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2018 06:30
Operator : AJ\SJ
Sample : J5887-15
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 02:50:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

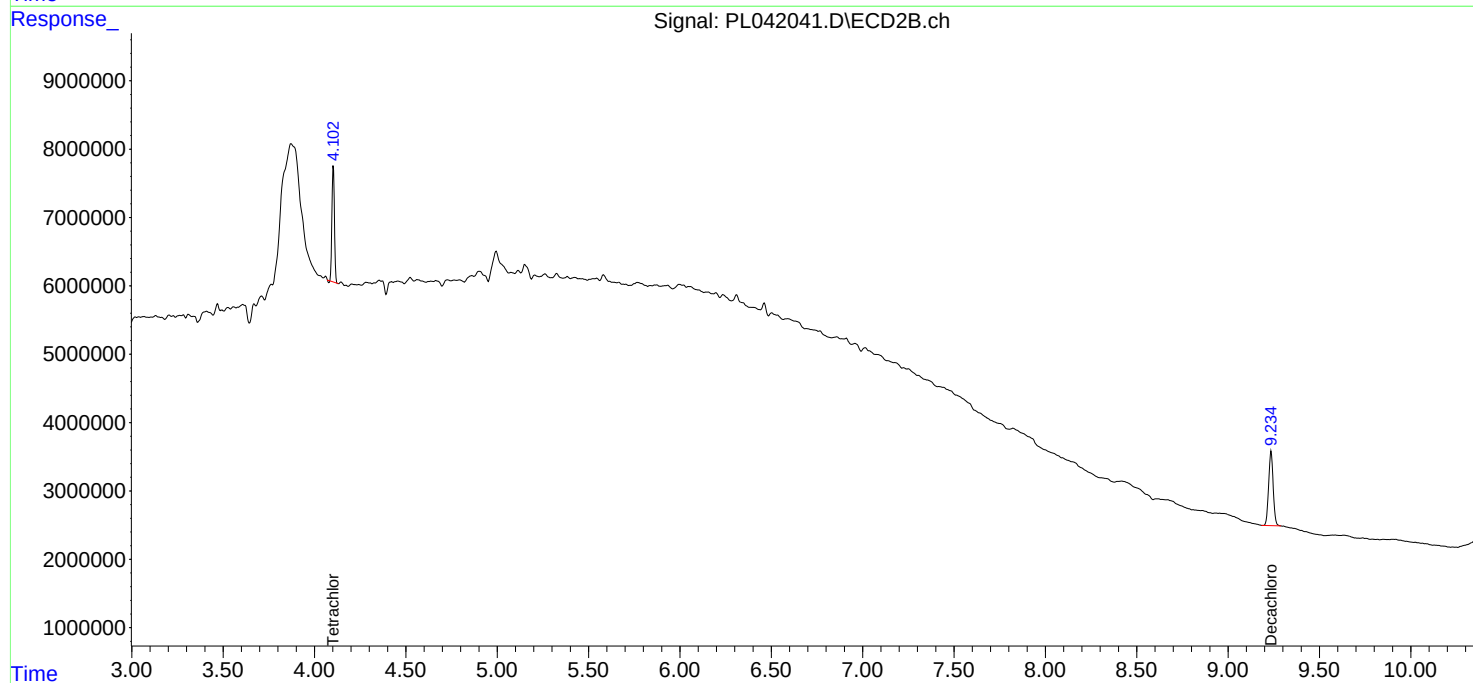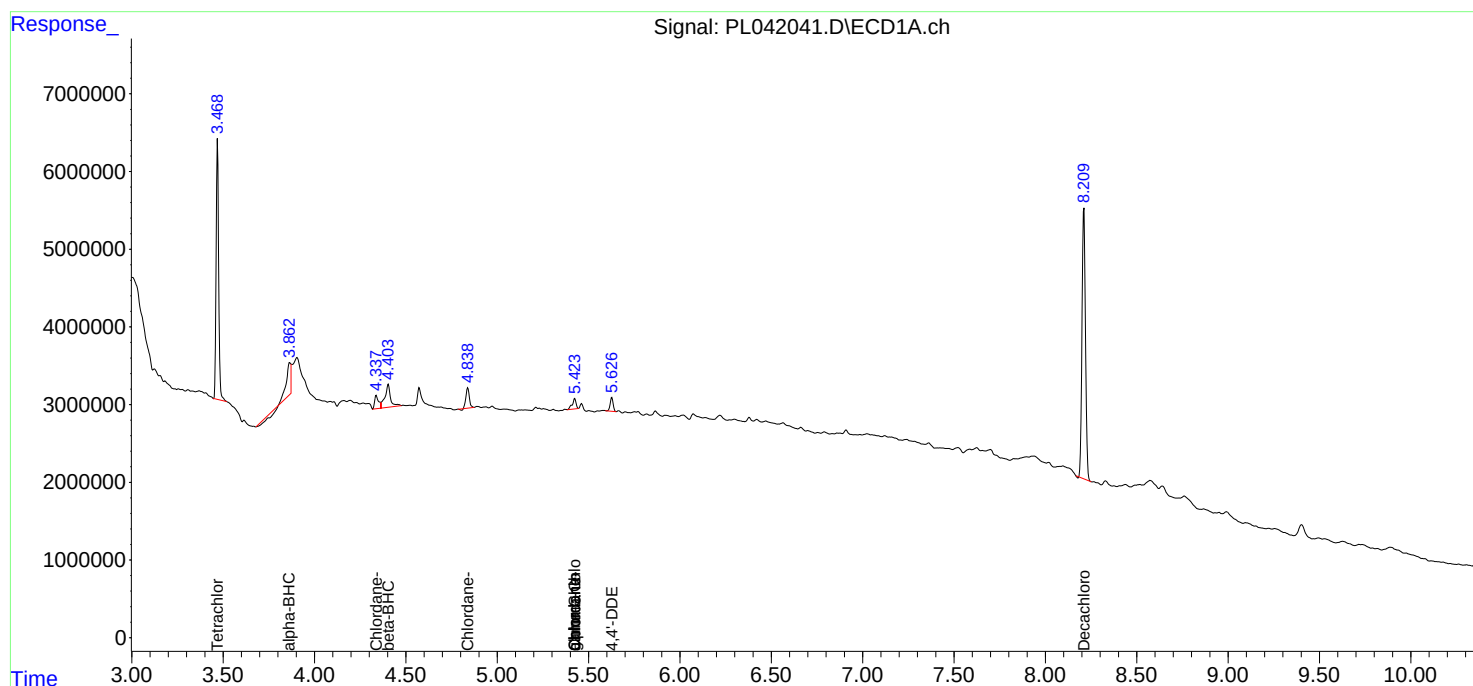


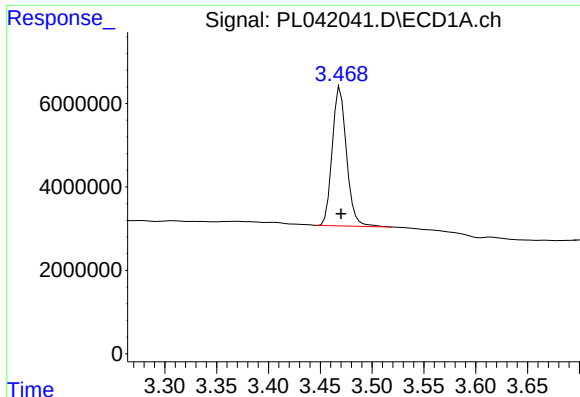

#1 Tetrachloro-m-xylene


R.T.: 3.469 min
Delta R.T.: 0.000 min
Response: 31843689
Conc: 5.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

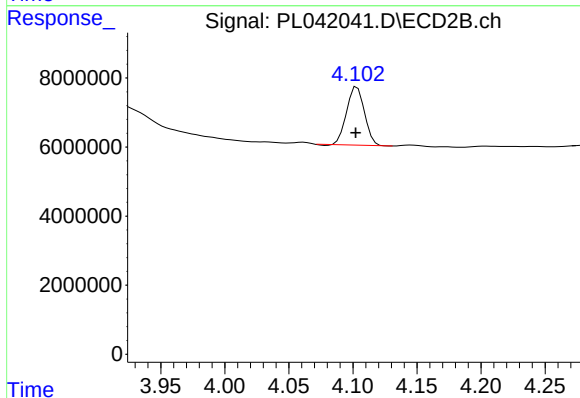


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: 0.001 min
Response: 16282315
Conc: 5.50 ng/ml

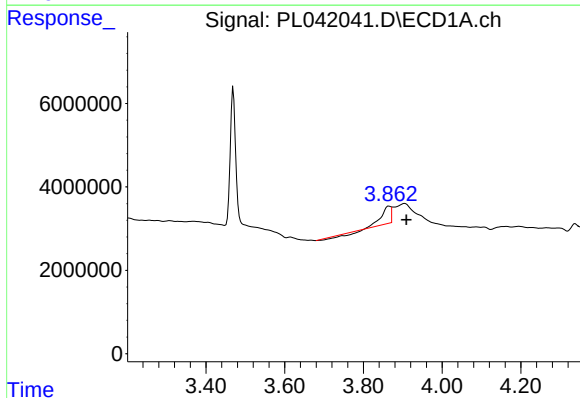


#2 alpha-BHC

R.T.: 3.864 min
Delta R.T.: -0.045 min
Response: 4997503
Conc: 0.53 ng/ml

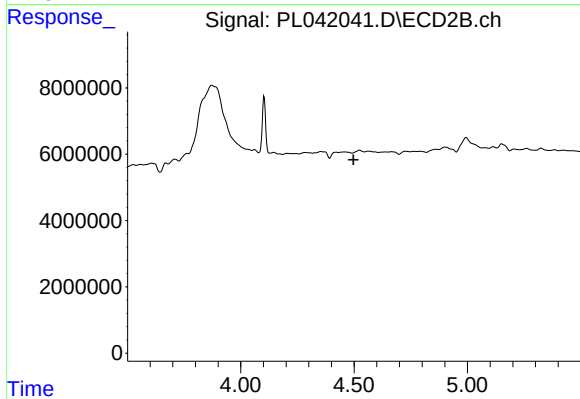

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.498 min
Response: 0
Conc: N.D.

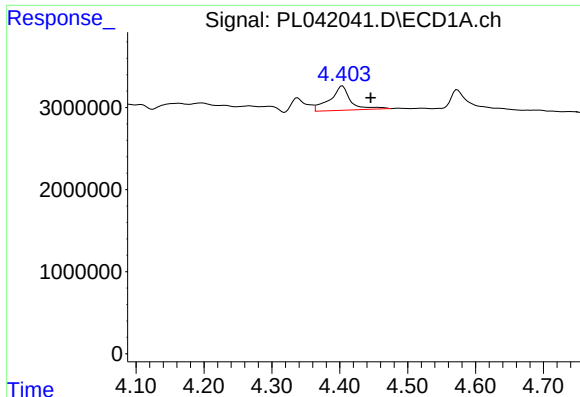

#6 beta-BHC


R.T.: 4.404 min
Delta R.T.: -0.041 min
Response: 6269879
Conc: 1.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

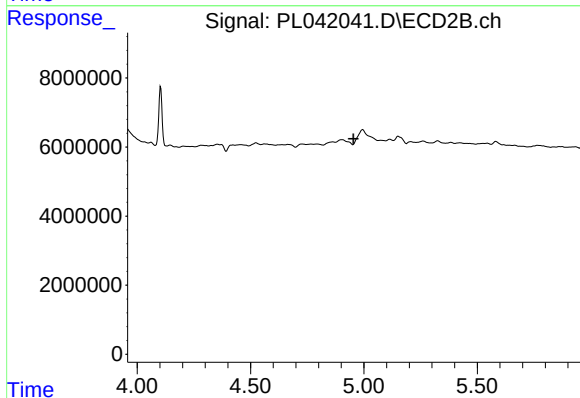


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

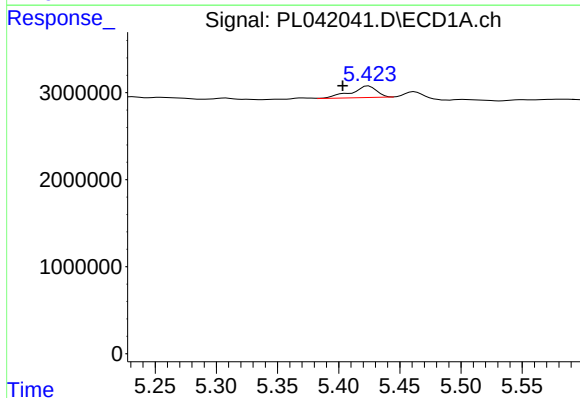


#10 gamma-Chlordane

R.T.: 5.424 min
Delta R.T.: 0.021 min
Response: 1928346
Conc: 0.24 ng/ml

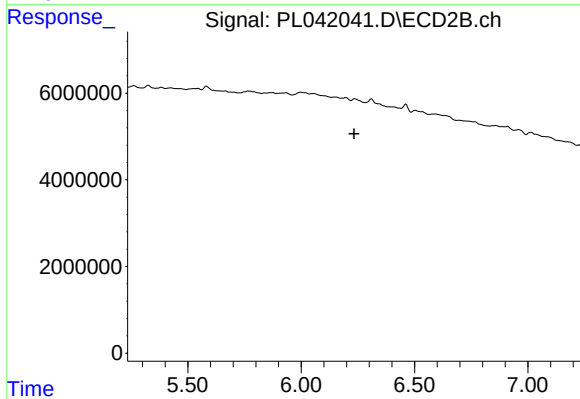

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.233 min
Response: 0
Conc: N.D.

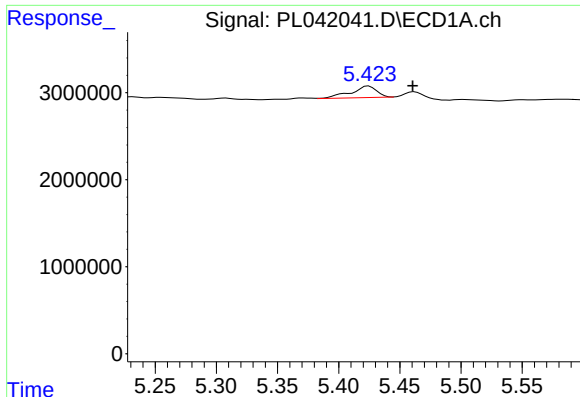

#11 alpha-Chlordane


R.T.: 5.424 min
Delta R.T.: -0.036 min
Response: 1928346
Conc: 0.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

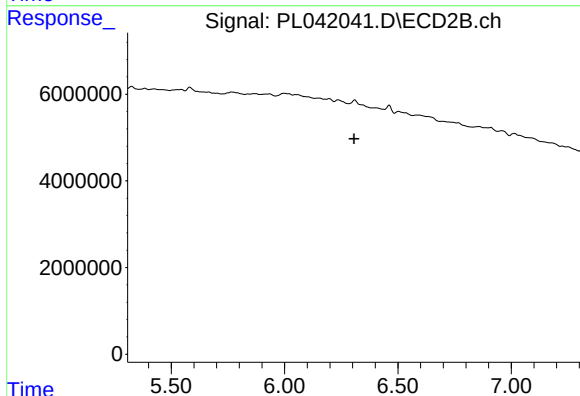


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.307 min
Response: 0
Conc: N.D.

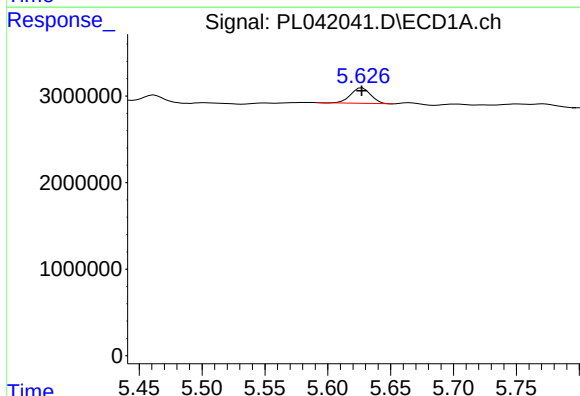


#12 4,4'-DDE

R.T.: 5.627 min
Delta R.T.: 0.000 min
Response: 1992467
Conc: 0.29 ng/ml

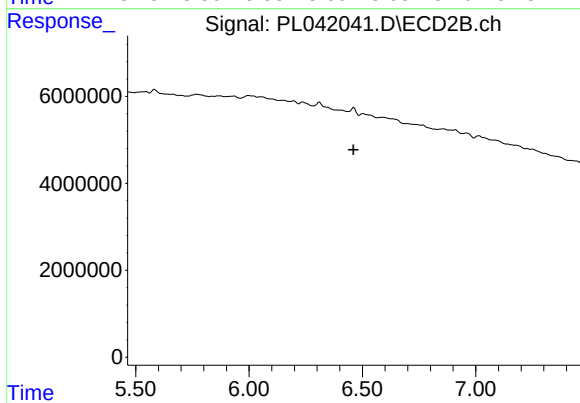

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.461 min
Response: 0
Conc: N.D.

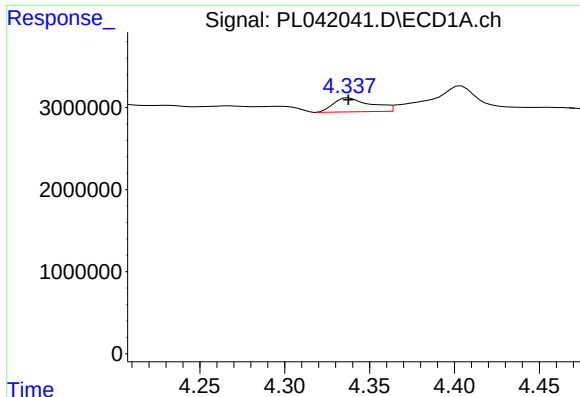

#23 Chlordane-1


R.T.: 4.338 min
Delta R.T.: 0.000 min
Response: 2584159
Conc: 8.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

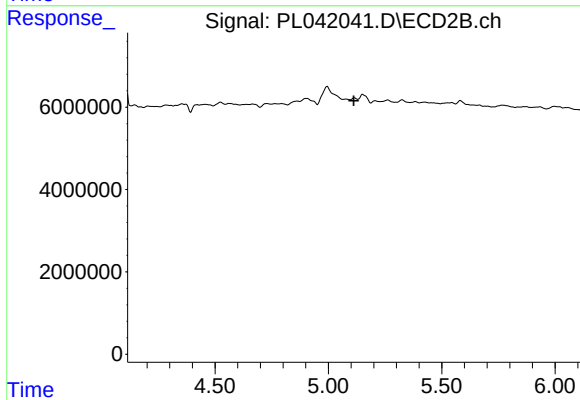


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.112 min
Response: 0
Conc: N.D.

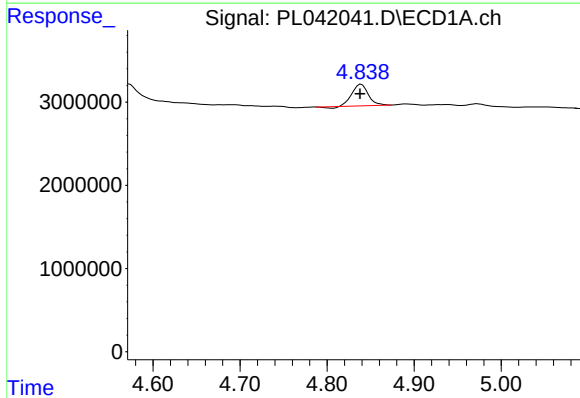


#24 Chlordane-2

R.T.: 4.839 min
Delta R.T.: 0.002 min
Response: 3306970
Conc: 10.42 ng/ml

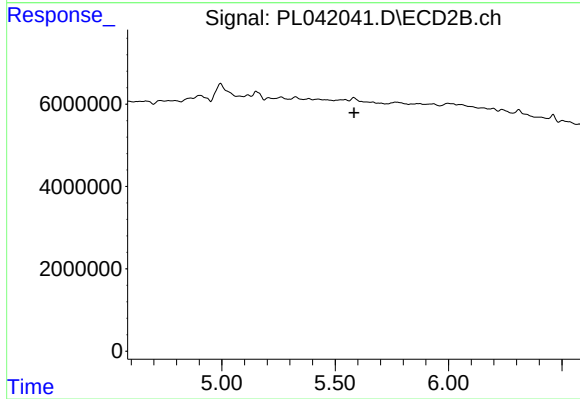

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.583 min
Response: 0
Conc: N.D.

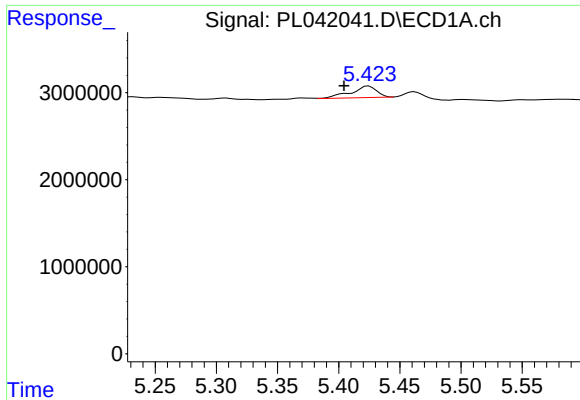

#25 Chlordane-3


R.T.: 5.424 min
Delta R.T.: 0.020 min
Response: 1928346
Conc: 2.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

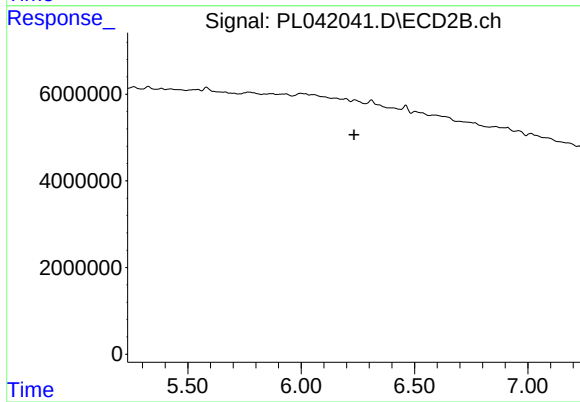


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.234 min
Response: 0
Conc: N.D.

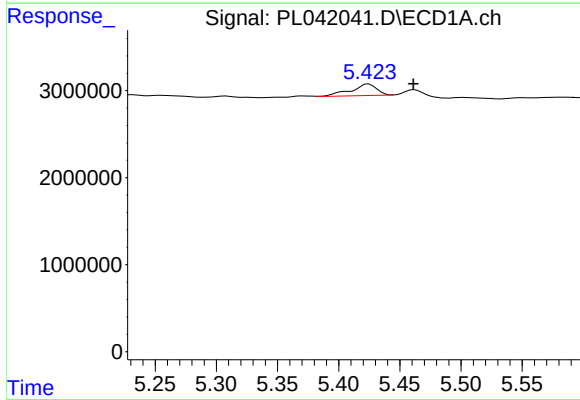


#26 Chlordane-4

R.T.: 5.424 min
Delta R.T.: -0.036 min
Response: 1928346
Conc: 2.31 ng/ml

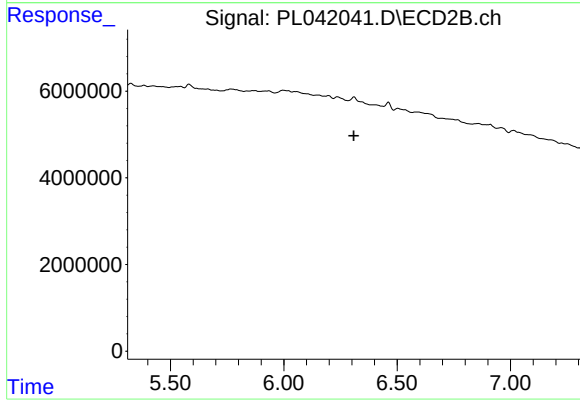

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.309 min
Response: 0
Conc: N.D.

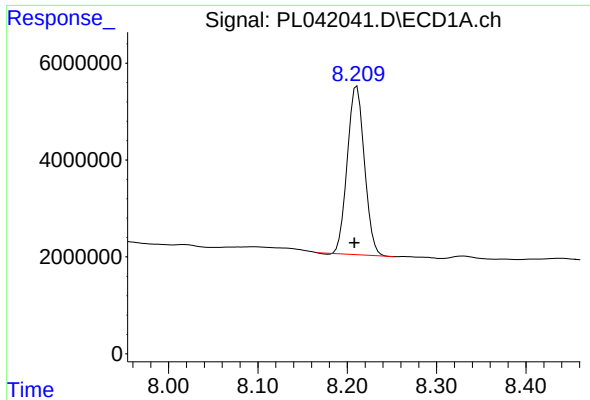

#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: 0.003 min
Response: 46332279
Conc: 6.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

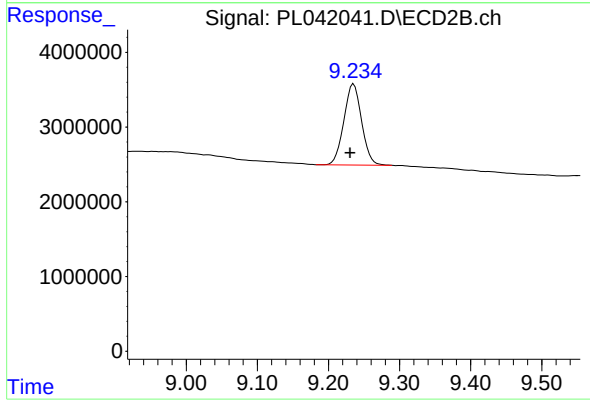

#28 Decachlorobiphenyl

R.T.: 9.235 min
Delta R.T.: 0.005 min
Response: 18798698
Conc: 7.37 ng/ml