

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110918\
 Data File : PL041960.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2018 11:27
 Operator : AJ\SJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 11:55:35 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 11:54:49 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.470	4.103	493.7E6	224.9E6	74.831	73.530
28)	SA Decachlor...	8.209	9.233	492.4E6	187.1E6	73.024	73.284
Target Compounds							
23)	Chlordane-1	4.338	5.112	224.6E6	109.5E6	755.102	743.504
24)	Chlordane-2	4.838	5.583	231.2E6	106.6E6	732.025	735.737
25)	Chlordane-3	5.405	6.234	732.3E6	381.4E6	769.548	745.254
26)	Chlordane-4	5.462	6.309	636.8E6	443.3E6	753.084	743.295
27)	Chlordane-5	6.297	7.120	200.7E6	85216375	760.415	742.647



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110918\
Data File : PL041960.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2018 11:27
Operator : AJ\SJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 11:55:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 11:54:49 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

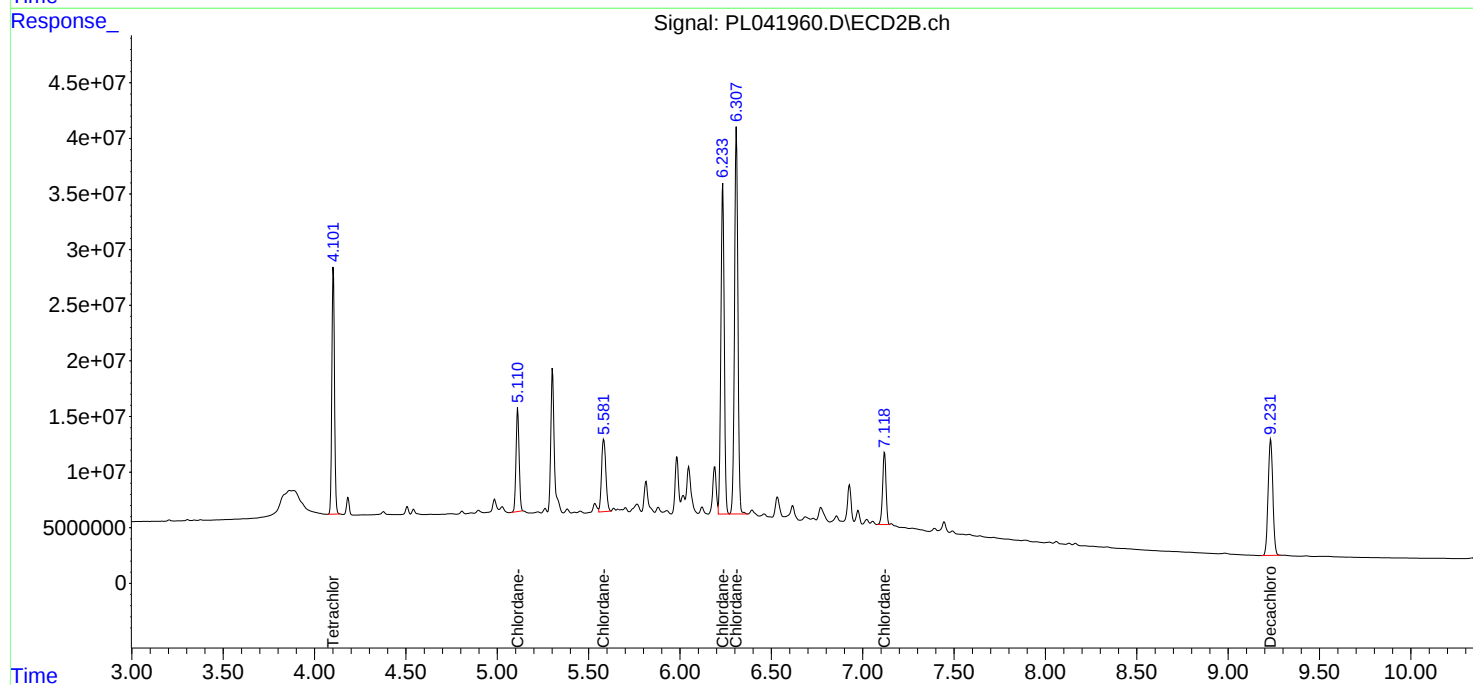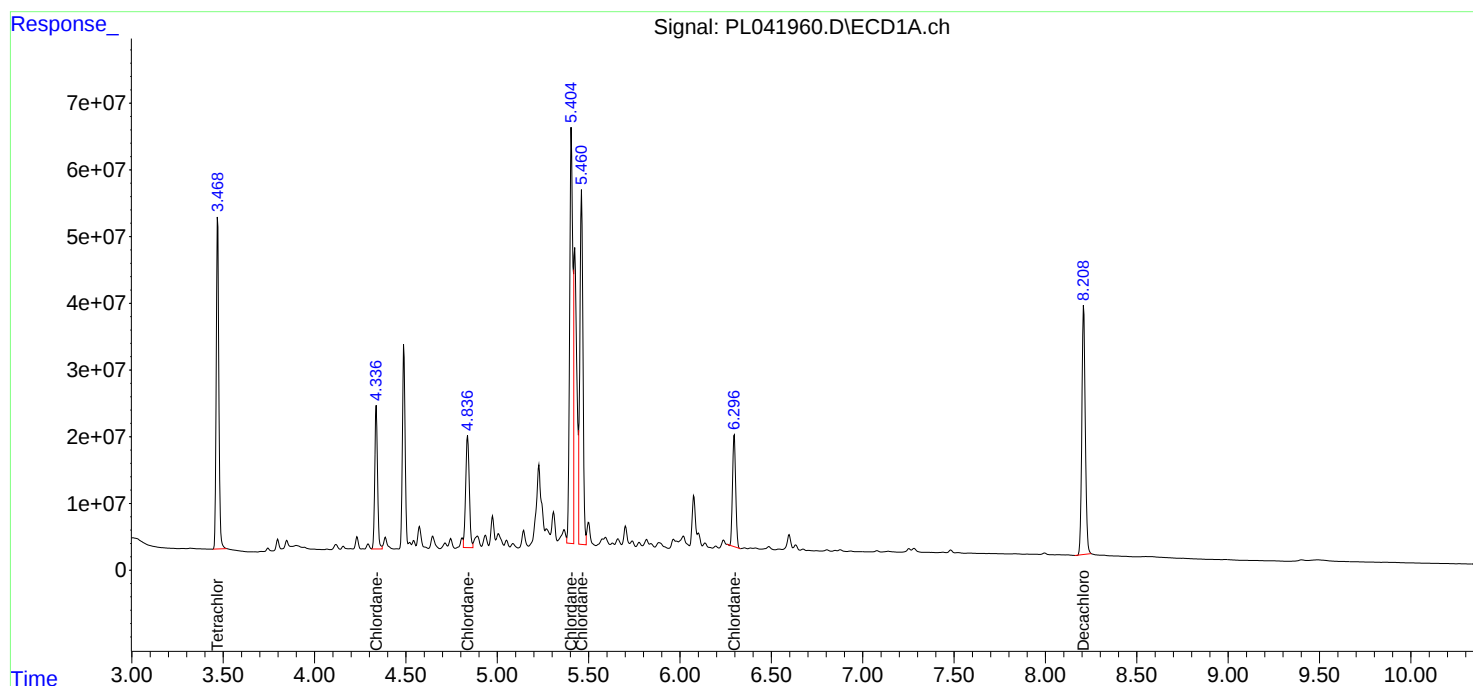


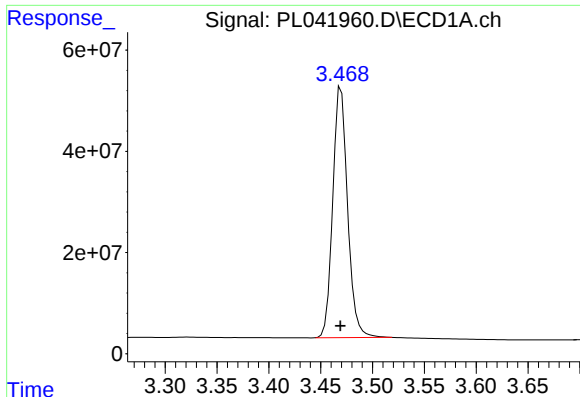

#1 Tetrachloro-m-xylene


R.T.: 3.470 min
Delta R.T.: 0.000 min
Response: 493734886
Conc: 74.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

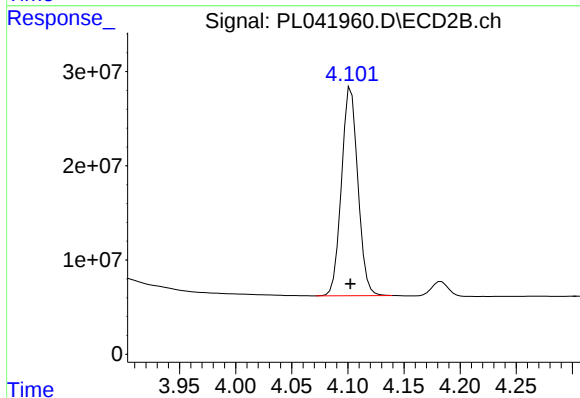


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: 0.000 min
Response: 224872880
Conc: 73.53 ng/ml

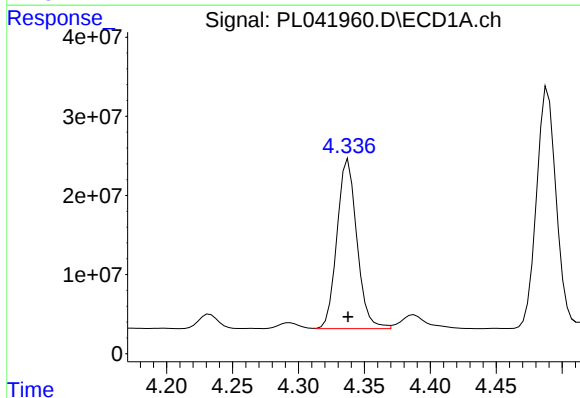


#23 Chlordane-1

R.T.: 4.338 min
Delta R.T.: 0.000 min
Response: 224641542
Conc: 755.10 ng/ml

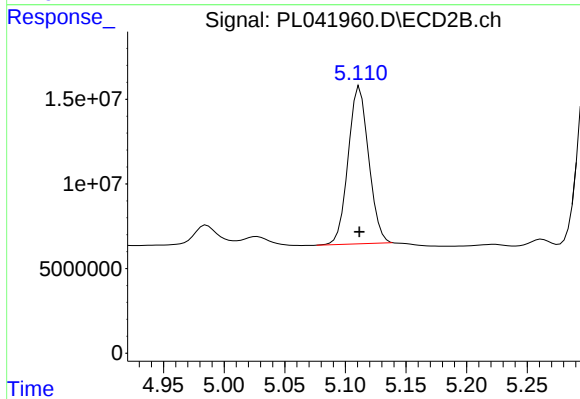

#23 Chlordane-1


R.T.: 5.112 min
Delta R.T.: 0.000 min
Response: 109473407
Conc: 743.50 ng/ml

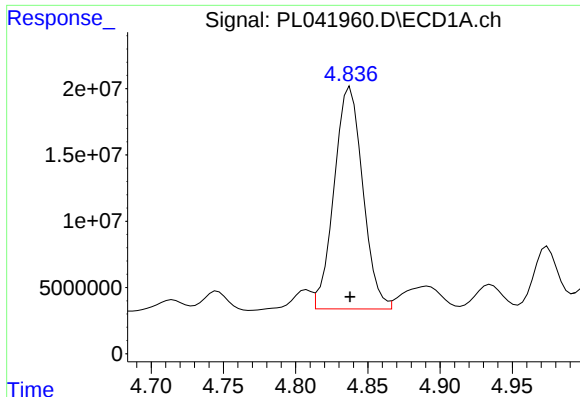

#24 Chlordane-2


R.T.: 4.838 min
Delta R.T.: 0.000 min
Response: 231157945
Conc: 732.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

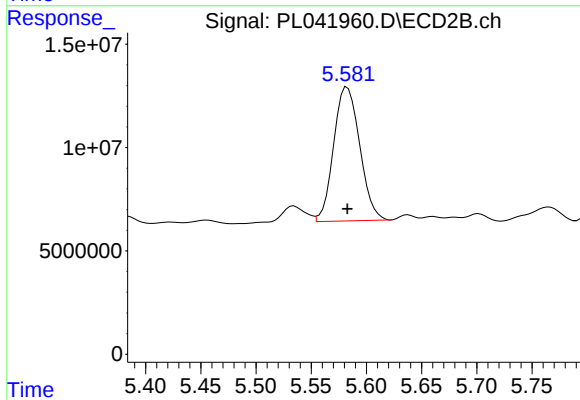


#24 Chlordane-2

R.T.: 5.583 min
Delta R.T.: 0.000 min
Response: 106626156
Conc: 735.74 ng/ml

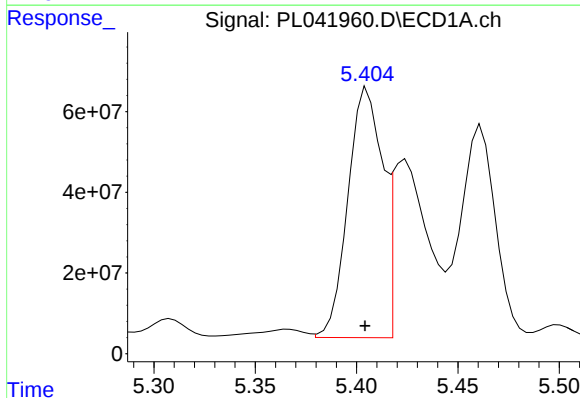


#25 Chlordane-3

R.T.: 5.405 min
Delta R.T.: 0.001 min
Response: 732329799
Conc: 769.55 ng/ml

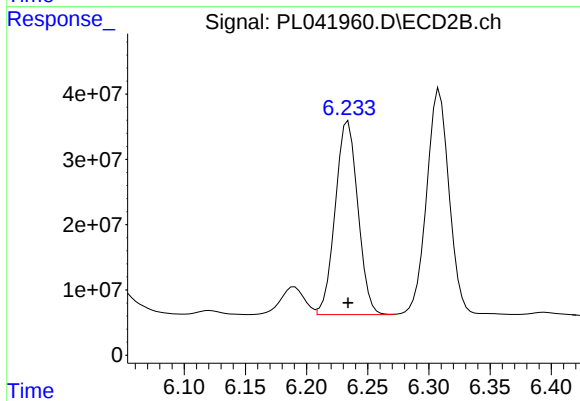

#25 Chlordane-3


R.T.: 6.234 min
Delta R.T.: 0.000 min
Response: 381420257
Conc: 745.25 ng/ml

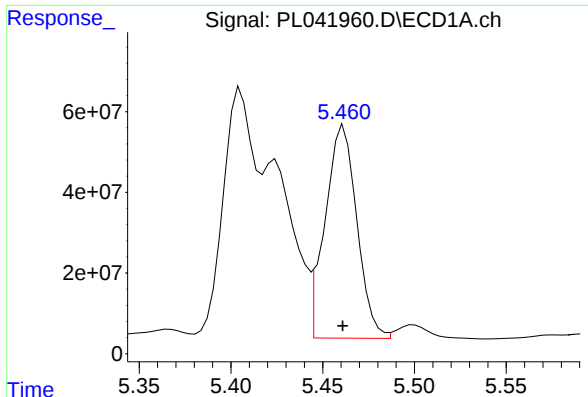

#26 Chlordane-4


R.T.: 5.462 min
Delta R.T.: 0.000 min
Response: 636771442
Conc: 753.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

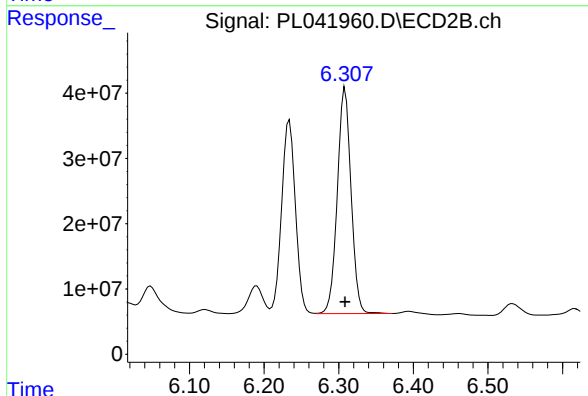


#26 Chlordane-4

R.T.: 6.309 min
Delta R.T.: 0.000 min
Response: 443290257
Conc: 743.30 ng/ml

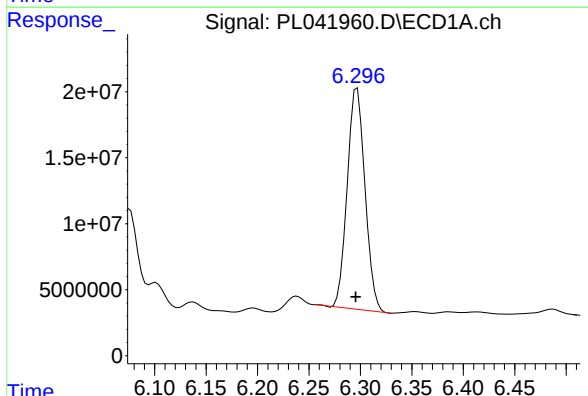


#27 Chlordane-5

R.T.: 6.297 min
Delta R.T.: 0.001 min
Response: 200706193
Conc: 760.41 ng/ml

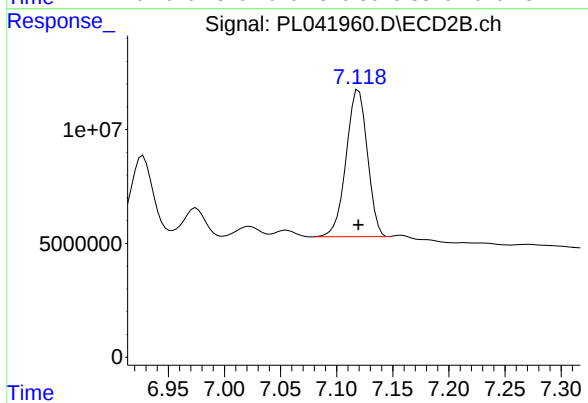

#27 Chlordane-5


R.T.: 7.120 min
Delta R.T.: 0.000 min
Response: 85216375
Conc: 742.65 ng/ml

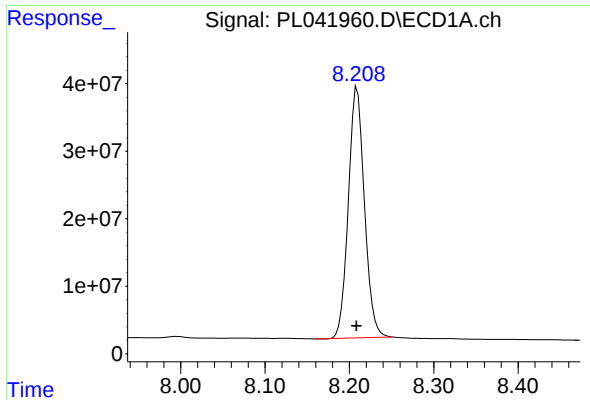

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: 0.001 min
Response: 492356407
Conc: 73.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

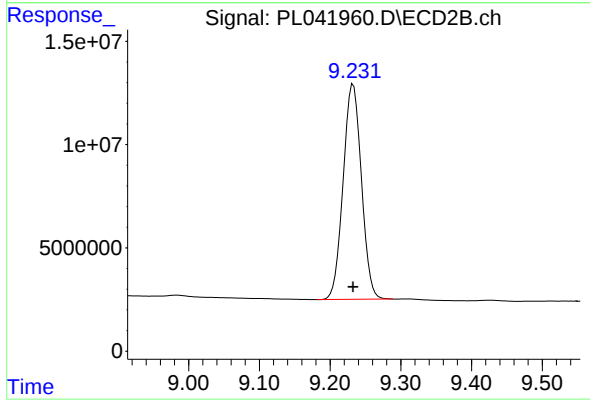

#28 Decachlorobiphenyl

R.T.: 9.233 min
Delta R.T.: 0.000 min
Response: 187129234
Conc: 73.28 ng/ml