

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110918\
 Data File : PL041961.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2018 11:41
 Operator : AJ\SJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 11:55:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 11:54:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	4.102	329.9E6	152.9E6	50.000	50.000
28)	SA Decachlor...	8.208	9.232	337.1E6	127.7E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.337	5.112	148.7E6	73619879	500.000	500.000
24)	Chlordane-2	4.838	5.583	157.9E6	72462141	500.000	500.000
25)	Chlordane-3	5.404	6.234	475.8E6	255.9E6	500.000	500.000
26)	Chlordane-4	5.461	6.309	422.8E6	298.2E6	500.000	500.000
27)	Chlordane-5	6.296	7.119	132.0E6	57373382	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110918\
Data File : PL041961.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2018 11:41
Operator : AJ\SJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 11:55:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 11:54:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

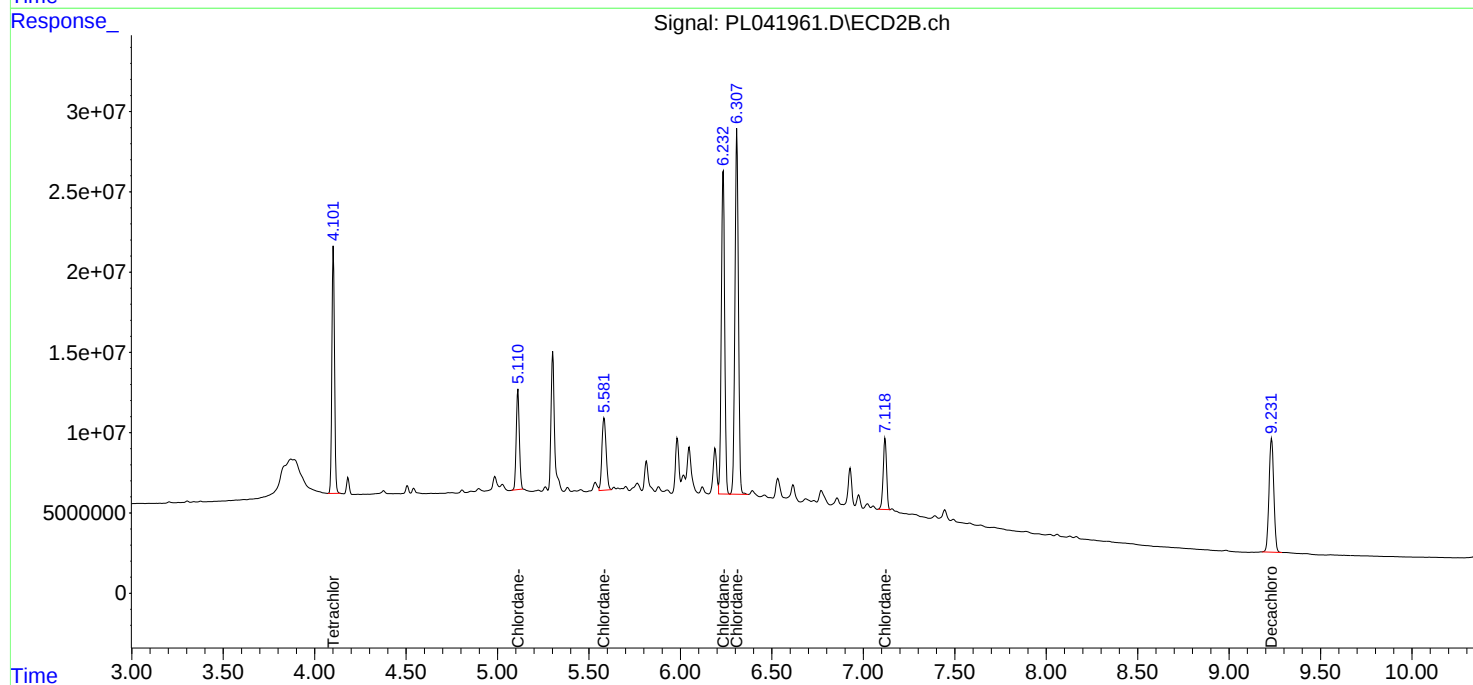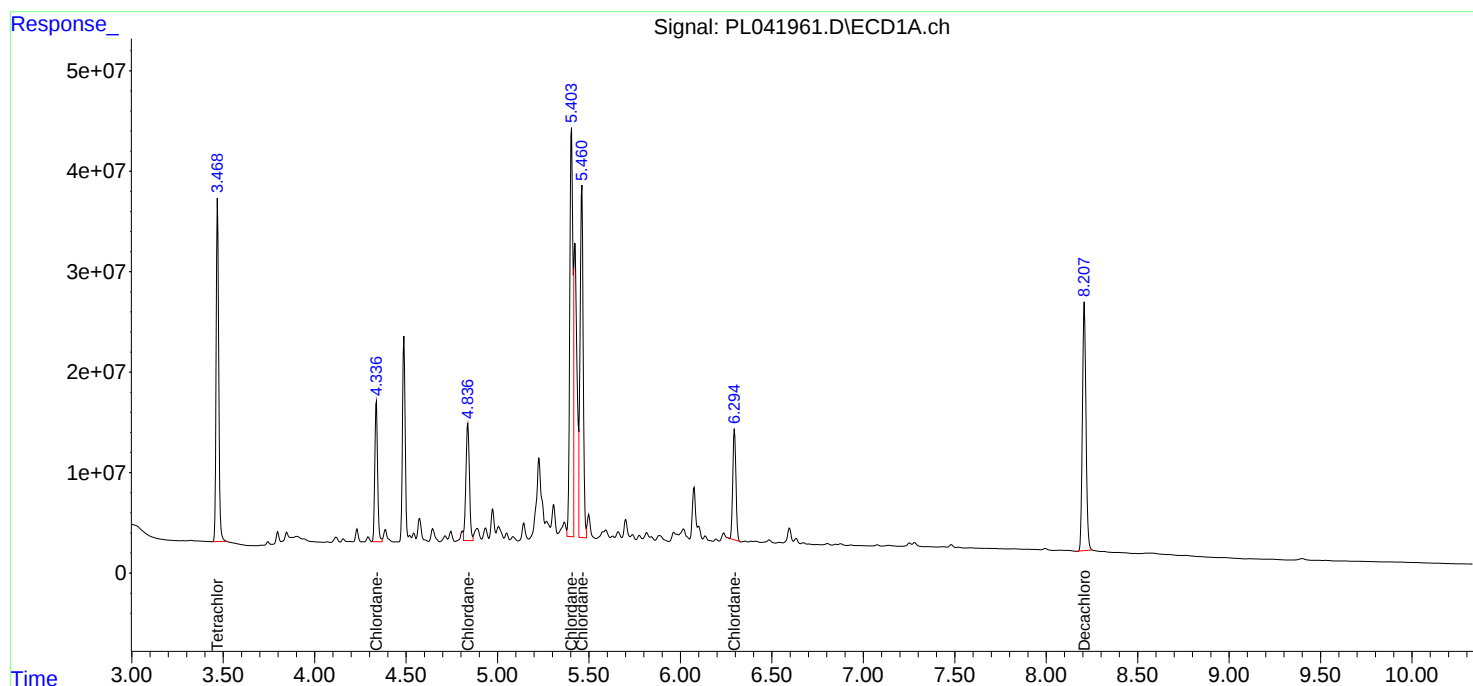


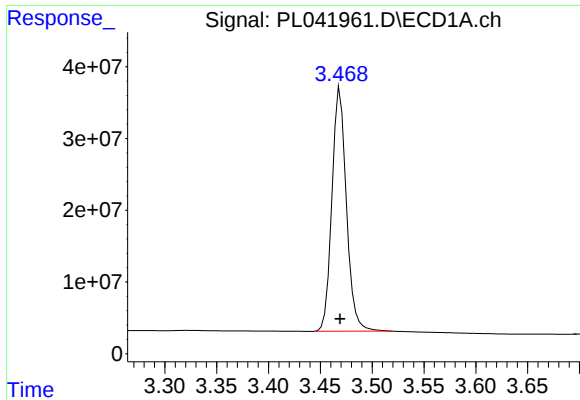

#1 Tetrachloro-m-xylene


R.T.: 3.469 min
Delta R.T.: 0.000 min
Response: 329897986
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

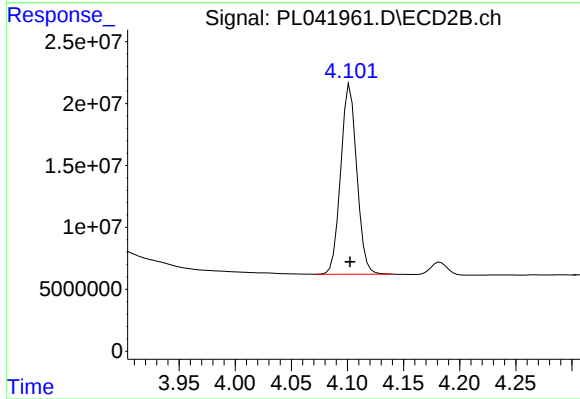


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 152912934
Conc: 50.00 ng/ml

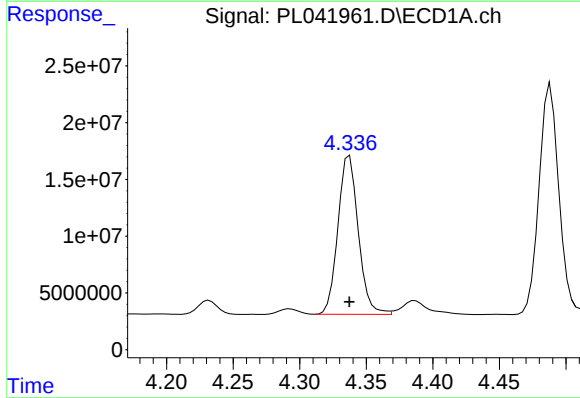


#23 Chlordane-1

R.T.: 4.337 min
Delta R.T.: 0.000 min
Response: 148749127
Conc: 500.00 ng/ml

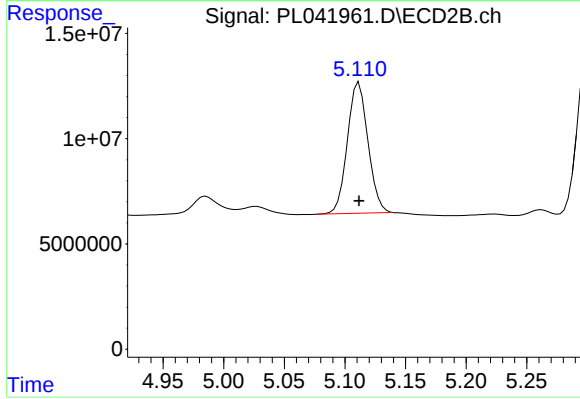

#23 Chlordane-1


R.T.: 5.112 min
Delta R.T.: 0.000 min
Response: 73619879
Conc: 500.00 ng/ml

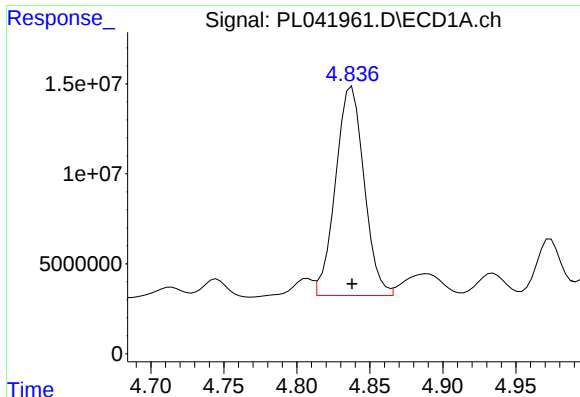

#24 Chlordane-2


R.T.: 4.838 min
Delta R.T.: 0.000 min
Response: 157889466
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

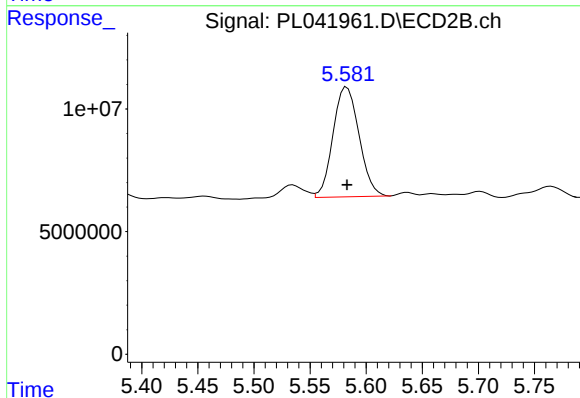


#24 Chlordane-2

R.T.: 5.583 min
Delta R.T.: 0.000 min
Response: 72462141
Conc: 500.00 ng/ml

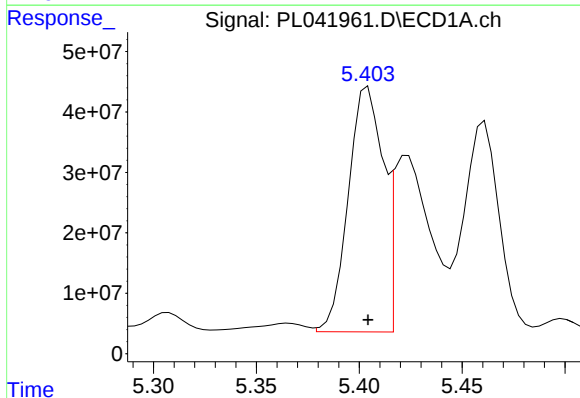


#25 Chlordane-3

R.T.: 5.404 min
Delta R.T.: 0.000 min
Response: 475818422
Conc: 500.00 ng/ml

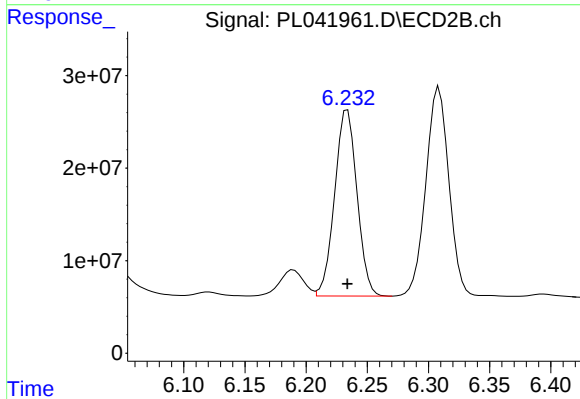

#25 Chlordane-3


R.T.: 6.234 min
Delta R.T.: 0.000 min
Response: 255899342
Conc: 500.00 ng/ml

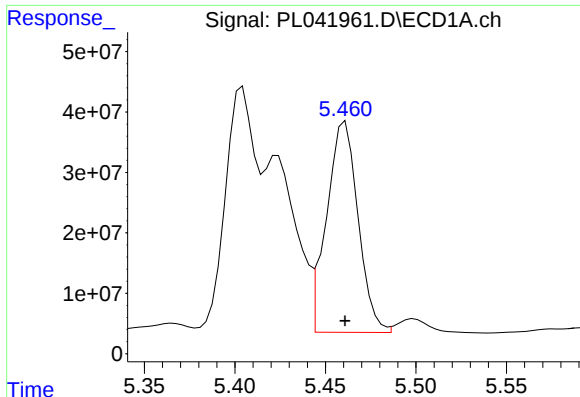

#26 Chlordane-4


R.T.: 5.461 min
Delta R.T.: 0.000 min
Response: 422775884
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

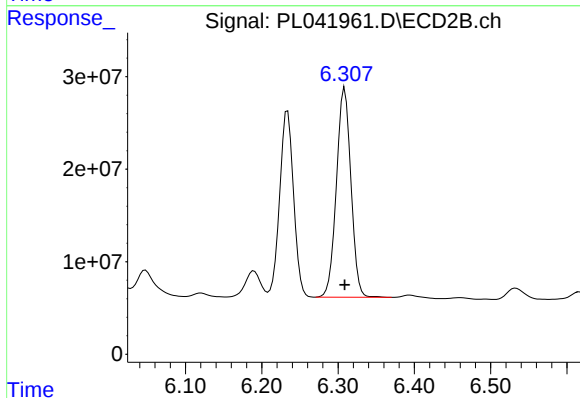


#26 Chlordane-4

R.T.: 6.309 min
Delta R.T.: 0.000 min
Response: 298192671
Conc: 500.00 ng/ml

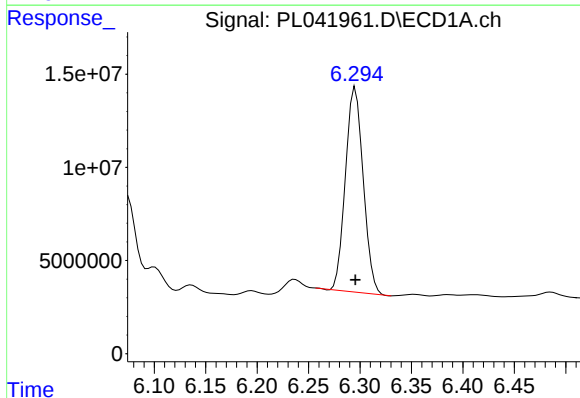


#27 Chlordane-5

R.T.: 6.296 min
Delta R.T.: 0.000 min
Response: 131971491
Conc: 500.00 ng/ml

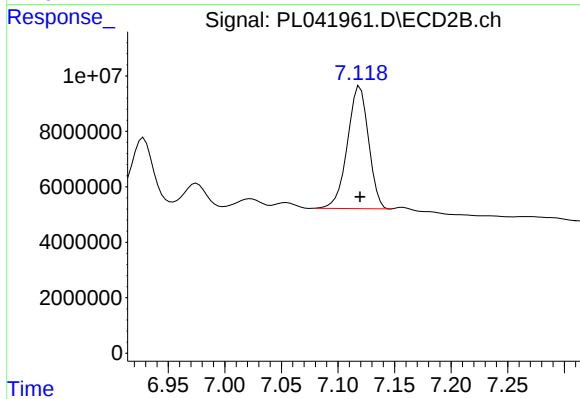

#27 Chlordane-5


R.T.: 7.119 min
Delta R.T.: 0.000 min
Response: 57373382
Conc: 500.00 ng/ml

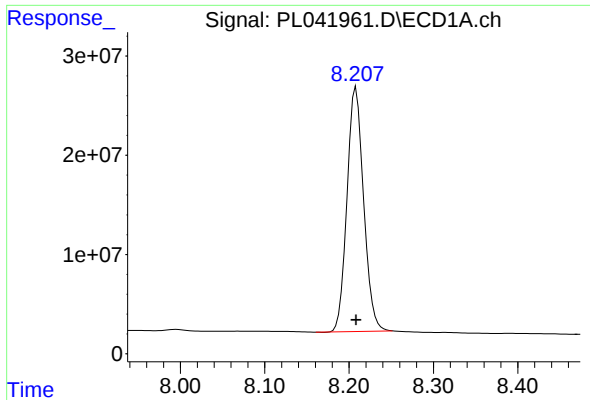

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: 0.000 min
Response: 337119613
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

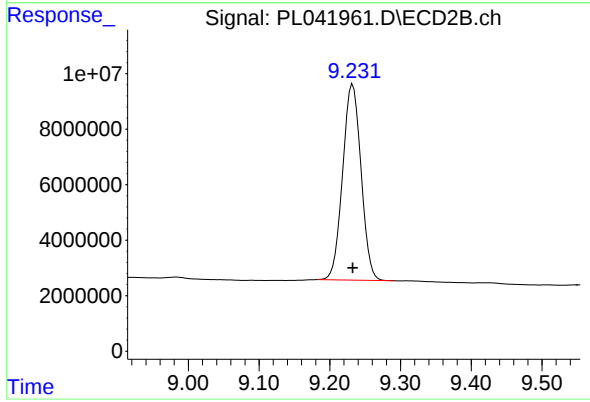

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.000 min
Response: 127673785
Conc: 50.00 ng/ml