

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110918\
 Data File : PL041963.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2018 12:09
 Operator : AJ\SJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Manual Integrations
 APPROVED

Sohil
 11/12/2018 1:46:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 12:35:03 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:09:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	4.102	33173895	15907349	5.114	5.317
28)	SA Decachlor...	8.208	9.232	40565984	14214476	6.105	5.654
Target Compounds							
23)	Chlordane-1	4.337	5.111	15646879	7049426	53.073	48.708
24)	Chlordane-2	4.836	5.582	17101919	7971766	54.985m	56.064
25)	Chlordane-3	5.404	6.233	45090401	26716083	47.804	52.926
26)	Chlordane-4	5.461	6.308	41997011	31684254	50.332	53.887
27)	Chlordane-5	6.296	7.119	13168492	6508950	50.338	57.164

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110918\
Data File : PL041963.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2018 12:09
Operator : AJ\SJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PCHLORICC050


Manual Integrations
APPROVED

Sohil
11/12/2018 1:46:23 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 12:35:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:09:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

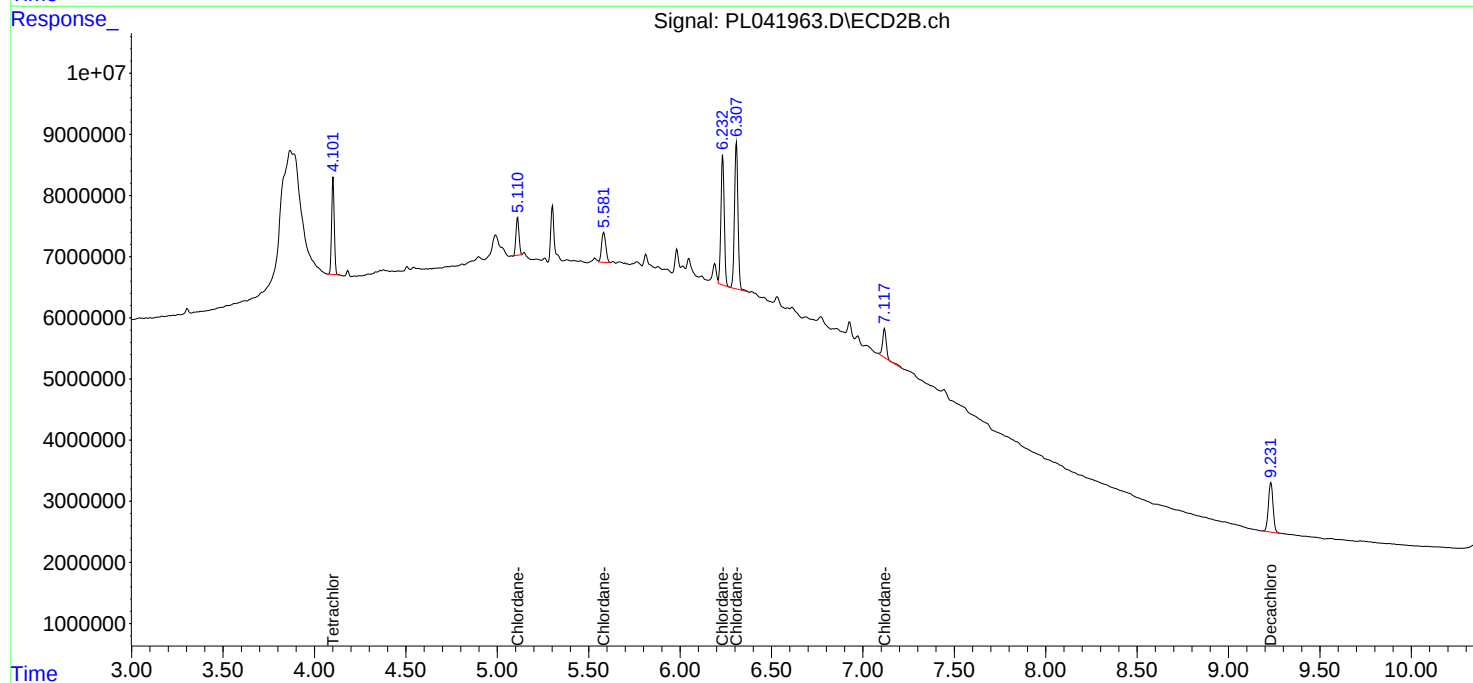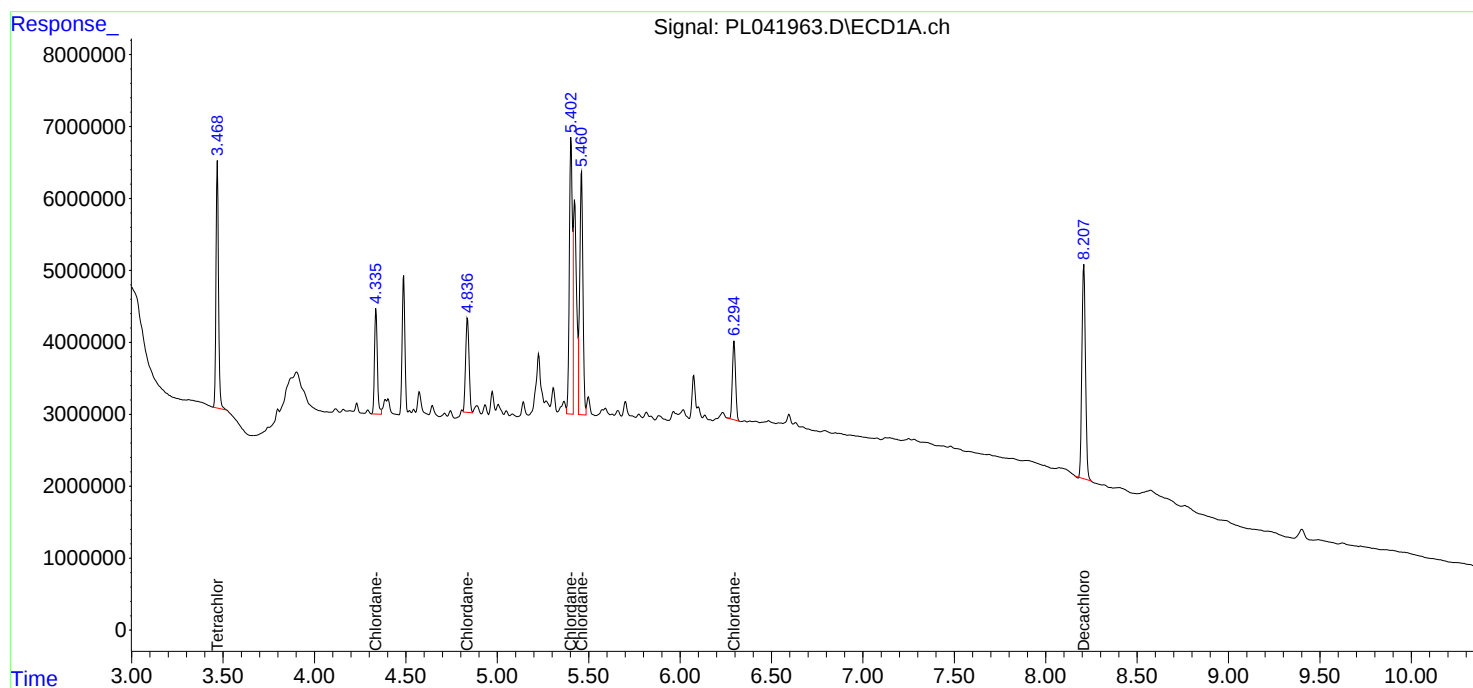

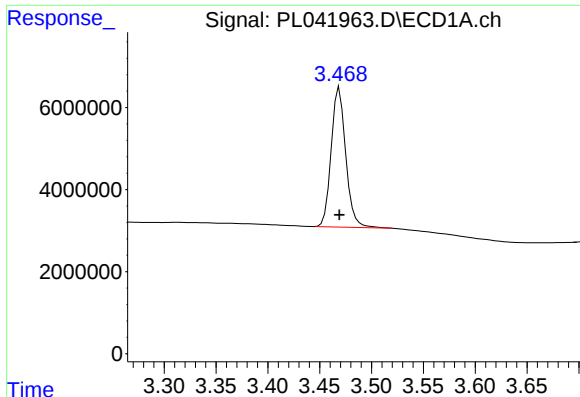


#1 Tetrachloro-m-xylene

R.T.: 3.469 min
Delta R.T.: 0.000 min
Response: 33173895
Conc: 5.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050


Manual Integrations
APPROVED

Sohil
11/12/2018 1:46:23 PM

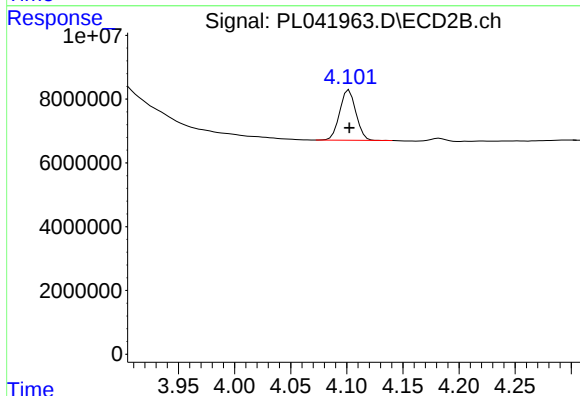


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 15907349
Conc: 5.32 ng/ml

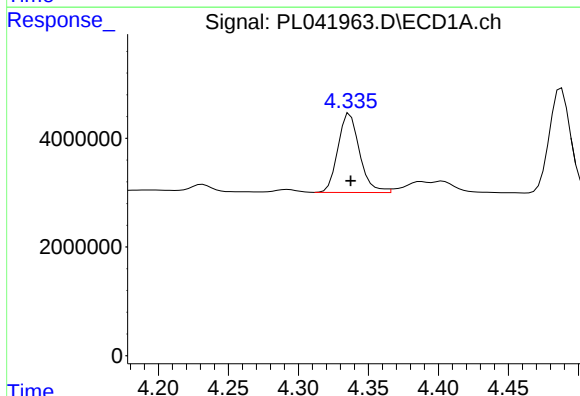


#23 Chlordane-1

R.T.: 4.337 min
Delta R.T.: 0.000 min
Response: 15646879
Conc: 53.07 ng/ml

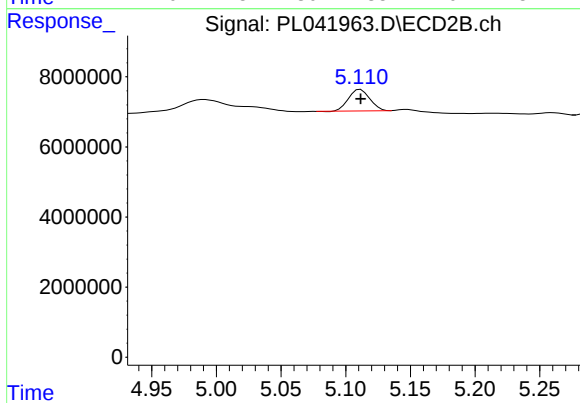

#23 Chlordane-1

R.T.: 5.111 min
Delta R.T.: 0.000 min
Response: 7049426
Conc: 48.71 ng/ml

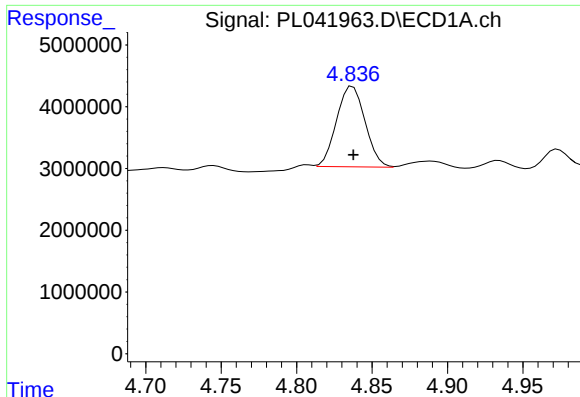


#24 Chlordane-2

R.T.: 4.836 min
Delta R.T.: -0.002 min
Response: 17101919
Conc: 54.98 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050


Manual Integrations
APPROVED

Sohil
11/12/2018 1:46:23 PM

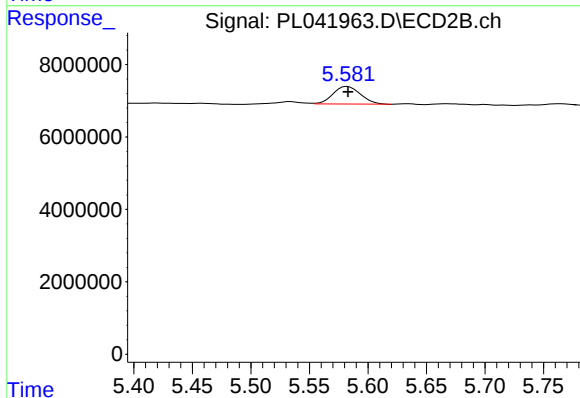


#24 Chlordane-2

R.T.: 5.582 min
Delta R.T.: 0.000 min
Response: 7971766
Conc: 56.06 ng/ml

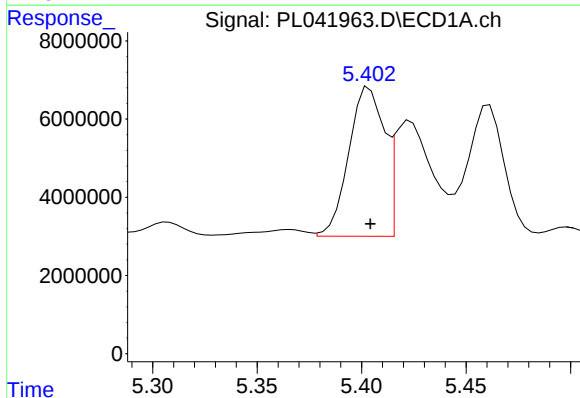


#25 Chlordane-3

R.T.: 5.404 min
Delta R.T.: 0.000 min
Response: 45090401
Conc: 47.80 ng/ml

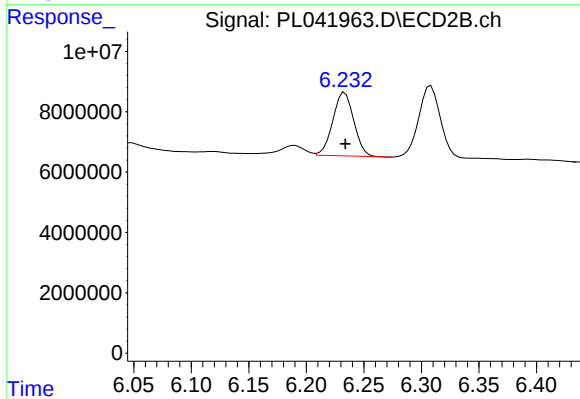

#25 Chlordane-3

R.T.: 6.233 min
Delta R.T.: 0.000 min
Response: 26716083
Conc: 52.93 ng/ml

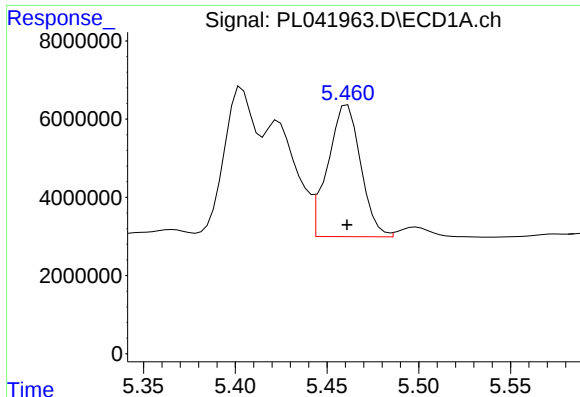


#26 Chlordane-4

R.T.: 5.461 min
Delta R.T.: 0.000 min
Response: 41997011
Conc: 50.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050


Manual Integrations
APPROVED

Sohil
11/12/2018 1:46:23 PM

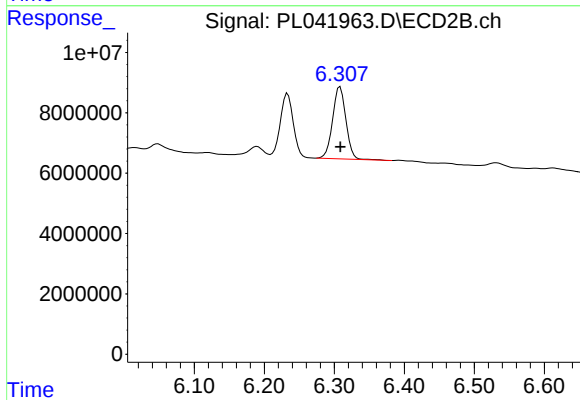


#26 Chlordane-4

R.T.: 6.308 min
Delta R.T.: 0.000 min
Response: 31684254
Conc: 53.89 ng/ml

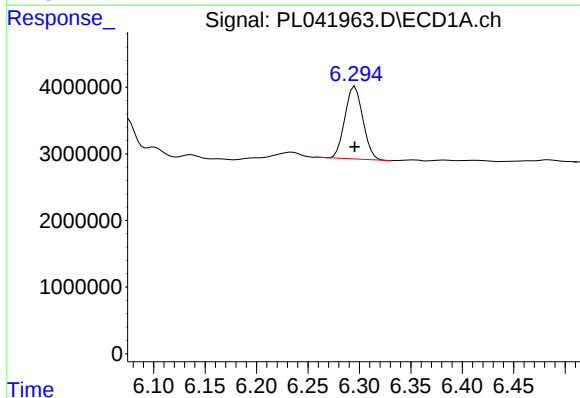


#27 Chlordane-5

R.T.: 6.296 min
Delta R.T.: 0.000 min
Response: 13168492
Conc: 50.34 ng/ml

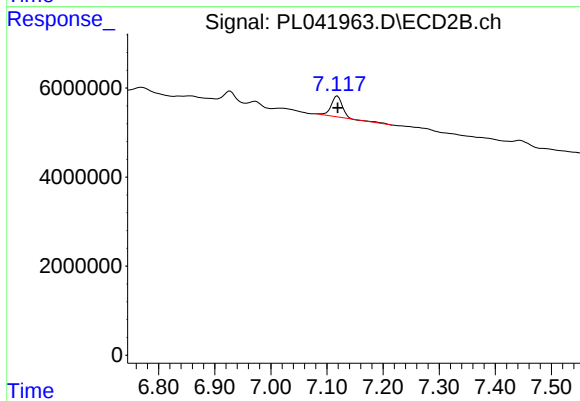

#27 Chlordane-5

R.T.: 7.119 min
Delta R.T.: 0.000 min
Response: 6508950
Conc: 57.16 ng/ml

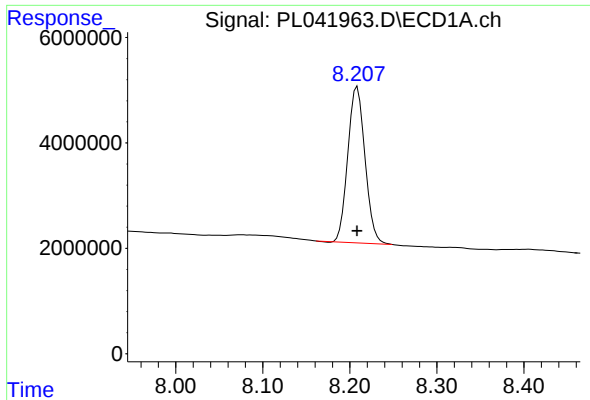


#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: 0.000 min
Response: 40565984
Conc: 6.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

Manual Integrations
APPROVED

Sohil
11/12/2018 1:46:23 PM

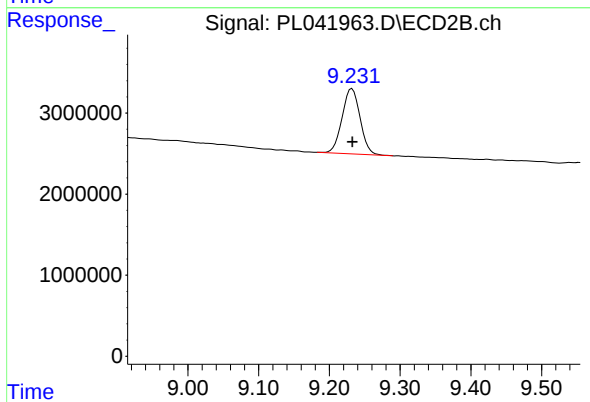

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.000 min
Response: 14214476
Conc: 5.65 ng/ml