

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110918\
 Data File : PL041975.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2018 14:58
 Operator : AJ\SJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 21:52:34 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	4.102	326.7E6	155.8E6	52.914	52.571
28)	SA Decachlor...	8.209	9.233	327.5E6	131.6E6	47.811	51.604
Target Compounds							
23)	Chlordane-1	4.338	5.111	148.2E6	75569816	496.492	524.859
24)	Chlordane-2	4.838	5.582	156.1E6	74790588	491.915	513.534
25)	Chlordane-3	5.404	6.234	471.0E6	264.7E6	503.731	518.281
26)	Chlordane-4	5.461	6.308	413.8E6	307.6E6	495.280	515.071
27)	Chlordane-5	6.296	7.120	131.0E6	60797194	499.903	519.068



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110918\
Data File : PL041975.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2018 14:58
Operator : AJ\SJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 21:52:34 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

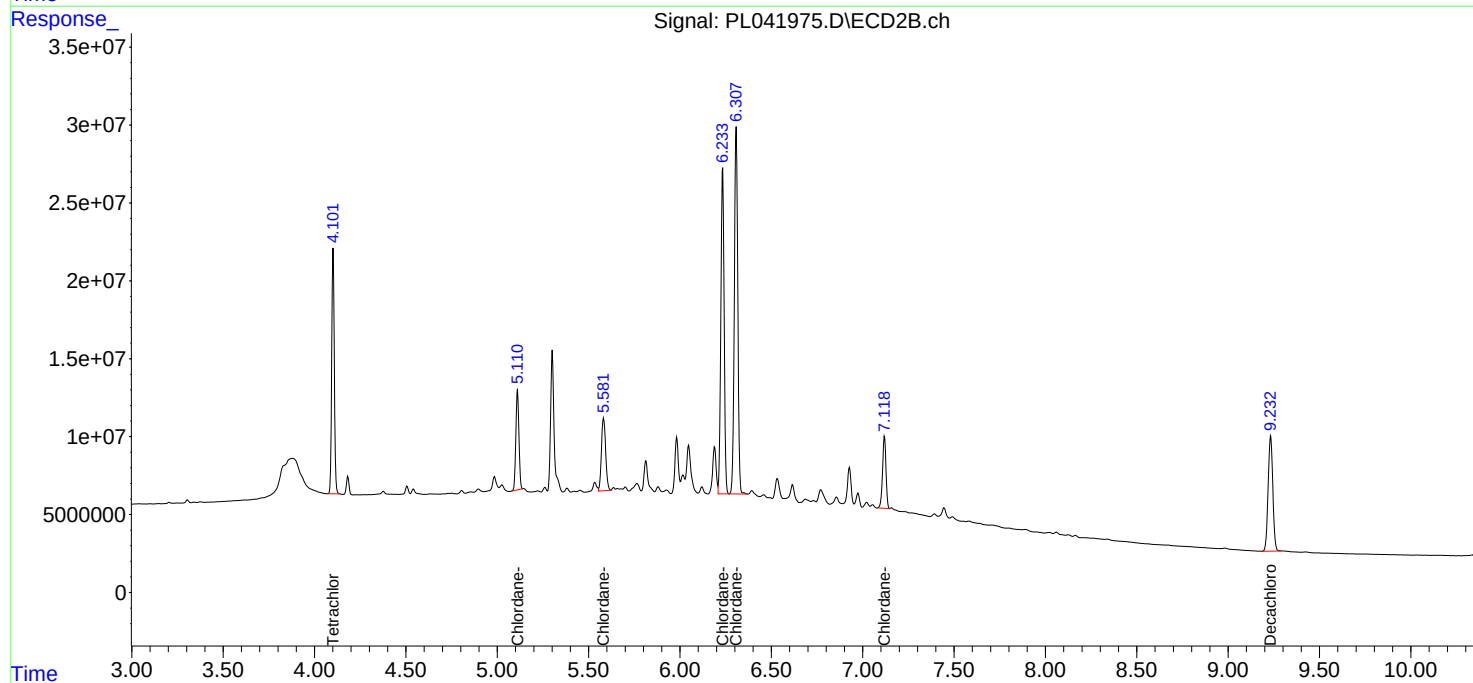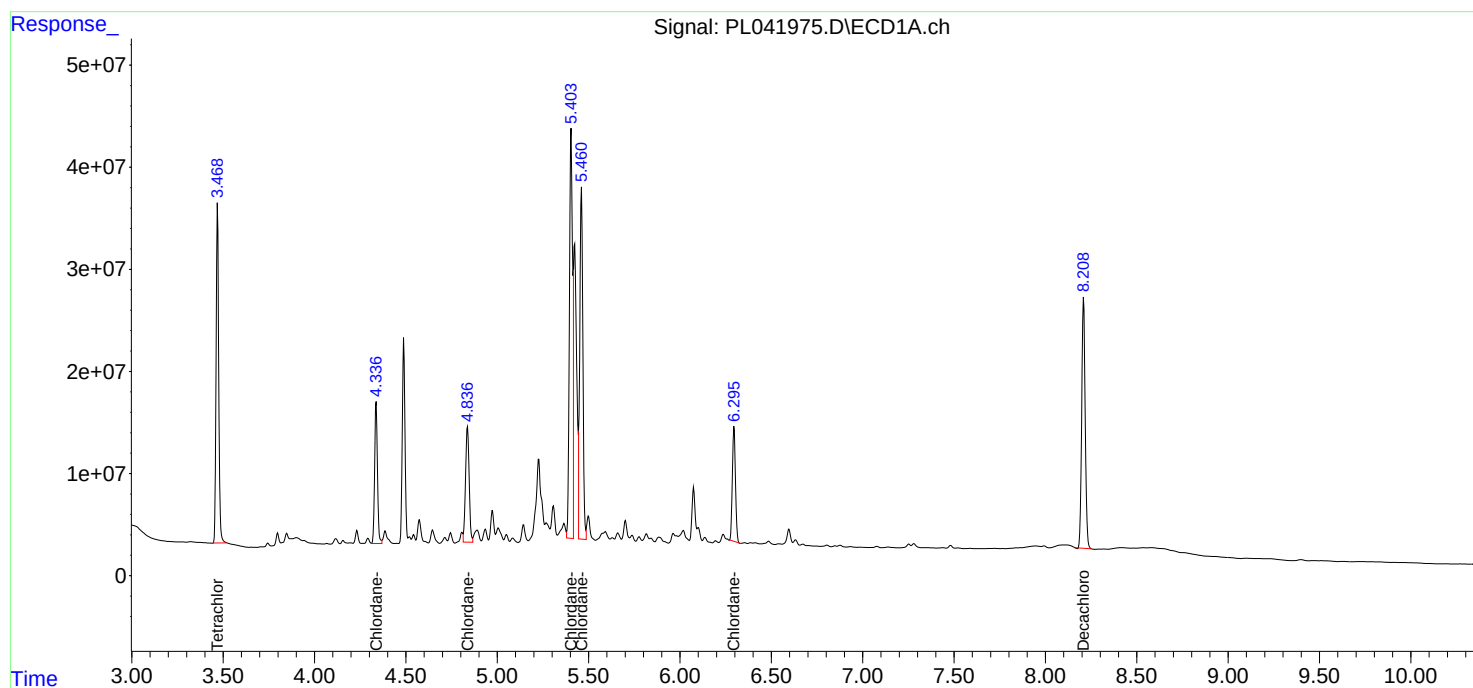


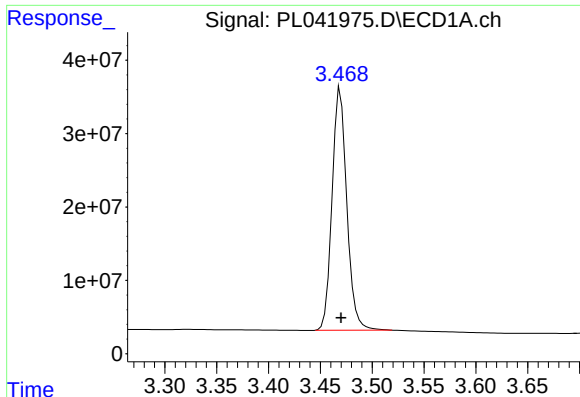

#1 Tetrachloro-m-xylene


R.T.: 3.469 min
Delta R.T.: 0.000 min
Response: 326738728
Conc: 52.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

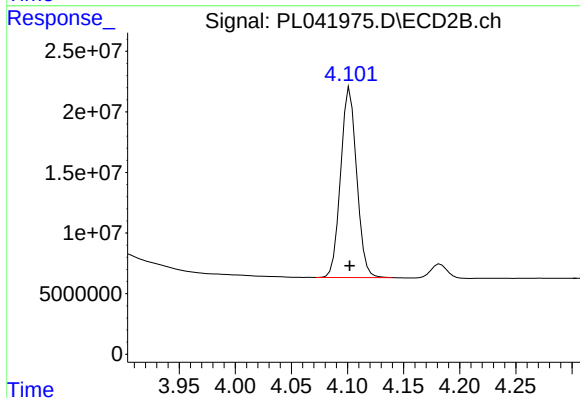


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 155751710
Conc: 52.57 ng/ml

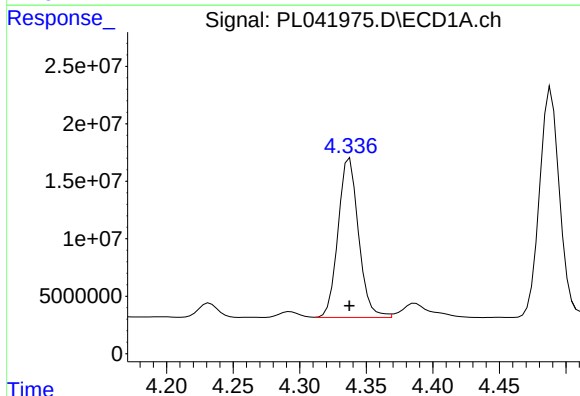


#23 Chlordane-1

R.T.: 4.338 min
Delta R.T.: 0.000 min
Response: 148173251
Conc: 496.49 ng/ml

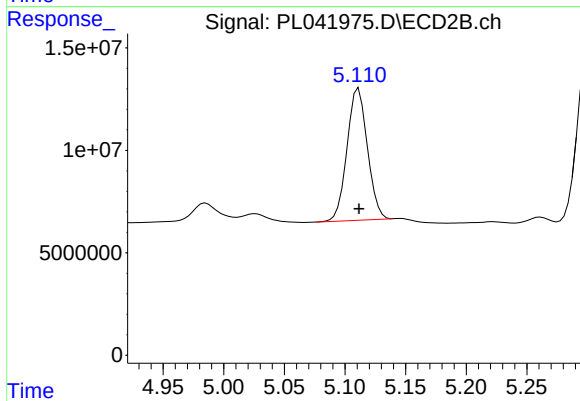

#23 Chlordane-1


R.T.: 5.111 min
Delta R.T.: 0.000 min
Response: 75569816
Conc: 524.86 ng/ml

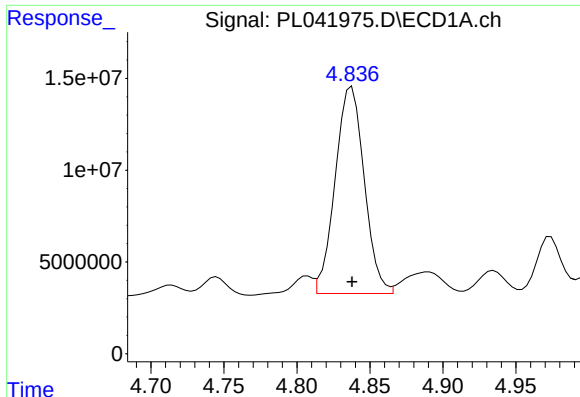

#24 Chlordane-2


R.T.: 4.838 min
Delta R.T.: 0.000 min
Response: 156051131
Conc: 491.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

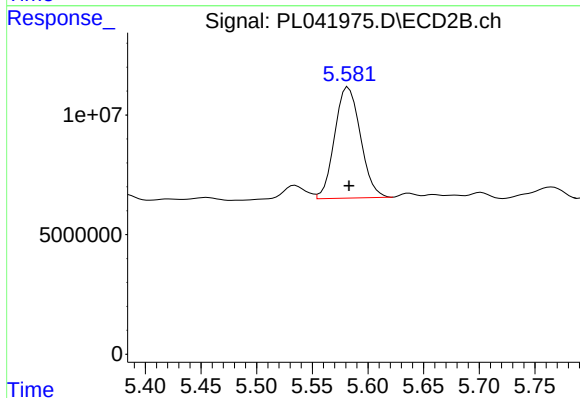


#24 Chlordane-2

R.T.: 5.582 min
Delta R.T.: 0.000 min
Response: 74790588
Conc: 513.53 ng/ml

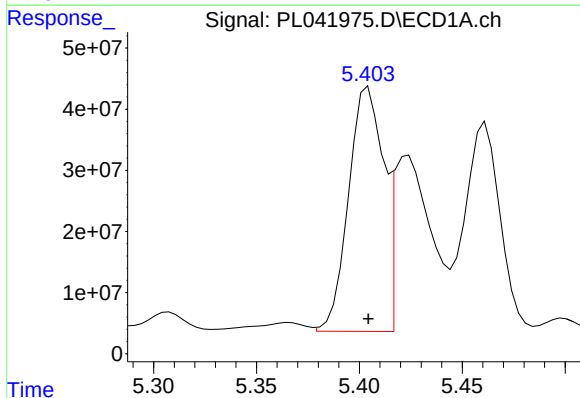


#25 Chlordane-3

R.T.: 5.404 min
Delta R.T.: 0.000 min
Response: 470966323
Conc: 503.73 ng/ml

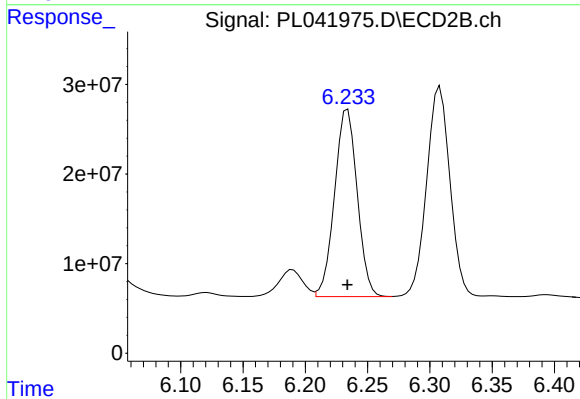

#25 Chlordane-3


R.T.: 6.234 min
Delta R.T.: 0.000 min
Response: 264680886
Conc: 518.28 ng/ml

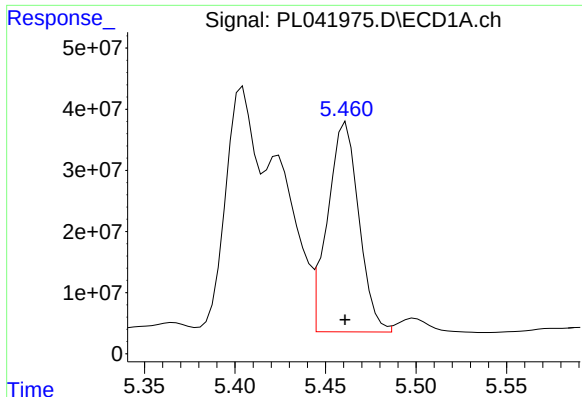

#26 Chlordane-4


R.T.: 5.461 min
Delta R.T.: 0.000 min
Response: 413808082
Conc: 495.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

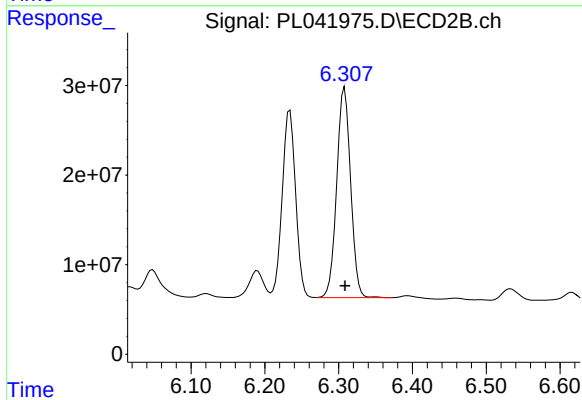


#26 Chlordane-4

R.T.: 6.308 min
Delta R.T.: 0.000 min
Response: 307560289
Conc: 515.07 ng/ml

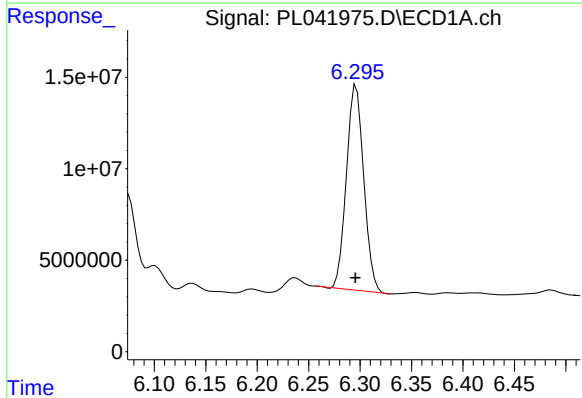


#27 Chlordane-5

R.T.: 6.296 min
Delta R.T.: 0.000 min
Response: 130951638
Conc: 499.90 ng/ml

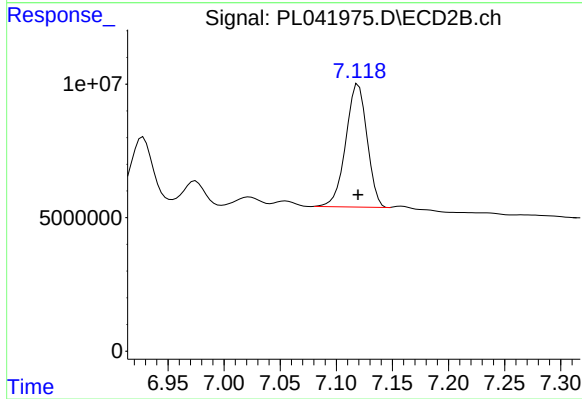

#27 Chlordane-5


R.T.: 7.120 min
Delta R.T.: 0.000 min
Response: 60797194
Conc: 519.07 ng/ml

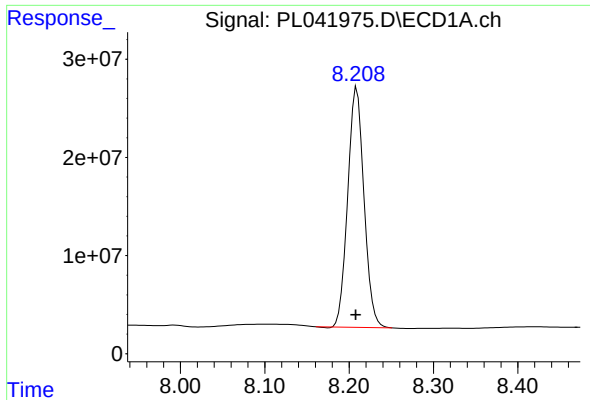

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: 0.001 min
Response: 327521404
Conc: 47.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

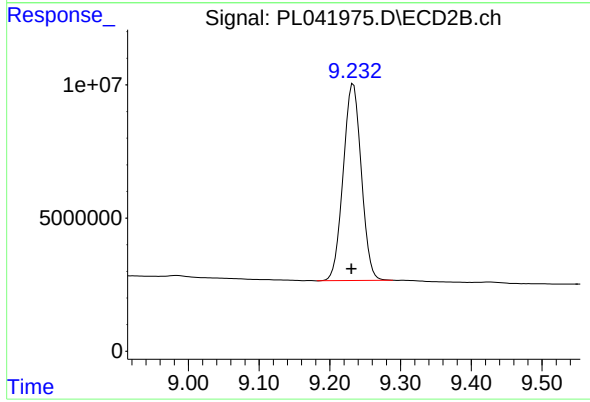

#28 Decachlorobiphenyl

R.T.: 9.233 min
Delta R.T.: 0.003 min
Response: 131620309
Conc: 51.60 ng/ml