

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110918\
 Data File : PL041990.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2018 18:30
 Operator : AJ\SJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 21:58:01 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.470	4.103	327.0E6	157.6E6	52.949	53.205
28)	SA Decachlor...	8.210	9.234	330.0E6	131.9E6	48.171	51.696
Target Compounds							
23)	Chlordane-1	4.338	5.112	146.6E6	76153122	491.230	528.910
24)	Chlordane-2	4.838	5.583	155.0E6	75470512	488.688	518.202
25)	Chlordane-3	5.405	6.234	461.2E6	268.2E6	493.292	525.158
26)	Chlordane-4	5.462	6.309	411.0E6	310.8E6	491.970	520.541
27)	Chlordane-5	6.297	7.120	129.3E6	61293390	493.584	523.304



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110918\
Data File : PL041990.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2018 18:30
Operator : AJ\SJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 21:58:01 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

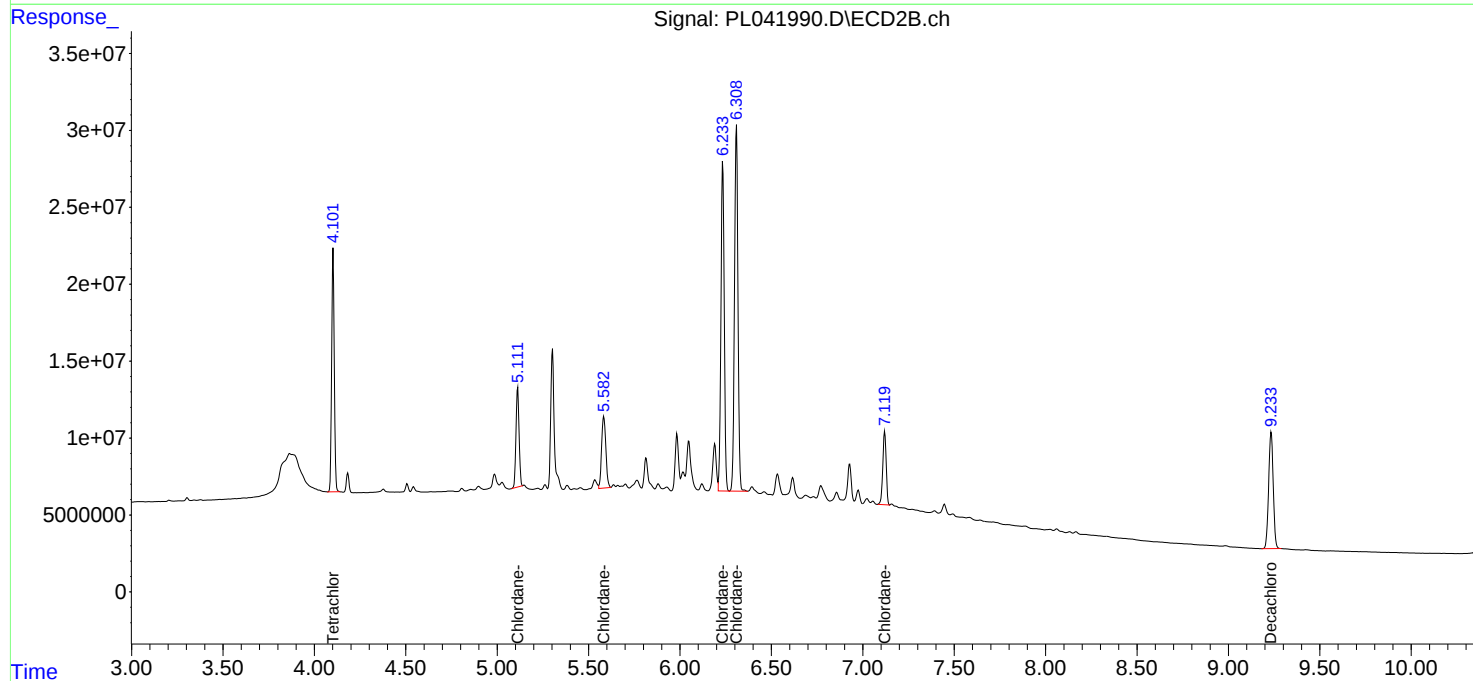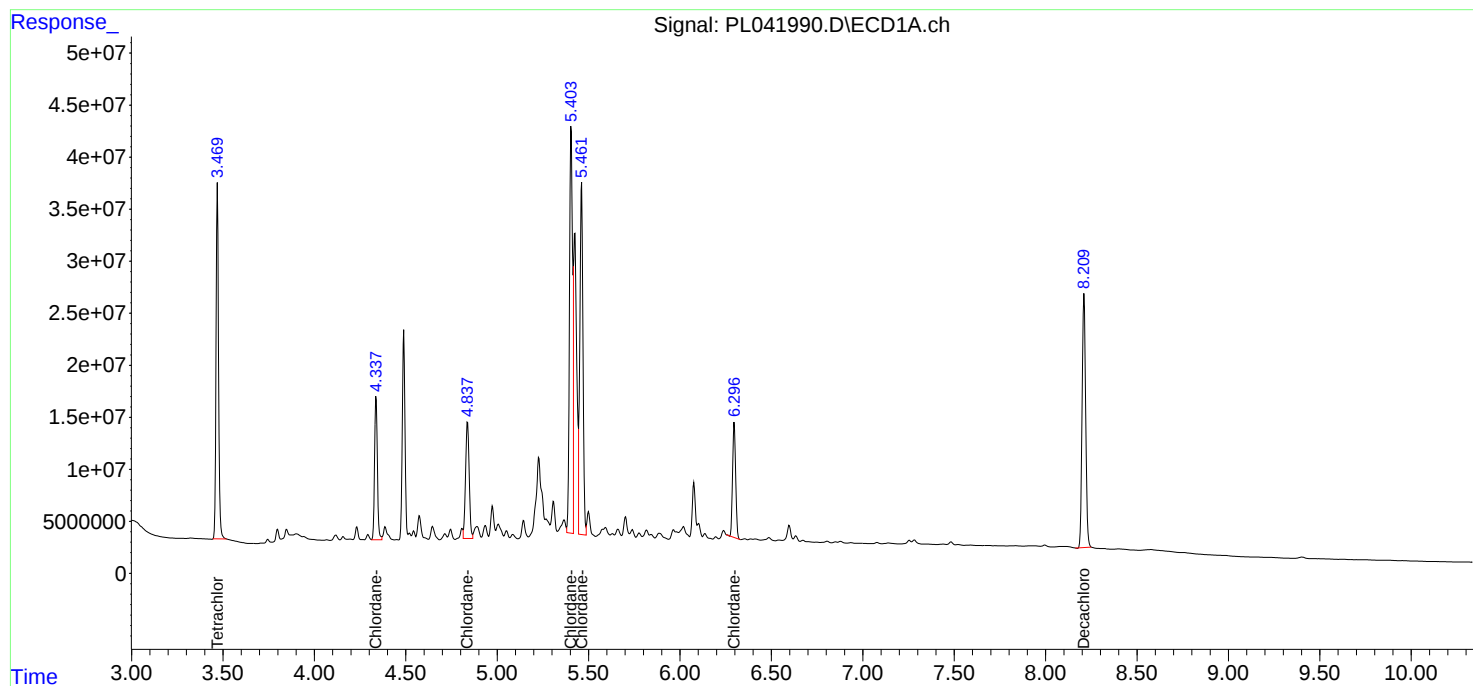


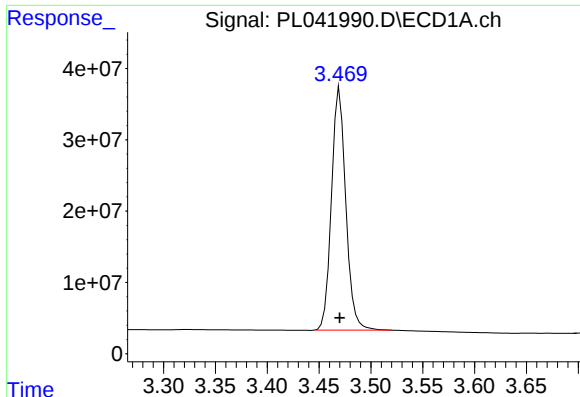

#1 Tetrachloro-m-xylene


R.T.: 3.470 min
Delta R.T.: 0.000 min
Response: 326956727
Conc: 52.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

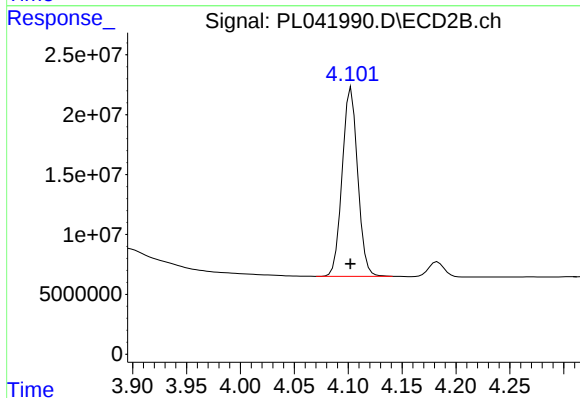


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: 0.000 min
Response: 157630963
Conc: 53.21 ng/ml

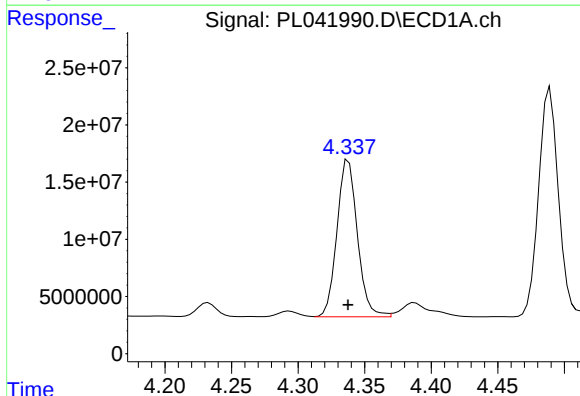


#23 Chlordane-1

R.T.: 4.338 min
Delta R.T.: 0.000 min
Response: 146602661
Conc: 491.23 ng/ml

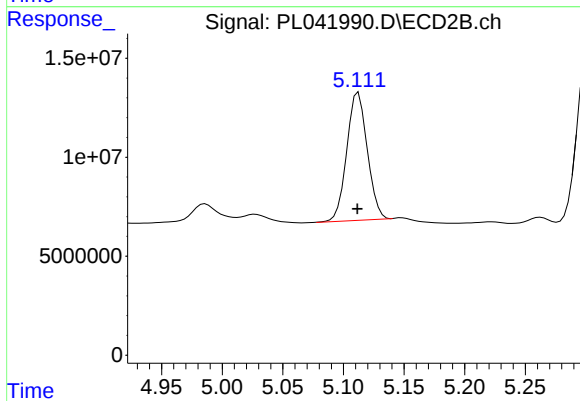

#23 Chlordane-1


R.T.: 5.112 min
Delta R.T.: 0.000 min
Response: 76153122
Conc: 528.91 ng/ml

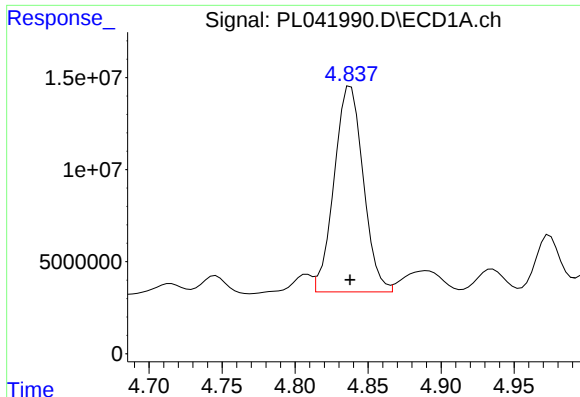

#24 Chlordane-2


R.T.: 4.838 min
Delta R.T.: 0.000 min
Response: 155027221
Conc: 488.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

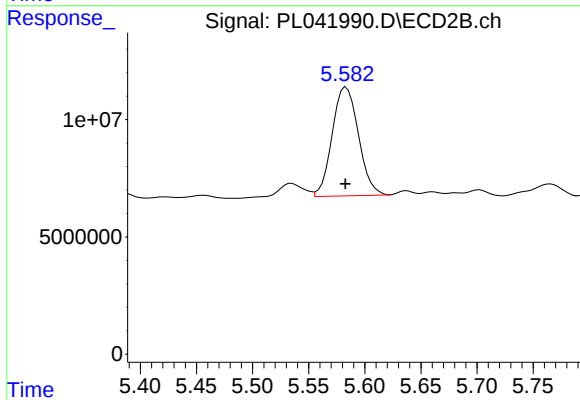


#24 Chlordane-2

R.T.: 5.583 min
Delta R.T.: 0.000 min
Response: 75470512
Conc: 518.20 ng/ml

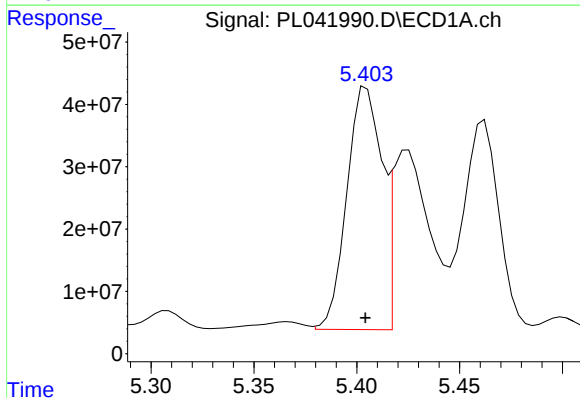


#25 Chlordane-3

R.T.: 5.405 min
Delta R.T.: 0.000 min
Response: 461206706
Conc: 493.29 ng/ml

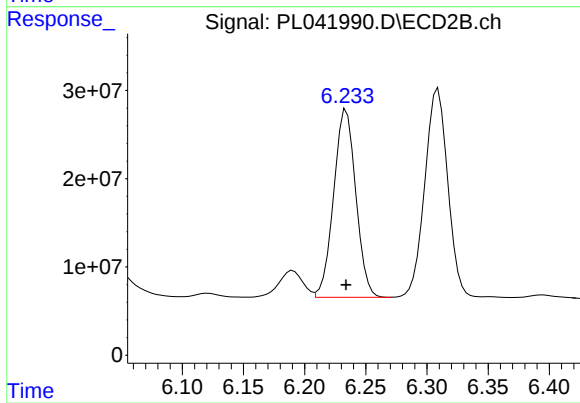

#25 Chlordane-3


R.T.: 6.234 min
Delta R.T.: 0.000 min
Response: 268192638
Conc: 525.16 ng/ml

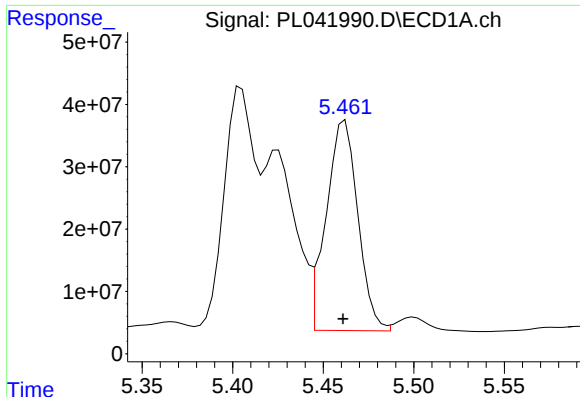

#26 Chlordane-4


R.T.: 5.462 min
Delta R.T.: 0.001 min
Response: 411042710
Conc: 491.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

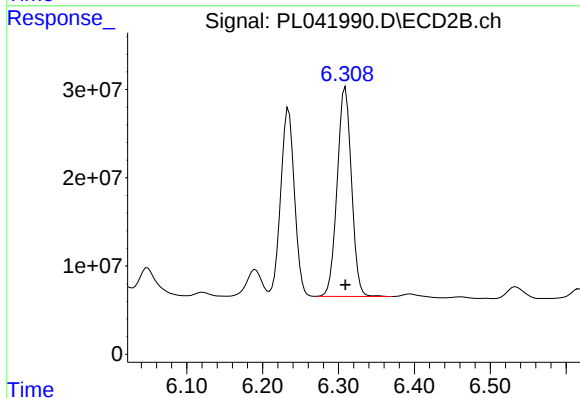


#26 Chlordane-4

R.T.: 6.309 min
Delta R.T.: 0.000 min
Response: 310826204
Conc: 520.54 ng/ml

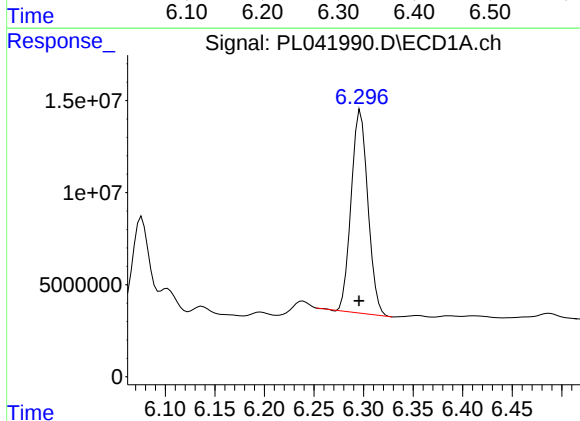


#27 Chlordane-5

R.T.: 6.297 min
Delta R.T.: 0.002 min
Response: 129296247
Conc: 493.58 ng/ml

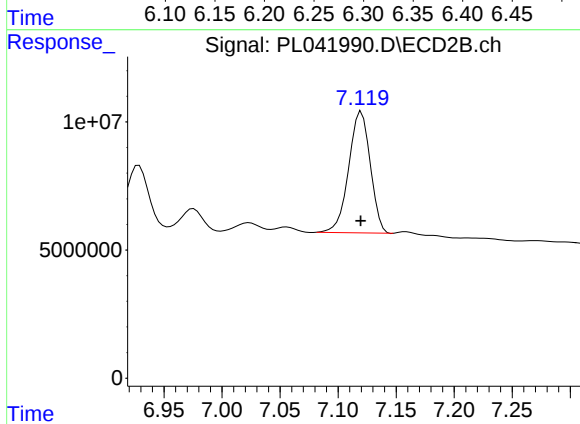

#27 Chlordane-5


R.T.: 7.120 min
Delta R.T.: 0.000 min
Response: 61293390
Conc: 523.30 ng/ml

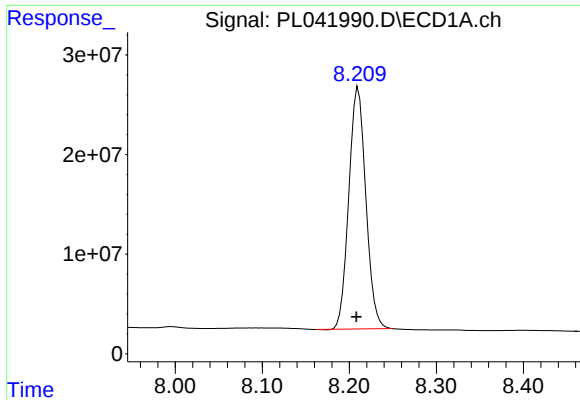

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: 0.002 min
Response: 329984908
Conc: 48.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

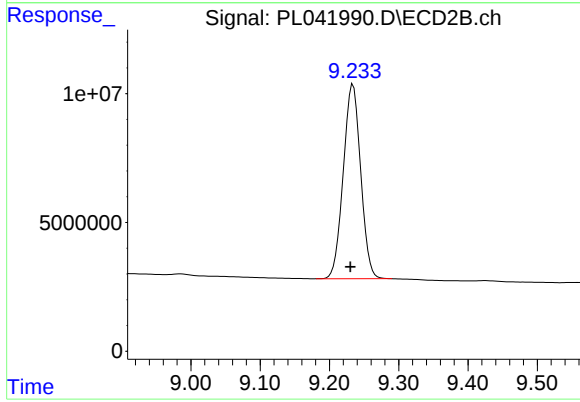

#28 Decachlorobiphenyl

R.T.: 9.234 min
Delta R.T.: 0.004 min
Response: 131855265
Conc: 51.70 ng/ml