

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110920\
 Data File : PL062903.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2020 14:02
 Operator : DD\AJ
 Sample : L4658-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 1998-CL

Manual Integrations
 APPROVED

Ankita
 11/11/2020 8:21:50 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 00:49:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.948	28299796	49589050	16.453	16.874m
28)	SA Decachlor...	8.124	8.988	28888891	40342175	18.007	19.275
Target Compounds							
14)	MA Endrin	5.931	6.639	2744148	1803233	1.649	0.646m#
16)	A 4,4'-DDD	6.062	6.771	1808176	13348641	1.278m	5.214m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110920\
Data File : PL062903.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2020 14:02
Operator : DD\AJ
Sample : L4658-08
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
1998-CL


Manual Integrations
APPROVED

Ankita
11/11/2020 8:21:50 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 00:49:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

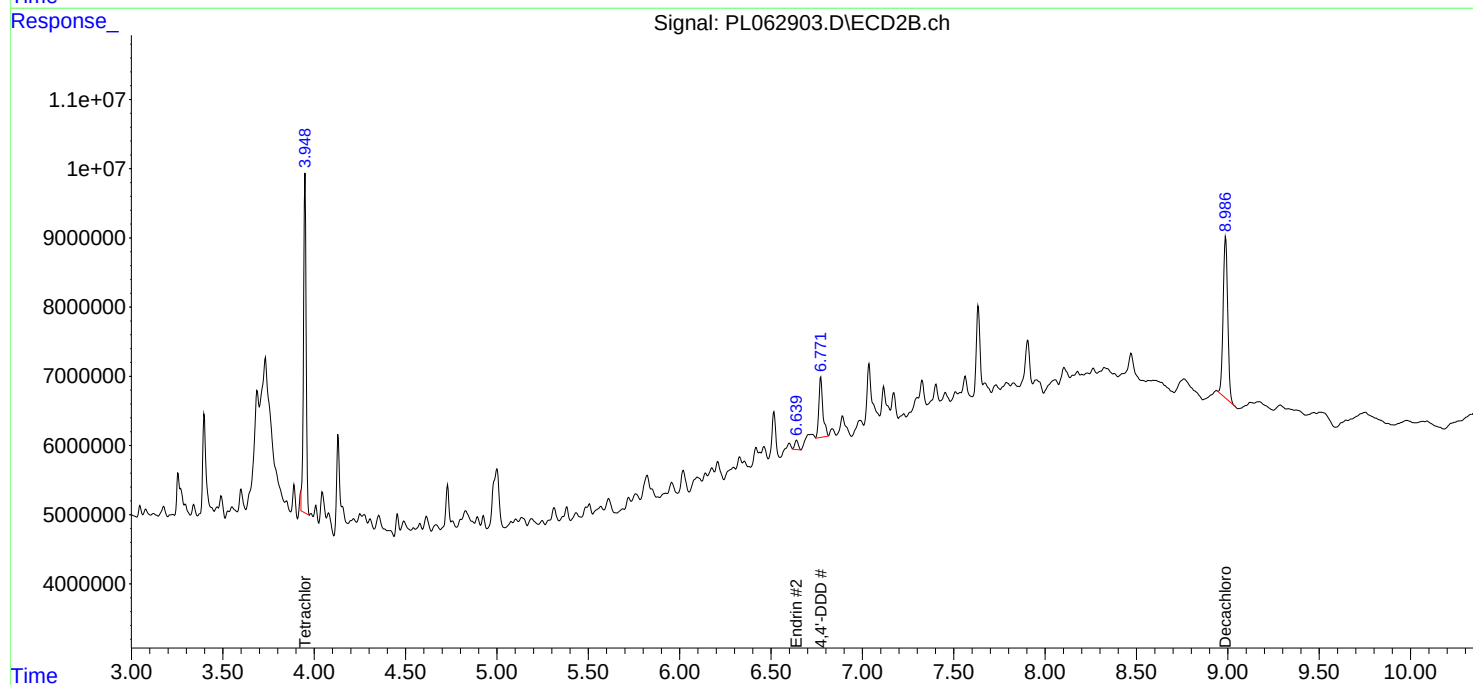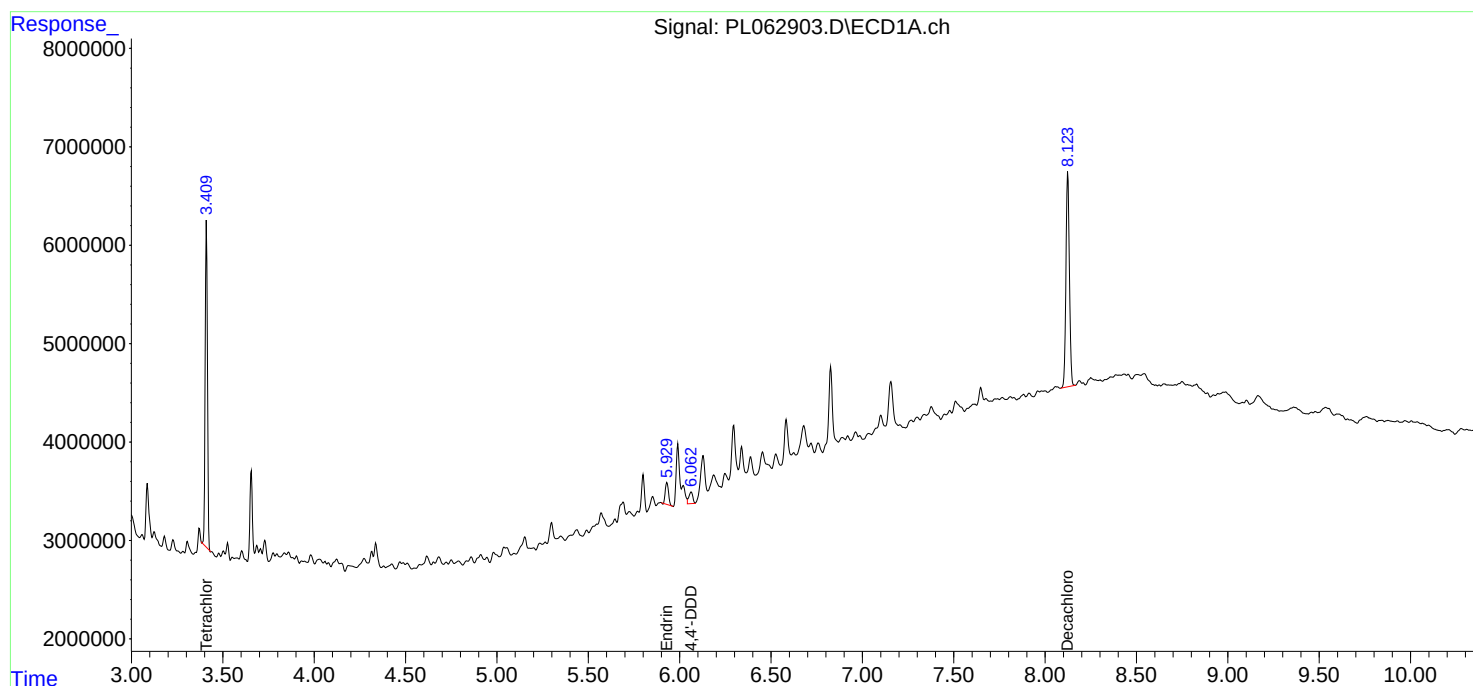

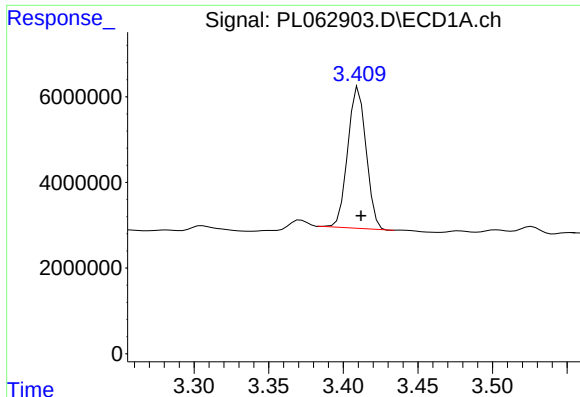


#1 Tetrachloro-m-xylene

R.T.: 3.410 min
Delta R.T.: -0.002 min
Response: 28299796
Conc: 16.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
1998-CL


Manual Integrations
APPROVED

Ankita
11/11/2020 8:21:50 AM

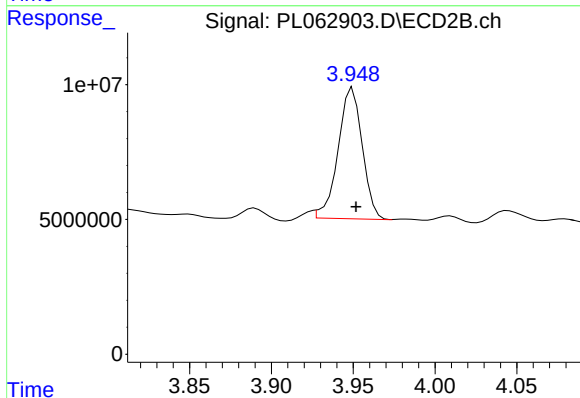


#1 Tetrachloro-m-xylene

R.T.: 3.948 min
Delta R.T.: -0.003 min
Response: 49589050
Conc: 16.87 ng/ml m

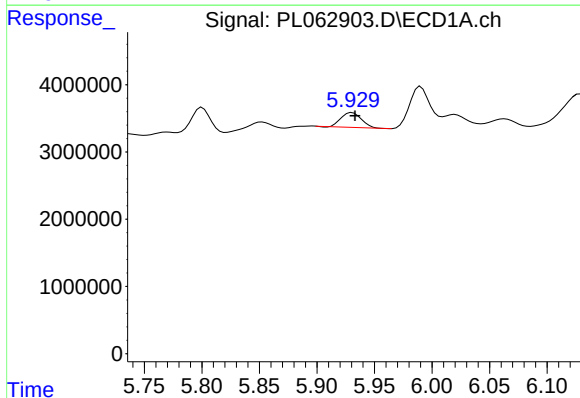


#14 Endrin

R.T.: 5.931 min
Delta R.T.: -0.003 min
Response: 2744148
Conc: 1.65 ng/ml

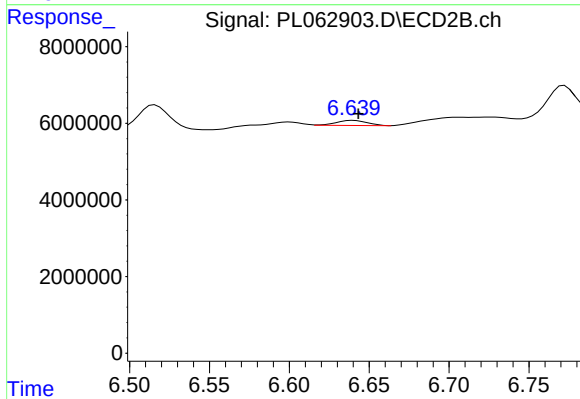

#14 Endrin

R.T.: 6.639 min
Delta R.T.: -0.005 min
Response: 1803233
Conc: 0.65 ng/ml m

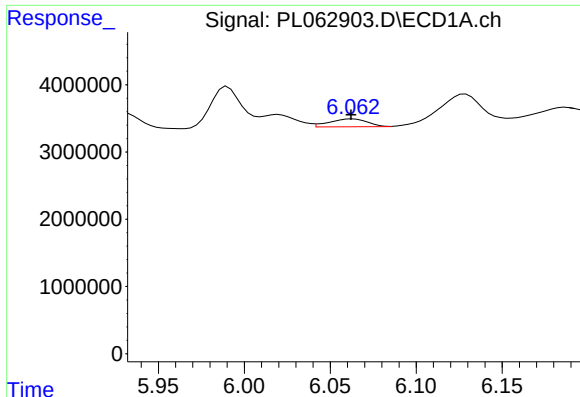


#16 4,4'-DDD

R.T.: 6.062 min
Delta R.T.: 0.000 min
Response: 1808176
Conc: 1.28 ng/ml m

Instrument :
ECD_L
ClientSampleId :
1998-CL


Manual Integrations
APPROVED

Ankita
11/11/2020 8:21:50 AM

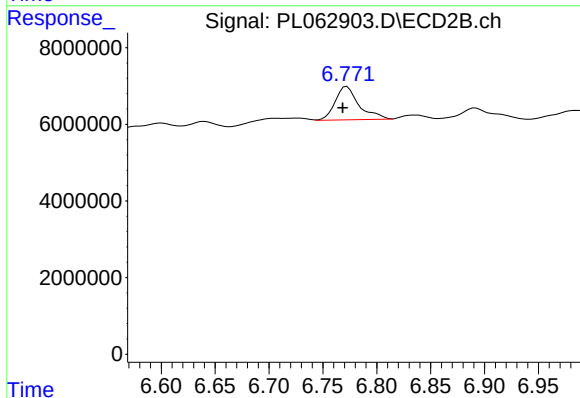


#16 4,4'-DDD

R.T.: 6.771 min
Delta R.T.: 0.002 min
Response: 13348641
Conc: 5.21 ng/ml m

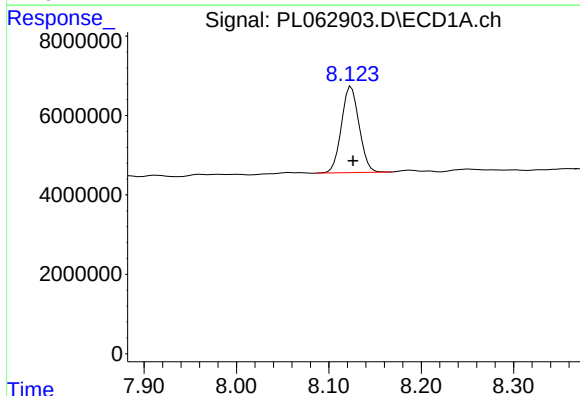

#28 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: -0.002 min
Response: 28888891
Conc: 18.01 ng/ml

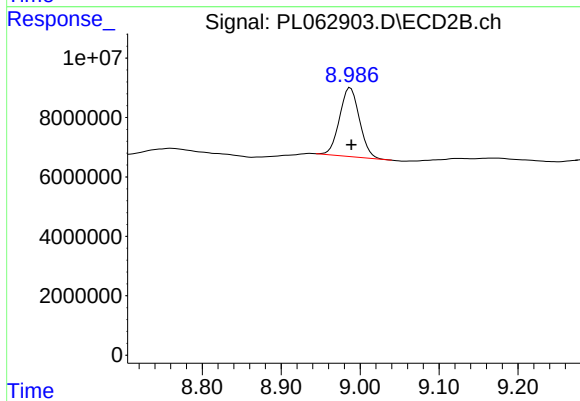

#28 Decachlorobiphenyl

R.T.: 8.988 min
Delta R.T.: -0.001 min
Response: 40342175
Conc: 19.28 ng/ml