

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110921\
 Data File : PL070876.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2021 13:02
 Operator : AR\AJ
 Sample : M4577-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 04:34:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 19:28:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.569	5.504	9824963	25568997	20.059	20.279
28)	SA Decachlor...	10.334	11.398	9610140	20751442	14.064	15.517
Target Compounds							
7)	B delta-BHC	0.000	7.026f	0	638707	N.D.	0.382 #
12)	B 4,4'-DDE	7.570	8.504	6717147	19054537	11.529	12.914
15)	B Endosulfa...	8.274f	9.104f	853778	1019172	1.410	0.834 #
17)	MA 4,4'-DDT	8.416	9.360	2631334	5803373	4.784	4.600
23)	Chlordane-1	0.000	6.904f	0	810707	N.D.	16.695 #
27)	Chlordane-5	8.274f	0.000	853778	0	38.187	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110921\
Data File : PL070876.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2021 13:02
Operator : AR\AJ
Sample : M4577-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 04:34:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 19:28:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

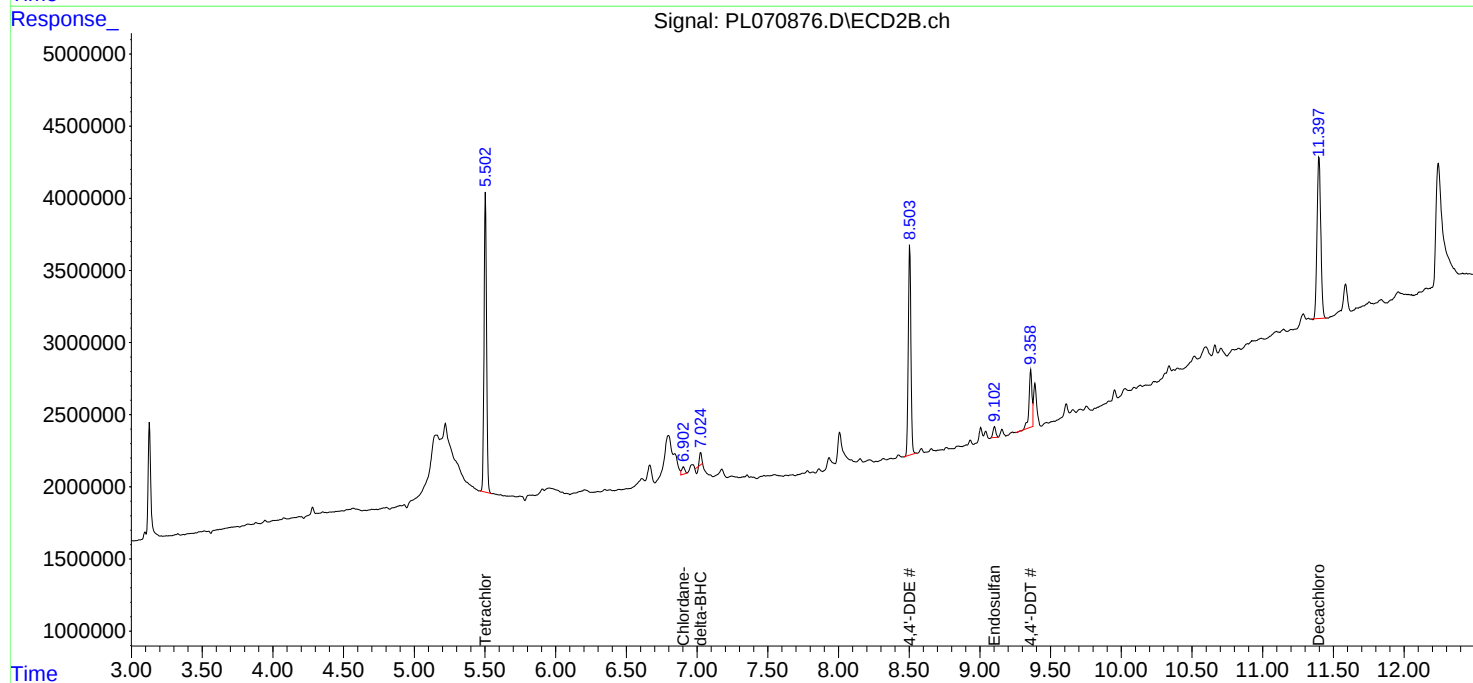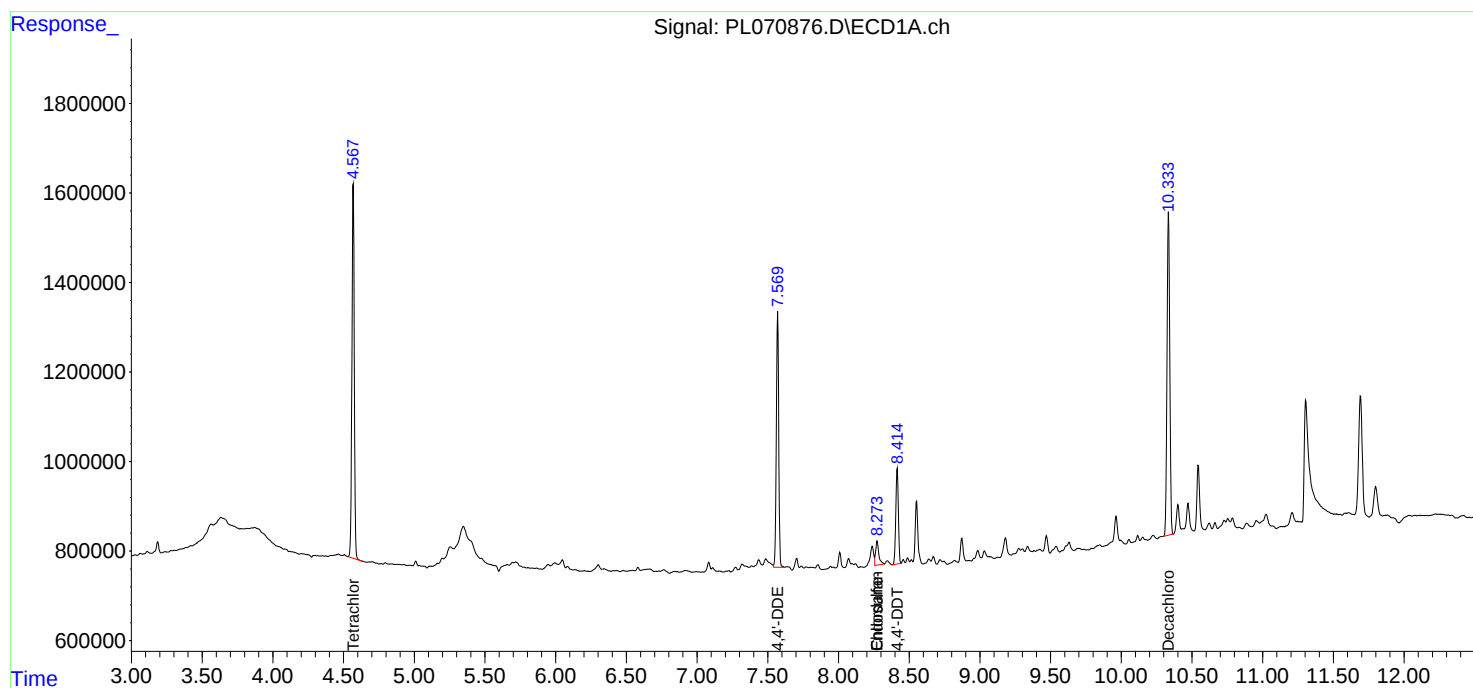


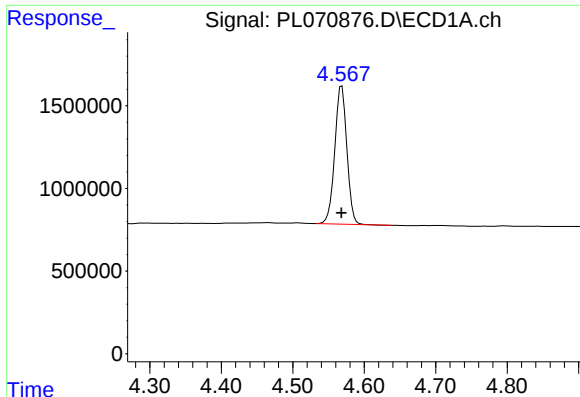

#1 Tetrachloro-m-xylene


R.T.: 4.569 min
Delta R.T.: 0.000 min
Response: 9824963
Conc: 20.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

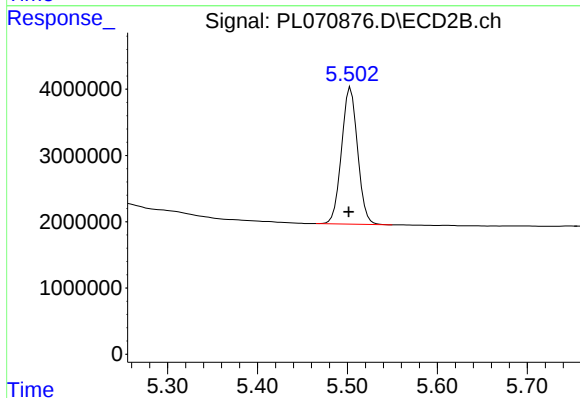


#1 Tetrachloro-m-xylene

R.T.: 5.504 min
Delta R.T.: 0.002 min
Response: 25568997
Conc: 20.28 ng/ml

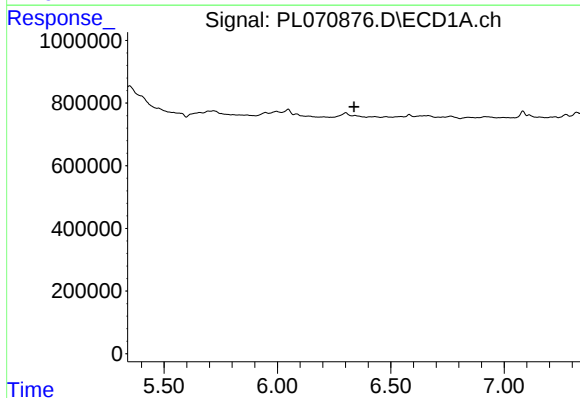


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.338 min
Response: 0
Conc: N.D.

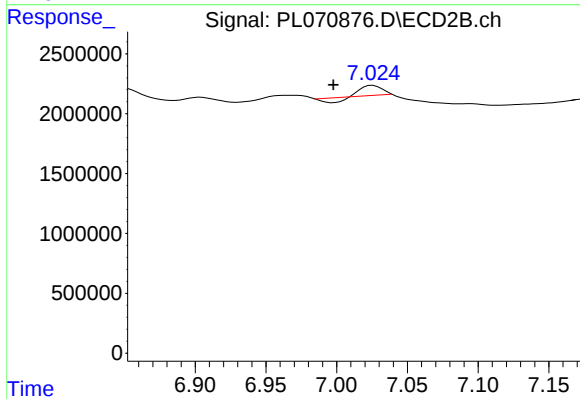

#7 delta-BHC


R.T.: 7.026 min
Delta R.T.: 0.028 min
Response: 638707
Conc: 0.38 ng/ml

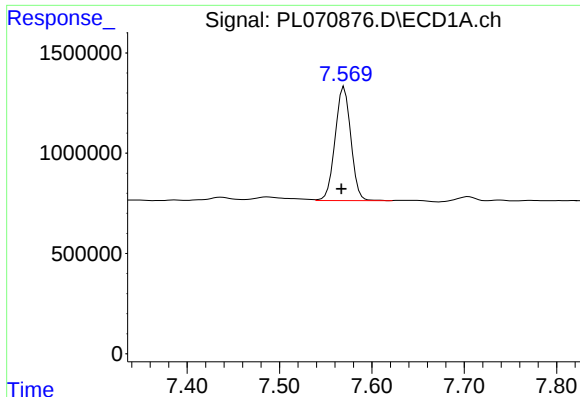

#12 4,4'-DDE


R.T.: 7.570 min
Delta R.T.: 0.003 min
Response: 6717147
Conc: 11.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

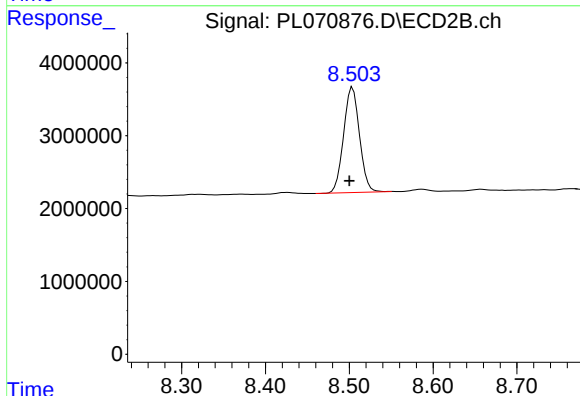


#12 4,4'-DDE

R.T.: 8.504 min
Delta R.T.: 0.004 min
Response: 19054537
Conc: 12.91 ng/ml

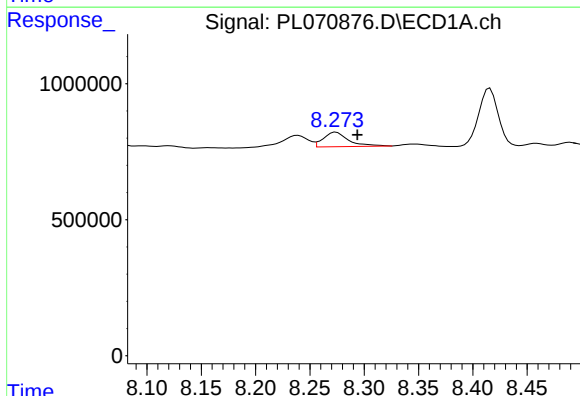


#15 Endosulfan II

R.T.: 8.274 min
Delta R.T.: -0.020 min
Response: 853778
Conc: 1.41 ng/ml

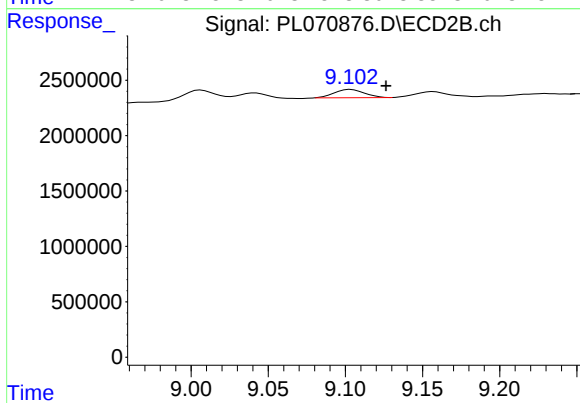

#15 Endosulfan II


R.T.: 9.104 min
Delta R.T.: -0.023 min
Response: 1019172
Conc: 0.83 ng/ml

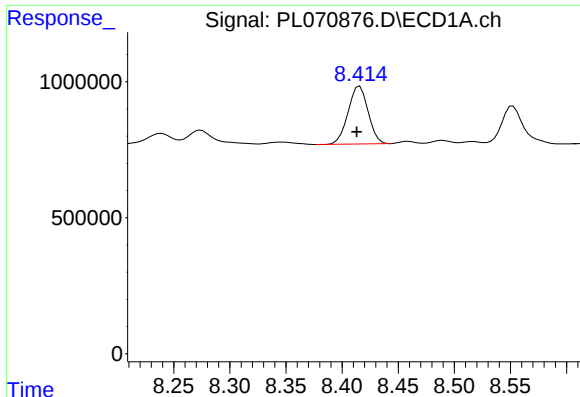

#17 4,4'-DDT


R.T.: 8.416 min
Delta R.T.: 0.003 min
Response: 2631334
Conc: 4.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

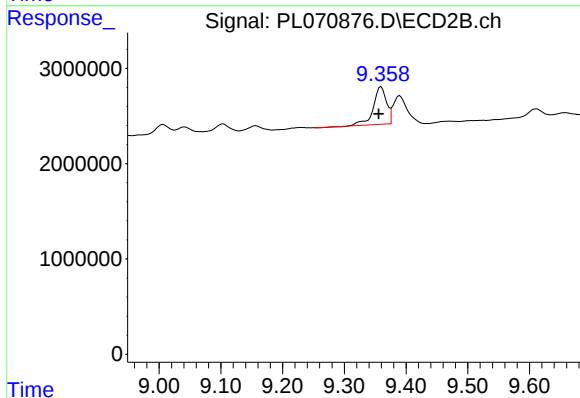


#17 4,4'-DDT

R.T.: 9.360 min
Delta R.T.: 0.004 min
Response: 5803373
Conc: 4.60 ng/ml

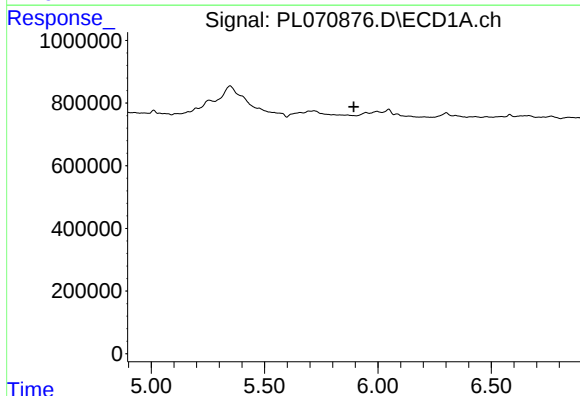


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.893 min
Response: 0
Conc: N.D.

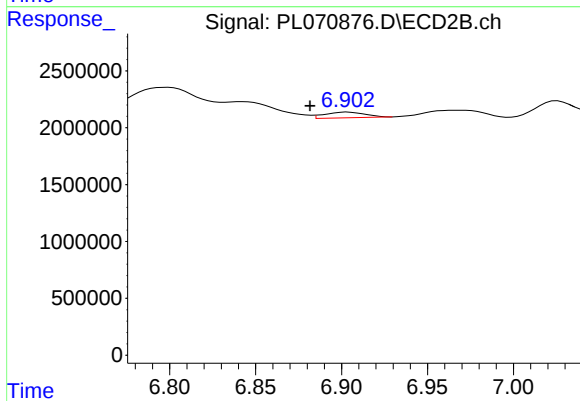

#23 Chlordane-1


R.T.: 6.904 min
Delta R.T.: 0.022 min
Response: 810707
Conc: 16.70 ng/ml

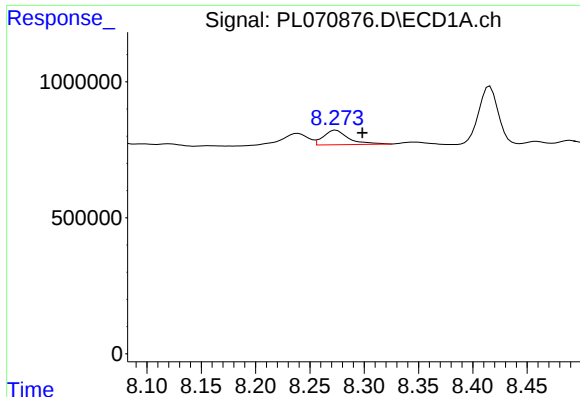

#27 Chlordane-5


R.T.: 8.274 min
Delta R.T.: -0.024 min
Response: 853778
Conc: 38.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

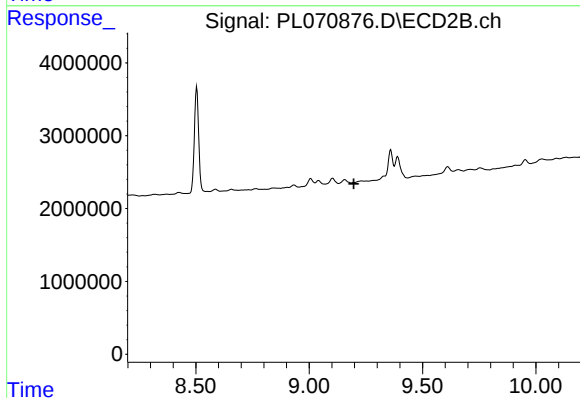


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.197 min
Response: 0
Conc: N.D.

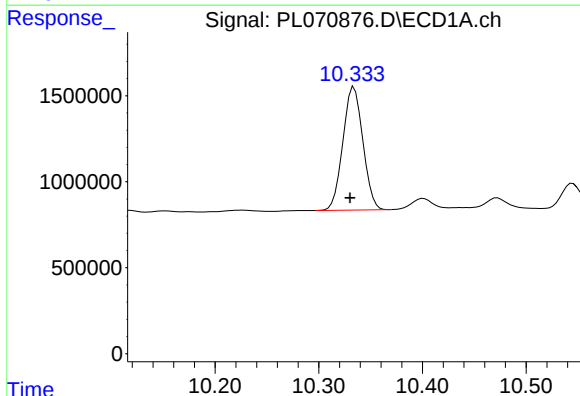

#28 Decachlorobiphenyl

R.T.: 10.334 min
Delta R.T.: 0.004 min
Response: 9610140
Conc: 14.06 ng/ml

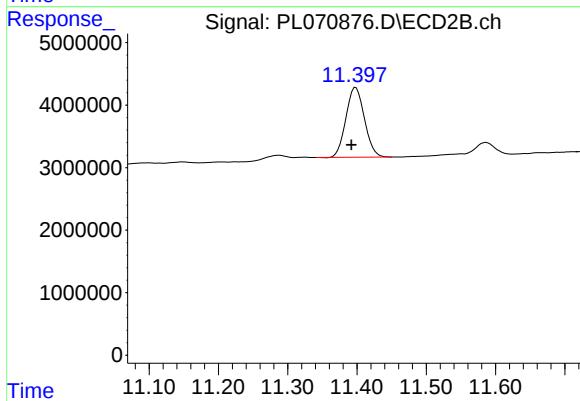

#28 Decachlorobiphenyl

R.T.: 11.398 min
Delta R.T.: 0.006 min
Response: 20751442
Conc: 15.52 ng/ml