

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110922\
 Data File : PL078961.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2022 15:14
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 21:06:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.322	2.568	39764405	52268434	20.852	20.472
28)	SA Decachlor...	8.770	7.635	29513335	34377044	19.619	18.150
Target Compounds							
5)	MB Aldrin	0.000	3.951f	0	5222616	N.D.	1.491 #
7)	B delta-BHC	0.000	3.896	0	2152946	N.D.	0.591 #
8)	B Heptachlo...	5.464	4.490	6813518	1416811	3.209	0.470 #
9)	A Endosulfan I	5.855	0.000	251514	0	0.118	N.D. #
14)	MA Endrin	0.000	5.390f	0	4901848	N.D.	1.882 #
16)	A 4,4'-DDD	6.514f	0.000	102530	0	0.062	N.D. #
17)	MA 4,4'-DDT	6.821	0.000	300396	0	0.168	N.D. #
20)	A Methoxychlor	7.285	0.000	373772	0	0.406	N.D. #
24)	Chlordane-2	0.000	4.098	0	6007578	N.D.	56.448 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110922\
Data File : PL078961.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2022 15:14
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 21:06:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

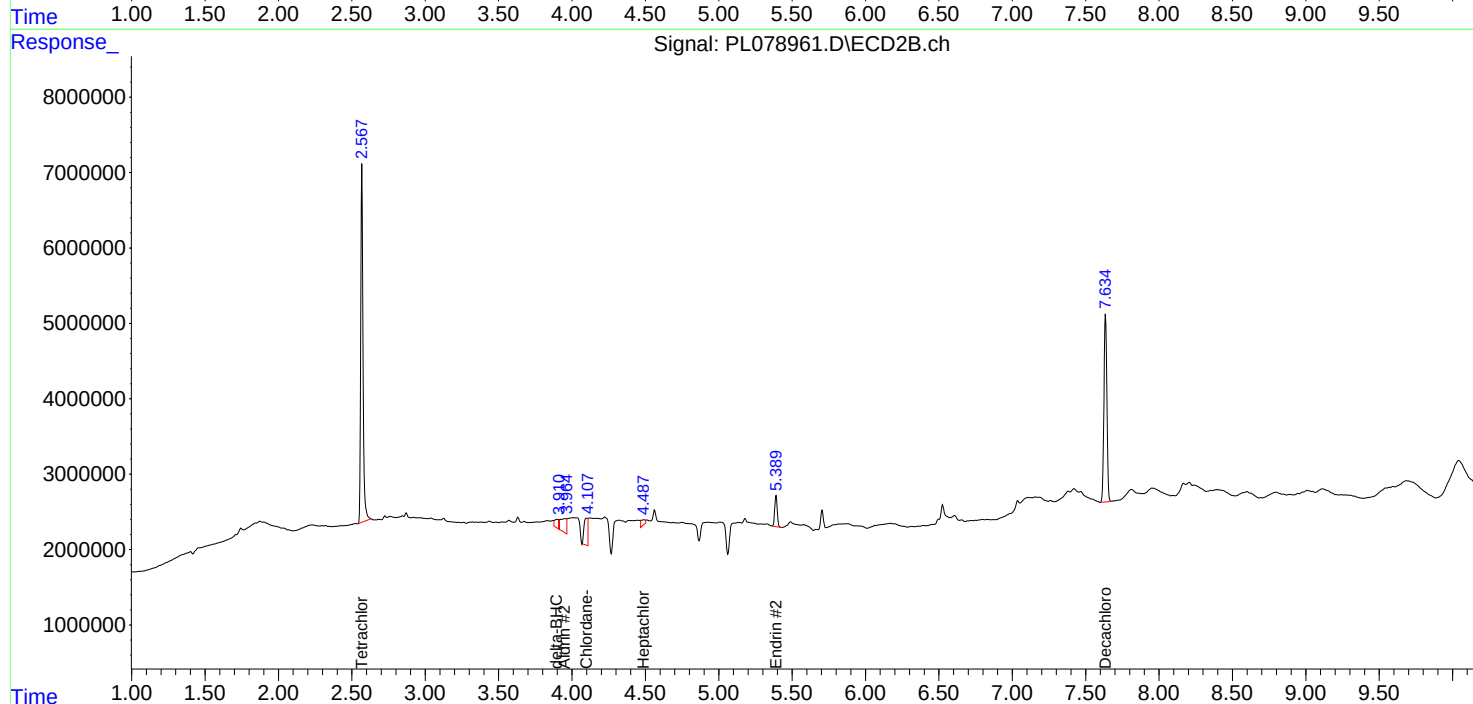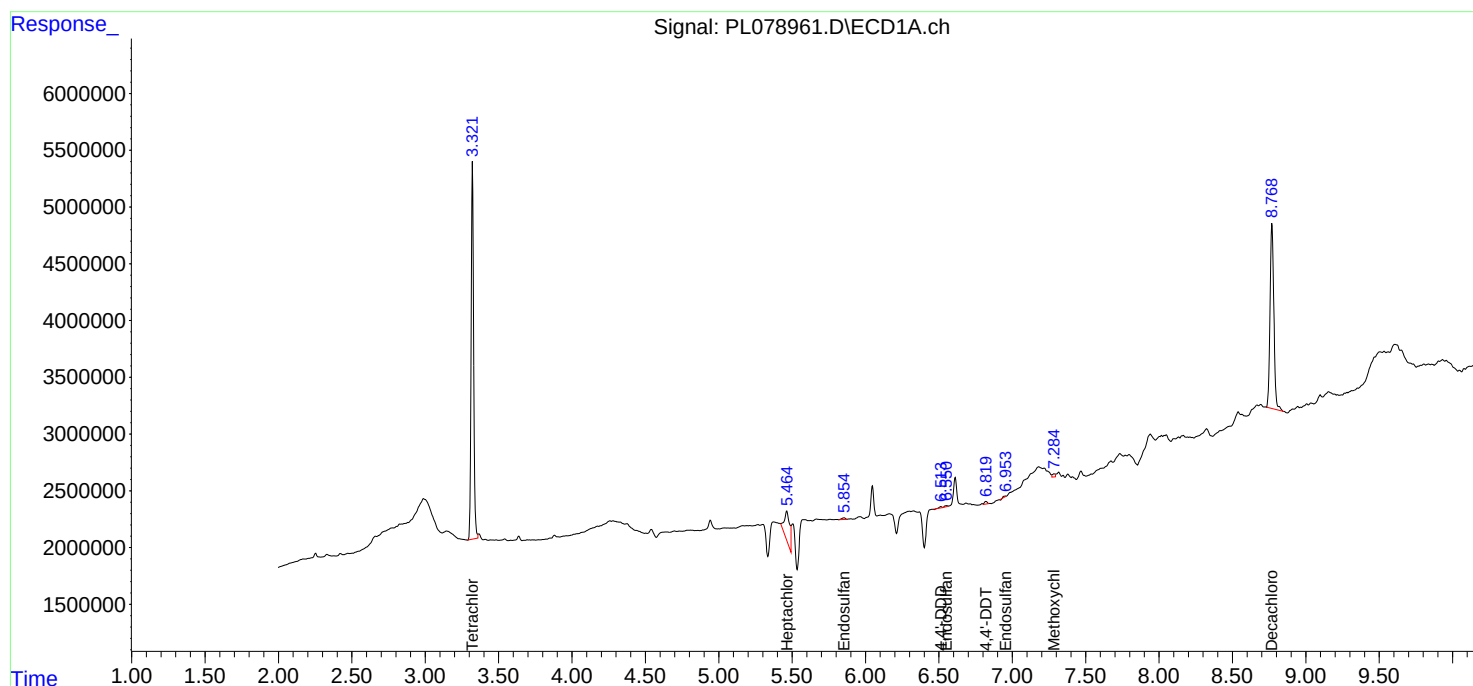


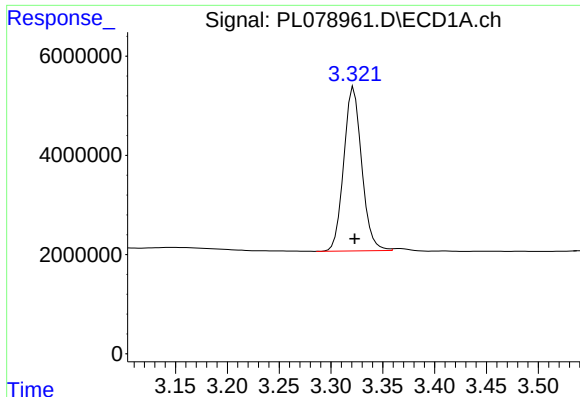

#1 Tetrachloro-m-xylene


R.T.: 3.322 min
Delta R.T.: 0.000 min
Response: 39764405
Conc: 20.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

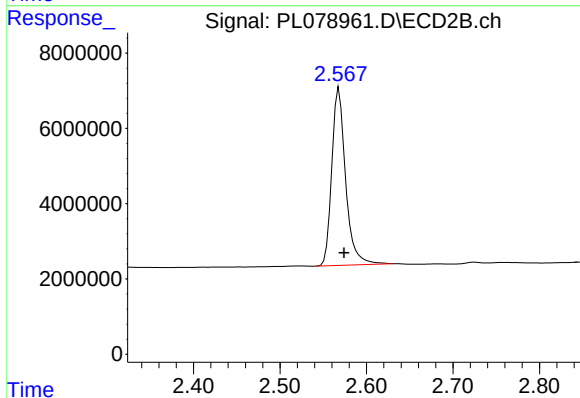


#1 Tetrachloro-m-xylene

R.T.: 2.568 min
Delta R.T.: -0.005 min
Response: 52268434
Conc: 20.47 ng/ml

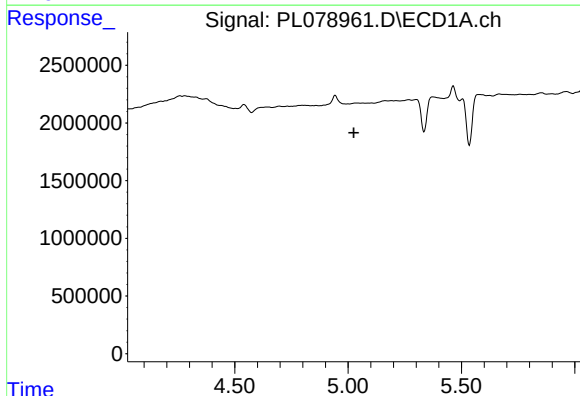


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.025 min
Response: 0
Conc: N.D.

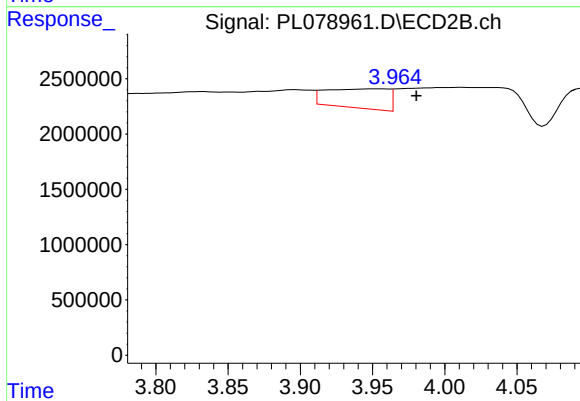

#5 Aldrin


R.T.: 3.951 min
Delta R.T.: -0.030 min
Response: 5222616
Conc: 1.49 ng/ml

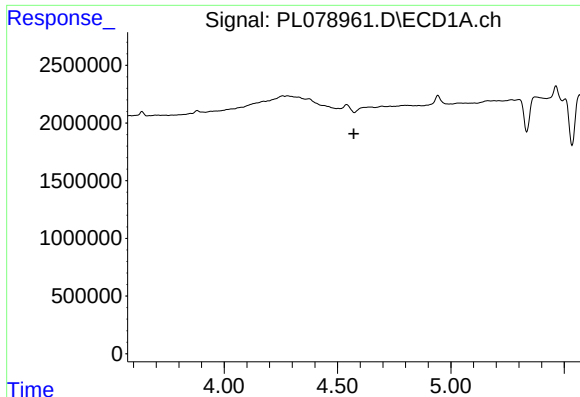

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.572 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

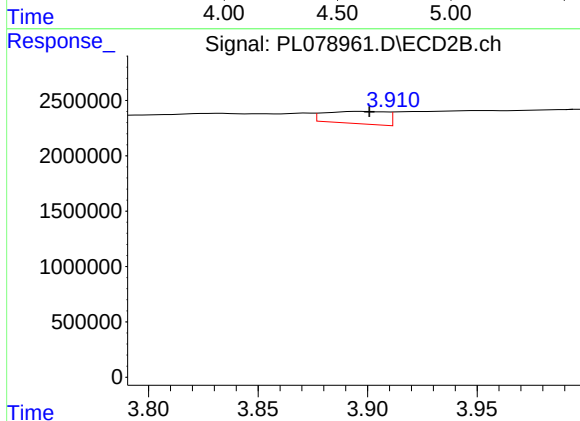


#7 delta-BHC

R.T.: 3.896 min
Delta R.T.: -0.005 min
Response: 2152946
Conc: 0.59 ng/ml

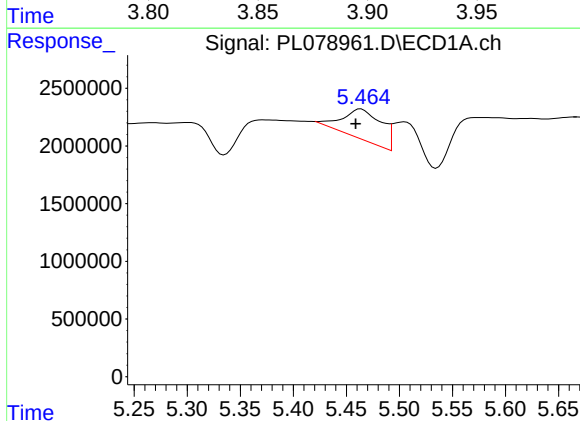


#8 Heptachlor epoxide

R.T.: 5.464 min
Delta R.T.: 0.005 min
Response: 6813518
Conc: 3.21 ng/ml

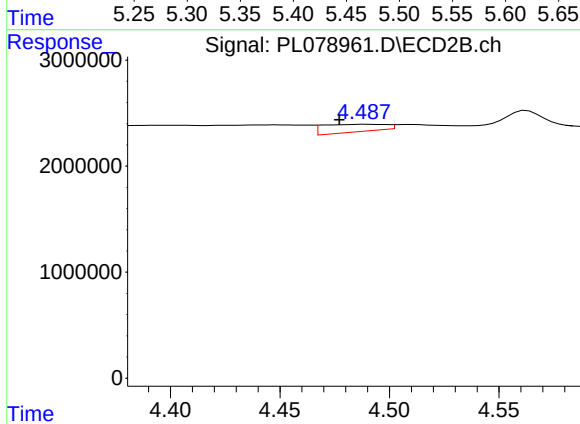

#8 Heptachlor epoxide


R.T.: 4.490 min
Delta R.T.: 0.013 min
Response: 1416811
Conc: 0.47 ng/ml

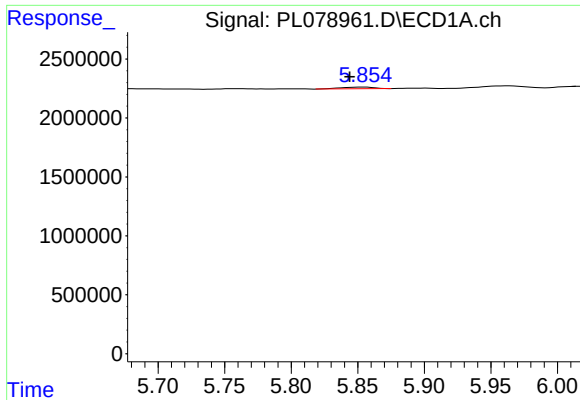

#9 Endosulfan I


R.T.: 5.855 min
Delta R.T.: 0.011 min
Response: 251514
Conc: 0.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

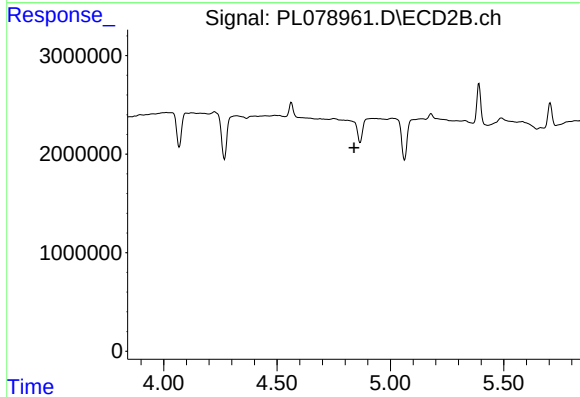


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 4.840 min
Response: 0
Conc: N.D.

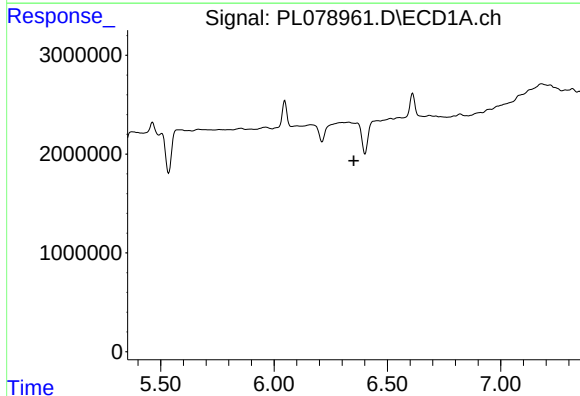


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.351 min
Response: 0
Conc: N.D.

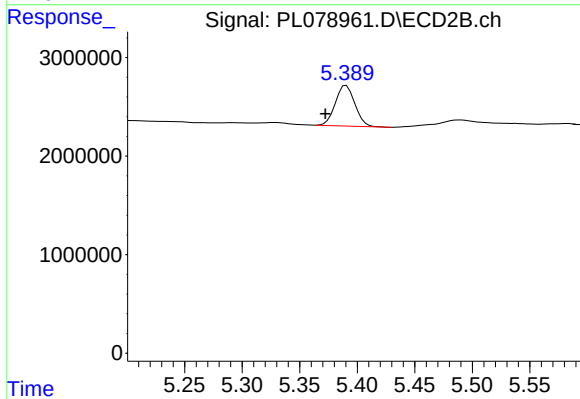

#14 Endrin


R.T.: 5.390 min
Delta R.T.: 0.018 min
Response: 4901848
Conc: 1.88 ng/ml

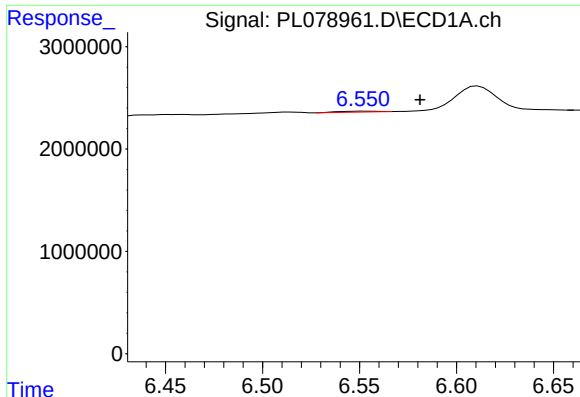

#15 Endosulfan II


R.T.: 6.553 min
Delta R.T.: -0.028 min
Response: 127077
Conc: 0.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

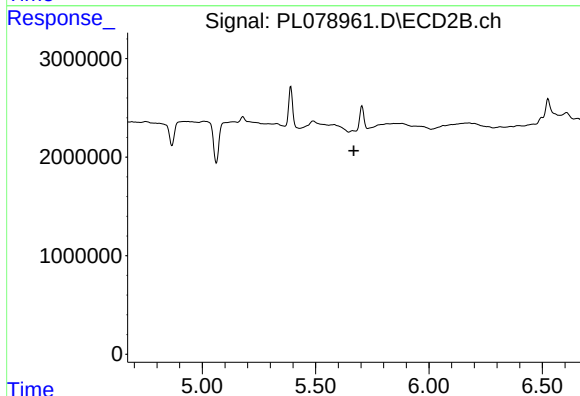


#15 Endosulfan II

R.T.: 5.663 min
Delta R.T.: -0.005 min
Response: -201065
Conc: N.D.

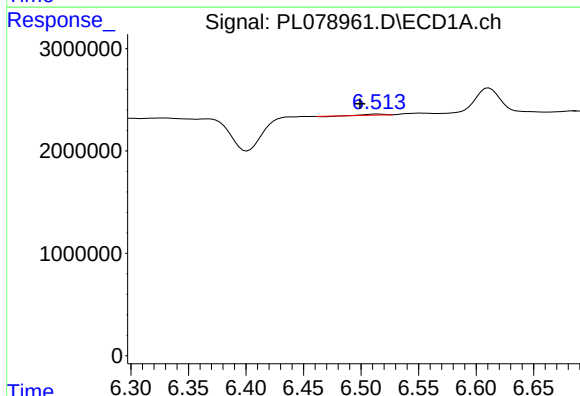


#16 4,4'-DDD

R.T.: 6.514 min
Delta R.T.: 0.015 min
Response: 102530
Conc: 0.06 ng/ml

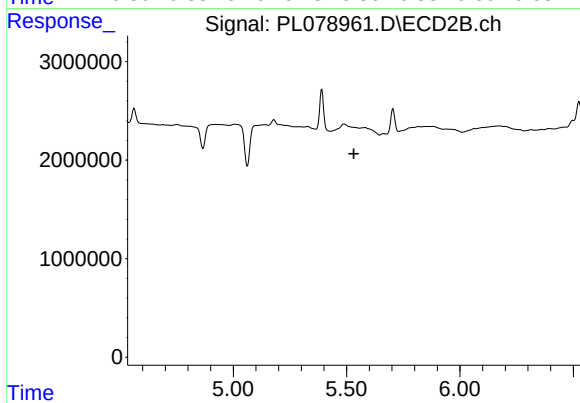

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.532 min
Response: 0
Conc: N.D.

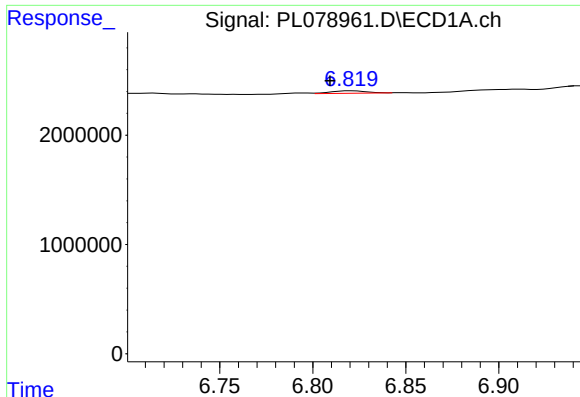

#17 4,4'-DDT


R.T.: 6.821 min
Delta R.T.: 0.011 min
Response: 300396
Conc: 0.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

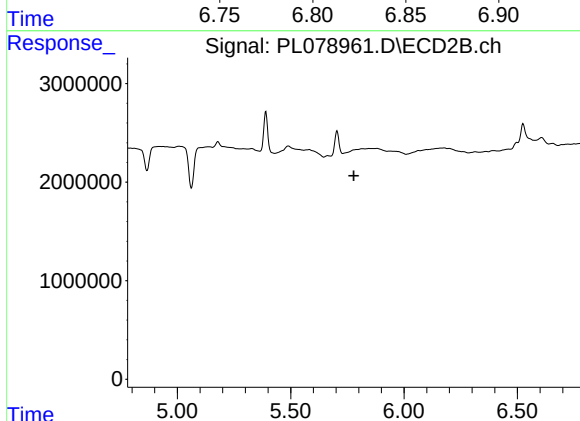


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 5.779 min
Response: 0
Conc: N.D.

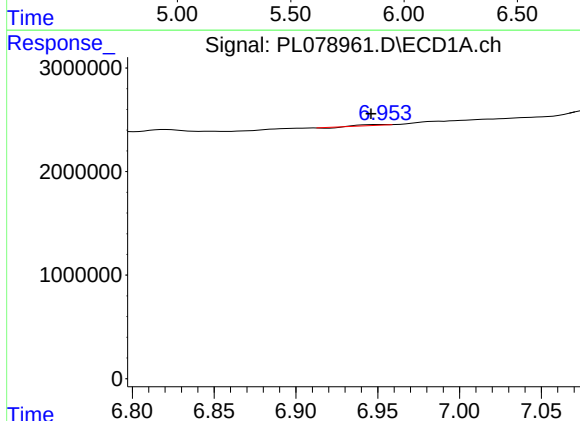


#19 Endosulfan Sulfate

R.T.: 6.954 min
Delta R.T.: 0.008 min
Response: 40362
Conc: 0.02 ng/ml

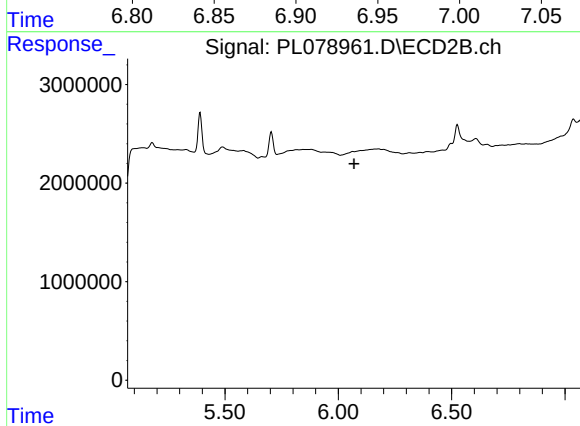

#19 Endosulfan Sulfate


R.T.: 6.064 min
Delta R.T.: -0.006 min
Response: -372818
Conc: N.D.

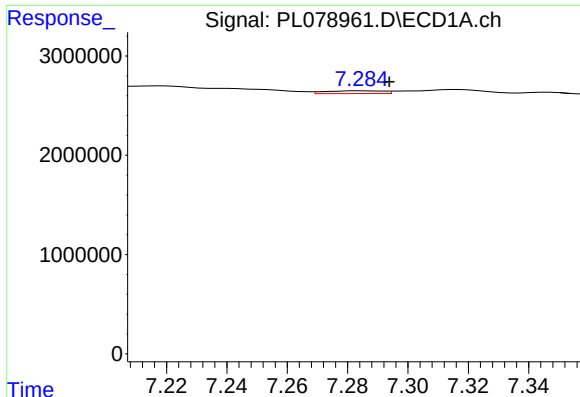

#20 Methoxychlor


R.T.: 7.285 min
Delta R.T.: -0.009 min
Response: 373772
Conc: 0.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

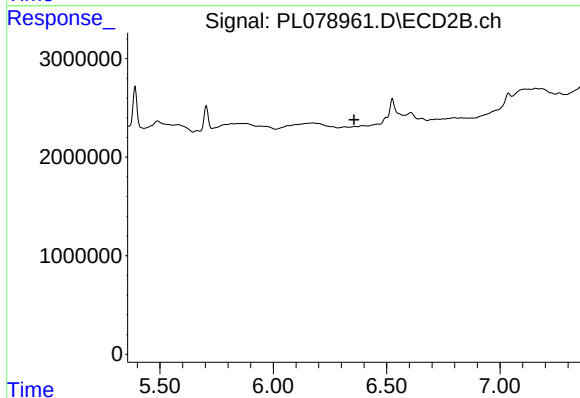


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.357 min
Response: 0
Conc: N.D.

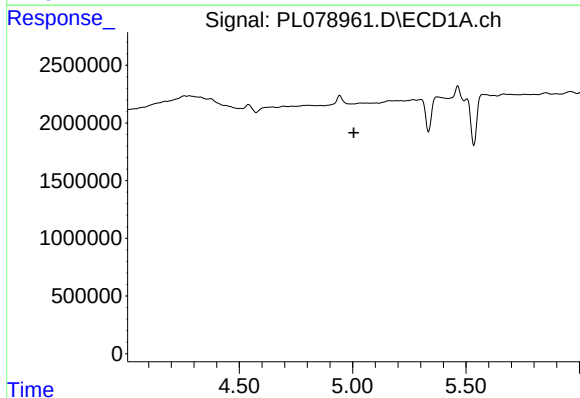


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.005 min
Response: 0
Conc: N.D.

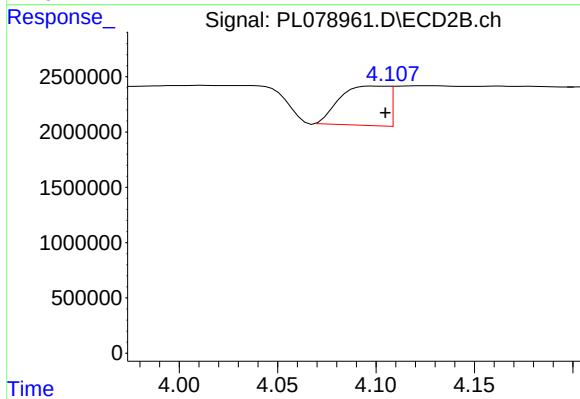

#24 Chlordane-2


R.T.: 4.098 min
Delta R.T.: -0.006 min
Response: 6007578
Conc: 56.45 ng/ml

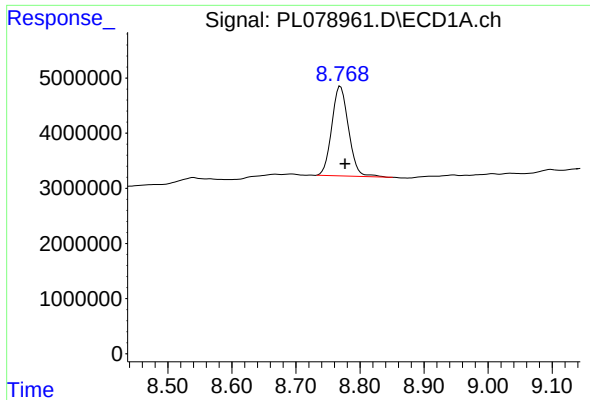

#28 Decachlorobiphenyl

R.T.: 8.770 min
Delta R.T.: -0.007 min
Response: 29513335
Conc: 19.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

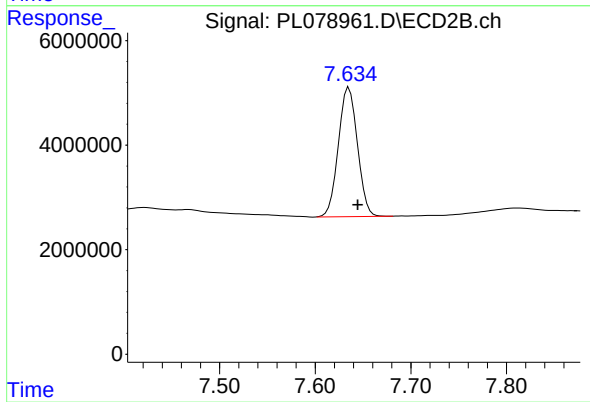

#28 Decachlorobiphenyl

R.T.: 7.635 min
Delta R.T.: -0.009 min
Response: 34377044
Conc: 18.15 ng/ml