

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110922\
 Data File : PL078971.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2022 17:52
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 21:16:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.321	2.568	40452088	53700770	21.212	21.033
28)	SA Decachlor...	8.768	7.634	27602913	34381097	18.349	18.152
Target Compounds							
8)	B Heptachlo...	5.462	4.494f	6734159	1641939	3.172	0.545 #
10)	B gamma-Chl...	5.704	0.000	427587	0	0.189	N.D. #
13)	MA Dieldrin	0.000	5.095	0	4900022	N.D.	1.654 #
14)	MA Endrin	0.000	5.390f	0	4525464	N.D.	1.737 #
17)	MA 4,4'-DDT	6.828f	0.000	510308	0	0.285	N.D. #
20)	A Methoxychlor	7.299	0.000	204899	0	0.223	N.D. #
24)	Chlordane-2	0.000	4.100	0	8052529	N.D.	75.663 #
25)	Chlordane-3	5.704	0.000	427587	0	1.280	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110922\
Data File : PL078971.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2022 17:52
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 21:16:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

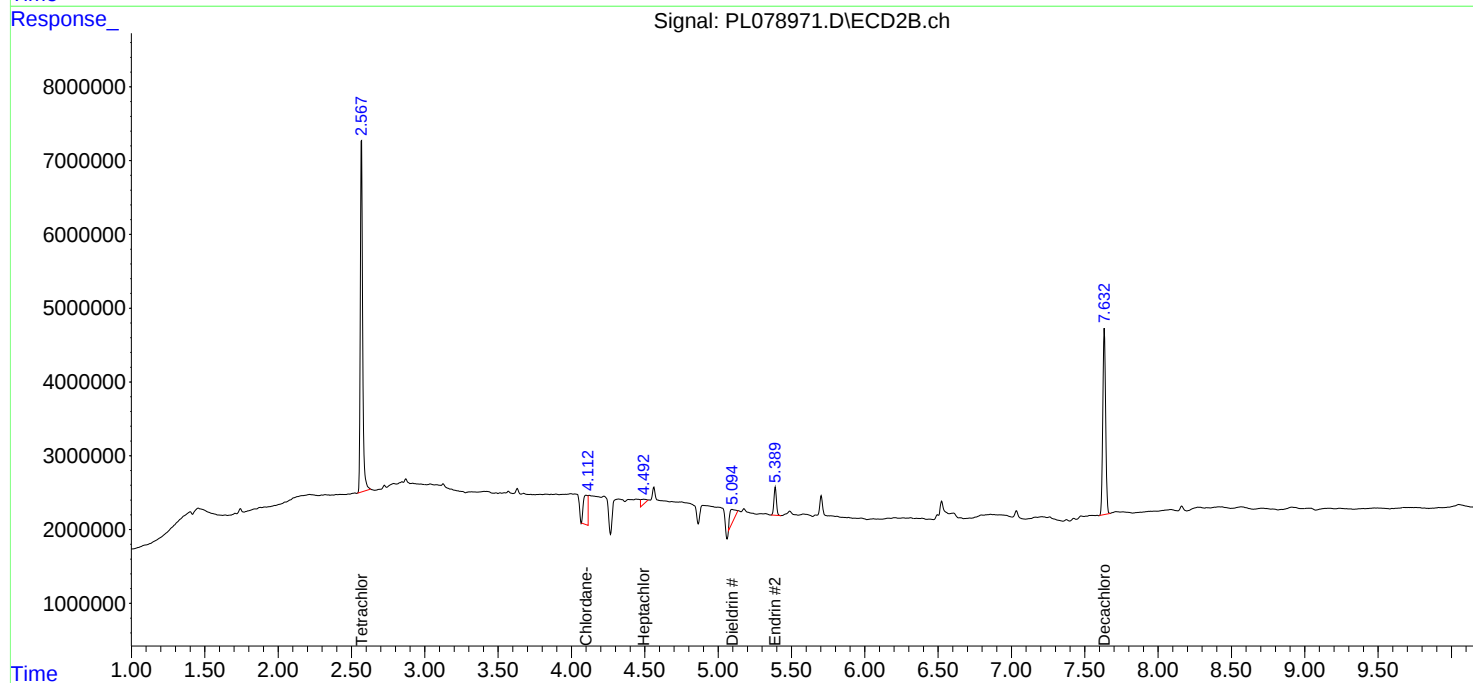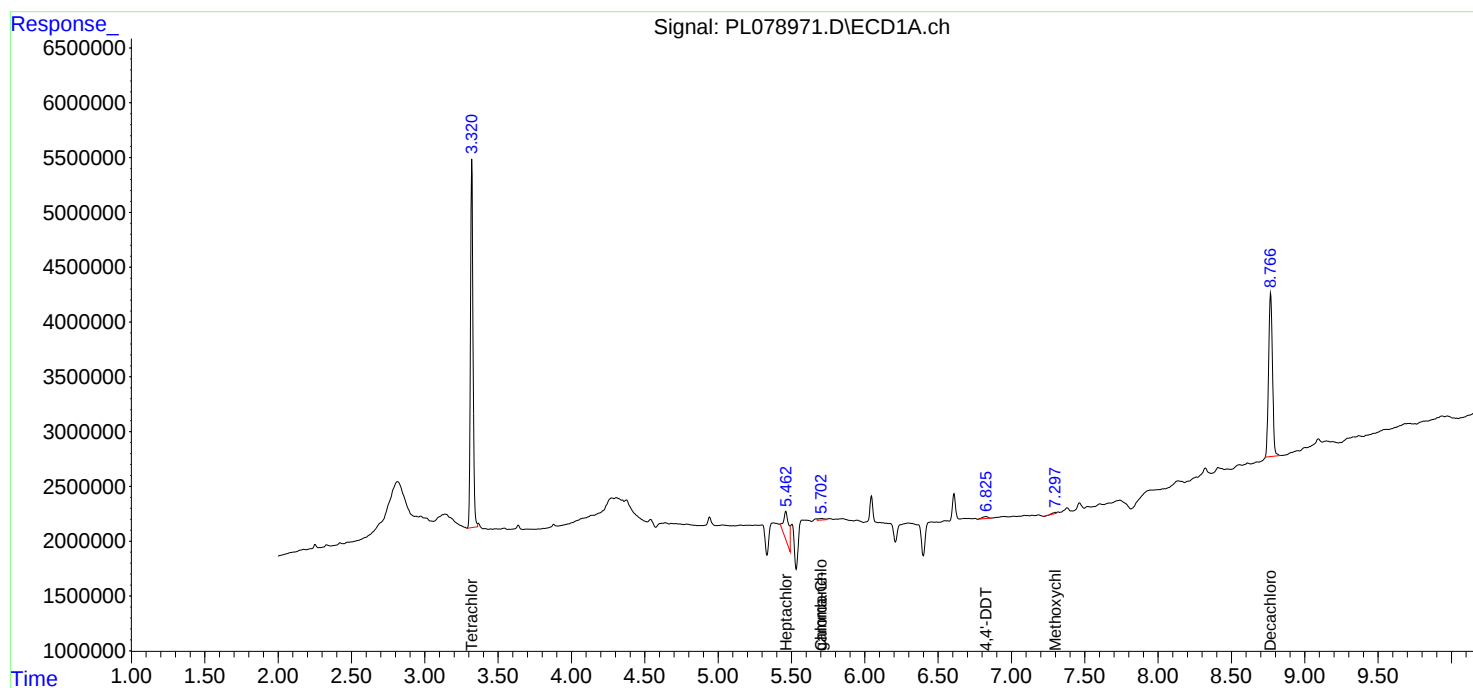


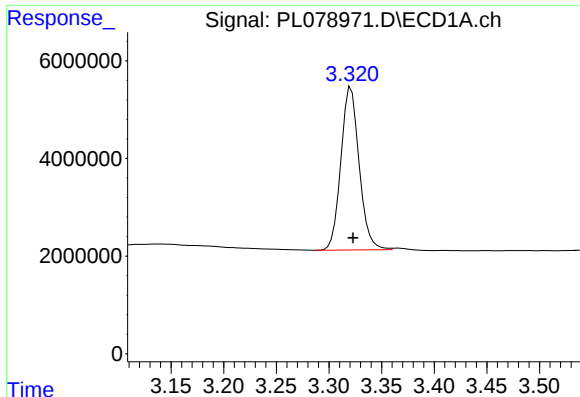

#1 Tetrachloro-m-xylene


R.T.: 3.321 min
Delta R.T.: -0.002 min
Response: 40452088
Conc: 21.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

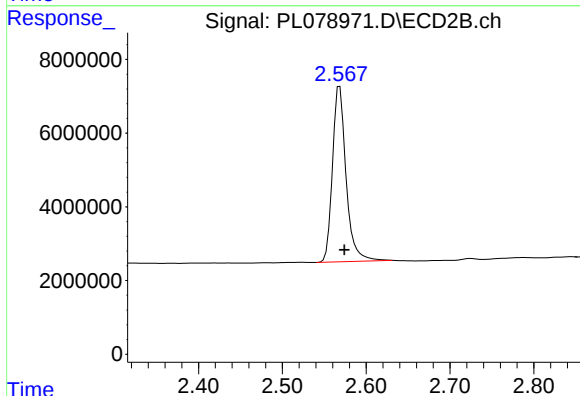


#1 Tetrachloro-m-xylene

R.T.: 2.568 min
Delta R.T.: -0.005 min
Response: 53700770
Conc: 21.03 ng/ml

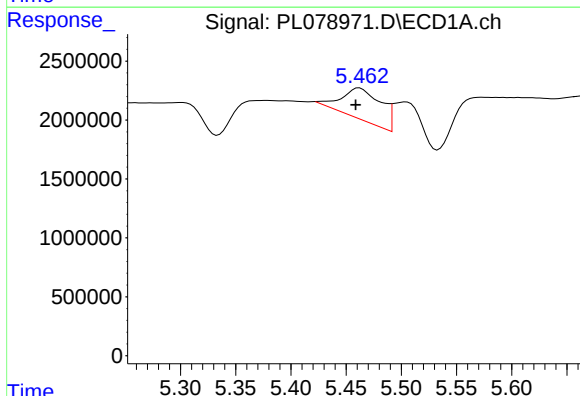


#8 Heptachlor epoxide

R.T.: 5.462 min
Delta R.T.: 0.003 min
Response: 6734159
Conc: 3.17 ng/ml

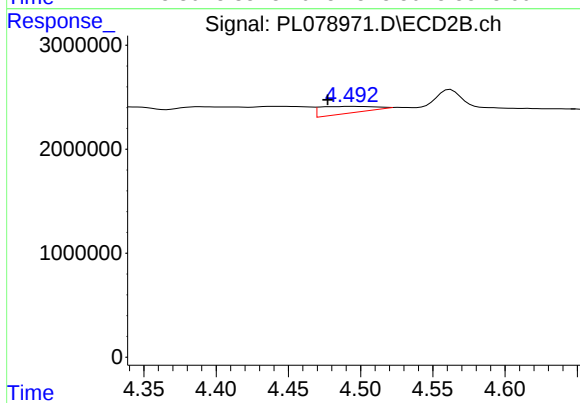

#8 Heptachlor epoxide


R.T.: 4.494 min
Delta R.T.: 0.017 min
Response: 1641939
Conc: 0.54 ng/ml

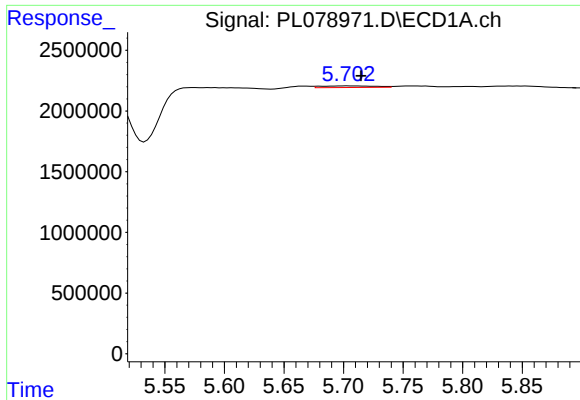

#10 gamma-Chlordane


R.T.: 5.704 min
Delta R.T.: -0.010 min
Response: 427587
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

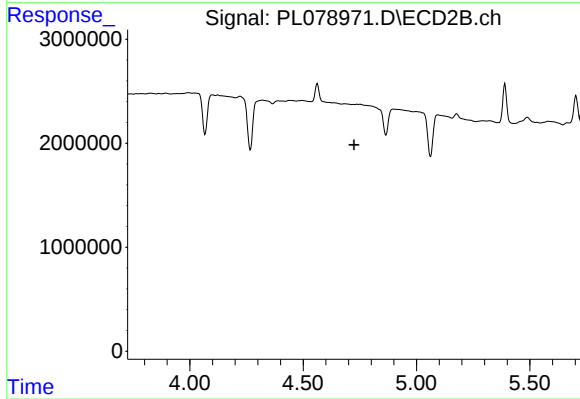


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.725 min
Response: 0
Conc: N.D.

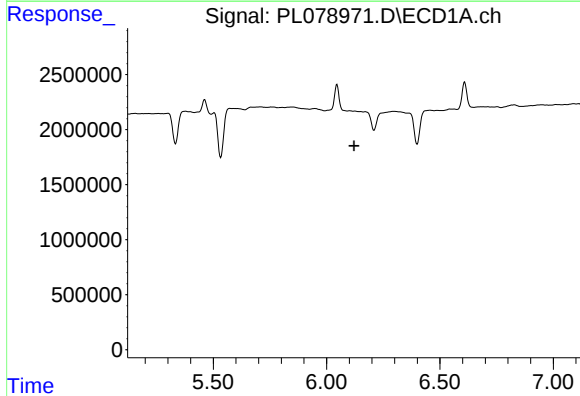


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.121 min
Response: 0
Conc: N.D.

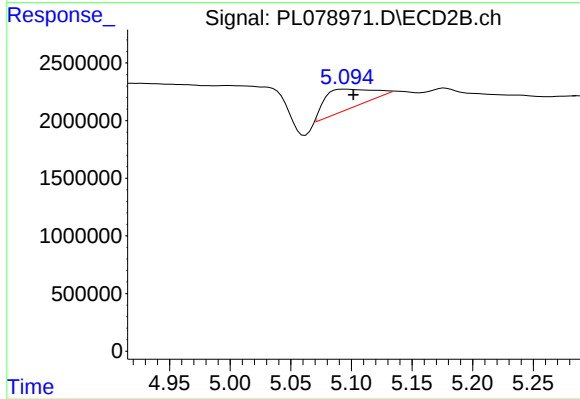

#13 Dieldrin


R.T.: 5.095 min
Delta R.T.: -0.006 min
Response: 490022
Conc: 1.65 ng/ml

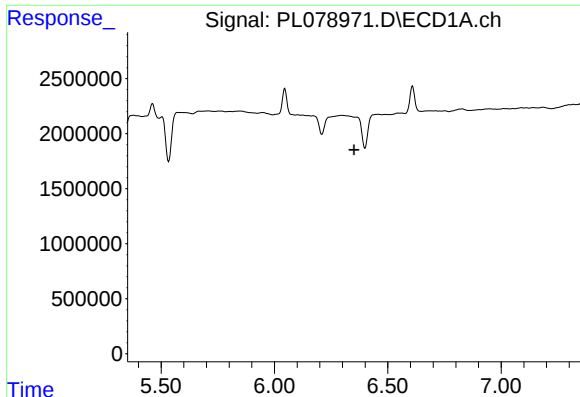

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.351 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

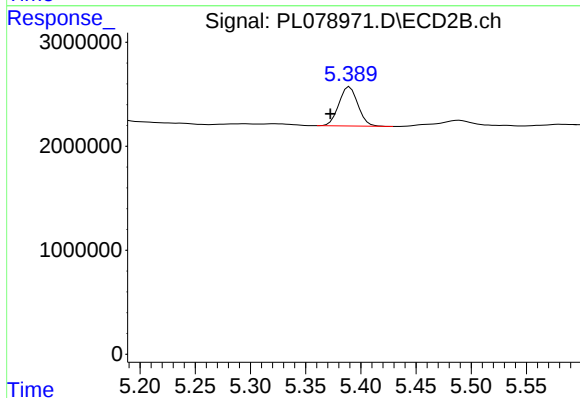


#14 Endrin

R.T.: 5.390 min
Delta R.T.: 0.017 min
Response: 4525464
Conc: 1.74 ng/ml

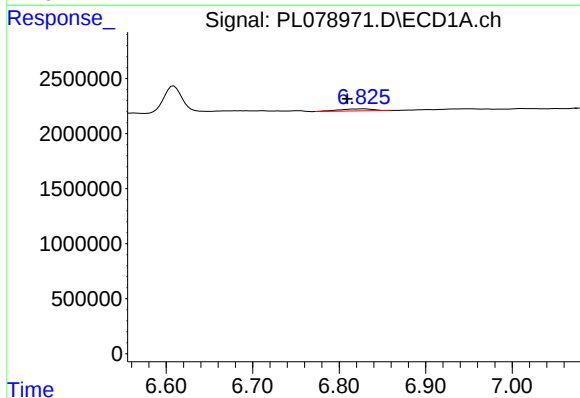


#17 4,4'-DDT

R.T.: 6.828 min
Delta R.T.: 0.018 min
Response: 510308
Conc: 0.28 ng/ml

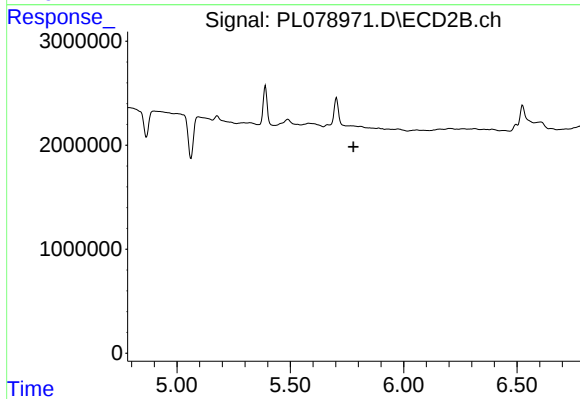

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 5.779 min
Response: 0
Conc: N.D.

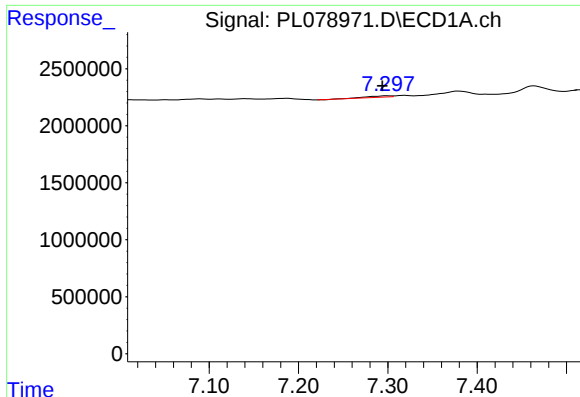

#20 Methoxychlor


R.T.: 7.299 min
Delta R.T.: 0.005 min
Response: 204899
Conc: 0.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

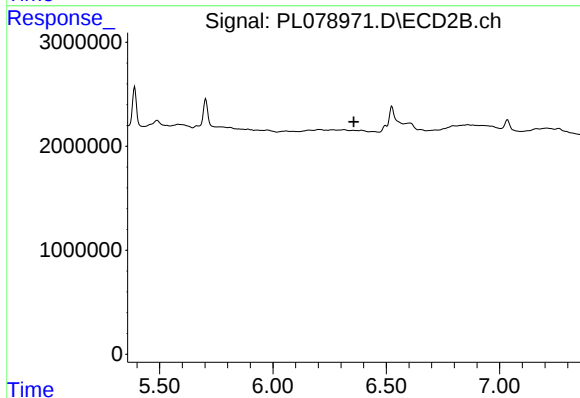


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.357 min
Response: 0
Conc: N.D.

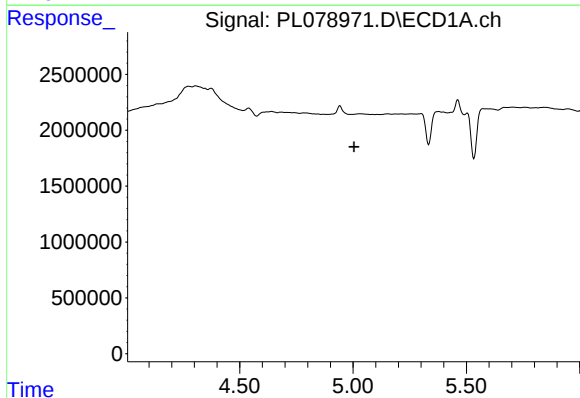


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.005 min
Response: 0
Conc: N.D.

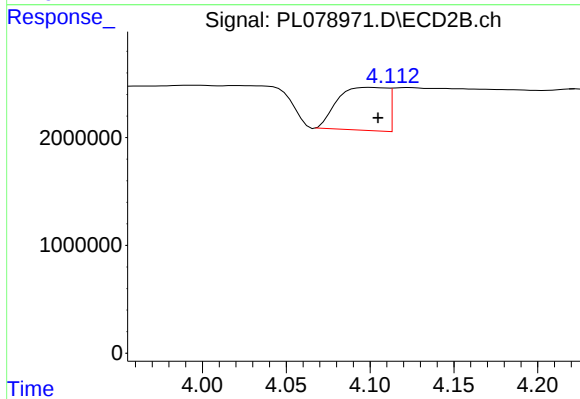

#24 Chlordane-2


R.T.: 4.100 min
Delta R.T.: -0.005 min
Response: 8052529
Conc: 75.66 ng/ml

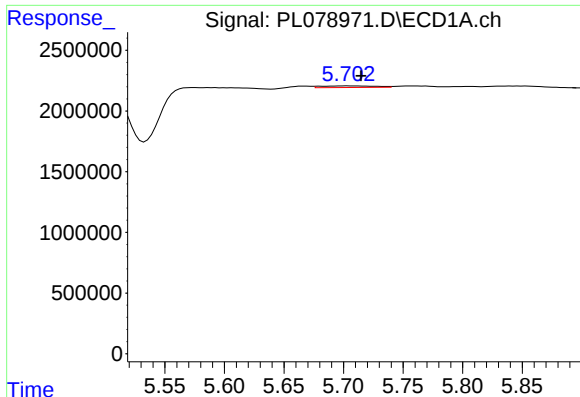

#25 Chlordane-3


R.T.: 5.704 min
Delta R.T.: -0.010 min
Response: 427587
Conc: 1.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

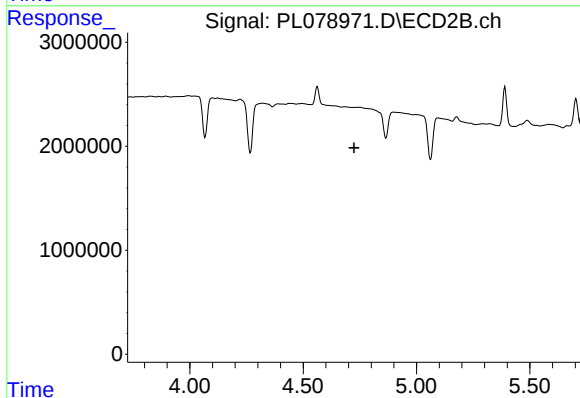


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 4.725 min
Response: 0
Conc: N.D.

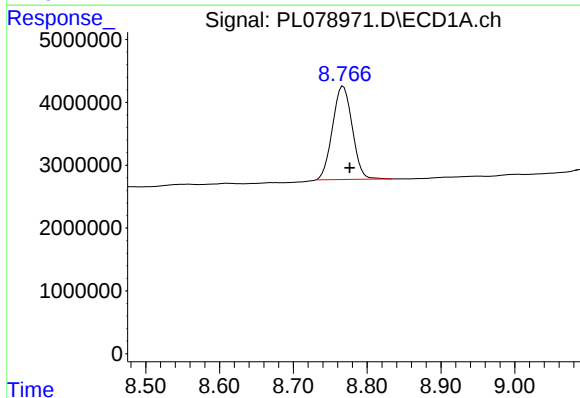

#28 Decachlorobiphenyl

R.T.: 8.768 min
Delta R.T.: -0.009 min
Response: 27602913
Conc: 18.35 ng/ml

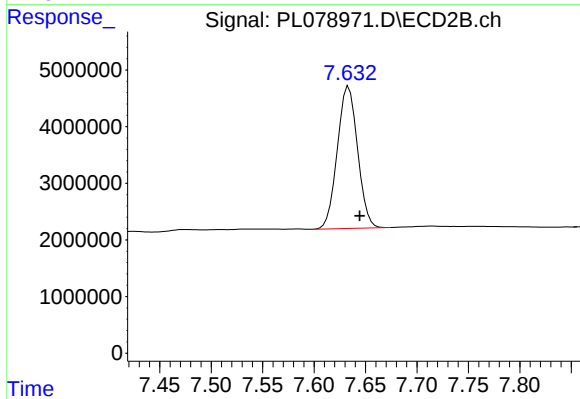

#28 Decachlorobiphenyl

R.T.: 7.634 min
Delta R.T.: -0.011 min
Response: 34381097
Conc: 18.15 ng/ml