

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110922\
 Data File : PL078977.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2022 20:24
 Operator : AR\AJ
 Sample : N5509-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 09:09:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.321	2.568	27180963	35885372	14.253	14.055
28)	SA Decachlor...	8.768	7.633	16546135	22805279	10.999	12.040
Target Compounds							
3)	MA gamma-BHC...	4.134f	0.000	139194	0	0.052	N.D. #
8)	B Heptachlo...	0.000	4.487	0	177564	N.D.	0.059 #
10)	B gamma-Chl...	0.000	4.743f	0	1214266	N.D.	0.396 #
11)	B alpha-Chl...	5.788	0.000	720574	0	0.311	N.D. #
12)	B 4,4'-DDE	0.000	5.012f	0	56457	N.D.	0.021 #
13)	MA Dieldrin	6.146f	0.000	87026	0	0.040	N.D. #
14)	MA Endrin	6.335f	5.389f	372694	475469	0.196	0.183
20)	A Methoxychlor	7.316f	0.000	163124	0	0.177	N.D. #
25)	Chlordane-3	0.000	4.743f	0	1214266	N.D.	3.984 #
26)	Chlordane-4	5.788	0.000	720574	0	1.755	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110922\
Data File : PL078977.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2022 20:24
Operator : AR\AJ
Sample : N5509-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 09:09:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

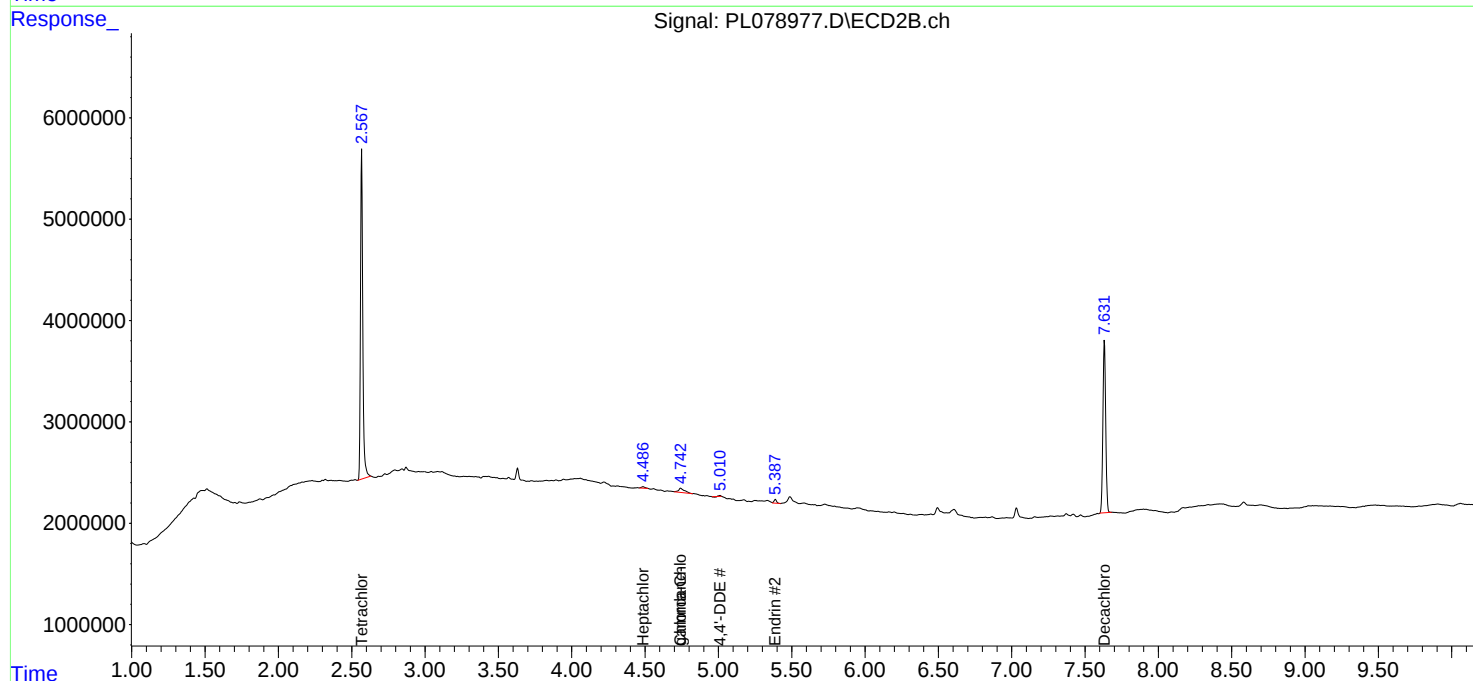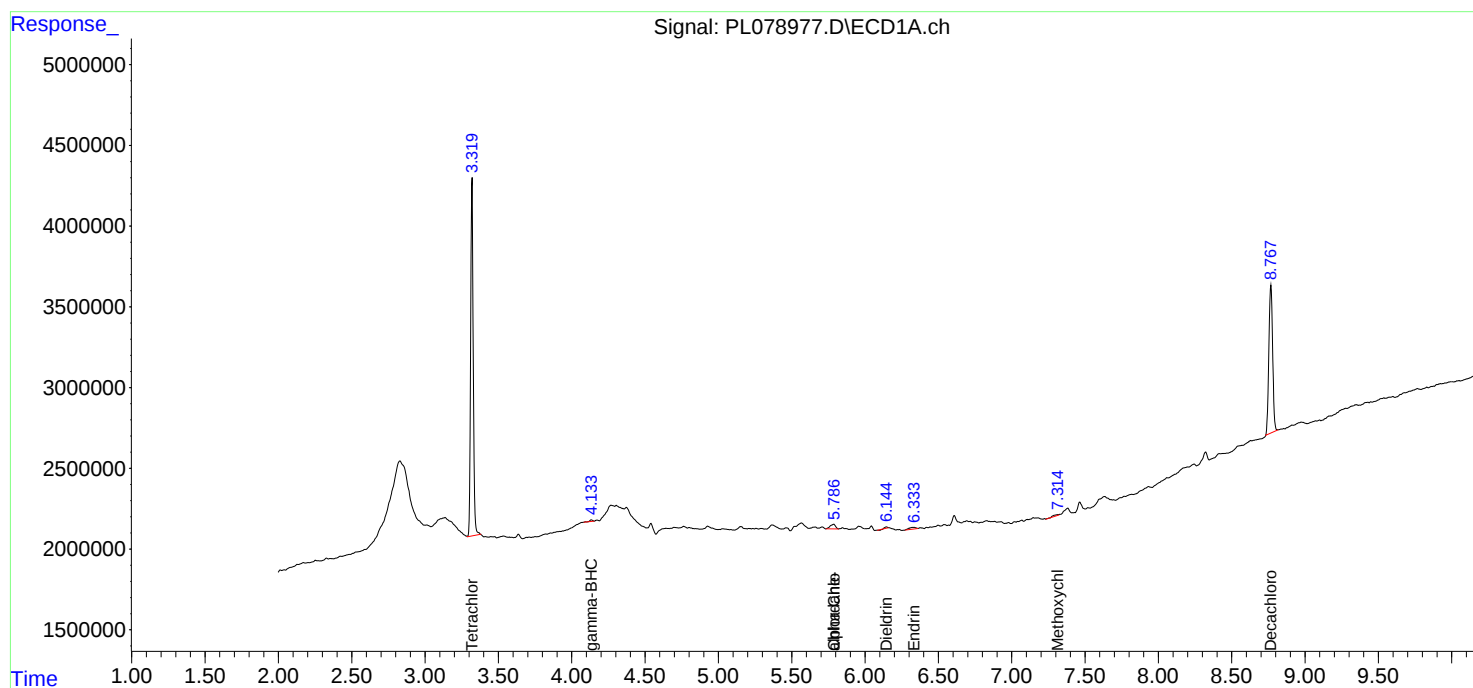


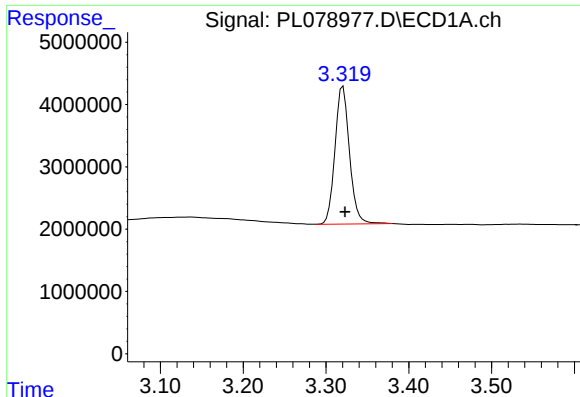

#1 Tetrachloro-m-xylene


R.T.: 3.321 min
Delta R.T.: -0.002 min
Response: 27180963
Conc: 14.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7

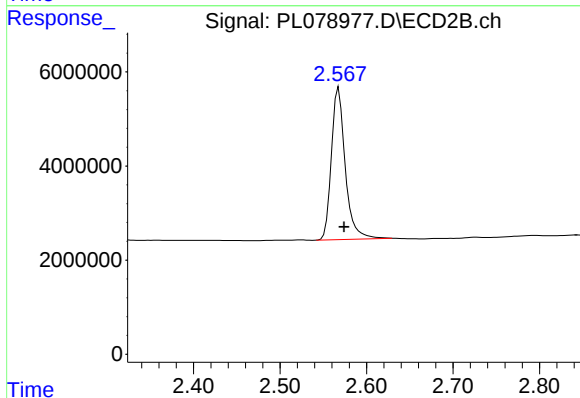


#1 Tetrachloro-m-xylene

R.T.: 2.568 min
Delta R.T.: -0.006 min
Response: 35885372
Conc: 14.06 ng/ml

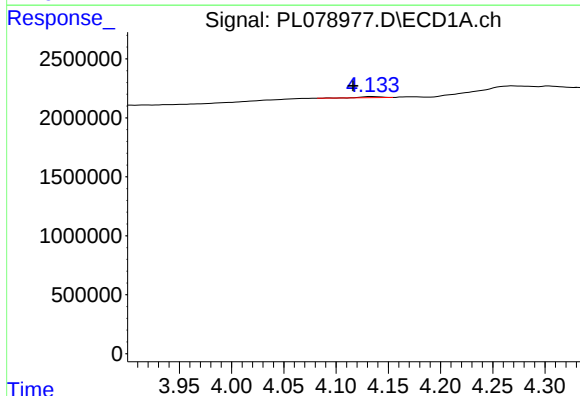


#3 gamma-BHC (Lindane)

R.T.: 4.134 min
Delta R.T.: 0.018 min
Response: 139194
Conc: 0.05 ng/ml

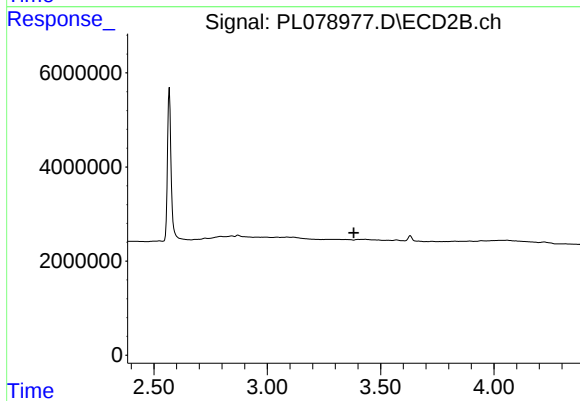

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 3.382 min
Response: 0
Conc: N.D.

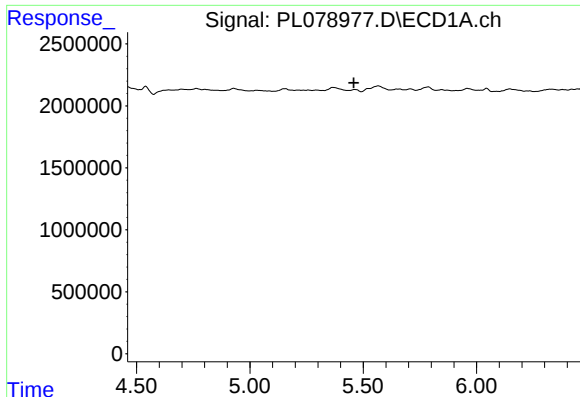

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.459 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-7

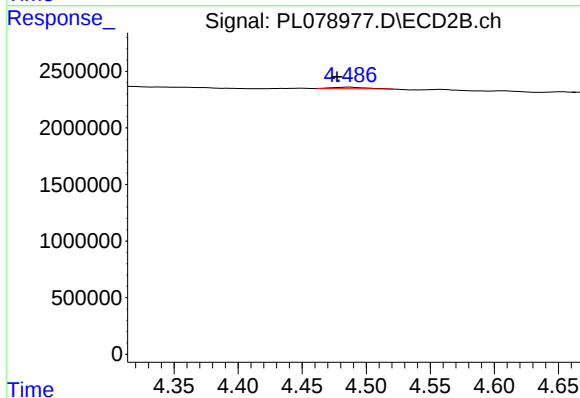


#8 Heptachlor epoxide

R.T.: 4.487 min
Delta R.T.: 0.010 min
Response: 177564
Conc: 0.06 ng/ml

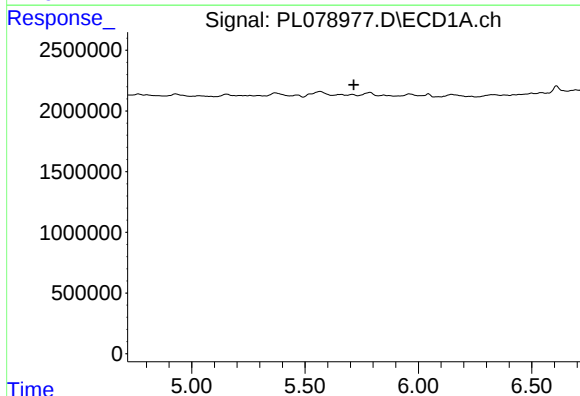


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.715 min
Response: 0
Conc: N.D.

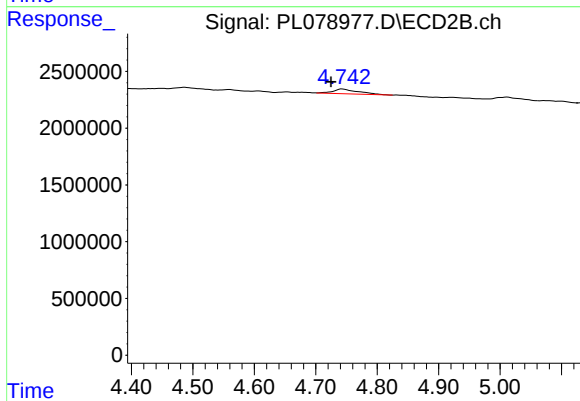

#10 gamma-Chlordane


R.T.: 4.743 min
Delta R.T.: 0.018 min
Response: 1214266
Conc: 0.40 ng/ml

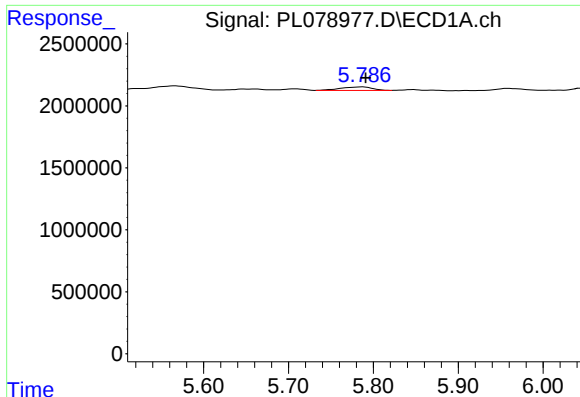

#11 alpha-Chlordane


R.T.: 5.788 min
Delta R.T.: -0.003 min
Response: 720574
Conc: 0.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7

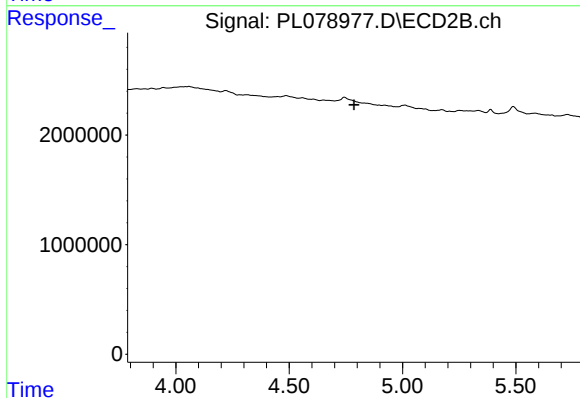


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.787 min
Response: 0
Conc: N.D.

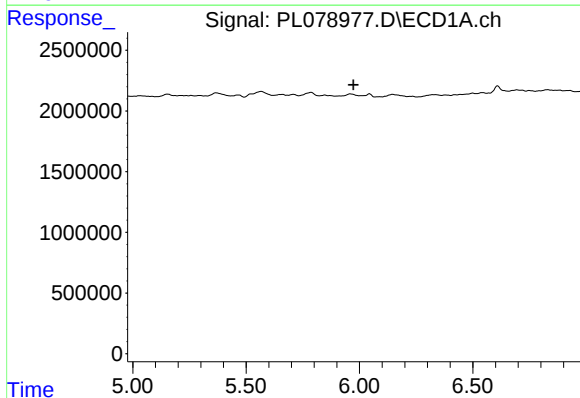


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.974 min
Response: 0
Conc: N.D.

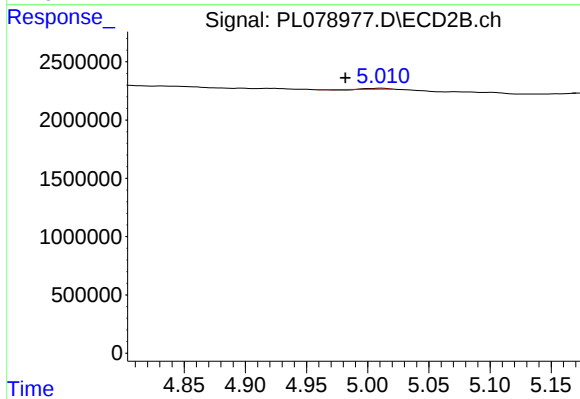

#12 4,4'-DDE


R.T.: 5.012 min
Delta R.T.: 0.030 min
Response: 56457
Conc: 0.02 ng/ml

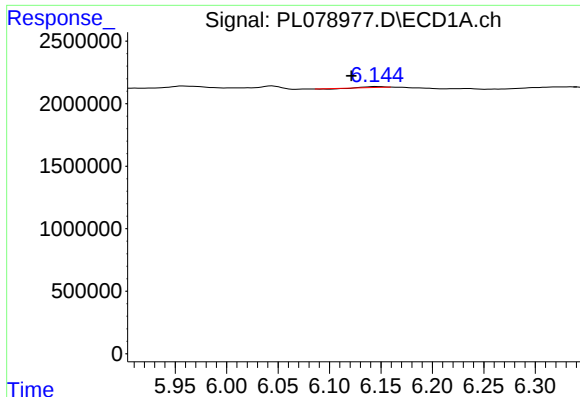

#13 Dieldrin


R.T.: 6.146 min
Delta R.T.: 0.025 min
Response: 87026
Conc: 0.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7

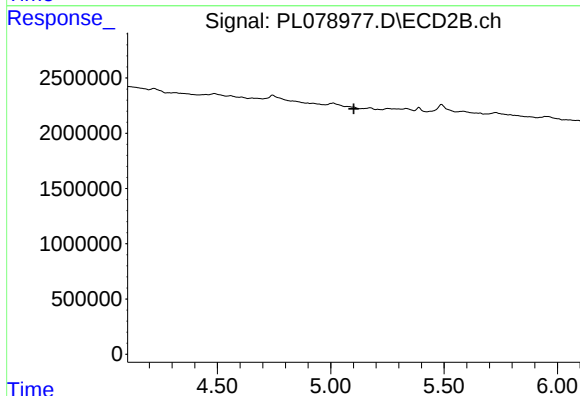


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 5.102 min
Response: 0
Conc: N.D.

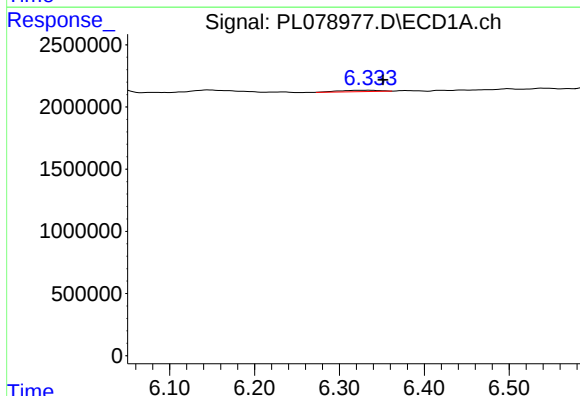


#14 Endrin

R.T.: 6.335 min
Delta R.T.: -0.017 min
Response: 372694
Conc: 0.20 ng/ml

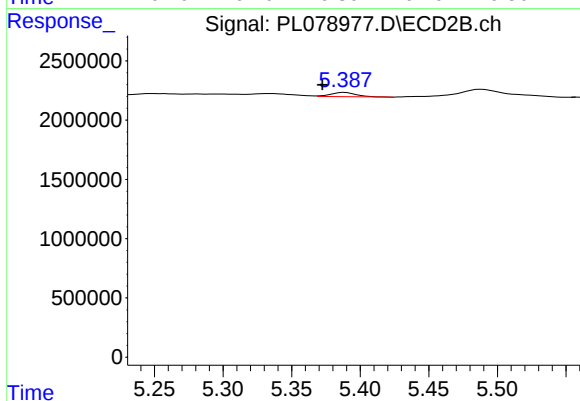

#14 Endrin


R.T.: 5.389 min
Delta R.T.: 0.016 min
Response: 475469
Conc: 0.18 ng/ml

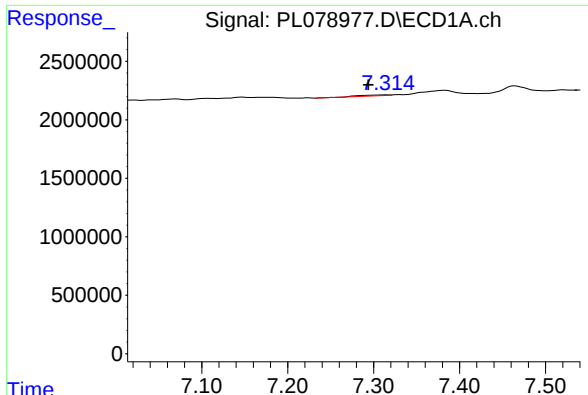

#20 Methoxychlor


R.T.: 7.316 min
Delta R.T.: 0.023 min
Response: 163124
Conc: 0.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7

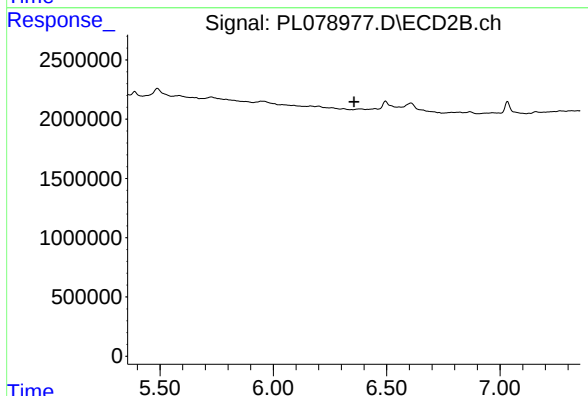


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.357 min
Response: 0
Conc: N.D.

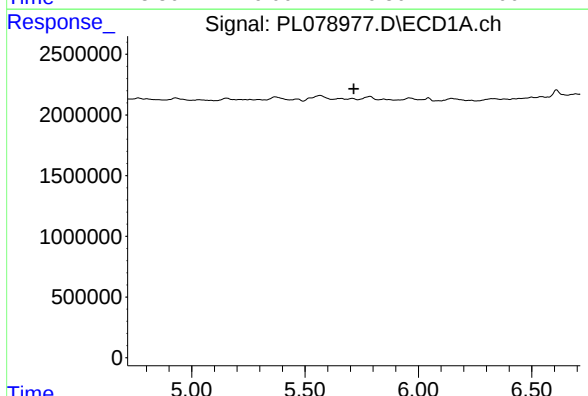


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.715 min
Response: 0
Conc: N.D.

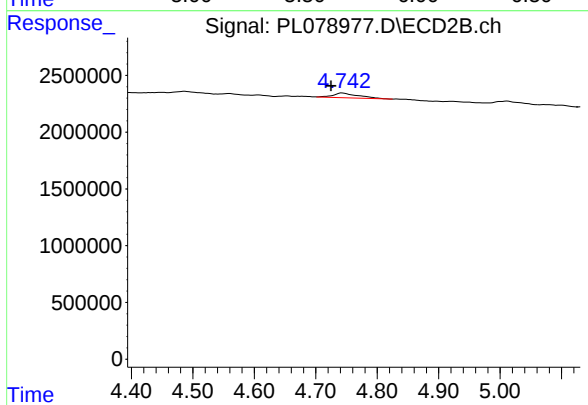

#25 Chlordane-3


R.T.: 4.743 min
Delta R.T.: 0.018 min
Response: 1214266
Conc: 3.98 ng/ml

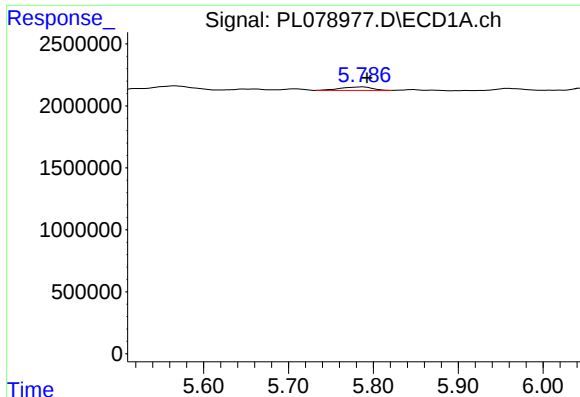

#26 Chlordane-4


R.T.: 5.788 min
Delta R.T.: -0.005 min
Response: 720574
Conc: 1.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7

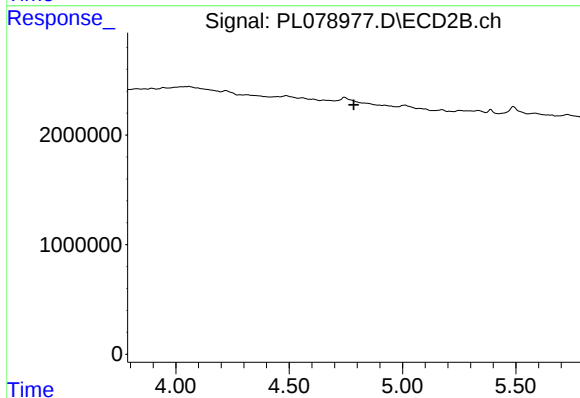


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 4.785 min
Response: 0
Conc: N.D.

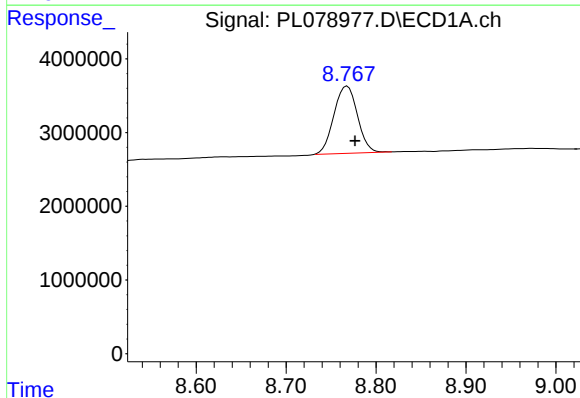

#28 Decachlorobiphenyl

R.T.: 8.768 min
Delta R.T.: -0.008 min
Response: 16546135
Conc: 11.00 ng/ml

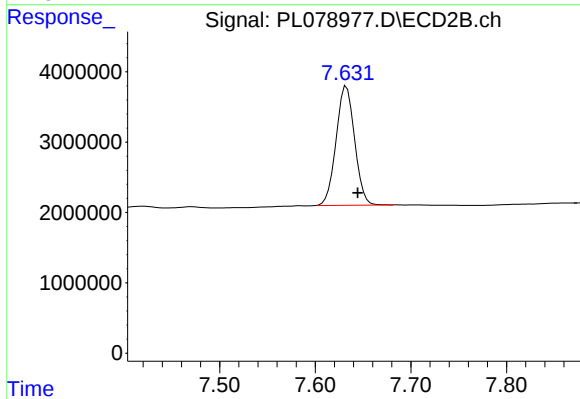

#28 Decachlorobiphenyl

R.T.: 7.633 min
Delta R.T.: -0.012 min
Response: 22805279
Conc: 12.04 ng/ml