

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110922\
 Data File : PL078965.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2022 16:15
 Operator : AR\AJ
 Sample : N5506-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 21:10:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.322	2.569	26227186	33966016	13.753	13.303
28)	SA Decachlor...	8.770	7.636	16522236	19662399	10.983	10.381
Target Compounds							
10)	B gamma-Chl...	5.713	4.720	10074865	8937221	4.464	2.916 #
11)	B alpha-Chl...	5.790	4.780	15922808	13667168	6.882	4.586 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110922\
Data File : PL078965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2022 16:15
Operator : AR\AJ
Sample : N5506-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 21:10:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

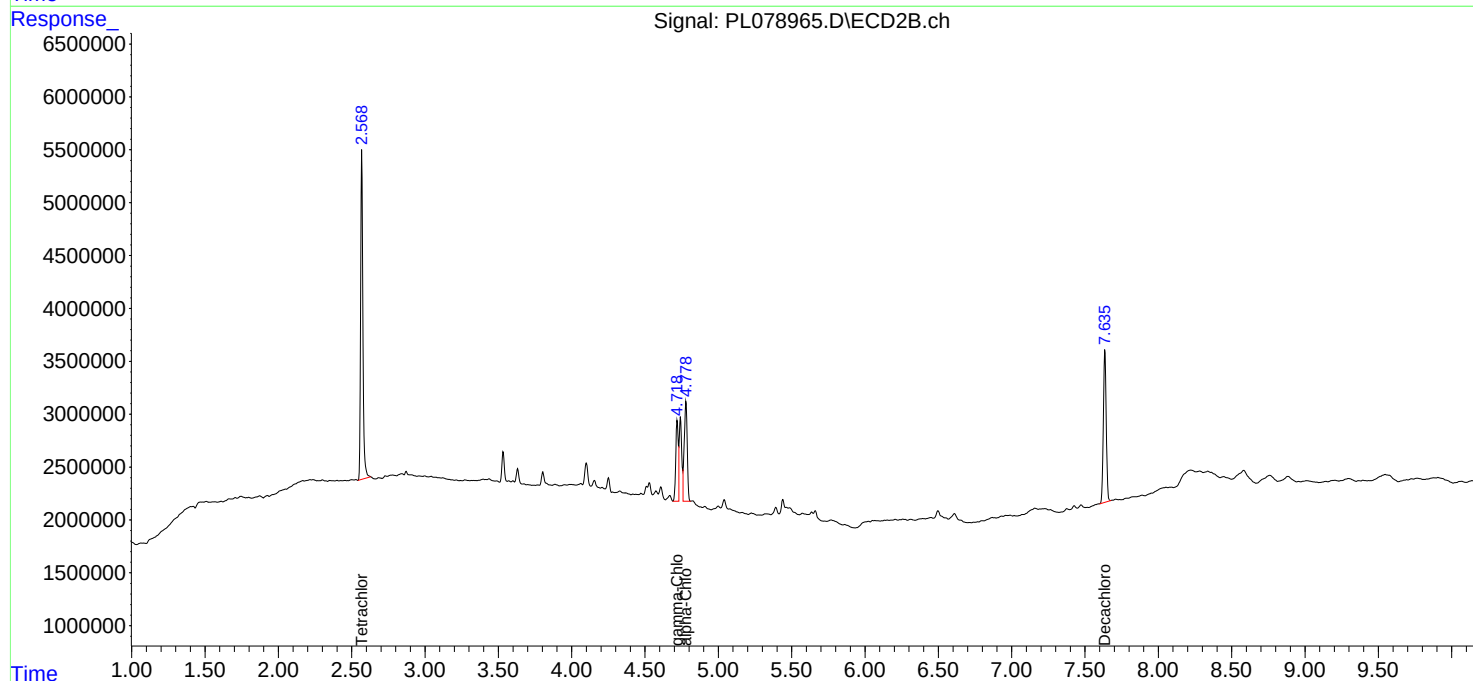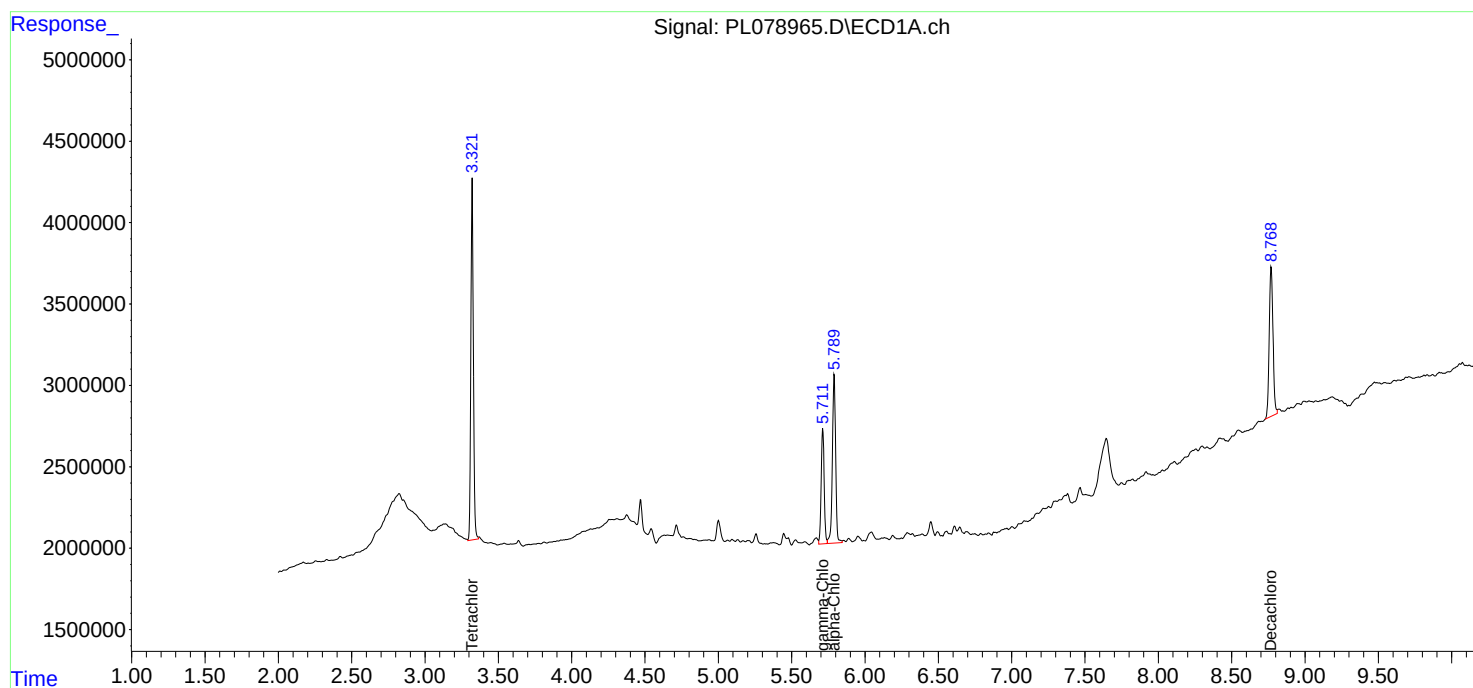


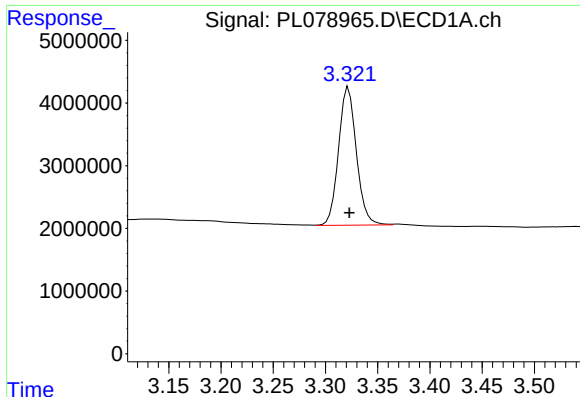

#1 Tetrachloro-m-xylene


R.T.: 3.322 min
Delta R.T.: 0.000 min
Response: 26227186
Conc: 13.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6

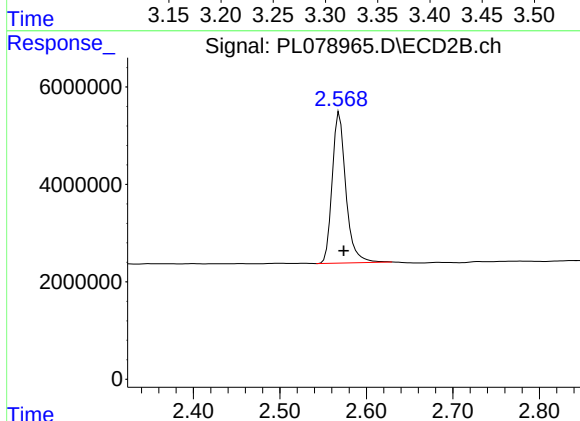


#1 Tetrachloro-m-xylene

R.T.: 2.569 min
Delta R.T.: -0.005 min
Response: 33966016
Conc: 13.30 ng/ml

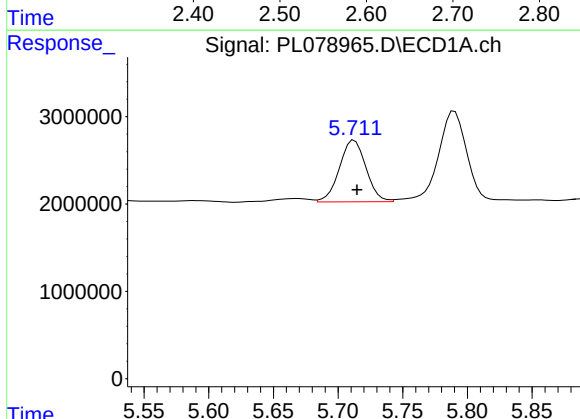


#10 gamma-Chlordane

R.T.: 5.713 min
Delta R.T.: -0.002 min
Response: 10074865
Conc: 4.46 ng/ml

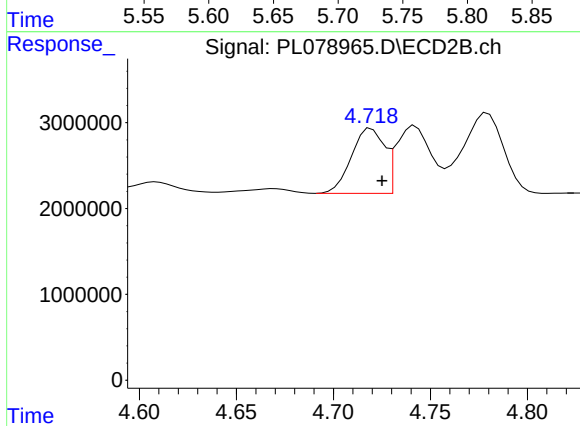

#10 gamma-Chlordane


R.T.: 4.720 min
Delta R.T.: -0.006 min
Response: 8937221
Conc: 2.92 ng/ml

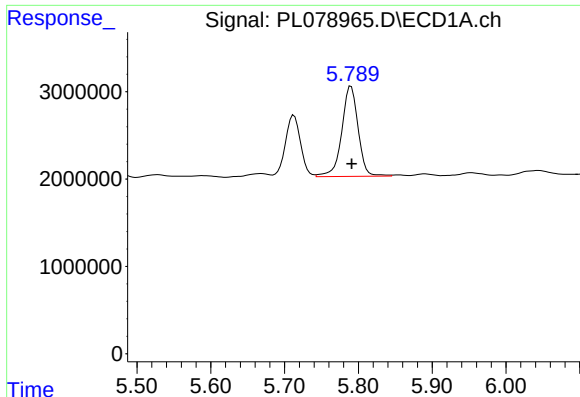

#11 alpha-Chlordane


R.T.: 5.790 min
Delta R.T.: 0.000 min
Response: 15922808
Conc: 6.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6

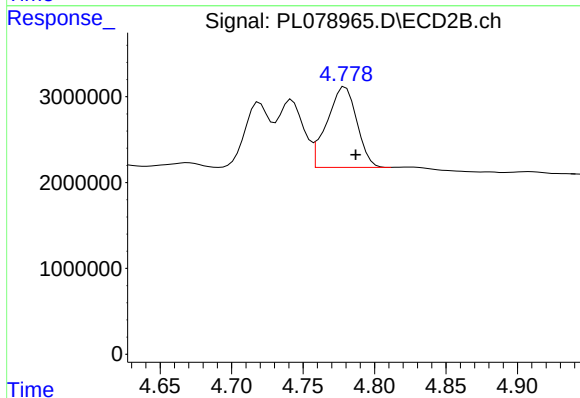


#11 alpha-Chlordane

R.T.: 4.780 min
Delta R.T.: -0.007 min
Response: 13667168
Conc: 4.59 ng/ml

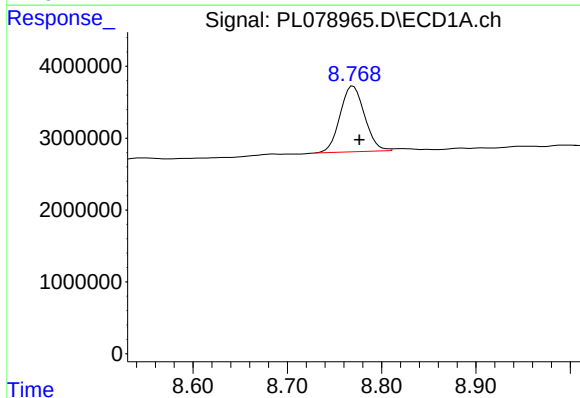

#28 Decachlorobiphenyl

R.T.: 8.770 min
Delta R.T.: -0.007 min
Response: 16522236
Conc: 10.98 ng/ml

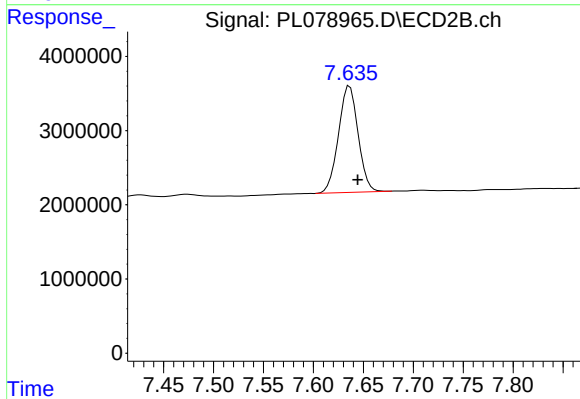

#28 Decachlorobiphenyl

R.T.: 7.636 min
Delta R.T.: -0.008 min
Response: 19662399
Conc: 10.38 ng/ml