

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111223\
 Data File : PD079551.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2023 14:01
 Operator : AR\AJ
 Sample : PB156874BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 20:18:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 20 04:44:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.804	28084986	43446710	17.395	18.765
28)	SA Decachlor...	9.117	7.949	37093259	50312983	18.491	20.641
Target Compounds							
2)	A alpha-BHC	0.000	3.296	0	112701	N.D.	0.033 #
7)	B delta-BHC	4.796	4.187f	377340	206905	0.141	0.062 #
11)	B alpha-Chl...	0.000	5.102f	0	312244	N.D.	0.109 #
13)	MA Dieldrin	6.392	0.000	675239	0	0.290	N.D. #
15)	B Endosulfa...	6.828	0.000	166070	0	0.081	N.D. #
19)	B Endosulfa...	0.000	6.369	0	574055	N.D.	0.246 #
20)	A Methoxychlor	0.000	6.641	0	30518	N.D.	0.022 #
21)	B Endrin ke...	7.714f	0.000	157041	0	0.072	N.D. #
26)	Chlordane-4	0.000	5.102f	0	312244	N.D.	1.272 #
27)	Chlordane-5	6.905	0.000	176626	0	2.514	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111223\
Data File : PD079551.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2023 14:01
Operator : AR\AJ
Sample : PB156874BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 20:18:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
Quant Title : GC Extractables
QLast Update : Fri Oct 20 04:44:01 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

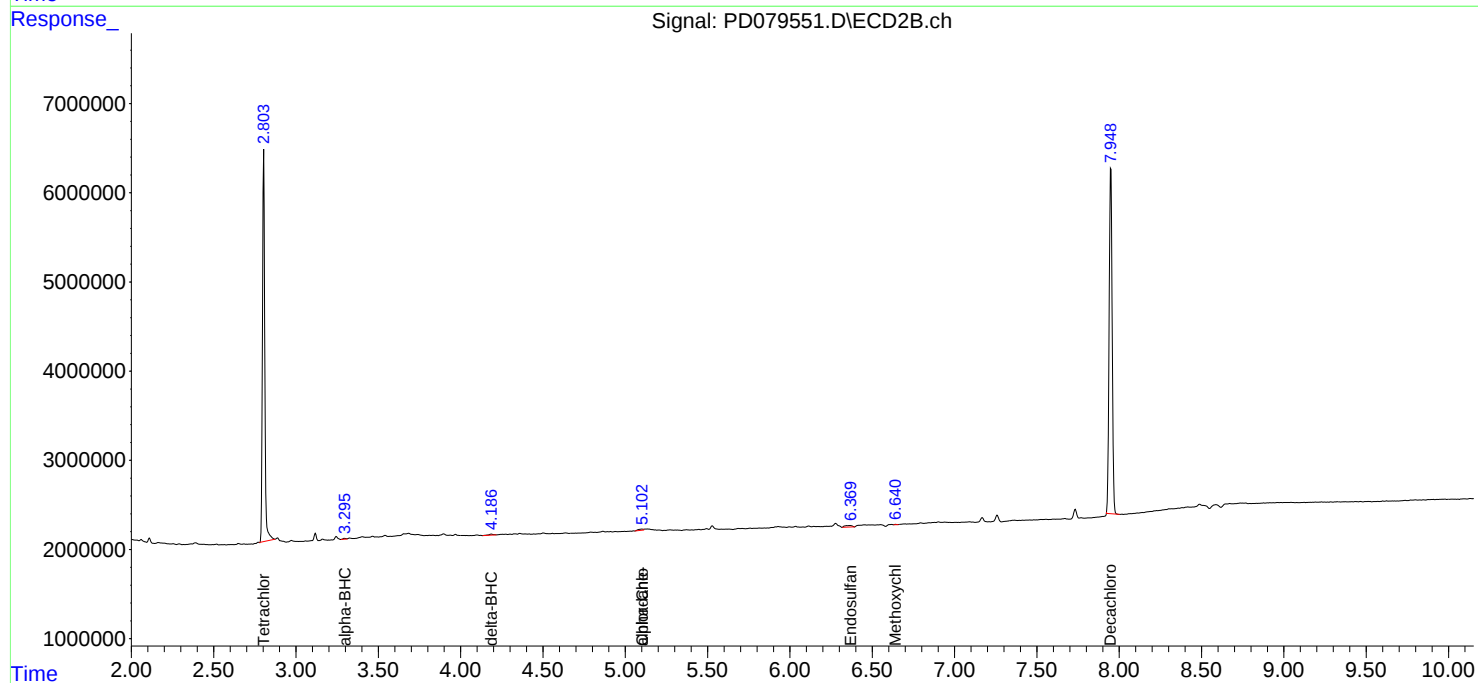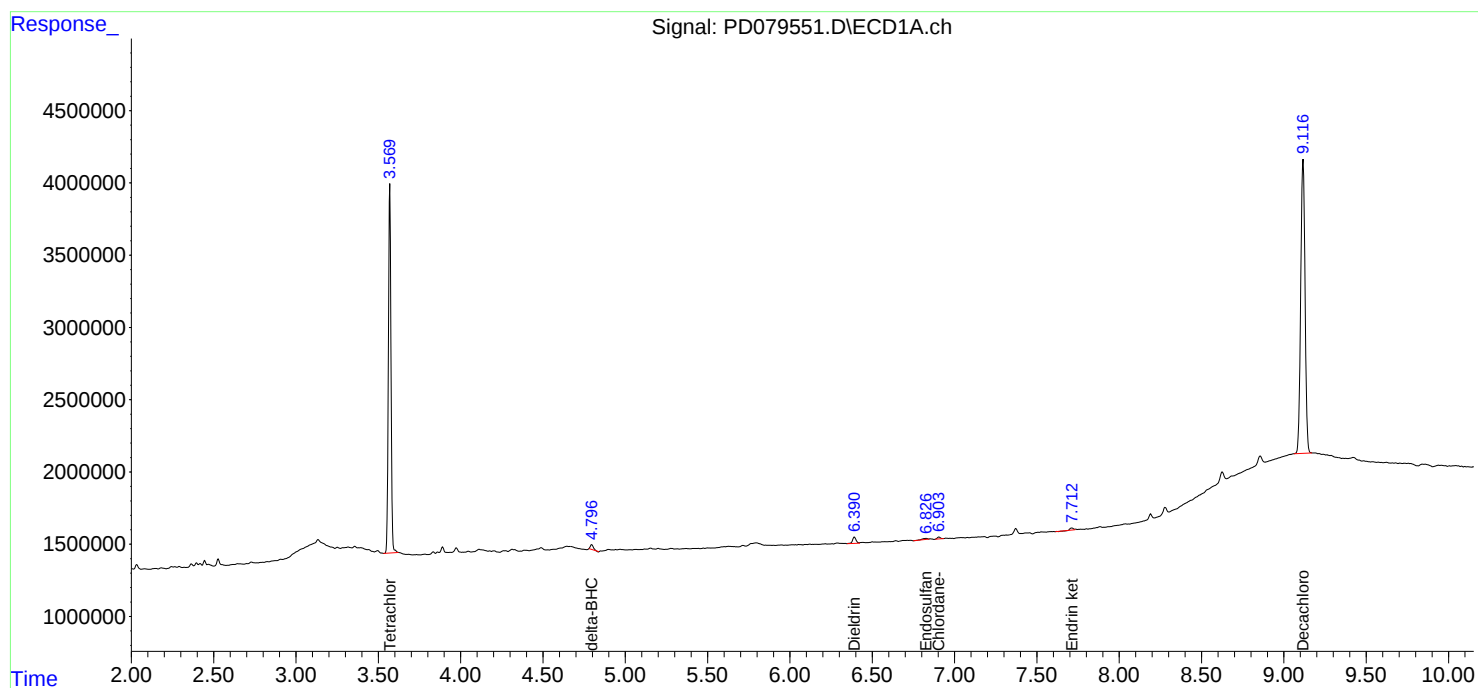

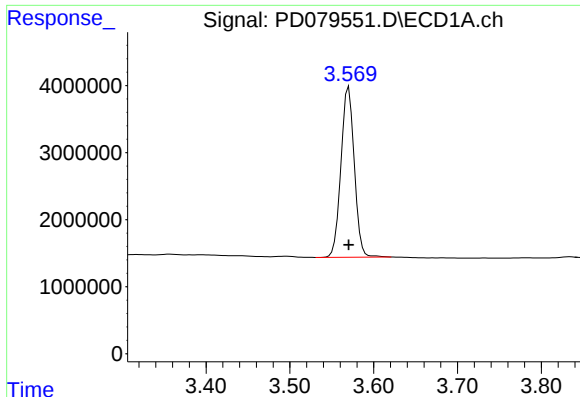


#1 Tetrachloro-m-xylene

R.T.: 3.570 min
Delta R.T.: 0.000 min
Response: 28084986
Conc: 17.39 ng/ml

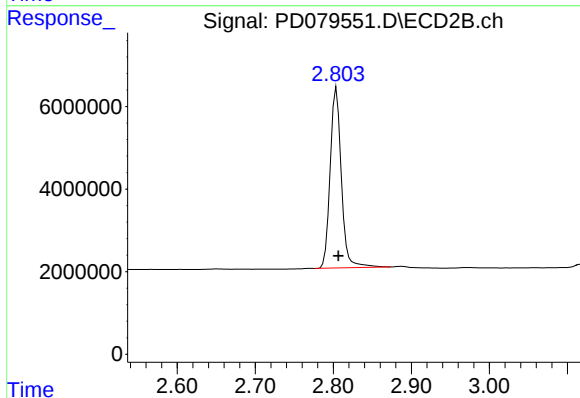


#1 Tetrachloro-m-xylene

R.T.: 2.804 min
Delta R.T.: -0.002 min
Response: 43446710
Conc: 18.77 ng/ml

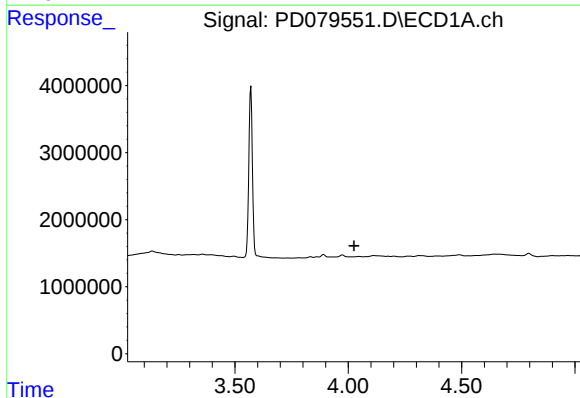


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 4.026 min
Response: 0
Conc: N.D.

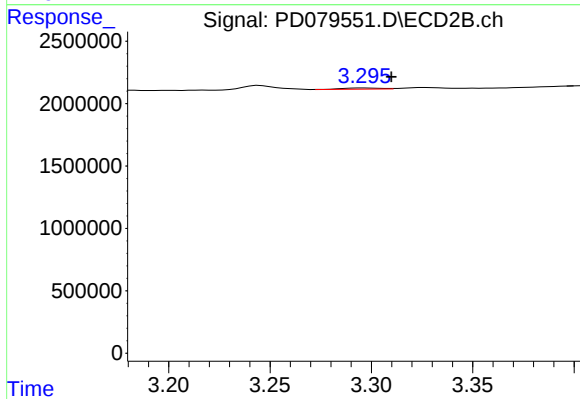


#2 alpha-BHC

R.T.: 3.296 min
Delta R.T.: -0.014 min
Response: 112701
Conc: 0.03 ng/ml

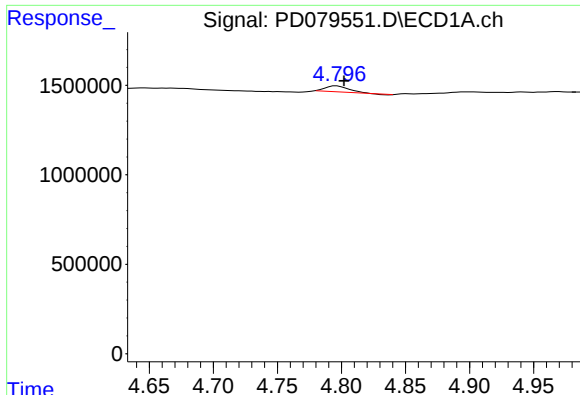


#7 delta-BHC

R.T.: 4.796 min
Delta R.T.: -0.006 min
Response: 377340
Conc: 0.14 ng/ml

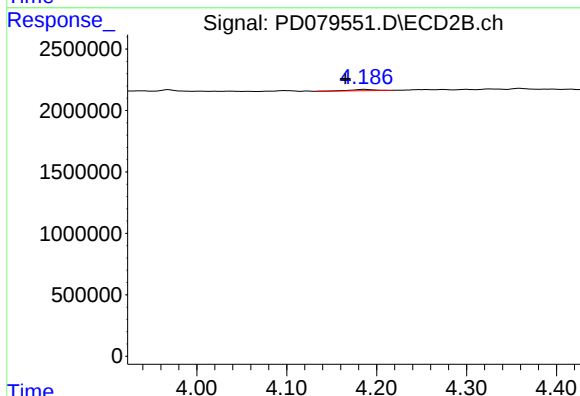


#7 delta-BHC

R.T.: 4.187 min
Delta R.T.: 0.021 min
Response: 206905
Conc: 0.06 ng/ml

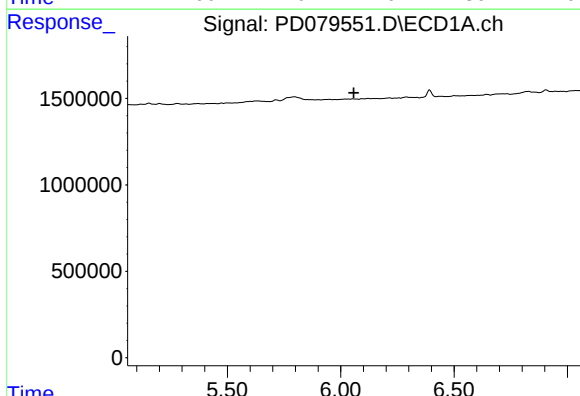


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.058 min
Response: 0
Conc: N.D.

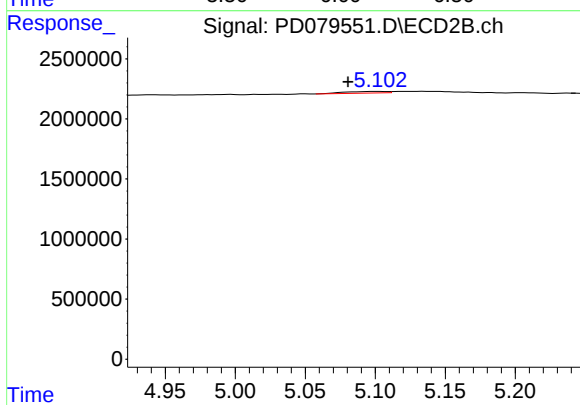


#11 alpha-Chlordane

R.T.: 5.102 min
Delta R.T.: 0.022 min
Response: 312244
Conc: 0.11 ng/ml

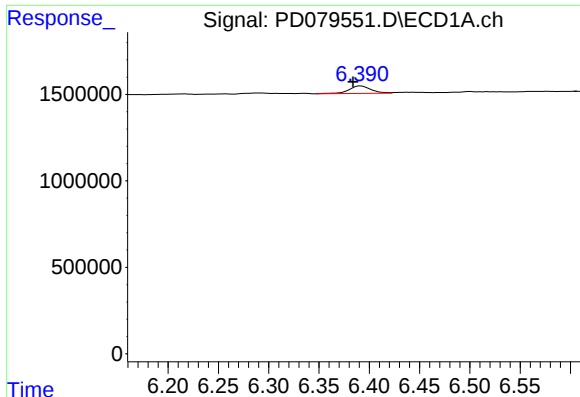


#13 Dieldrin

R.T.: 6.392 min
Delta R.T.: 0.008 min
Response: 675239
Conc: 0.29 ng/ml

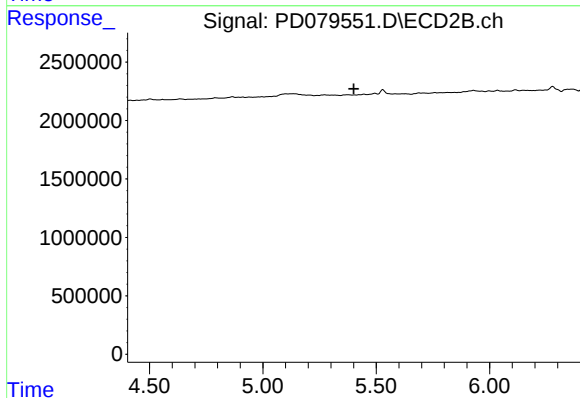


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 5.401 min
Response: 0
Conc: N.D.

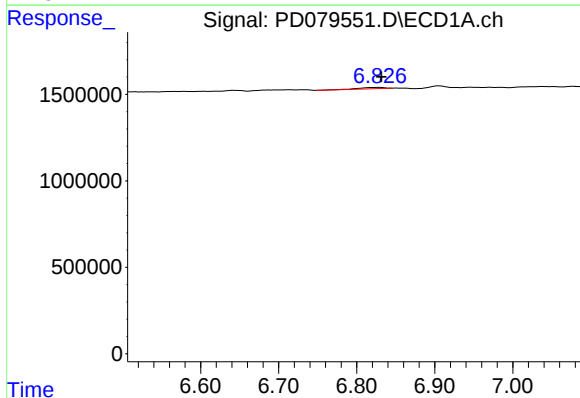


#15 Endosulfan II

R.T.: 6.828 min
Delta R.T.: -0.004 min
Response: 166070
Conc: 0.08 ng/ml

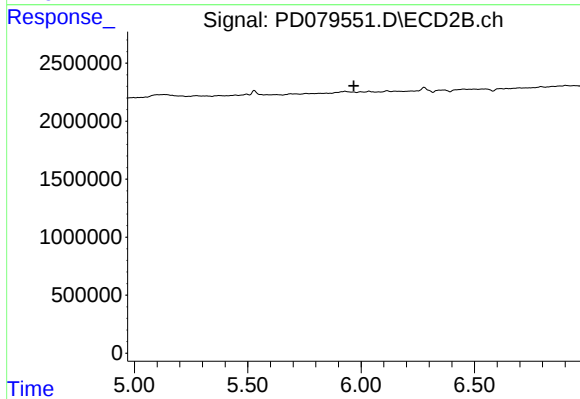


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.968 min
Response: 0
Conc: N.D.

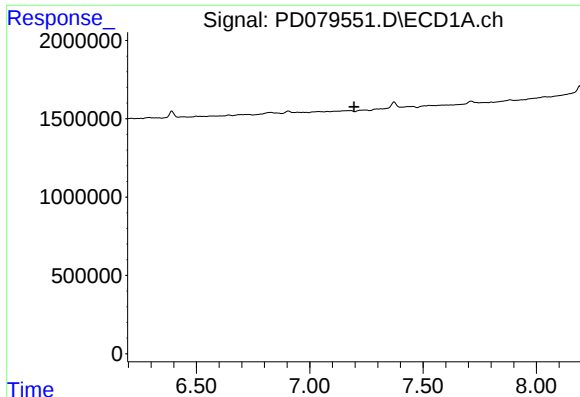


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.196 min
Response: 0
Conc: N.D.

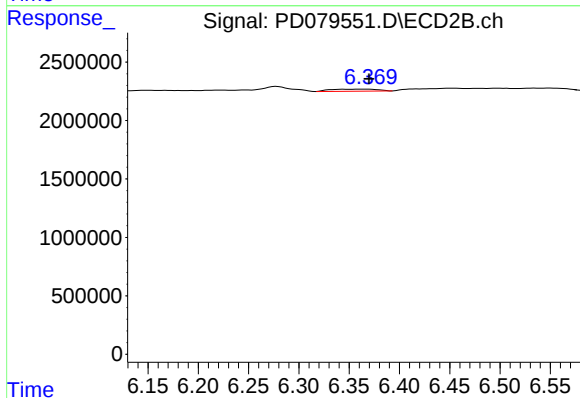


#19 Endosulfan Sulfate

R.T.: 6.369 min
Delta R.T.: 0.000 min
Response: 574055
Conc: 0.25 ng/ml

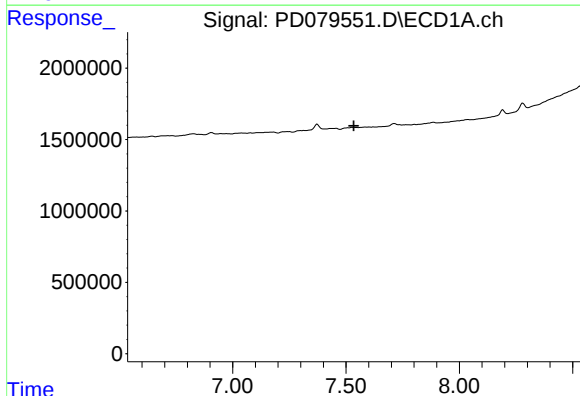


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.534 min
Response: 0
Conc: N.D.

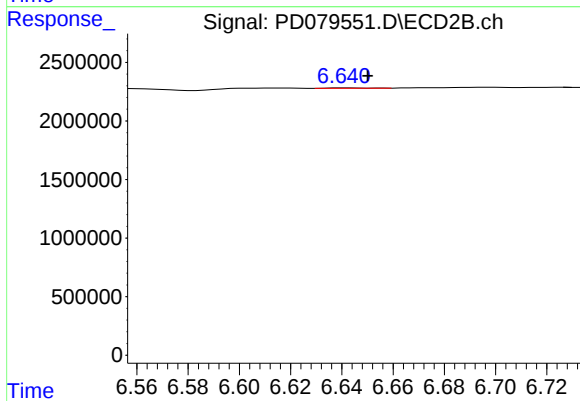


#20 Methoxychlor

R.T.: 6.641 min
Delta R.T.: -0.009 min
Response: 30518
Conc: 0.02 ng/ml

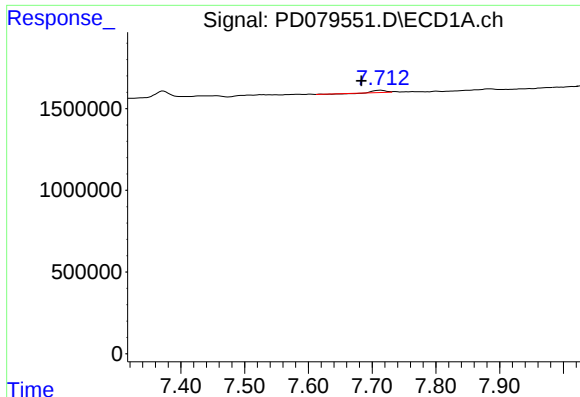


#21 Endrin ketone

R.T.: 7.714 min
Delta R.T.: 0.030 min
Response: 157041
Conc: 0.07 ng/ml

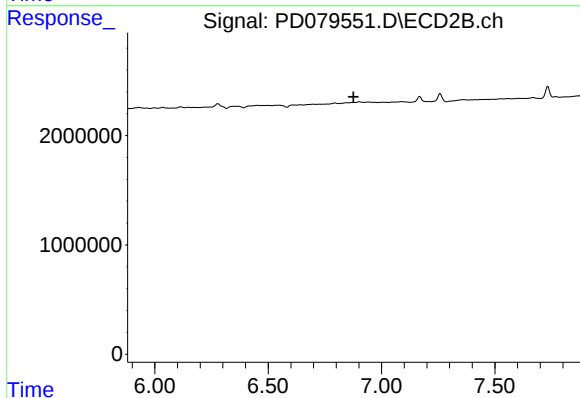


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.876 min
Response: 0
Conc: N.D.

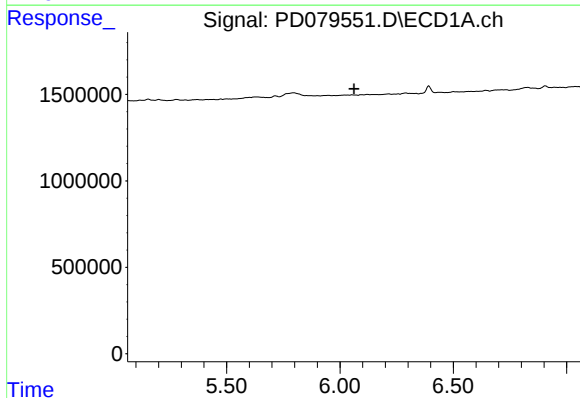


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.062 min
Response: 0
Conc: N.D.

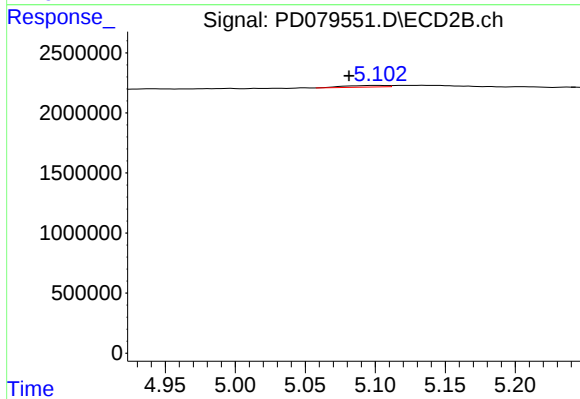


#26 Chlordane-4

R.T.: 5.102 min
Delta R.T.: 0.021 min
Response: 312244
Conc: 1.27 ng/ml

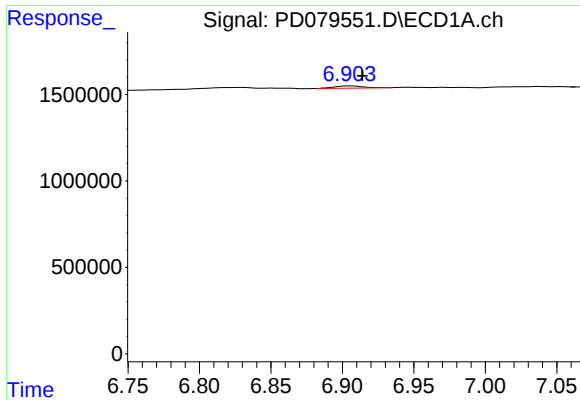


#27 Chlordane-5

R.T.: 6.905 min
Delta R.T.: -0.009 min
Response: 176626
Conc: 2.51 ng/ml

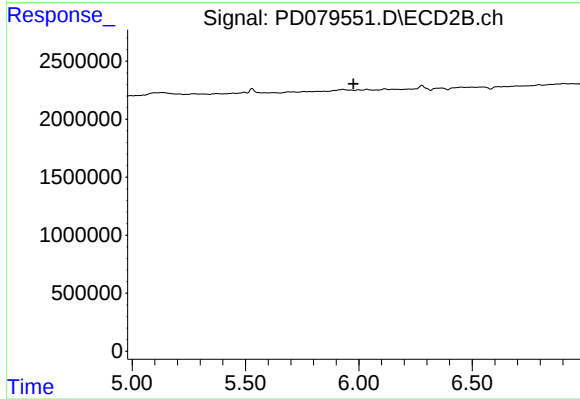


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 5.977 min
Response: 0
Conc: N.D.

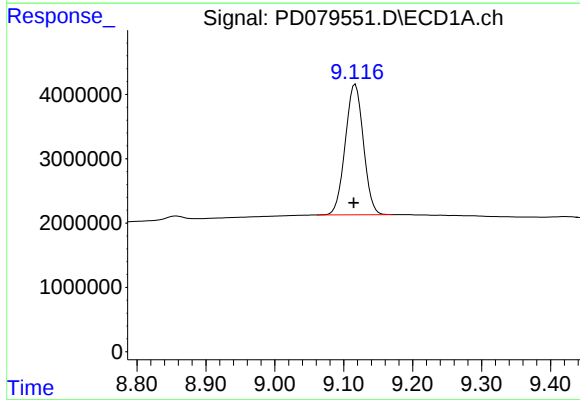

#28 Decachlorobiphenyl

R.T.: 9.117 min
Delta R.T.: 0.002 min
Response: 37093259
Conc: 18.49 ng/ml

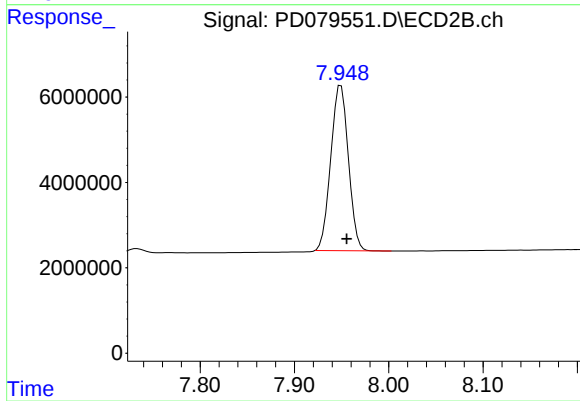

#28 Decachlorobiphenyl

R.T.: 7.949 min
Delta R.T.: -0.006 min
Response: 50312983
Conc: 20.64 ng/ml