

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110923\
 Data File : PL086547.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2023 17:16
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 21:55:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110923CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 08 21:53:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.352	2.618	57628870	17359507	20.000	20.000
27)	SA Decachlor...	8.853	7.768	105.7E6	44435118	40.000	39.958
Target Compounds							
2)	A alpha-BHC	3.805	3.116	85267088	23698965	20.000	20.000
3)	MA gamma-BHC...	4.137	3.443	82102417	23426170	20.000	20.000
4)	MA Heptachlor	4.724	3.779	85849766	24240826	20.000	20.000
9)	A Endosulfan I	5.877	4.927	73139892	21028621	20.000	20.000
13)	MA Dieldrin	6.155	5.193	145.6E6	44674851	40.000	40.000
14)	MA Endrin	6.383	5.466	122.8E6	41486790	40.000	40.000
16)	A 4,4'-DDD	6.533	5.631	95534256	31054507	40.000	40.000
17)	MA 4,4'-DDT	6.849	5.881	102.3E6	35967461	40.000	40.000
20)	A Methoxychlor	7.334	6.466	277.0E6	108.5E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110923\
Data File : PL086547.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2023 17:16
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 21:55:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110923CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 08 21:53:51 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

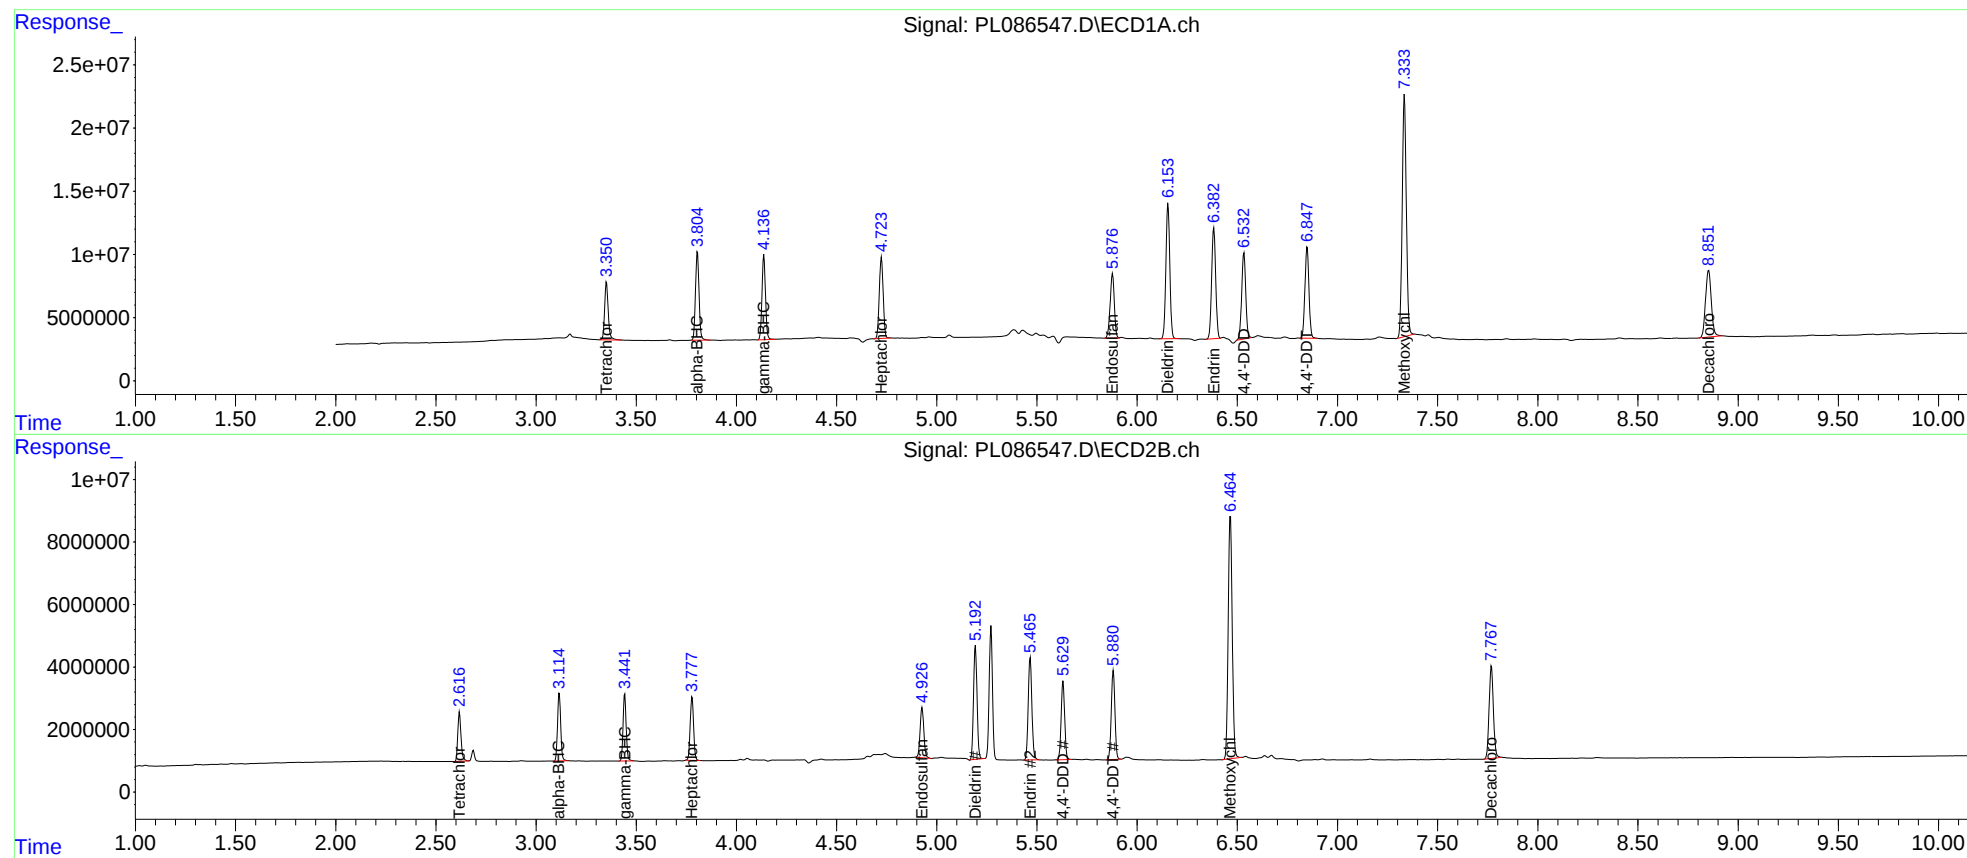

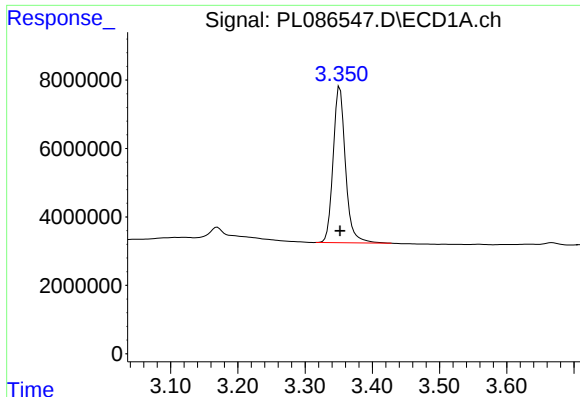


#1 Tetrachloro-m-xylene

R.T.: 3.352 min
Delta R.T.: 0.000 min
Response: 57628870
Conc: 20.00 ng/ml

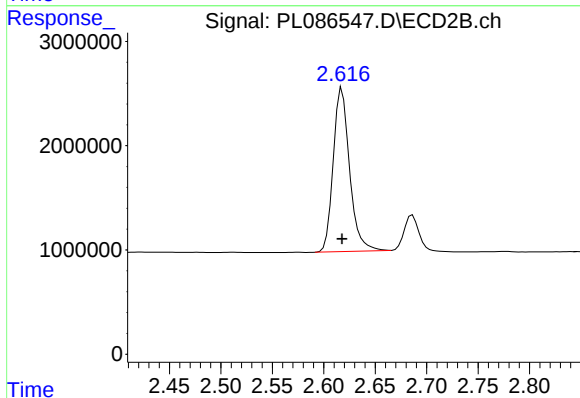


#1 Tetrachloro-m-xylene

R.T.: 2.618 min
Delta R.T.: 0.000 min
Response: 17359507
Conc: 20.00 ng/ml

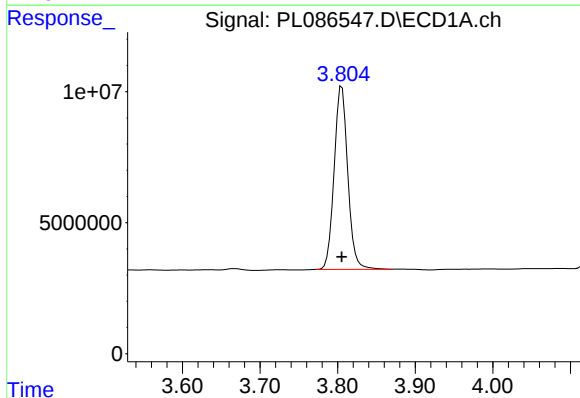


#2 alpha-BHC

R.T.: 3.805 min
Delta R.T.: 0.000 min
Response: 85267088
Conc: 20.00 ng/ml

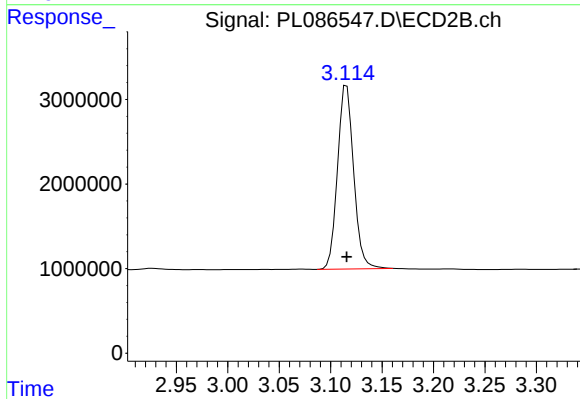


#2 alpha-BHC

R.T.: 3.116 min
Delta R.T.: 0.000 min
Response: 23698965
Conc: 20.00 ng/ml

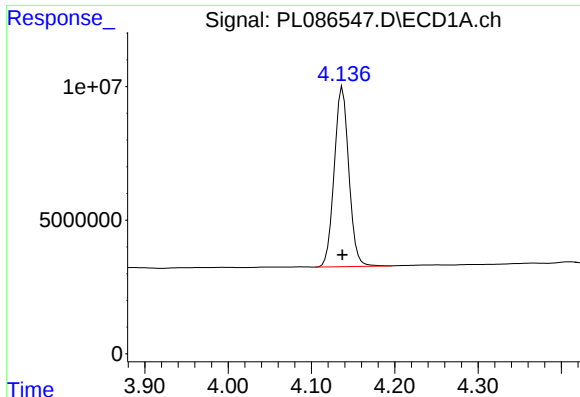


#3 gamma-BHC (Lindane)

R.T.: 4.137 min
Delta R.T.: 0.000 min
Response: 82102417
Conc: 20.00 ng/ml

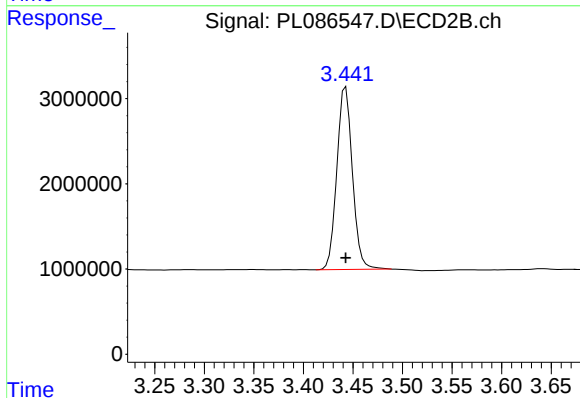


#3 gamma-BHC (Lindane)

R.T.: 3.443 min
Delta R.T.: 0.000 min
Response: 23426170
Conc: 20.00 ng/ml

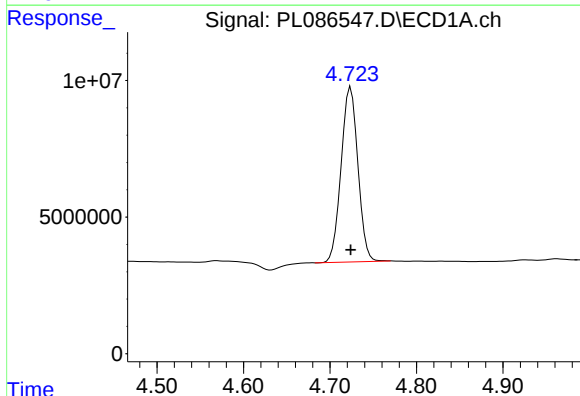


#4 Heptachlor

R.T.: 4.724 min
Delta R.T.: 0.000 min
Response: 85849766
Conc: 20.00 ng/ml

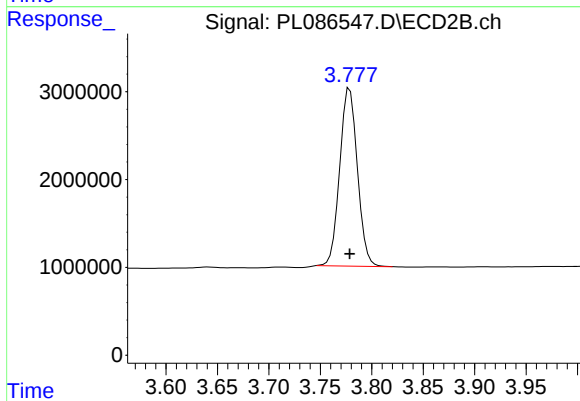


#4 Heptachlor

R.T.: 3.779 min
Delta R.T.: 0.000 min
Response: 24240826
Conc: 20.00 ng/ml

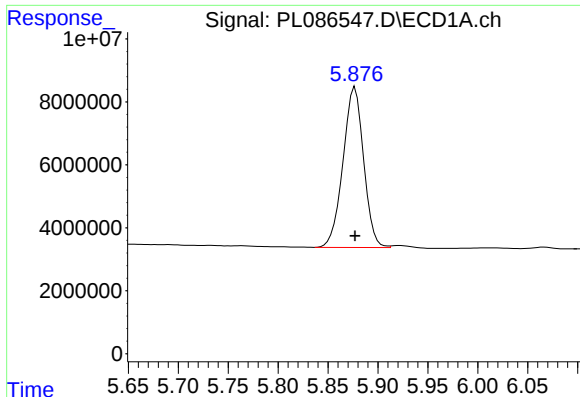


#9 Endosulfan I

R.T.: 5.877 min
Delta R.T.: 0.000 min
Response: 73139892
Conc: 20.00 ng/ml

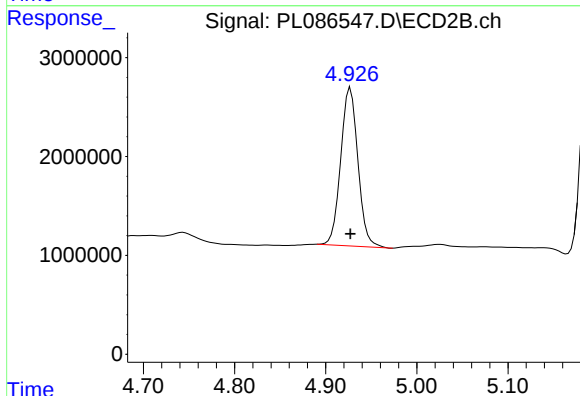


#9 Endosulfan I

R.T.: 4.927 min
Delta R.T.: 0.000 min
Response: 21028621
Conc: 20.00 ng/ml

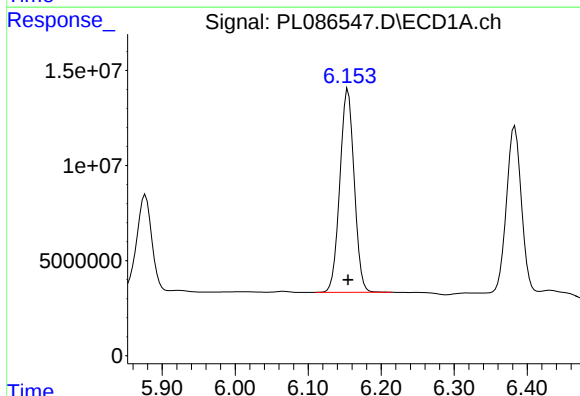


#13 Dieldrin

R.T.: 6.155 min
Delta R.T.: 0.000 min
Response: 145608885
Conc: 40.00 ng/ml

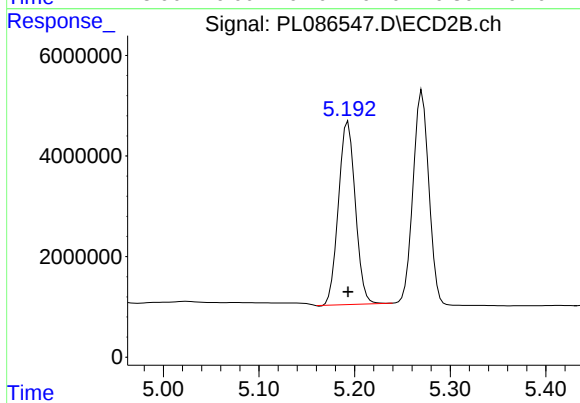


#13 Dieldrin

R.T.: 5.193 min
Delta R.T.: 0.000 min
Response: 44674851
Conc: 40.00 ng/ml

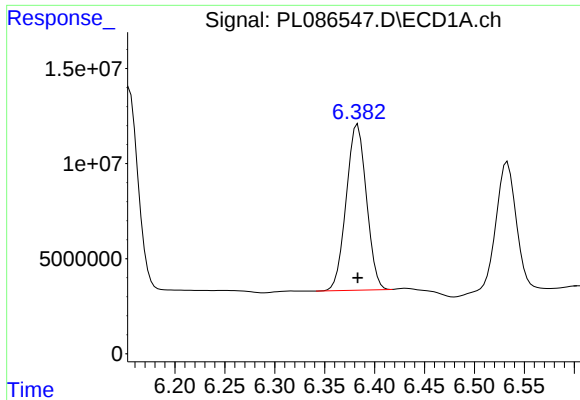


#14 Endrin

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 122785057
Conc: 40.00 ng/ml

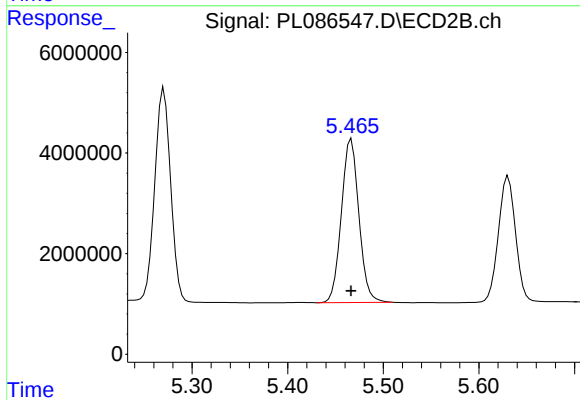


#14 Endrin

R.T.: 5.466 min
Delta R.T.: 0.000 min
Response: 41486790
Conc: 40.00 ng/ml

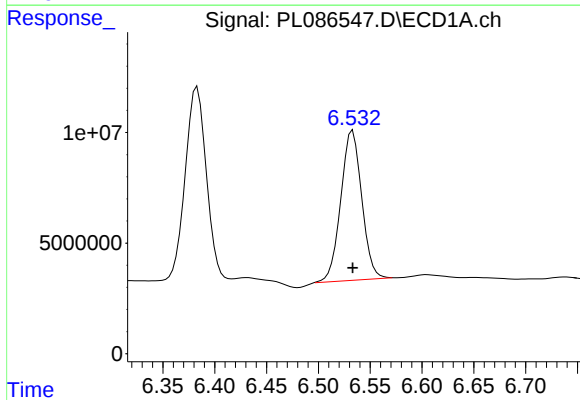


#16 4,4'-DDD

R.T.: 6.533 min
Delta R.T.: 0.000 min
Response: 95534256
Conc: 40.00 ng/ml

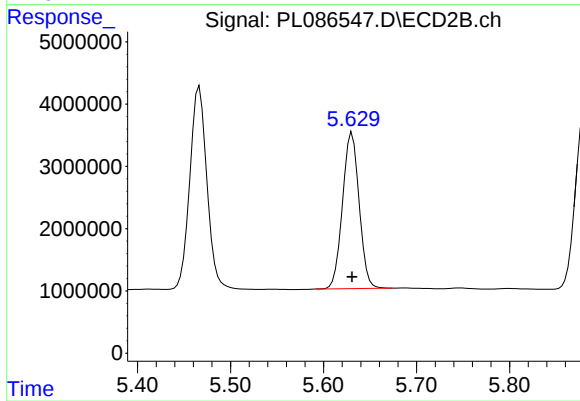


#16 4,4'-DDD

R.T.: 5.631 min
Delta R.T.: 0.000 min
Response: 31054507
Conc: 40.00 ng/ml

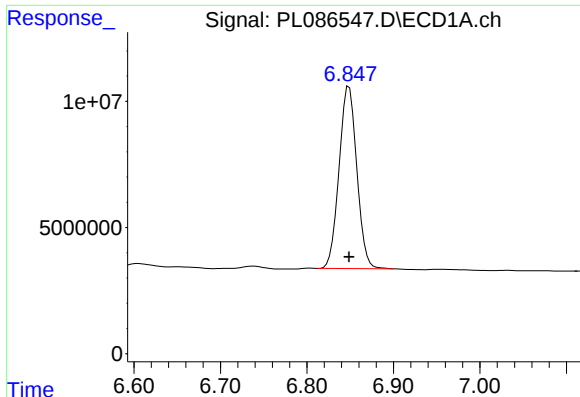


#17 4,4'-DDT

R.T.: 6.849 min
Delta R.T.: 0.000 min
Response: 102330748
Conc: 40.00 ng/ml

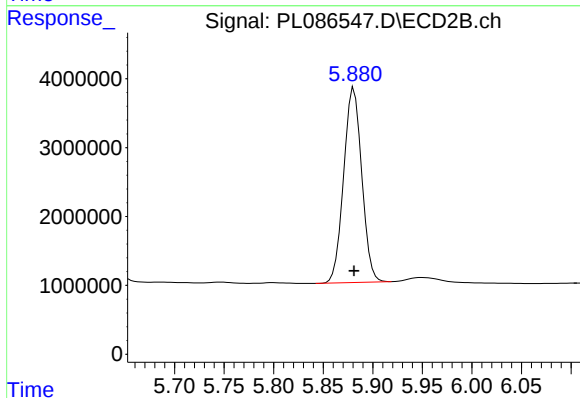


#17 4,4'-DDT

R.T.: 5.881 min
Delta R.T.: 0.000 min
Response: 35967461
Conc: 40.00 ng/ml

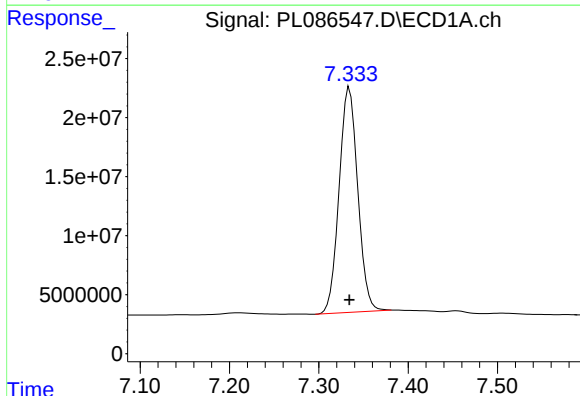


#20 Methoxychlor

R.T.: 7.334 min
Delta R.T.: 0.000 min
Response: 277043338
Conc: 200.00 ng/ml

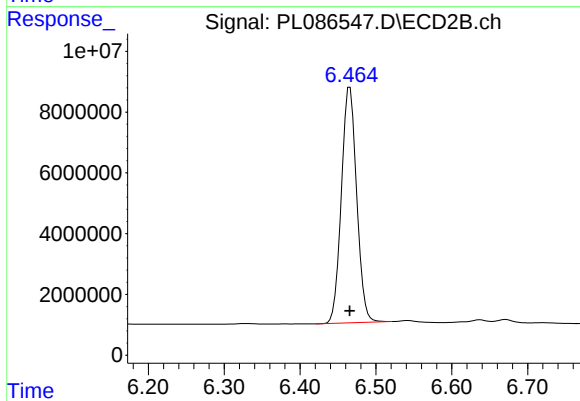


#20 Methoxychlor

R.T.: 6.466 min
Delta R.T.: 0.000 min
Response: 108542482
Conc: 200.00 ng/ml

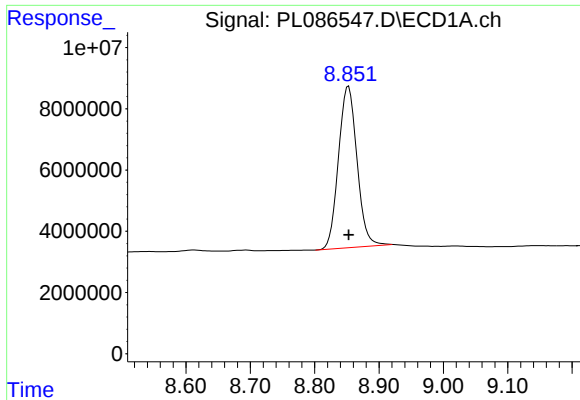

#27 Decachlorobiphenyl

R.T.: 8.853 min
Delta R.T.: 0.000 min
Response: 105685463
Conc: 40.00 ng/ml

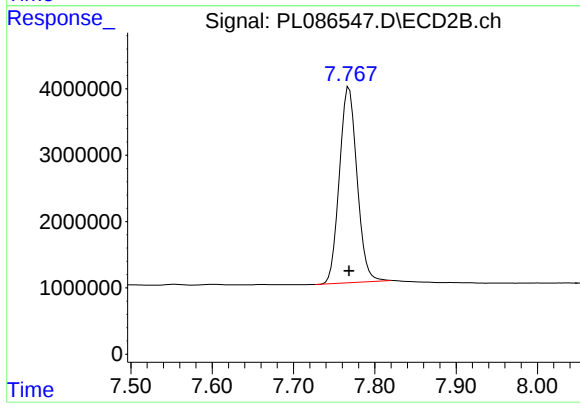

#27 Decachlorobiphenyl

R.T.: 7.768 min
Delta R.T.: 0.000 min
Response: 44435118
Conc: 39.96 ng/ml