

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110923\
 Data File : PL086549.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2023 17:43
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 21:55:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110923CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 08 21:53:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.352	2.618	120.3E6	35923840	41.748	41.388
27)	SA Decachlor...	8.853	7.767	202.6E6	83659481	76.688	75.229
Target Compounds							
2)	A alpha-BHC	3.806	3.116	188.3E6	52525699	44.176	44.327
3)	MA gamma-BHC...	4.138	3.443	178.0E6	50450424	43.356	43.072
4)	MA Heptachlor	4.724	3.779	182.4E6	51495420	42.483	42.487
9)	A Endosulfan I	5.878	4.928	133.6E6	42050830	36.543	39.994
13)	MA Dieldrin	6.155	5.193	305.7E6	97575553	83.983	87.365
14)	MA Endrin	6.383	5.467	249.8E6	86114388	81.365	83.028
16)	A 4,4'-DDD	6.534	5.631	192.5E6	65795716	80.617	84.749
17)	MA 4,4'-DDT	6.849	5.881	211.2E6	75479133	82.544	83.942
20)	A Methoxychlor	7.335	6.466	536.8E6	211.7E6	387.520	390.132


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110923\
Data File : PL086549.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2023 17:43
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 21:55:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110923CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 08 21:53:51 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

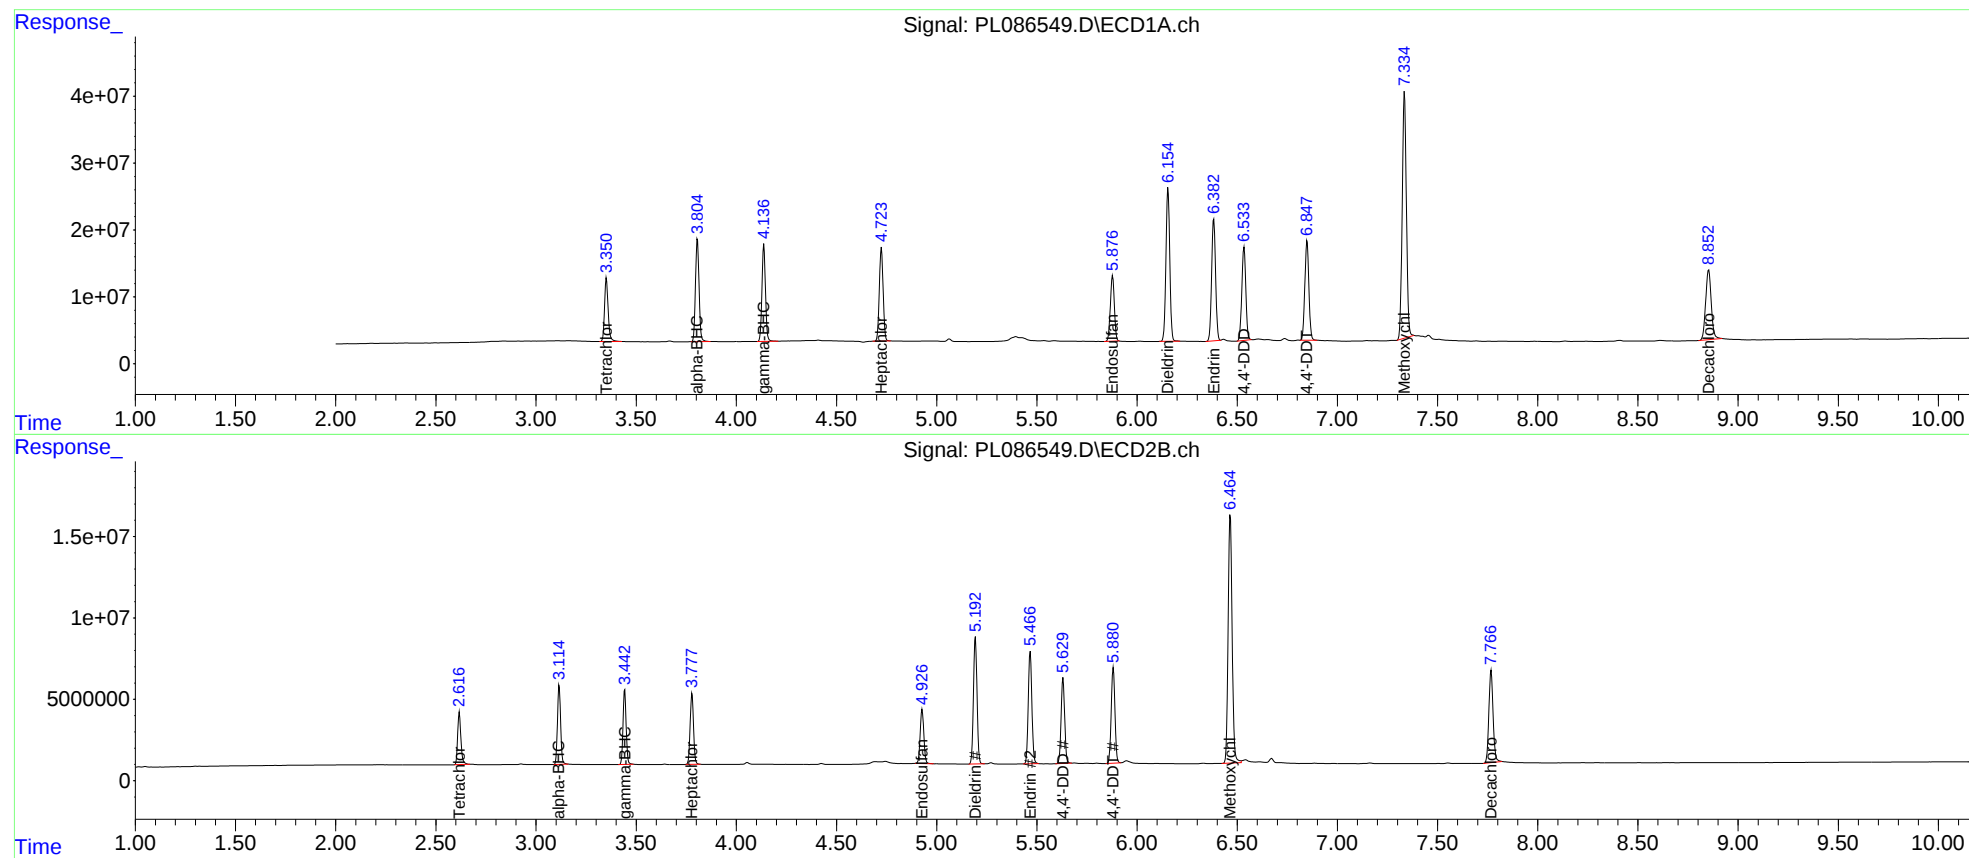

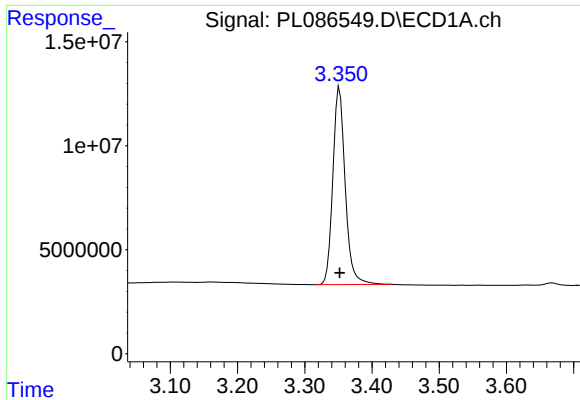


#1 Tetrachloro-m-xylene

R.T.: 3.352 min
Delta R.T.: 0.000 min
Response: 120293310
Conc: 41.75 ng/ml

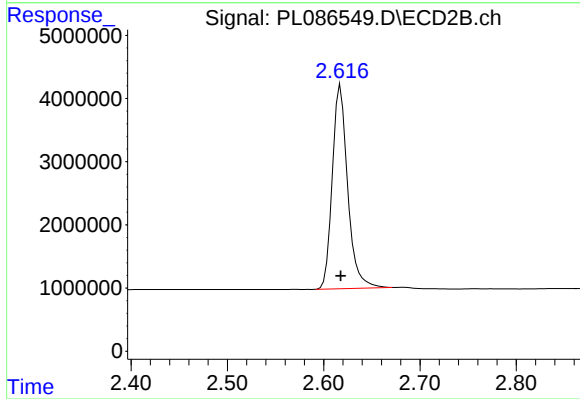


#1 Tetrachloro-m-xylene

R.T.: 2.618 min
Delta R.T.: 0.000 min
Response: 35923840
Conc: 41.39 ng/ml

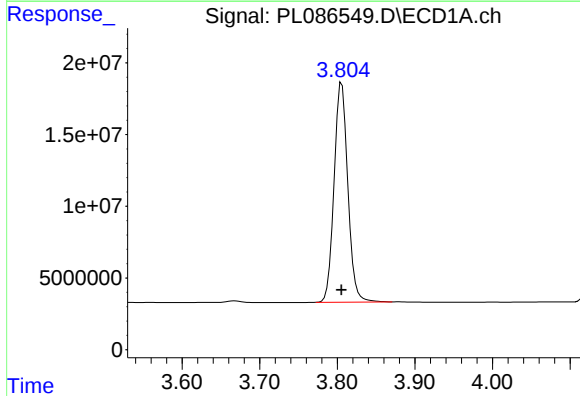


#2 alpha-BHC

R.T.: 3.806 min
Delta R.T.: 0.000 min
Response: 188338543
Conc: 44.18 ng/ml

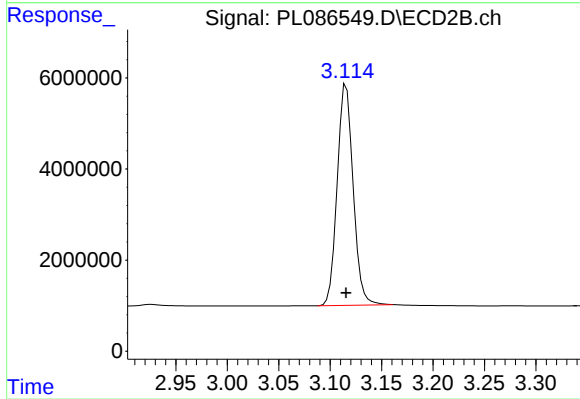


#2 alpha-BHC

R.T.: 3.116 min
Delta R.T.: 0.000 min
Response: 52525699
Conc: 44.33 ng/ml

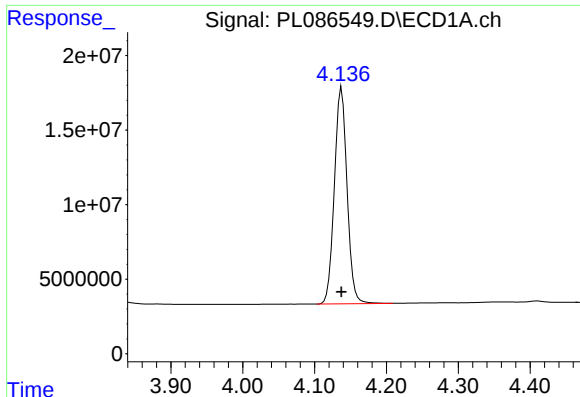


#3 gamma-BHC (Lindane)

R.T.: 4.138 min
Delta R.T.: 0.000 min
Response: 177982762
Conc: 43.36 ng/ml

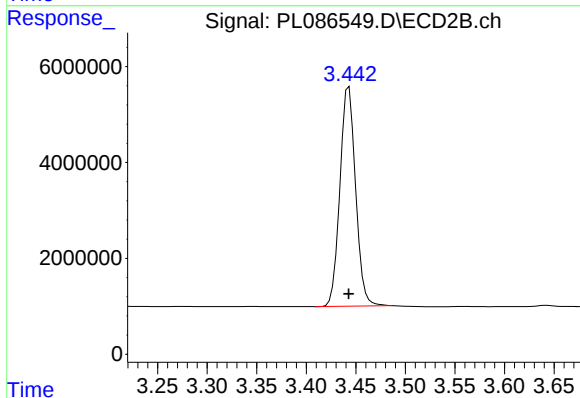


#3 gamma-BHC (Lindane)

R.T.: 3.443 min
Delta R.T.: 0.000 min
Response: 50450424
Conc: 43.07 ng/ml

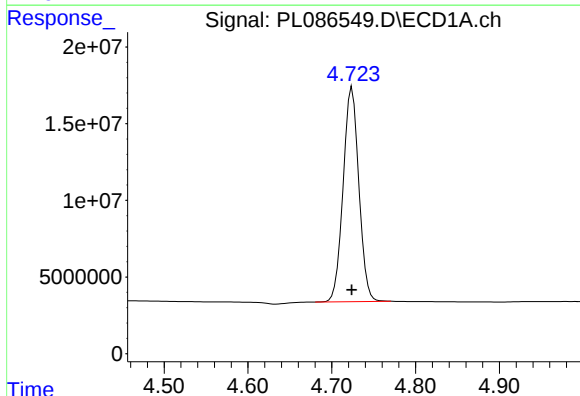


#4 Heptachlor

R.T.: 4.724 min
Delta R.T.: 0.000 min
Response: 182357358
Conc: 42.48 ng/ml

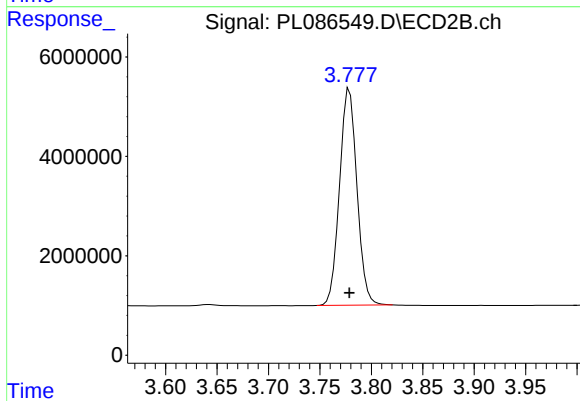


#4 Heptachlor

R.T.: 3.779 min
Delta R.T.: 0.000 min
Response: 51495420
Conc: 42.49 ng/ml

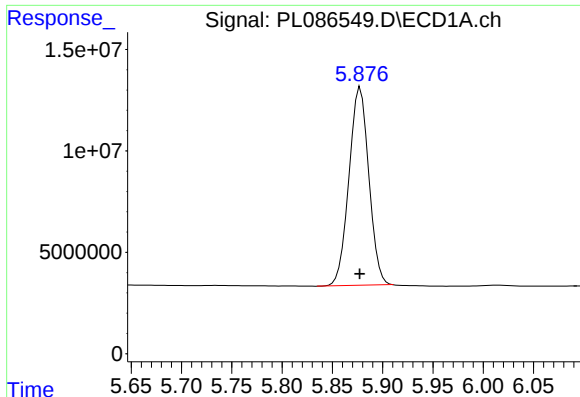


#9 Endosulfan I

R.T.: 5.878 min
Delta R.T.: 0.000 min
Response: 133637110
Conc: 36.54 ng/ml

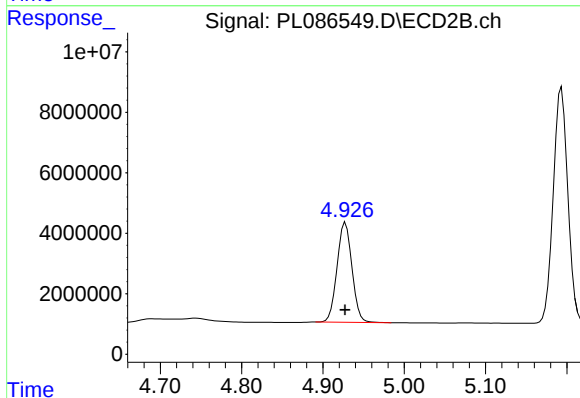


#9 Endosulfan I

R.T.: 4.928 min
Delta R.T.: 0.000 min
Response: 42050830
Conc: 39.99 ng/ml

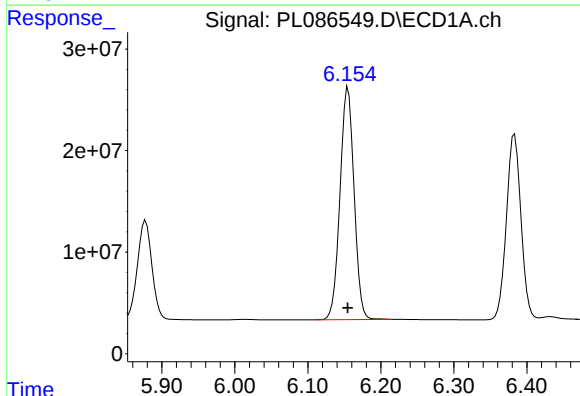


#13 Dieldrin

R.T.: 6.155 min
Delta R.T.: 0.000 min
Response: 305716095
Conc: 83.98 ng/ml

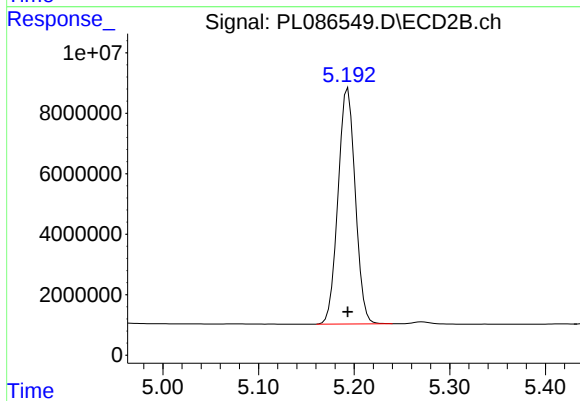


#13 Dieldrin

R.T.: 5.193 min
Delta R.T.: 0.000 min
Response: 97575553
Conc: 87.37 ng/ml

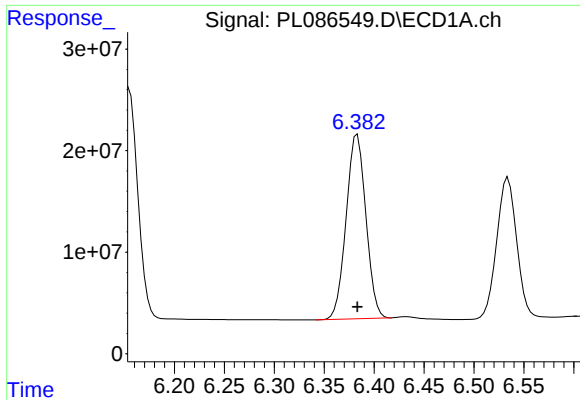


#14 Endrin

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 249761450
Conc: 81.37 ng/ml

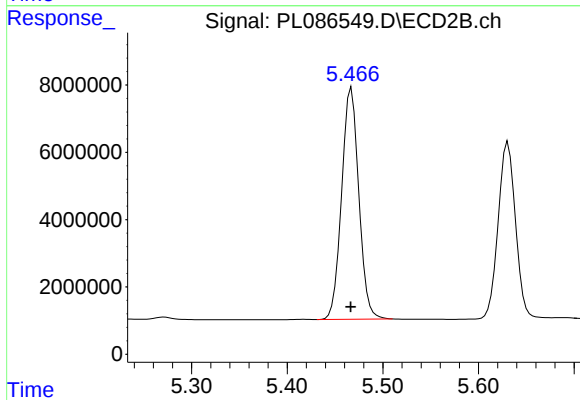


#14 Endrin

R.T.: 5.467 min
Delta R.T.: 0.000 min
Response: 86114388
Conc: 83.03 ng/ml

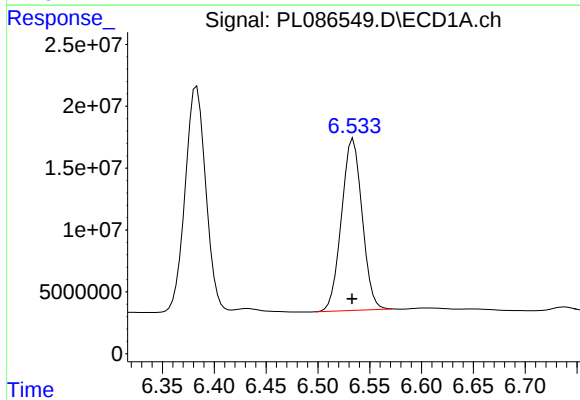


#16 4,4'-DDD

R.T.: 6.534 min
Delta R.T.: 0.001 min
Response: 192541723
Conc: 80.62 ng/ml

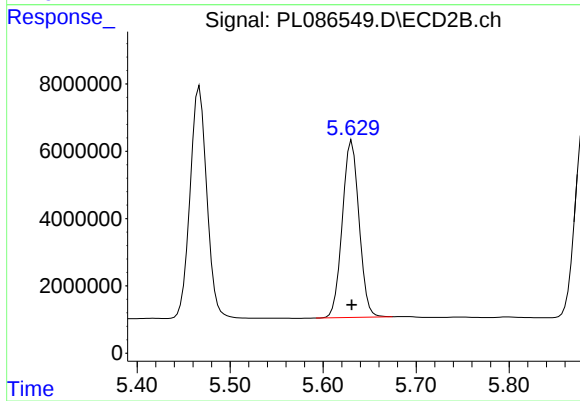


#16 4,4'-DDD

R.T.: 5.631 min
Delta R.T.: 0.000 min
Response: 65795716
Conc: 84.75 ng/ml

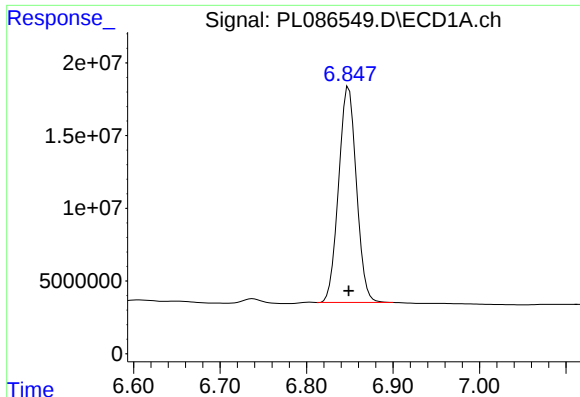


#17 4,4'-DDT

R.T.: 6.849 min
Delta R.T.: 0.000 min
Response: 211170574
Conc: 82.54 ng/ml

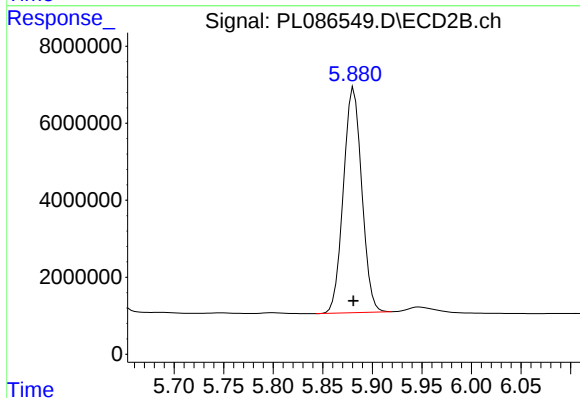


#17 4,4'-DDT

R.T.: 5.881 min
Delta R.T.: 0.000 min
Response: 75479133
Conc: 83.94 ng/ml

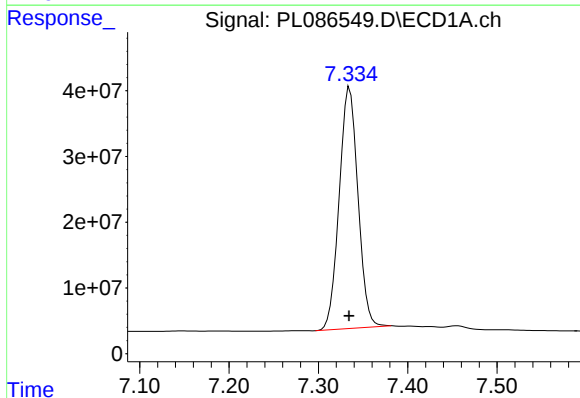


#20 Methoxychlor

R.T.: 7.335 min
Delta R.T.: 0.000 min
Response: 536799691
Conc: 387.52 ng/ml

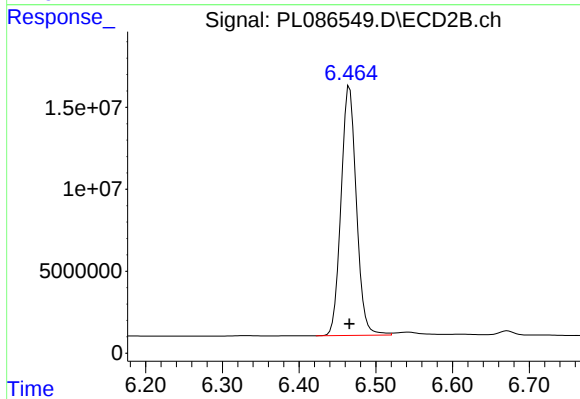


#20 Methoxychlor

R.T.: 6.466 min
Delta R.T.: 0.000 min
Response: 211729632
Conc: 390.13 ng/ml

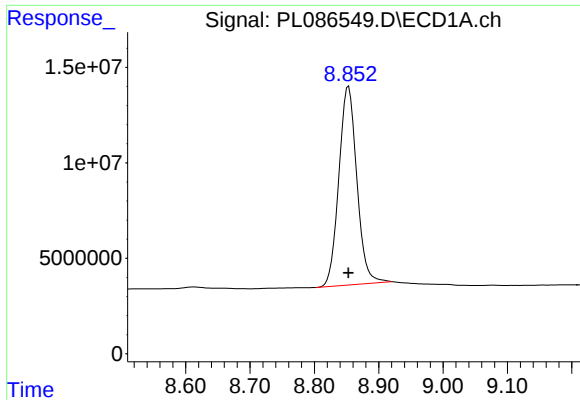

#27 Decachlorobiphenyl

R.T.: 8.853 min
Delta R.T.: 0.000 min
Response: 202620463
Conc: 76.69 ng/ml

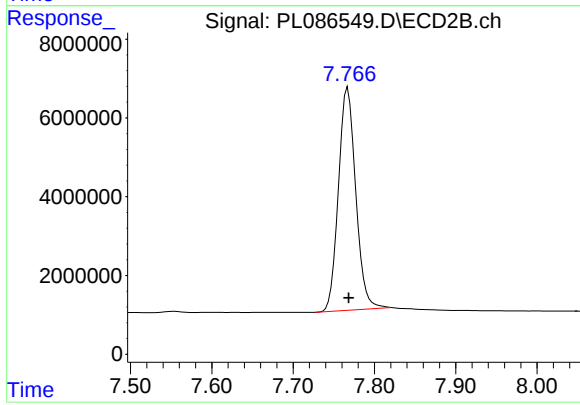

#27 Decachlorobiphenyl

R.T.: 7.767 min
Delta R.T.: -0.001 min
Response: 83659481
Conc: 75.23 ng/ml