

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110923\
 Data File : PL086551.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2023 18:11
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 21:55:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110923CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 08 21:53:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.352	2.618	242.5E6	74388171	84.143	85.703
27)	SA Decachlor...	8.853	7.768	407.7E6	168.9E6	154.323	151.869
Target Compounds							
2)	A alpha-BHC	3.806	3.116	399.9E6	118.2E6	93.811	99.762
3)	MA gamma-BHC...	4.138	3.443	373.9E6	110.8E6	91.071	94.599
4)	MA Heptachlor	4.725	3.779	371.7E6	109.5E6	86.591	90.355
9)	A Endosulfan I	5.878	4.927	293.6E6	89732387	80.276	85.343
13)	MA Dieldrin	6.155	5.193	644.4E6	201.1E6	177.027	180.038
14)	MA Endrin	6.383	5.467	533.5E6	188.4E6	173.816	181.601
16)	A 4,4'-DDD	6.534	5.631	427.1E6	147.6E6	178.816	190.067
17)	MA 4,4'-DDT	6.849	5.882	461.5E6	168.6E6	180.398	187.526
20)	A Methoxychlor	7.335	6.466	1130.9E6	438.7E6	816.380	808.327


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110923\
Data File : PL086551.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2023 18:11
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 21:55:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110923CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 08 21:53:51 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

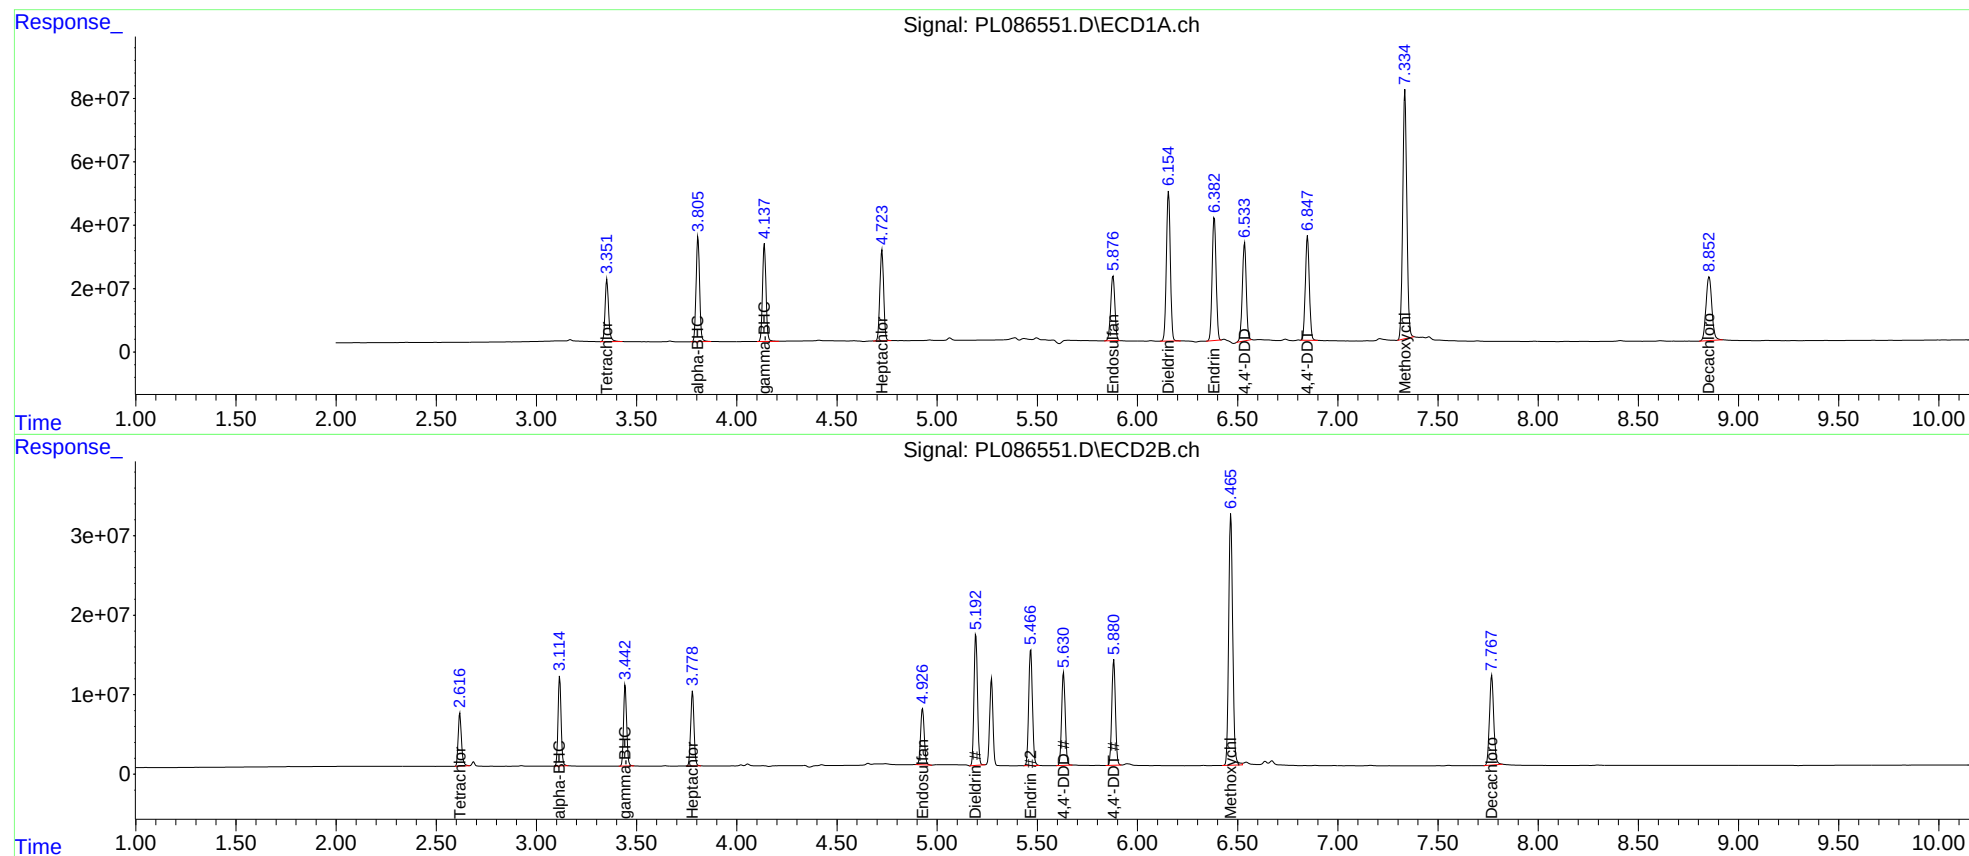

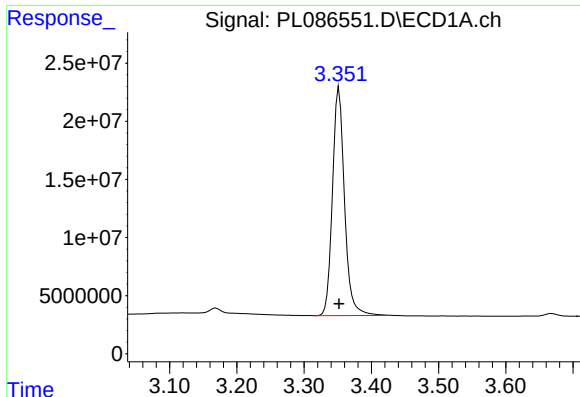


#1 Tetrachloro-m-xylene

R.T.: 3.352 min
Delta R.T.: 0.000 min
Response: 242453959
Conc: 84.14 ng/ml

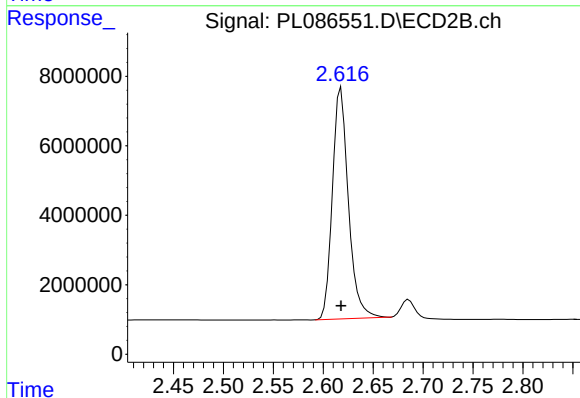


#1 Tetrachloro-m-xylene

R.T.: 2.618 min
Delta R.T.: 0.000 min
Response: 74388171
Conc: 85.70 ng/ml

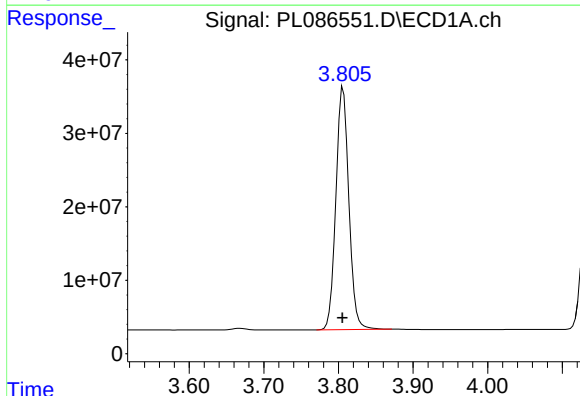


#2 alpha-BHC

R.T.: 3.806 min
Delta R.T.: 0.001 min
Response: 399947544
Conc: 93.81 ng/ml

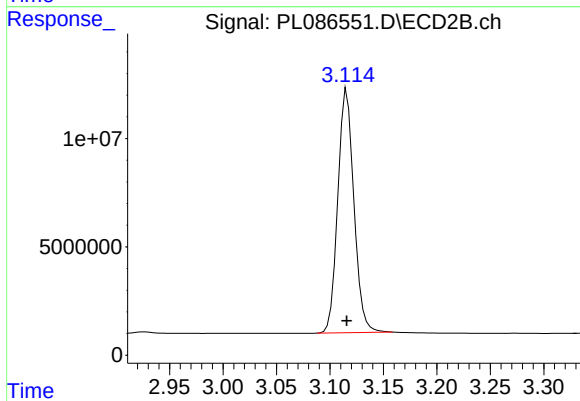


#2 alpha-BHC

R.T.: 3.116 min
Delta R.T.: 0.000 min
Response: 118213157
Conc: 99.76 ng/ml

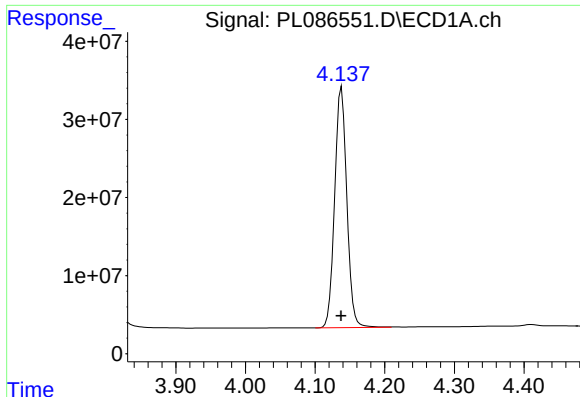


#3 gamma-BHC (Lindane)

R.T.: 4.138 min
Delta R.T.: 0.000 min
Response: 373857247
Conc: 91.07 ng/ml

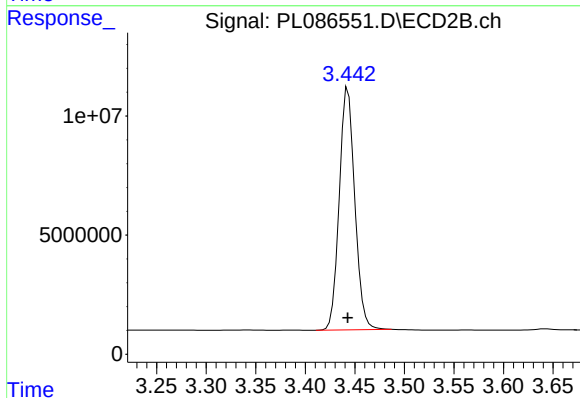


#3 gamma-BHC (Lindane)

R.T.: 3.443 min
Delta R.T.: 0.000 min
Response: 110804394
Conc: 94.60 ng/ml

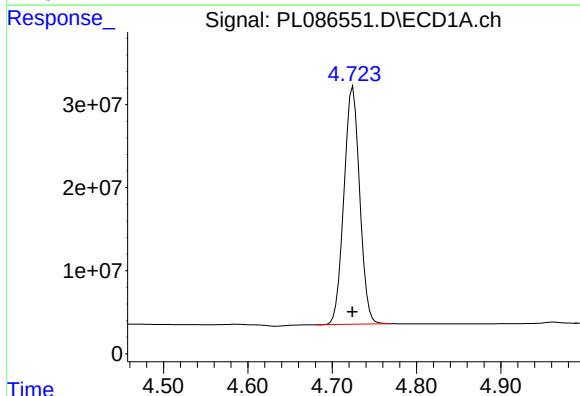


#4 Heptachlor

R.T.: 4.725 min
Delta R.T.: 0.000 min
Response: 371690672
Conc: 86.59 ng/ml

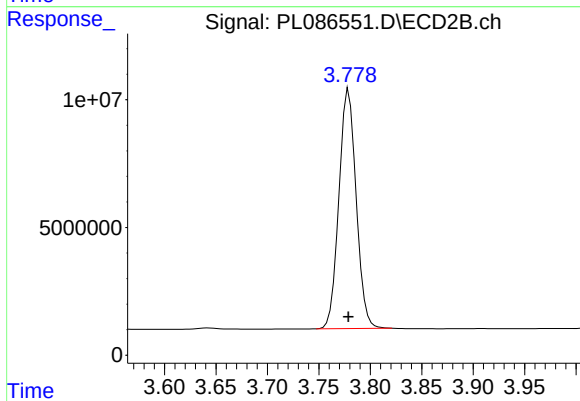


#4 Heptachlor

R.T.: 3.779 min
Delta R.T.: 0.000 min
Response: 109513913
Conc: 90.35 ng/ml

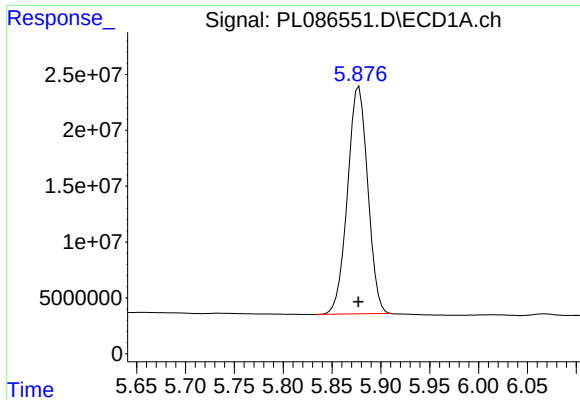


#9 Endosulfan I

R.T.: 5.878 min
Delta R.T.: 0.000 min
Response: 293569207
Conc: 80.28 ng/ml

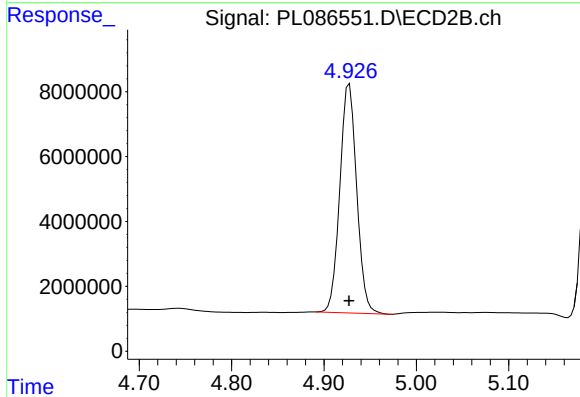


#9 Endosulfan I

R.T.: 4.927 min
Delta R.T.: 0.000 min
Response: 89732387
Conc: 85.34 ng/ml

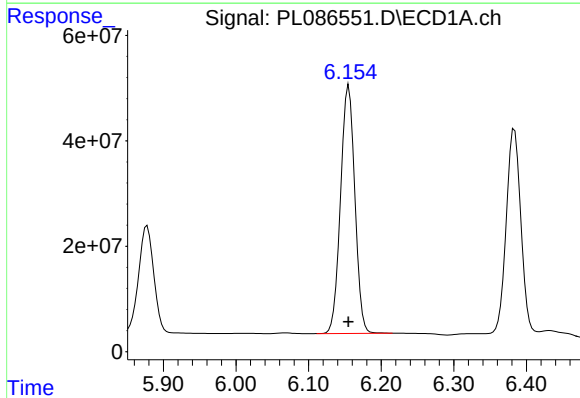


#13 Dieldrin

R.T.: 6.155 min
Delta R.T.: 0.000 min
Response: 644417240
Conc: 177.03 ng/ml

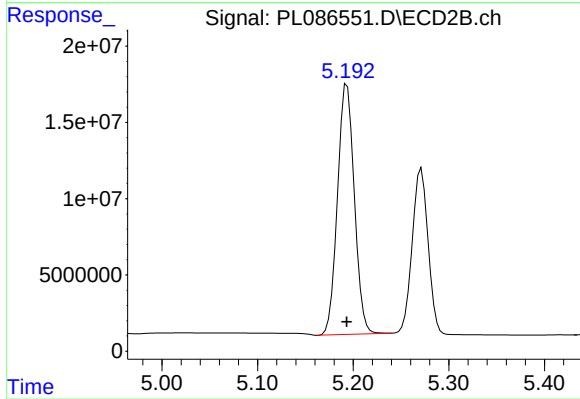


#13 Dieldrin

R.T.: 5.193 min
Delta R.T.: 0.000 min
Response: 201079378
Conc: 180.04 ng/ml

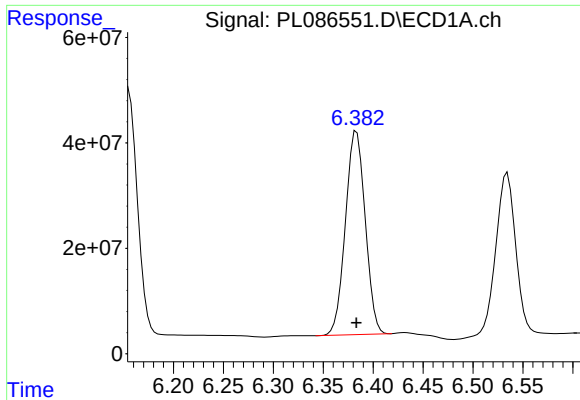


#14 Endrin

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 533548672
Conc: 173.82 ng/ml

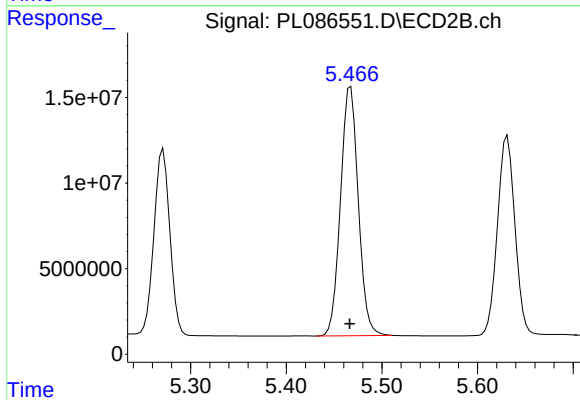


#14 Endrin

R.T.: 5.467 min
Delta R.T.: 0.000 min
Response: 188351087
Conc: 181.60 ng/ml

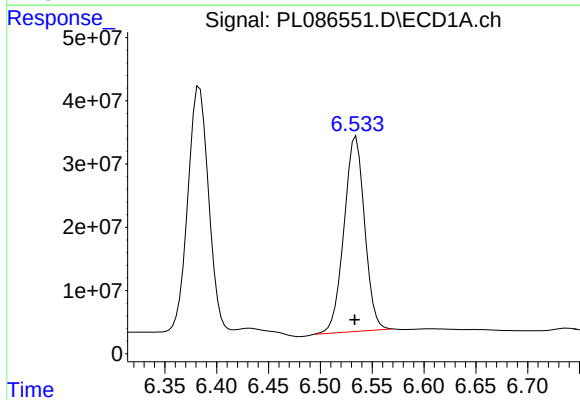


#16 4,4'-DDD

R.T.: 6.534 min
Delta R.T.: 0.001 min
Response: 427075411
Conc: 178.82 ng/ml

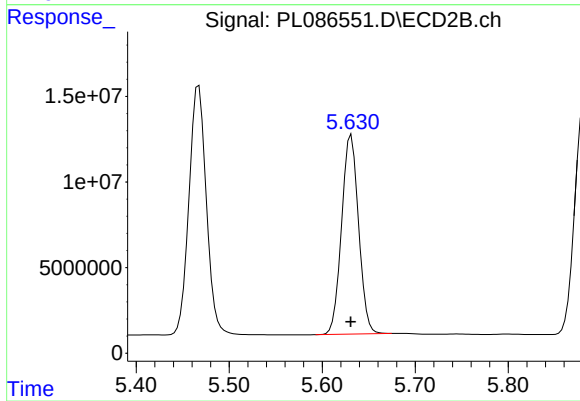


#16 4,4'-DDD

R.T.: 5.631 min
Delta R.T.: 0.000 min
Response: 147560714
Conc: 190.07 ng/ml

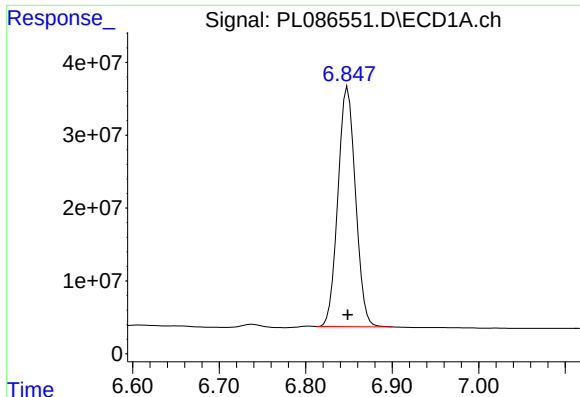


#17 4,4'-DDT

R.T.: 6.849 min
Delta R.T.: 0.000 min
Response: 461506368
Conc: 180.40 ng/ml

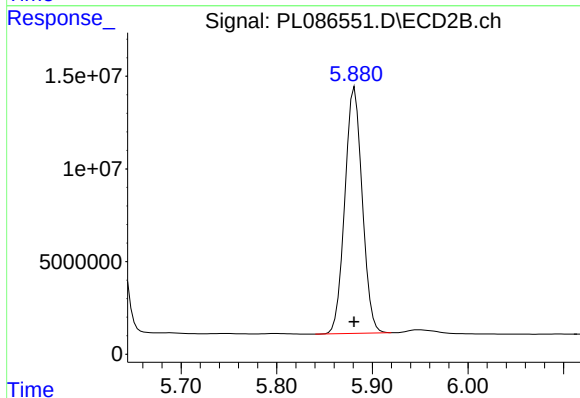


#17 4,4'-DDT

R.T.: 5.882 min
Delta R.T.: 0.000 min
Response: 168621142
Conc: 187.53 ng/ml

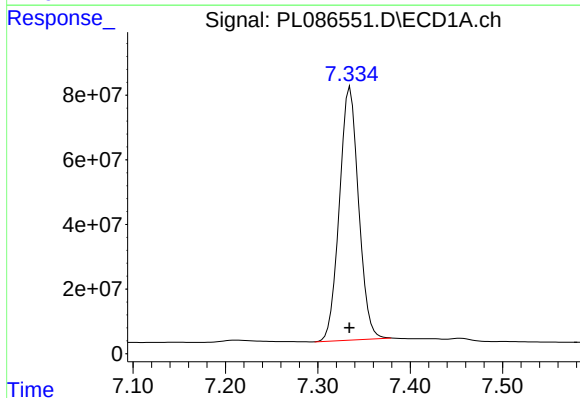


#20 Methoxychlor

R.T.: 7.335 min
Delta R.T.: 0.000 min
Response: 1130862636
Conc: 816.38 ng/ml

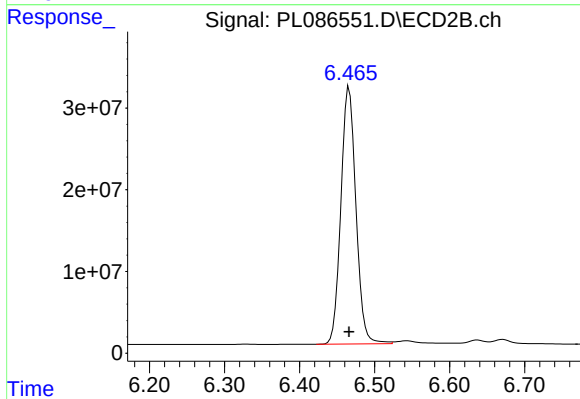


#20 Methoxychlor

R.T.: 6.466 min
Delta R.T.: 0.000 min
Response: 438689326
Conc: 808.33 ng/ml

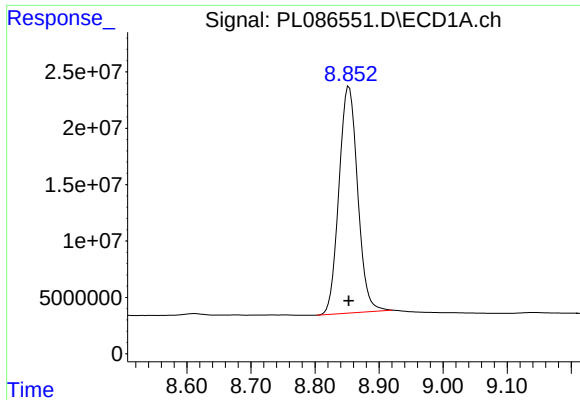

#27 Decachlorobiphenyl

R.T.: 8.853 min
Delta R.T.: 0.000 min
Response: 407743541
Conc: 154.32 ng/ml

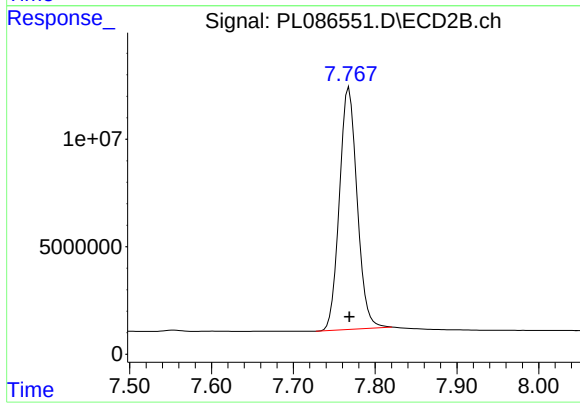

#27 Decachlorobiphenyl

R.T.: 7.768 min
Delta R.T.: 0.000 min
Response: 168887018
Conc: 151.87 ng/ml