

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111020\
 Data File : PL062928.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2020 16:18
 Operator : DD\AJ
 Sample : L4680-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 00:50:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.411	3.950	26179151	45094318	15.220	15.345
28)	SA Decachlor...	8.126	8.990	20297432	24847445	12.652	11.872
Target Compounds							
9)	A Endosulfan I	5.452	0.000	14402	0	0.009	N.D. #
15)	B Endosulfa...	0.000	6.866	0	2454177	N.D.	0.859 #
23)	Chlordane-1	4.274	0.000	1465326	0	28.425	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111020\
Data File : PL062928.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2020 16:18
Operator : DD\AJ
Sample : L4680-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 00:50:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

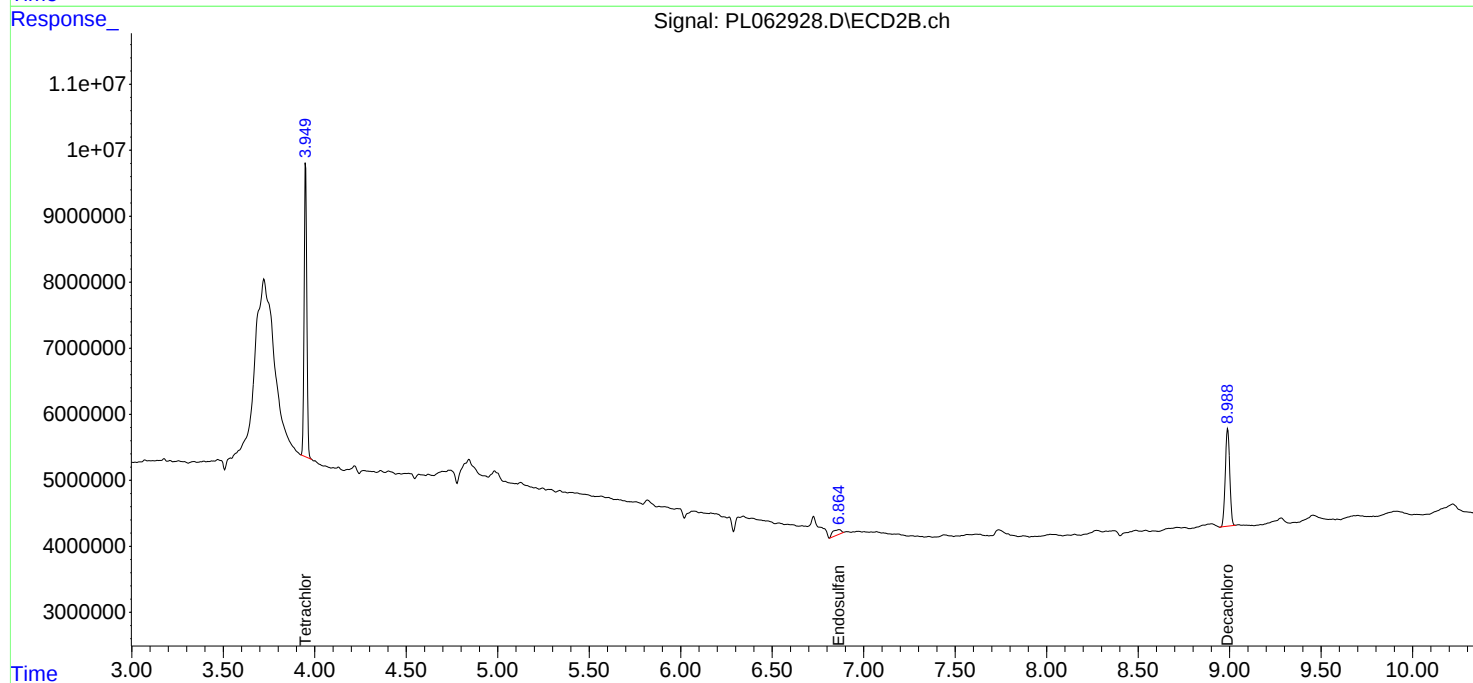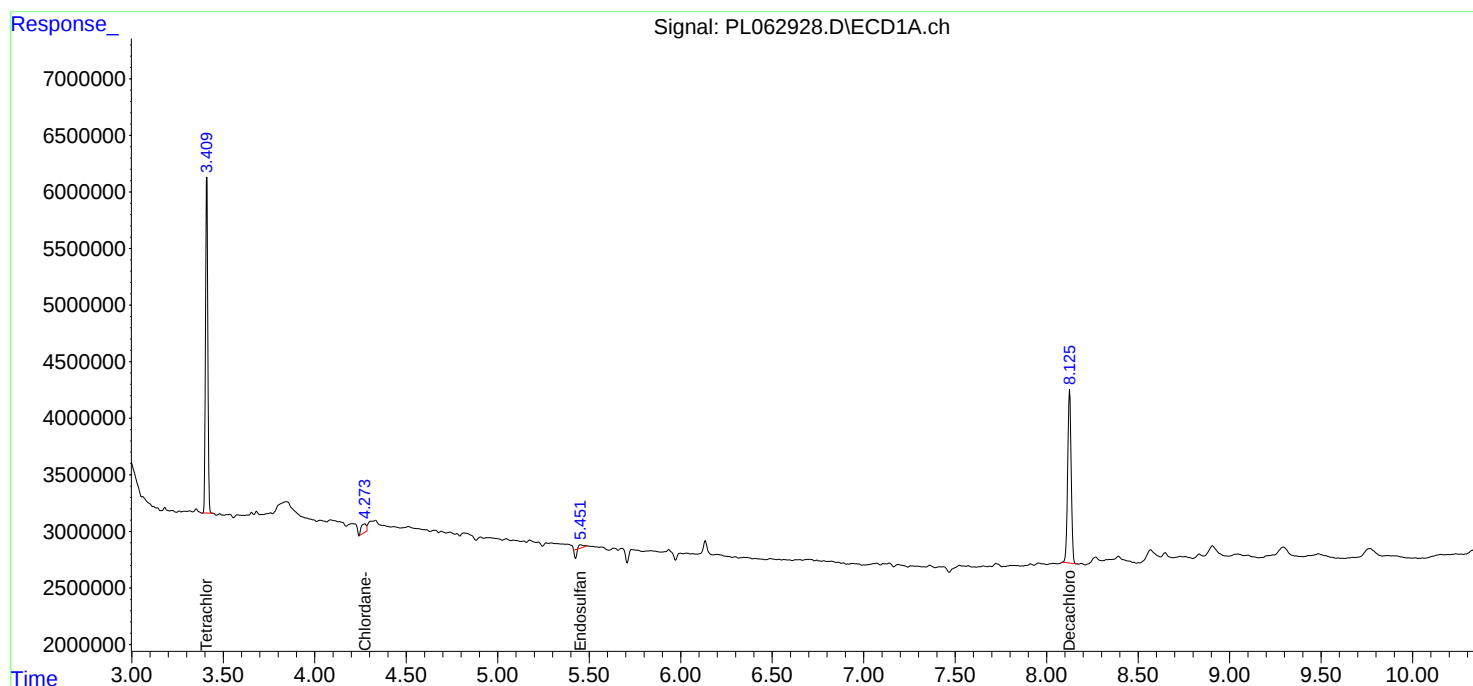


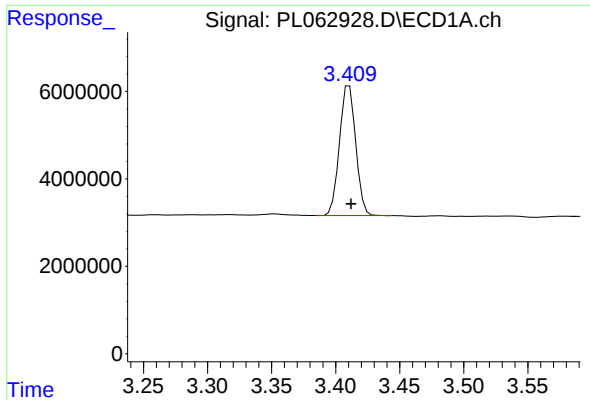

#1 Tetrachloro-m-xylene


R.T.: 3.411 min
Delta R.T.: -0.001 min
Response: 26179151
Conc: 15.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

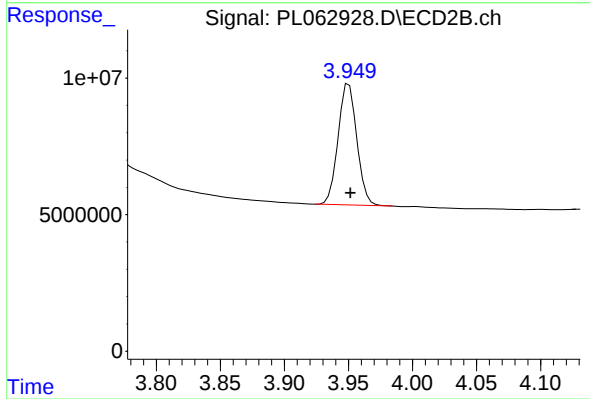


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: -0.001 min
Response: 45094318
Conc: 15.34 ng/ml

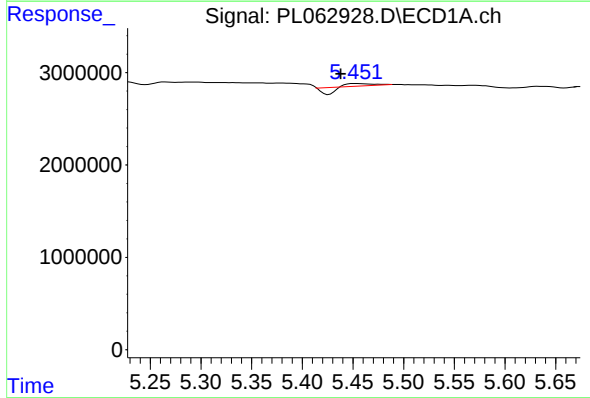


#9 Endosulfan I

R.T.: 5.452 min
Delta R.T.: 0.014 min
Response: 14402
Conc: 0.01 ng/ml

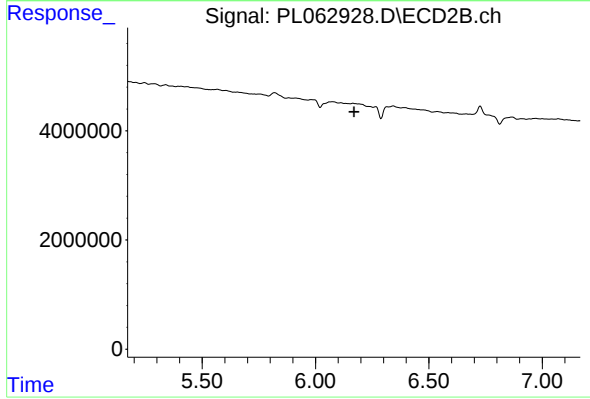

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.170 min
Response: 0
Conc: N.D.

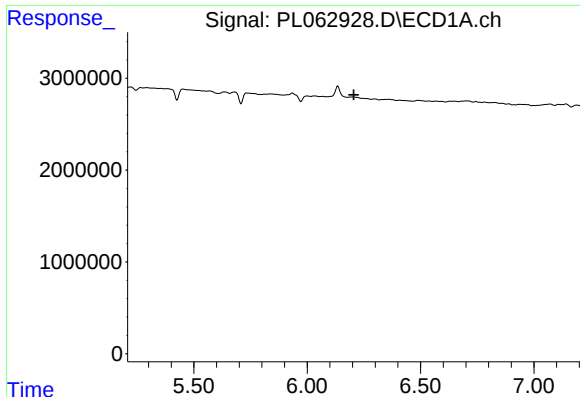

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.205 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

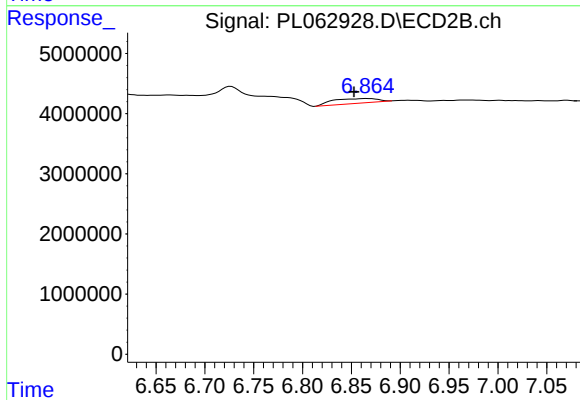


#15 Endosulfan II

R.T.: 6.866 min
Delta R.T.: 0.013 min
Response: 2454177
Conc: 0.86 ng/ml

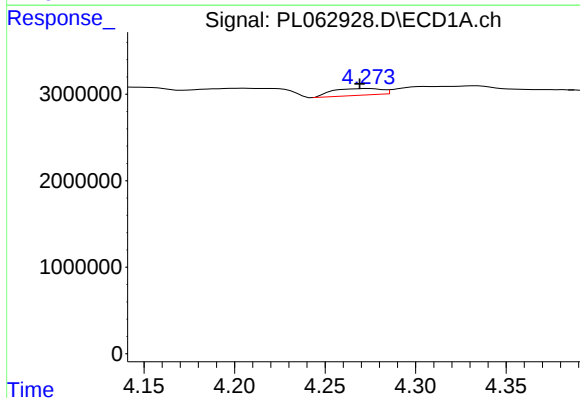


#23 Chlordane-1

R.T.: 4.274 min
Delta R.T.: 0.005 min
Response: 1465326
Conc: 28.43 ng/ml

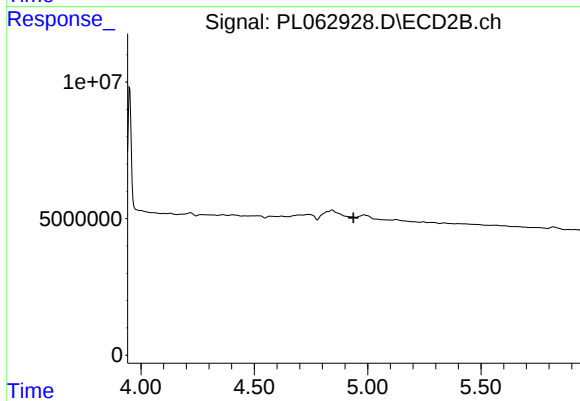

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.938 min
Response: 0
Conc: N.D.

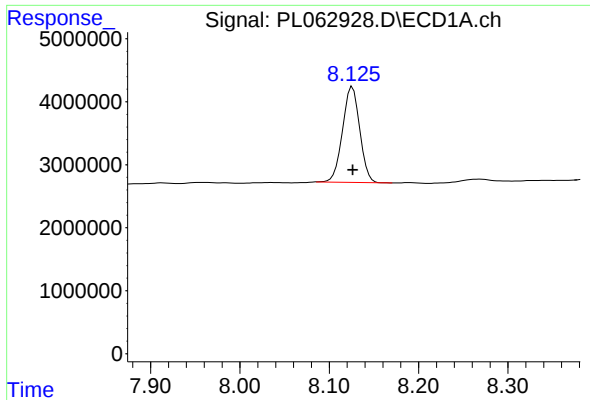

#28 Decachlorobiphenyl

R.T.: 8.126 min
Delta R.T.: 0.000 min
Response: 20297432
Conc: 12.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

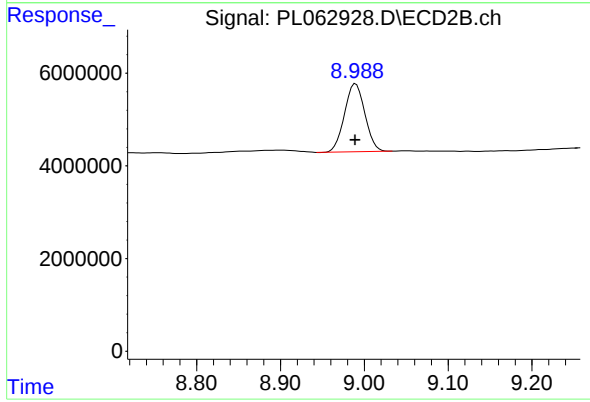

#28 Decachlorobiphenyl

R.T.: 8.990 min
Delta R.T.: 0.000 min
Response: 24847445
Conc: 11.87 ng/ml