

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111020\
 Data File : PL062930.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2020 16:46
 Operator : DD\AJ
 Sample : L4681-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 00:50:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.411	3.950	29430582	51974290	17.110	17.686
28)	SA Decachlor...	8.125	8.988	27079530	33807675	16.879	16.153
Target Compounds							
5)	MB Aldrin	4.656	5.422	2900752	2420706	1.520	0.669 #
8)	B Heptachlo...	5.097	5.825	2955803	8079469	1.620	2.495 #
9)	A Endosulfan I	5.451	6.166	1541386	1111906	0.922	0.353 #
11)	B alpha-Chl...	0.000	6.092f	0	7406444	N.D.	2.198 #
14)	MA Endrin	5.936	0.000	1697350	0	1.020	N.D. #
15)	B Endosulfa...	0.000	6.866	0	4550090	N.D.	1.592 #
17)	MA 4,4'-DDT	6.298	0.000	205900	0	0.154	N.D. #
18)	B Endrin al...	6.343f	6.958f	933322	2547307	0.643	1.117 #
24)	Chlordane-2	0.000	5.422f	0	2420706	N.D.	22.201 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111020\
Data File : PL062930.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2020 16:46
Operator : DD\AJ
Sample : L4681-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 00:50:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

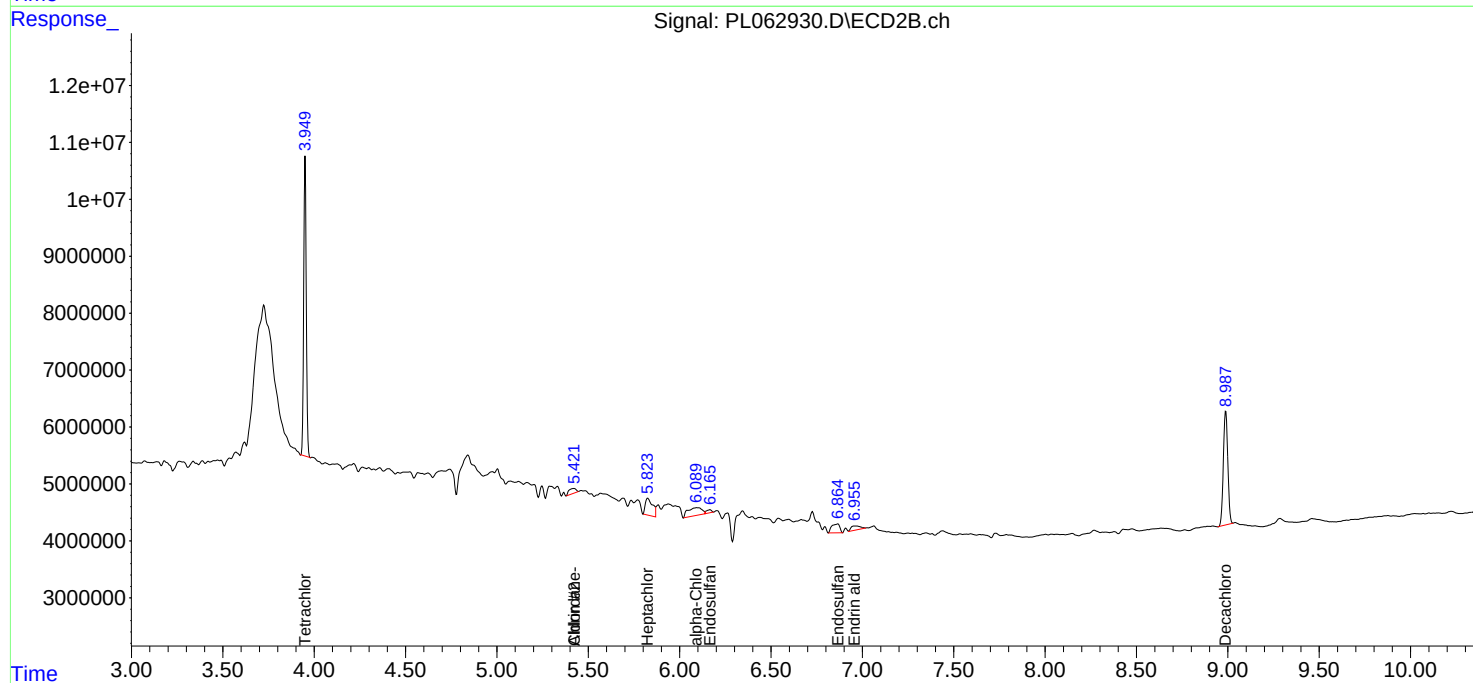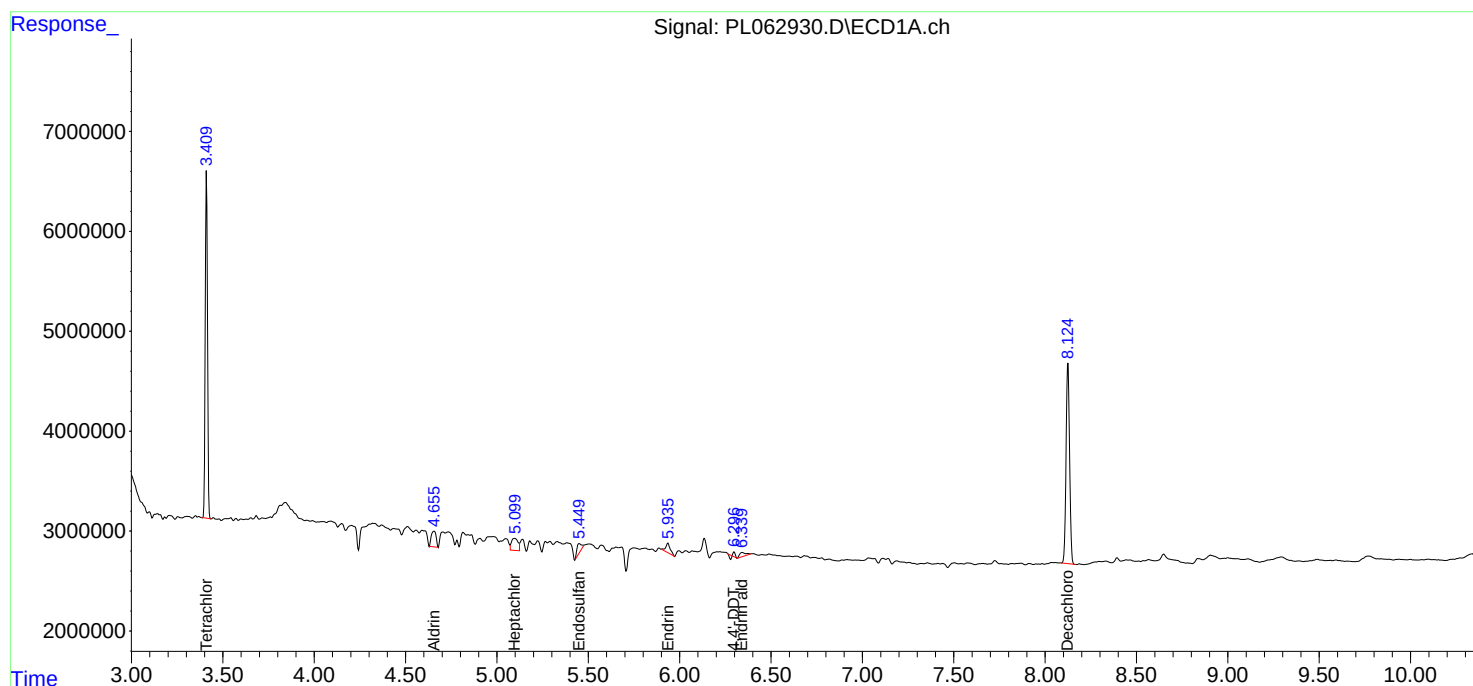


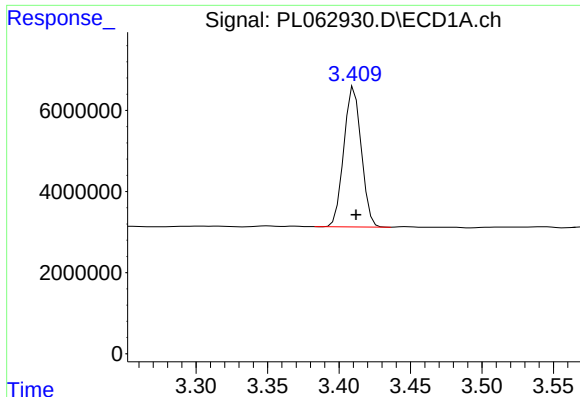

#1 Tetrachloro-m-xylene


R.T.: 3.411 min
Delta R.T.: -0.001 min
Response: 29430582
Conc: 17.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

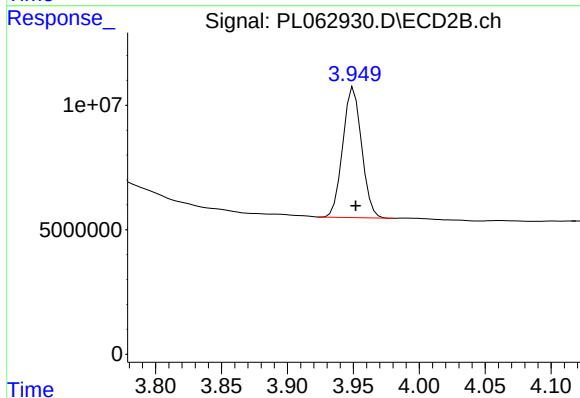


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: -0.001 min
Response: 51974290
Conc: 17.69 ng/ml

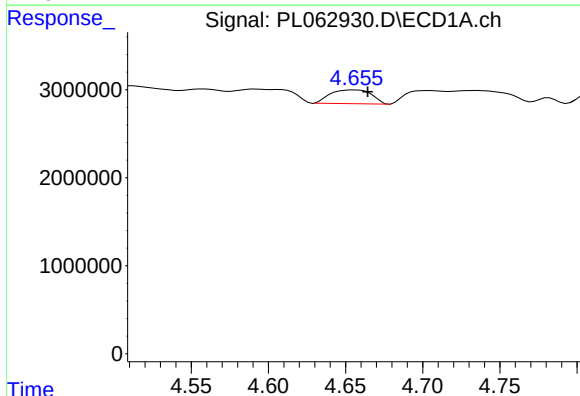


#5 Aldrin

R.T.: 4.656 min
Delta R.T.: -0.008 min
Response: 2900752
Conc: 1.52 ng/ml

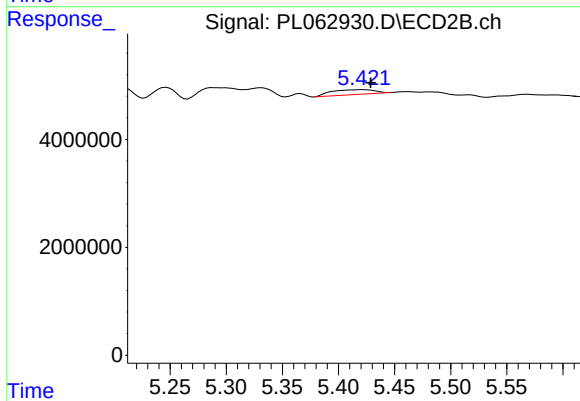

#5 Aldrin


R.T.: 5.422 min
Delta R.T.: -0.007 min
Response: 2420706
Conc: 0.67 ng/ml

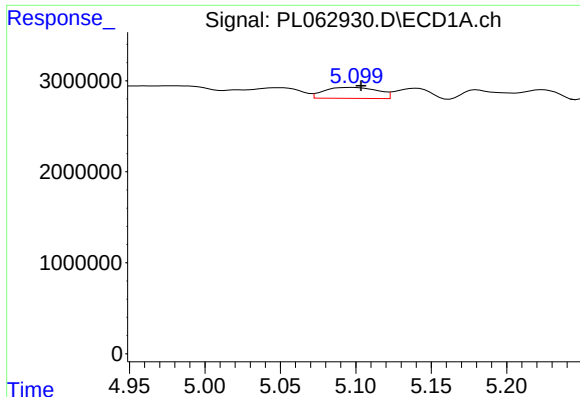

#8 Heptachlor epoxide


R.T.: 5.097 min
Delta R.T.: -0.006 min
Response: 2955803
Conc: 1.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

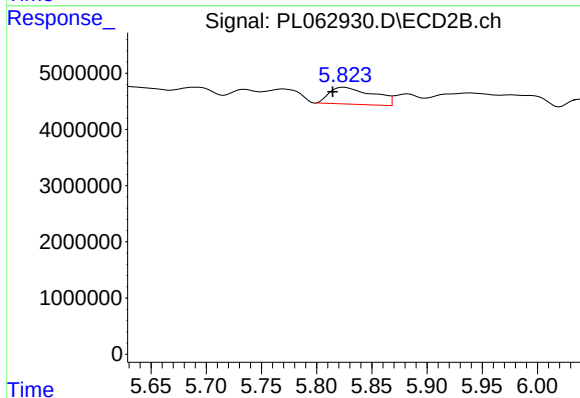


#8 Heptachlor epoxide

R.T.: 5.825 min
Delta R.T.: 0.010 min
Response: 8079469
Conc: 2.49 ng/ml

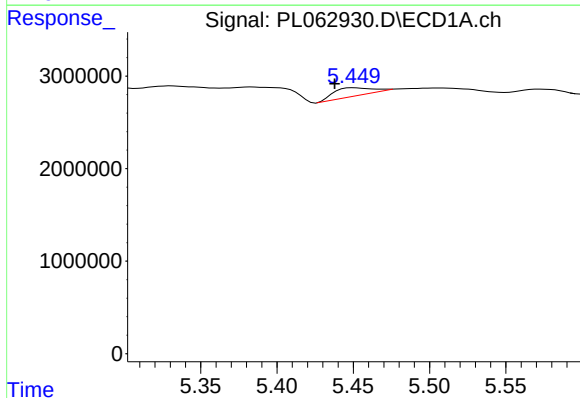


#9 Endosulfan I

R.T.: 5.451 min
Delta R.T.: 0.013 min
Response: 1541386
Conc: 0.92 ng/ml

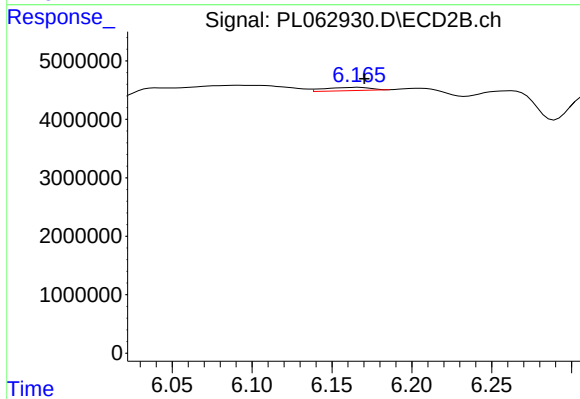

#9 Endosulfan I


R.T.: 6.166 min
Delta R.T.: -0.004 min
Response: 1111906
Conc: 0.35 ng/ml

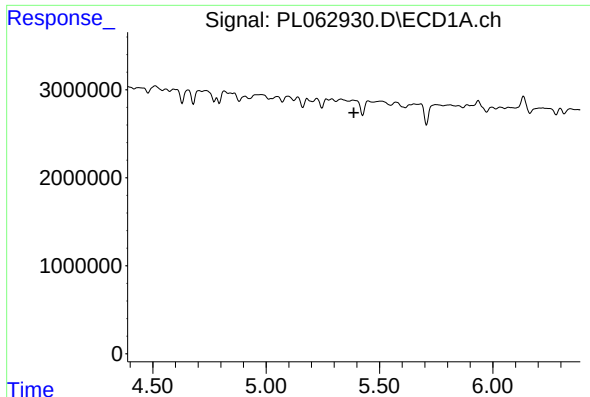

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.386 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

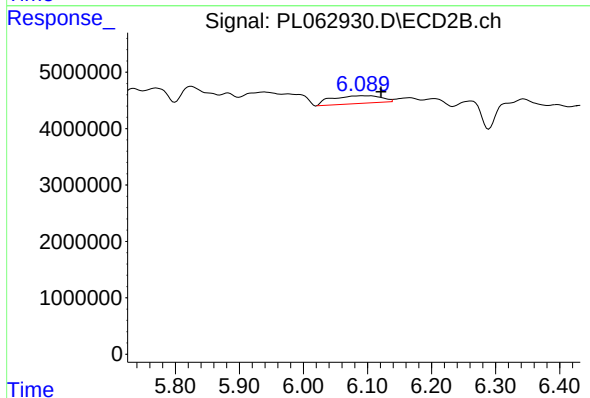


#11 alpha-Chlordane

R.T.: 6.092 min
Delta R.T.: -0.029 min
Response: 7406444
Conc: 2.20 ng/ml

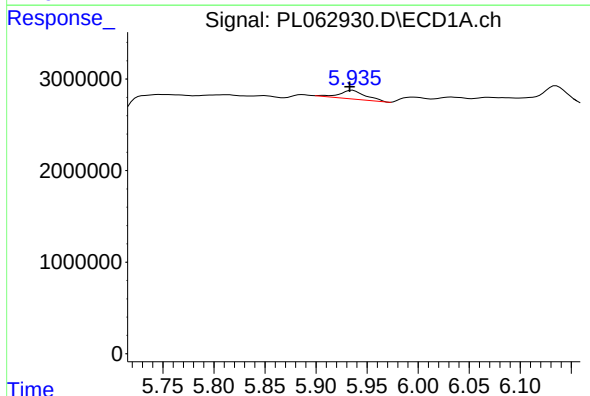


#14 Endrin

R.T.: 5.936 min
Delta R.T.: 0.002 min
Response: 1697350
Conc: 1.02 ng/ml

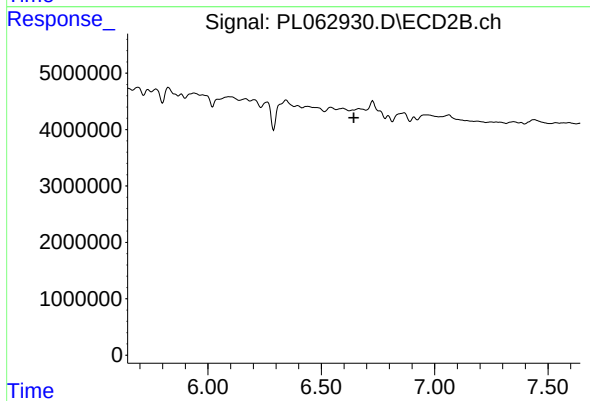

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.643 min
Response: 0
Conc: N.D.

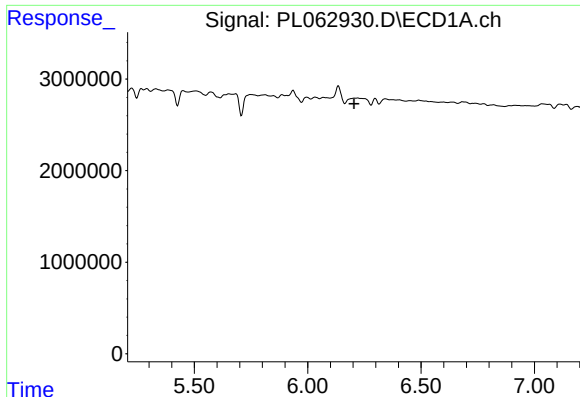

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.205 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

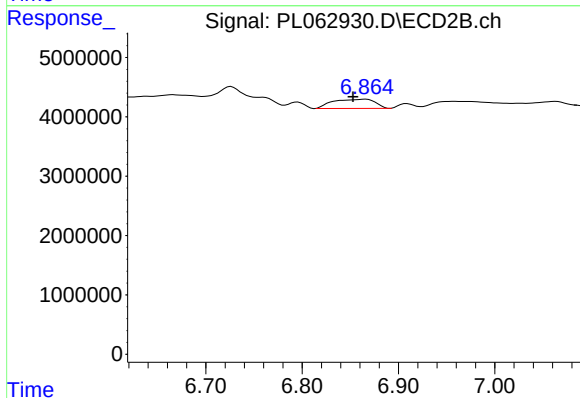


#15 Endosulfan II

R.T.: 6.866 min
Delta R.T.: 0.013 min
Response: 4550090
Conc: 1.59 ng/ml

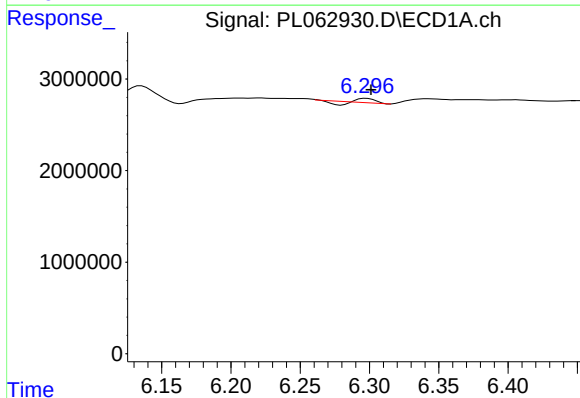


#17 4,4'-DDT

R.T.: 6.298 min
Delta R.T.: -0.003 min
Response: 205900
Conc: 0.15 ng/ml

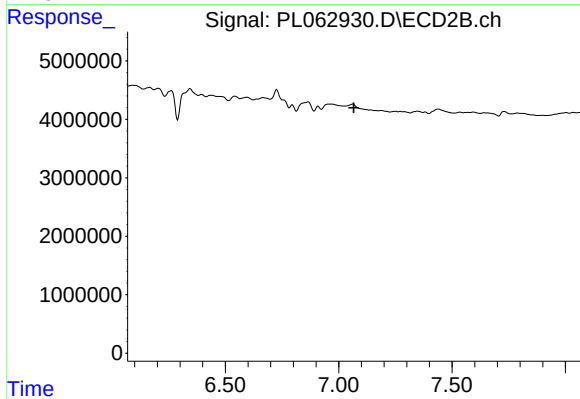

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.066 min
Response: 0
Conc: N.D.

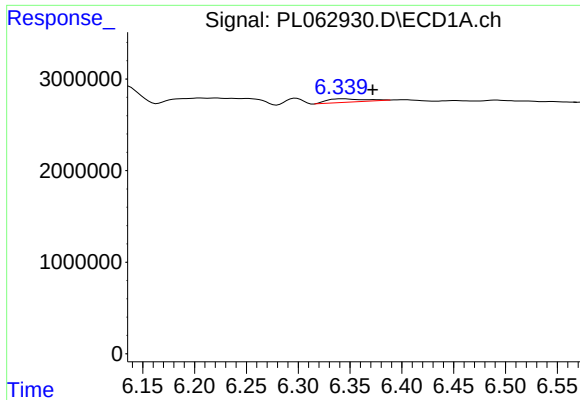

#18 Endrin aldehyde


R.T.: 6.343 min
Delta R.T.: -0.029 min
Response: 933322
Conc: 0.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

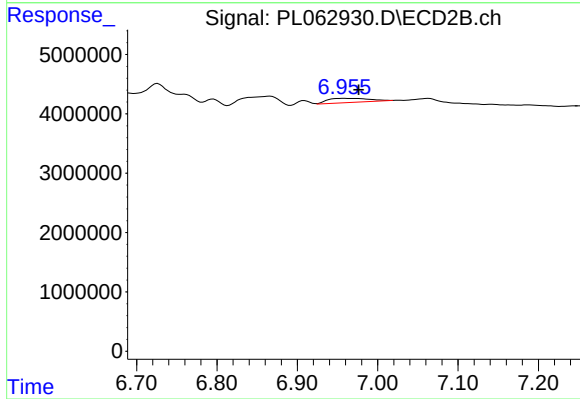


#18 Endrin aldehyde

R.T.: 6.958 min
Delta R.T.: -0.018 min
Response: 2547307
Conc: 1.12 ng/ml

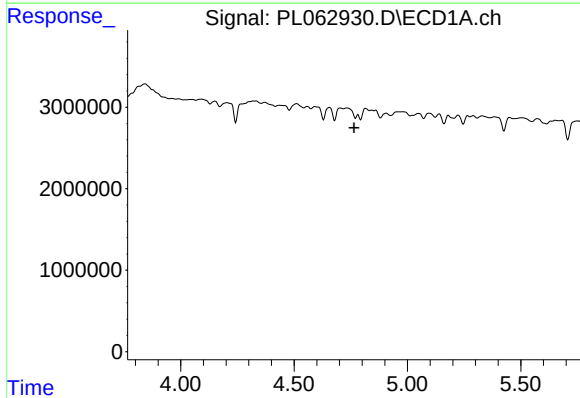


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.765 min
Response: 0
Conc: N.D.

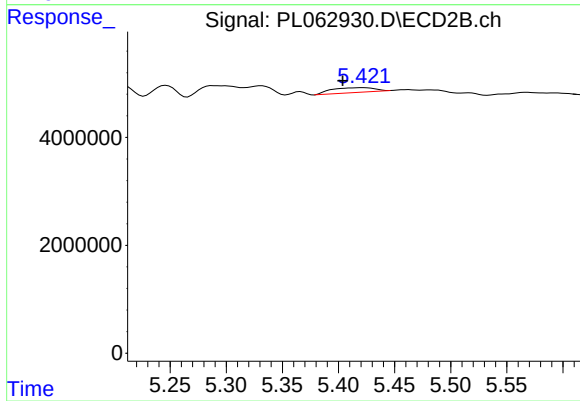

#24 Chlordane-2


R.T.: 5.422 min
Delta R.T.: 0.018 min
Response: 2420706
Conc: 22.20 ng/ml

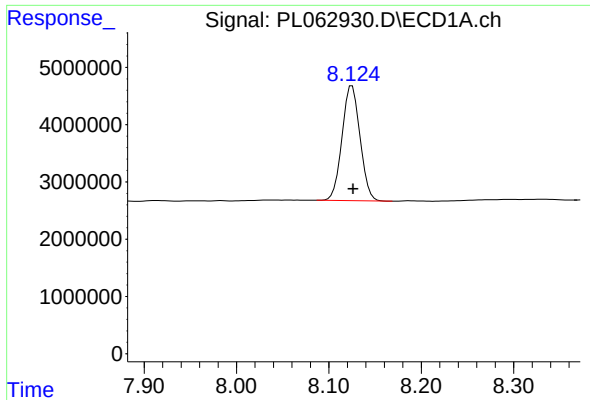

#28 Decachlorobiphenyl

R.T.: 8.125 min
Delta R.T.: -0.001 min
Response: 27079530
Conc: 16.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

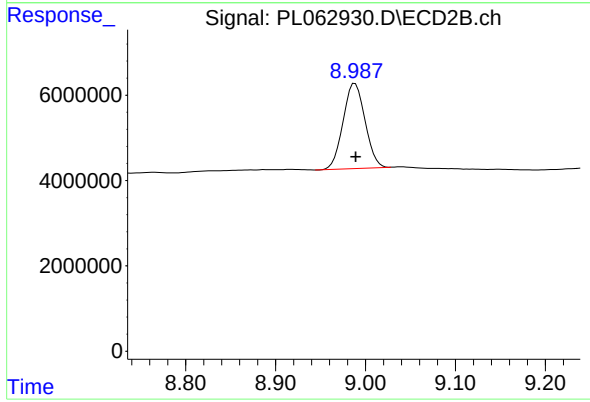

#28 Decachlorobiphenyl

R.T.: 8.988 min
Delta R.T.: 0.000 min
Response: 33807675
Conc: 16.15 ng/ml