

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111020\
 Data File : PL062927.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2020 16:03
 Operator : DD\AJ
 Sample : L4680-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PAV-B7-110520-DP

Manual Integrations
 APPROVED

Ankita
 11/11/2020 9:04:18 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 00:50:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.411	3.950	27119247	44830559	15.766	15.255
28)	SA Decachlor...	8.126	8.988	23440374	28661508	14.611	13.694
Target Compounds							
16)	A 4,4'-DDD	6.061	6.765	1194547	3446974	0.845m	1.346m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111020\
Data File : PL062927.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2020 16:03
Operator : DD\AJ
Sample : L4680-03
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PAV-B7-110520-DP


Manual Integrations
APPROVED

Ankita
11/11/2020 9:04:18 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 00:50:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

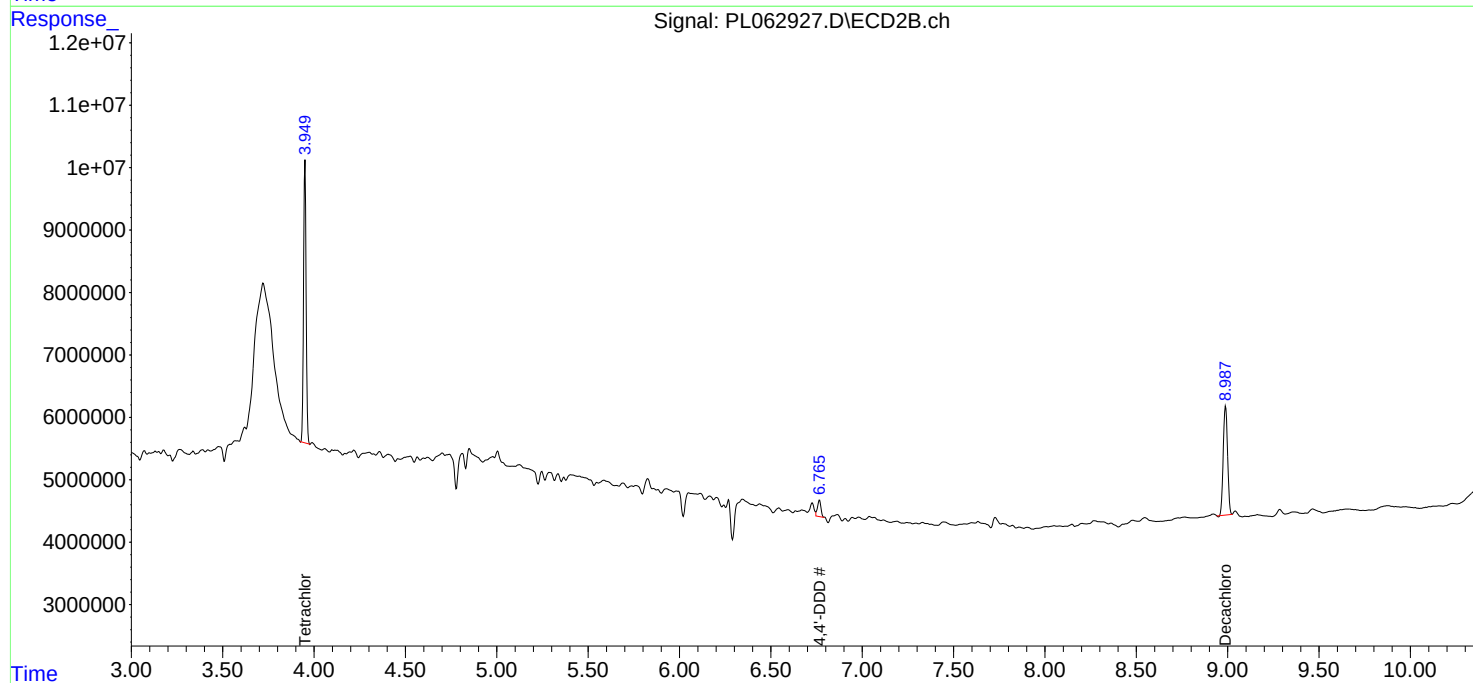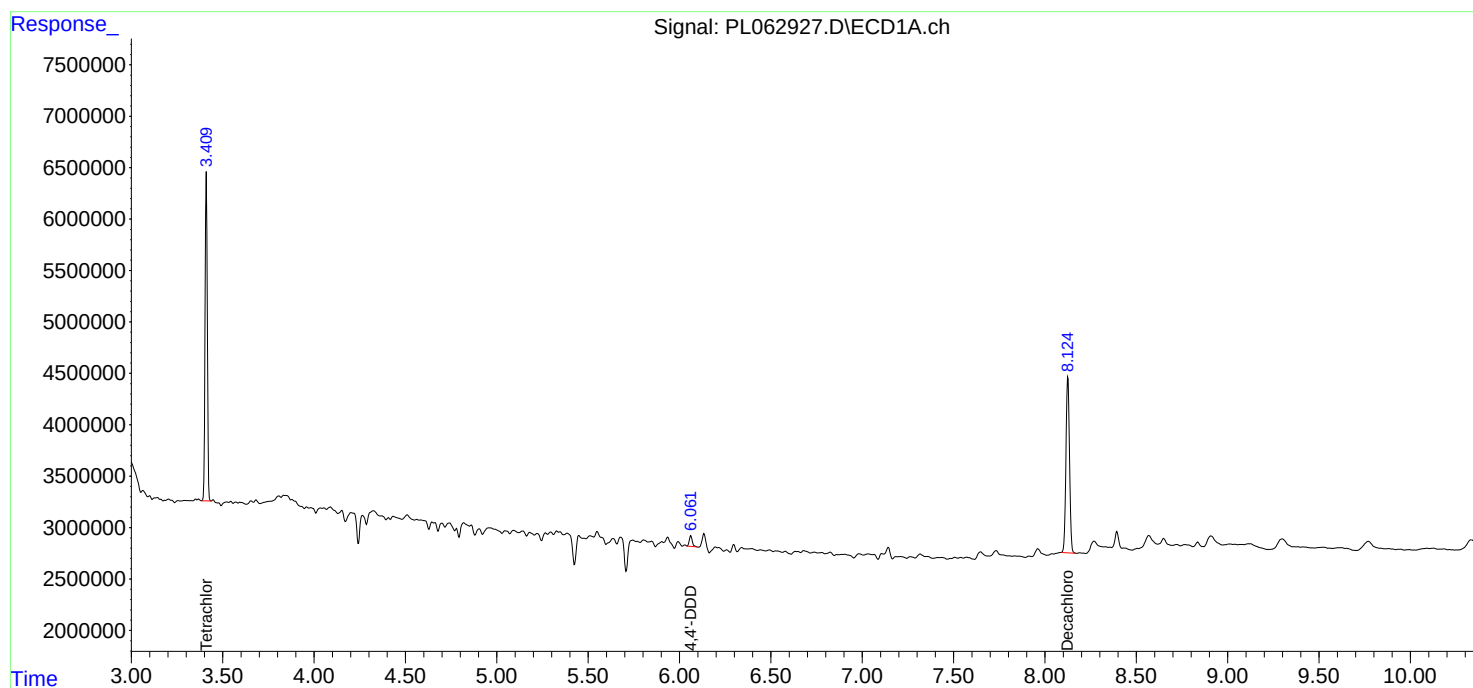

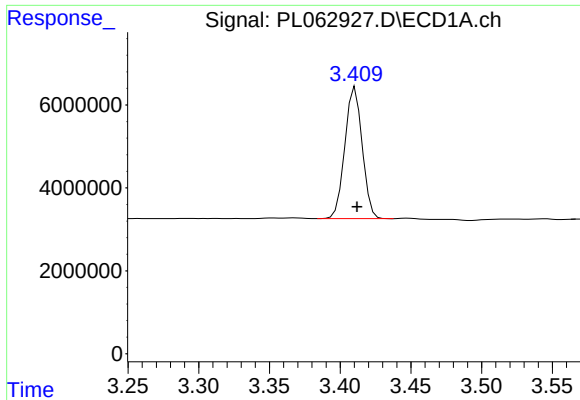


#1 Tetrachloro-m-xylene

R.T.: 3.411 min
Delta R.T.: -0.001 min
Response: 27119247
Conc: 15.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
PAV-B7-110520-DP


Manual Integrations
APPROVED

Ankita
11/11/2020 9:04:18 AM

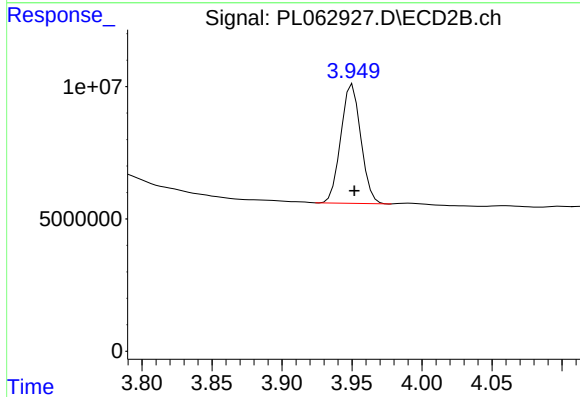


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: -0.001 min
Response: 44830559
Conc: 15.26 ng/ml

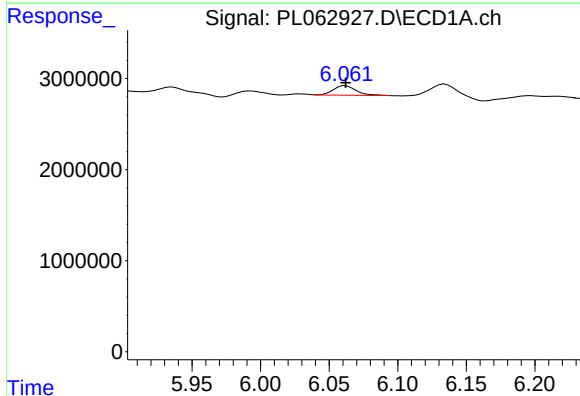


#16 4,4'-DDD

R.T.: 6.061 min
Delta R.T.: -0.001 min
Response: 1194547
Conc: 0.84 ng/ml m

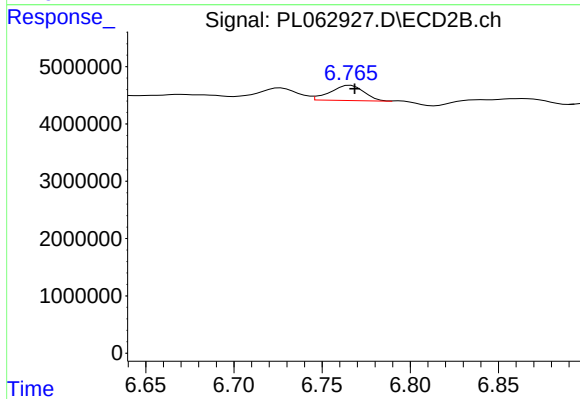

#16 4,4'-DDD

R.T.: 6.765 min
Delta R.T.: -0.004 min
Response: 3446974
Conc: 1.35 ng/ml m

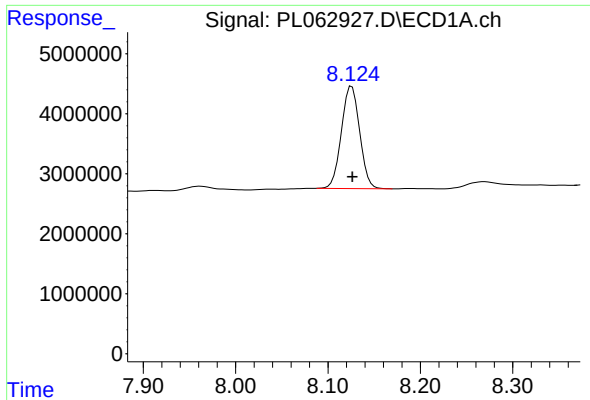


#28 Decachlorobiphenyl

R.T.: 8.126 min
Delta R.T.: 0.000 min
Response: 23440374
Conc: 14.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
PAV-B7-110520-DP

Manual Integrations
APPROVED

Ankita
11/11/2020 9:04:18 AM

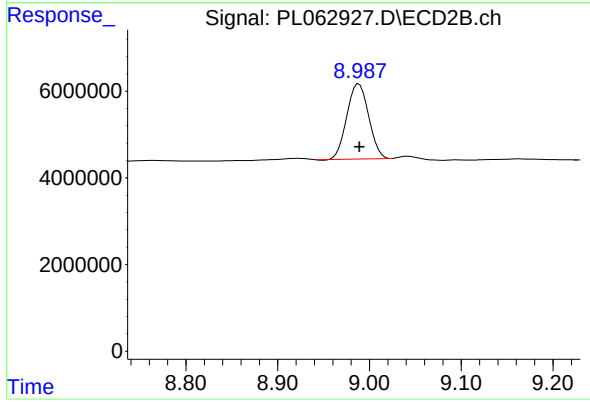

#28 Decachlorobiphenyl

R.T.: 8.988 min
Delta R.T.: 0.000 min
Response: 28661508
Conc: 13.69 ng/ml