

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111022\
 Data File : PL079006.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2022 17:47
 Operator : AR\AJ
 Sample : N5532-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 20:49:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.322	2.569	33159634	43043999	17.388	16.859
28)	SA Decachlor...	8.769	7.634	19344262	26845589	12.859	14.173
Target Compounds							
5)	MB Aldrin	5.013	0.000	83136	0	0.034	N.D. #
9)	A Endosulfan I	5.852	0.000	324659	0	0.152	N.D. #
14)	MA Endrin	0.000	5.390f	0	503976	N.D.	0.193 #
15)	B Endosulfa...	6.552f	0.000	3540507	0	1.887	N.D. #
17)	MA 4,4'-DDT	6.789f	0.000	625743	0	0.349	N.D. #
18)	B Endrin al...	0.000	5.869f	0	806179	N.D.	0.430 #
19)	B Endosulfa...	0.000	6.052f	0	793626	N.D.	0.333 #
20)	A Methoxychlor	0.000	6.353	0	26356	N.D.	0.023 #
23)	Chlordane-1	0.000	3.551	0	1008344	N.D.	9.998 #
24)	Chlordane-2	5.013	0.000	83136	0	1.005	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111022\
Data File : PL079006.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2022 17:47
Operator : AR\AJ
Sample : N5532-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 20:49:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

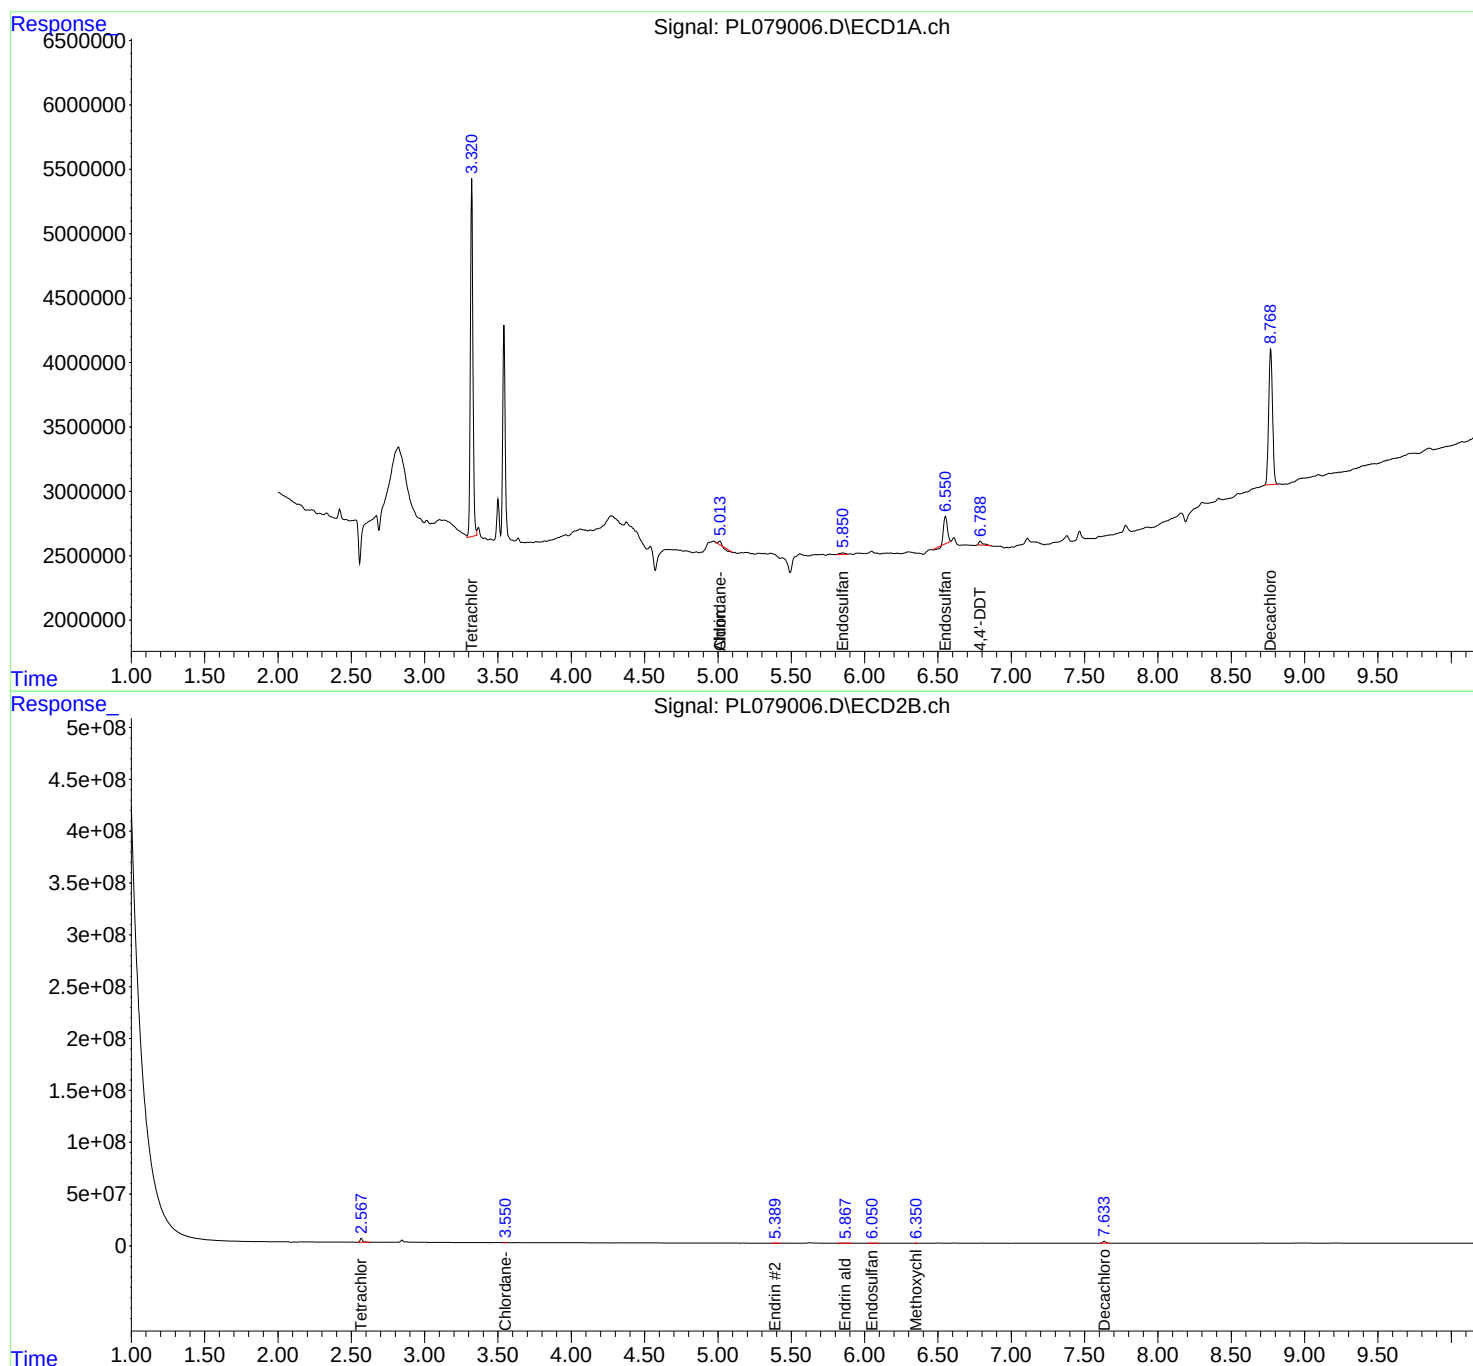


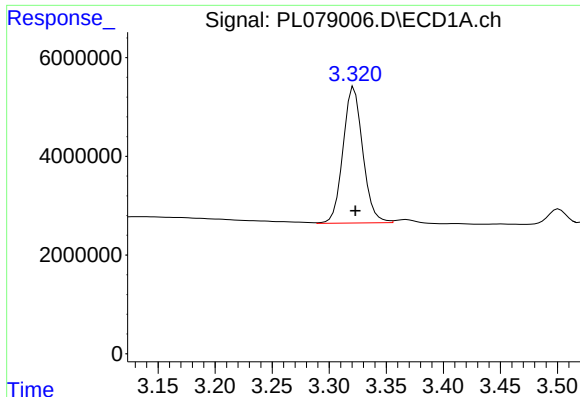

#1 Tetrachloro-m-xylene


R.T.: 3.322 min
Delta R.T.: -0.001 min
Response: 33159634
Conc: 17.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

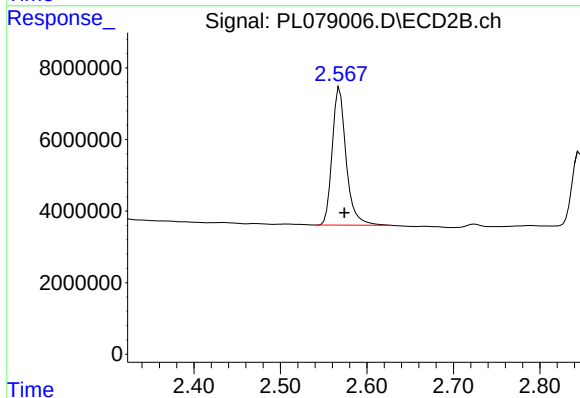


#1 Tetrachloro-m-xylene

R.T.: 2.569 min
Delta R.T.: -0.005 min
Response: 43043999
Conc: 16.86 ng/ml

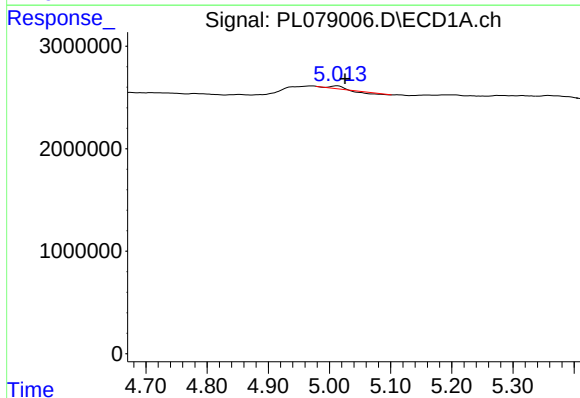


#5 Aldrin

R.T.: 5.013 min
Delta R.T.: -0.012 min
Response: 83136
Conc: 0.03 ng/ml

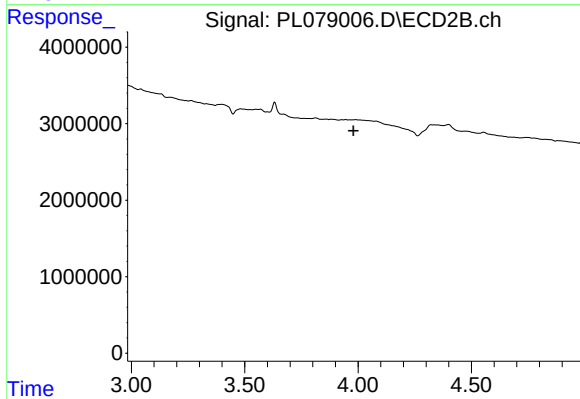

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 3.980 min
Response: 0
Conc: N.D.

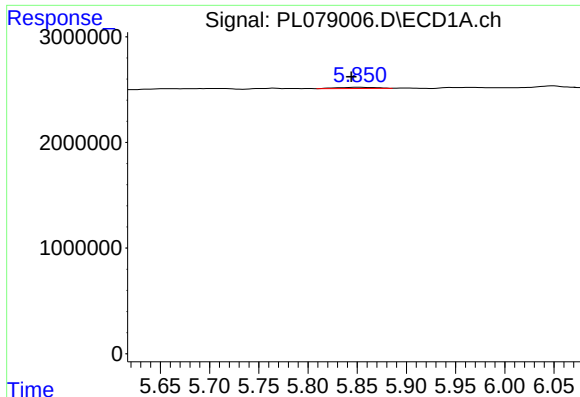

#9 Endosulfan I


R.T.: 5.852 min
Delta R.T.: 0.008 min
Response: 324659
Conc: 0.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

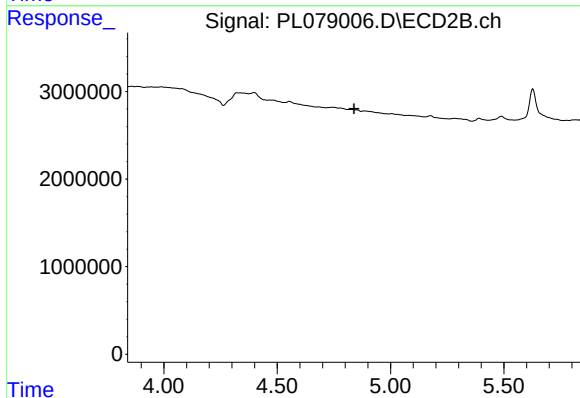


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 4.840 min
Response: 0
Conc: N.D.

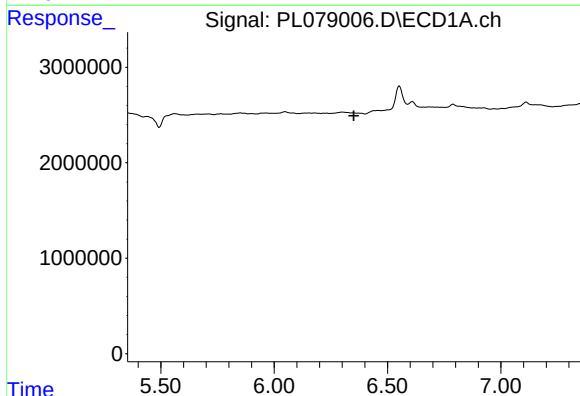


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.351 min
Response: 0
Conc: N.D.

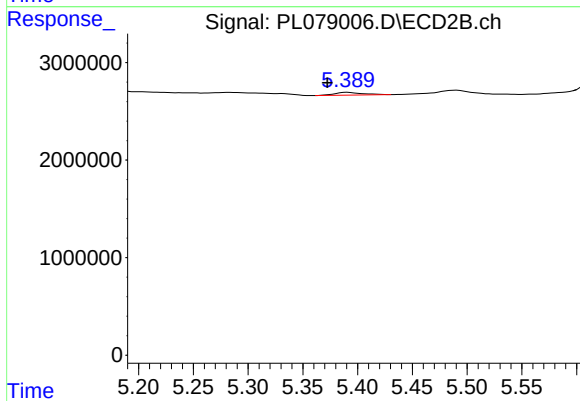

#14 Endrin


R.T.: 5.390 min
Delta R.T.: 0.018 min
Response: 503976
Conc: 0.19 ng/ml

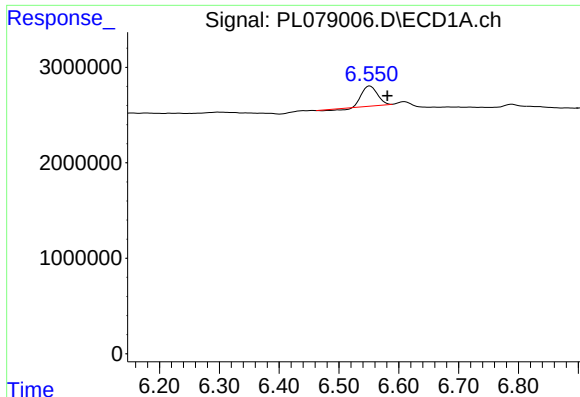

#15 Endosulfan II


R.T.: 6.552 min
Delta R.T.: -0.030 min
Response: 3540507
Conc: 1.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

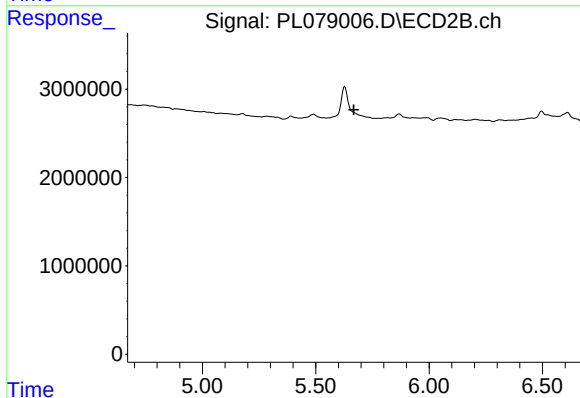


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.669 min
Response: 0
Conc: N.D.

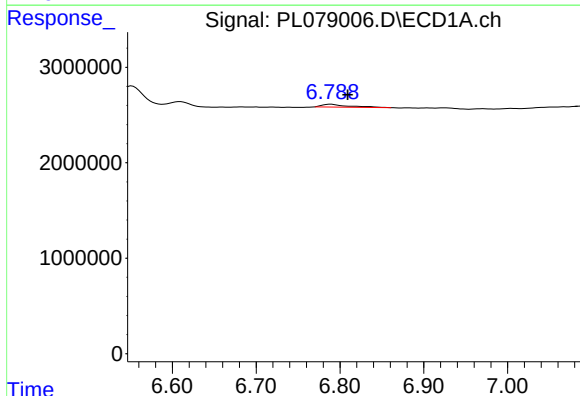


#17 4,4'-DDT

R.T.: 6.789 min
Delta R.T.: -0.020 min
Response: 625743
Conc: 0.35 ng/ml

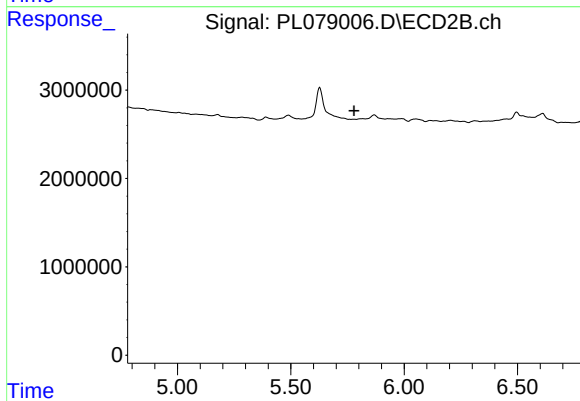

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 5.779 min
Response: 0
Conc: N.D.

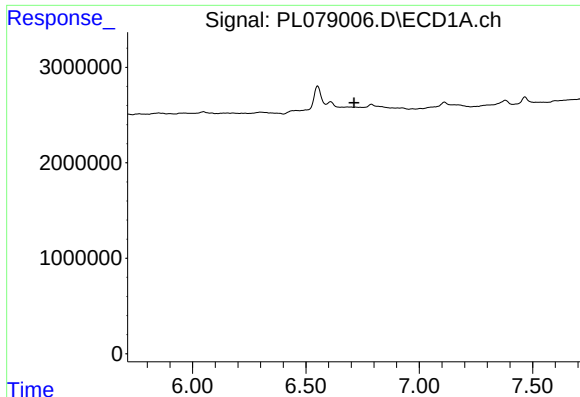

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.713 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

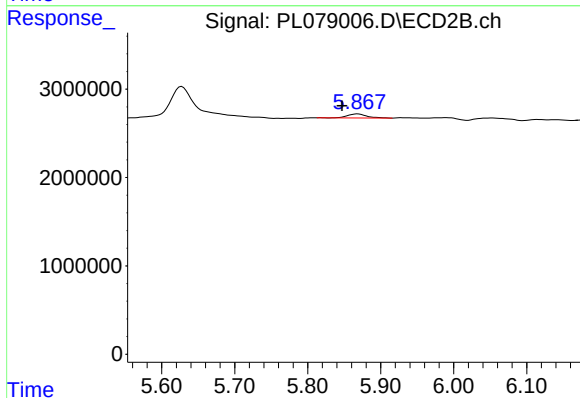


#18 Endrin aldehyde

R.T.: 5.869 min
Delta R.T.: 0.021 min
Response: 806179
Conc: 0.43 ng/ml

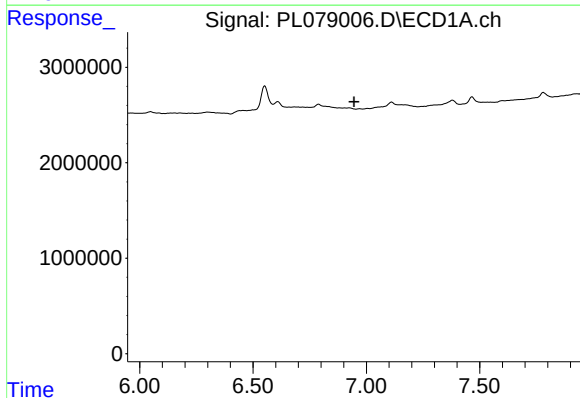


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 6.946 min
Response: 0
Conc: N.D.

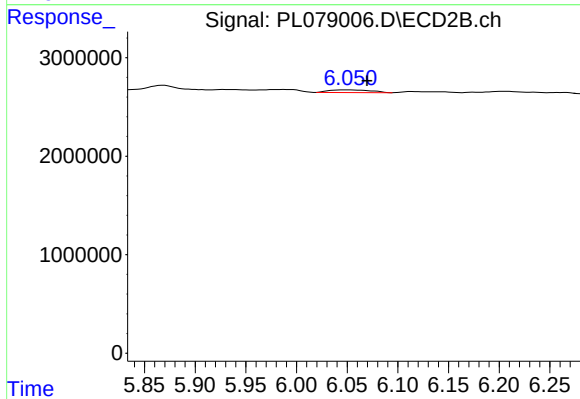

#19 Endosulfan Sulfate


R.T.: 6.052 min
Delta R.T.: -0.018 min
Response: 793626
Conc: 0.33 ng/ml

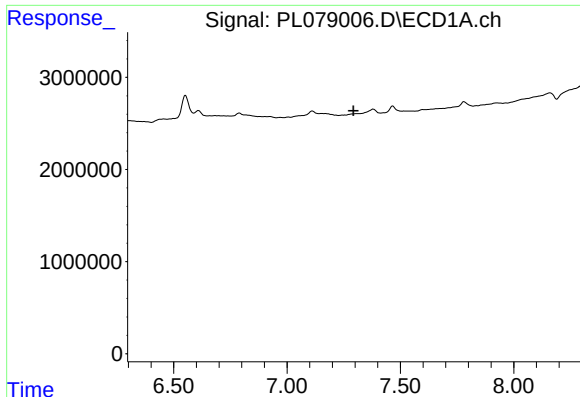

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.294 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

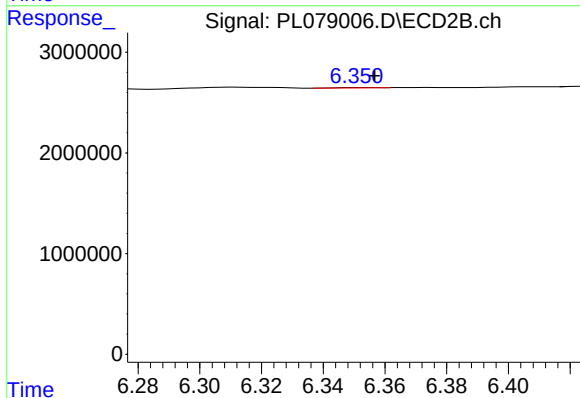


#20 Methoxychlor

R.T.: 6.353 min
Delta R.T.: -0.004 min
Response: 26356
Conc: 0.02 ng/ml

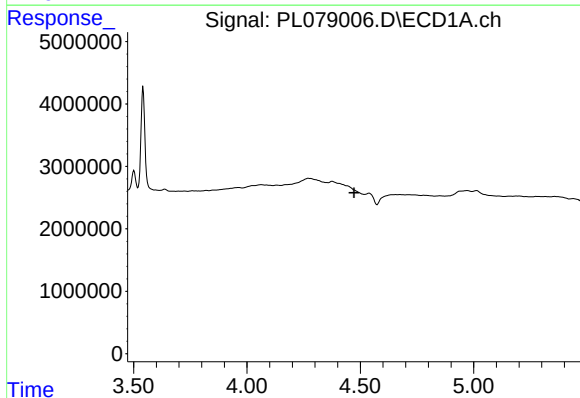


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.472 min
Response: 0
Conc: N.D.

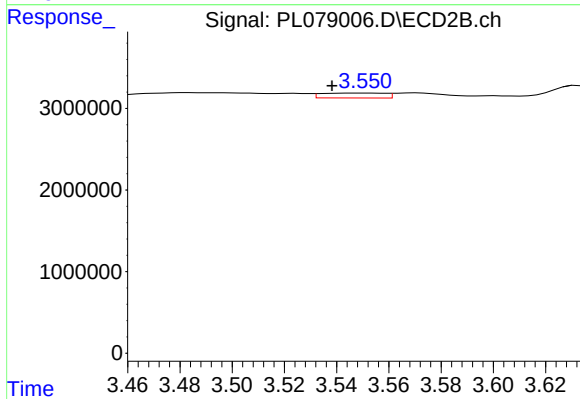

#23 Chlordane-1


R.T.: 3.551 min
Delta R.T.: 0.013 min
Response: 1008344
Conc: 10.00 ng/ml

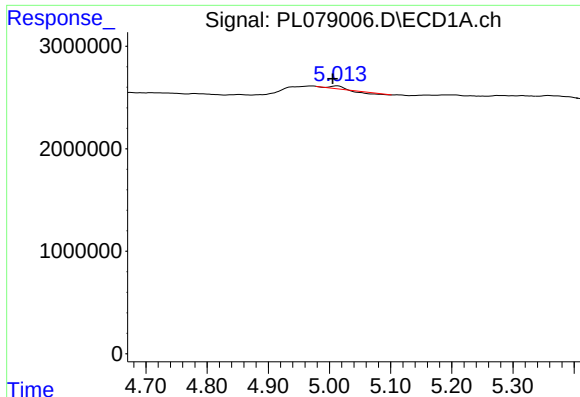

#24 Chlordane-2


R.T.: 5.013 min
Delta R.T.: 0.008 min
Response: 83136
Conc: 1.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

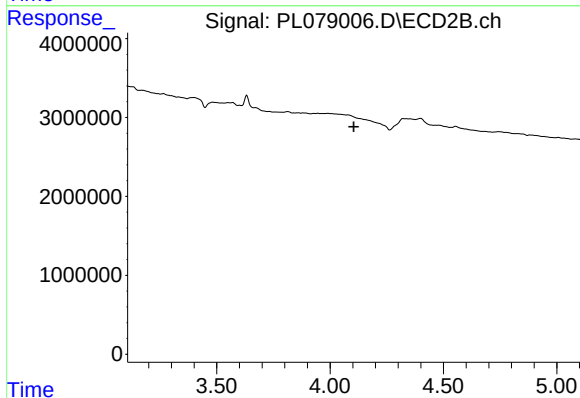


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.105 min
Response: 0
Conc: N.D.

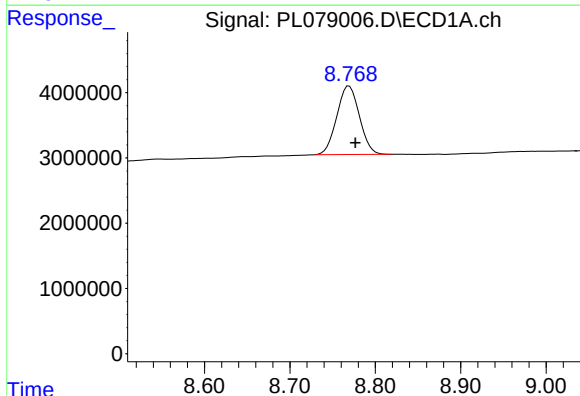

#28 Decachlorobiphenyl

R.T.: 8.769 min
Delta R.T.: -0.007 min
Response: 19344262
Conc: 12.86 ng/ml

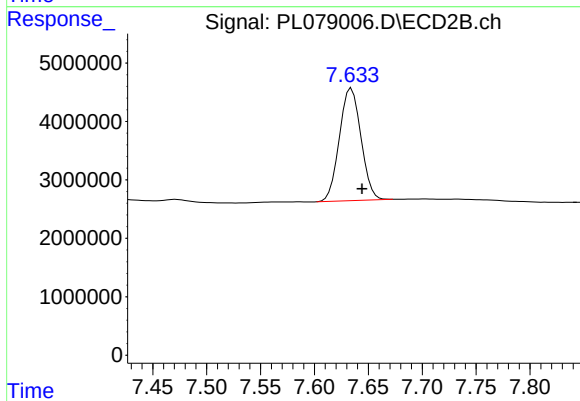

#28 Decachlorobiphenyl

R.T.: 7.634 min
Delta R.T.: -0.010 min
Response: 26845589
Conc: 14.17 ng/ml