

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111022\
 Data File : PL078999.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2022 15:07
 Operator : AR\AJ
 Sample : N5436-10DL 2X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 250FERRYBLVD-TFS-10DL

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/11/2022
 Supervised By :Ankita Jodhani 11/11/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 15:17:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.322	2.568	22983284	13229580	12.052	5.182 #
28) SA Decachlor...	8.771	7.635	138.8E6	170.1E6	92.256	89.812
Target Compounds						
13) MA Dieldrin	6.117	5.104	122.2E6	46117454	56.666	15.564m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111022\
Data File : PL078999.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2022 15:07
Operator : AR\AJ
Sample : N5436-10DL 2X
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-10DL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/11/2022
Supervised By :Ankita Jodhani 11/11/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 15:17:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

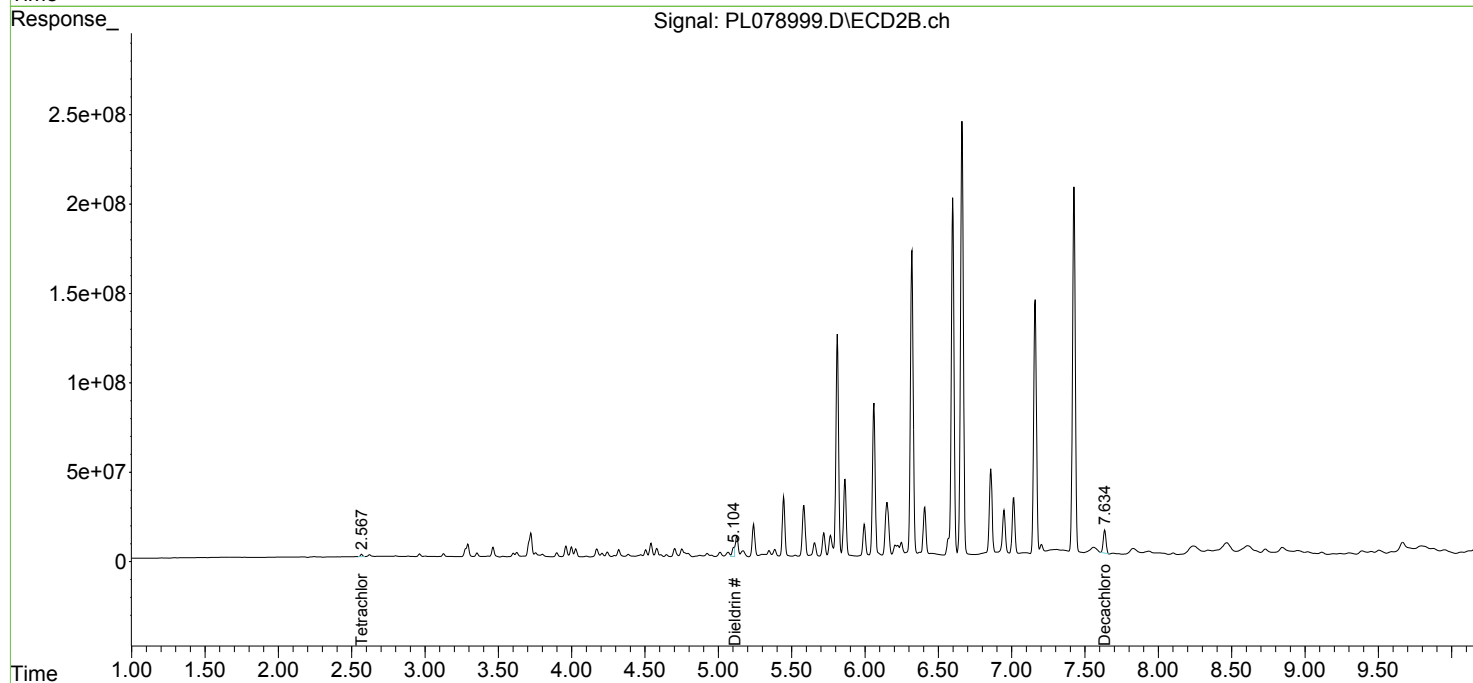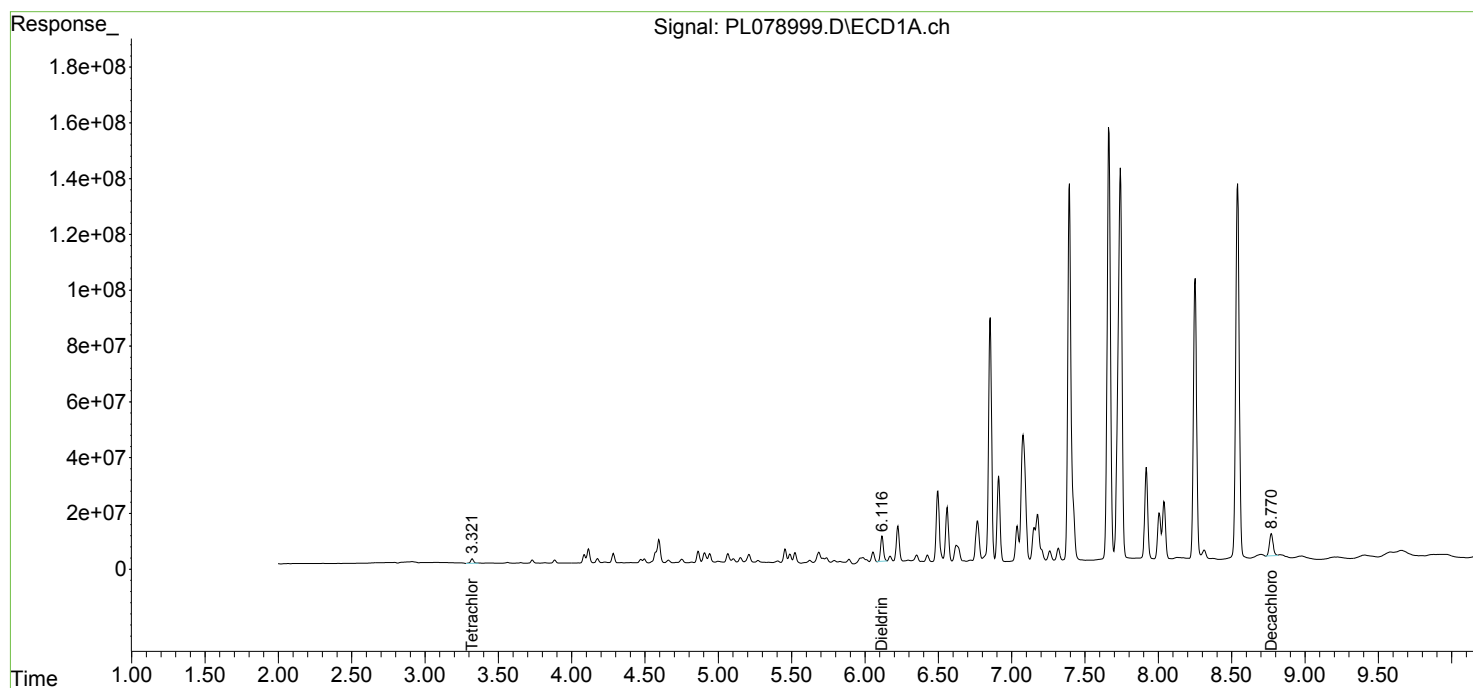

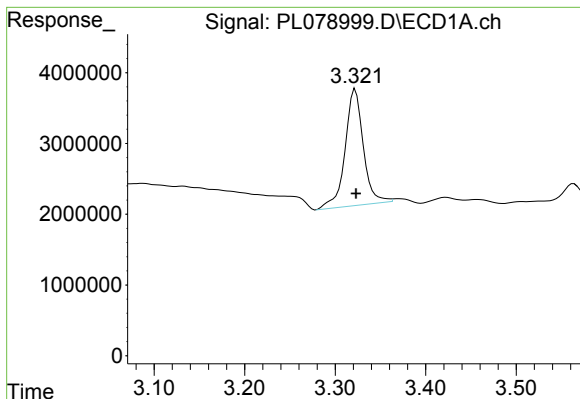


#1 Tetrachloro-m-xylene

R.T.: 3.322 min
Delta R.T.: 0.000 min
Response: 22983284
Conc: 12.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
250FERRYBLVD-TFS-10DL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/11/2022
Supervised By :Ankita Jodhani 11/11/2022

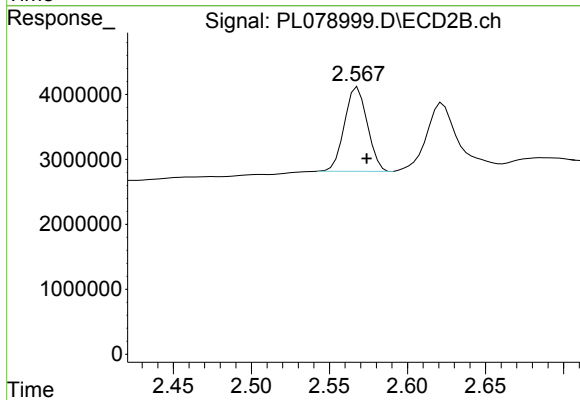


#1 Tetrachloro-m-xylene

R.T.: 2.568 min
Delta R.T.: -0.006 min
Response: 13229580
Conc: 5.18 ng/ml

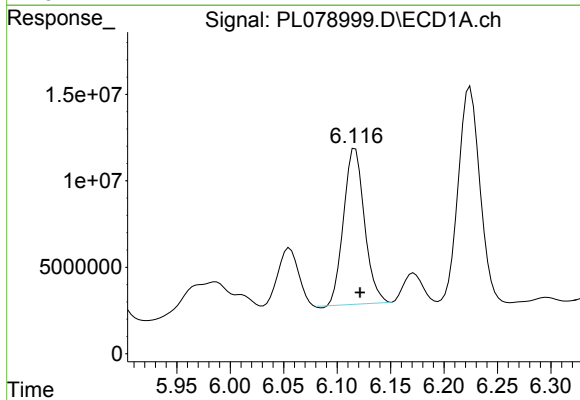


#13 Dieldrin

R.T.: 6.117 min
Delta R.T.: -0.004 min
Response: 122201276
Conc: 56.67 ng/ml

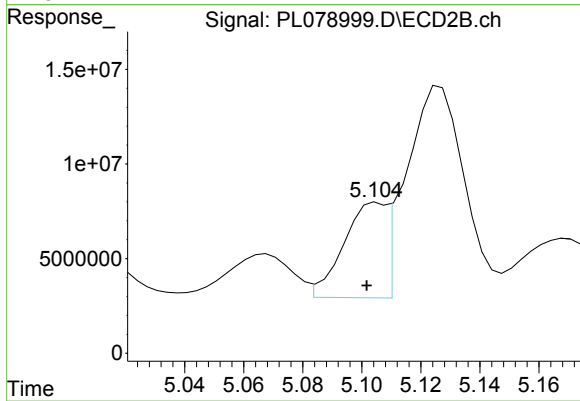

#13 Dieldrin

R.T.: 5.104 min
Delta R.T.: 0.002 min
Response: 46117454
Conc: 15.56 ng/ml m

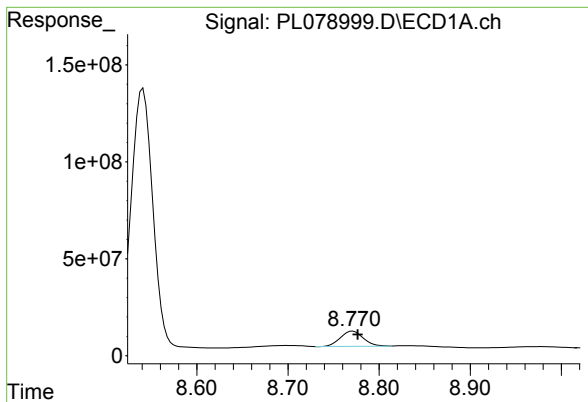

#28 Decachlorobiphenyl

R.T.: 8.771 min
Delta R.T.: -0.005 min
Response: 138785397
Conc: 92.26 ng/ml

Instrument :

ECD_L

ClientSampleId :


250FERRYBLVD-TFS-10DL

Manual Integrations

APPROVED

Reviewed By :Abdul Mirza 11/11/2022

Supervised By :Ankita Jodhani 11/11/2022

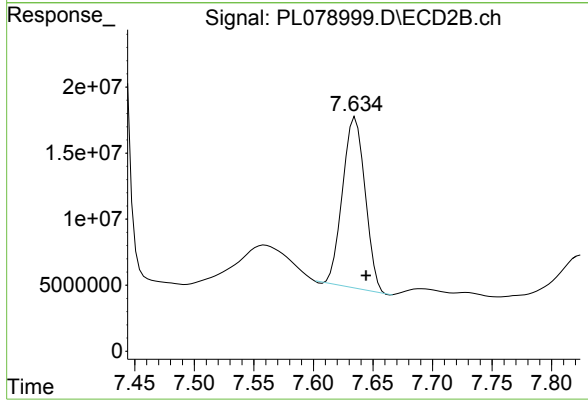

#28 Decachlorobiphenyl

R.T.: 7.635 min
Delta R.T.: -0.009 min
Response: 170112417
Conc: 89.81 ng/ml