

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111119\
 Data File : PL054163.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2019 13:49
 Operator : SG\AJ
 Sample : PB124671BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 00:24:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	4.043	214.9E6	48832957	19.829	19.515
28)	SA Decachlor...	8.323	9.122	175.3E6	49658873	17.868	17.634
Target Compounds							
16)	A 4,4'-DDD	6.260	0.000	1168895	0	0.131	N.D. #
23)	Chlordane-1	0.000	5.030	0	5720003	N.D.	68.203 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111119\
Data File : PL054163.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2019 13:49
Operator : SG\AJ
Sample : PB124671BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 00:24:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

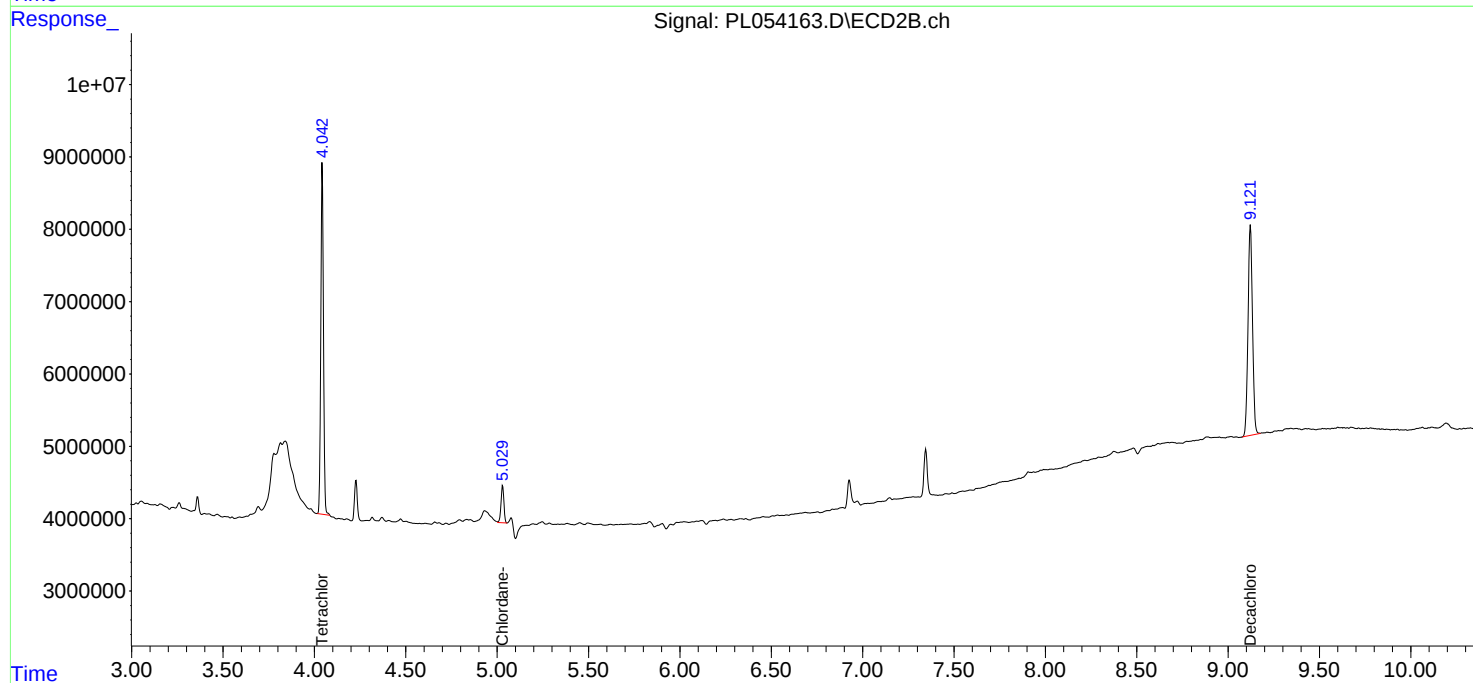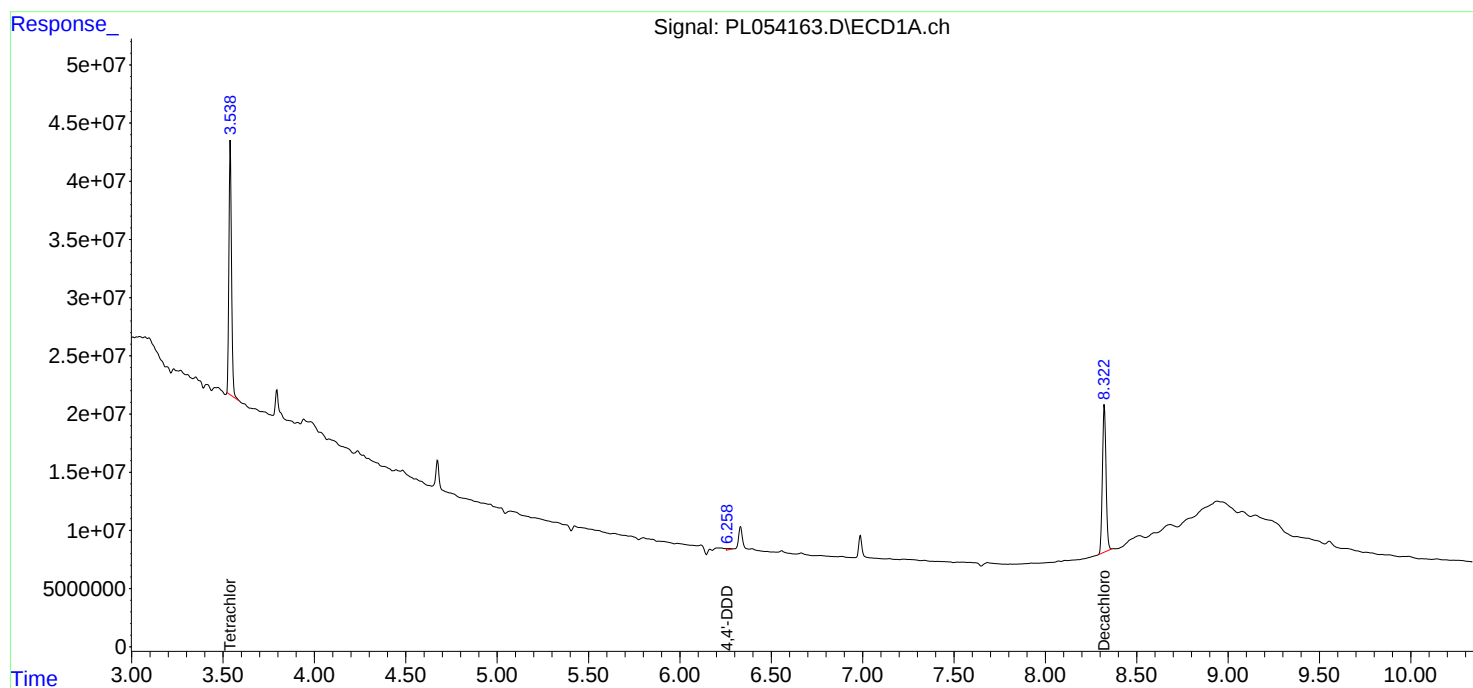


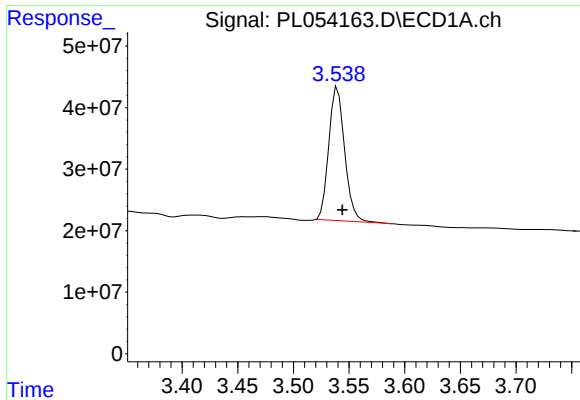

#1 Tetrachloro-m-xylene


R.T.: 3.540 min
Delta R.T.: -0.004 min
Response: 214936046
Conc: 19.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

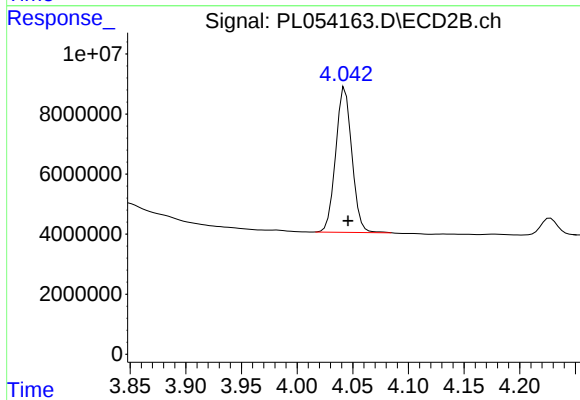


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: -0.003 min
Response: 48832957
Conc: 19.51 ng/ml

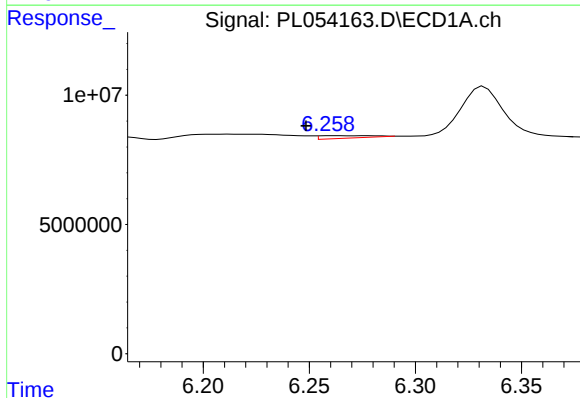


#16 4,4'-DDD

R.T.: 6.260 min
Delta R.T.: 0.012 min
Response: 1168895
Conc: 0.13 ng/ml

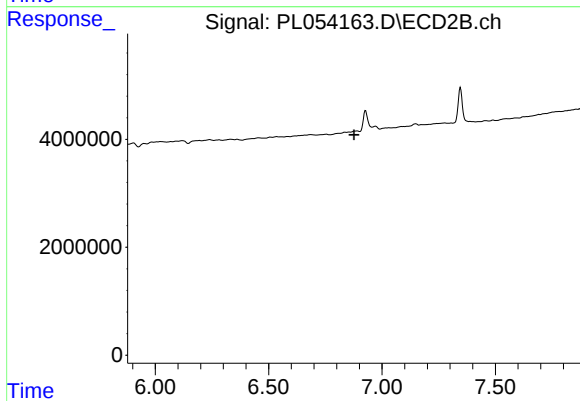

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.877 min
Response: 0
Conc: N.D.

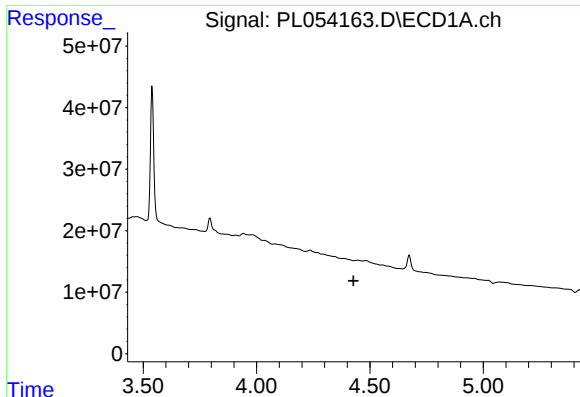

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.428 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

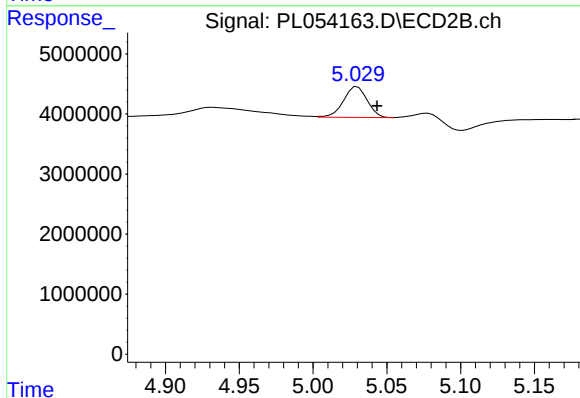


#23 Chlordane-1

R.T.: 5.030 min
Delta R.T.: -0.013 min
Response: 5720003
Conc: 68.20 ng/ml

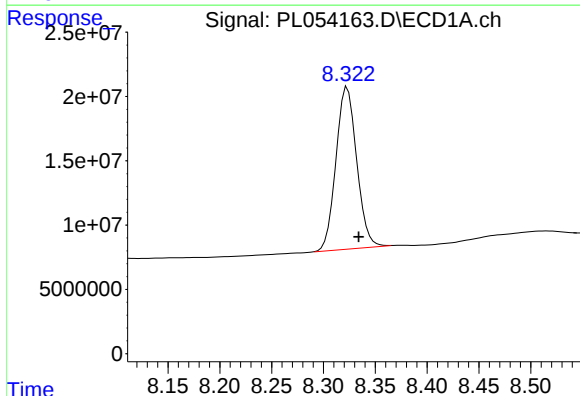

#28 Decachlorobiphenyl

R.T.: 8.323 min
Delta R.T.: -0.011 min
Response: 175316258
Conc: 17.87 ng/ml

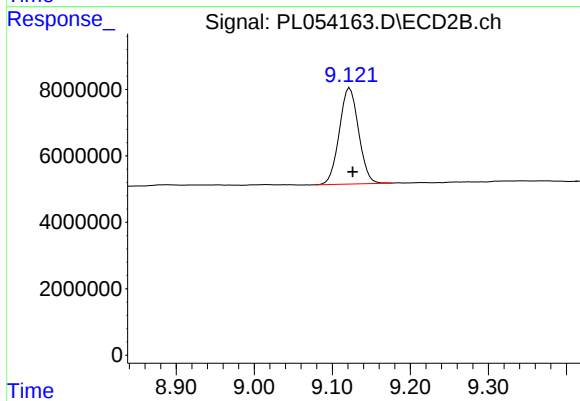

#28 Decachlorobiphenyl

R.T.: 9.122 min
Delta R.T.: -0.004 min
Response: 49658873
Conc: 17.63 ng/ml