

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111119\
 Data File : PL054172.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2019 16:00
 Operator : SG\AJ
 Sample : K5760-12
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 00:26:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	4.043	108.9E6	26686015	10.051	10.664
28)	SA Decachlor...	8.325	9.123	77340518	19790952	7.883	7.028
Target Compounds							
4)	MA Heptachlor	4.554f	0.000	2988629	0	0.189	N.D. #
6)	B beta-BHC	4.554f	0.000	2988629	0	0.454	N.D. #
10)	B gamma-Chl...	5.524f	0.000	3632369	0	0.266	N.D. #
12)	B 4,4'-DDE	5.725	0.000	1943893	0	0.164	N.D. #
22)	Mirex	7.465	0.000	21384956	0	2.500	N.D. #
25)	Chlordane-3	5.524f	0.000	3632369	0	3.151	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111119\
Data File : PL054172.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2019 16:00
Operator : SG\AJ
Sample : K5760-12
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 00:26:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

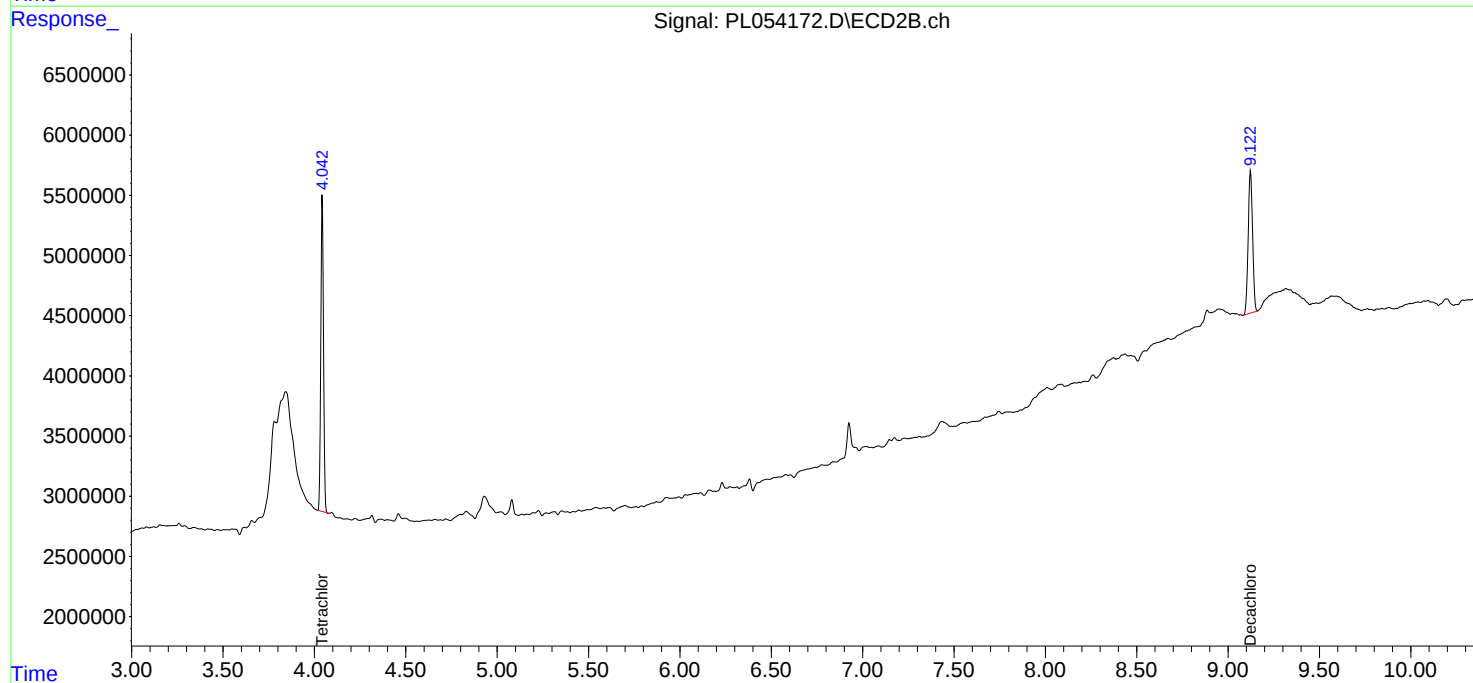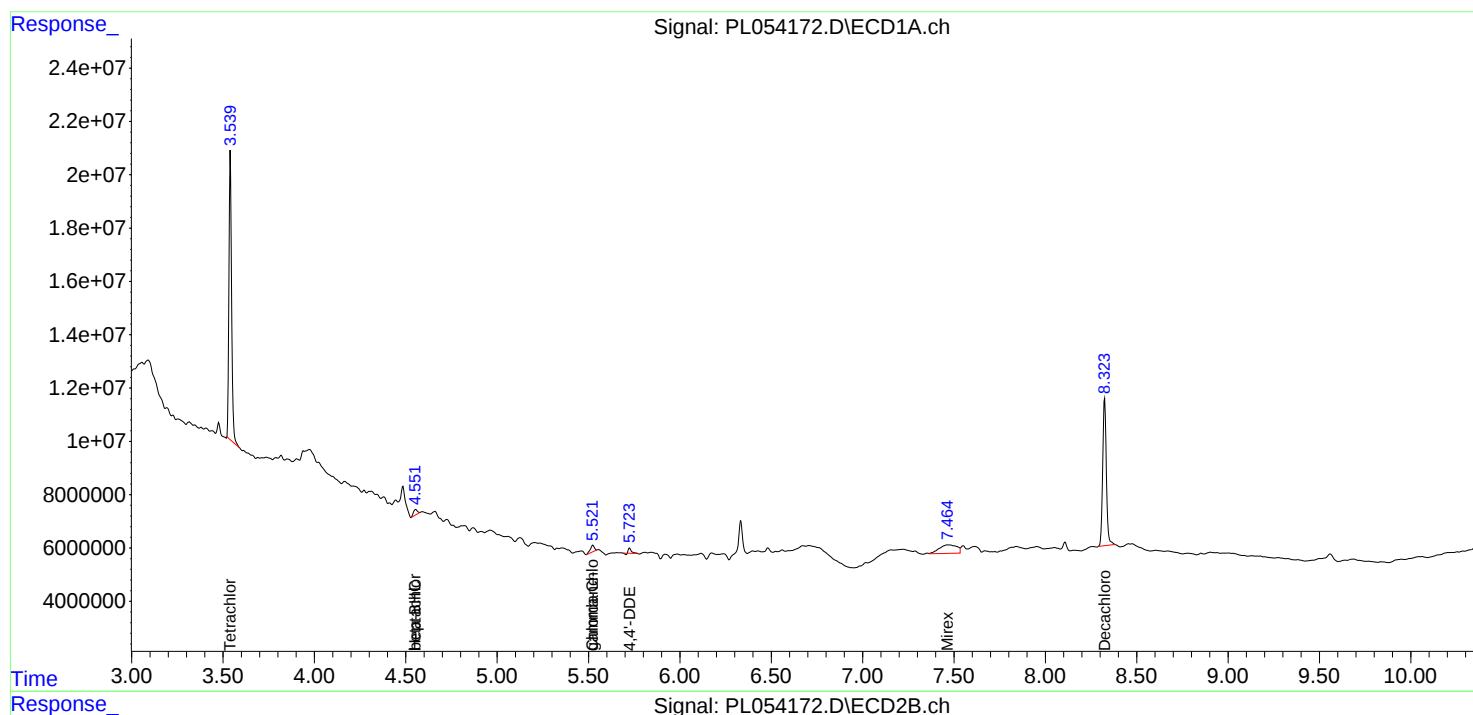


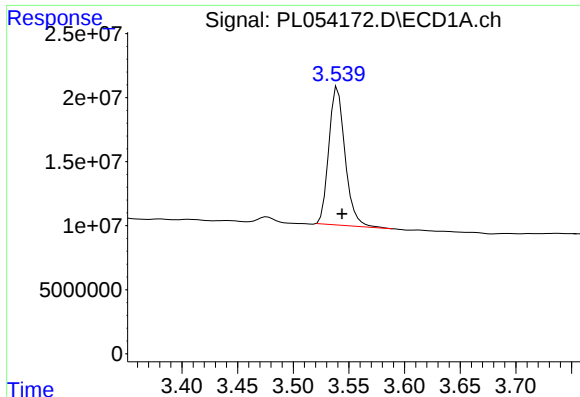

#1 Tetrachloro-m-xylene


R.T.: 3.540 min
Delta R.T.: -0.004 min
Response: 108946041
Conc: 10.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

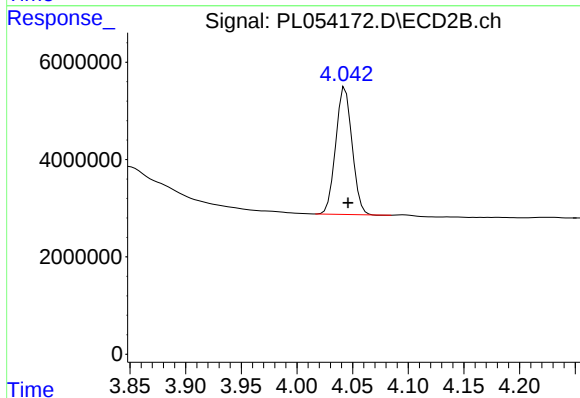


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: -0.003 min
Response: 26686015
Conc: 10.66 ng/ml

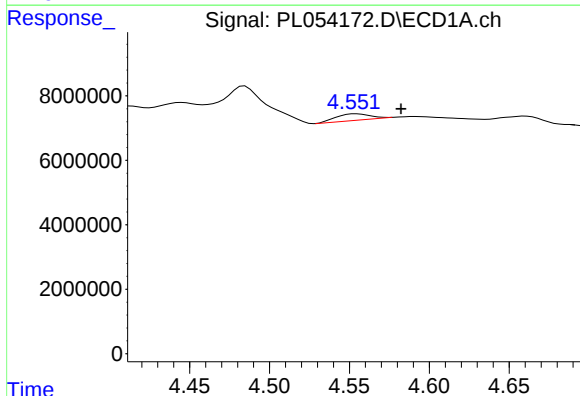


#4 Heptachlor

R.T.: 4.554 min
Delta R.T.: -0.028 min
Response: 2988629
Conc: 0.19 ng/ml

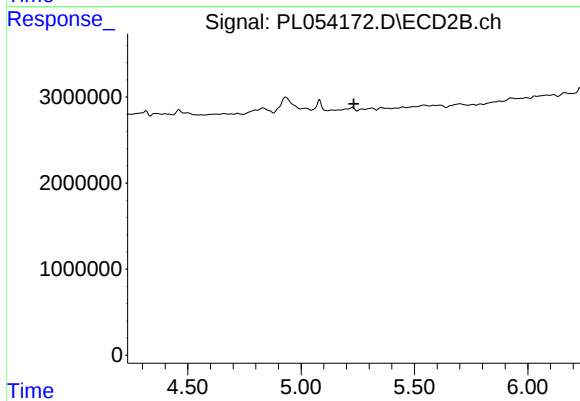

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.232 min
Response: 0
Conc: N.D.

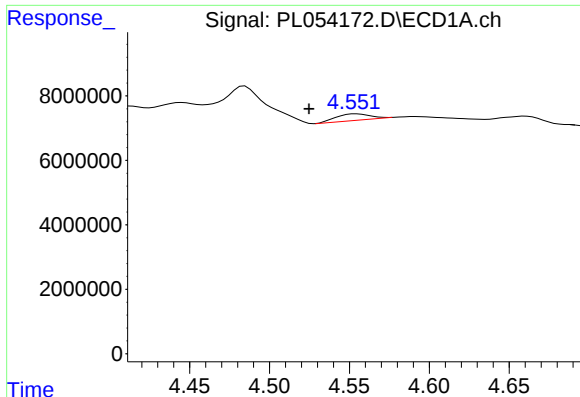

#6 beta-BHC


R.T.: 4.554 min
Delta R.T.: 0.030 min
Response: 2988629
Conc: 0.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

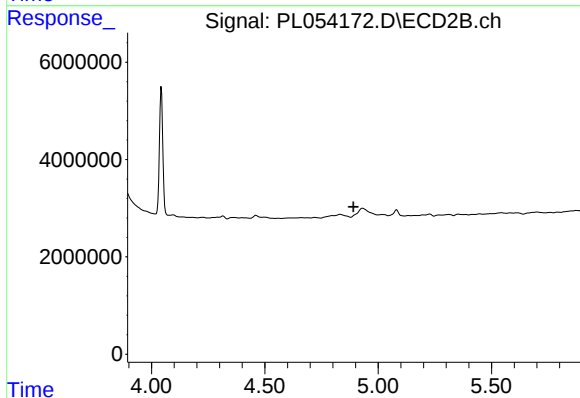


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.892 min
Response: 0
Conc: N.D.

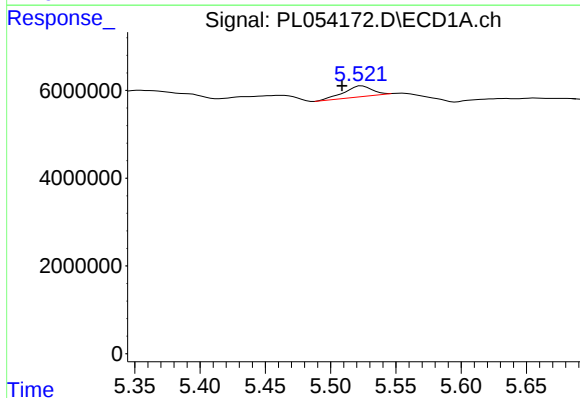


#10 gamma-Chlordane

R.T.: 5.524 min
Delta R.T.: 0.015 min
Response: 3632369
Conc: 0.27 ng/ml

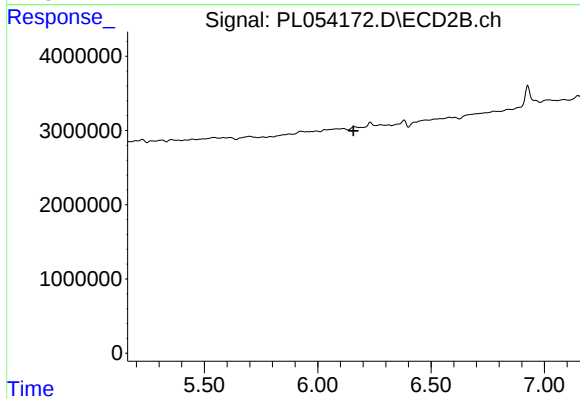

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.158 min
Response: 0
Conc: N.D.

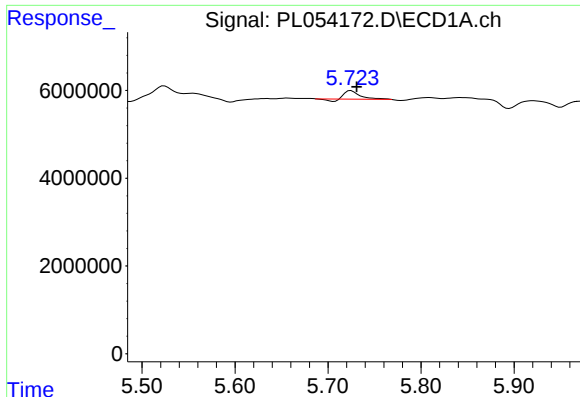

#12 4,4'-DDE


R.T.: 5.725 min
Delta R.T.: -0.006 min
Response: 1943893
Conc: 0.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

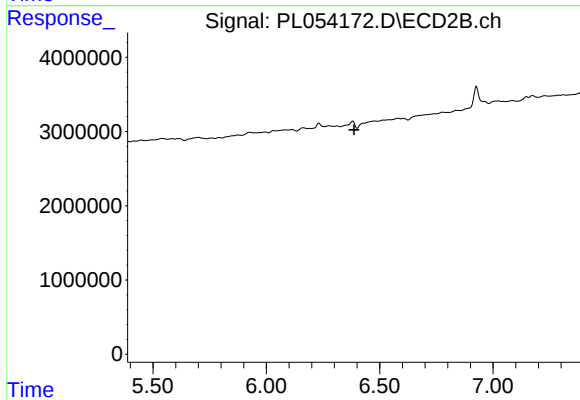


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.387 min
Response: 0
Conc: N.D.

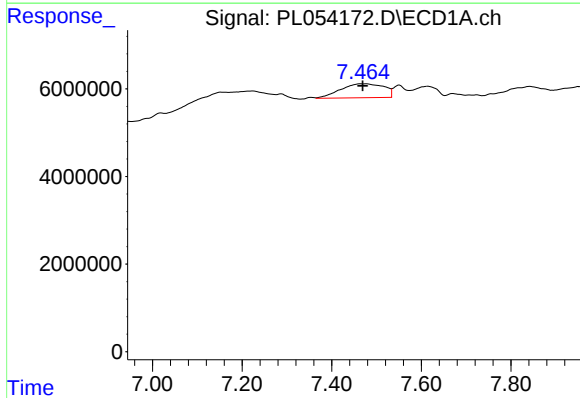


#22 Mirex

R.T.: 7.465 min
Delta R.T.: -0.004 min
Response: 21384956
Conc: 2.50 ng/ml

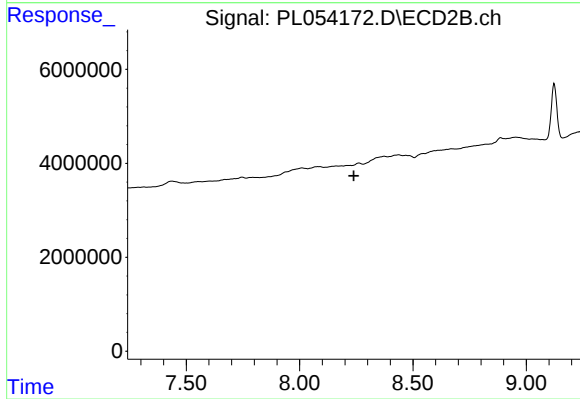

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 8.239 min
Response: 0
Conc: N.D.

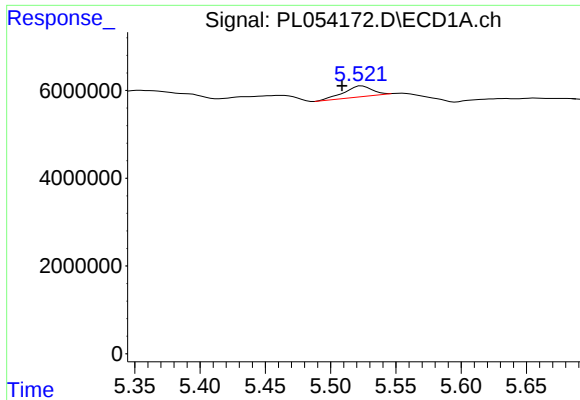

#25 Chlordane-3


R.T.: 5.524 min
Delta R.T.: 0.015 min
Response: 3632369
Conc: 3.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

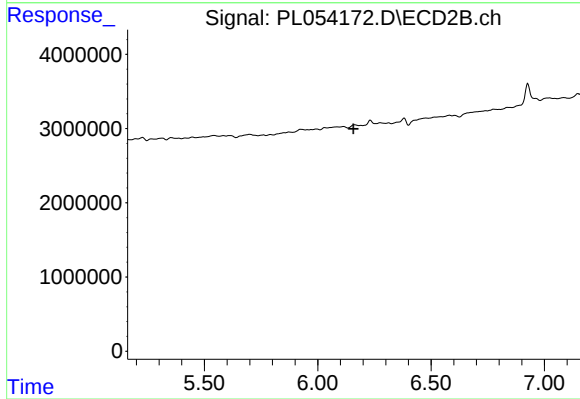


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.158 min
Response: 0
Conc: N.D.

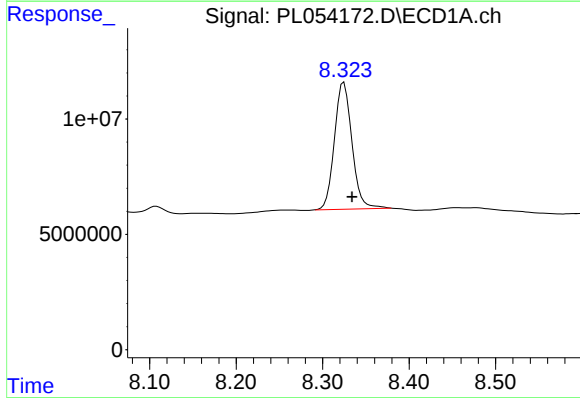

#28 Decachlorobiphenyl

R.T.: 8.325 min
Delta R.T.: -0.009 min
Response: 77340518
Conc: 7.88 ng/ml

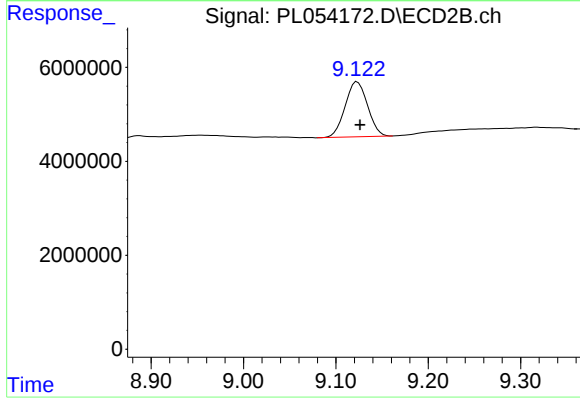

#28 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: -0.003 min
Response: 19790952
Conc: 7.03 ng/ml