

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111119\
 Data File : PL054156.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2019 11:38
 Operator : SG\AJ
 Sample : K5683-02 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OILY-WATER

Manual Integrations
 APPROVED

Ankita
 11/12/2019 10:54:49 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 11:52:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	4.038	27959000	2411860	2.579m	0.964m#
28)	SA Decachlor...	8.326	9.125	8648353	7481380	0.881m	2.657m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111119\
Data File : PL054156.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2019 11:38
Operator : SG\AJ
Sample : K5683-02 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
OILY-WATER


Manual Integrations
APPROVED

Ankita
11/12/2019 10:54:49 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 11:52:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

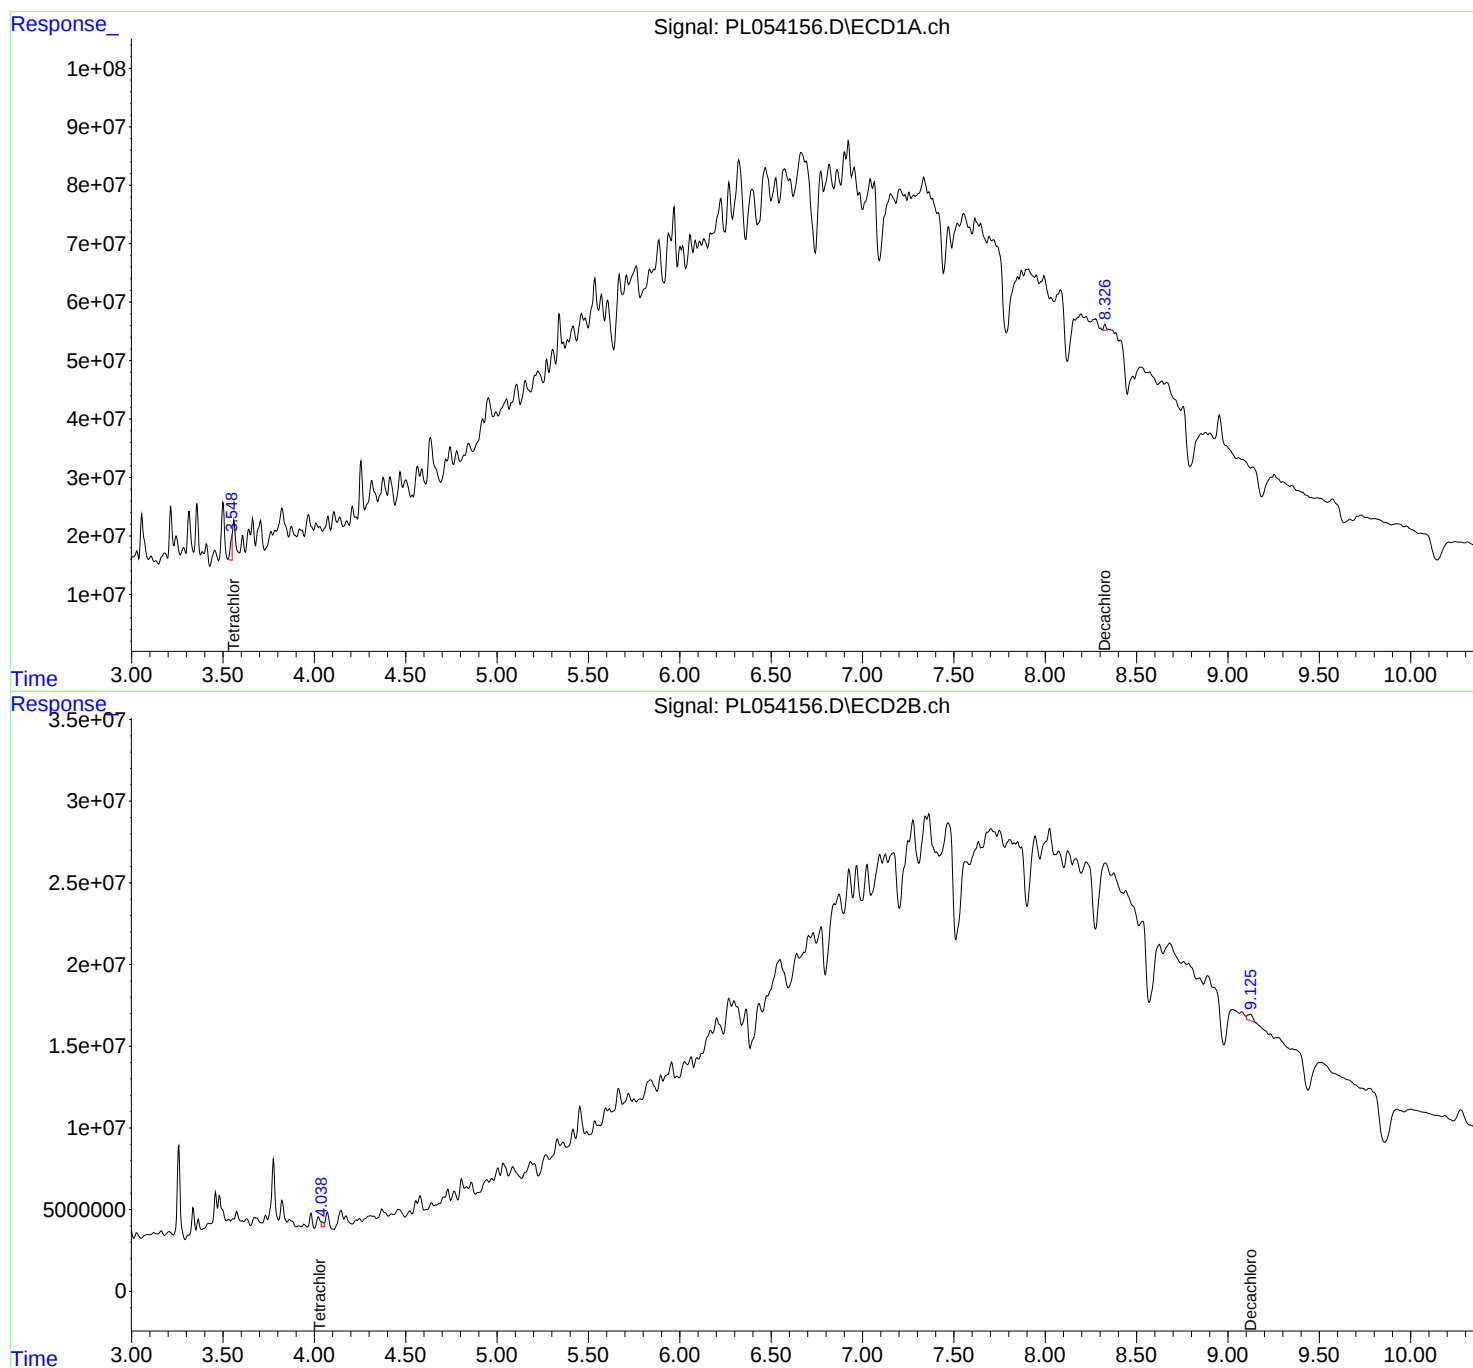

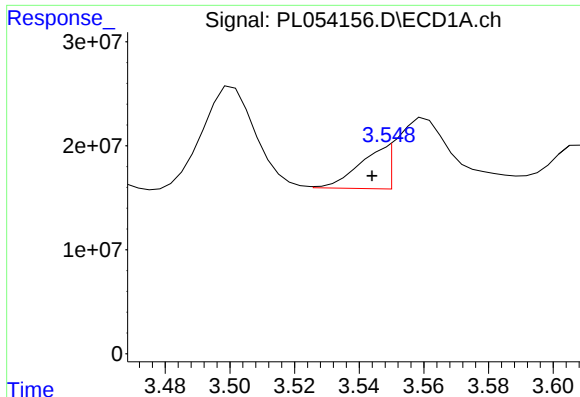


#1 Tetrachloro-m-xylene

R.T.: 3.548 min
Delta R.T.: 0.004 min
Response: 27959000
Conc: 2.58 ng/ml m

Instrument :
ECD_L
ClientSampleId :
OILY-WATER


Manual Integrations
APPROVED

Ankita
11/12/2019 10:54:49 AM

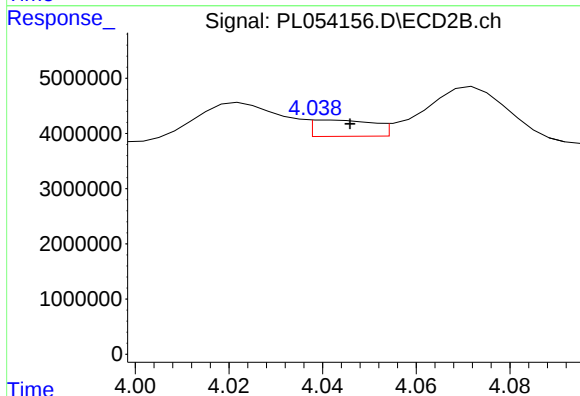


#1 Tetrachloro-m-xylene

R.T.: 4.038 min
Delta R.T.: -0.008 min
Response: 2411860
Conc: 0.96 ng/ml m

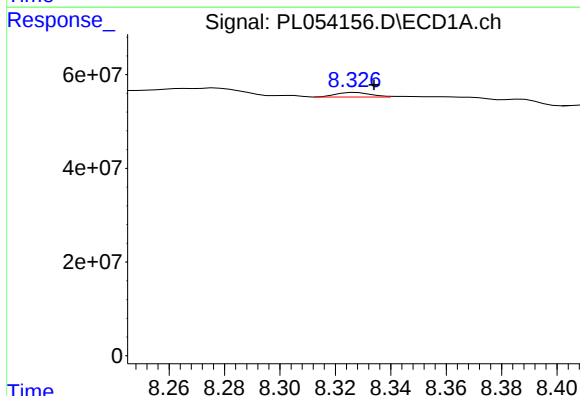

#28 Decachlorobiphenyl

R.T.: 8.326 min
Delta R.T.: -0.008 min
Response: 8648353
Conc: 0.88 ng/ml m

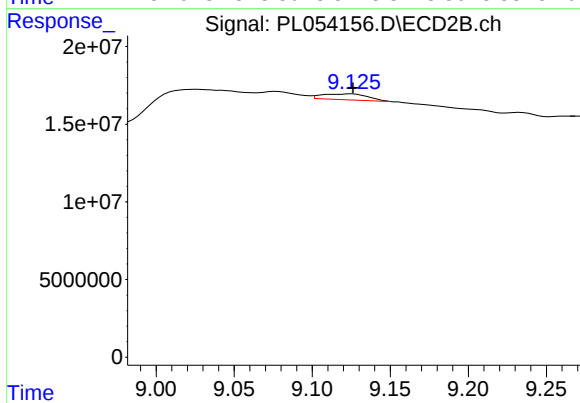

#28 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: -0.001 min
Response: 7481380
Conc: 2.66 ng/ml m