

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111119\
 Data File : PL054175.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2019 16:42
 Operator : SG\AJ
 Sample : K5763-11
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-34-D

Manual Integrations
 APPROVED

Ankita
 11/12/2019 10:55:10 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 00:27:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.540	4.043	209.5E6	50132999	19.329	20.034
28) SA Decachlor...	8.324	9.123	147.2E6	40973747	15.006	14.550
Target Compounds						
10) B gamma-Chl...	5.501	6.151	7413323	3391079	0.543m	1.162m#
11) B alpha-Chl...	5.558	6.229	9675470	2903683	0.727m	0.995 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111119\
Data File : PL054175.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2019 16:42
Operator : SG\AJ
Sample : K5763-11
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-34-D


Manual Integrations
APPROVED

Ankita
11/12/2019 10:55:10 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 00:27:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

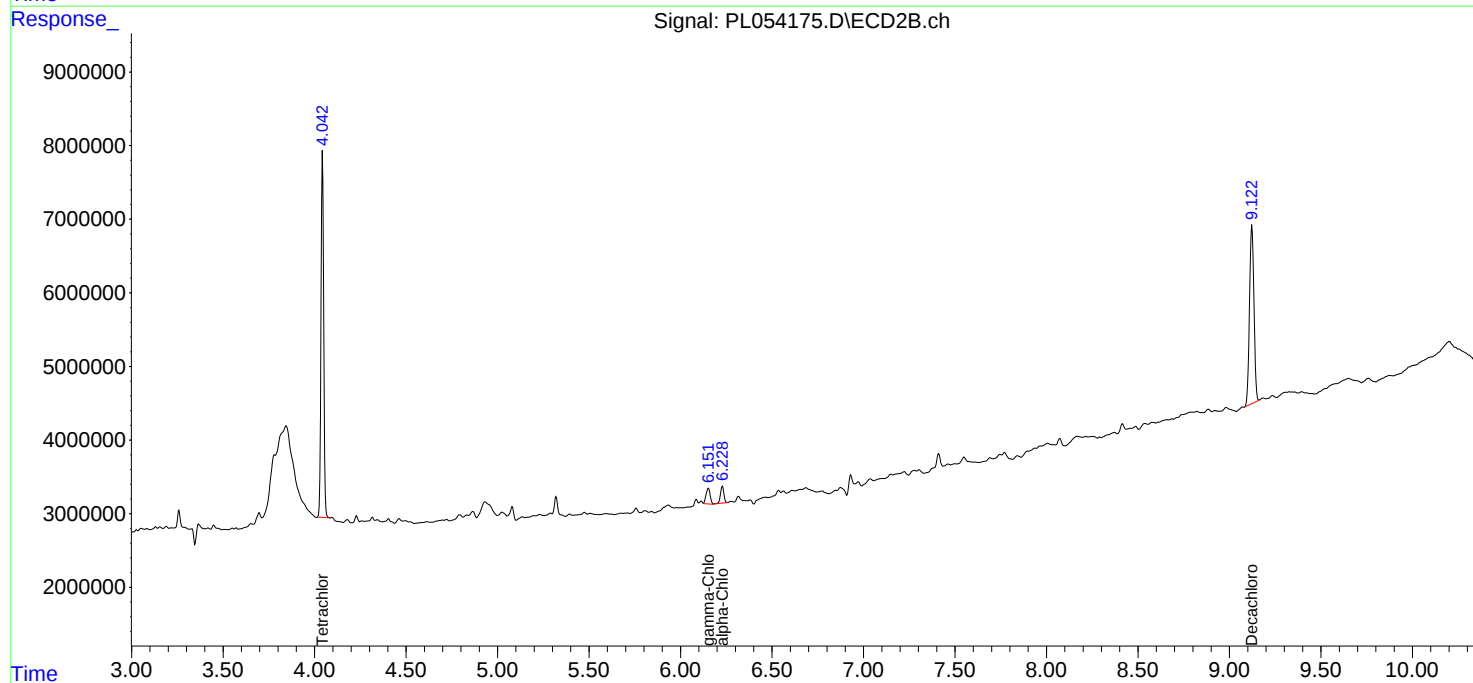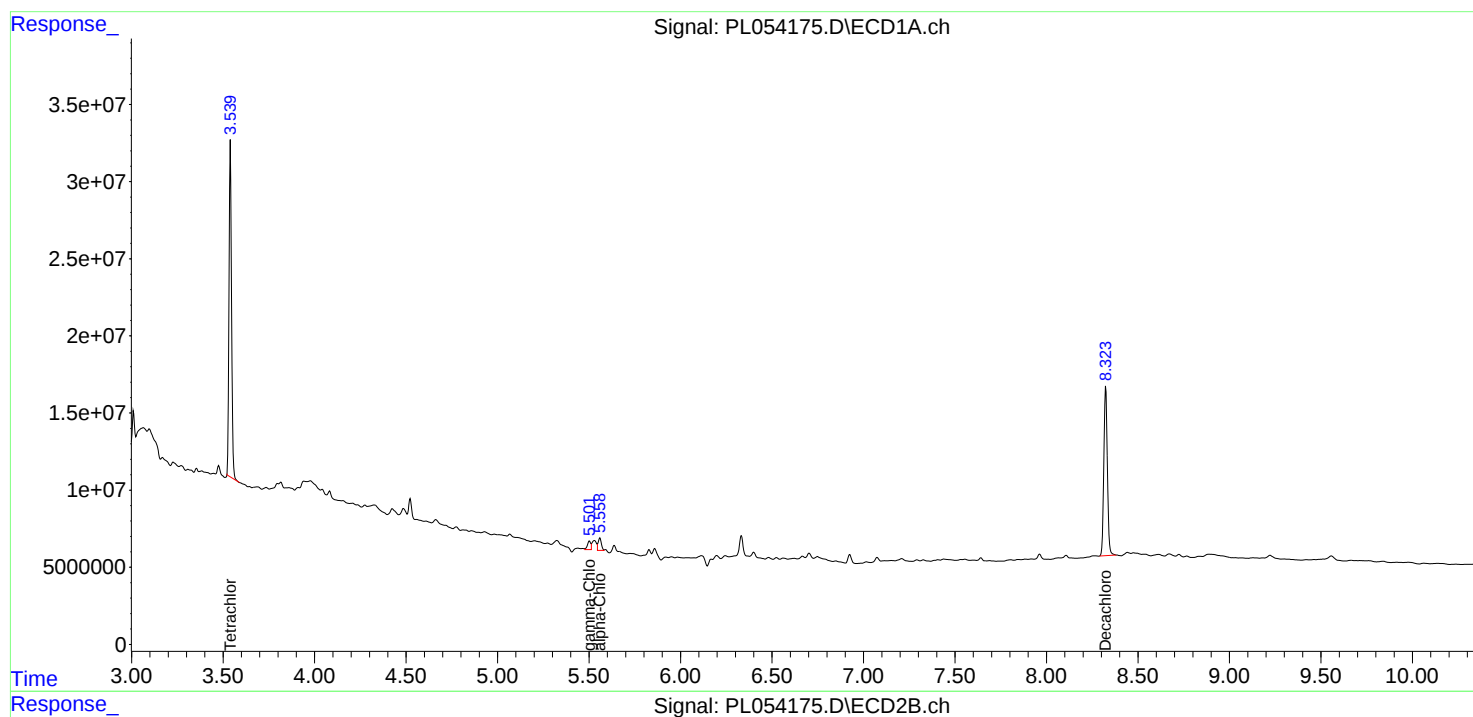

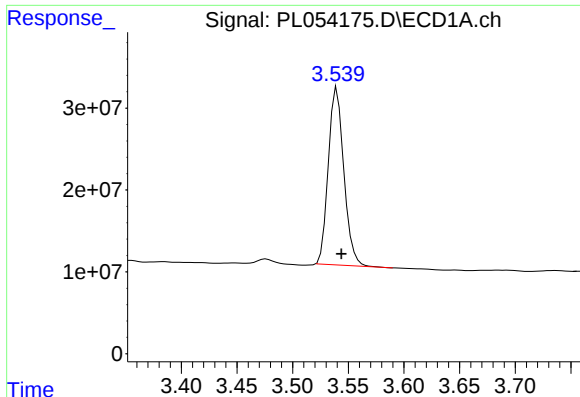


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: -0.004 min
Response: 209511969
Conc: 19.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-34-D


Manual Integrations
APPROVED

Ankita
11/12/2019 10:55:10 AM

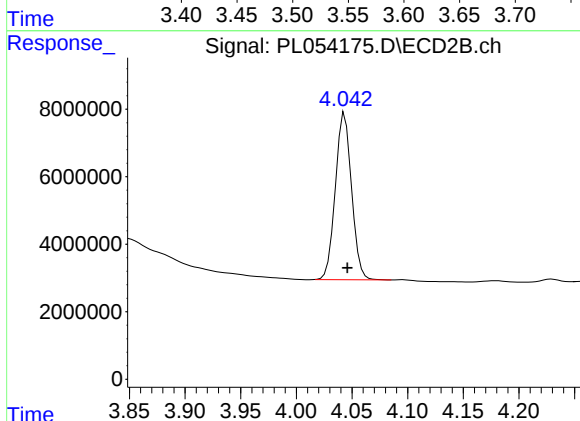


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: -0.002 min
Response: 50132999
Conc: 20.03 ng/ml

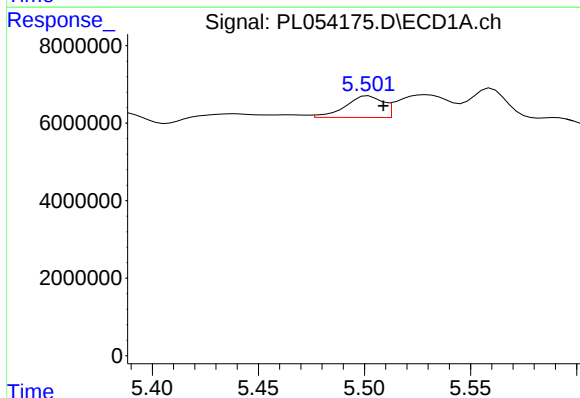


#10 gamma-Chlordane

R.T.: 5.501 min
Delta R.T.: -0.008 min
Response: 7413323
Conc: 0.54 ng/ml m

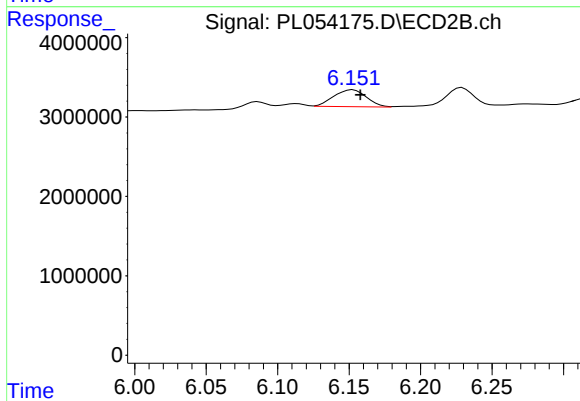

#10 gamma-Chlordane

R.T.: 6.151 min
Delta R.T.: -0.007 min
Response: 3391079
Conc: 1.16 ng/ml m

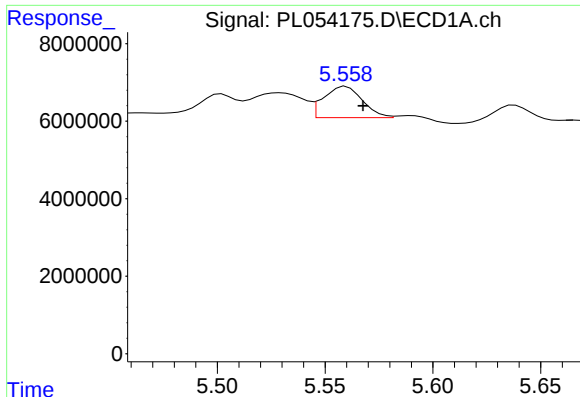


#11 alpha-Chlordane

R.T.: 5.558 min
Delta R.T.: -0.009 min
Response: 9675470
Conc: 0.73 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-34-D


Manual Integrations
APPROVED

Ankita
11/12/2019 10:55:10 AM

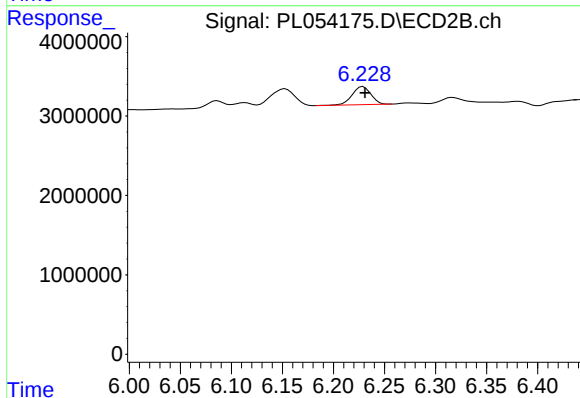


#11 alpha-Chlordane

R.T.: 6.229 min
Delta R.T.: -0.002 min
Response: 2903683
Conc: 0.99 ng/ml

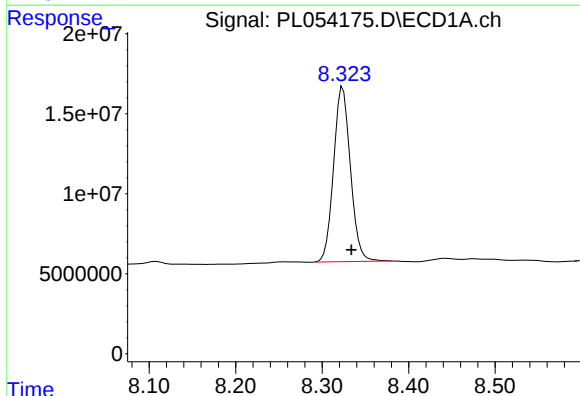

#28 Decachlorobiphenyl

R.T.: 8.324 min
Delta R.T.: -0.010 min
Response: 147234565
Conc: 15.01 ng/ml

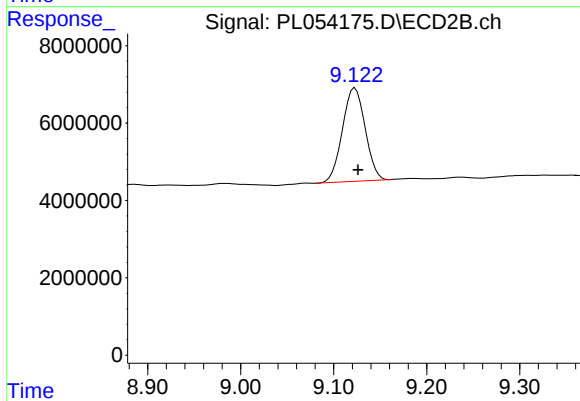

#28 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: -0.003 min
Response: 40973747
Conc: 14.55 ng/ml