

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111119\
 Data File : PL054176.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2019 16:56
 Operator : SG\AJ
 Sample : K5771-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SP

Manual Integrations
 APPROVED

Ankita
 11/12/2019 10:55:12 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 00:27:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	4.043	129.0E6	26188435	11.900m	10.465
28)	SA Decachlor...	8.324	9.123	102.1E6	28030604	10.405	9.954
Target Compounds							
12)	B 4,4'-DDE	5.722	6.379	8490522	2842263	0.715m	1.009m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111119\
Data File : PL054176.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2019 16:56
Operator : SG\AJ
Sample : K5771-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SP


Manual Integrations
APPROVED

Ankita
11/12/2019 10:55:12 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 00:27:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

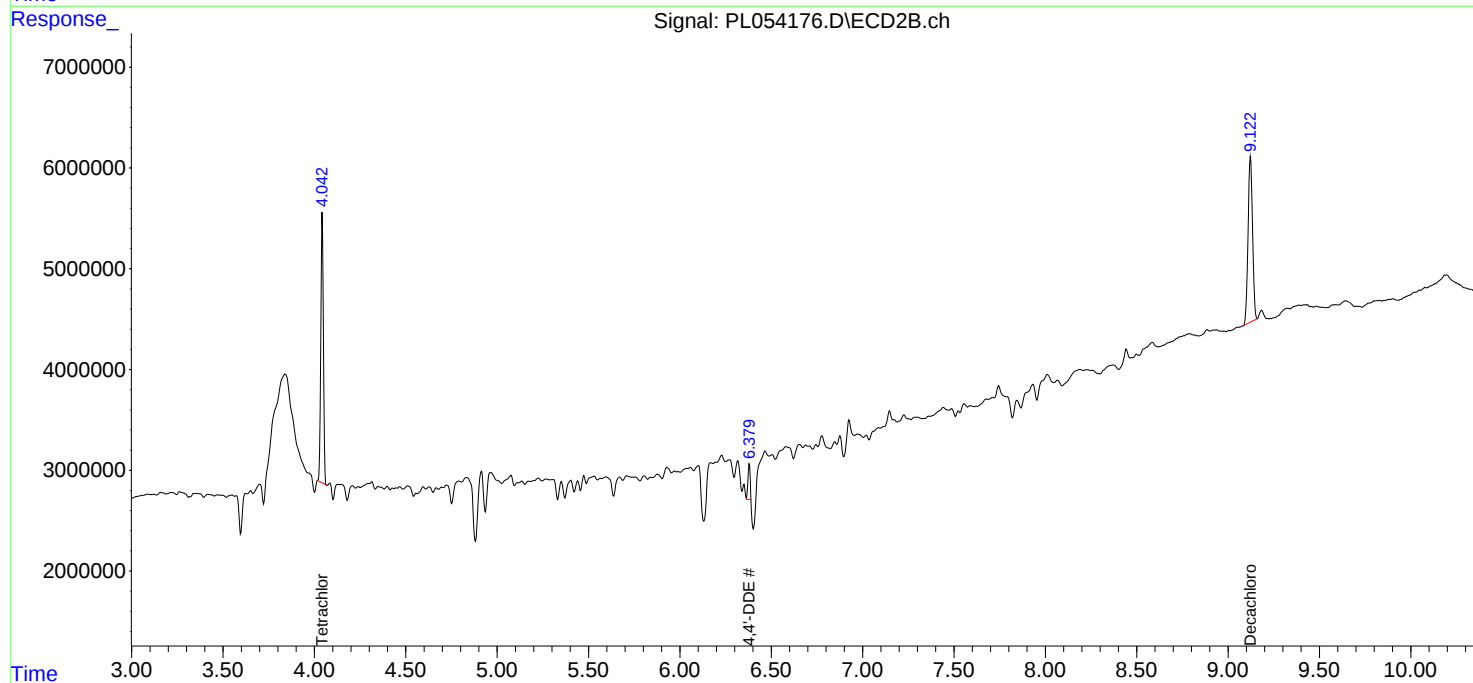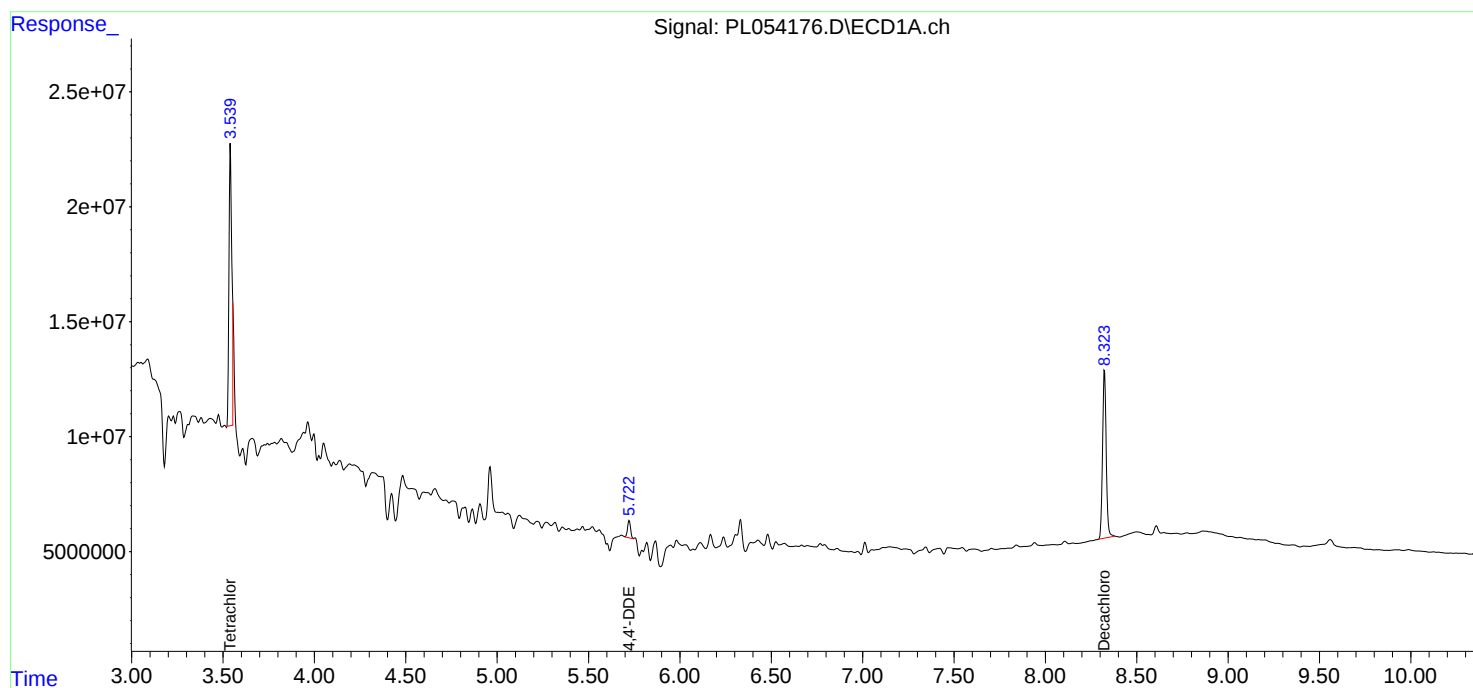

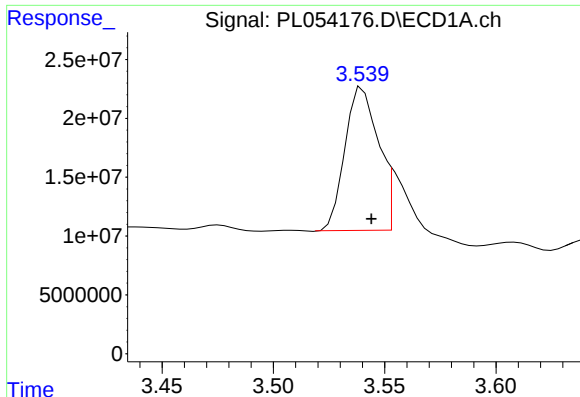


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: -0.005 min
Response: 128984514
Conc: 11.90 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SP


Manual Integrations
APPROVED

Ankita
11/12/2019 10:55:12 AM

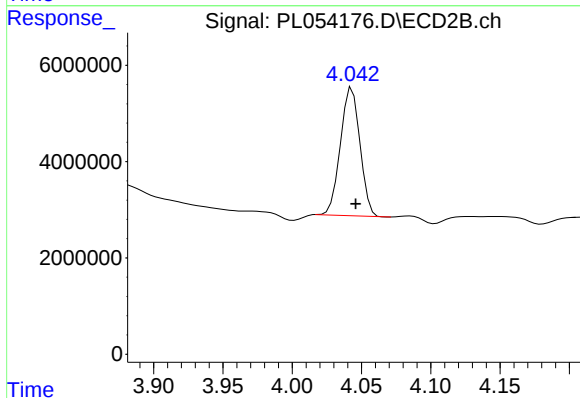


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: -0.003 min
Response: 26188435
Conc: 10.47 ng/ml

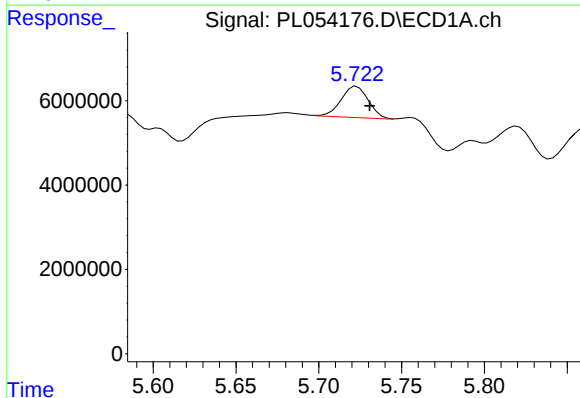


#12 4,4'-DDE

R.T.: 5.722 min
Delta R.T.: -0.009 min
Response: 8490522
Conc: 0.71 ng/ml m

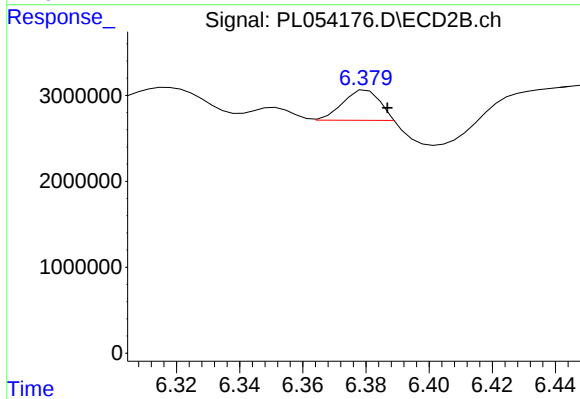

#12 4,4'-DDE

R.T.: 6.379 min
Delta R.T.: -0.008 min
Response: 2842263
Conc: 1.01 ng/ml m

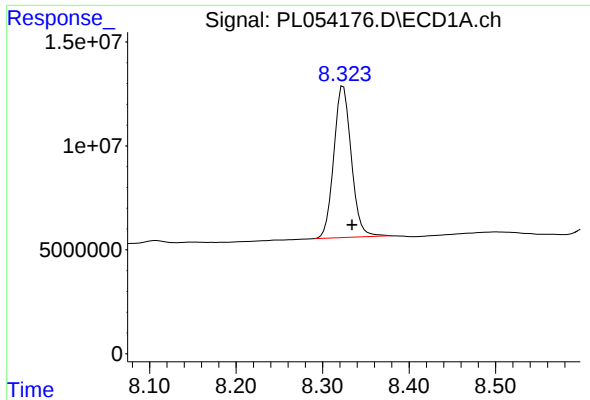


#28 Decachlorobiphenyl

R.T.: 8.324 min
Delta R.T.: -0.010 min
Response: 102087864
Conc: 10.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP

Manual Integrations
APPROVED

Ankita
11/12/2019 10:55:12 AM

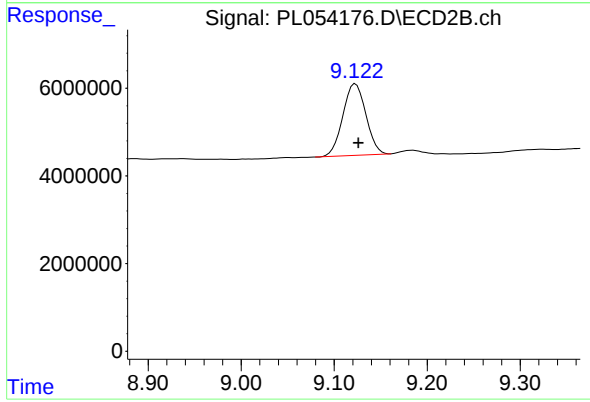

#28 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: -0.003 min
Response: 28030604
Conc: 9.95 ng/ml