

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111119\
 Data File : PL054177.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2019 17:10
 Operator : SG\AJ
 Sample : K5778-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-33-S

Manual Integrations
 APPROVED

Ankita
 11/12/2019 10:55:14 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 00:27:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	4.043	131.4E6	31674872	12.125	12.658
28)	SA Decachlor...	8.324	9.124	104.0E6	29087466	10.595	10.329
Target Compounds							
20)	A Methoxychlor	7.026	7.632	3501383	951967	0.710m	0.733m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111119\
Data File : PL054177.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2019 17:10
Operator : SG\AJ
Sample : K5778-03
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TP-33-S


Manual Integrations
APPROVED

Ankita
11/12/2019 10:55:14 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 00:27:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

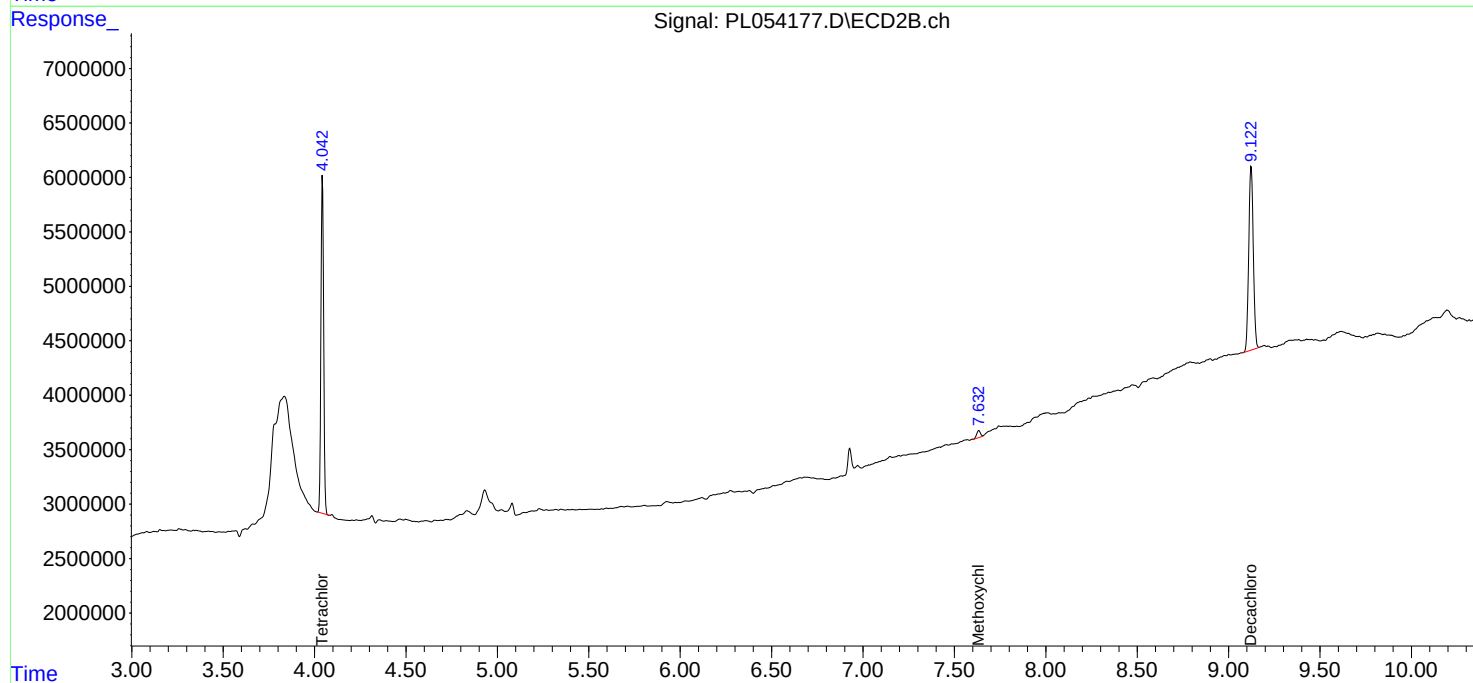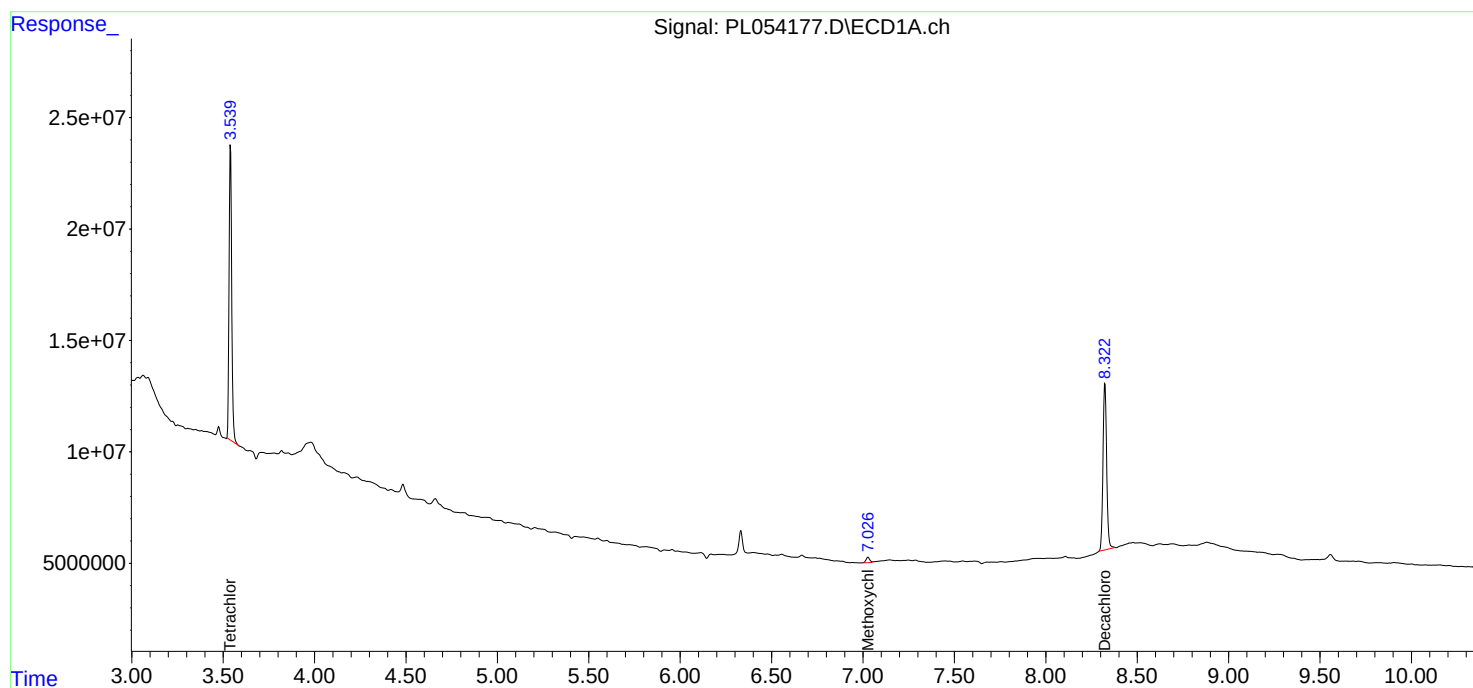

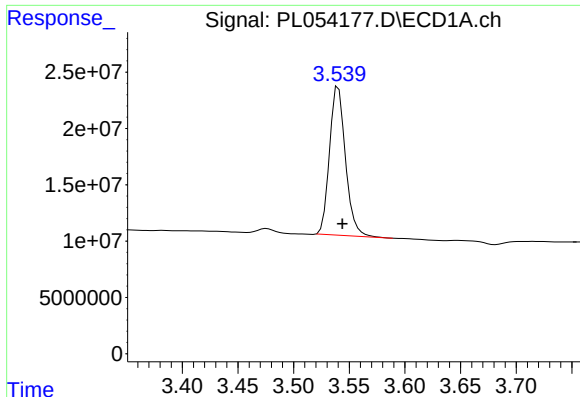


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: -0.004 min
Response: 131431900
Conc: 12.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-33-S


Manual Integrations
APPROVED

Ankita
11/12/2019 10:55:14 AM

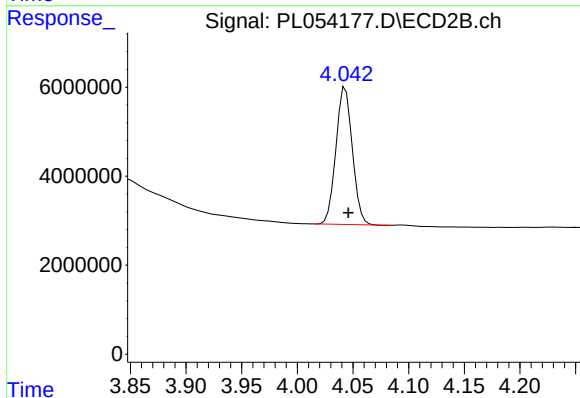


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: -0.003 min
Response: 31674872
Conc: 12.66 ng/ml

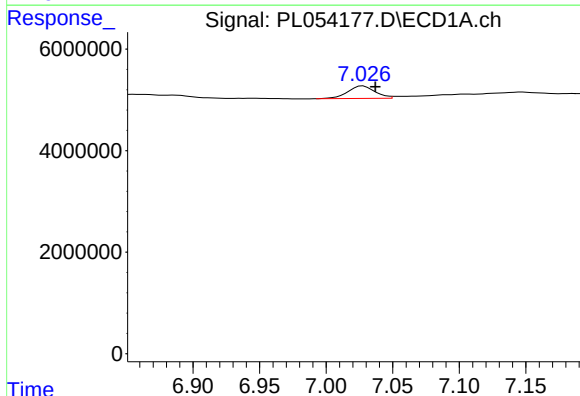


#20 Methoxychlor

R.T.: 7.026 min
Delta R.T.: -0.011 min
Response: 3501383
Conc: 0.71 ng/ml m

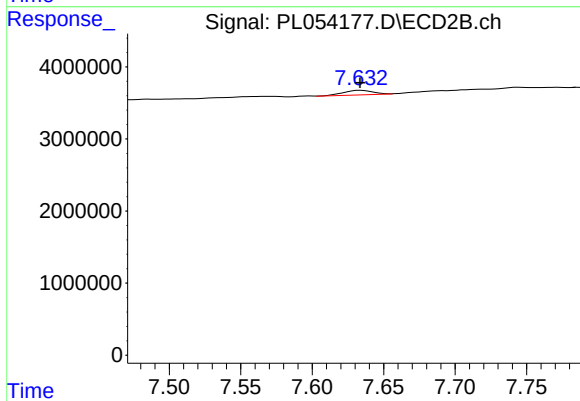

#20 Methoxychlor

R.T.: 7.632 min
Delta R.T.: 0.000 min
Response: 951967
Conc: 0.73 ng/ml m

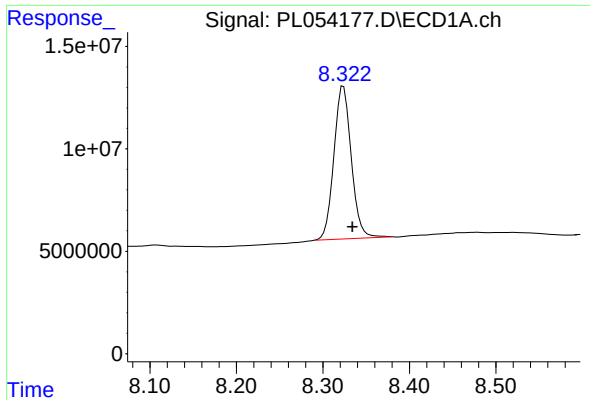


#28 Decachlorobiphenyl

R.T.: 8.324 min
Delta R.T.: -0.010 min
Response: 103955982
Conc: 10.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-33-S

Manual Integrations
APPROVED

Ankita
11/12/2019 10:55:14 AM

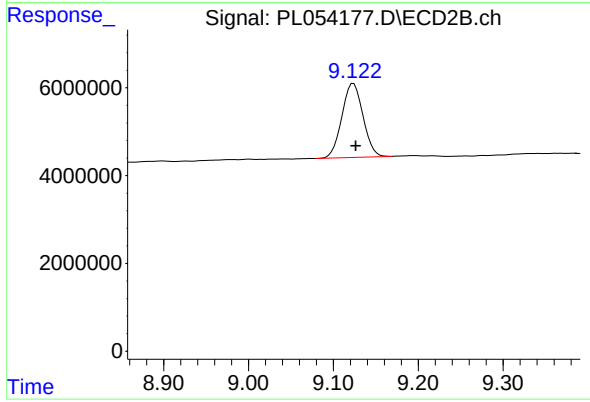

#28 Decachlorobiphenyl

R.T.: 9.124 min
Delta R.T.: -0.003 min
Response: 29087466
Conc: 10.33 ng/ml