

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111120\
 Data File : PL062944.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2020 14:06
 Operator : DD\AJ
 Sample : L4697-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-2-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 00:40:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.412	3.951	46431985	83224957	26.994	28.320
28) SA	Decachlor...	8.127	8.991	34842230	44472773	21.718	21.249
Target Compounds							
7) B	delta-BHC	0.000	5.004	0	2732015	N.D.	0.781 #
8) B	Heptachlo...	0.000	5.827	0	2825922	N.D.	0.873 #
15) B	Endosulfa...	0.000	6.869f	0	2403927	N.D.	0.841 #
23)	Chlordane-1	4.269	0.000	134216	0	2.604	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111120\
Data File : PL062944.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2020 14:06
Operator : DD\AJ
Sample : L4697-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-2-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 00:40:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

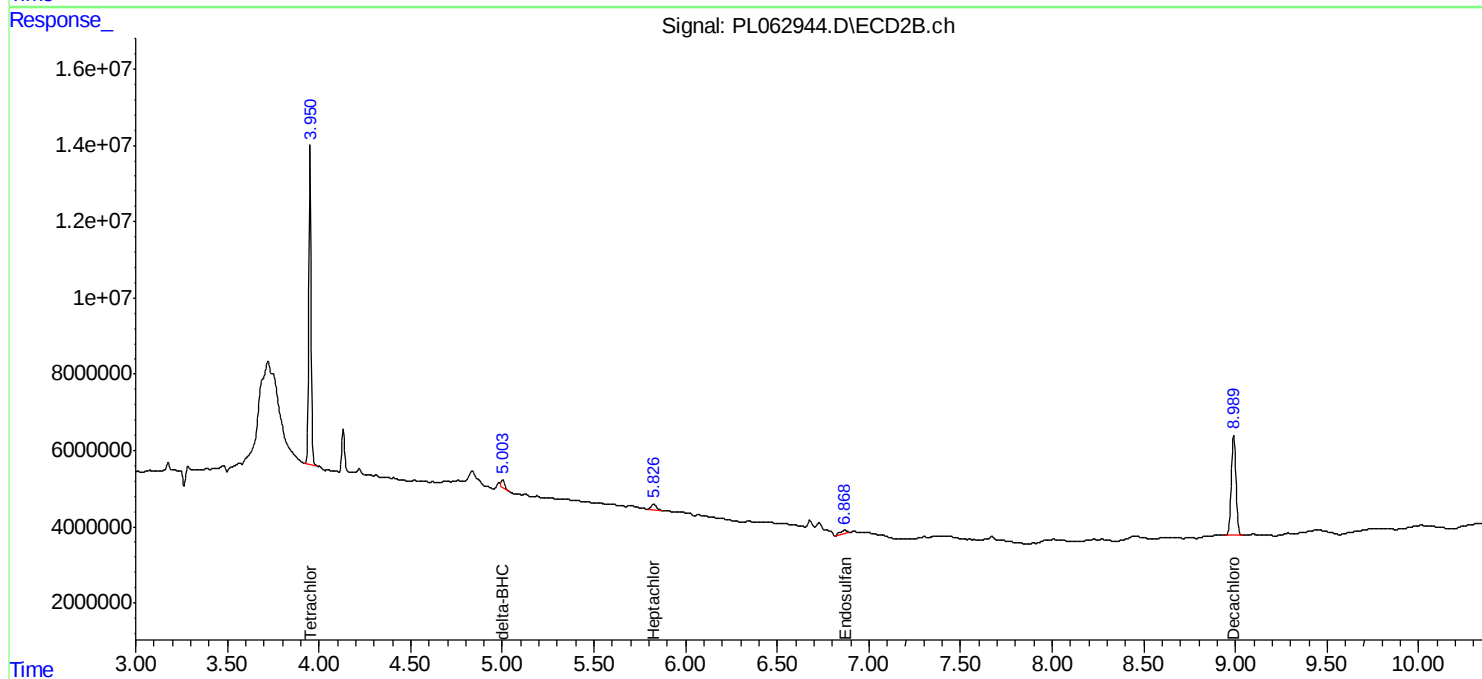


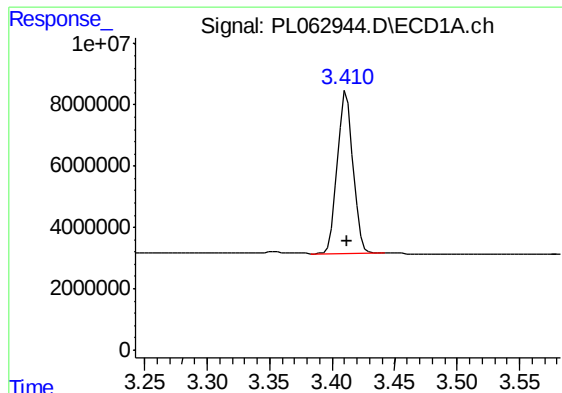

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 46431985
Conc: 26.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2-D

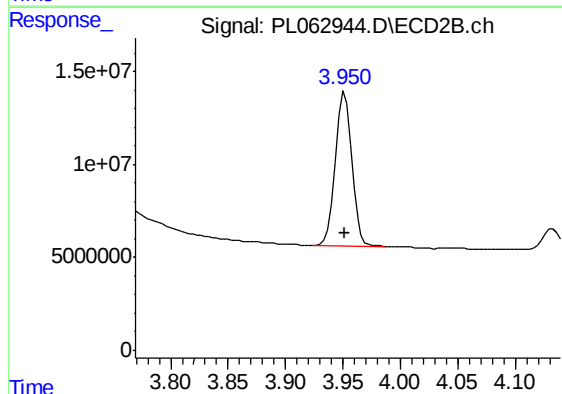


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 83224957
Conc: 28.32 ng/ml

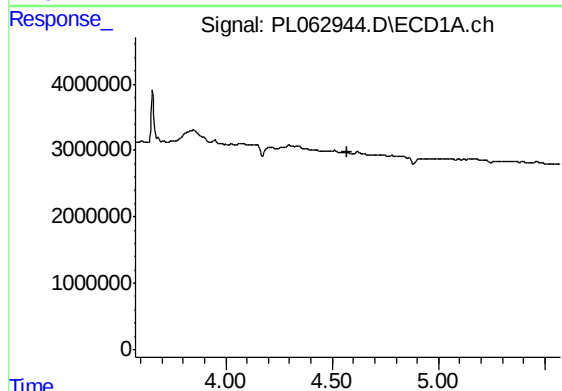


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.573 min
Response: 0
Conc: N.D.

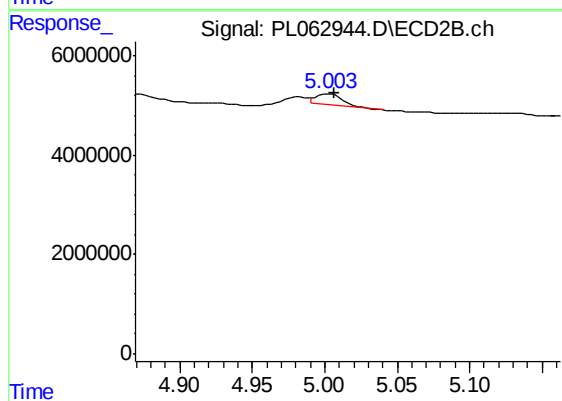

#7 delta-BHC


R.T.: 5.004 min
Delta R.T.: -0.003 min
Response: 2732015
Conc: 0.78 ng/ml

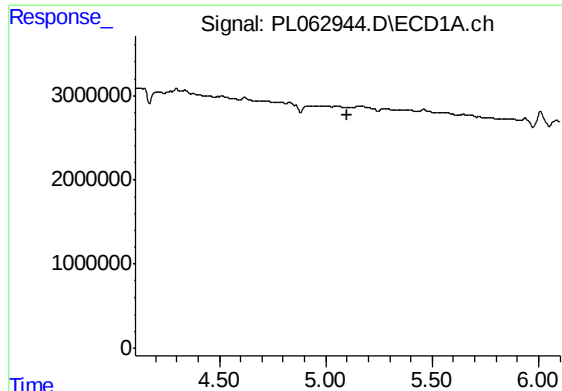

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.103 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-2-D

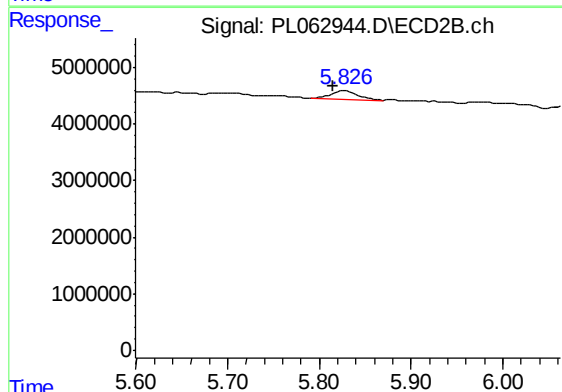


#8 Heptachlor epoxide

R.T.: 5.827 min
Delta R.T.: 0.012 min
Response: 2825922
Conc: 0.87 ng/ml

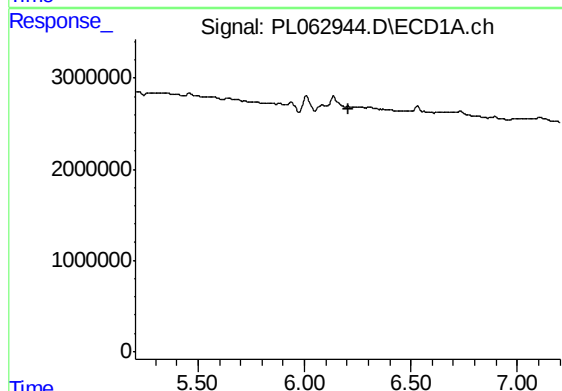


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.205 min
Response: 0
Conc: N.D.

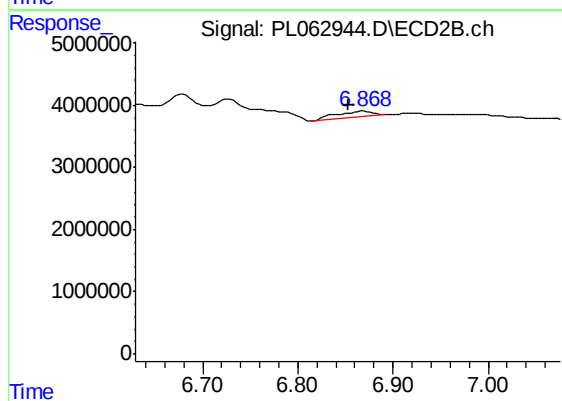

#15 Endosulfan II


R.T.: 6.869 min
Delta R.T.: 0.016 min
Response: 2403927
Conc: 0.84 ng/ml

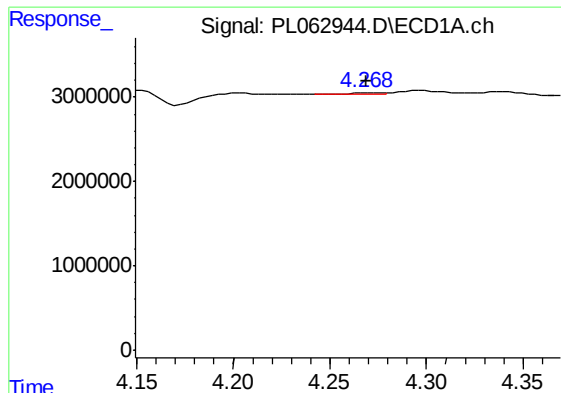

#23 Chlordane-1


R.T.: 4.269 min
Delta R.T.: 0.000 min
Response: 134216
Conc: 2.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2-D

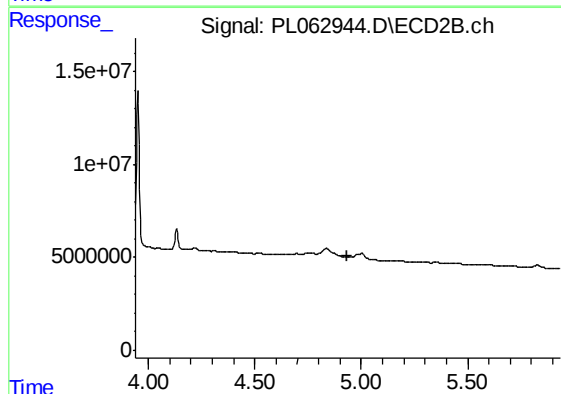


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.938 min
Response: 0
Conc: N.D.

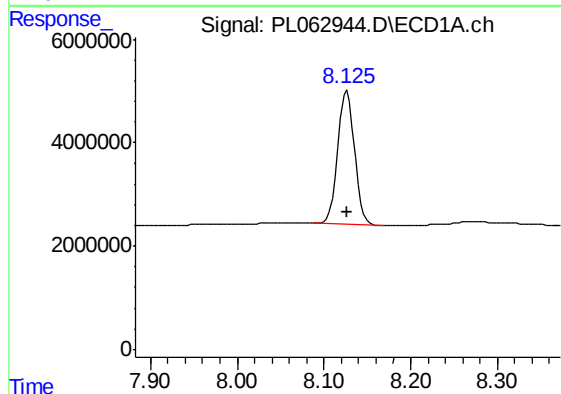

#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.000 min
Response: 34842230
Conc: 21.72 ng/ml

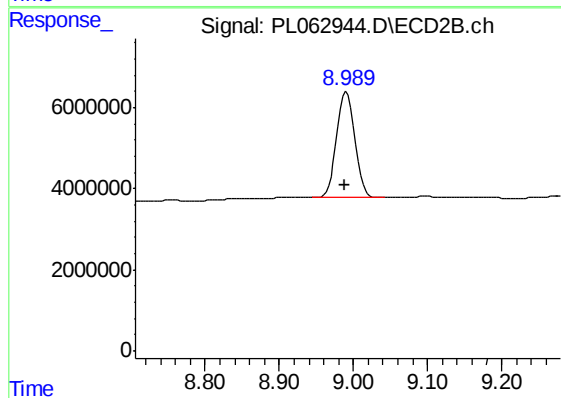

#28 Decachlorobiphenyl

R.T.: 8.991 min
Delta R.T.: 0.002 min
Response: 44472773
Conc: 21.25 ng/ml