

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111121\
 Data File : PL070930.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2021 16:23
 Operator : AR\AJ
 Sample : M4625-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 03:32:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 19:28:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.567	5.501	6269555	16602900	12.800	13.168
28)	SA Decachlor...	10.329	11.390	8936601	17631073	13.079	13.183
Target Compounds							
6)	B beta-BHC	0.000	6.733	0	1406263	N.D.	1.641 #
10)	B gamma-Chl...	0.000	8.227	0	557512	N.D.	0.360 #
11)	B alpha-Chl...	0.000	8.308	0	1860174	N.D.	1.223 #
14)	MA Endrin	0.000	8.920f	0	811098	N.D.	0.700 #
17)	MA 4,4'-DDT	0.000	9.384f	0	955717	N.D.	0.758 #
21)	B Endrin ke...	0.000	10.015f	0	397366	N.D.	0.277 #
25)	Chlordane-3	0.000	8.227	0	557512	N.D.	2.758 #
26)	Chlordane-4	0.000	8.308	0	1860174	N.D.	7.665 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111121\
Data File : PL070930.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2021 16:23
Operator : AR\AJ
Sample : M4625-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 03:32:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 19:28:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

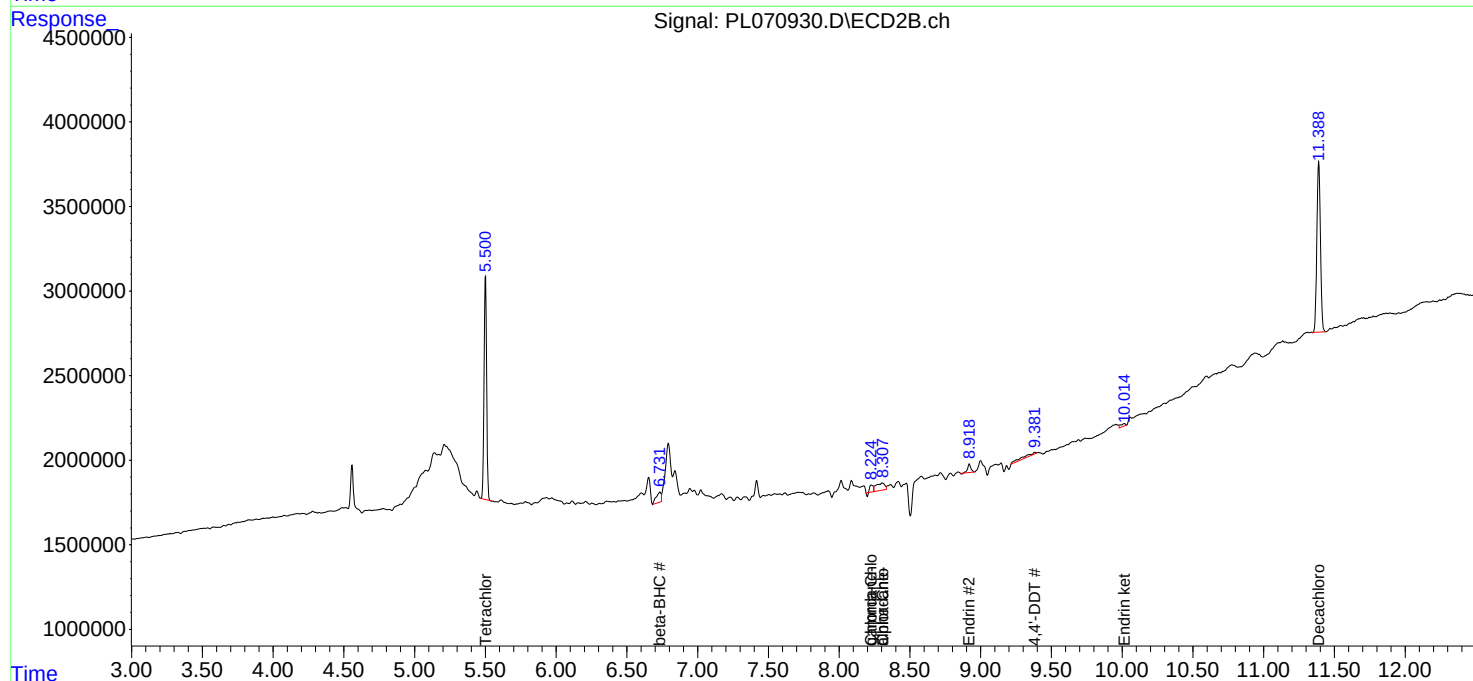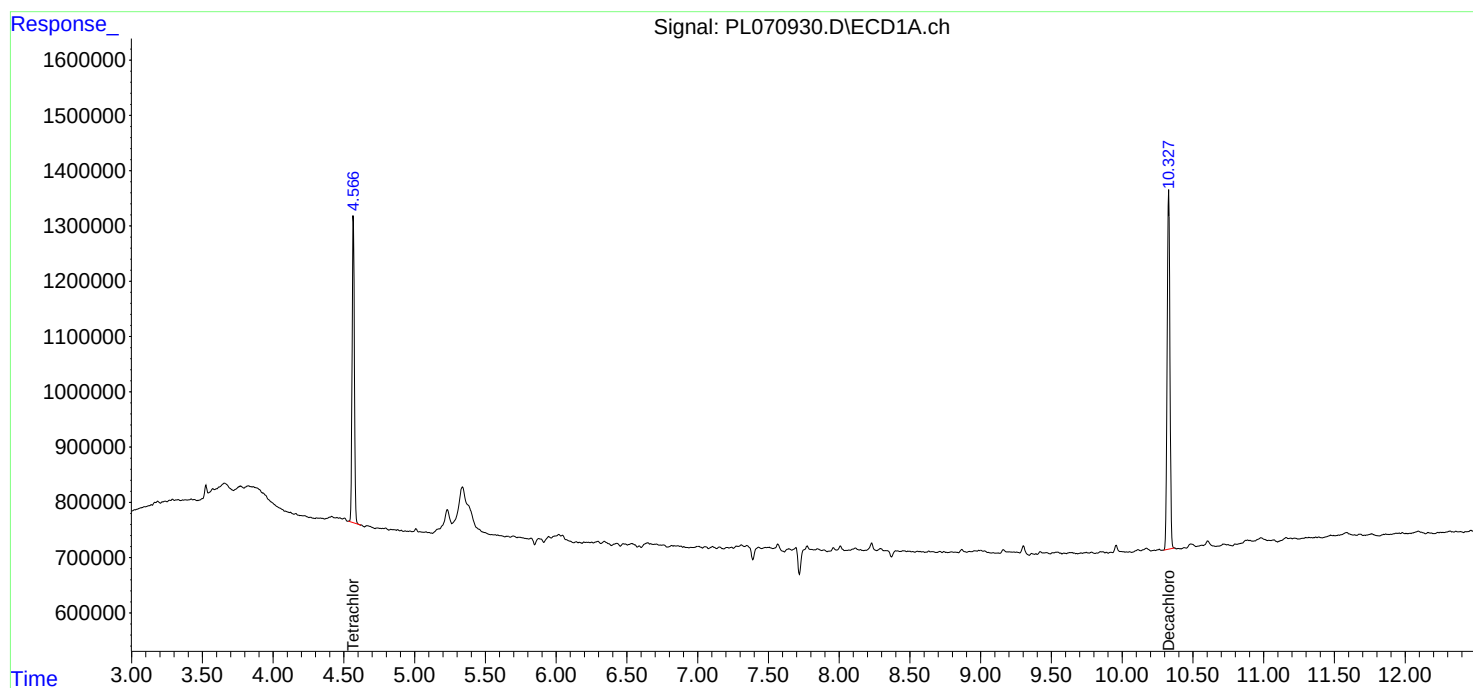


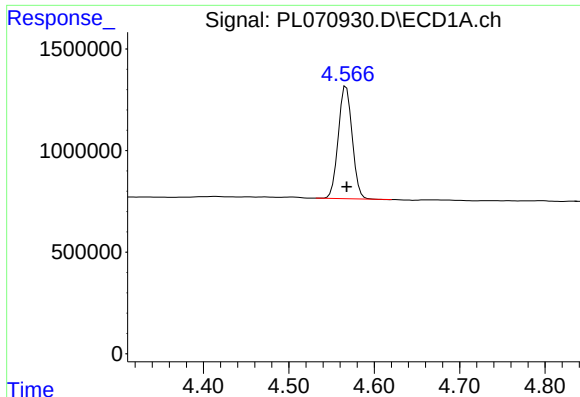

#1 Tetrachloro-m-xylene


R.T.: 4.567 min
Delta R.T.: 0.000 min
Response: 6269555
Conc: 12.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

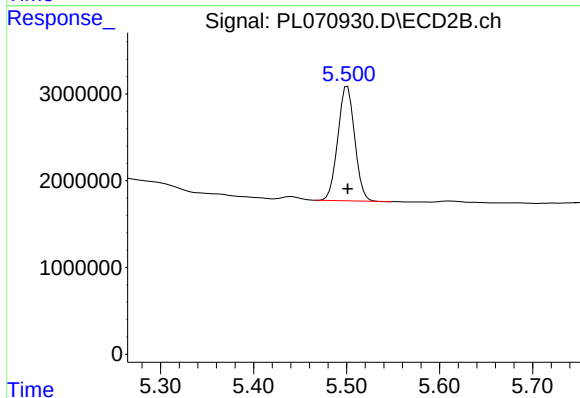


#1 Tetrachloro-m-xylene

R.T.: 5.501 min
Delta R.T.: 0.000 min
Response: 16602900
Conc: 13.17 ng/ml

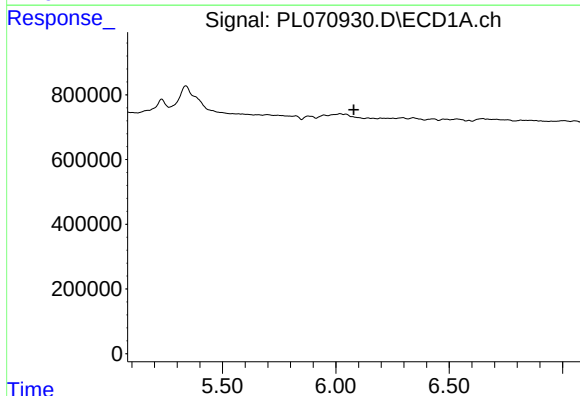


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.079 min
Response: 0
Conc: N.D.

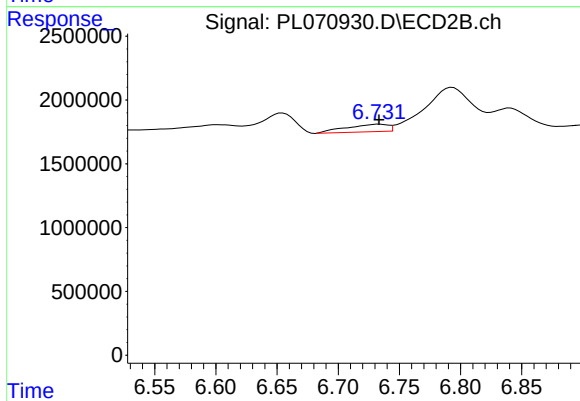

#6 beta-BHC


R.T.: 6.733 min
Delta R.T.: 0.000 min
Response: 1406263
Conc: 1.64 ng/ml

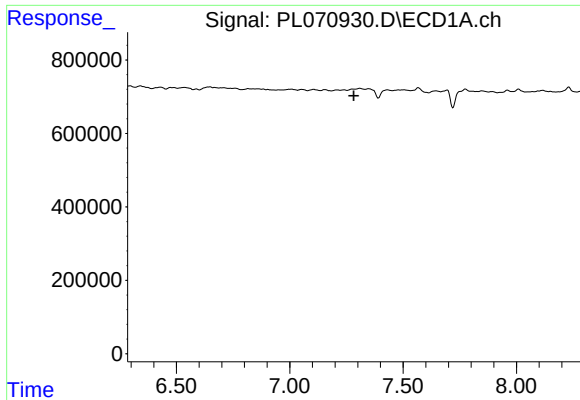

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.283 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

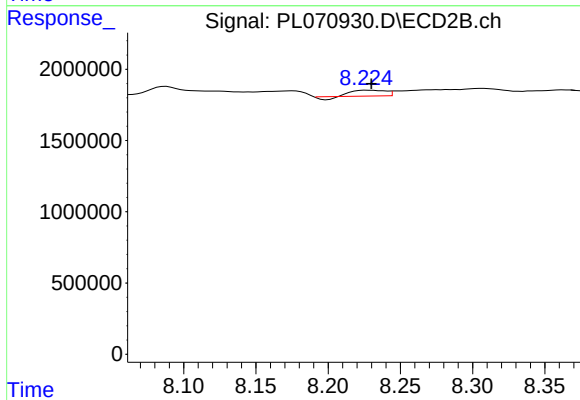


#10 gamma-Chlordane

R.T.: 8.227 min
Delta R.T.: -0.003 min
Response: 557512
Conc: 0.36 ng/ml

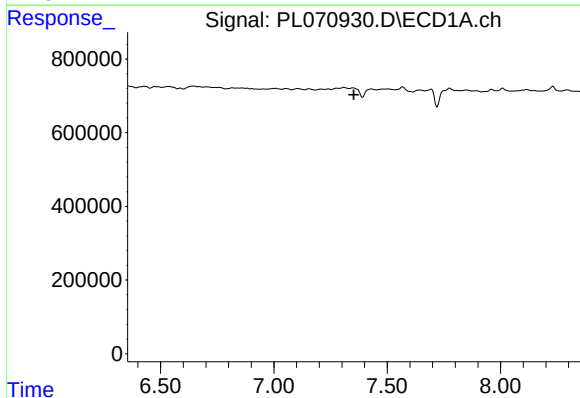


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.352 min
Response: 0
Conc: N.D.

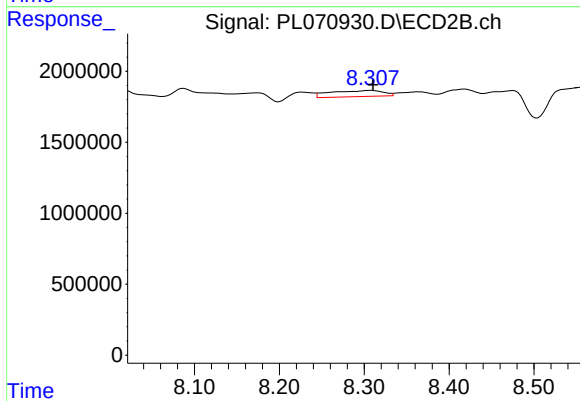

#11 alpha-Chlordane


R.T.: 8.308 min
Delta R.T.: -0.003 min
Response: 1860174
Conc: 1.22 ng/ml

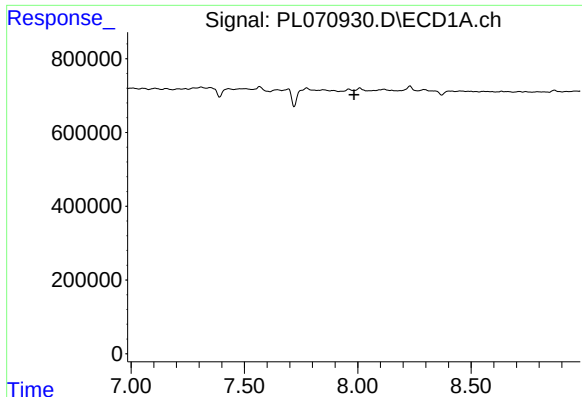

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 7.984 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

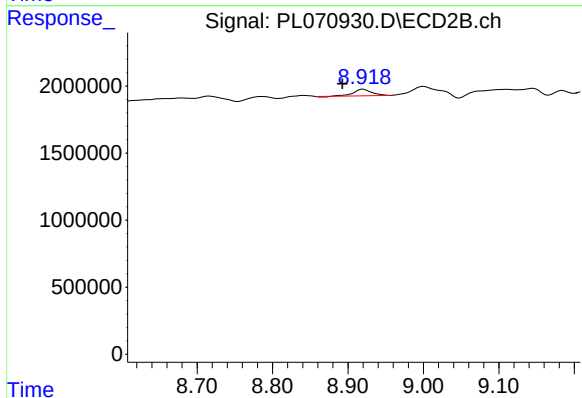


#14 Endrin

R.T.: 8.920 min
Delta R.T.: 0.027 min
Response: 811098
Conc: 0.70 ng/ml

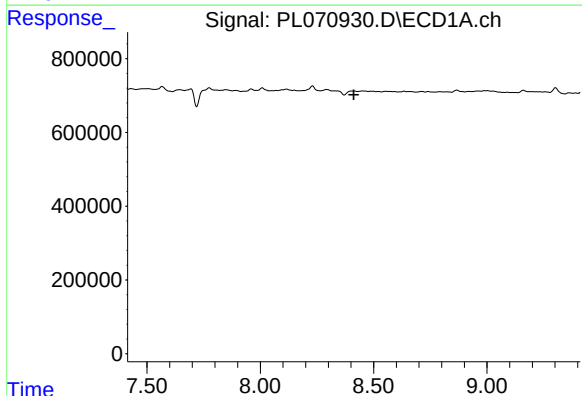


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 8.413 min
Response: 0
Conc: N.D.

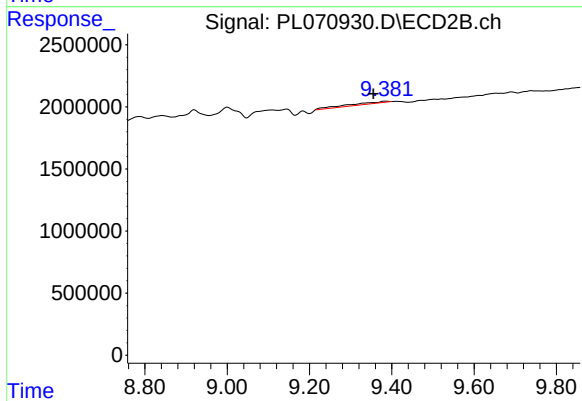

#17 4,4'-DDT


R.T.: 9.384 min
Delta R.T.: 0.028 min
Response: 955717
Conc: 0.76 ng/ml

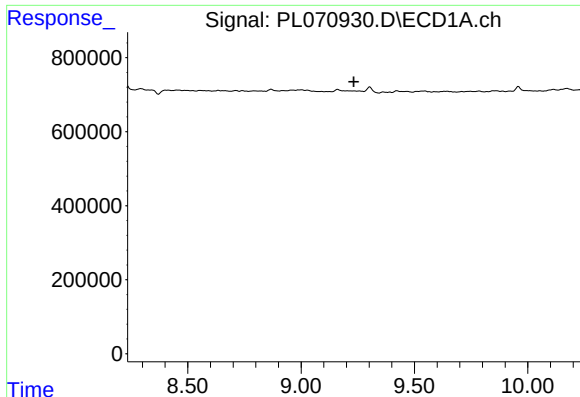

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.232 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

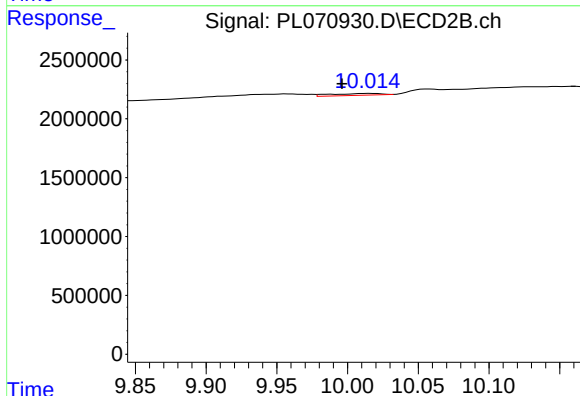


#21 Endrin ketone

R.T.: 10.015 min
Delta R.T.: 0.019 min
Response: 397366
Conc: 0.28 ng/ml

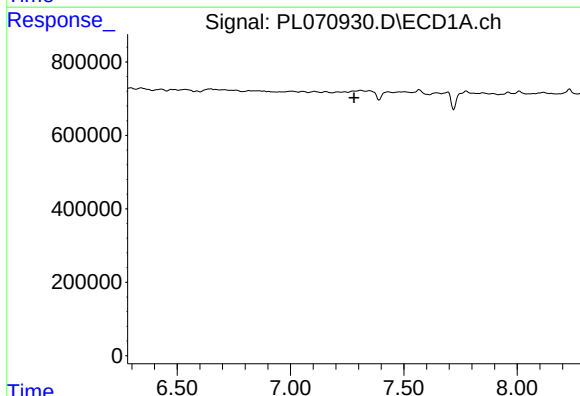


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.281 min
Response: 0
Conc: N.D.

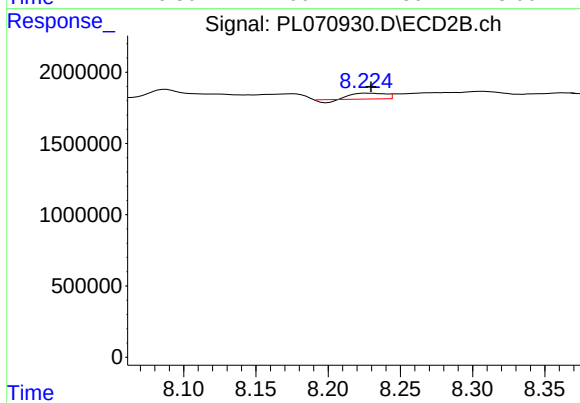

#25 Chlordane-3


R.T.: 8.227 min
Delta R.T.: -0.003 min
Response: 557512
Conc: 2.76 ng/ml

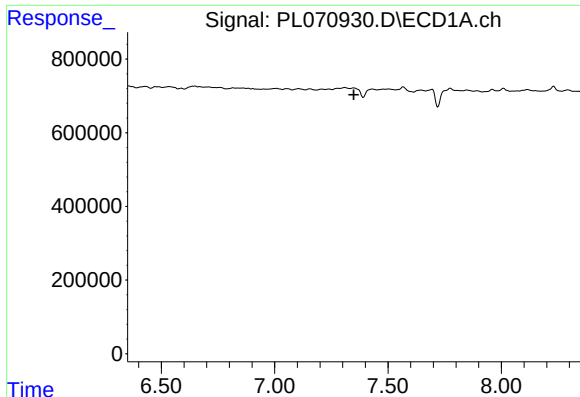

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

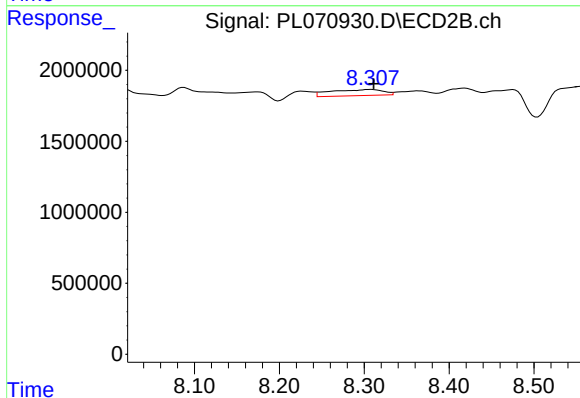


#26 Chlordane-4

R.T.: 8.308 min
Delta R.T.: -0.003 min
Response: 1860174
Conc: 7.67 ng/ml

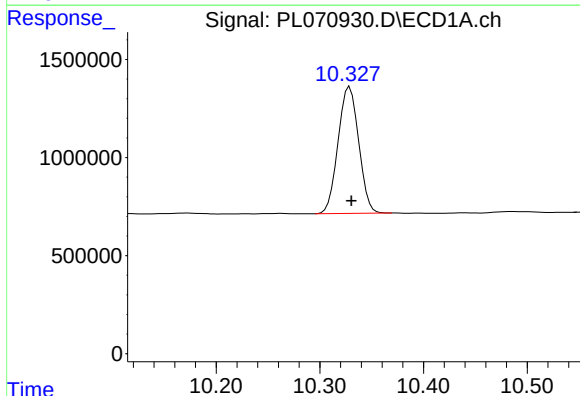

#28 Decachlorobiphenyl

R.T.: 10.329 min
Delta R.T.: -0.002 min
Response: 8936601
Conc: 13.08 ng/ml

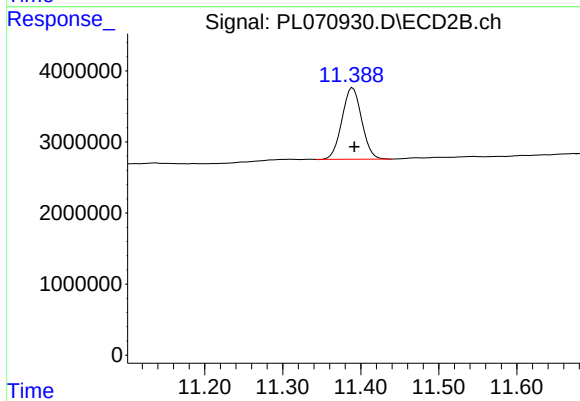

#28 Decachlorobiphenyl

R.T.: 11.390 min
Delta R.T.: -0.002 min
Response: 17631073
Conc: 13.18 ng/ml