

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111121\
 Data File : PL070936.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2021 18:03
 Operator : AR\AJ
 Sample : M4605-08
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VWE-B19-110821-GW

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/12/2021
 Supervised By : mohammad ahmed 11/12/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 03:33:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 19:28:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.567	5.500	8792262	24030518	17.951	19.059
2) SA Decachlor...	10.327	11.392	7165913	8233988	10.487	6.157m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111121\
Data File : PL070936.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2021 18:03
Operator : AR\AJ
Sample : M4605-08
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
VWE-B19-110821-GW


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/12/2021
Supervised By : mohammad ahmed 11/12/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 03:33:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 19:28:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

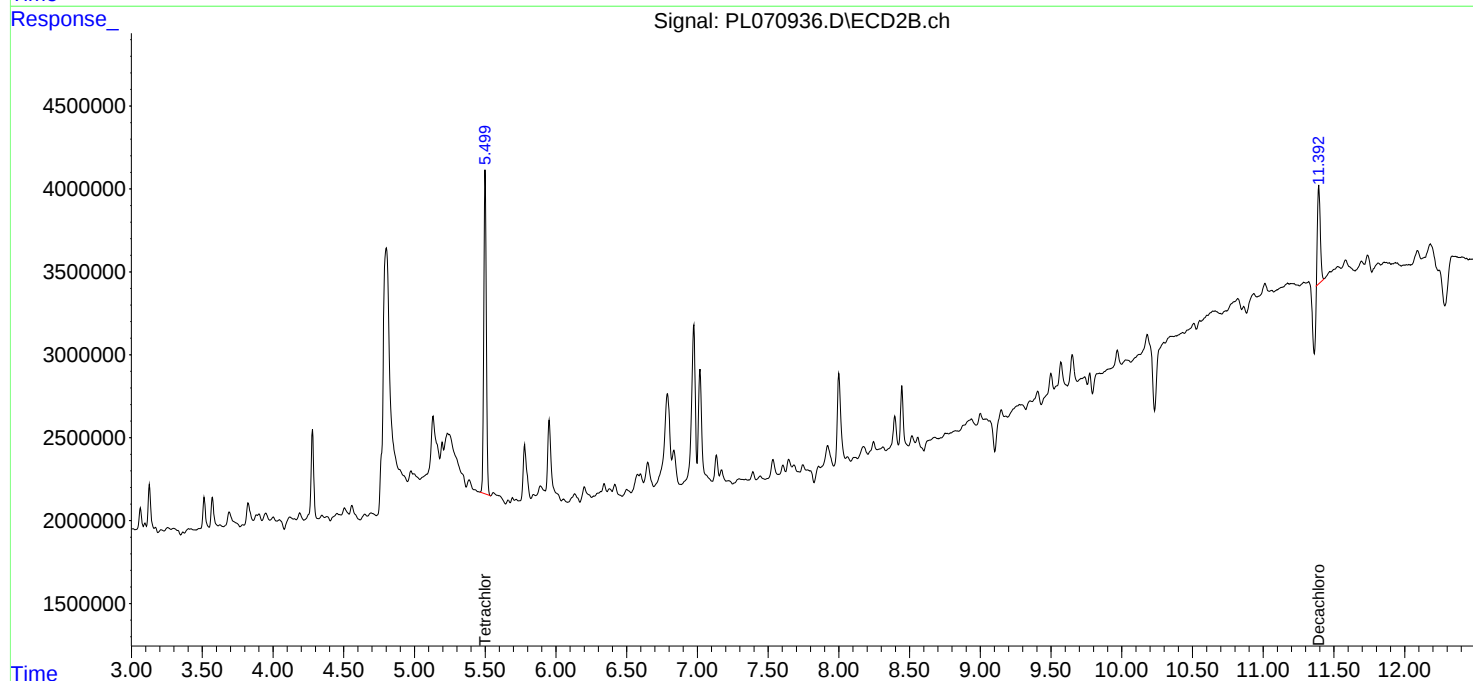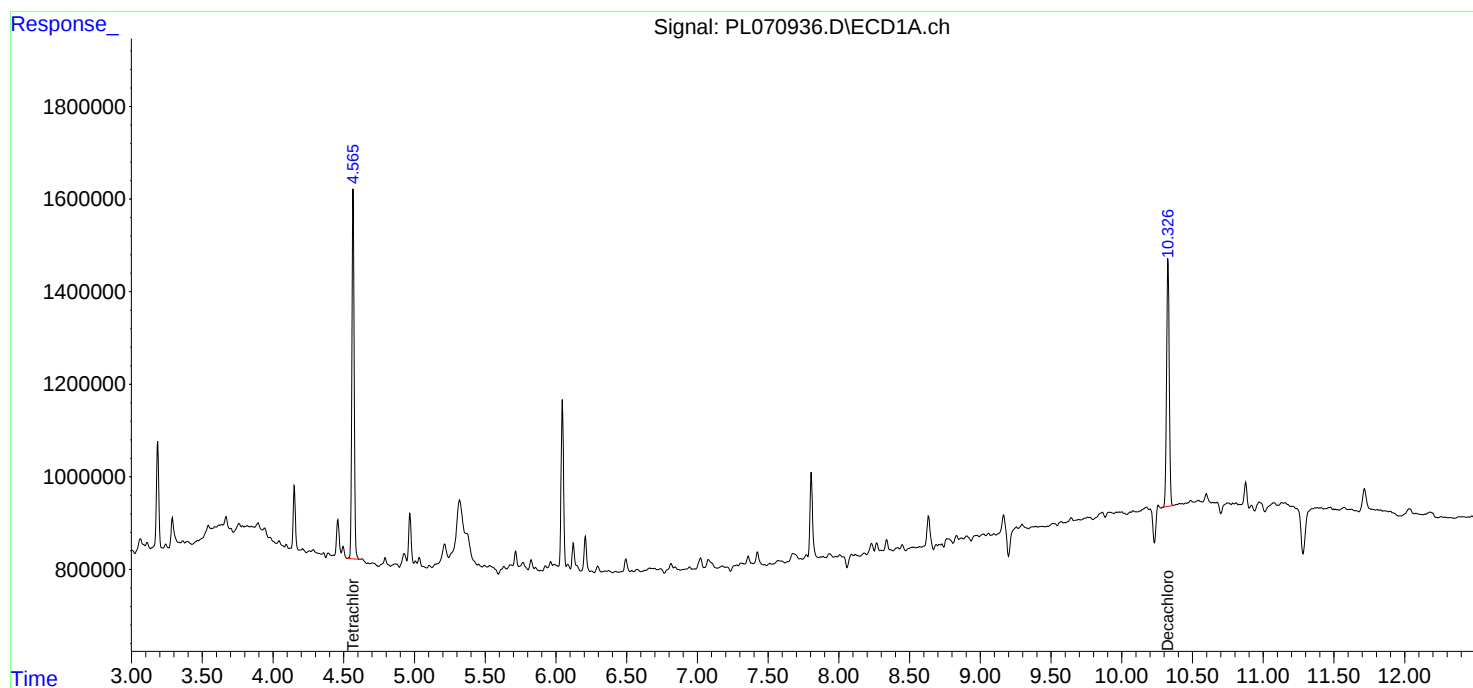

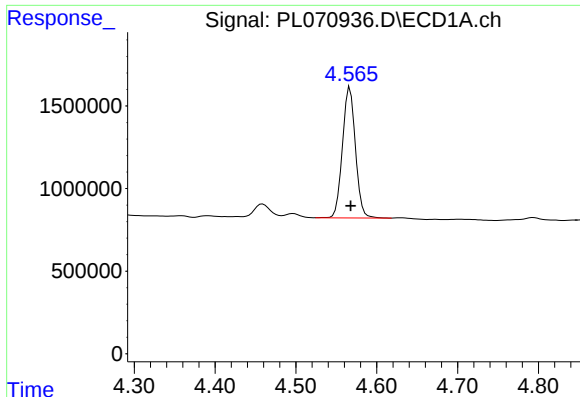


#1 Tetrachloro-m-xylene

R.T.: 4.567 min
Delta R.T.: -0.001 min
Response: 8792262
Conc: 17.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
VWE-B19-110821-GW


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/12/2021
Supervised By :mohammad ahmed 11/12/2021

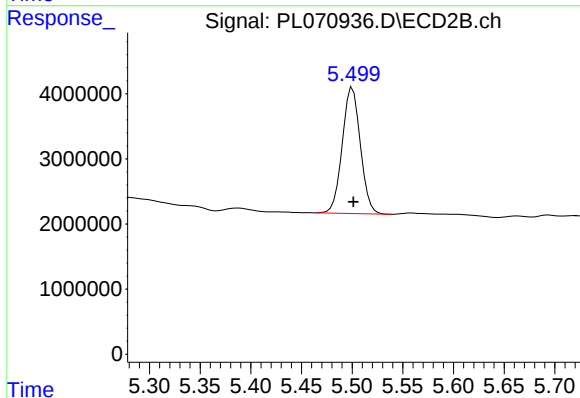


#1 Tetrachloro-m-xylene

R.T.: 5.500 min
Delta R.T.: 0.000 min
Response: 24030518
Conc: 19.06 ng/ml

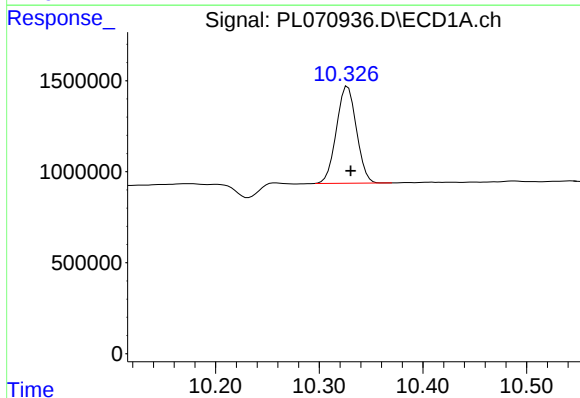

#28 Decachlorobiphenyl

R.T.: 10.327 min
Delta R.T.: -0.003 min
Response: 7165913
Conc: 10.49 ng/ml

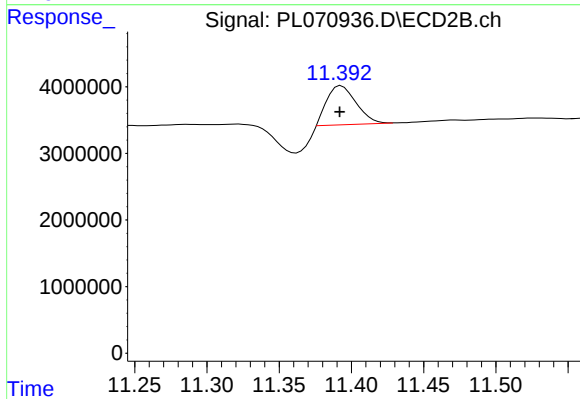

#28 Decachlorobiphenyl

R.T.: 11.392 min
Delta R.T.: 0.000 min
Response: 8233988
Conc: 6.16 ng/ml m