

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111122\
 Data File : PL079049.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2022 22:09
 Operator : AR\AJ
 Sample : N5509-01
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 01:52:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.321	2.568	30704559	40288623	16.101	15.780
28)	SA Decachlor...	8.770	7.635	19580920	26727518	13.016	14.111
Target Compounds							
5)	MB Aldrin	0.000	3.995	0	907322	N.D.	0.259 #
9)	A Endosulfan I	5.845	0.000	287861	0	0.135	N.D. #
10)	B gamma-Chl...	0.000	4.740f	0	372053	N.D.	0.121 #
11)	B alpha-Chl...	5.789	0.000	448355	0	0.194	N.D. #
14)	MA Endrin	0.000	5.389f	0	419660	N.D.	0.161 #
17)	MA 4,4'-DDT	6.819	0.000	126678	0	0.071	N.D. #
20)	A Methoxychlor	7.308	0.000	104932	0	0.114	N.D. #
22)	Mirex	7.895	0.000	471913	0	0.323	N.D. #
23)	Chlordane-1	0.000	3.532	0	599714	N.D.	5.946 #
25)	Chlordane-3	0.000	4.740f	0	372053	N.D.	1.221 #
26)	Chlordane-4	5.789	0.000	448355	0	1.092	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111122\
Data File : PL079049.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2022 22:09
Operator : AR\AJ
Sample : N5509-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 01:52:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

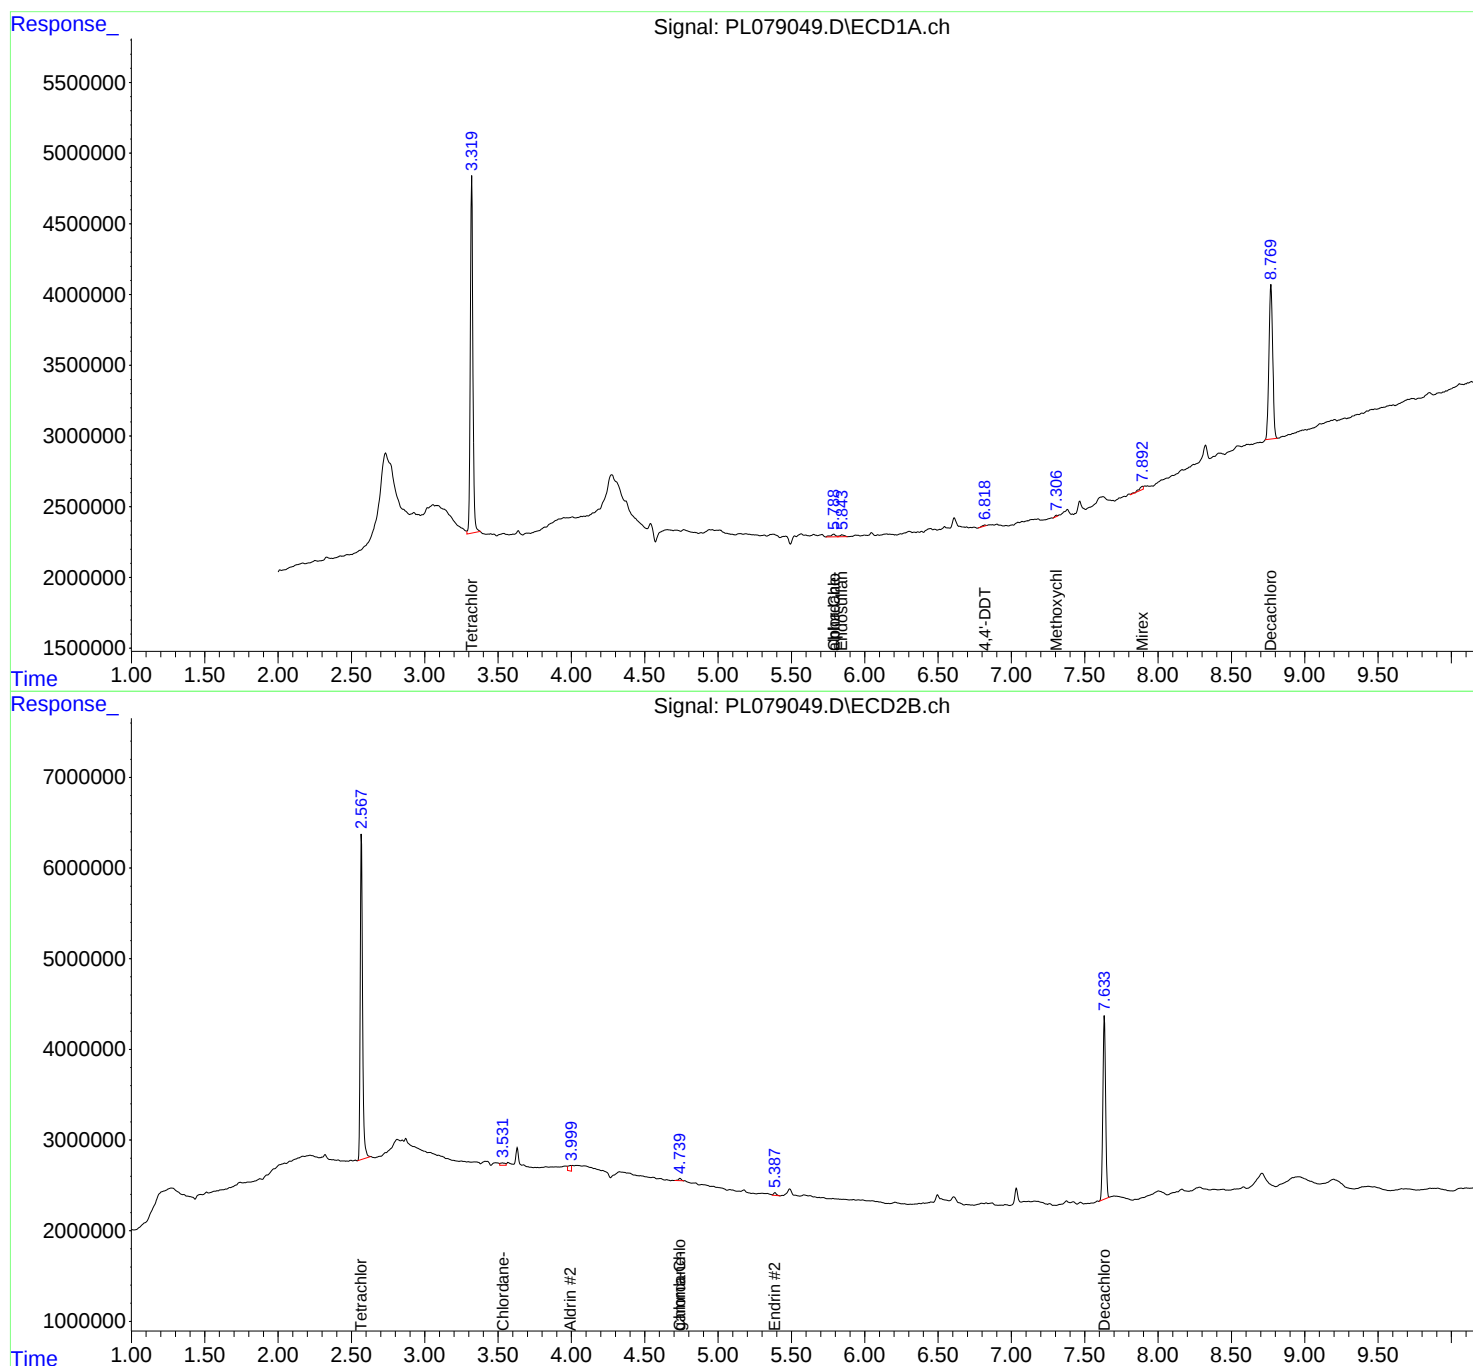


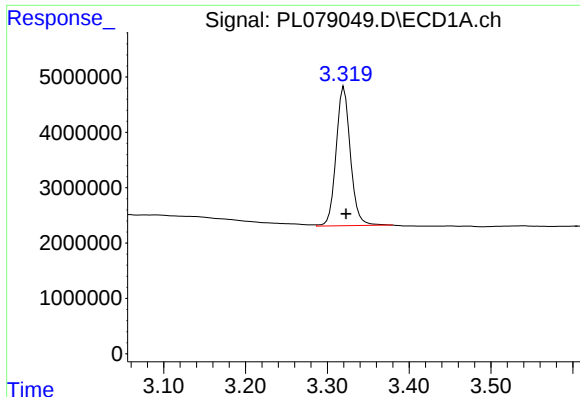

#1 Tetrachloro-m-xylene


R.T.: 3.321 min
Delta R.T.: -0.002 min
Response: 30704559
Conc: 16.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

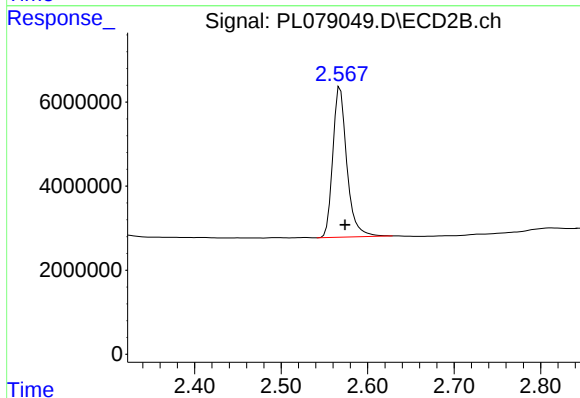


#1 Tetrachloro-m-xylene

R.T.: 2.568 min
Delta R.T.: -0.005 min
Response: 40288623
Conc: 15.78 ng/ml

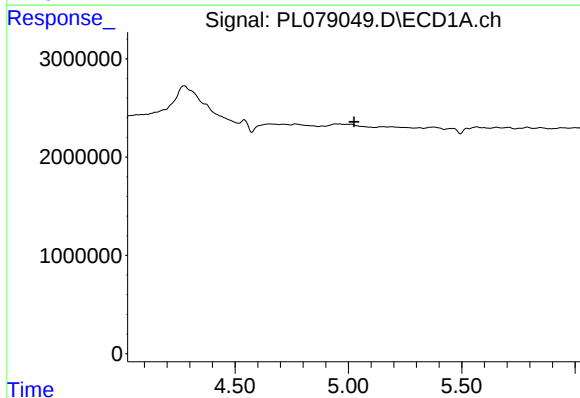


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.025 min
Response: 0
Conc: N.D.

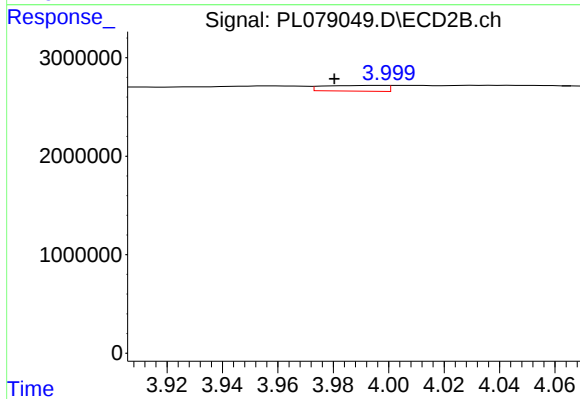

#5 Aldrin


R.T.: 3.995 min
Delta R.T.: 0.015 min
Response: 907322
Conc: 0.26 ng/ml

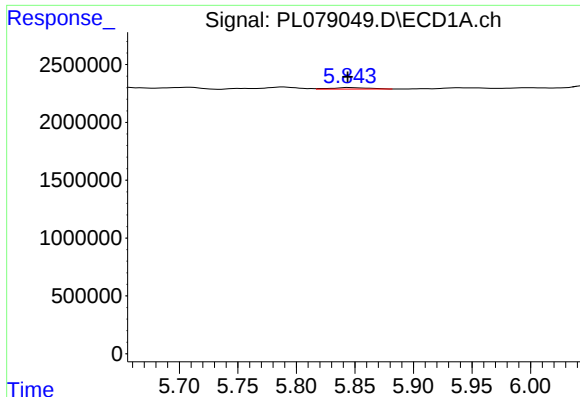

#9 Endosulfan I


R.T.: 5.845 min
Delta R.T.: 0.001 min
Response: 287861
Conc: 0.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

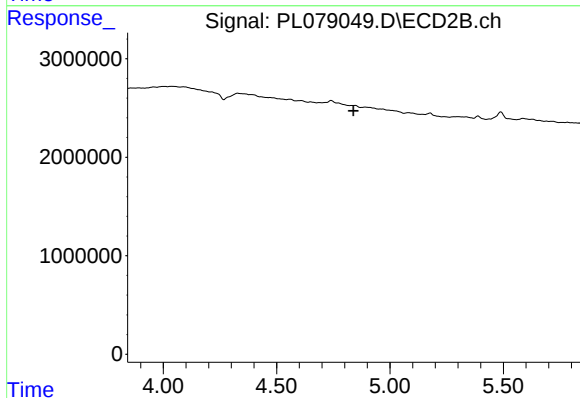


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 4.840 min
Response: 0
Conc: N.D.

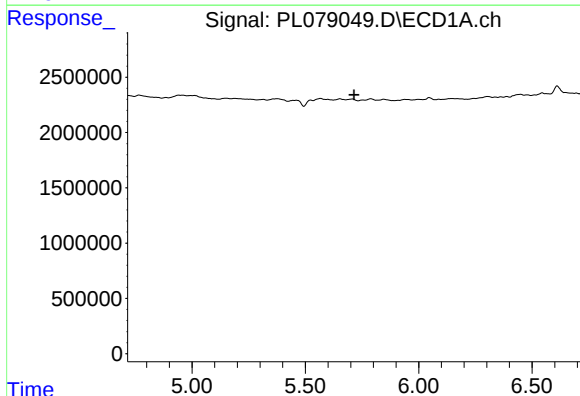


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.715 min
Response: 0
Conc: N.D.

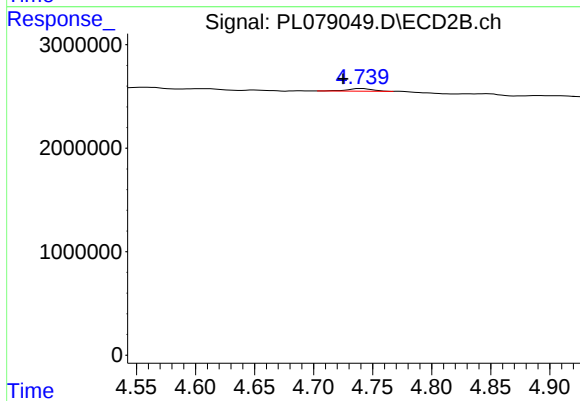

#10 gamma-Chlordane


R.T.: 4.740 min
Delta R.T.: 0.015 min
Response: 372053
Conc: 0.12 ng/ml

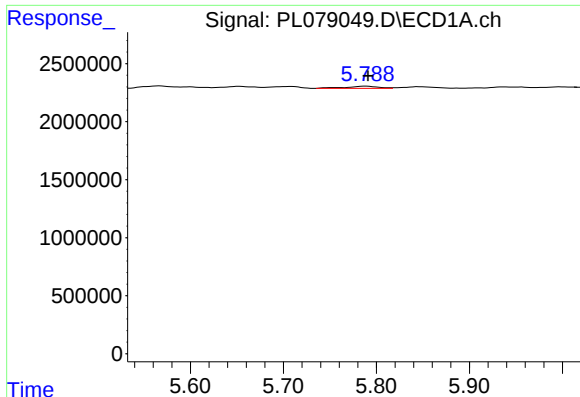

#11 alpha-Chlordane


R.T.: 5.789 min
Delta R.T.: -0.002 min
Response: 448355
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

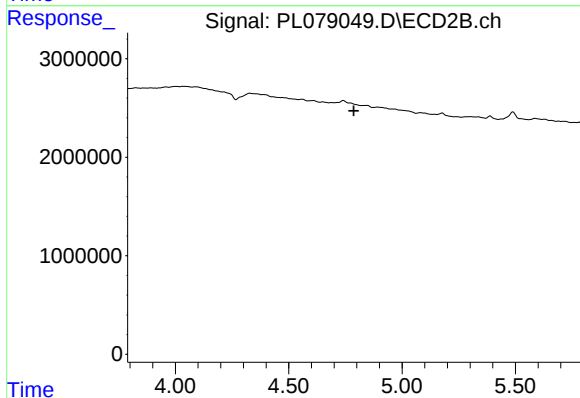


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.787 min
Response: 0
Conc: N.D.

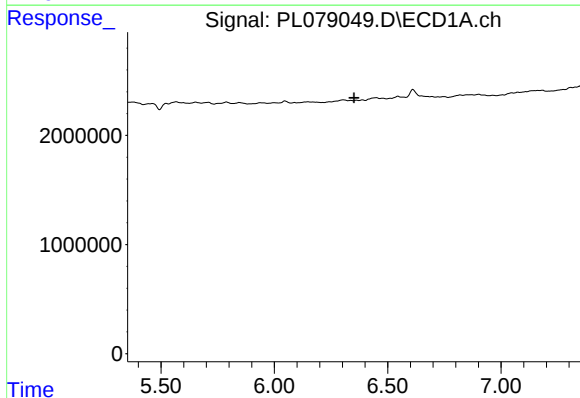


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.351 min
Response: 0
Conc: N.D.

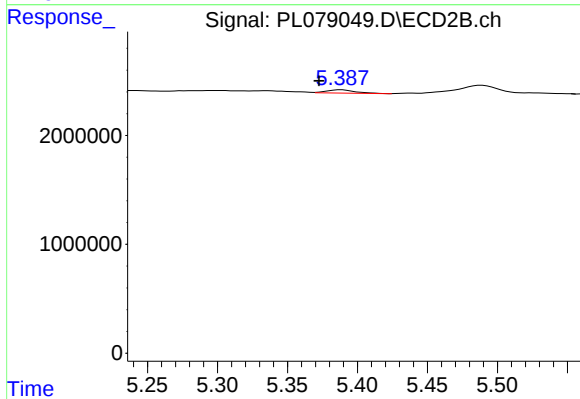

#14 Endrin


R.T.: 5.389 min
Delta R.T.: 0.016 min
Response: 419660
Conc: 0.16 ng/ml

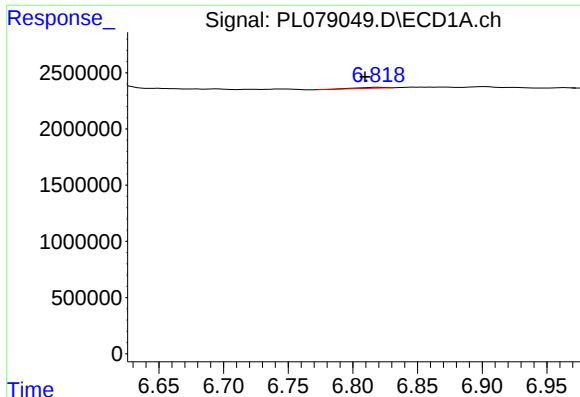

#17 4,4'-DDT


R.T.: 6.819 min
Delta R.T.: 0.010 min
Response: 126678
Conc: 0.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

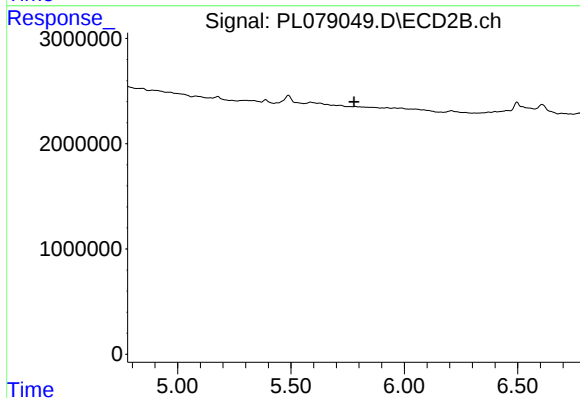


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 5.779 min
Response: 0
Conc: N.D.

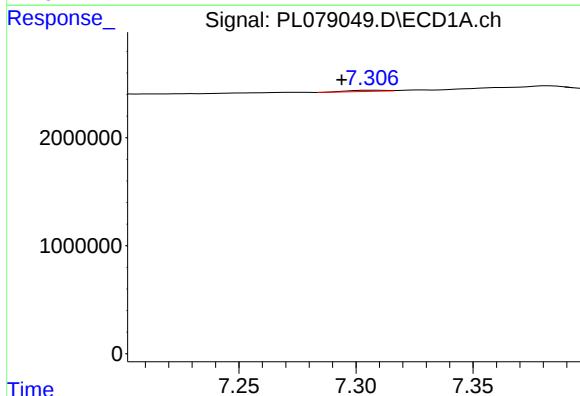


#20 Methoxychlor

R.T.: 7.308 min
Delta R.T.: 0.014 min
Response: 104932
Conc: 0.11 ng/ml

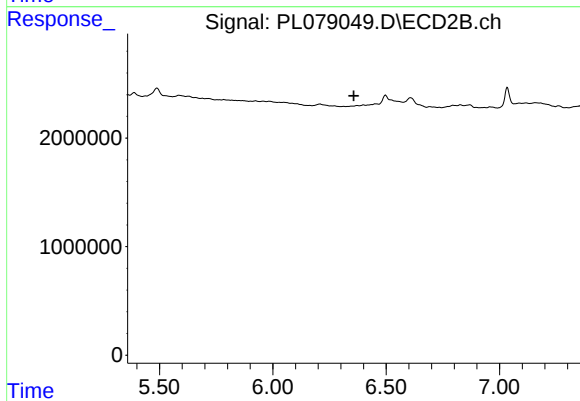

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 6.357 min
Response: 0
Conc: N.D.

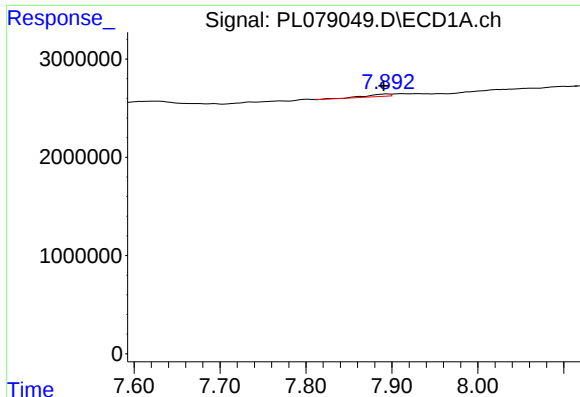

#22 Mirex


R.T.: 7.895 min
Delta R.T.: 0.004 min
Response: 471913
Conc: 0.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

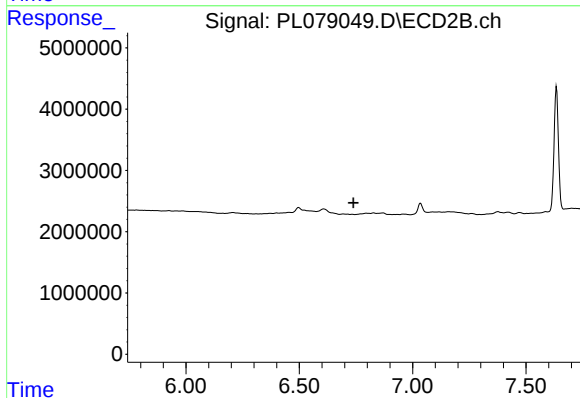


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 6.739 min
Response: 0
Conc: N.D.

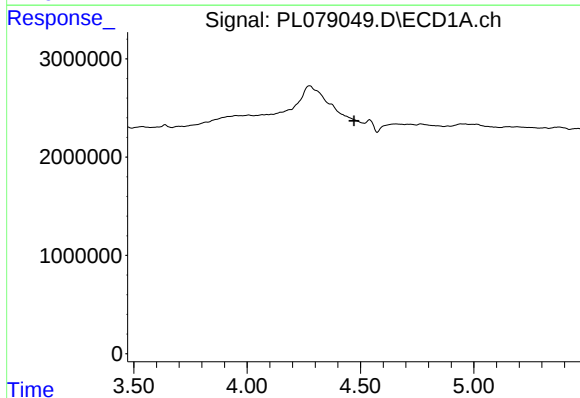


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.472 min
Response: 0
Conc: N.D.

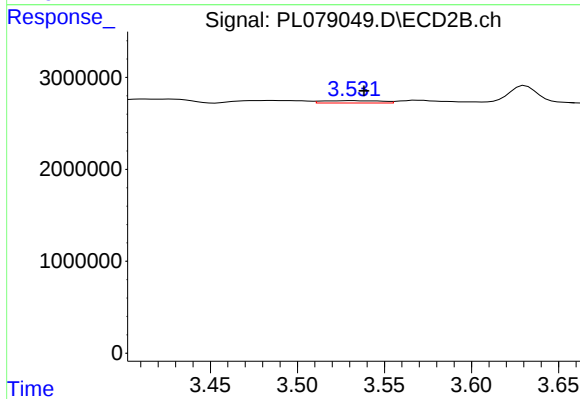

#23 Chlordane-1


R.T.: 3.532 min
Delta R.T.: -0.006 min
Response: 599714
Conc: 5.95 ng/ml

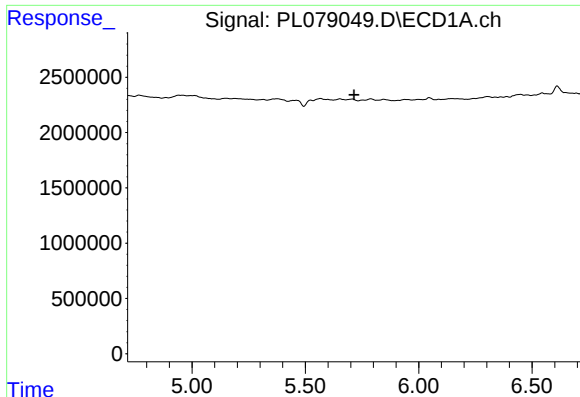

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.715 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

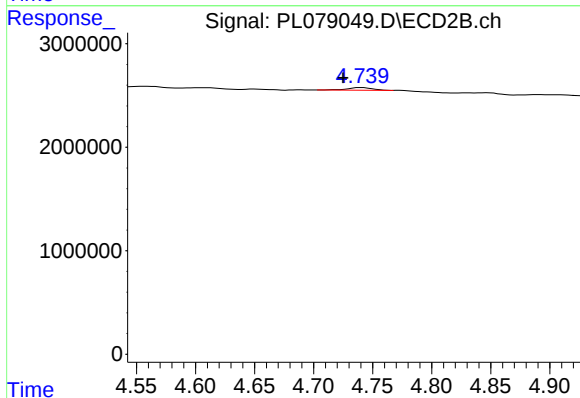


#25 Chlordane-3

R.T.: 4.740 min
Delta R.T.: 0.016 min
Response: 372053
Conc: 1.22 ng/ml

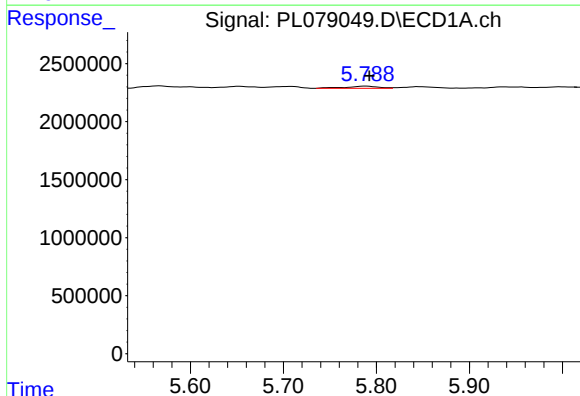


#26 Chlordane-4

R.T.: 5.789 min
Delta R.T.: -0.004 min
Response: 448355
Conc: 1.09 ng/ml

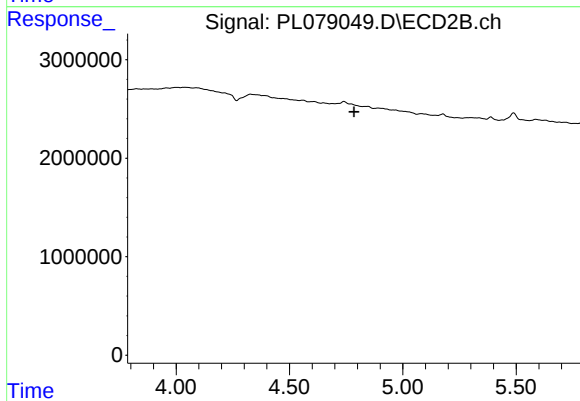

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 4.785 min
Response: 0
Conc: N.D.

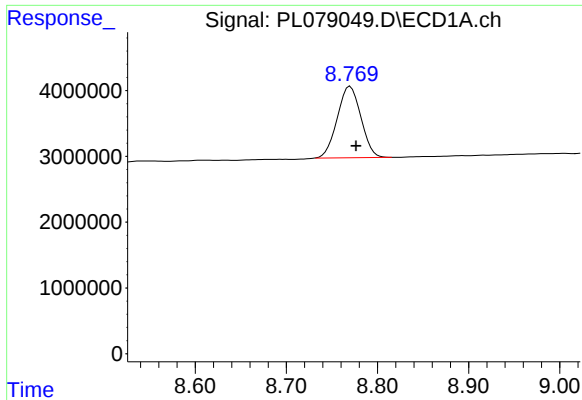

#28 Decachlorobiphenyl

R.T.: 8.770 min
Delta R.T.: -0.006 min
Response: 19580920
Conc: 13.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

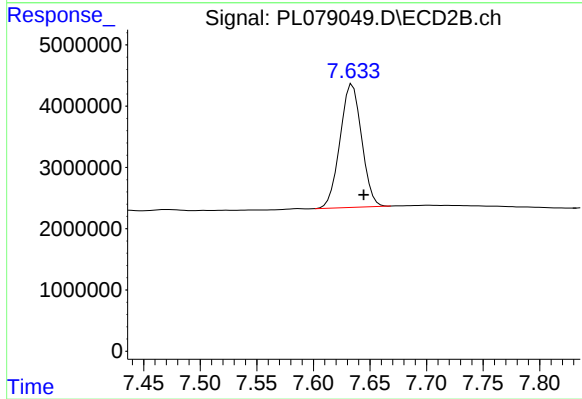

#28 Decachlorobiphenyl

R.T.: 7.635 min
Delta R.T.: -0.010 min
Response: 26727518
Conc: 14.11 ng/ml