

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111122\
 Data File : PL079080.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2022 09:41
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 10:27:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.322	2.570	45231789	57529703	23.719	22.532
28)	SA Decachlor...	8.776	7.639	30799210	42041703	20.473	22.196
Target Compounds							
5)	MB Aldrin	0.000	3.994	0	3597211	N.D.	1.027 #
6)	B beta-BHC	0.000	3.678	0	690289	N.D.	0.481 #
8)	B Heptachlo...	5.467	4.484	3056328	518618	1.440	0.172 #
9)	A Endosulfan I	5.864f	0.000	988910	0	0.463	N.D. #
13)	MA Dieldrin	0.000	5.093	0	1591346	N.D.	0.537 #
14)	MA Endrin	0.000	5.393f	0	983827	N.D.	0.378 #
17)	MA 4,4'-DDT	6.826f	0.000	402146	0	0.224	N.D. #
20)	A Methoxychlor	0.000	6.370	0	225909	N.D.	0.199 #
23)	Chlordane-1	0.000	3.537	0	419158	N.D.	4.156 #
24)	Chlordane-2	0.000	4.099	0	3081384	N.D.	28.953 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111122\
Data File : PL079080.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2022 09:41
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 10:27:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

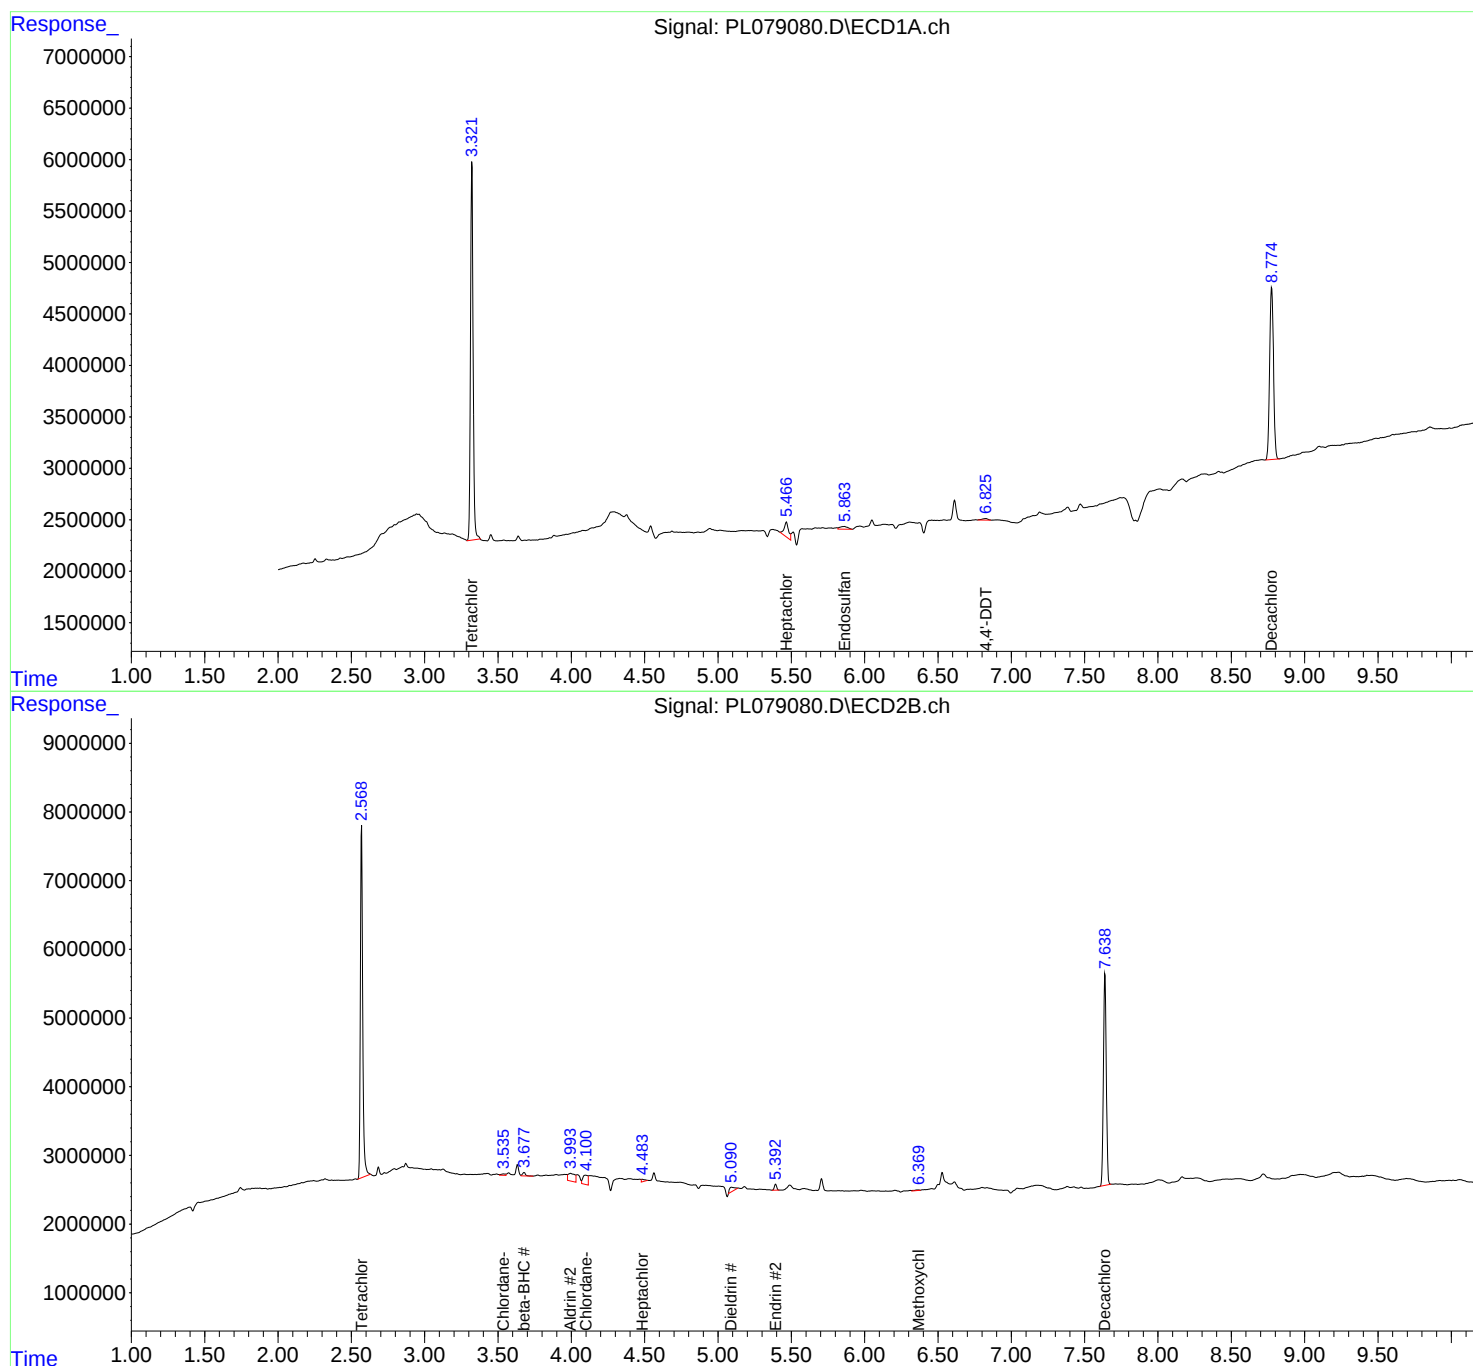


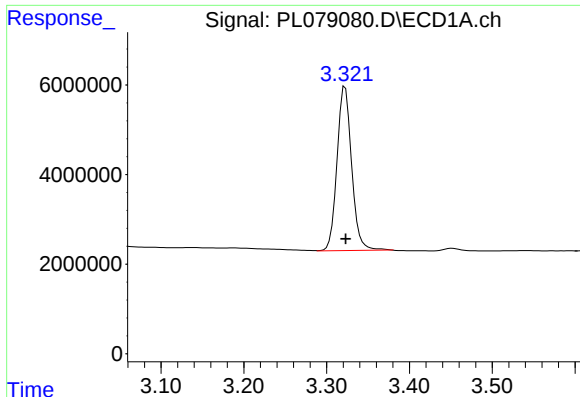

#1 Tetrachloro-m-xylene


R.T.: 3.322 min
Delta R.T.: 0.000 min
Response: 45231789
Conc: 23.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

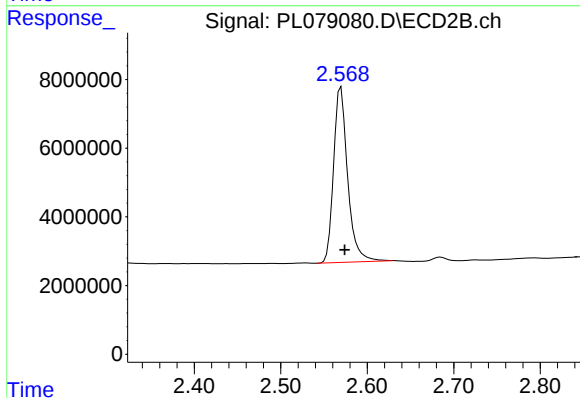


#1 Tetrachloro-m-xylene

R.T.: 2.570 min
Delta R.T.: -0.004 min
Response: 57529703
Conc: 22.53 ng/ml

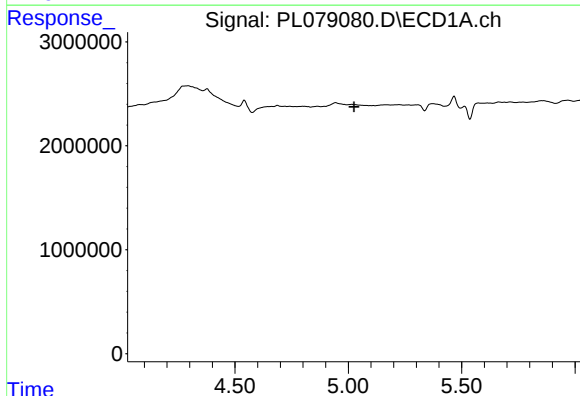


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.025 min
Response: 0
Conc: N.D.

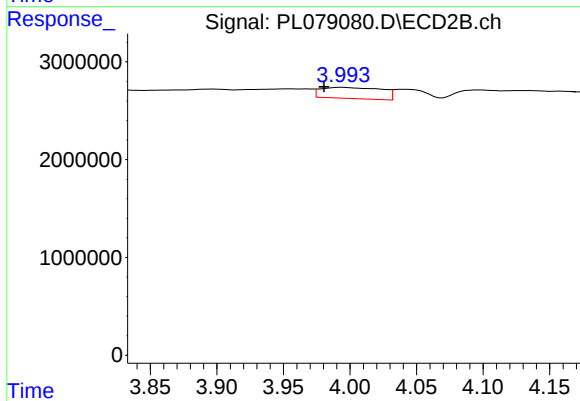

#5 Aldrin


R.T.: 3.994 min
Delta R.T.: 0.014 min
Response: 3597211
Conc: 1.03 ng/ml

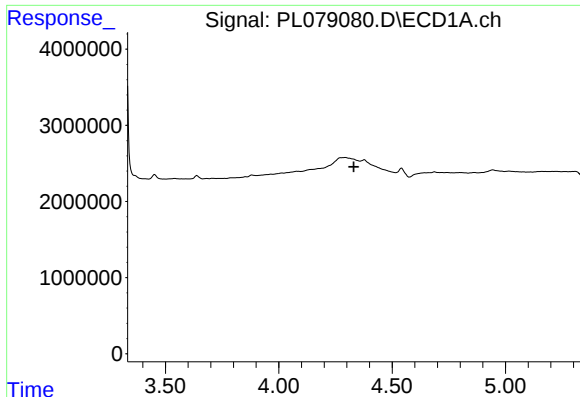

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.331 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

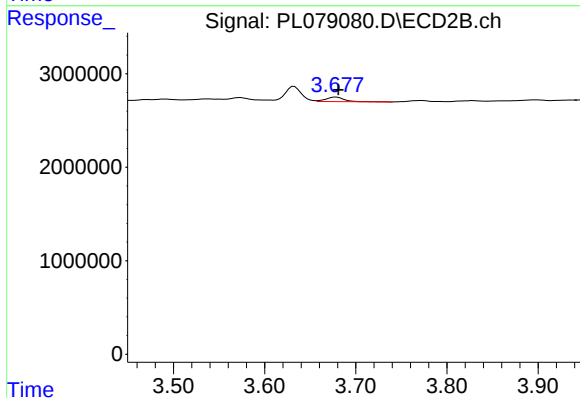


#6 beta-BHC

R.T.: 3.678 min
Delta R.T.: -0.003 min
Response: 690289
Conc: 0.48 ng/ml

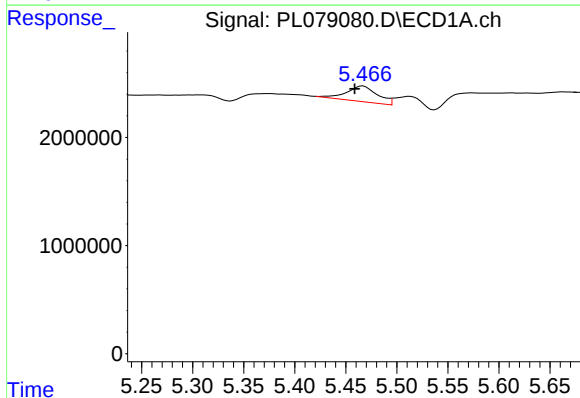


#8 Heptachlor epoxide

R.T.: 5.467 min
Delta R.T.: 0.008 min
Response: 3056328
Conc: 1.44 ng/ml

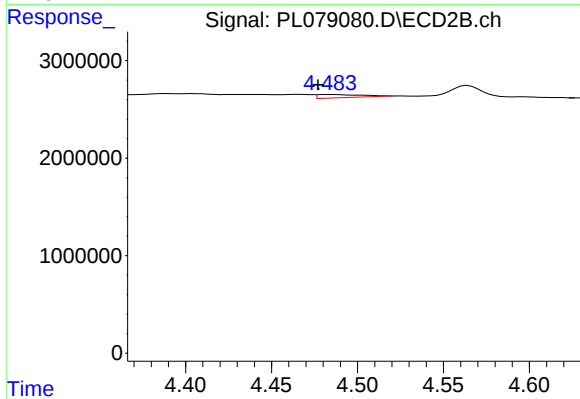

#8 Heptachlor epoxide


R.T.: 4.484 min
Delta R.T.: 0.007 min
Response: 518618
Conc: 0.17 ng/ml

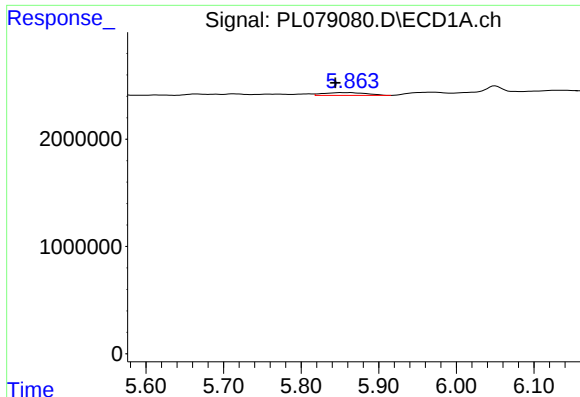

#9 Endosulfan I


R.T.: 5.864 min
Delta R.T.: 0.020 min
Response: 988910
Conc: 0.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

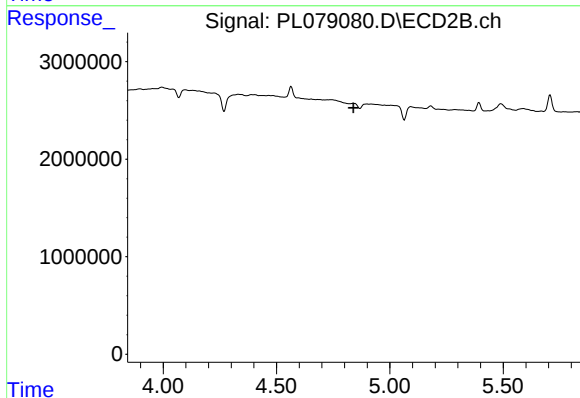


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 4.840 min
Response: 0
Conc: N.D.

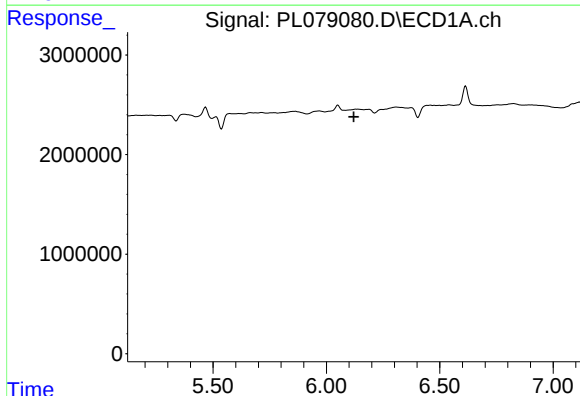


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.121 min
Response: 0
Conc: N.D.

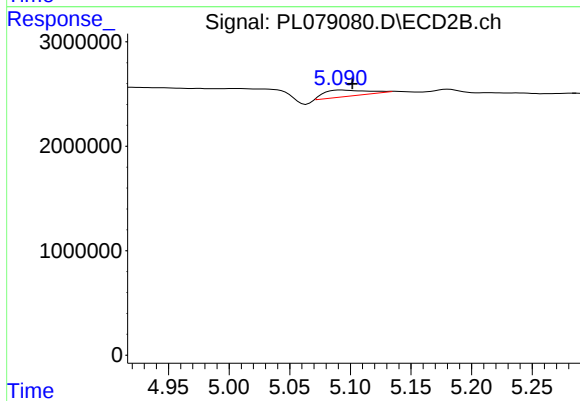

#13 Dieldrin


R.T.: 5.093 min
Delta R.T.: -0.009 min
Response: 1591346
Conc: 0.54 ng/ml

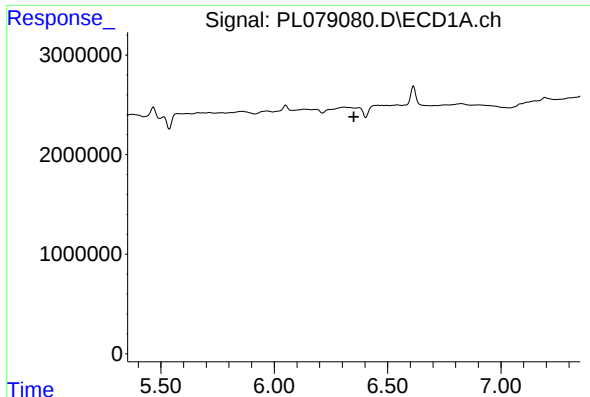

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.351 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

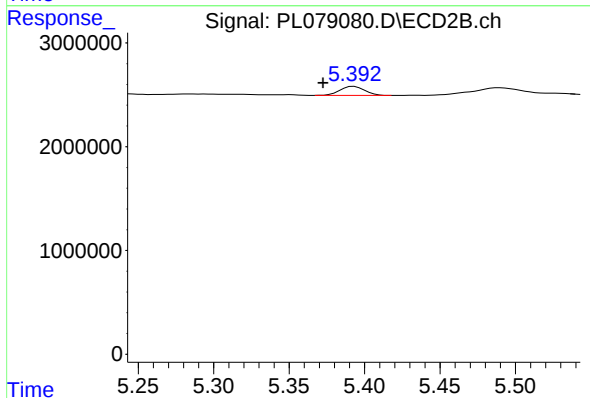


#14 Endrin

R.T.: 5.393 min
Delta R.T.: 0.021 min
Response: 983827
Conc: 0.38 ng/ml

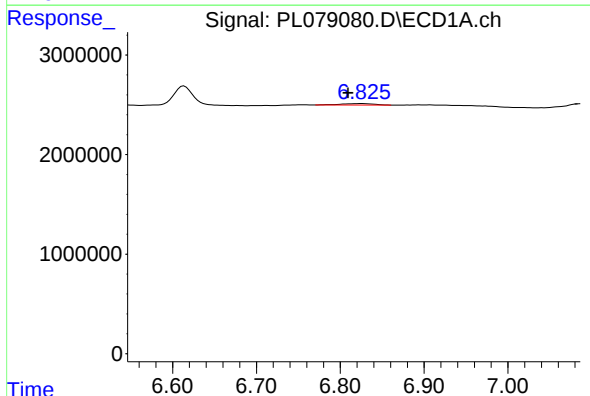


#17 4,4'-DDT

R.T.: 6.826 min
Delta R.T.: 0.017 min
Response: 402146
Conc: 0.22 ng/ml

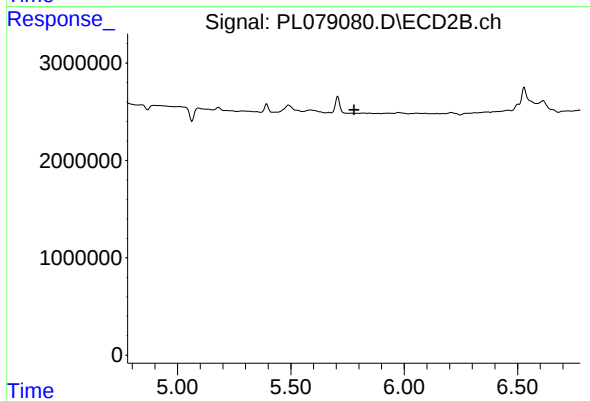

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 5.779 min
Response: 0
Conc: N.D.

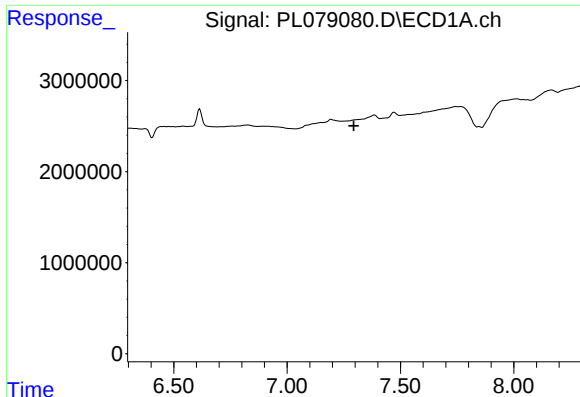

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.294 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

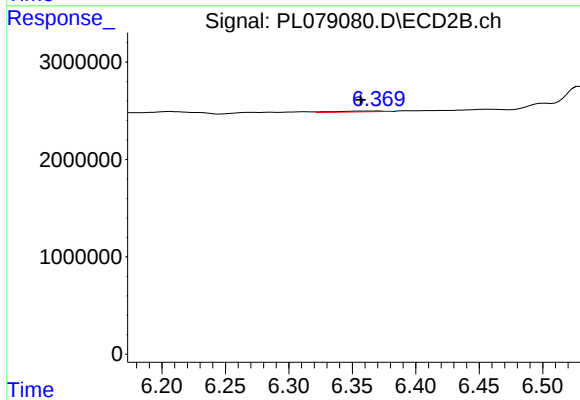


#20 Methoxychlor

R.T.: 6.370 min
Delta R.T.: 0.013 min
Response: 225909
Conc: 0.20 ng/ml

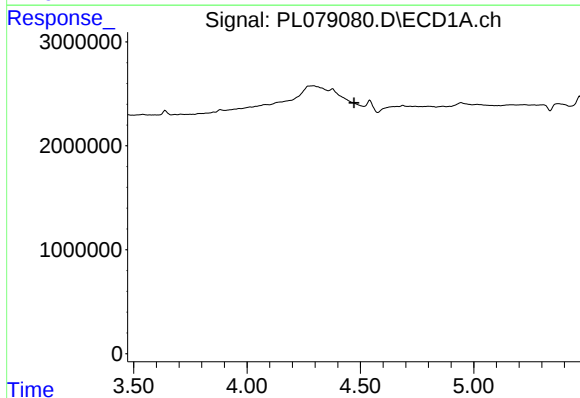


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.472 min
Response: 0
Conc: N.D.

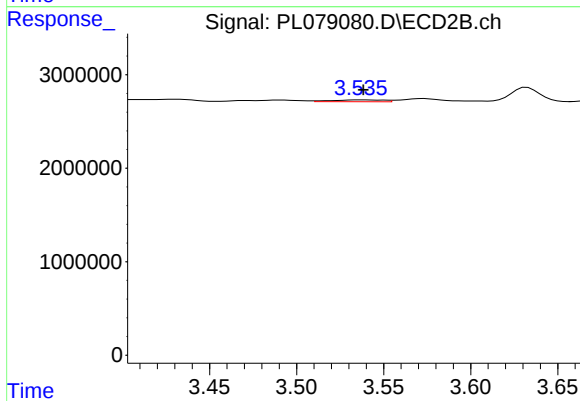

#23 Chlordane-1


R.T.: 3.537 min
Delta R.T.: -0.002 min
Response: 419158
Conc: 4.16 ng/ml

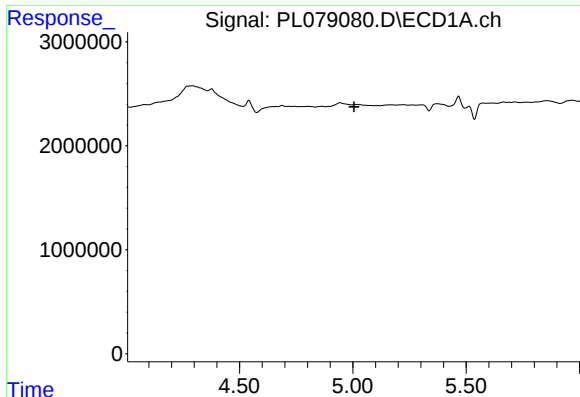

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.005 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

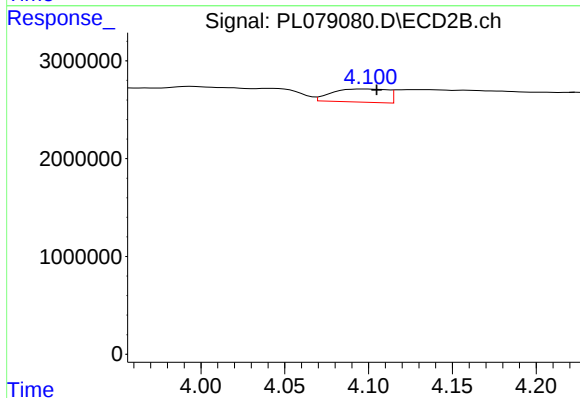


#24 Chlordane-2

R.T.: 4.099 min
Delta R.T.: -0.006 min
Response: 3081384
Conc: 28.95 ng/ml

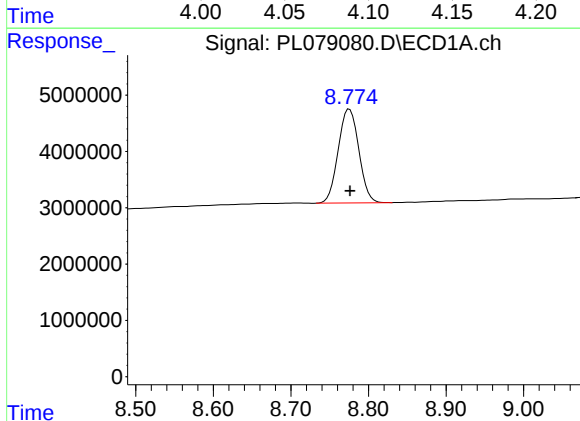

#28 Decachlorobiphenyl

R.T.: 8.776 min
Delta R.T.: -0.001 min
Response: 30799210
Conc: 20.47 ng/ml

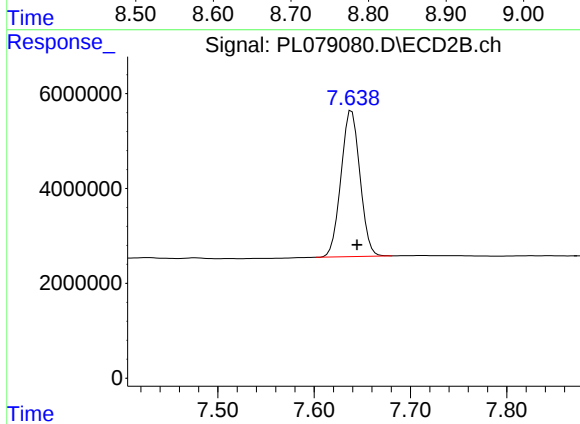

#28 Decachlorobiphenyl

R.T.: 7.639 min
Delta R.T.: -0.005 min
Response: 42041703
Conc: 22.20 ng/ml