

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111124\
 Data File : PL092975.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2024 20:56
 Operator : AR\AJ
 Sample : P4722-10
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-2(0-6)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 00:30:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.779	47470908	53231234	19.374	19.562
28)	SA Decachlor...	9.063	7.920	31739699	43903803	16.492	16.086
Target Compounds							
2)	A alpha-BHC	0.000	3.279	0	1118390	N.D.	0.280 #
4)	MA Heptachlor	0.000	3.945	0	6658967	N.D.	1.764 #
7)	B delta-BHC	4.774	4.134	10476668	473045	3.347	0.123 #
10)	B gamma-Chl...	0.000	4.982	0	529148	N.D.	0.157 #
11)	B alpha-Chl...	0.000	5.071f	0	569671	N.D.	0.171 #
13)	MA Dieldrin	0.000	5.354	0	968501	N.D.	0.290 #
14)	MA Endrin	0.000	5.662f	0	901706	N.D.	0.312 #
17)	MA 4,4'-DDT	0.000	6.043	0	269060	N.D.	0.100 #
18)	B Endrin al...	0.000	6.096f	0	469592	N.D.	0.204 #
22)	Mirex	0.000	7.025	0	316125	N.D.	0.121 #
24)	Chlordane-2	0.000	4.383f	0	22215	N.D.	0.179 #
25)	Chlordane-3	0.000	4.982	0	529148	N.D.	1.459 #
26)	Chlordane-4	0.000	5.019f	0	656594	N.D.	1.877 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111124\
Data File : PL092975.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2024 20:56
Operator : AR\AJ
Sample : P4722-10
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
WC-2(0-6)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 00:30:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

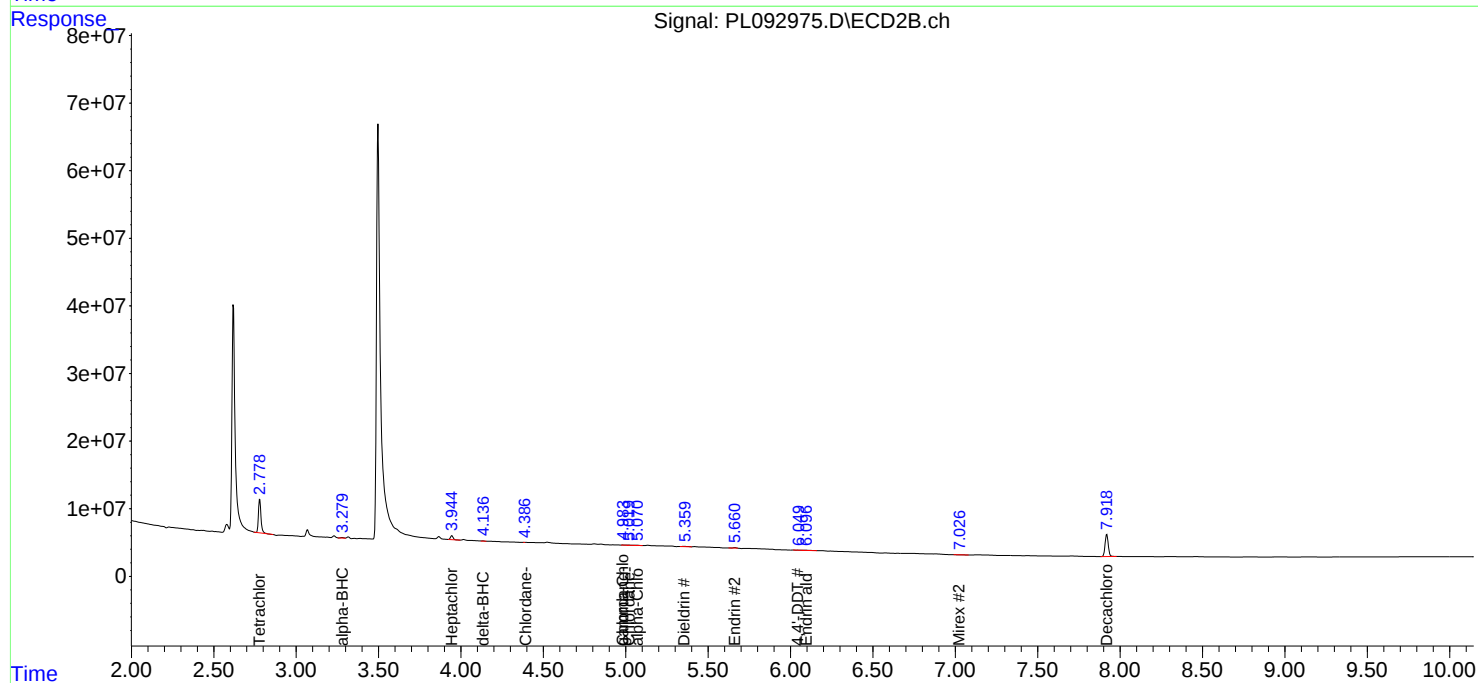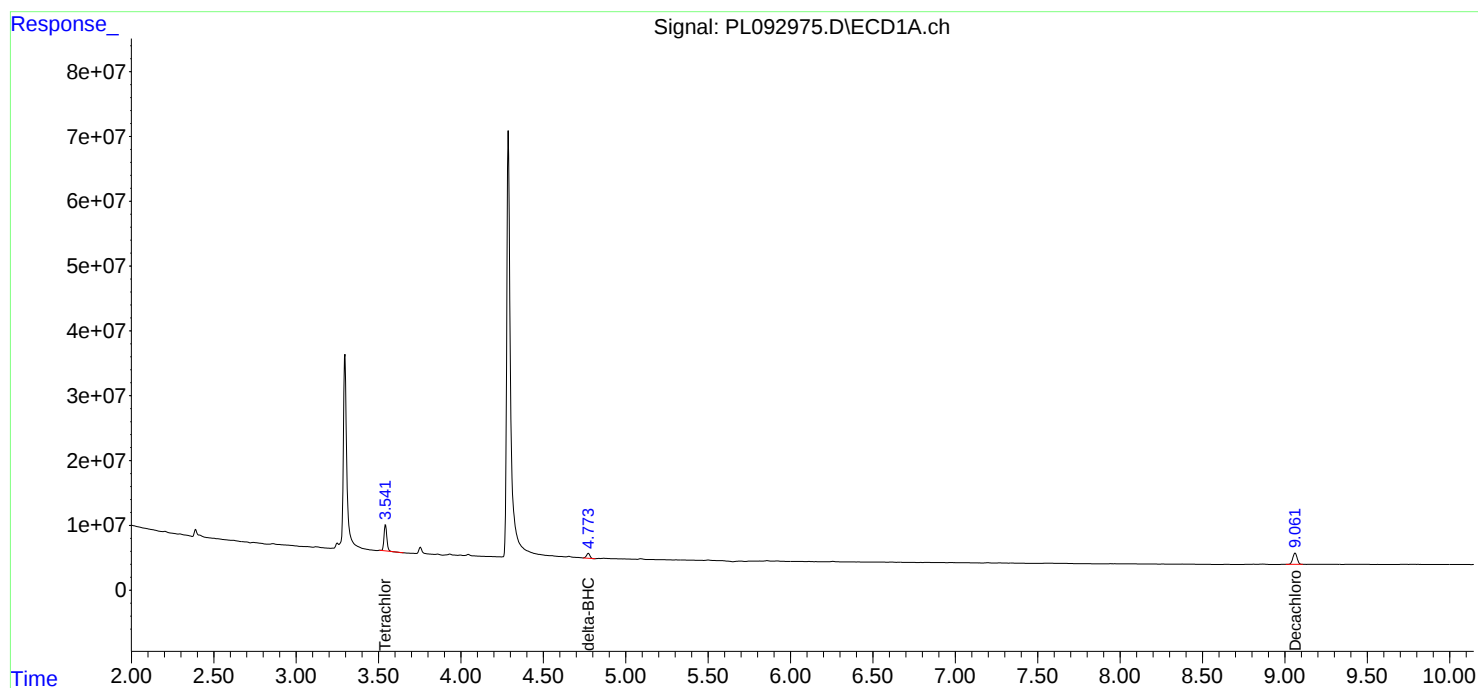


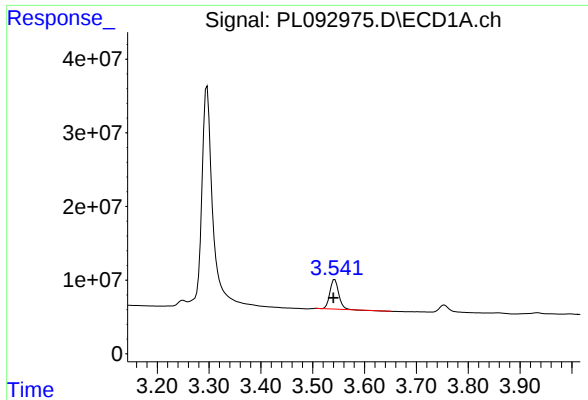

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: 0.002 min
Response: 47470908
Conc: 19.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-2(0-6)

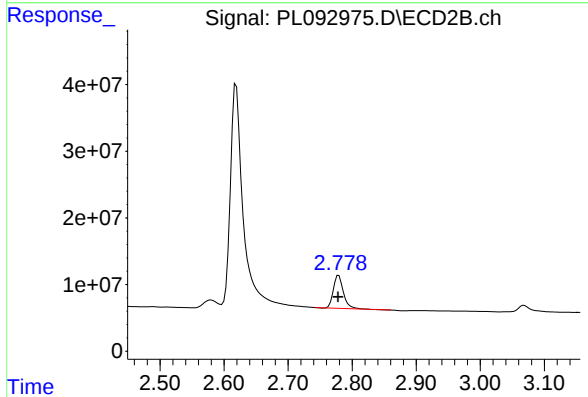


#1 Tetrachloro-m-xylene

R.T.: 2.779 min
Delta R.T.: 0.001 min
Response: 53231234
Conc: 19.56 ng/ml

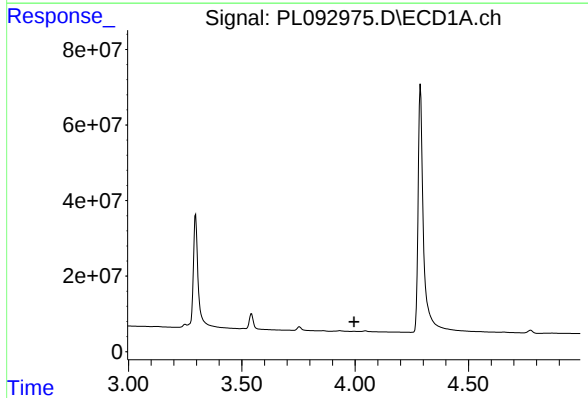


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.996 min
Response: 0
Conc: N.D.

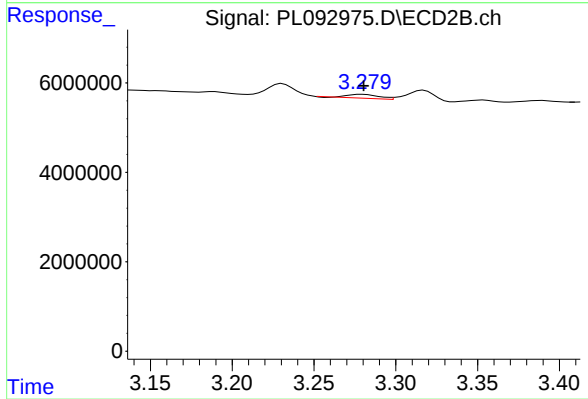

#2 alpha-BHC


R.T.: 3.279 min
Delta R.T.: -0.001 min
Response: 1118390
Conc: 0.28 ng/ml

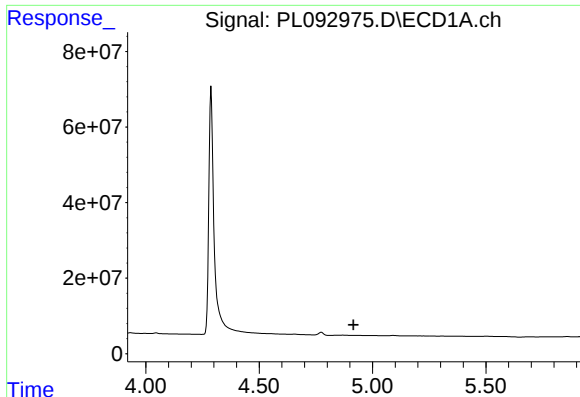

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.917 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WC-2(0-6)

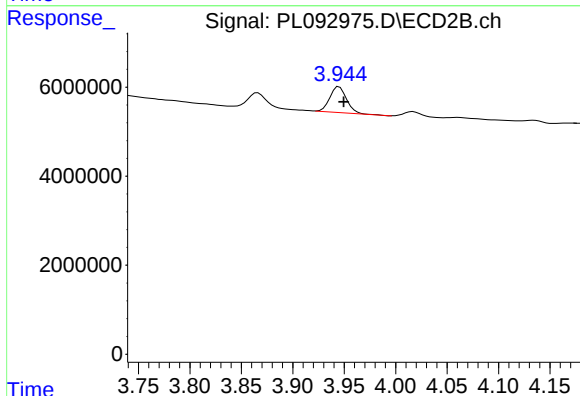


#4 Heptachlor

R.T.: 3.945 min
Delta R.T.: -0.004 min
Response: 6658967
Conc: 1.76 ng/ml

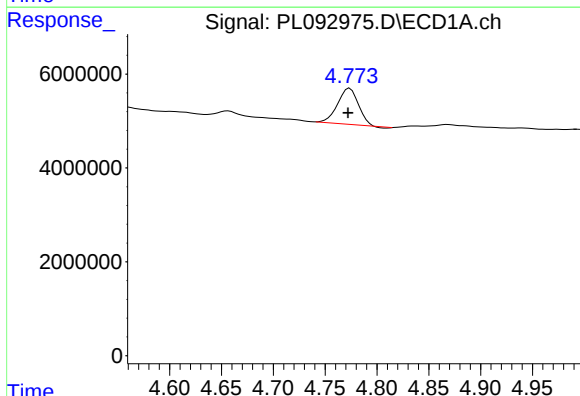


#7 delta-BHC

R.T.: 4.774 min
Delta R.T.: 0.002 min
Response: 10476668
Conc: 3.35 ng/ml

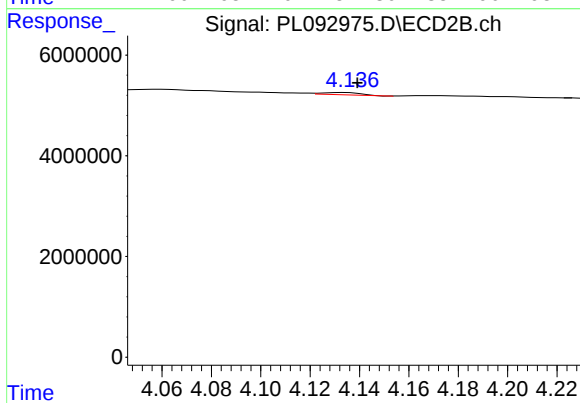

#7 delta-BHC


R.T.: 4.134 min
Delta R.T.: -0.005 min
Response: 473045
Conc: 0.12 ng/ml

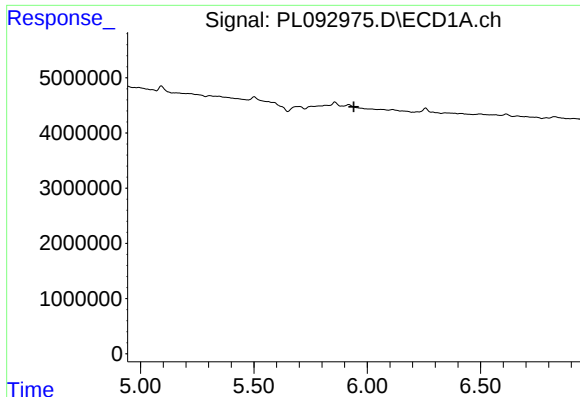

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.941 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WC-2(0-6)

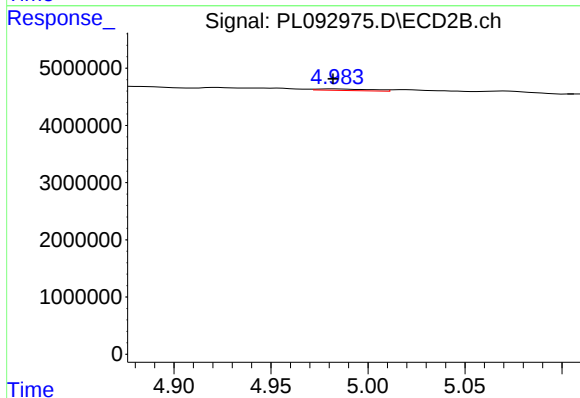


#10 gamma-Chlordane

R.T.: 4.982 min
Delta R.T.: 0.000 min
Response: 529148
Conc: 0.16 ng/ml

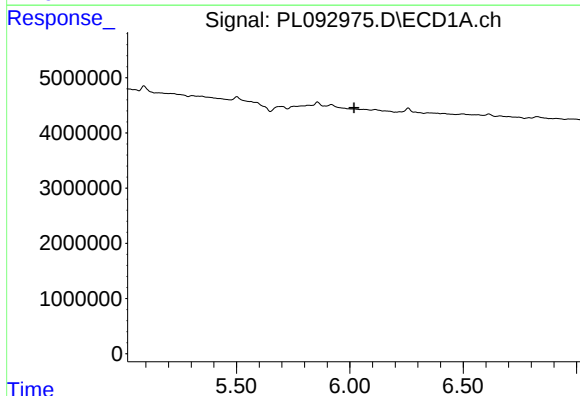


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 6.019 min
Response: 0
Conc: N.D.

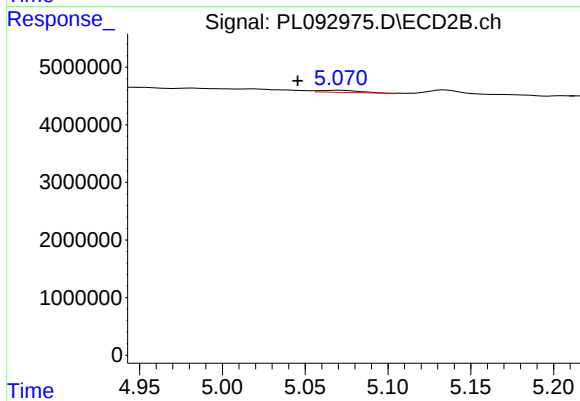

#11 alpha-Chlordane


R.T.: 5.071 min
Delta R.T.: 0.026 min
Response: 569671
Conc: 0.17 ng/ml

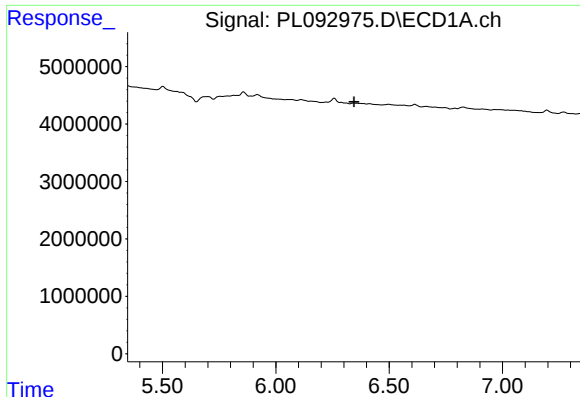

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.345 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WC-2(0-6)

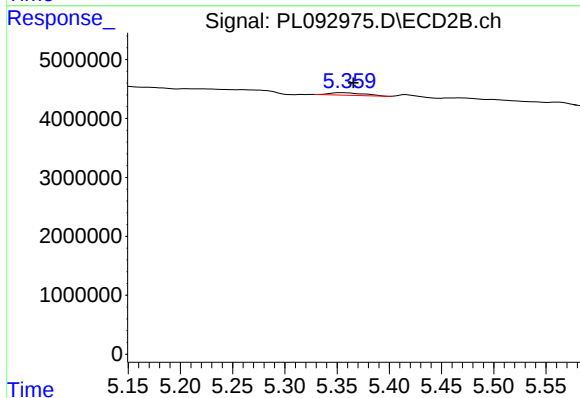


#13 Dieldrin

R.T.: 5.354 min
Delta R.T.: -0.012 min
Response: 968501
Conc: 0.29 ng/ml

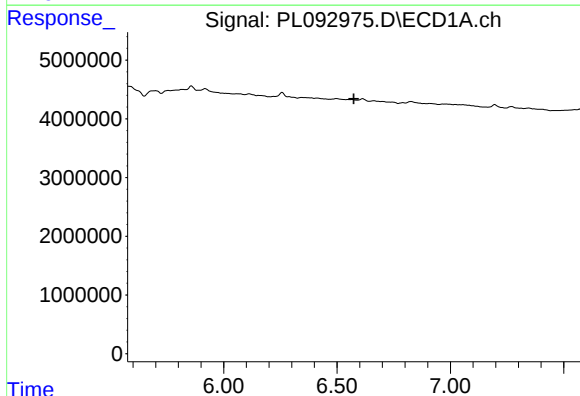


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.574 min
Response: 0
Conc: N.D.

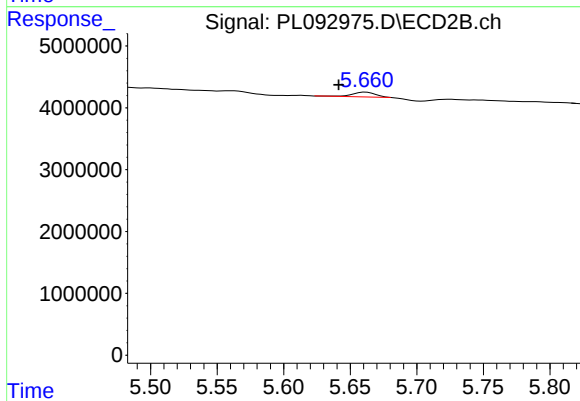

#14 Endrin


R.T.: 5.662 min
Delta R.T.: 0.020 min
Response: 901706
Conc: 0.31 ng/ml

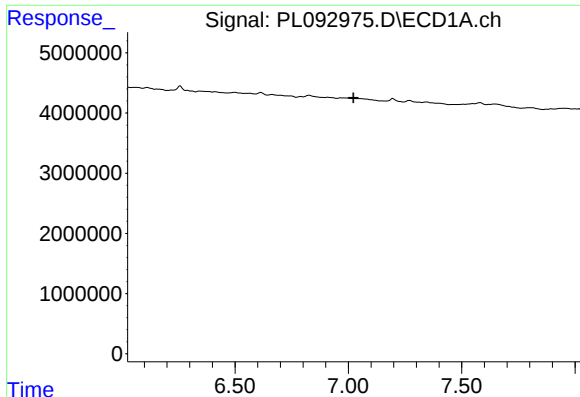

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.023 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WC-2(0-6)

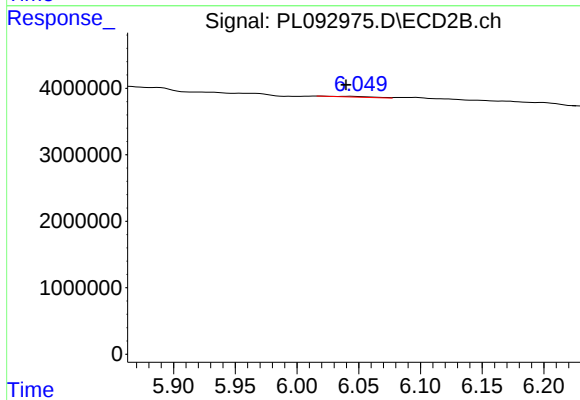


#17 4,4'-DDT

R.T.: 6.043 min
Delta R.T.: 0.003 min
Response: 269060
Conc: 0.10 ng/ml

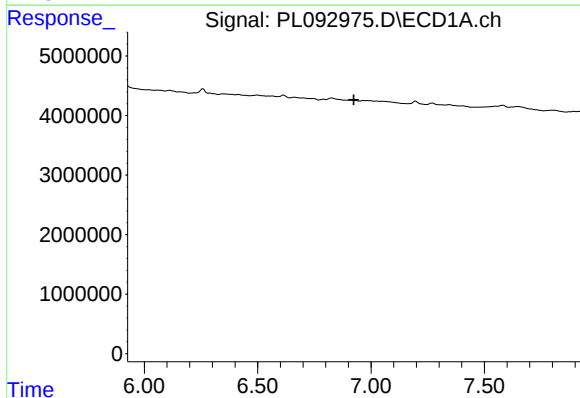


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.924 min
Response: 0
Conc: N.D.

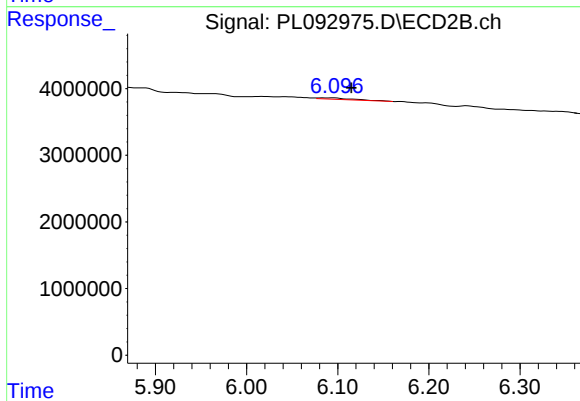

#18 Endrin aldehyde


R.T.: 6.096 min
Delta R.T.: -0.019 min
Response: 469592
Conc: 0.20 ng/ml

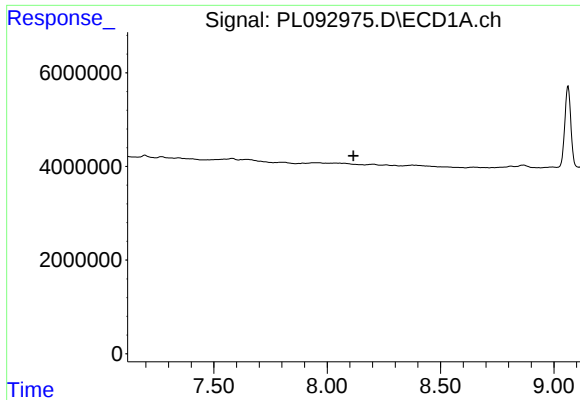

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 8.116 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WC-2(0-6)

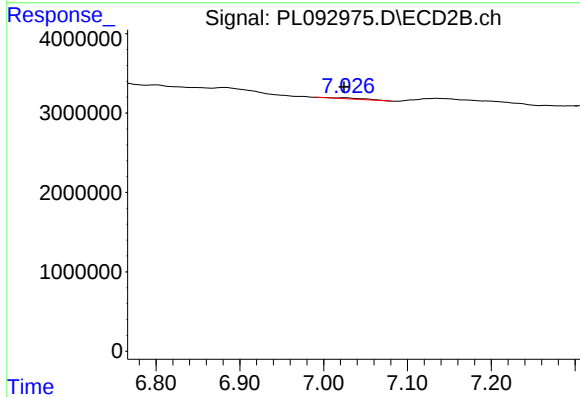


#22 Mirex

R.T.: 7.025 min
Delta R.T.: 0.001 min
Response: 316125
Conc: 0.12 ng/ml

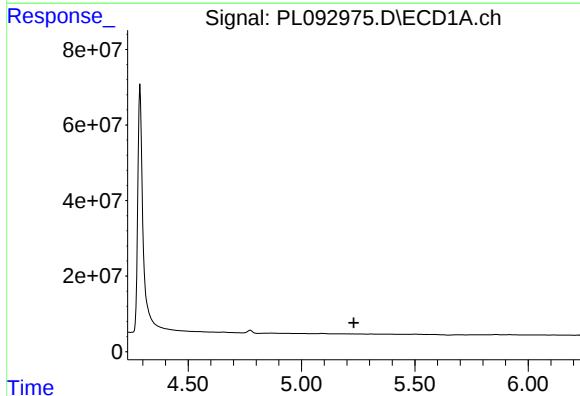


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.231 min
Response: 0
Conc: N.D.

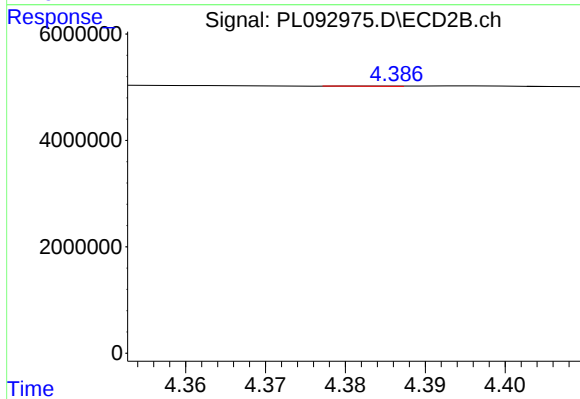

#24 Chlordane-2


R.T.: 4.383 min
Delta R.T.: 0.031 min
Response: 22215
Conc: 0.18 ng/ml

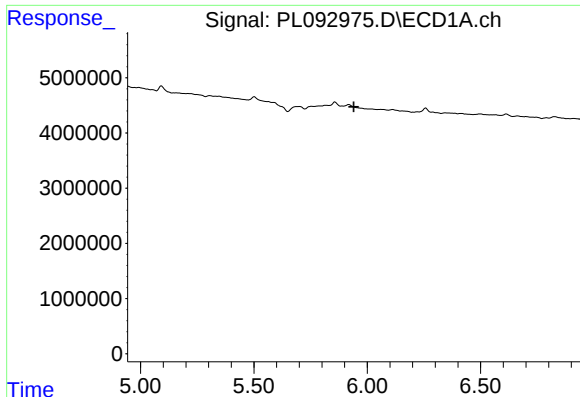

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.941 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WC-2(0-6)

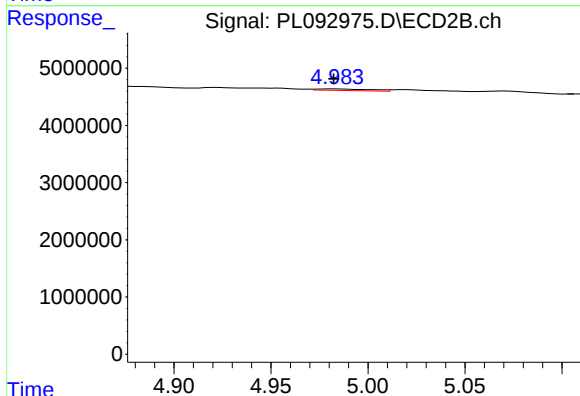


#25 Chlordane-3

R.T.: 4.982 min
Delta R.T.: 0.000 min
Response: 529148
Conc: 1.46 ng/ml

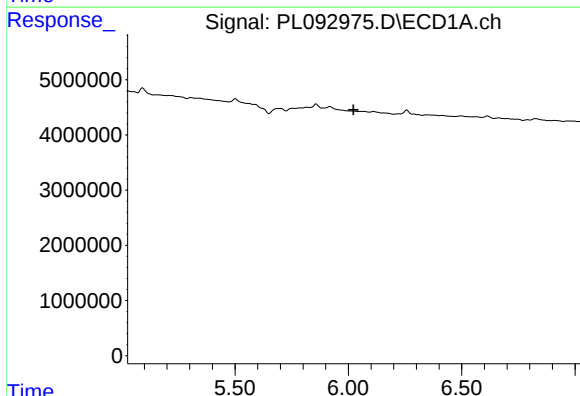


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.023 min
Response: 0
Conc: N.D.

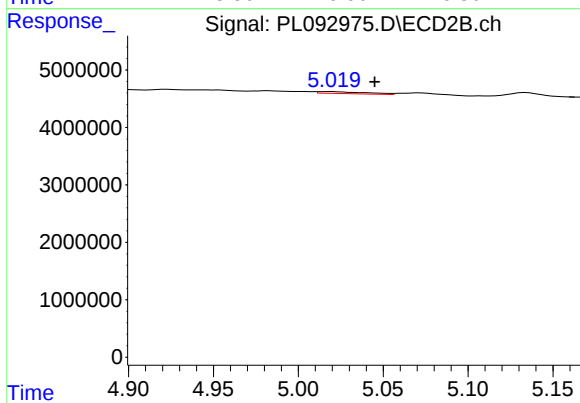

#26 Chlordane-4


R.T.: 5.019 min
Delta R.T.: -0.026 min
Response: 656594
Conc: 1.88 ng/ml

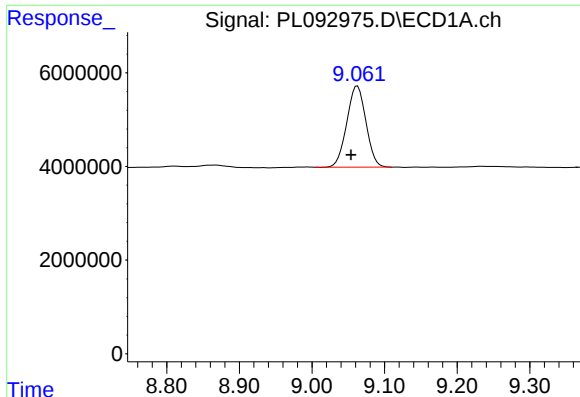

#28 Decachlorobiphenyl

R.T.: 9.063 min
Delta R.T.: 0.009 min
Response: 31739699
Conc: 16.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-2(0-6)

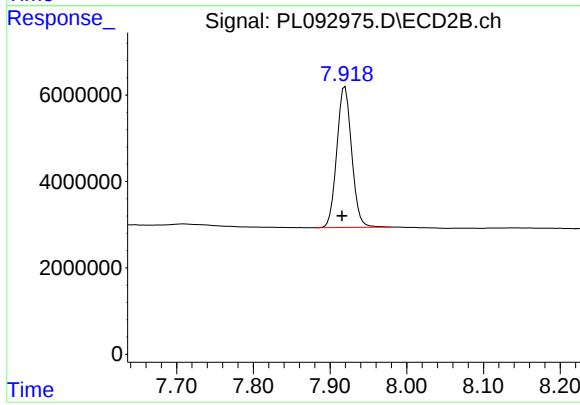

#28 Decachlorobiphenyl

R.T.: 7.920 min
Delta R.T.: 0.004 min
Response: 43903803
Conc: 16.09 ng/ml