

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111124\
 Data File : PL092980.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2024 22:05
 Operator : AR\AJ
 Sample : P4789-01
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BP-F21

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/12/2024
 Supervised By :Ankita Jodhani 11/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 00:34:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.778	57596171	61642108	23.506m	22.653
28) SA Decachlor...	9.061	7.919	33542994	44869429	17.429	16.440

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111124\
Data File : PL092980.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2024 22:05
Operator : AR\AJ
Sample : P4789-01
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BP-F21


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/12/2024
Supervised By : Ankita Jodhani 11/12/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 00:34:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

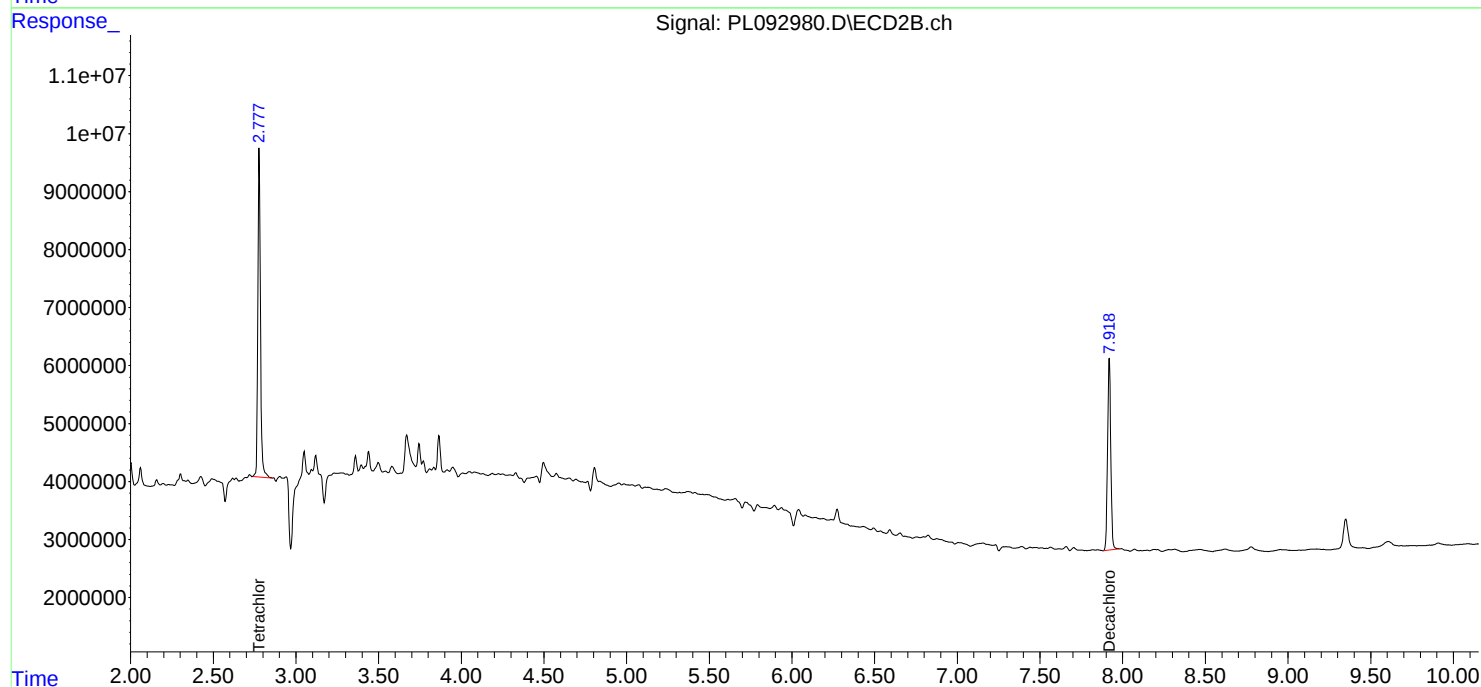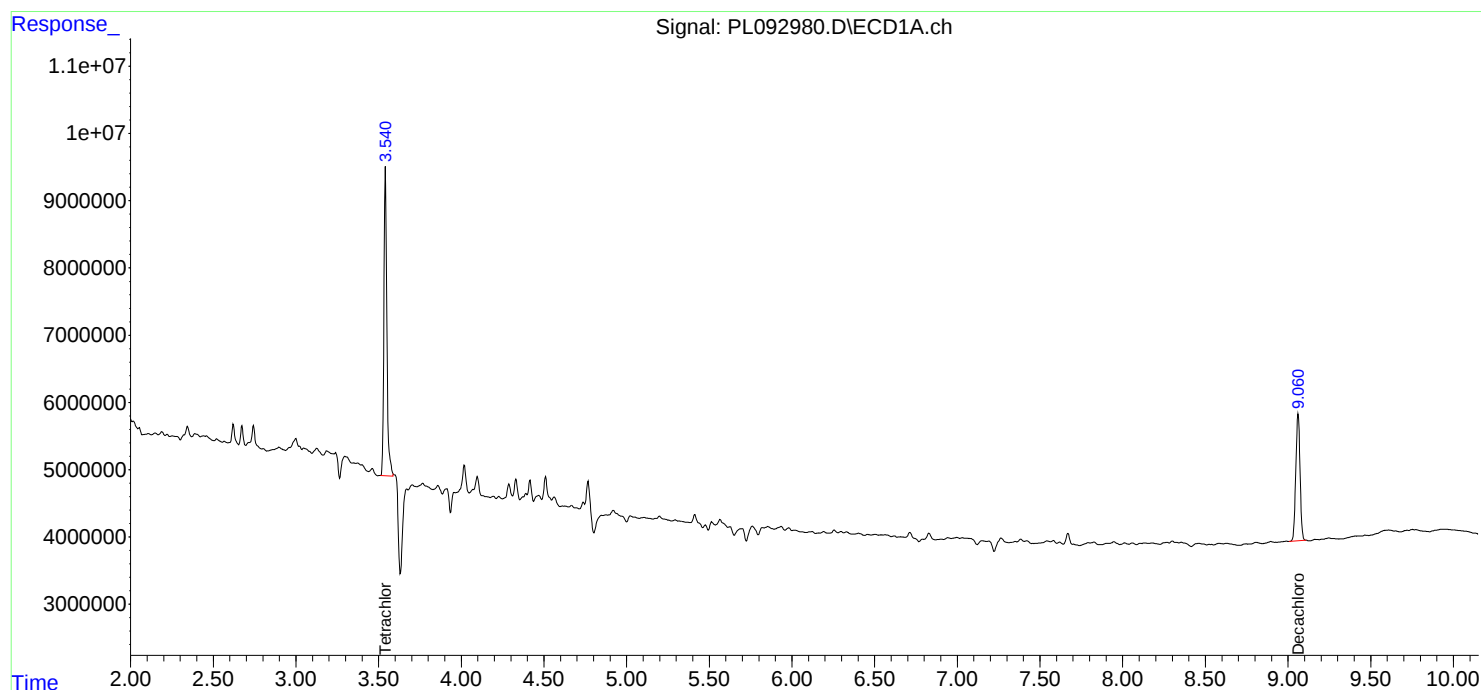

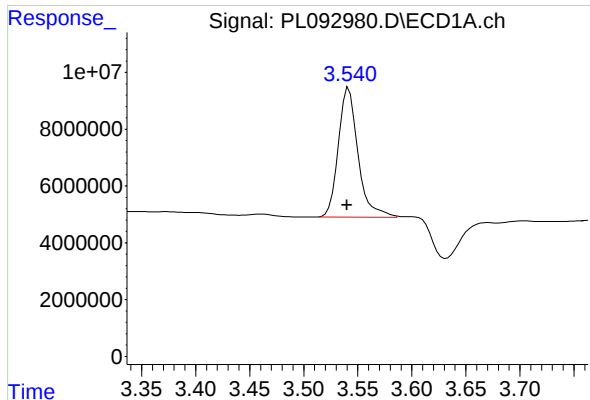


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: 0.000 min
Response: 57596171
Conc: 23.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
BP-F21


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/12/2024
Supervised By :Ankita Jodhani 11/12/2024

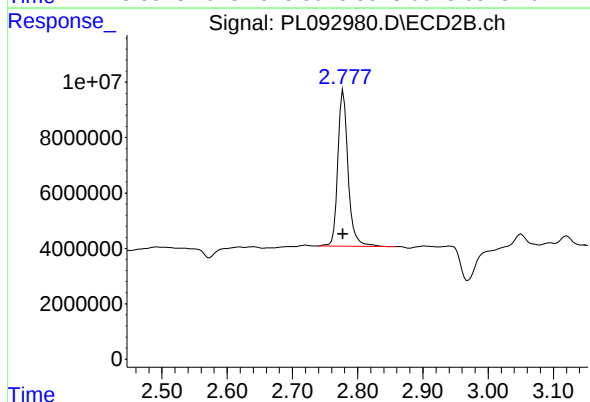


#1 Tetrachloro-m-xylene

R.T.: 2.778 min
Delta R.T.: 0.000 min
Response: 61642108
Conc: 22.65 ng/ml

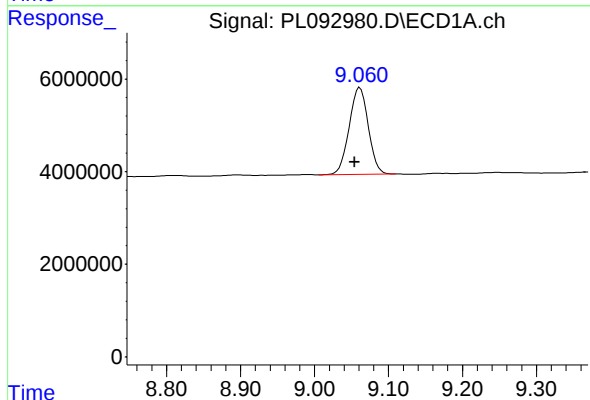

#28 Decachlorobiphenyl

R.T.: 9.061 min
Delta R.T.: 0.007 min
Response: 33542994
Conc: 17.43 ng/ml

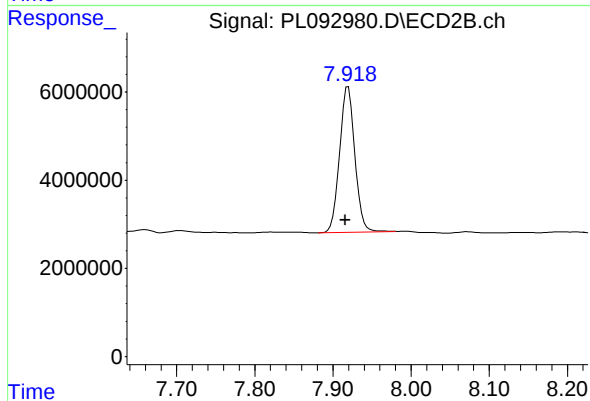

#28 Decachlorobiphenyl

R.T.: 7.919 min
Delta R.T.: 0.004 min
Response: 44869429
Conc: 16.44 ng/ml