

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111218\
 Data File : PL042049.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2018 14:20
 Operator : AJ\SJ
 Sample : J5887-15RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 03:34:51 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	4.102	31058472	15998504	5.030	5.400
28)	SA Decachlor...	8.207	9.230	42678620	17851912	6.230	6.999
Target Compounds							
6)	B beta-BHC	4.403f	0.000	3493447	0	0.947	N.D. #
10)	B gamma-Chl...	5.422	0.000	1908064	0	0.237	N.D. #
11)	B alpha-Chl...	5.422f	0.000	1908064	0	0.239	N.D. #
12)	B 4,4'-DDE	5.626	0.000	1698441	0	0.248	N.D. #
23)	Chlordane-1	4.337	0.000	874677	0	2.931	N.D. #
24)	Chlordane-2	4.838	0.000	3055570	0	9.632	N.D. #
25)	Chlordane-3	5.422	0.000	1908064	0	2.041	N.D. #
26)	Chlordane-4	5.422	0.000	1908064	0	2.284	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111218\
Data File : PL042049.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2018 14:20
Operator : AJ\SJ
Sample : J5887-15RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 03:34:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

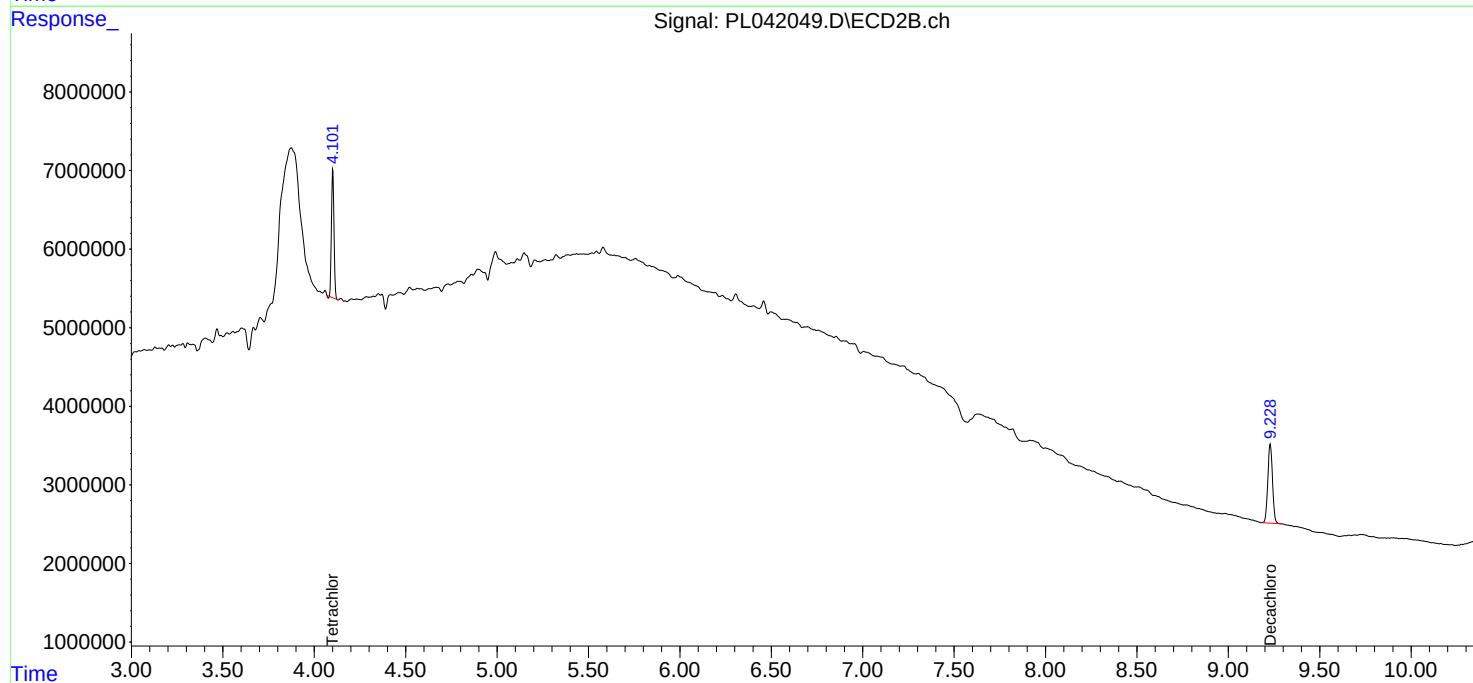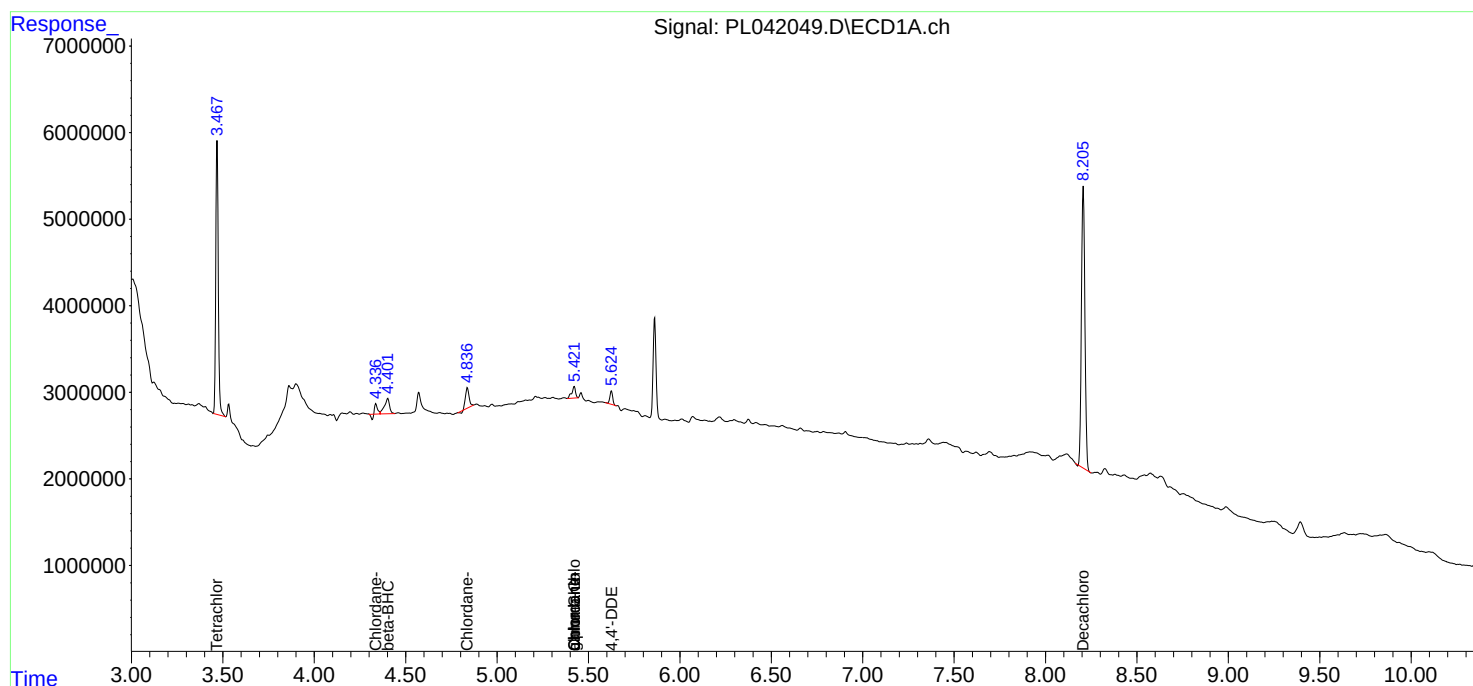


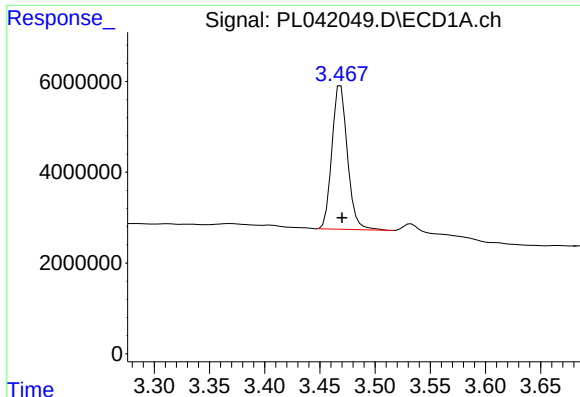

#1 Tetrachloro-m-xylene


R.T.: 3.469 min
Delta R.T.: -0.001 min
Response: 31058472
Conc: 5.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

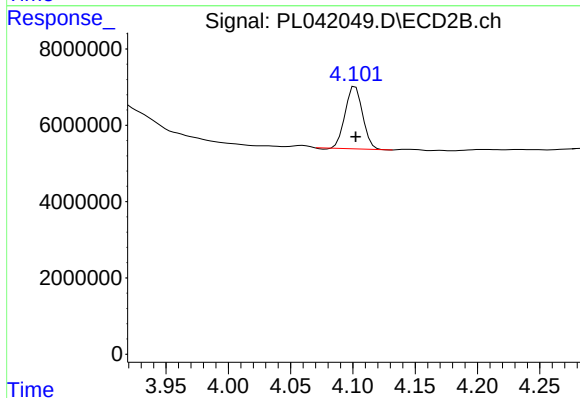


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 15998504
Conc: 5.40 ng/ml

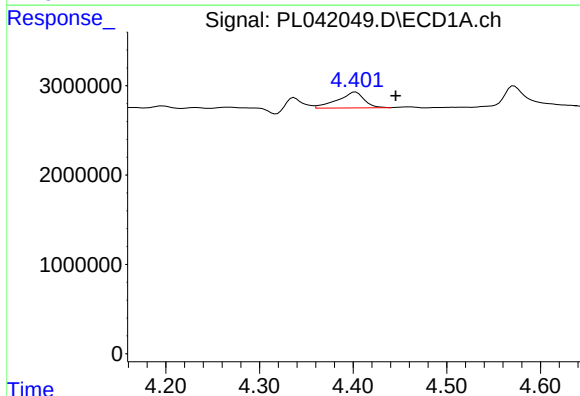


#6 beta-BHC

R.T.: 4.403 min
Delta R.T.: -0.043 min
Response: 3493447
Conc: 0.95 ng/ml

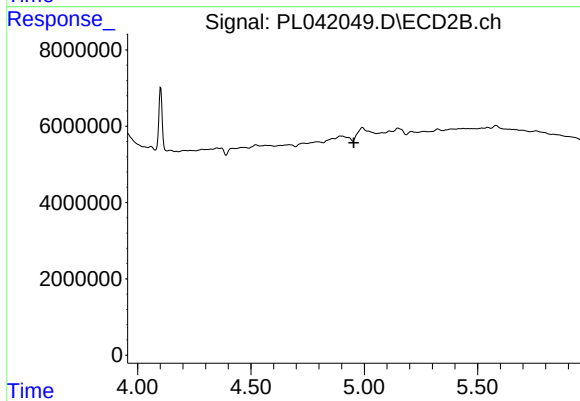

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

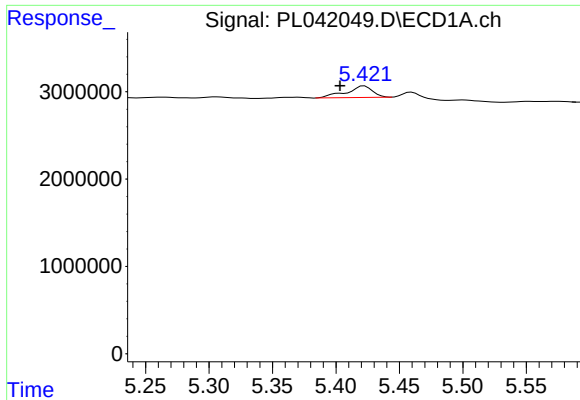

#10 gamma-Chlordane


R.T.: 5.422 min
Delta R.T.: 0.019 min
Response: 1908064
Conc: 0.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

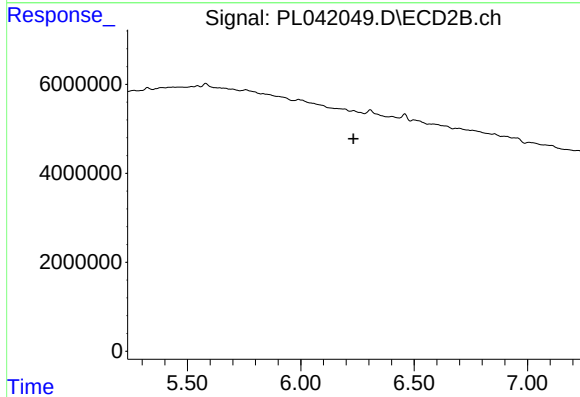


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.233 min
Response: 0
Conc: N.D.

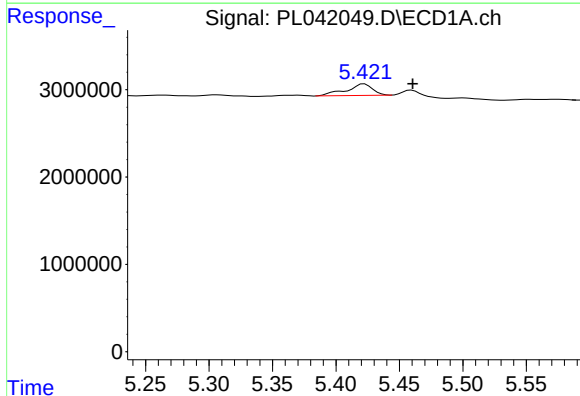


#11 alpha-Chlordane

R.T.: 5.422 min
Delta R.T.: -0.038 min
Response: 1908064
Conc: 0.24 ng/ml

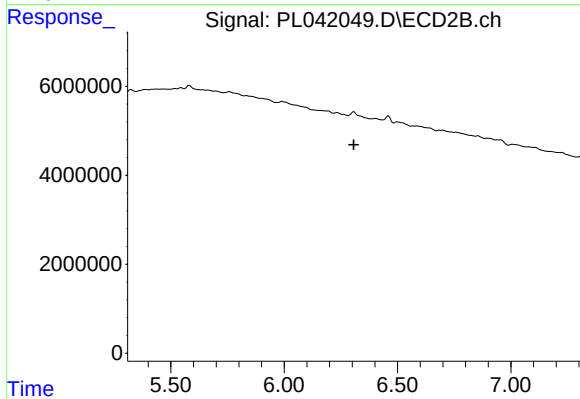

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.307 min
Response: 0
Conc: N.D.

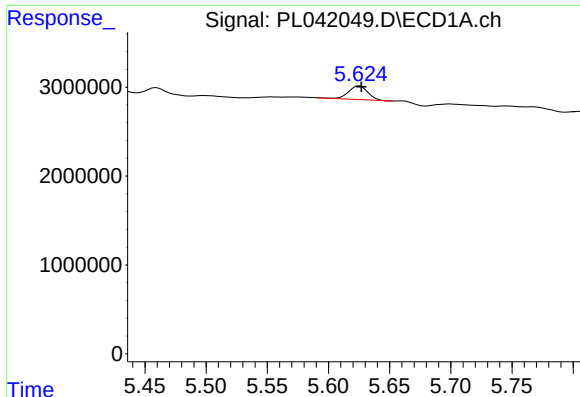

#12 4,4'-DDE


R.T.: 5.626 min
Delta R.T.: -0.001 min
Response: 1698441
Conc: 0.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

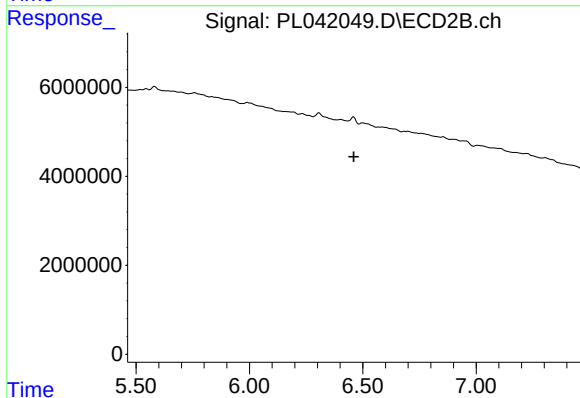


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.461 min
Response: 0
Conc: N.D.

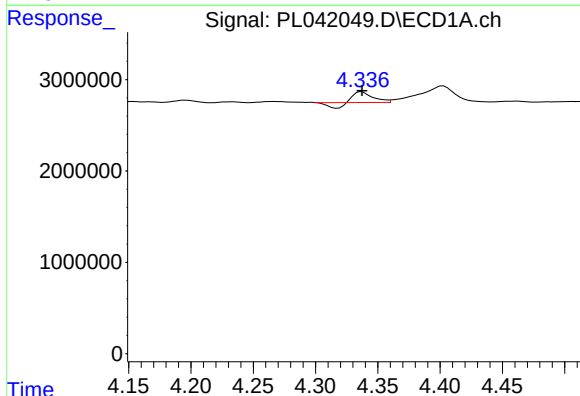


#23 Chlordane-1

R.T.: 4.337 min
Delta R.T.: 0.000 min
Response: 874677
Conc: 2.93 ng/ml

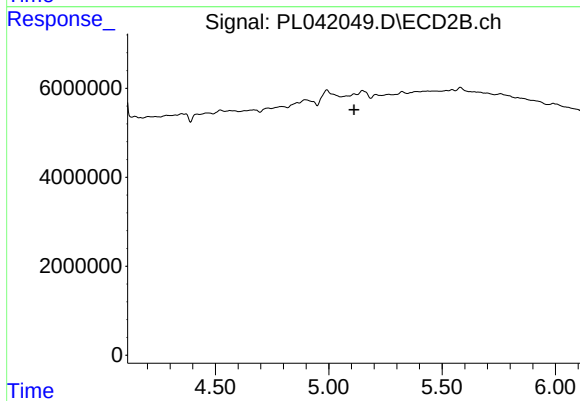

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.112 min
Response: 0
Conc: N.D.

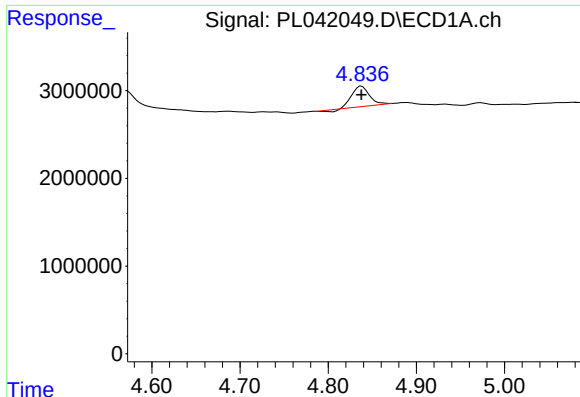

#24 Chlordane-2


R.T.: 4.838 min
Delta R.T.: 0.000 min
Response: 3055570
Conc: 9.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

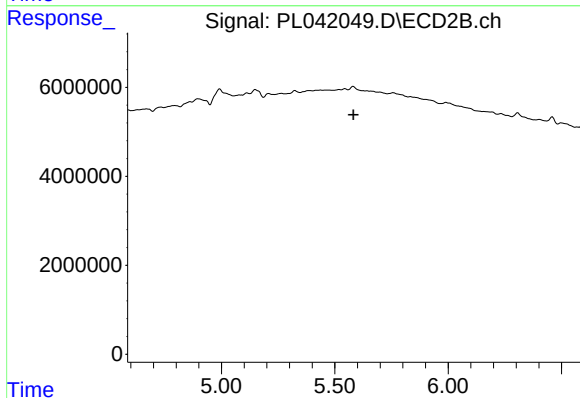


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.583 min
Response: 0
Conc: N.D.

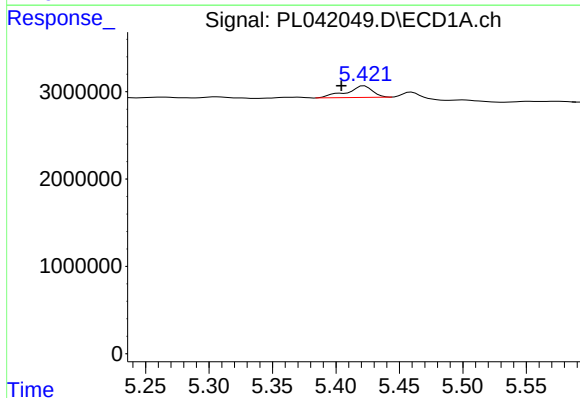


#25 Chlordane-3

R.T.: 5.422 min
Delta R.T.: 0.018 min
Response: 1908064
Conc: 2.04 ng/ml

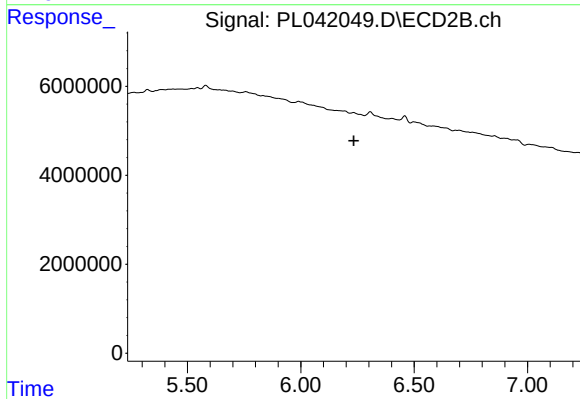

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.234 min
Response: 0
Conc: N.D.

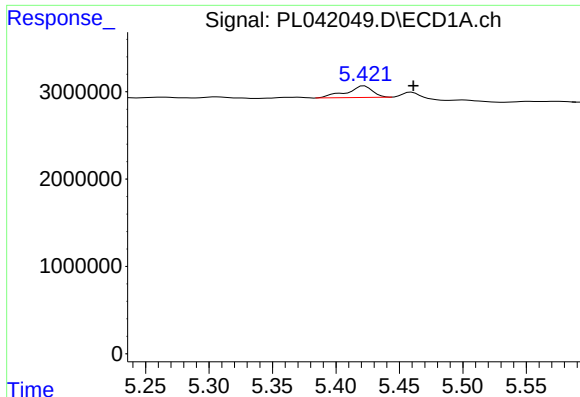

#26 Chlordane-4


R.T.: 5.422 min
Delta R.T.: -0.039 min
Response: 1908064
Conc: 2.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

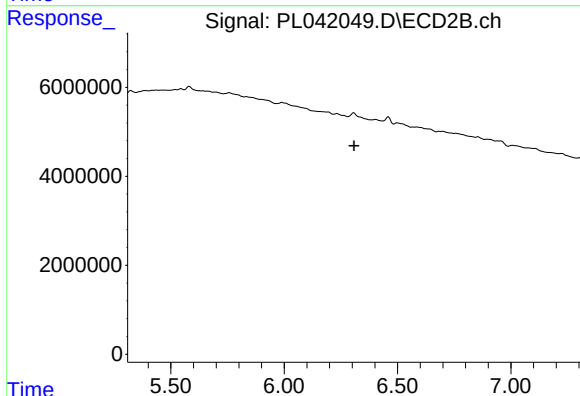


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.309 min
Response: 0
Conc: N.D.

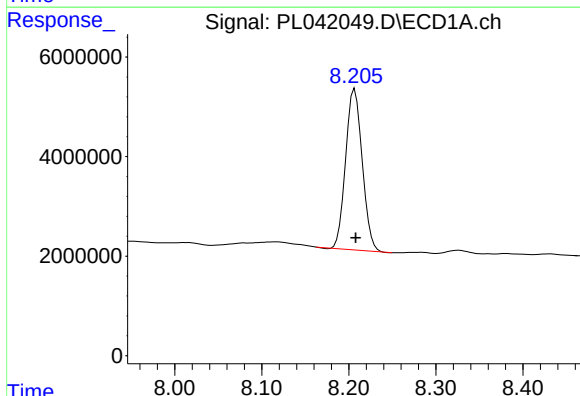

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: -0.001 min
Response: 42678620
Conc: 6.23 ng/ml

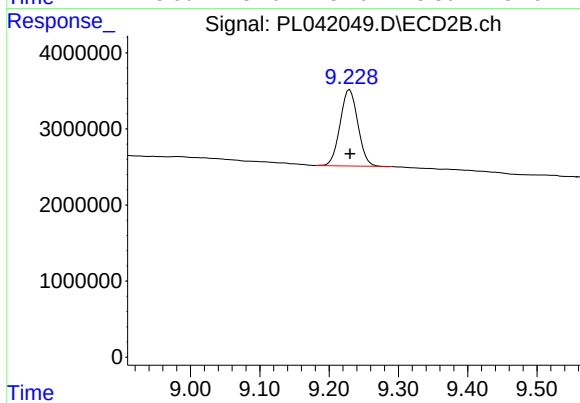

#28 Decachlorobiphenyl

R.T.: 9.230 min
Delta R.T.: 0.000 min
Response: 17851912
Conc: 7.00 ng/ml