

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111218\
 Data File : PL042064.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2018 18:36
 Operator : AJ\SJ
 Sample : J5269-14
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 03:37:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	4.102	111.7E6	58059605	18.088	19.597
28)	SA Decachlor...	8.207	9.229	120.1E6	50282296	17.535	19.714
Target Compounds							
2)	A alpha-BHC	3.905	4.503	3514794	-489085	0.371	N.D. #
3)	MA gamma-BHC...	4.200	0.000	2193704	0	0.254	N.D. #
6)	B beta-BHC	4.404f	0.000	21276487	0	5.765	N.D. #
8)	B Heptachlo...	5.243f	5.996	4810010	2956236	0.610	0.823 #
9)	A Endosulfan I	5.542	0.000	1377949	0	0.189	N.D. #
19)	B Endosulfa...	6.656	7.383	6897616	2892752	1.082	1.064
20)	A Methoxychlor	0.000	7.646f	0	4017424	N.D.	2.924 #
21)	B Endrin ke...	7.202f	0.000	1792919	0	0.249	N.D. #
23)	Chlordane-1	4.404	0.000	21276487	0	71.292	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111218\
Data File : PL042064.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2018 18:36
Operator : AJ\SJ
Sample : J5269-14
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 03:37:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

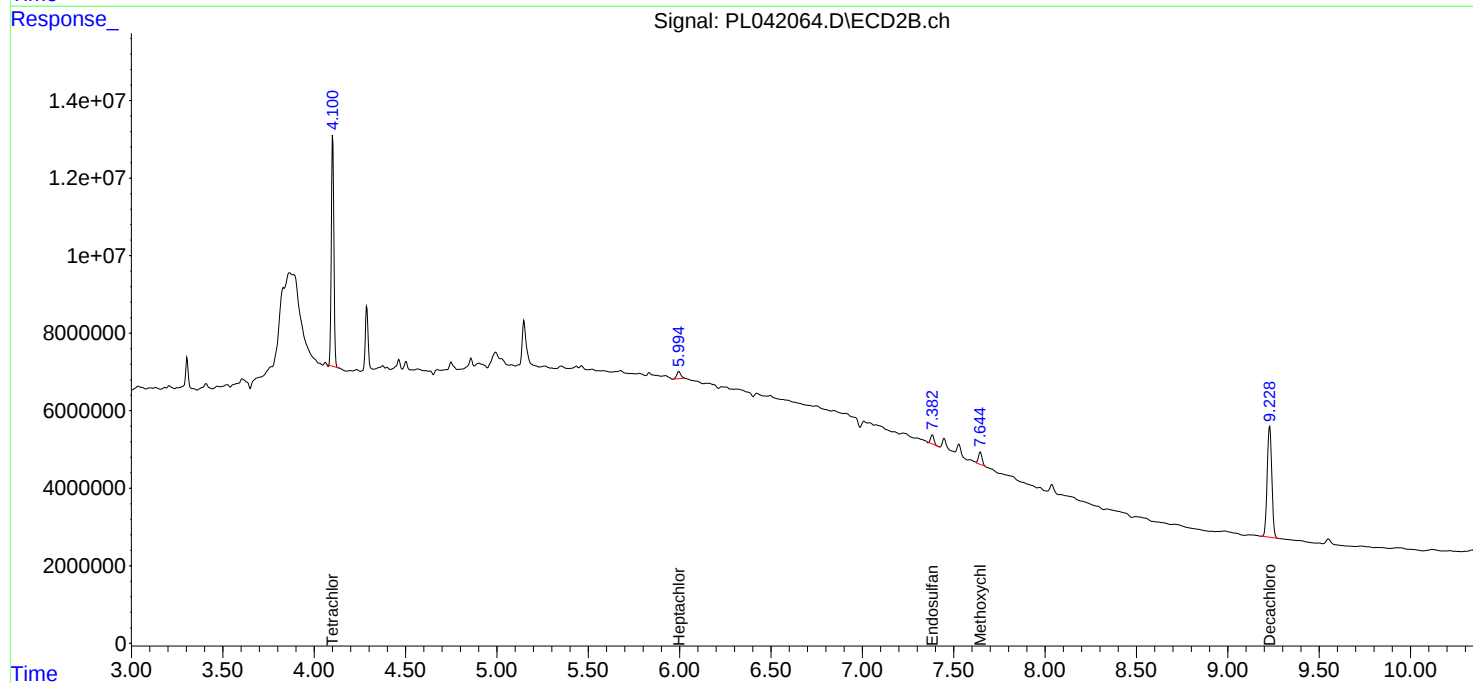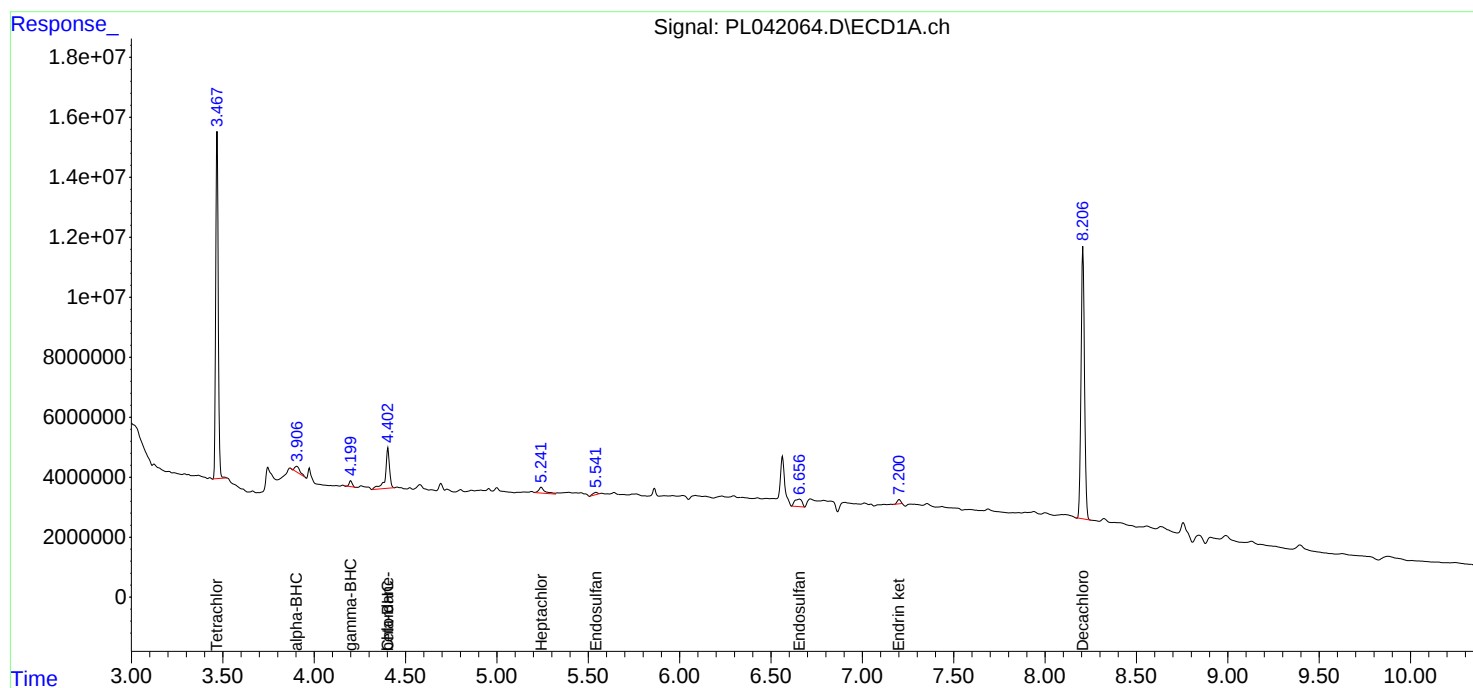


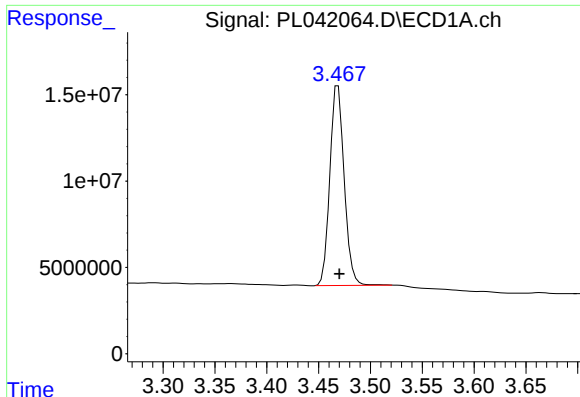

#1 Tetrachloro-m-xylene


R.T.: 3.469 min
Delta R.T.: -0.001 min
Response: 111693783
Conc: 18.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

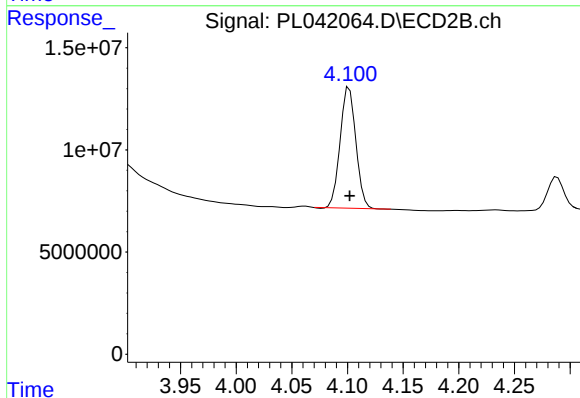


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 58059605
Conc: 19.60 ng/ml

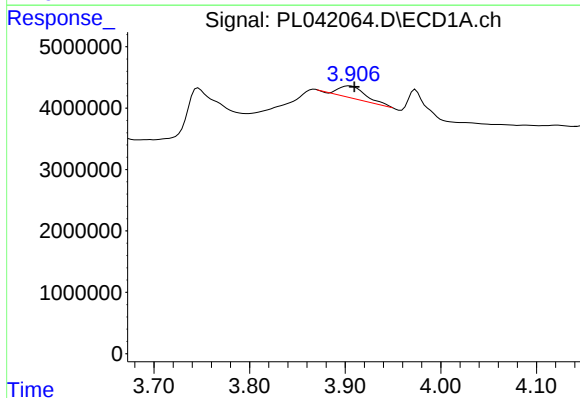


#2 alpha-BHC

R.T.: 3.905 min
Delta R.T.: -0.005 min
Response: 3514794
Conc: 0.37 ng/ml

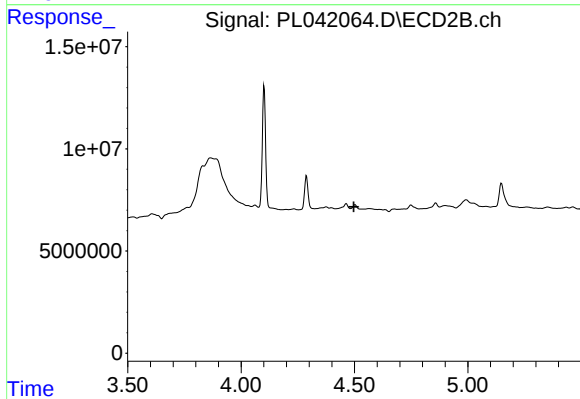

#2 alpha-BHC


R.T.: 4.503 min
Delta R.T.: 0.005 min
Response: -489085
Conc: N.D.

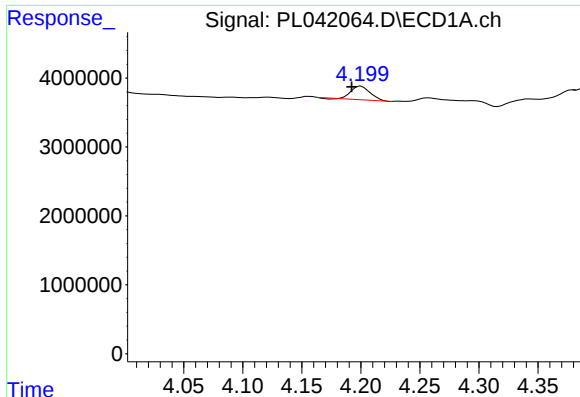

#3 gamma-BHC (Lindane)


R.T.: 4.200 min
Delta R.T.: 0.008 min
Response: 2193704
Conc: 0.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

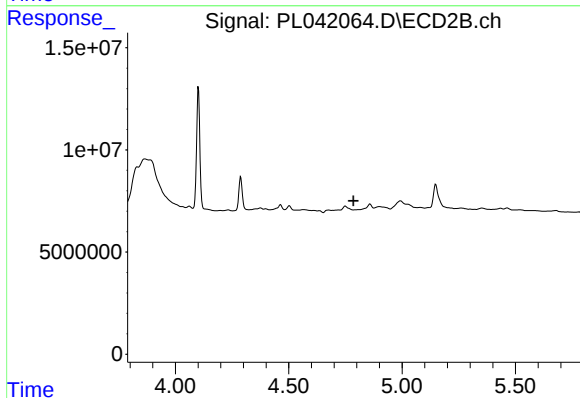


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.786 min
Response: 0
Conc: N.D.

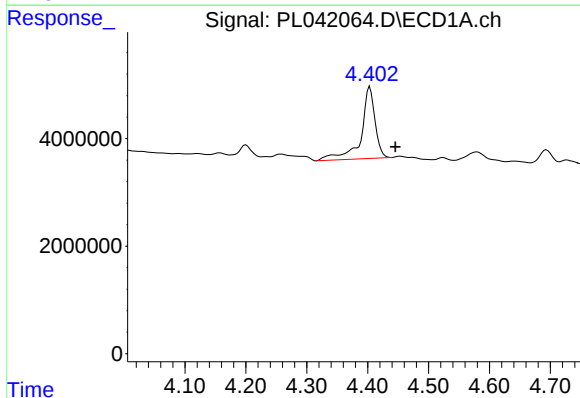


#6 beta-BHC

R.T.: 4.404 min
Delta R.T.: -0.042 min
Response: 21276487
Conc: 5.77 ng/ml

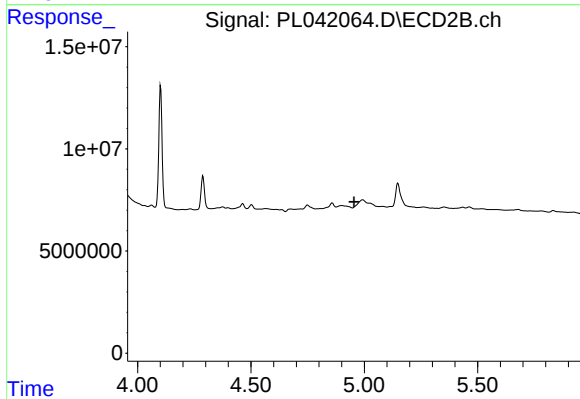

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

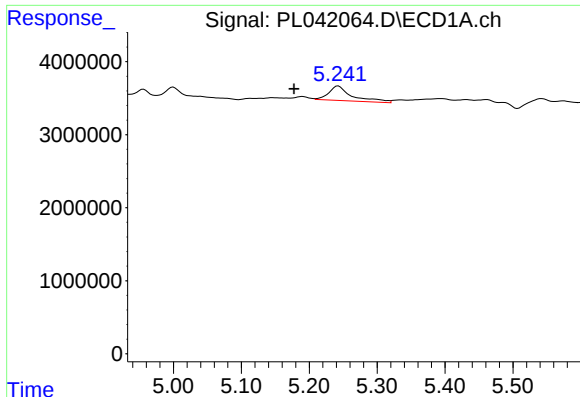

#8 Heptachlor epoxide


R.T.: 5.243 min
Delta R.T.: 0.065 min
Response: 4810010
Conc: 0.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

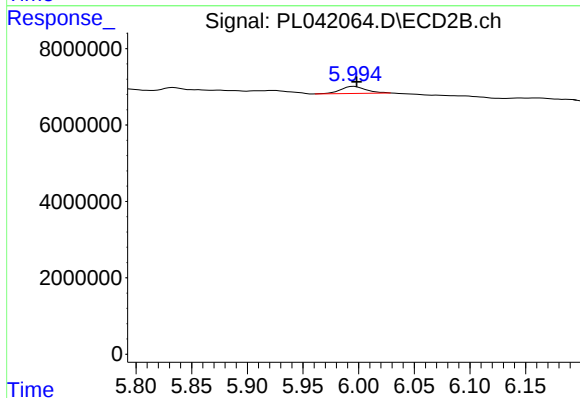


#8 Heptachlor epoxide

R.T.: 5.996 min
Delta R.T.: -0.003 min
Response: 2956236
Conc: 0.82 ng/ml

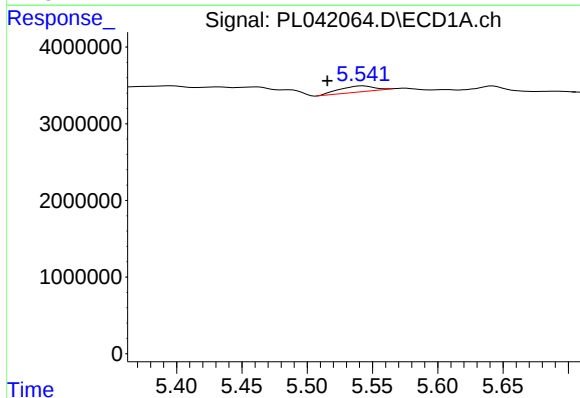


#9 Endosulfan I

R.T.: 5.542 min
Delta R.T.: 0.027 min
Response: 1377949
Conc: 0.19 ng/ml

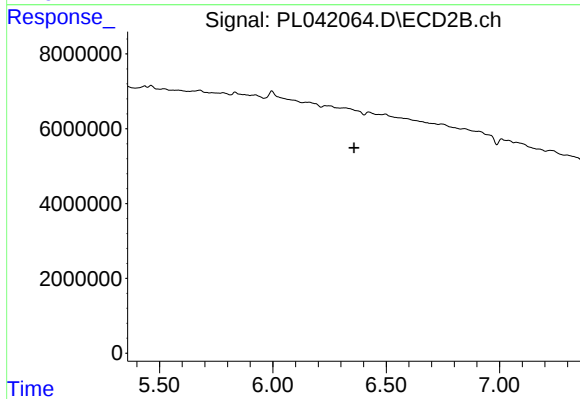

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.358 min
Response: 0
Conc: N.D.

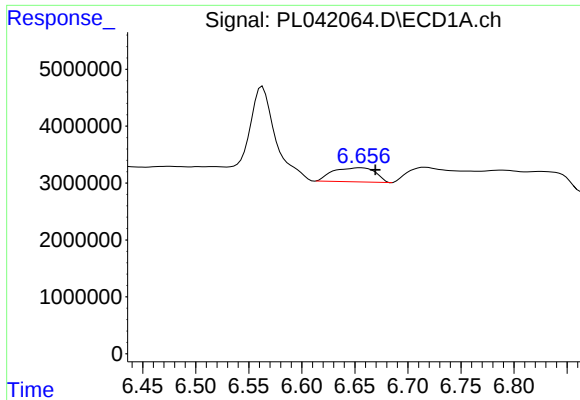

#19 Endosulfan Sulfate


R.T.: 6.656 min
Delta R.T.: -0.013 min
Response: 6897616
Conc: 1.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

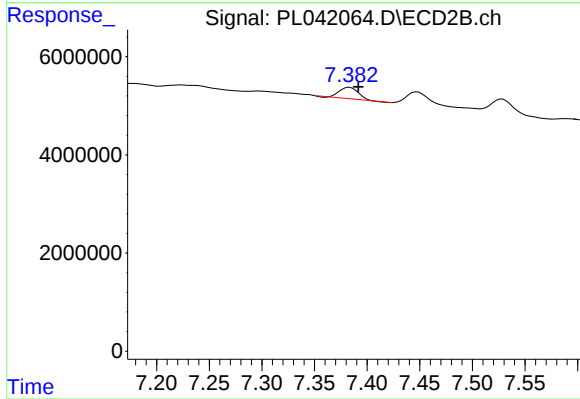


#19 Endosulfan Sulfate

R.T.: 7.383 min
Delta R.T.: -0.008 min
Response: 2892752
Conc: 1.06 ng/ml

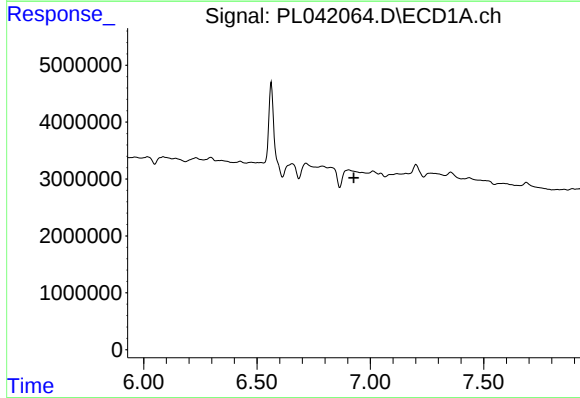


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.928 min
Response: 0
Conc: N.D.

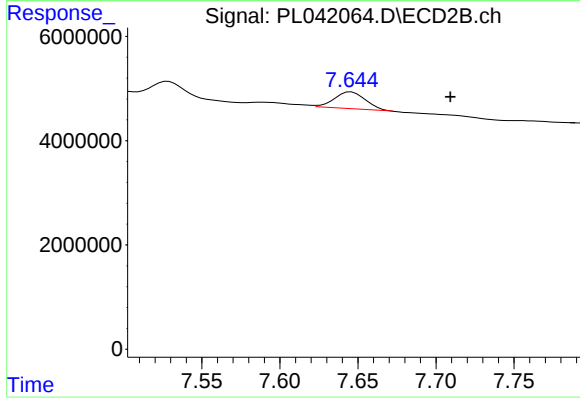

#20 Methoxychlor


R.T.: 7.646 min
Delta R.T.: -0.063 min
Response: 4017424
Conc: 2.92 ng/ml

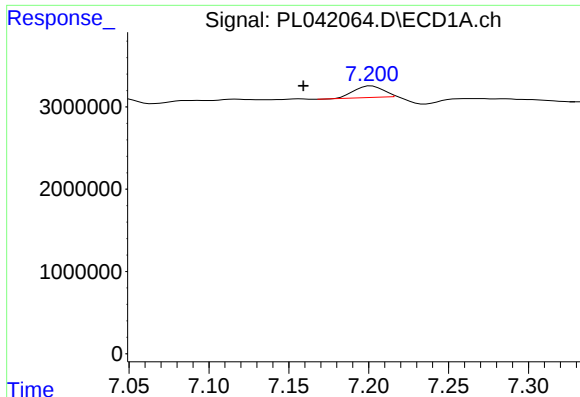

#21 Endrin ketone


R.T.: 7.202 min
Delta R.T.: 0.042 min
Response: 1792919
Conc: 0.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

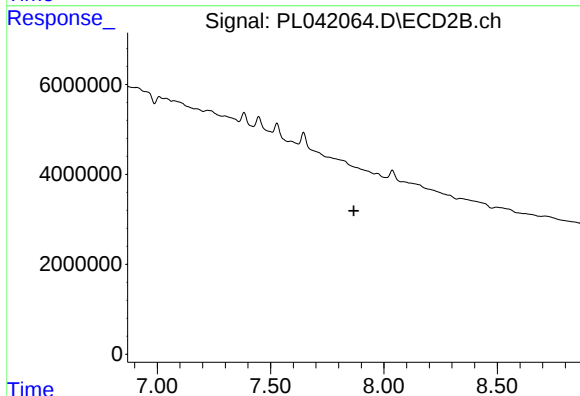


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.867 min
Response: 0
Conc: N.D.

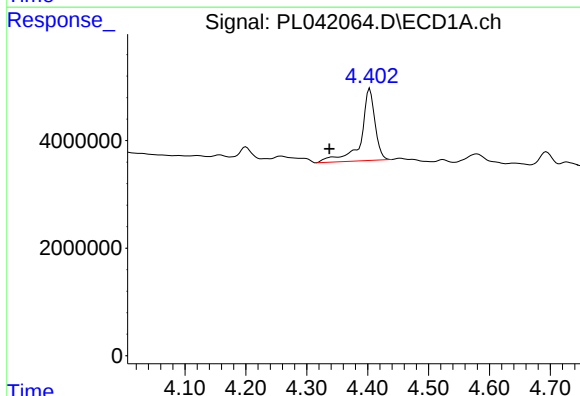


#23 Chlordane-1

R.T.: 4.404 min
Delta R.T.: 0.066 min
Response: 21276487
Conc: 71.29 ng/ml

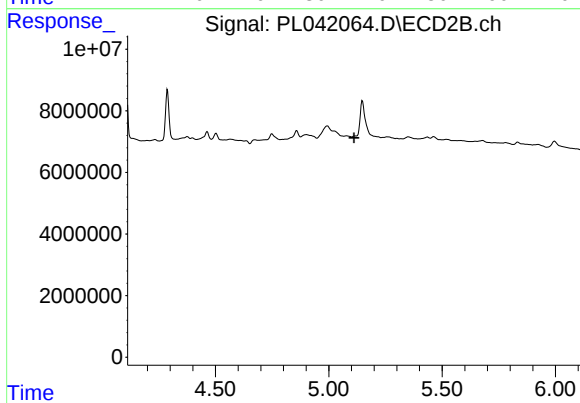

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.112 min
Response: 0
Conc: N.D.

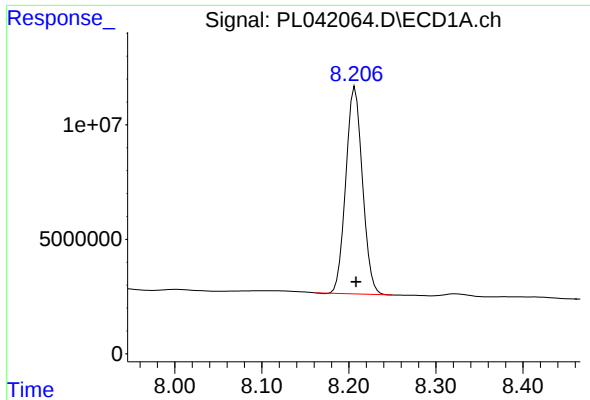

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 120120859
Conc: 17.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

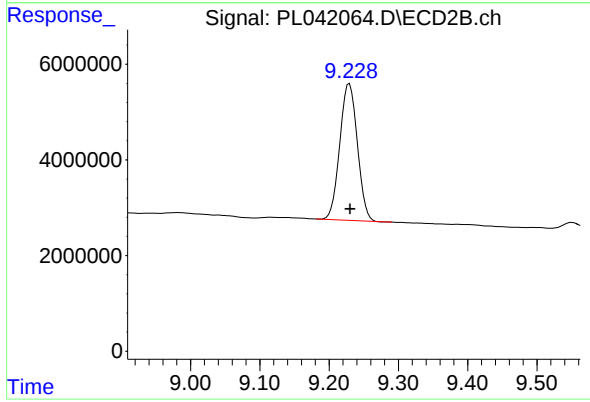

#28 Decachlorobiphenyl

R.T.: 9.229 min
Delta R.T.: -0.001 min
Response: 50282296
Conc: 19.71 ng/ml