

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111218\
 Data File : PL042074.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2018 20:57
 Operator : AJ\SJ
 Sample : J5766-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 03:38:26 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	4.102	120.0E6	64111732	19.427	21.640
28)	SA Decachlor...	8.207	9.231	107.4E6	47766023	15.675	18.727
Target Compounds							
3)	MA gamma-BHC...	0.000	4.832f	0	736354	N.D.	0.179 #
6)	B beta-BHC	4.403f	0.000	11697797	0	3.170	N.D. #
8)	B Heptachlo...	0.000	5.997	0	2629472	N.D.	0.732 #
9)	A Endosulfan I	5.525	0.000	3238741	0	0.444	N.D. #
11)	B alpha-Chl...	5.525f	0.000	3238741	0	0.406	N.D. #
16)	A 4,4'-DDD	6.141	0.000	2123356	0	0.384	N.D. #
19)	B Endosulfa...	6.664	0.000	2265762	0	0.355	N.D. #
23)	Chlordane-1	4.379	0.000	2943993	0	9.865	N.D. #
26)	Chlordane-4	5.525	0.000	3238741	0	3.876	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111218\
Data File : PL042074.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2018 20:57
Operator : AJ\SJ
Sample : J5766-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 03:38:26 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

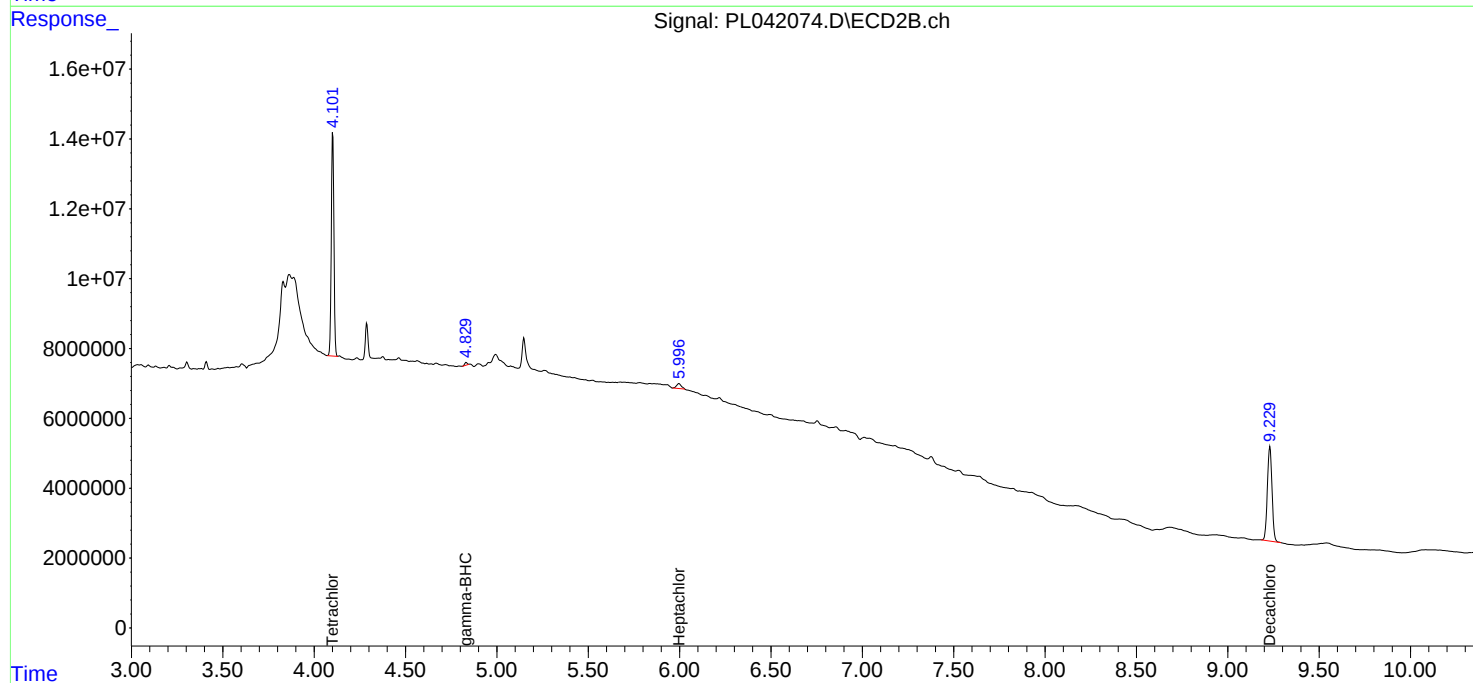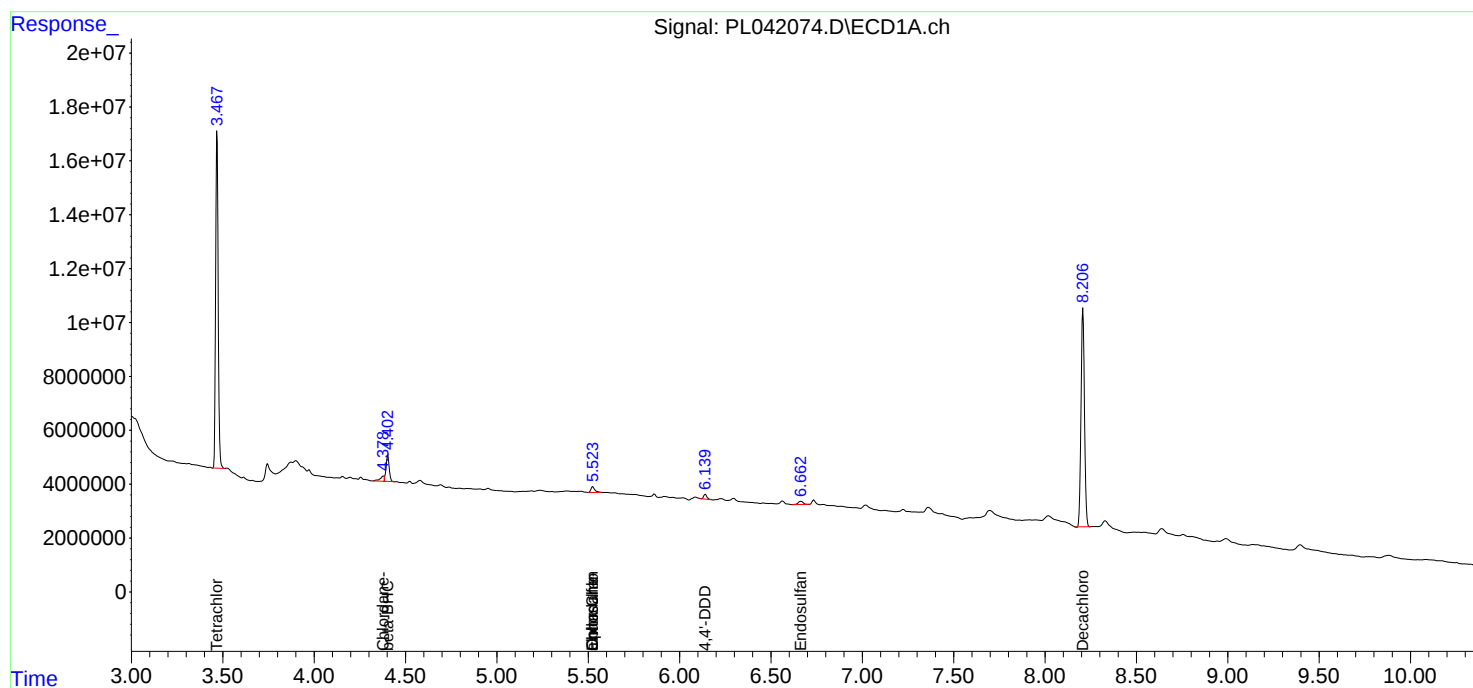


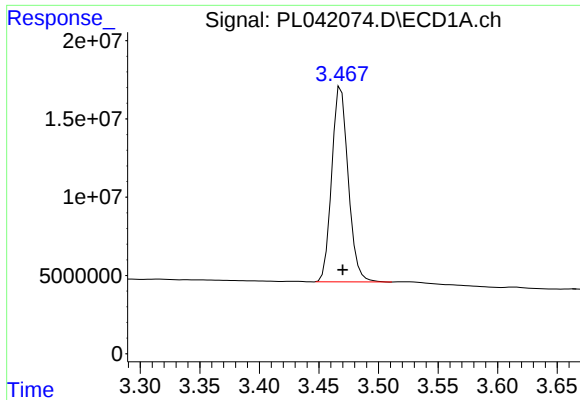

#1 Tetrachloro-m-xylene


R.T.: 3.469 min
Delta R.T.: -0.001 min
Response: 119961100
Conc: 19.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

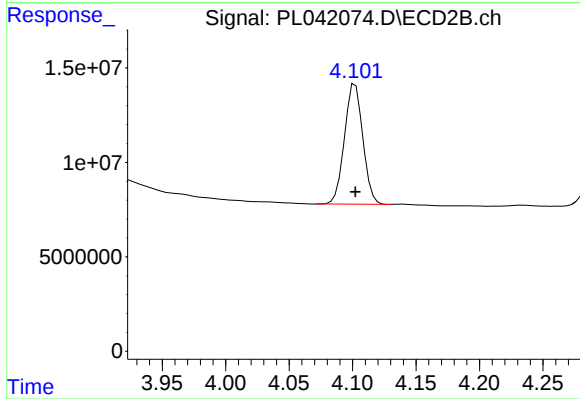


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 64111732
Conc: 21.64 ng/ml

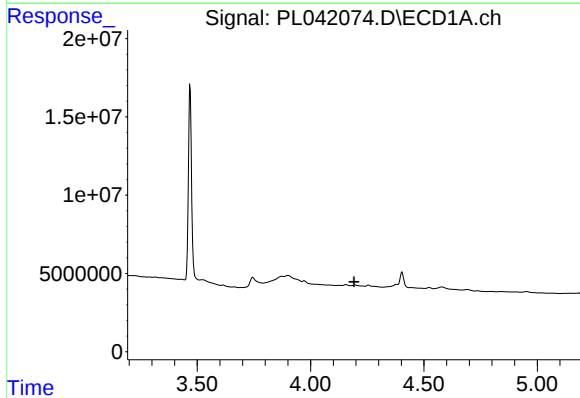


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.192 min
Response: 0
Conc: N.D.

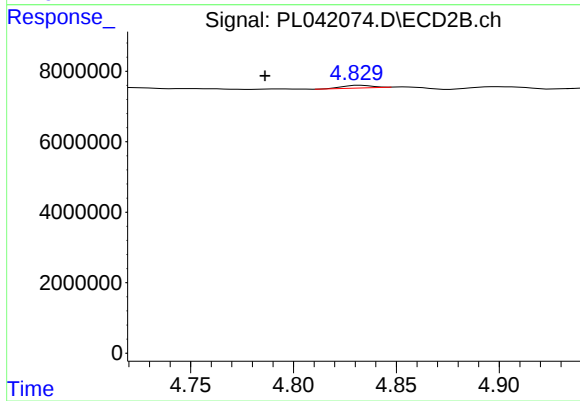

#3 gamma-BHC (Lindane)


R.T.: 4.832 min
Delta R.T.: 0.046 min
Response: 736354
Conc: 0.18 ng/ml

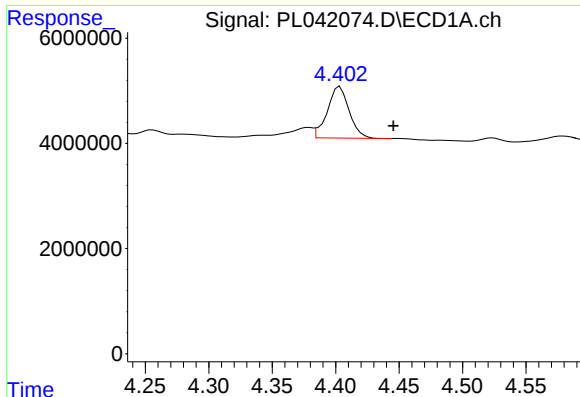

#6 beta-BHC


R.T.: 4.403 min
Delta R.T.: -0.042 min
Response: 11697797
Conc: 3.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

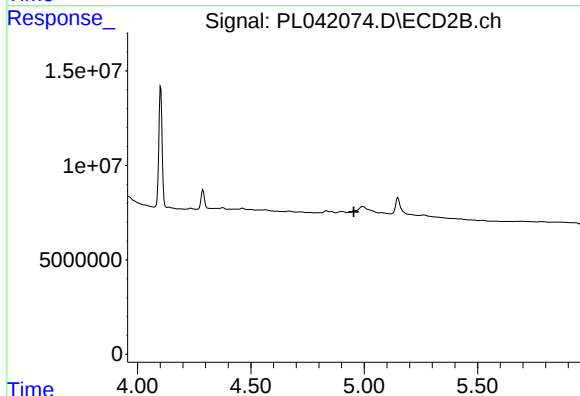


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

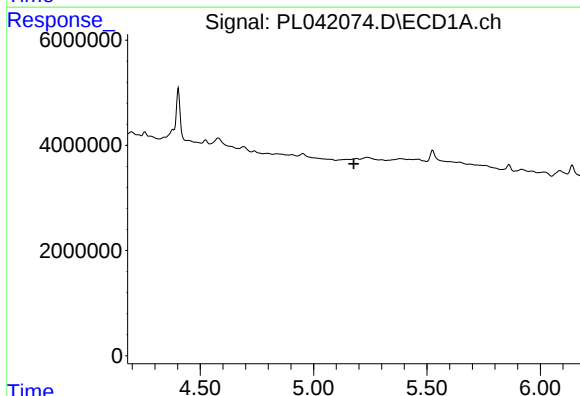


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.178 min
Response: 0
Conc: N.D.

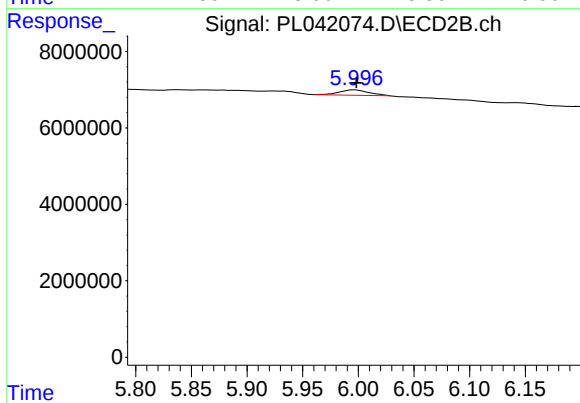

#8 Heptachlor epoxide


R.T.: 5.997 min
Delta R.T.: -0.002 min
Response: 2629472
Conc: 0.73 ng/ml

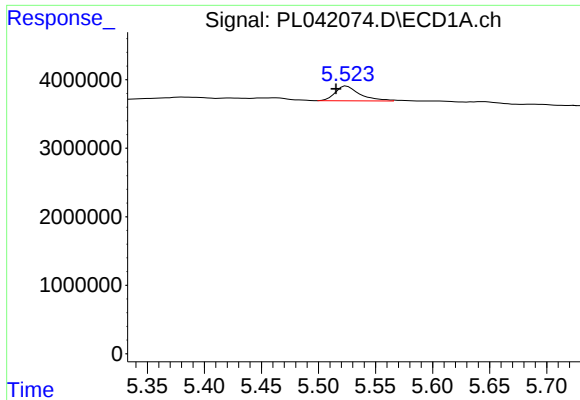

#9 Endosulfan I


R.T.: 5.525 min
Delta R.T.: 0.009 min
Response: 3238741
Conc: 0.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

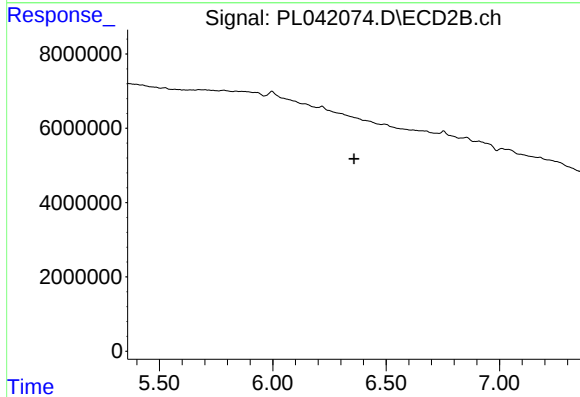


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.358 min
Response: 0
Conc: N.D.

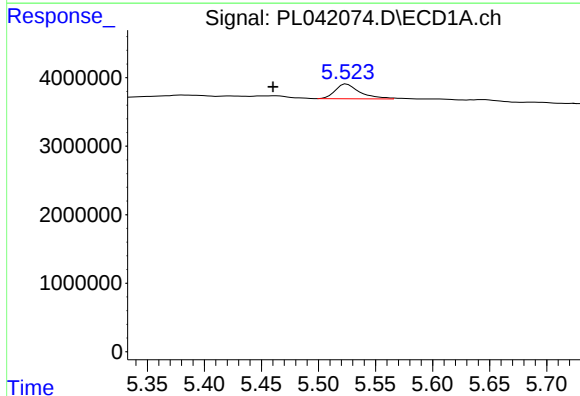


#11 alpha-Chlordane

R.T.: 5.525 min
Delta R.T.: 0.064 min
Response: 3238741
Conc: 0.41 ng/ml

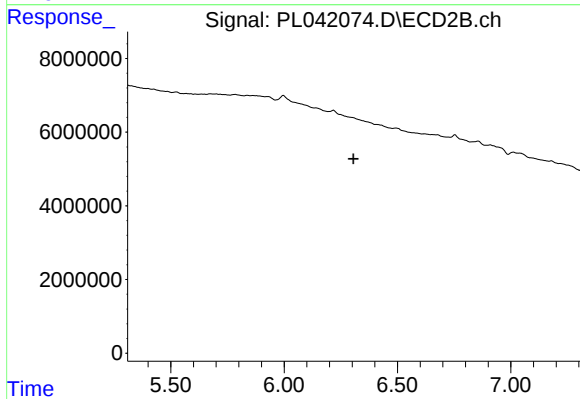

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.307 min
Response: 0
Conc: N.D.

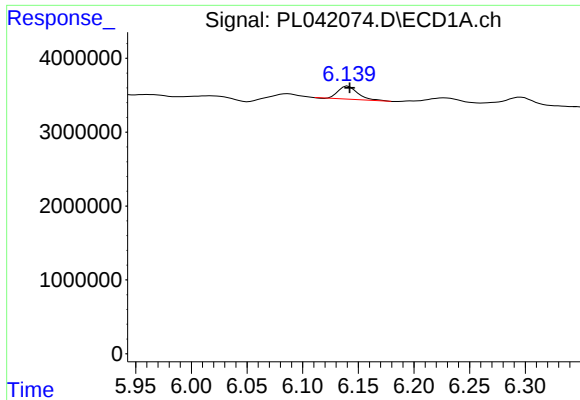

#16 4,4'-DDD


R.T.: 6.141 min
Delta R.T.: -0.002 min
Response: 2123356
Conc: 0.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

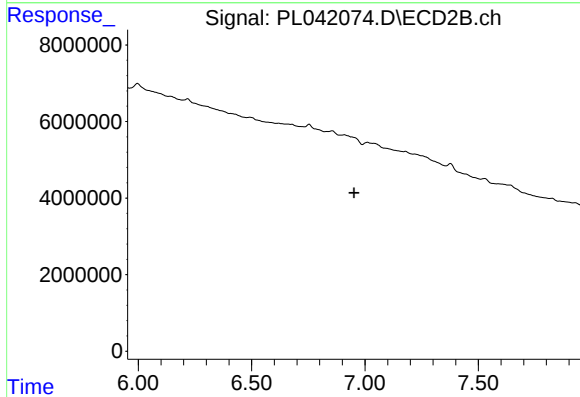


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.952 min
Response: 0
Conc: N.D.

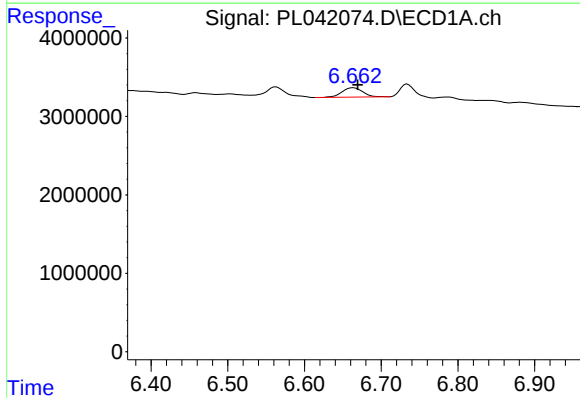


#19 Endosulfan Sulfate

R.T.: 6.664 min
Delta R.T.: -0.006 min
Response: 2265762
Conc: 0.36 ng/ml

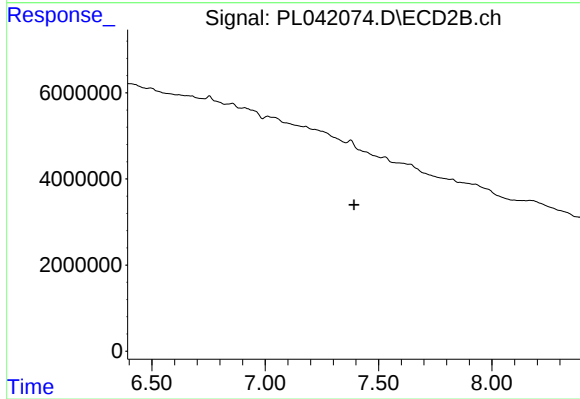

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.392 min
Response: 0
Conc: N.D.

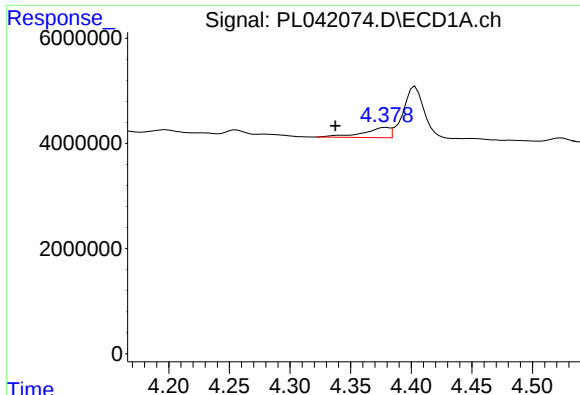

#23 Chlordane-1


R.T.: 4.379 min
Delta R.T.: 0.042 min
Response: 2943993
Conc: 9.86 ng/ml

Instrument :
ECD_L
ClientSampleId :

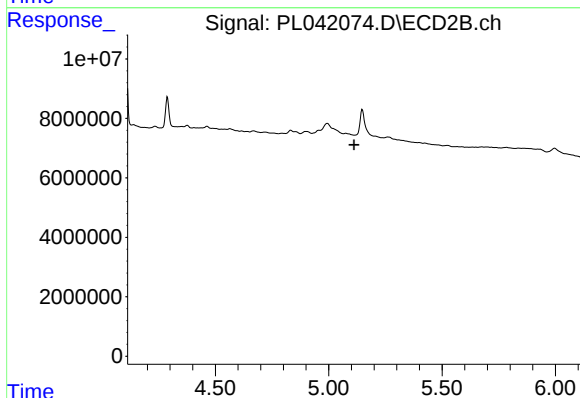


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.112 min
Response: 0
Conc: N.D.

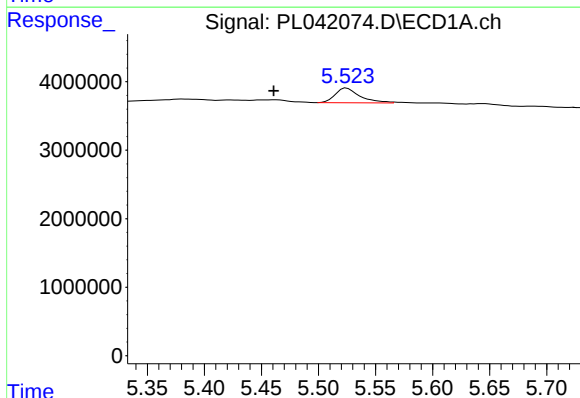


#26 Chlordane-4

R.T.: 5.525 min
Delta R.T.: 0.064 min
Response: 3238741
Conc: 3.88 ng/ml

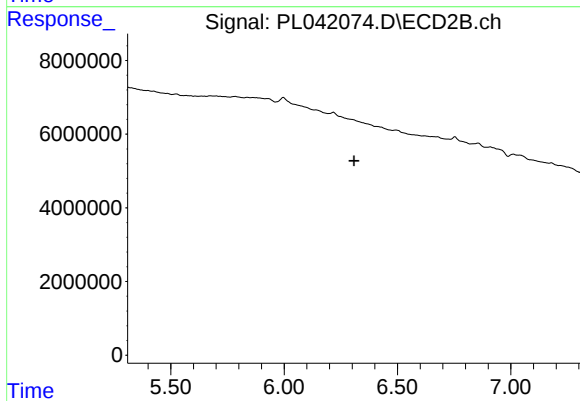

#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.309 min
Response: 0
Conc: N.D.

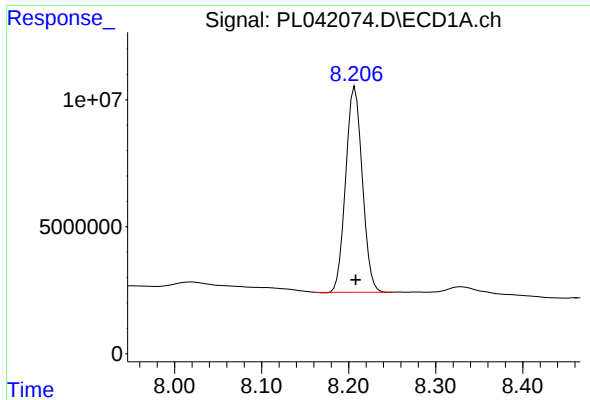

#28 Decachlorobiphenyl


R.T.: 8.207 min

Delta R.T.: 0.000 min

Response: 107379085

Conc: 15.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

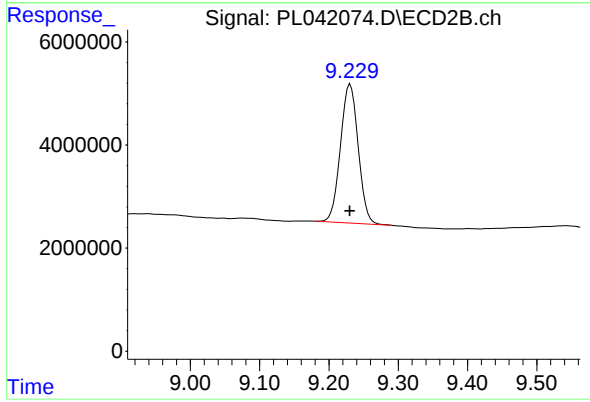

#28 Decachlorobiphenyl

R.T.: 9.231 min

Delta R.T.: 0.000 min

Response: 47766023

Conc: 18.73 ng/ml