

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111218\
 Data File : PL042084.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2018 23:18
 Operator : AJ\SJ
 Sample : J5907-16
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 03:39:32 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	4.102	123.5E6	65832256	20.003	22.220
28)	SA Decachlor...	8.207	9.231	121.5E6	50288034	17.739	19.716
Target Compounds							
2)	A alpha-BHC	3.906	4.503	4175261	2102253	0.440	0.474
4)	MA Heptachlor	4.455	0.000	2194897	0	0.247	N.D. #
6)	B beta-BHC	4.455	0.000	2194897	0	0.595	N.D. #
8)	B Heptachlo...	0.000	5.994	0	2054574	N.D.	0.572 #
13)	MA Dieldrin	5.756	0.000	2218340	0	0.285	N.D. #
14)	MA Endrin	6.068f	0.000	899302	0	0.126	N.D. #
19)	B Endosulfa...	6.656	7.384	10806877	8659361	1.695	3.184 #
20)	A Methoxychlor	0.000	7.647f	0	9835080	N.D.	7.157 #
21)	B Endrin ke...	7.200f	0.000	4596565	0	0.638	N.D. #
23)	Chlordane-1	4.405	5.148	18465266	-3429758	61.873	N.D. #
24)	Chlordane-2	4.803	0.000	1905348	0	6.006	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111218\
Data File : PL042084.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2018 23:18
Operator : AJ\SJ
Sample : J5907-16
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 03:39:32 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

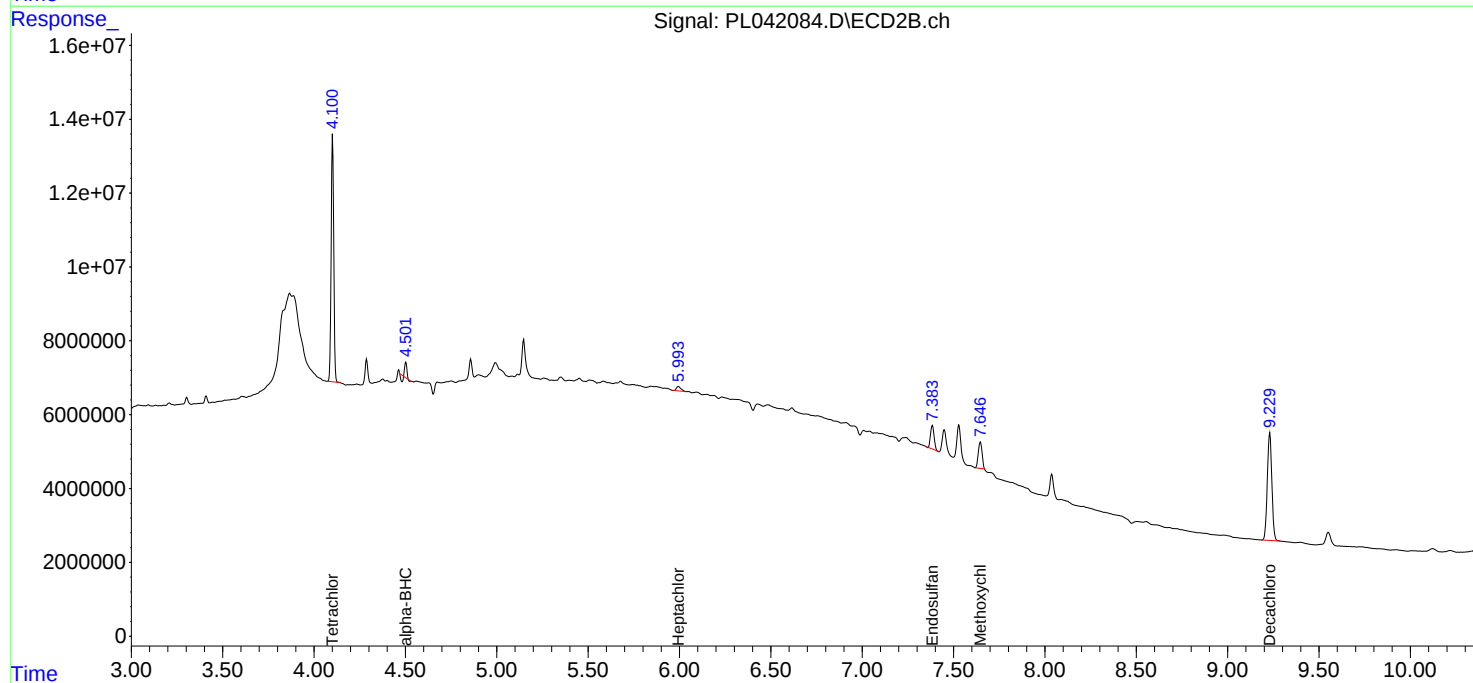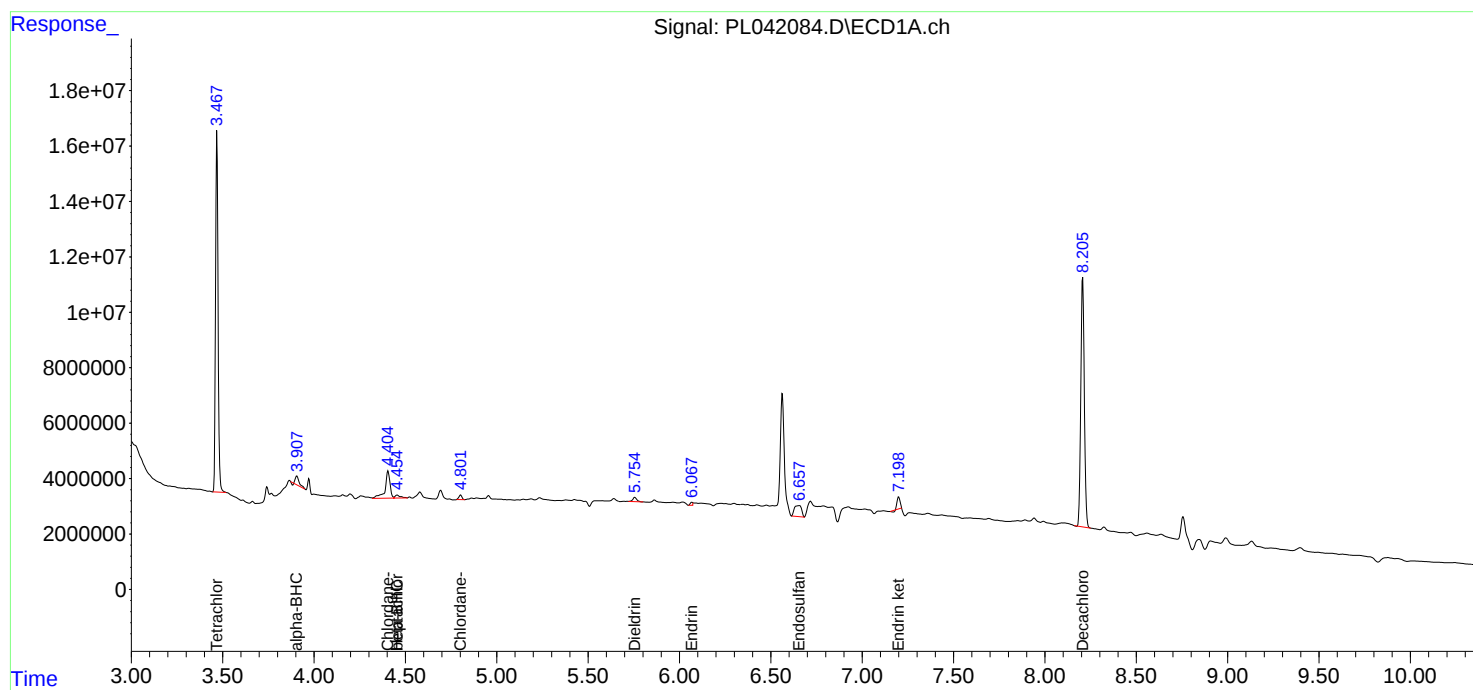


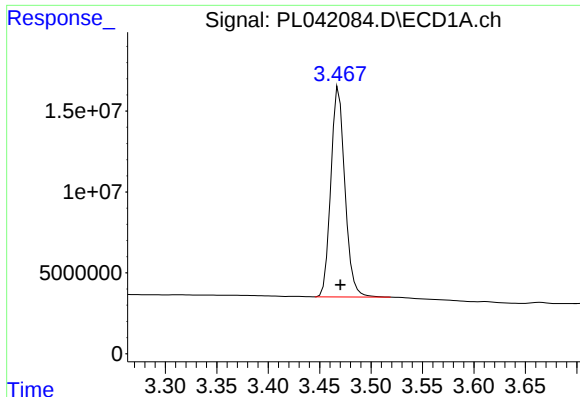

#1 Tetrachloro-m-xylene


R.T.: 3.469 min
Delta R.T.: -0.001 min
Response: 123518717
Conc: 20.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

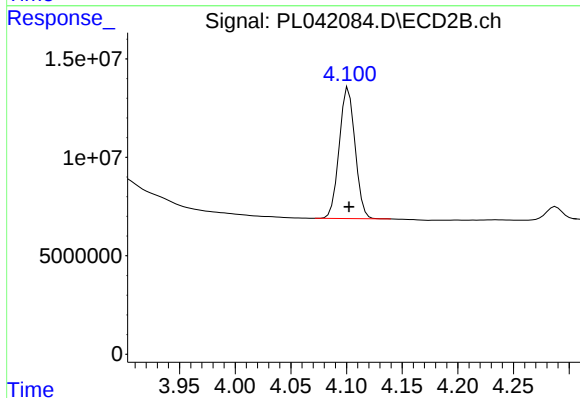


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 65832256
Conc: 22.22 ng/ml

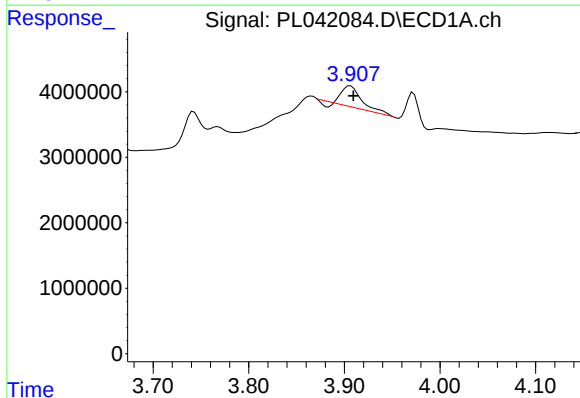


#2 alpha-BHC

R.T.: 3.906 min
Delta R.T.: -0.003 min
Response: 4175261
Conc: 0.44 ng/ml

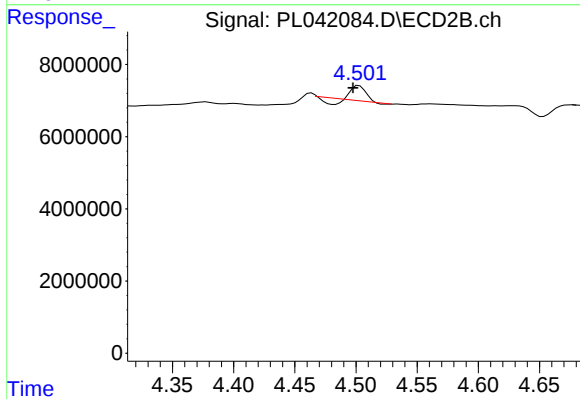

#2 alpha-BHC


R.T.: 4.503 min
Delta R.T.: 0.005 min
Response: 2102253
Conc: 0.47 ng/ml

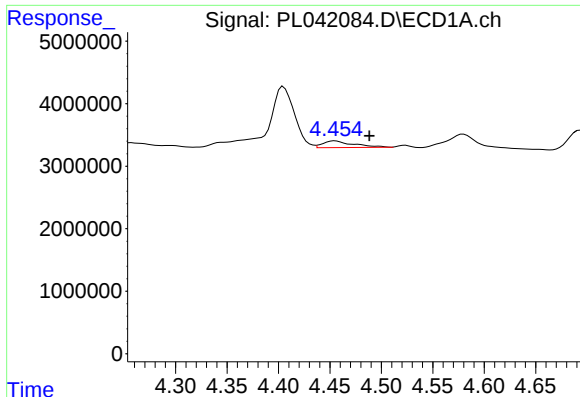

#4 Heptachlor


R.T.: 4.455 min
Delta R.T.: -0.033 min
Response: 2194897
Conc: 0.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

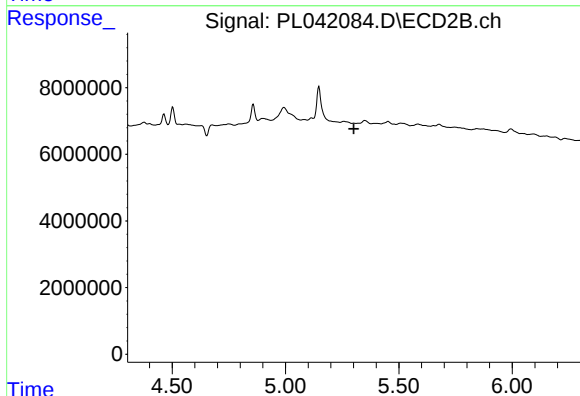


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.302 min
Response: 0
Conc: N.D.

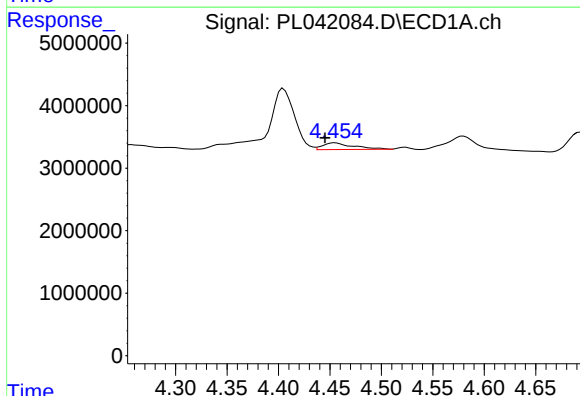


#6 beta-BHC

R.T.: 4.455 min
Delta R.T.: 0.010 min
Response: 2194897
Conc: 0.59 ng/ml

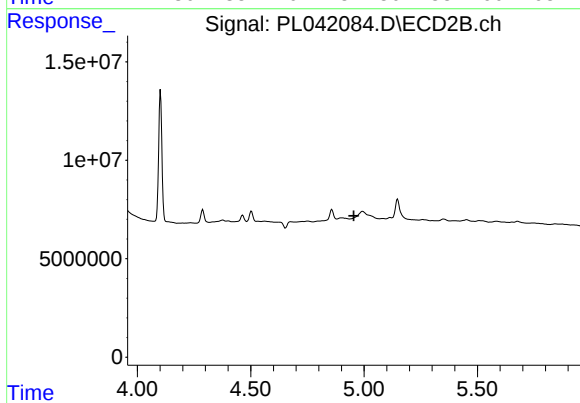

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

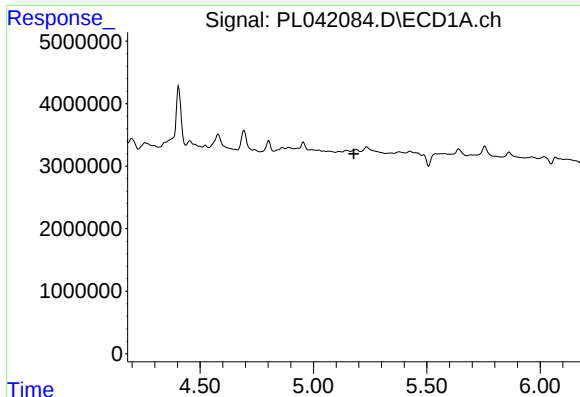

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.178 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

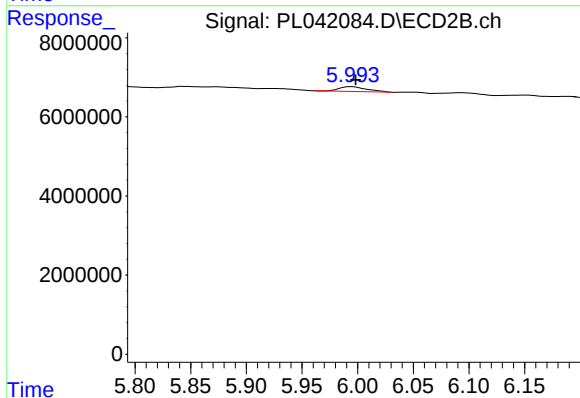


#8 Heptachlor epoxide

R.T.: 5.994 min
Delta R.T.: -0.004 min
Response: 2054574
Conc: 0.57 ng/ml

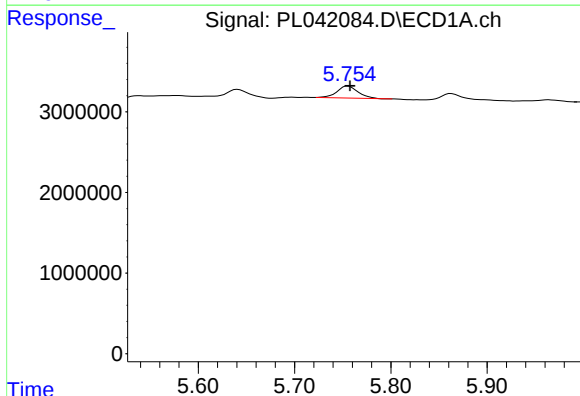


#13 Dieldrin

R.T.: 5.756 min
Delta R.T.: -0.002 min
Response: 2218340
Conc: 0.29 ng/ml

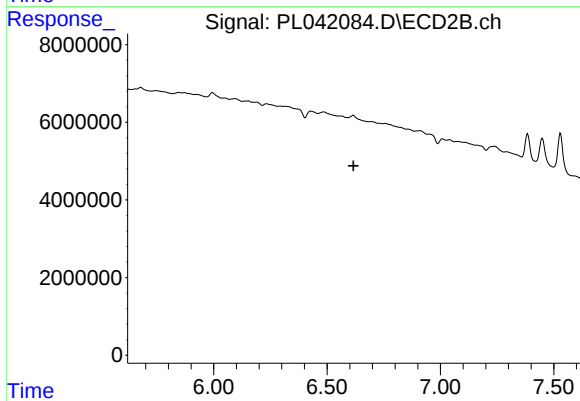

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.617 min
Response: 0
Conc: N.D.

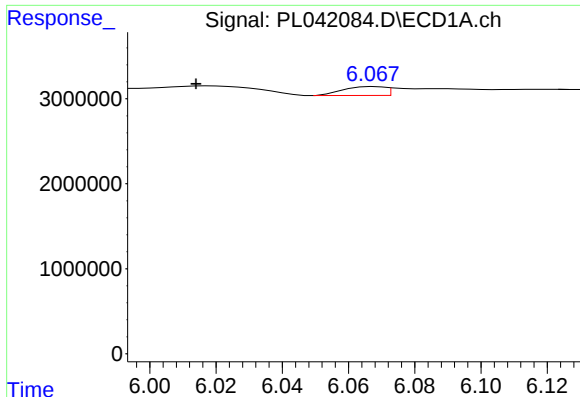

#14 Endrin


R.T.: 6.068 min
Delta R.T.: 0.054 min
Response: 899302
Conc: 0.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

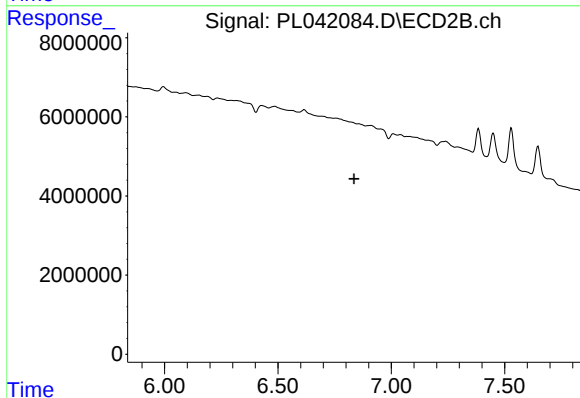


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.836 min
Response: 0
Conc: N.D.

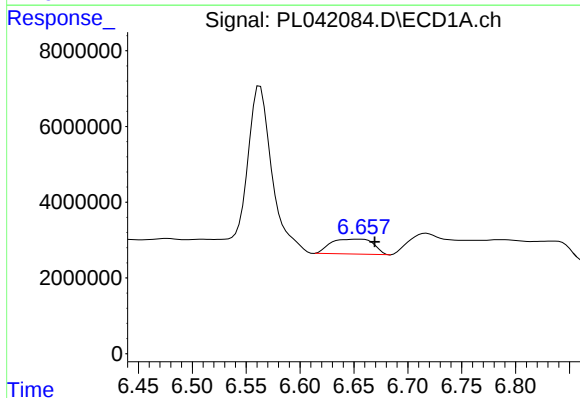


#19 Endosulfan Sulfate

R.T.: 6.656 min
Delta R.T.: -0.013 min
Response: 10806877
Conc: 1.69 ng/ml

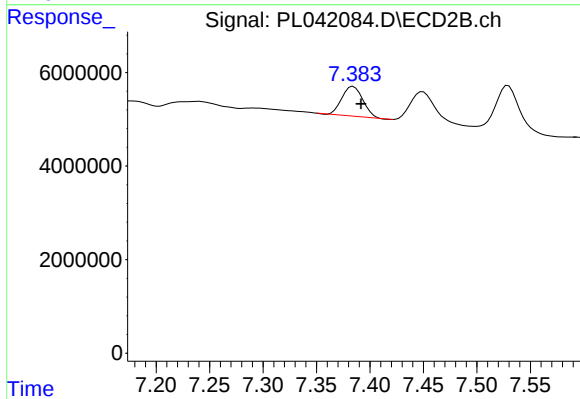

#19 Endosulfan Sulfate


R.T.: 7.384 min
Delta R.T.: -0.007 min
Response: 8659361
Conc: 3.18 ng/ml

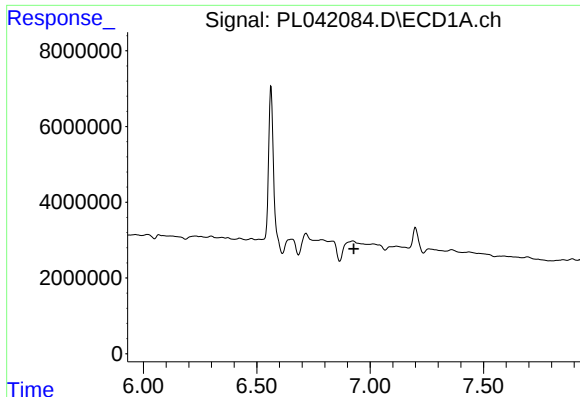

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.928 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

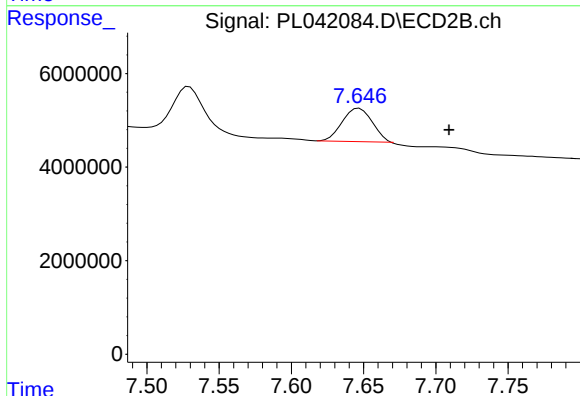


#20 Methoxychlor

R.T.: 7.647 min
Delta R.T.: -0.062 min
Response: 9835080
Conc: 7.16 ng/ml

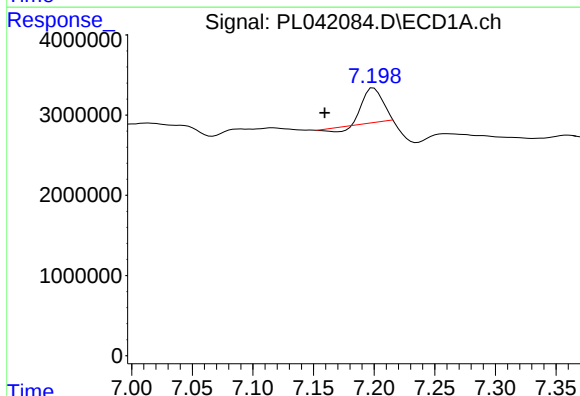


#21 Endrin ketone

R.T.: 7.200 min
Delta R.T.: 0.040 min
Response: 4596565
Conc: 0.64 ng/ml

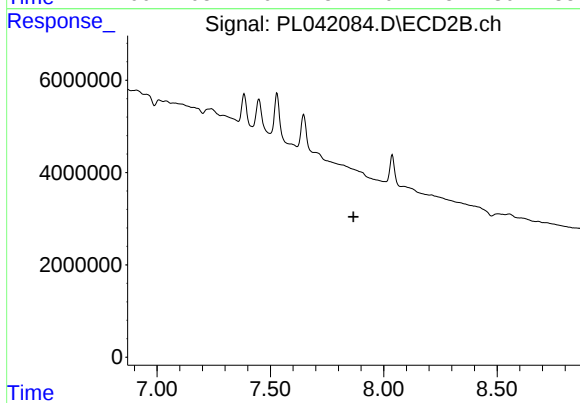

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.867 min
Response: 0
Conc: N.D.

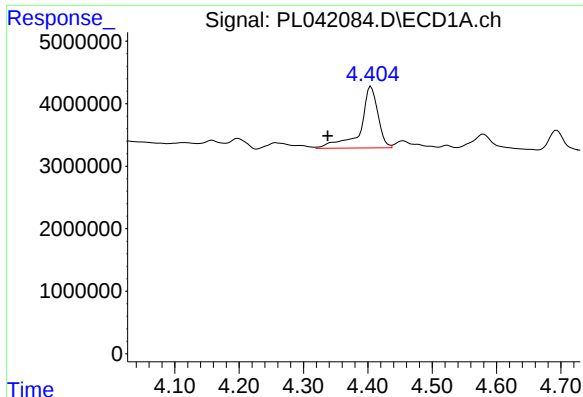

#23 Chlordane-1


R.T.: 4.405 min
Delta R.T.: 0.068 min
Response: 18465266
Conc: 61.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

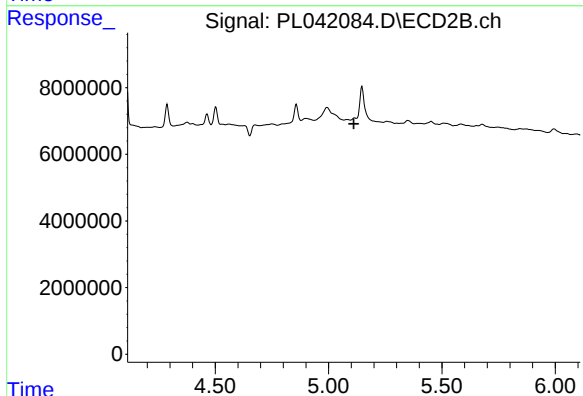


#23 Chlordane-1

R.T.: 5.148 min
Delta R.T.: 0.036 min
Response: -3429758
Conc: N.D.

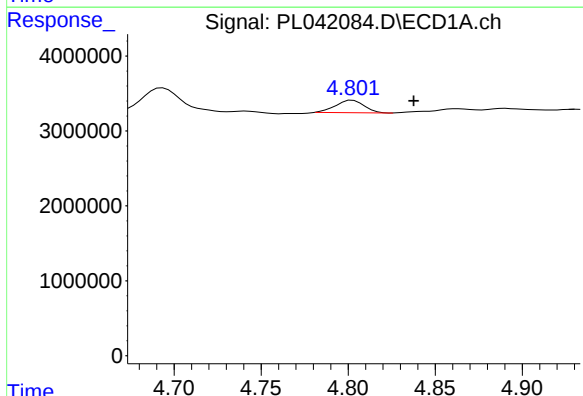


#24 Chlordane-2

R.T.: 4.803 min
Delta R.T.: -0.035 min
Response: 1905348
Conc: 6.01 ng/ml

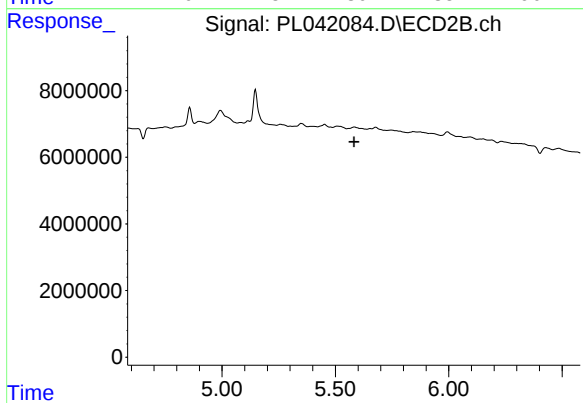

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.583 min
Response: 0
Conc: N.D.

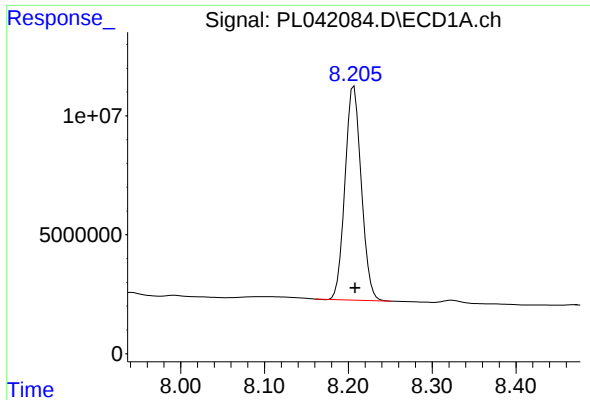

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: -0.001 min
Response: 121520833
Conc: 17.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

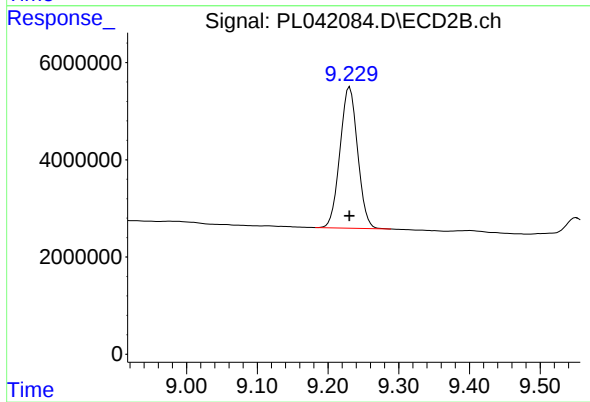

#28 Decachlorobiphenyl

R.T.: 9.231 min
Delta R.T.: 0.000 min
Response: 50288034
Conc: 19.72 ng/ml